

Sample Report



Sample Metadata

Sample Name	Scan 00073
Hazard Level	Clear
Sample Type	USP/Pharmaceutical
Last Modified	2024-03-06 14:34:01-05:00
Created	2024-03-06 14:34:01-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	3.07 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Bottle (Position 3)
Smart Tip Serial Number	6075060600601336

Spectral Data

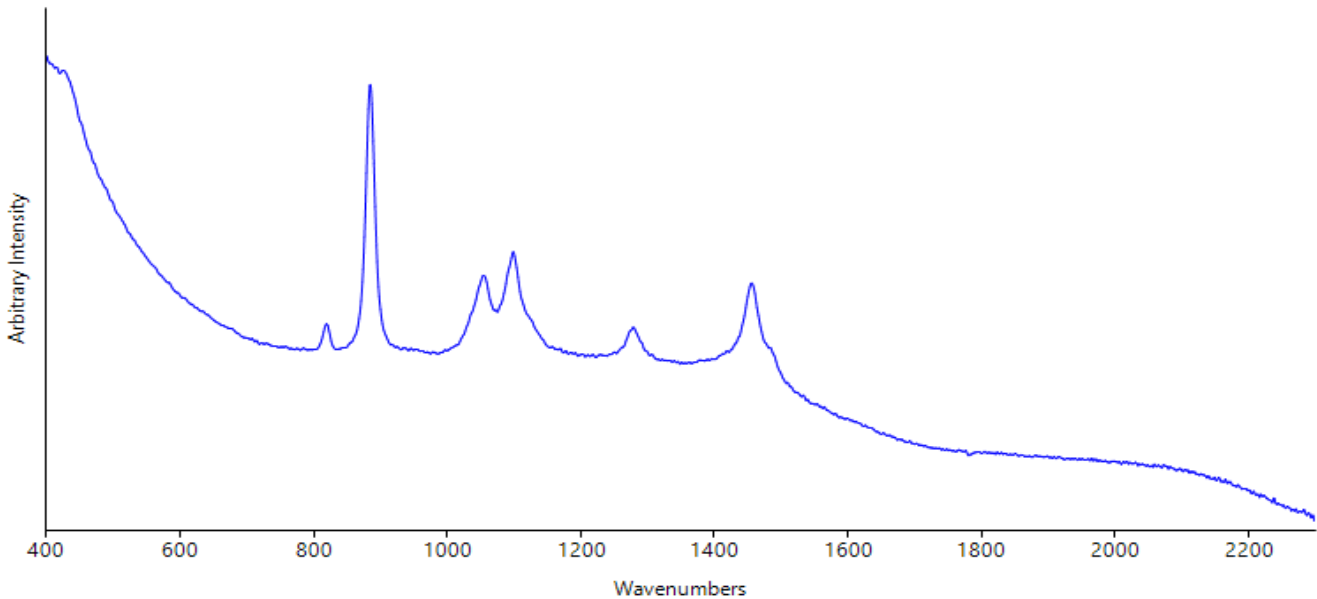


Identification Results

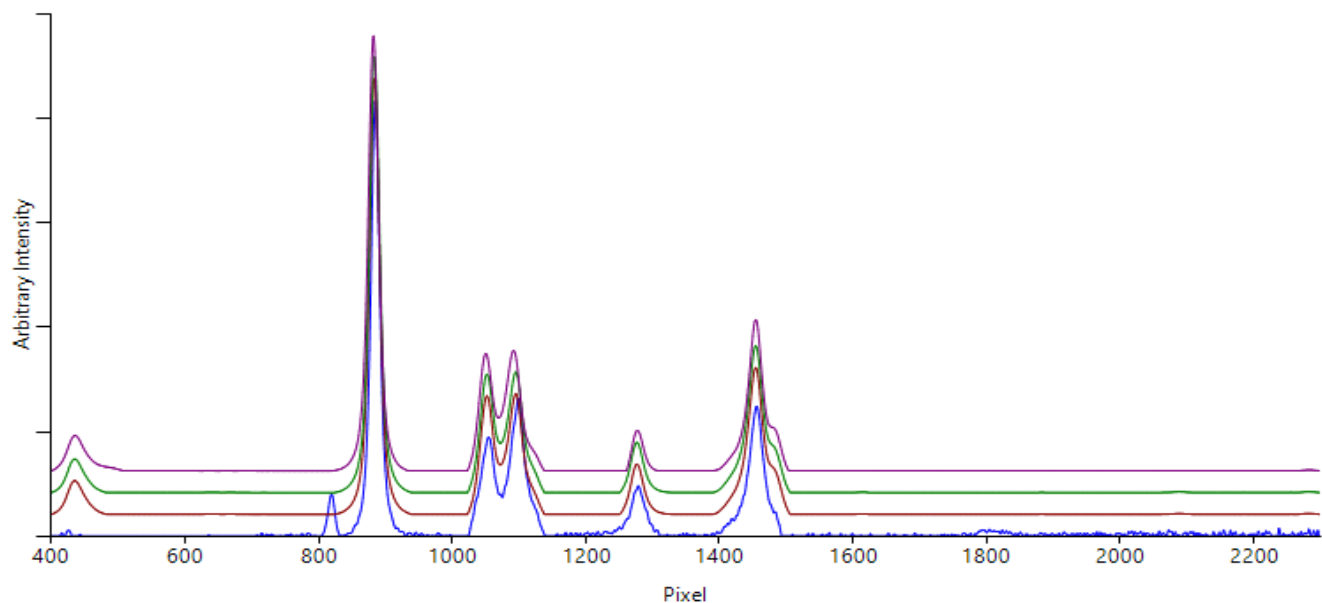

■ Scan 00073 ■ Ethanol ■ Ethanol ■ Ethanol (75% solution)

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Ethanol	USP/Pharmaceutical	0.96	Illicit, Version: 41
Precursor	Ethanol	Chemical Warfare Agent	0.96	CWA, Version: 3
Clear	Ethanol (75% solution)	Chemical	0.91	Illicit, Version: 41

Mixture Identification Results

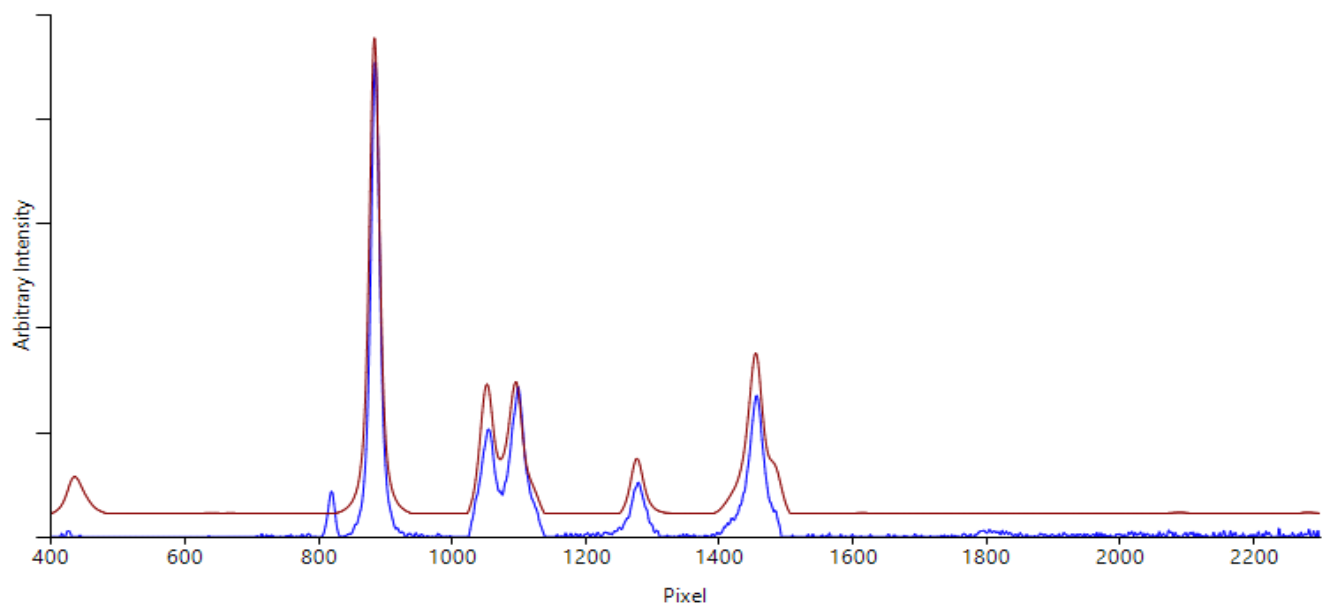

■ Scan 00073 ■ Ethanol

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Ethanol	USP/Pharmaceutical	Illicit, Version: 41	90%