

Sample Report



Sample Metadata

Sample Name	Scan 00079
Hazard Level	Warning
Sample Type	USP/Pharmaceutical
Last Modified	2024-03-06 14:45:36-05:00
Created	2024-03-06 14:45:36-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	2.20 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

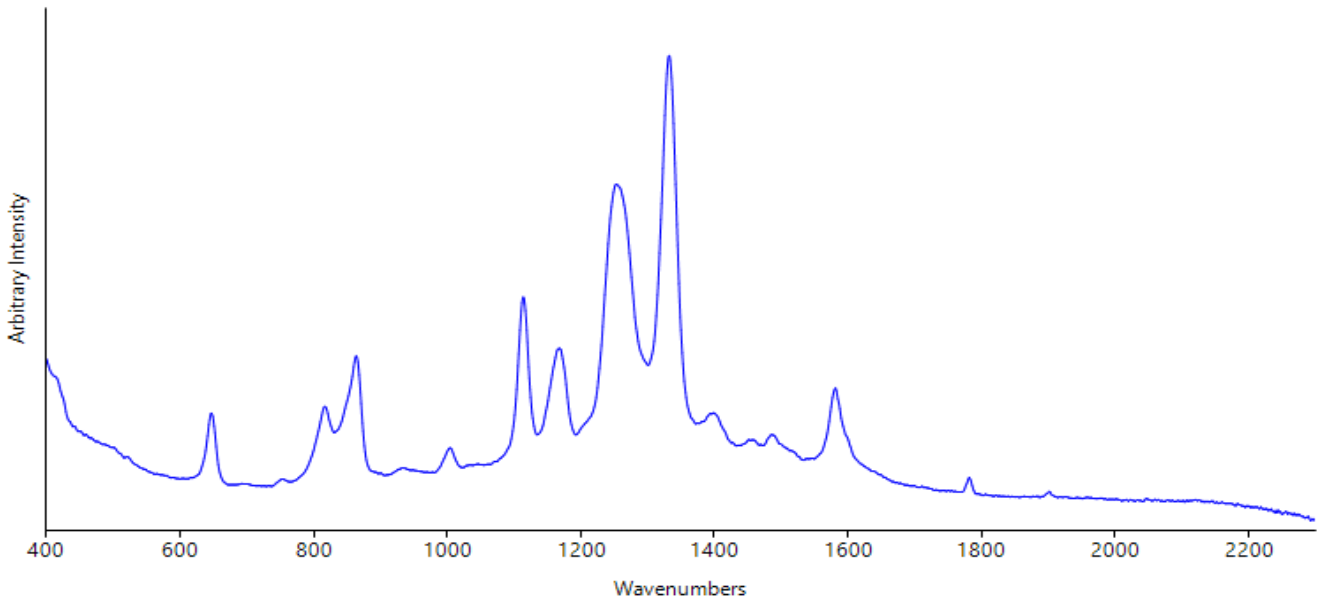

Mixture Identification Results

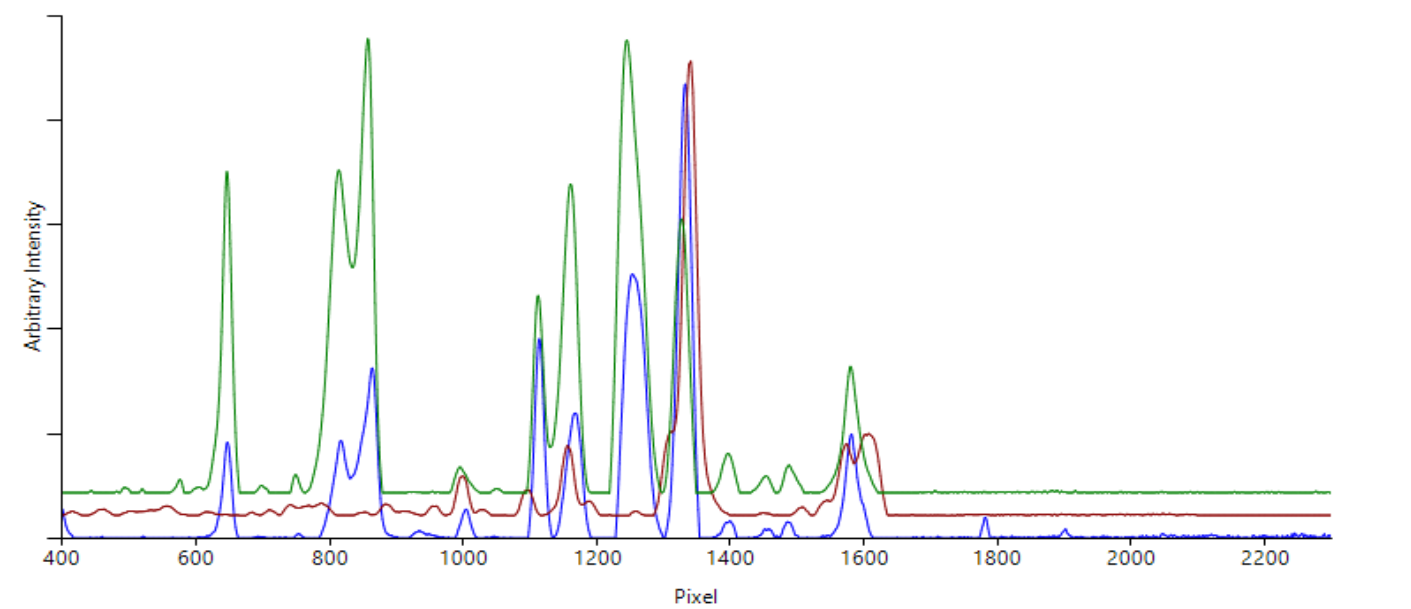

■ Scan 00079 ■ Nitrazepam ■ Nitrophenol SERS 1e-3				
Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Warning	Nitrazepam	USP/Pharmaceutical	Illicit, Version: 41	53%
Unknown	Nitrophenol SERS 1e-3		NATO SERS, Version: 1	39%