

Sample Report



Sample Metadata

Sample Name	Scan 00108
Hazard Level	Alarm
Sample Type	Explosive
Last Modified	2024-03-07 08:29:22-05:00
Created	2024-03-07 08:29:22-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	7.76 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

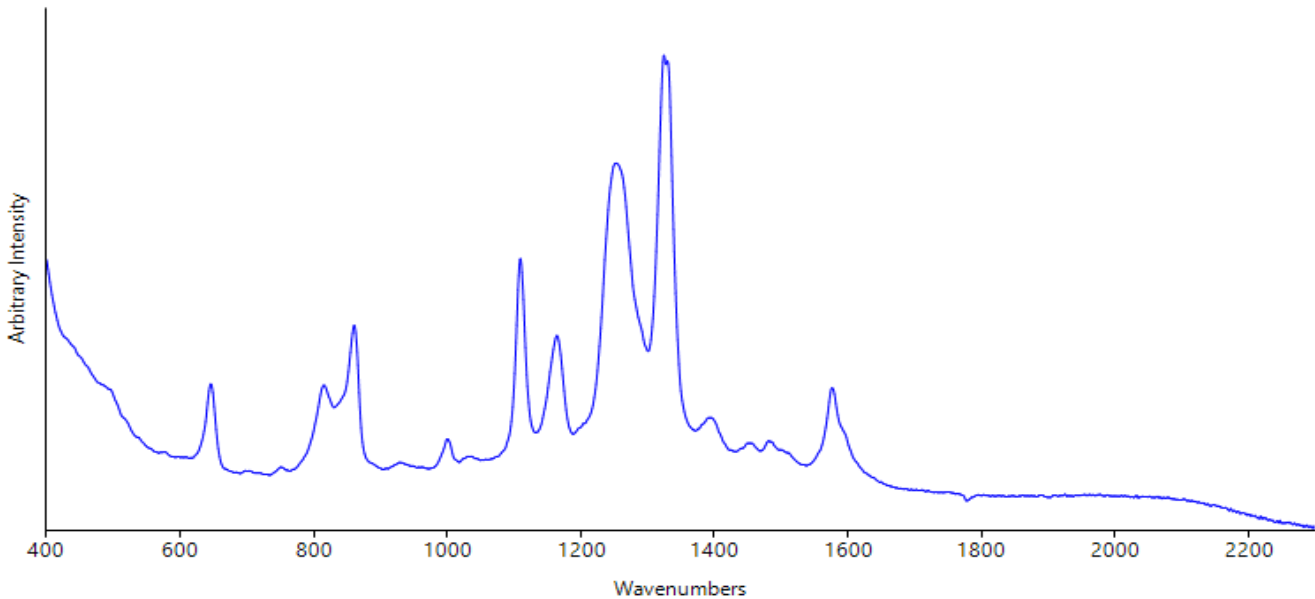

Mixture Identification Results

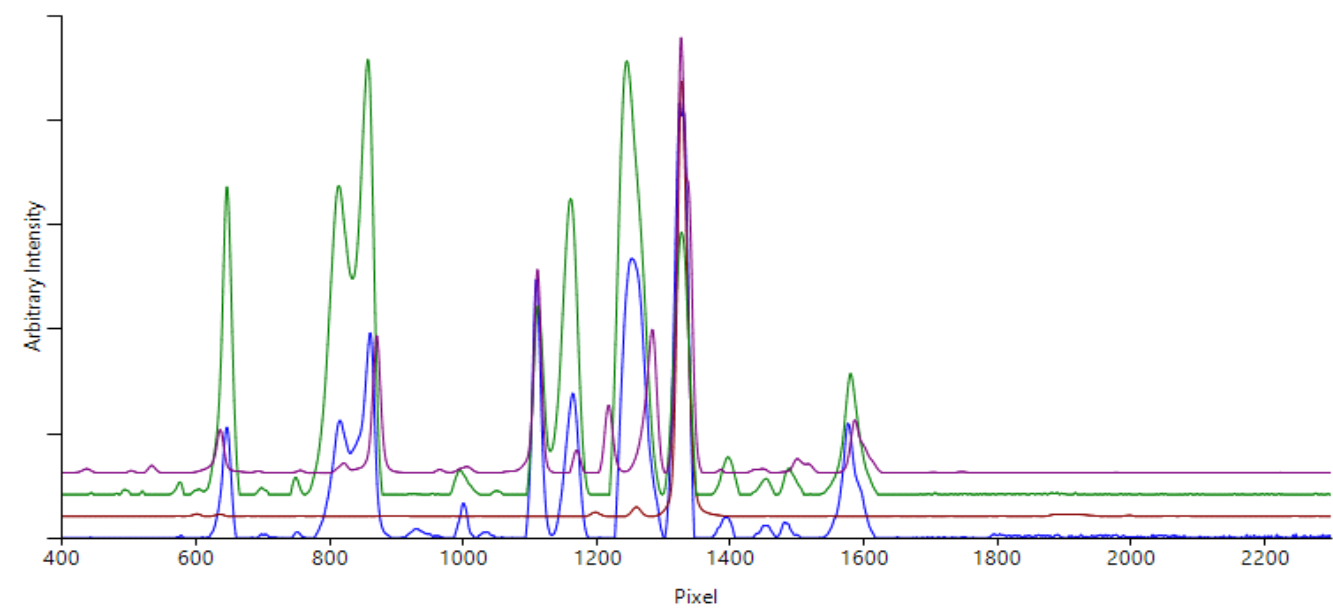

■ Scan 00108 ■ Silver Azide ■ Nitrophenol SERS 1e-3 ■ 4-Nitrophenol (Acetaminophen RCFR)				
Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Alarm	Silver Azide	Explosive	Explosives, Version: 1	32%
Unknown	Nitrophenol SERS 1e-3		NATO SERS, Version: 1	30%
Clear	4-Nitrophenol (Acetaminophen RCFR)	USP/Pharmaceutical	Illicit, Version: 41	19%