

# Sample Report



## Sample Metadata

|               |                           |
|---------------|---------------------------|
| Sample Name   | Scan 00117                |
| Hazard Level  | Alarm                     |
| Sample Type   | Explosive                 |
| Last Modified | 2024-03-07 10:19:41-05:00 |
| Created       | 2024-03-07 10:19:41-05:00 |


## Instrument

|                              |                                 |
|------------------------------|---------------------------------|
| Serial Number                | 192601100201104                 |
| Firmware Package             | 8.0.3.56                        |
| Last Calibration             | 2024-03-06 10:07:19-05:00       |
| Last System Suitability Test | Pass, 2024-03-06 10:07:29-05:00 |


## Acquisition Parameters

|                             |                                      |
|-----------------------------|--------------------------------------|
| Operating Procedure Name    | Default Procedure                    |
| Operating Procedure Version | 1                                    |
| Integration Time            | 7.58 s                               |
| Auto Integration            | On                                   |
| Averages                    | 1                                    |
| Laser Power                 | 5                                    |
| Smart Tip Type              | Intelligent UA, Surface (Position 1) |
| Smart Tip Serial Number     | 6075060600601336                     |

## Spectral Data

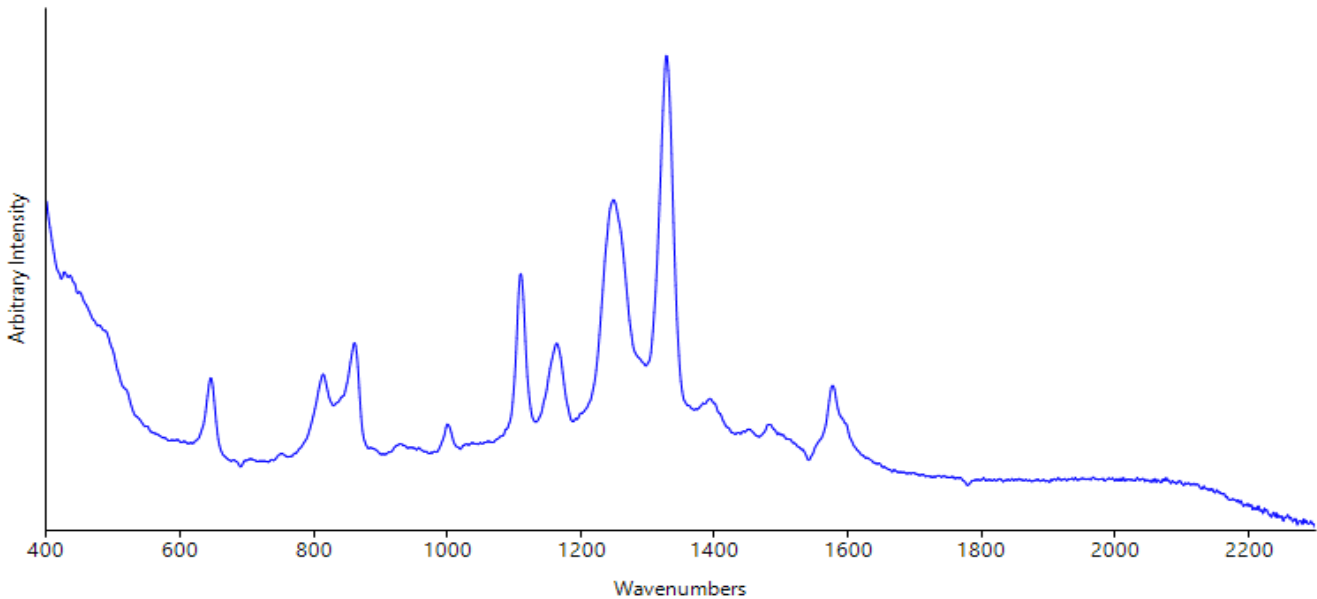

# Mixture Identification Results

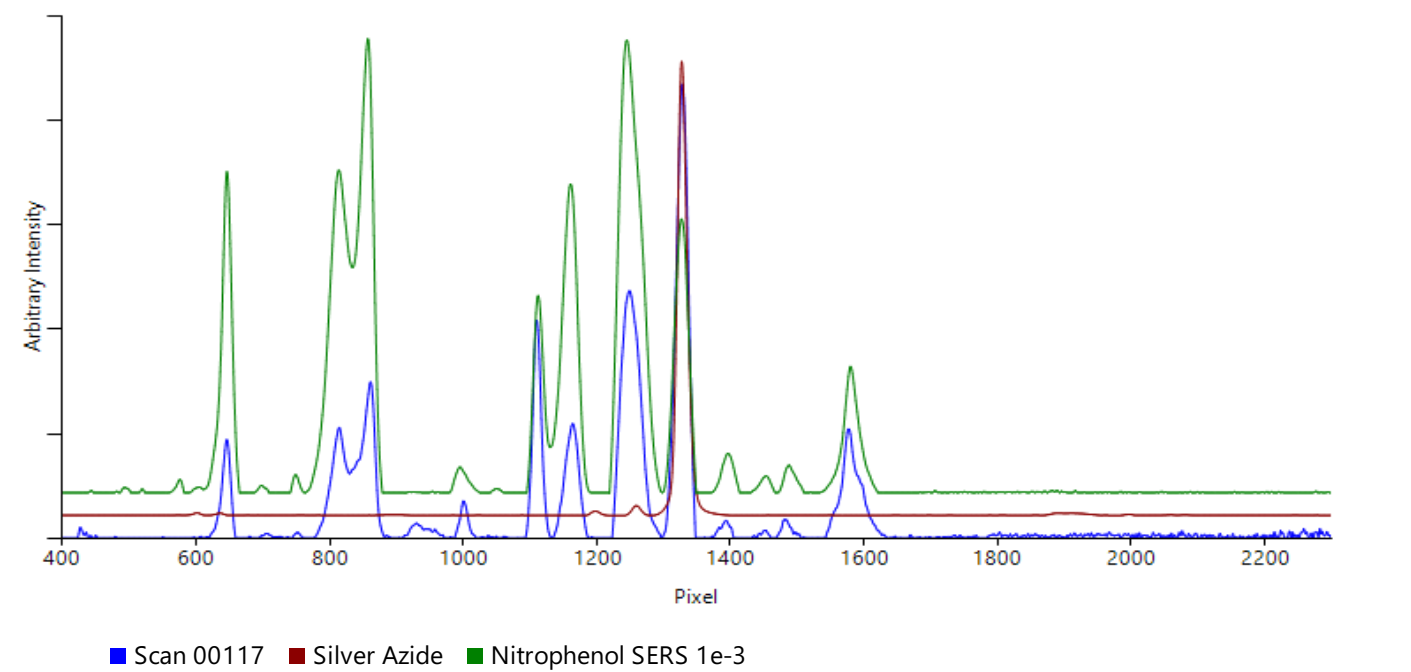

| Hazard Level | Match                 | Sample Type | Source Library         | Spectral Weight % |
|--------------|-----------------------|-------------|------------------------|-------------------|
| Alarm        | Silver Azide          | Explosive   | Explosives, Version: 1 | 63%               |
| Unknown      | Nitrophenol SERS 1e-3 |             | NATO SERS, Version: 1  | 32%               |