

Sample Report



Sample Metadata

Sample Name	Scan 00121
Hazard Level	Clear
Sample Type	Inorganic/Organometallic Chemical, Chemical
Last Modified	2024-03-07 10:32:19-05:00
Created	2024-03-07 10:32:19-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	5.28 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

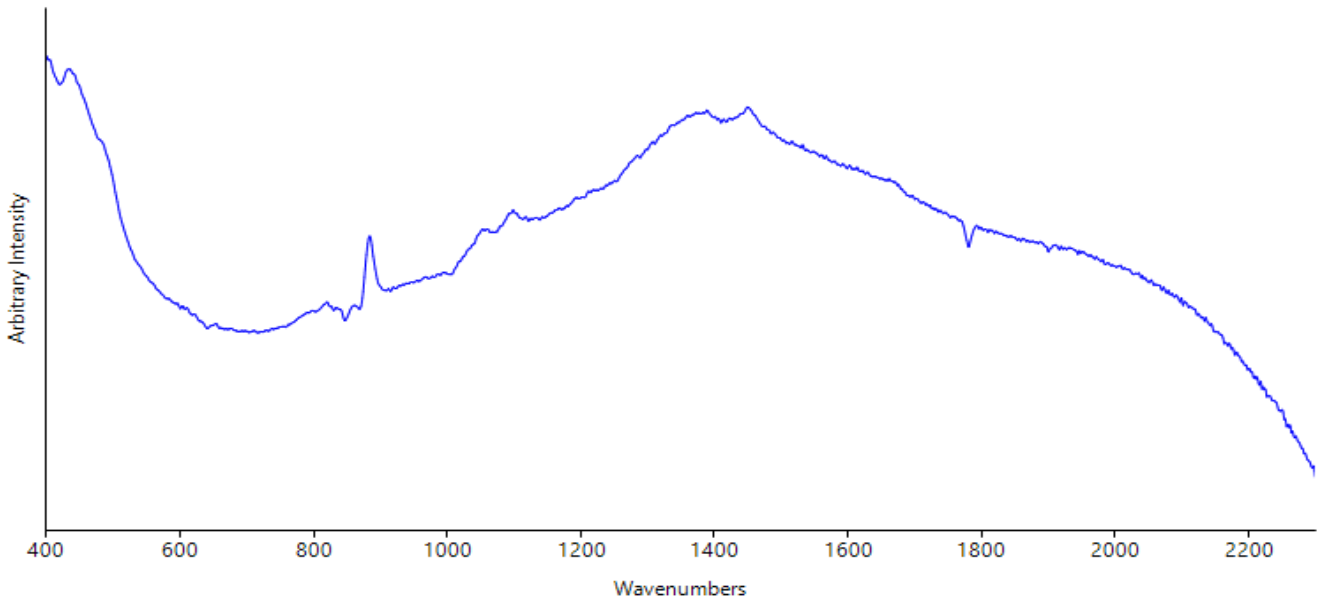


Identification Results

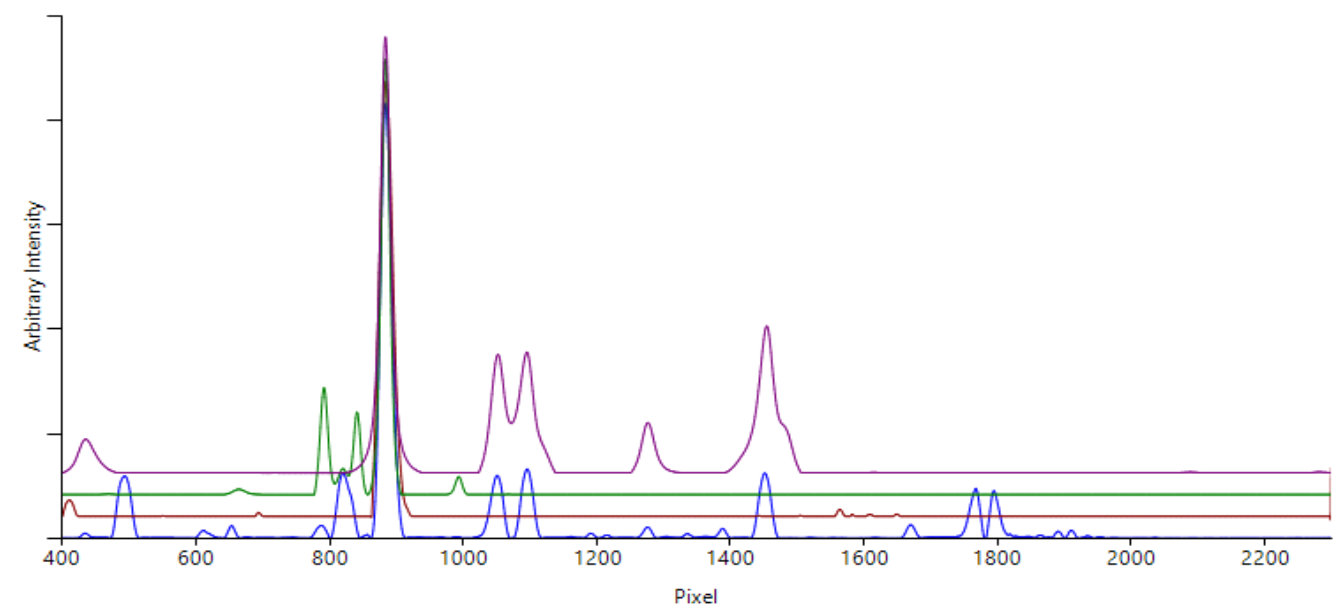

■ Scan 00121 ■ Cobalt(II) tungsten oxide ■ STRONTIUM MOLYBDENUM OXIDE ■ Ethanol

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Cobalt(II) tungsten oxide	Inorganic/Organometallic Chemical	0.86	MCRL Inorganic-Organometallics, Version: 1
Clear	STRONTIUM MOLYBDENUM OXIDE	Inorganic/Organometallic Chemical	0.81	MCRL Inorganic-Organometallics, Version: 1
Clear	Ethanol	USP/Pharmaceutical	0.80	Illicit, Version: 41

Mixture Identification Results

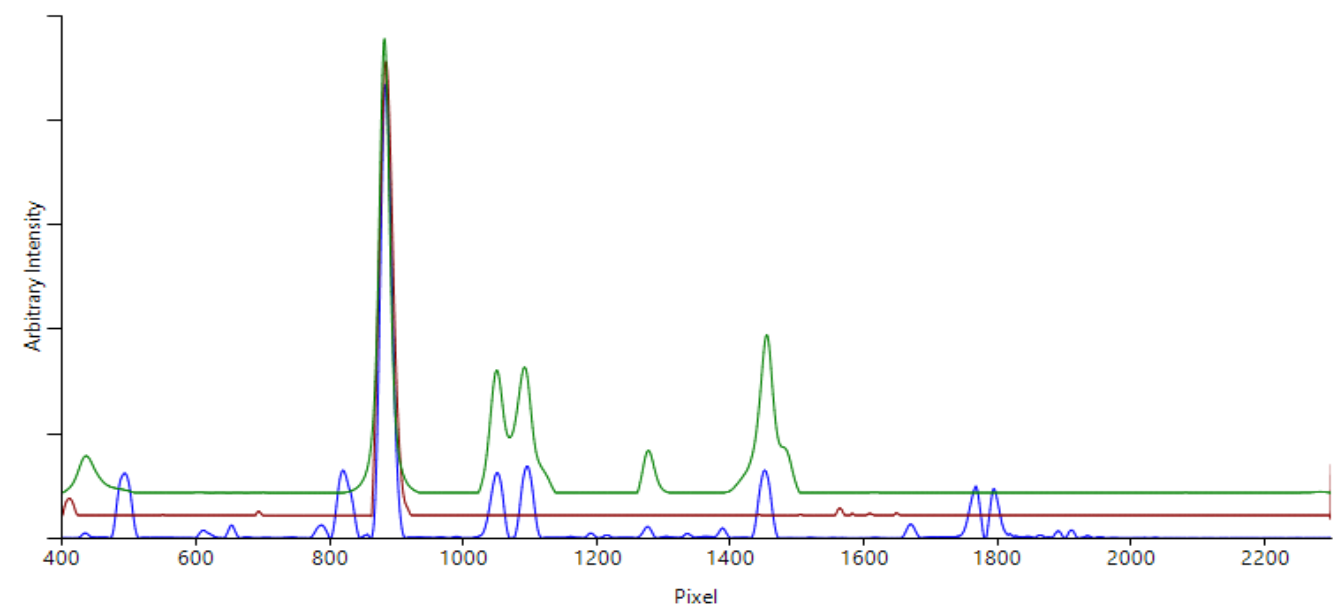

■ Scan 00121 ■ Cobalt(II) tungsten oxide ■ Ethanol (75% solution)

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Cobalt(II) tungsten oxide	Inorganic/Organometallic Chemical	MCRL Inorganic-Organometallics, Version: 1	72%
Clear	Ethanol (75% solution)	Chemical	Illicit, Version: 41	13%