

Sample Report



Sample Metadata

Sample Name	Scan 00167
Hazard Level	Clear
Sample Type	USP/Pharmaceutical
Last Modified	2024-03-07 14:29:03-05:00
Created	2024-03-07 14:29:03-05:00


Instrument

Serial Number	192601100201104
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:07:19-05:00
Last System Suitability Test	Pass, 2024-03-06 10:07:29-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	2.55 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600601336

Spectral Data

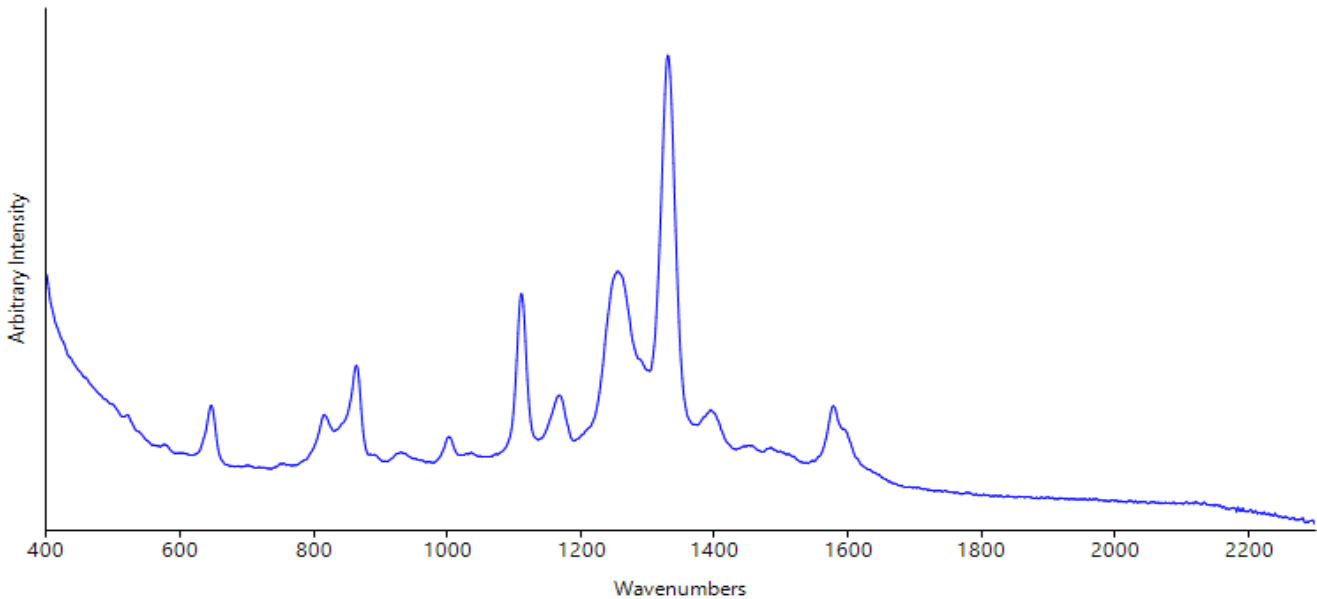


Identification Results

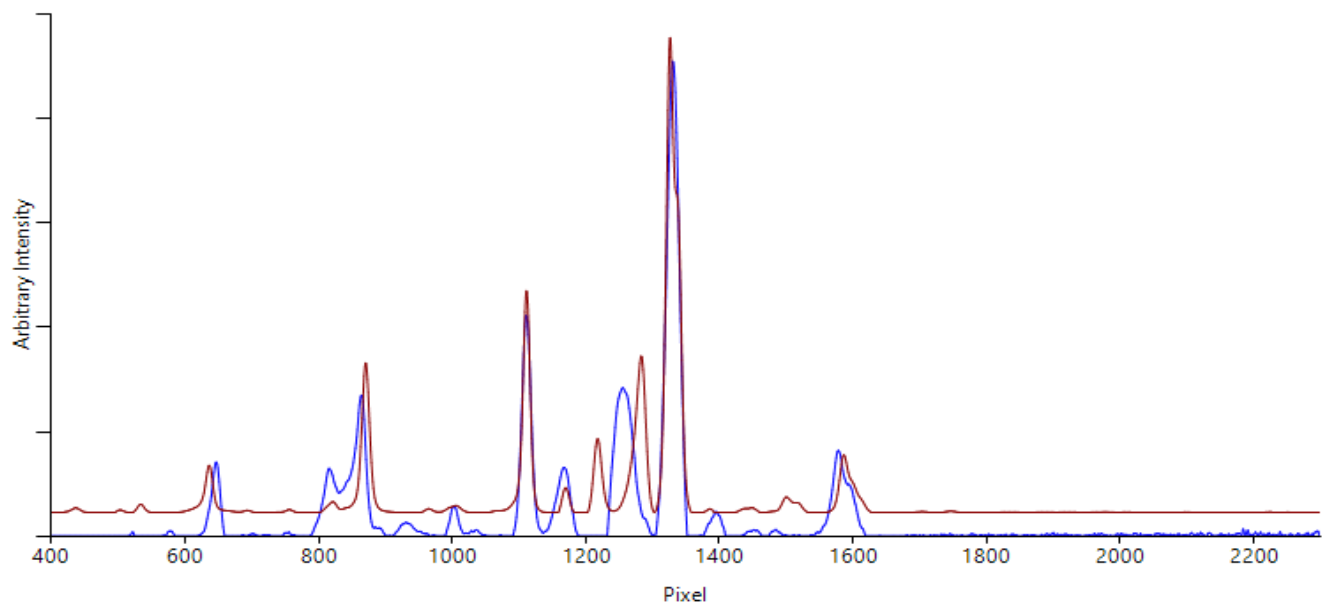

■ Scan 00167 ■ 4-Nitrophenol (Acetaminophen RCFR)

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	4-Nitrophenol (Acetaminophen RCFR)	USP/Pharmaceutical	0.77	Illicit, Version: 41

Mixture Identification Results

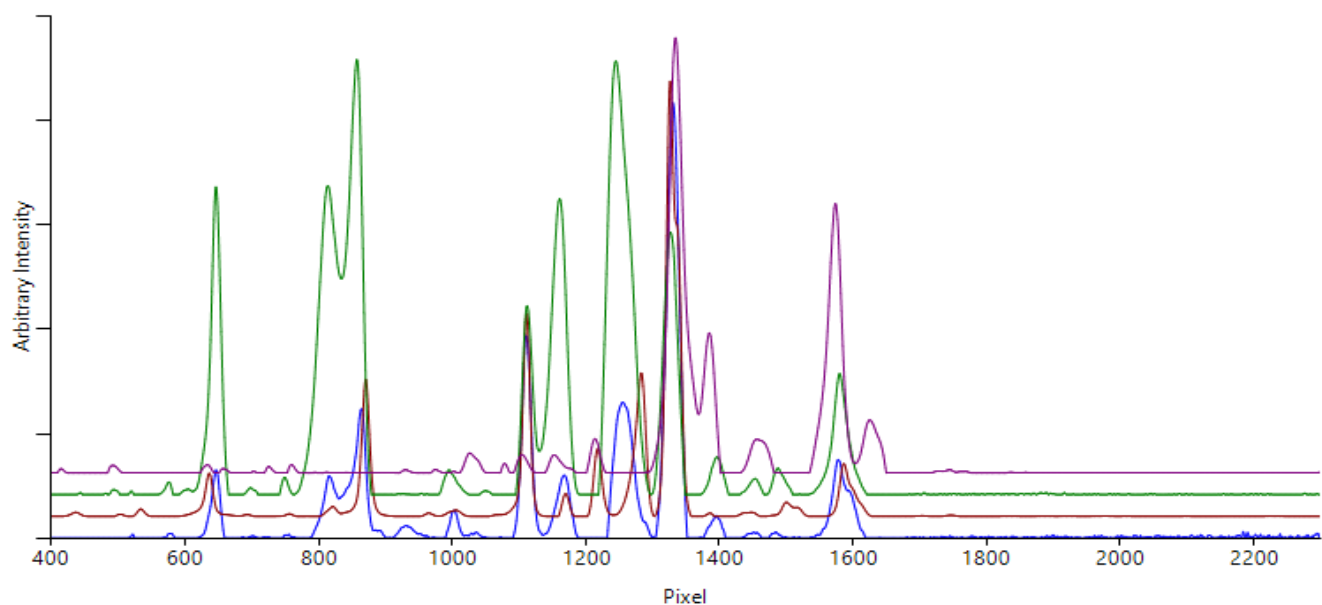

■ Scan 00167 ■ 4-Nitrophenol (Acetaminophen RCFR) ■ Nitrophenol SERS 1e-3 ■ Rifampin

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	4-Nitrophenol (Acetaminophen RCFR)	USP/Pharmaceutical	Illicit, Version: 41	60%
Unknown	Nitrophenol SERS 1e-3		NATO SERS, Version: 1	16%
Clear	Rifampin	USP/Pharmaceutical	Illicit, Version: 41	15%