

Sample Report



Sample Metadata

Sample Name	Scan 00017
Hazard Level	Alarm
Sample Type	Illicit Drug
Last Modified	2024-03-06 10:31:00-05:00
Created	2024-03-06 10:31:00-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	2.04 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

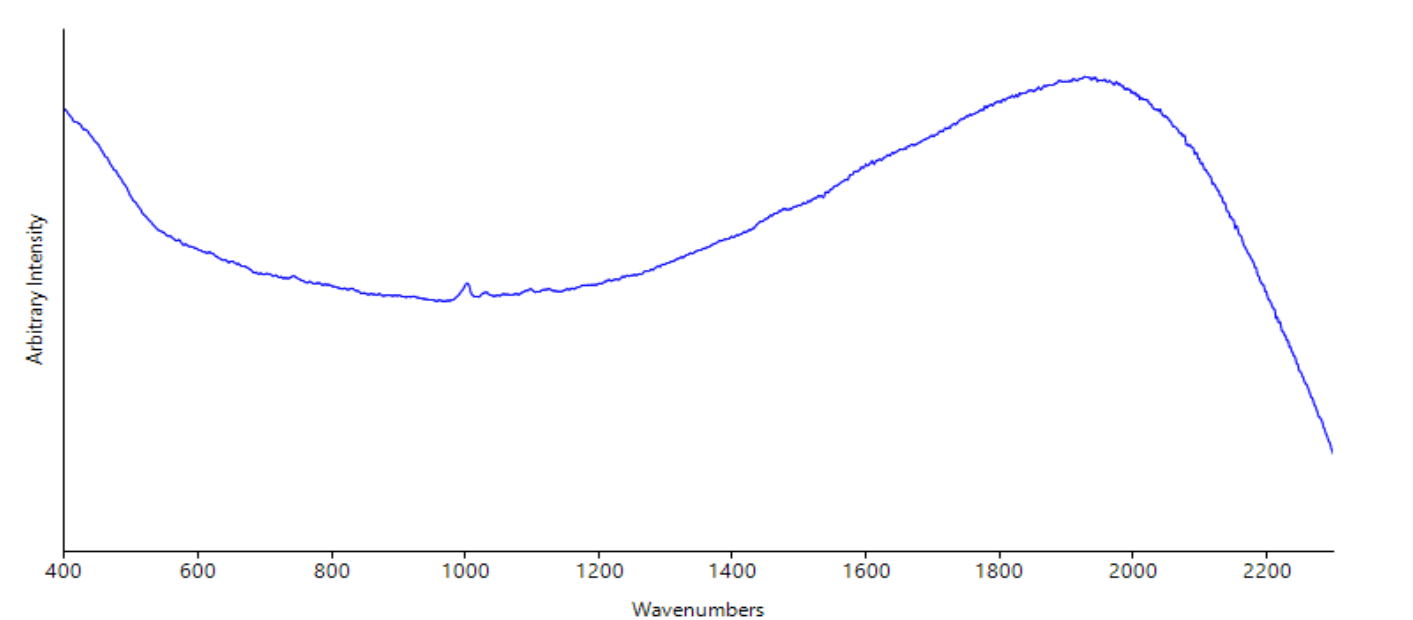


Identification Results

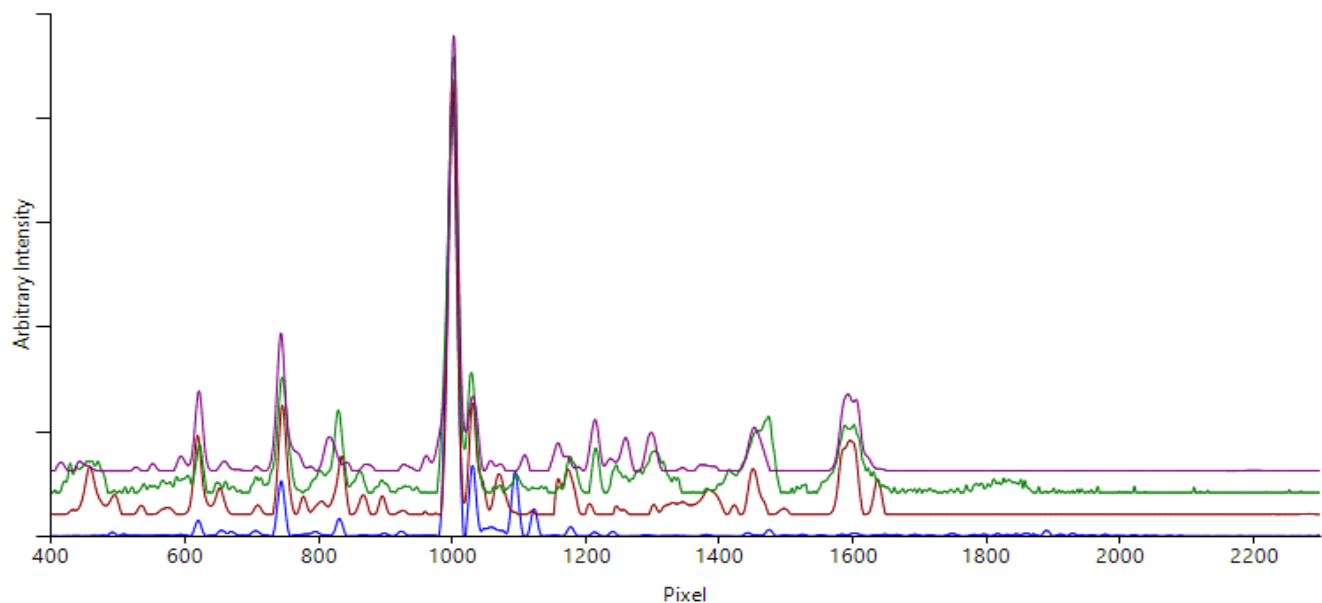

■ Scan 00017 ■ β -hydroxy Fentanyl (hydrochloride) ■ Benzyl Fentanyl PSERS-Ag 1e-3 ■ (±)-cis-Isofentanyl (hydrochloride)

Hazard Level	Match	Sample Type	Match Score	Result Library
Alarm	β -hydroxy Fentanyl (hydrochloride)	Illicit Drug	0.83	Illicit v41, Version: 41
Unknown	Benzyl Fentanyl PSERS-Ag 1e-3		0.81	NATO SERS, Version: 1
Alarm	(±)-cis-Isofentanyl (hydrochloride)	Illicit Drug	0.80	Illicit v41, Version: 41

Mixture Identification Results

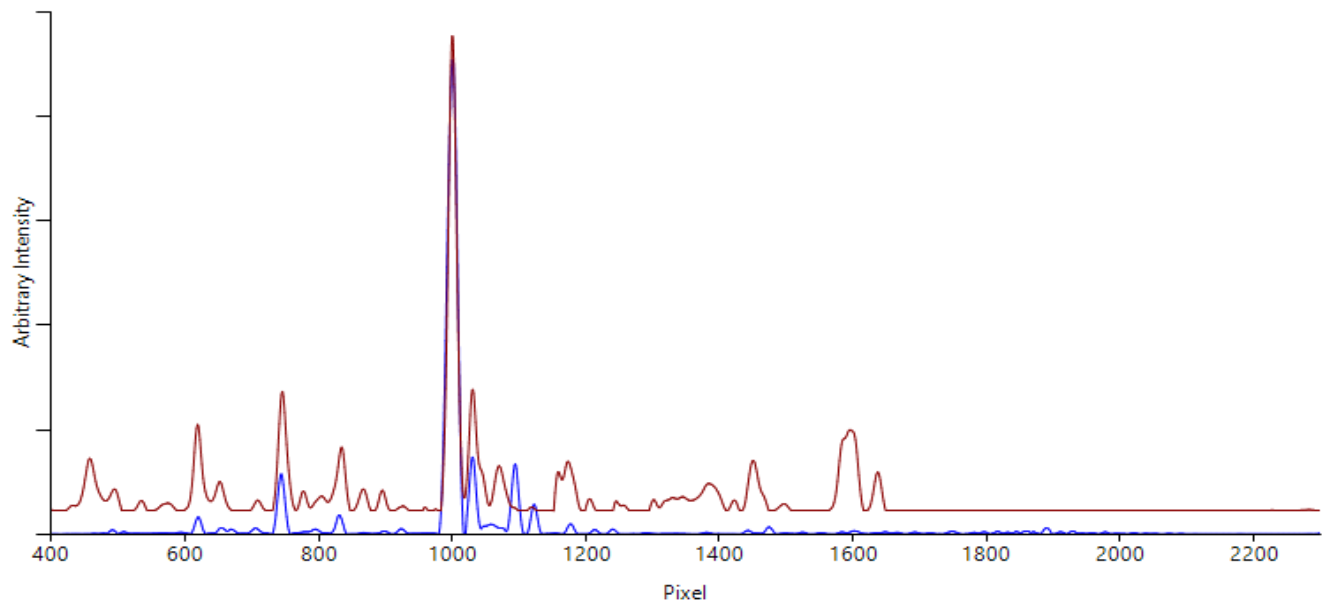

■ Scan 00017 ■ β -hydroxy Fentanyl (hydrochloride)

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Alarm	β -hydroxy Fentanyl (hydrochloride)	Illicit Drug	Illicit v41, Version: 41	86%