

Sample Report



Sample Metadata

Sample Name	Scan 00018
Hazard Level	Alarm
Sample Type	Illicit Drug
Last Modified	2024-03-06 10:35:53-05:00
Created	2024-03-06 10:35:53-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	0.91 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

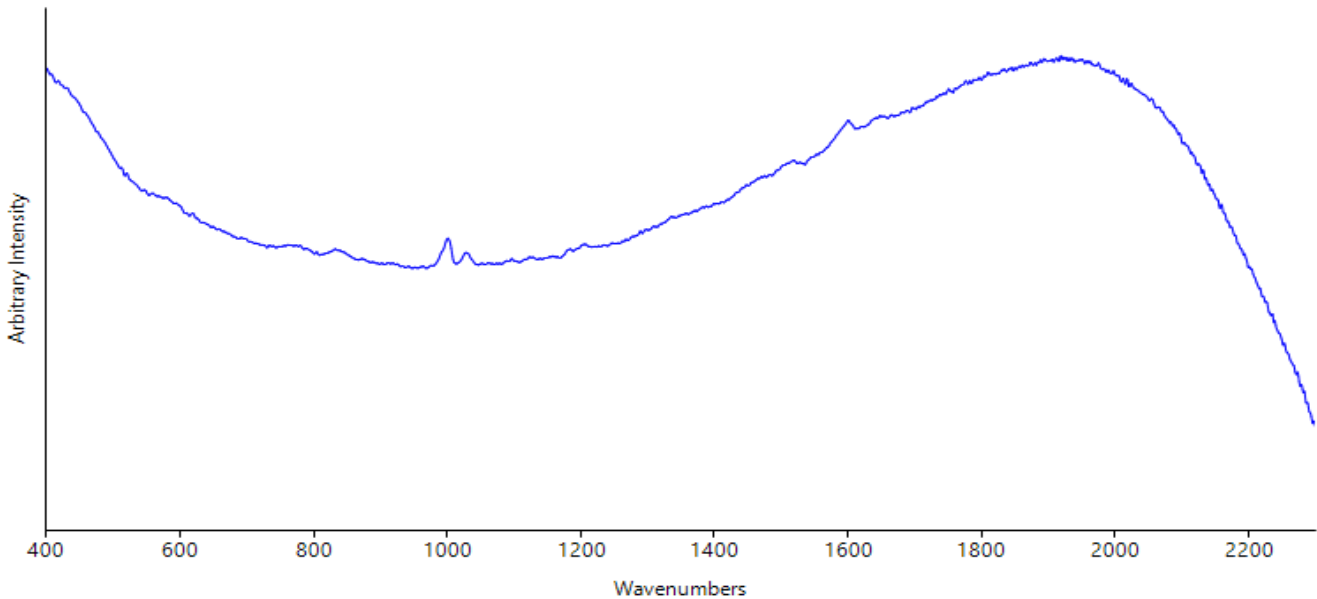


Identification Results

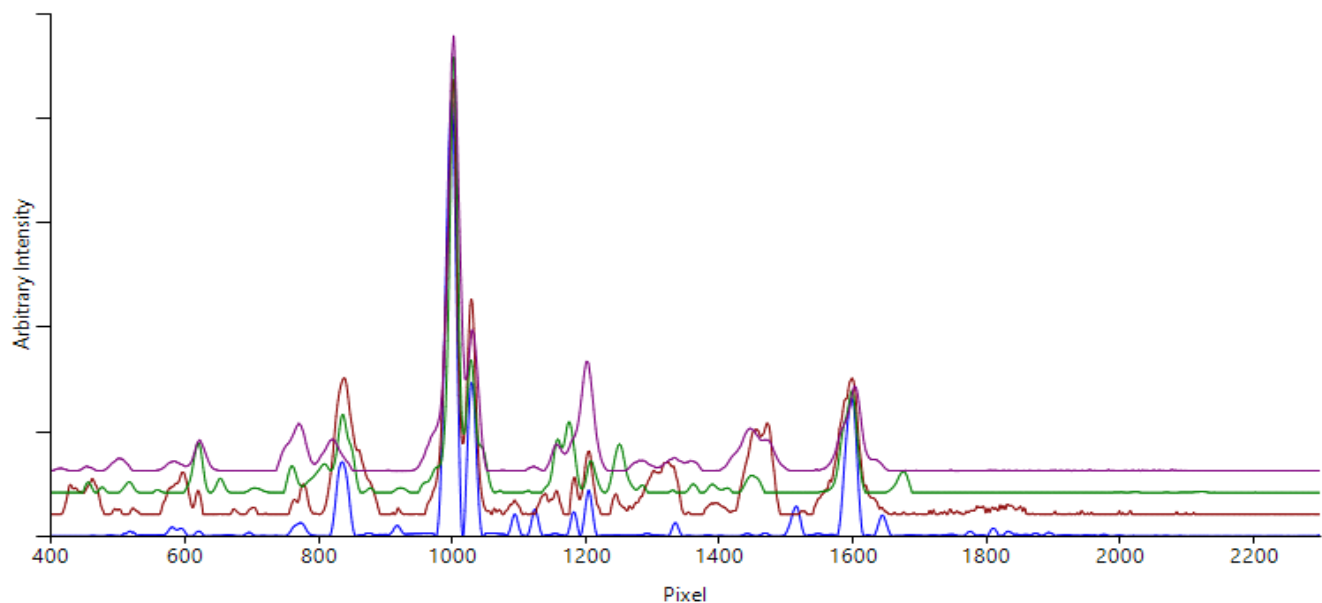

■ Scan 00018 ■ 4-ANPP PSERS-Ag 1e-4 ■ Phenoxyacetyl fentanyl (hydrochloride) ■ N-Methyl-2-phenylethanamine

Hazard Level	Match	Sample Type	Match Score	Result Library
Unknown	4-ANPP PSERS-Ag 1e-4		0.80	NATO SERS, Version: 1
Alarm	Phenoxyacetyl fentanyl (hydrochloride)	Illicit Drug	0.78	Illicit v41, Version: 41
Precursor	N-Methyl-2-phenylethanamine	Chemical	0.77	Illicit v41, Version: 41

Mixture Identification Results

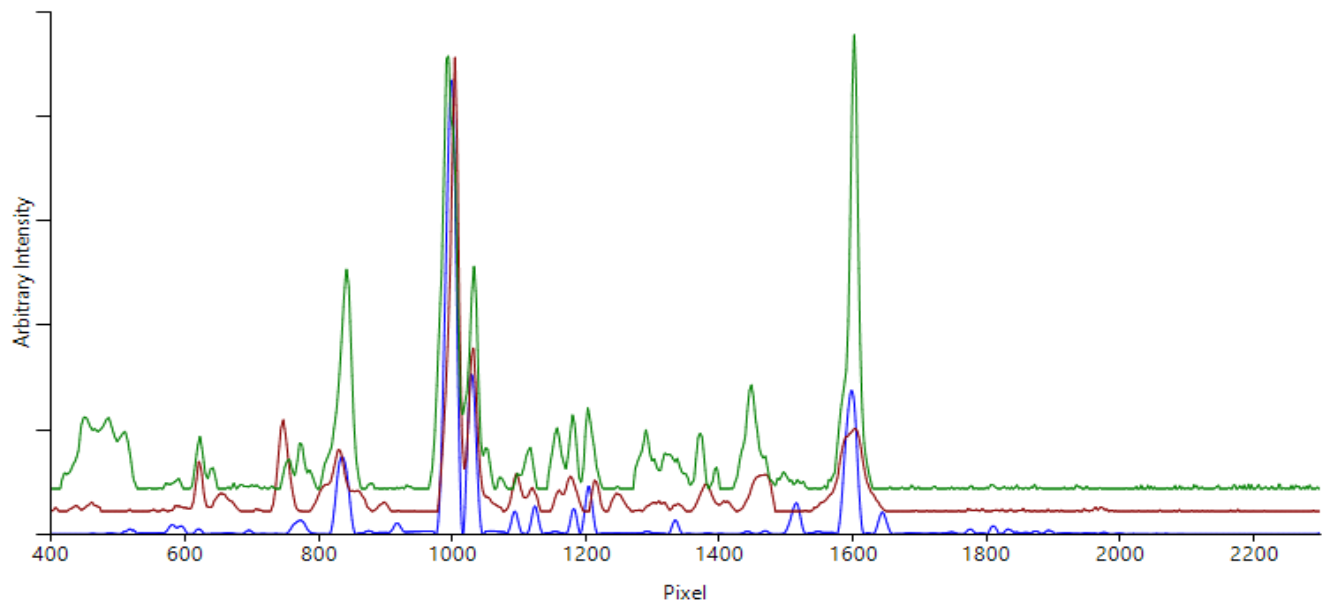

■ Scan 00018 ■ Fentanyl-Benzyl Fentanyl SERS ■ 4-Anilino-N-phenethylpiperidine

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Alarm	Fentanyl-Benzyl Fentanyl SERS	Illicit Drug	DEVCOM CBC SERS, Version: 6	62%
Alarm	4-Anilino-N-phenethylpiperidine	Illicit Drug	Illicit v41, Version: 41	29%