

Sample Report



Sample Metadata

Sample Name	Scan 00032
Hazard Level	Precursor
Sample Type	Explosive
Last Modified	2024-03-06 11:25:17-05:00
Created	2024-03-06 11:25:17-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	2.67 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Bottle (Position 3)
Smart Tip Serial Number	6075060600301151

Spectral Data

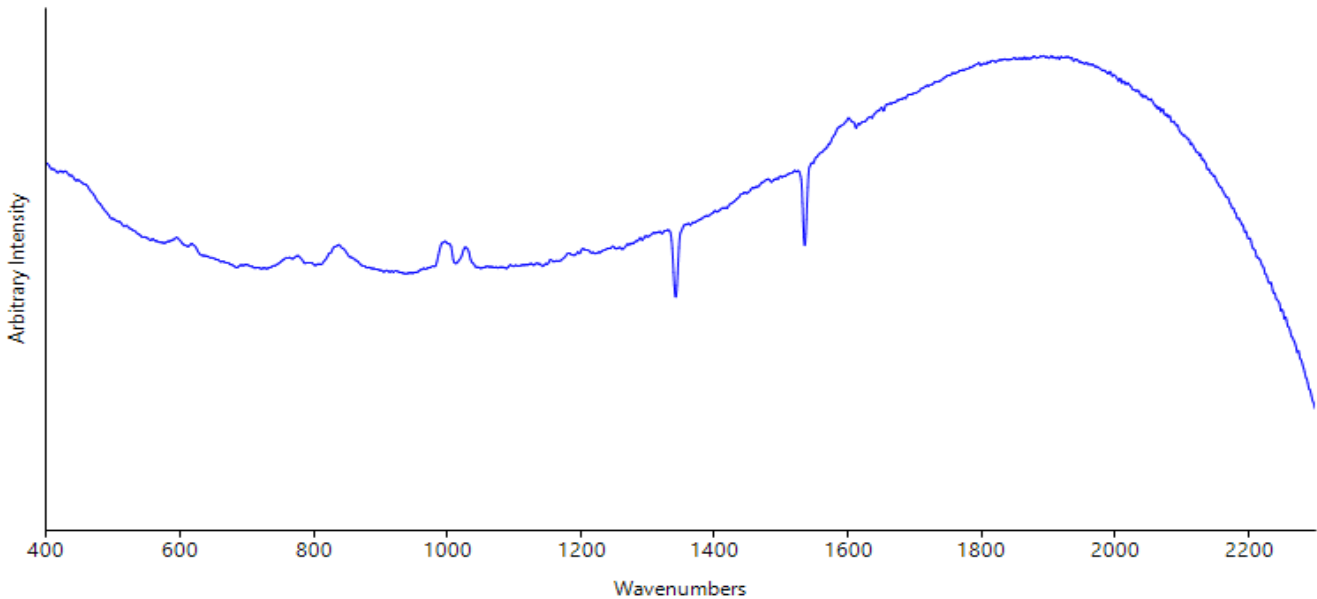

Mixture Identification Results

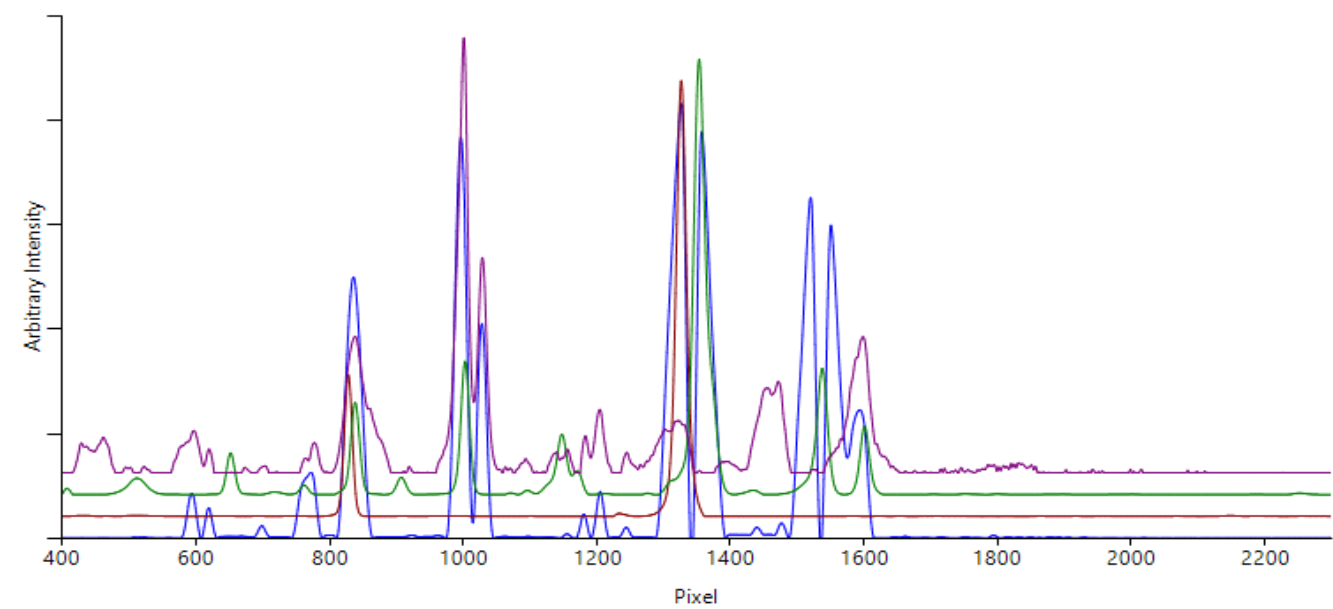

■ Scan 00032 ■ Sodium Nitrite ■ 1,3-Dinitrobenzene ■ 4-ANPP PSERS-Ag 1e-4				
Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Sodium Nitrite	Chemical	Illicit v41, Version: 41	26%
Precursor	1,3-Dinitrobenzene	Explosive	Explosives, Version: 1	25%
Unknown	4-ANPP PSERS-Ag 1e-4		NATO SERS, Version: 1	23%