

Sample Report



Sample Metadata

Sample Name	Scan 00039
Hazard Level	Warning
Sample Type	Steroid
Last Modified	2024-03-06 11:48:46-05:00
Created	2024-03-06 11:48:46-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	0.60 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Bottle (Position 3)
Smart Tip Serial Number	6075060600301151

Spectral Data

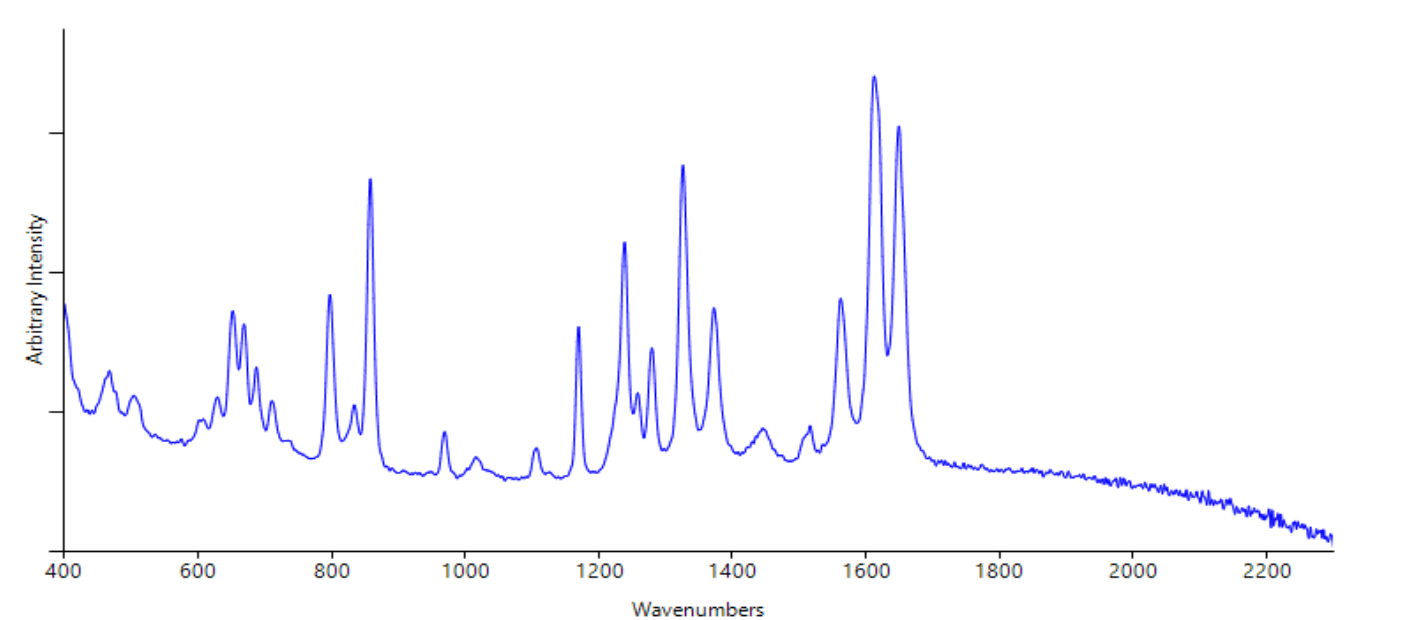


Identification Results

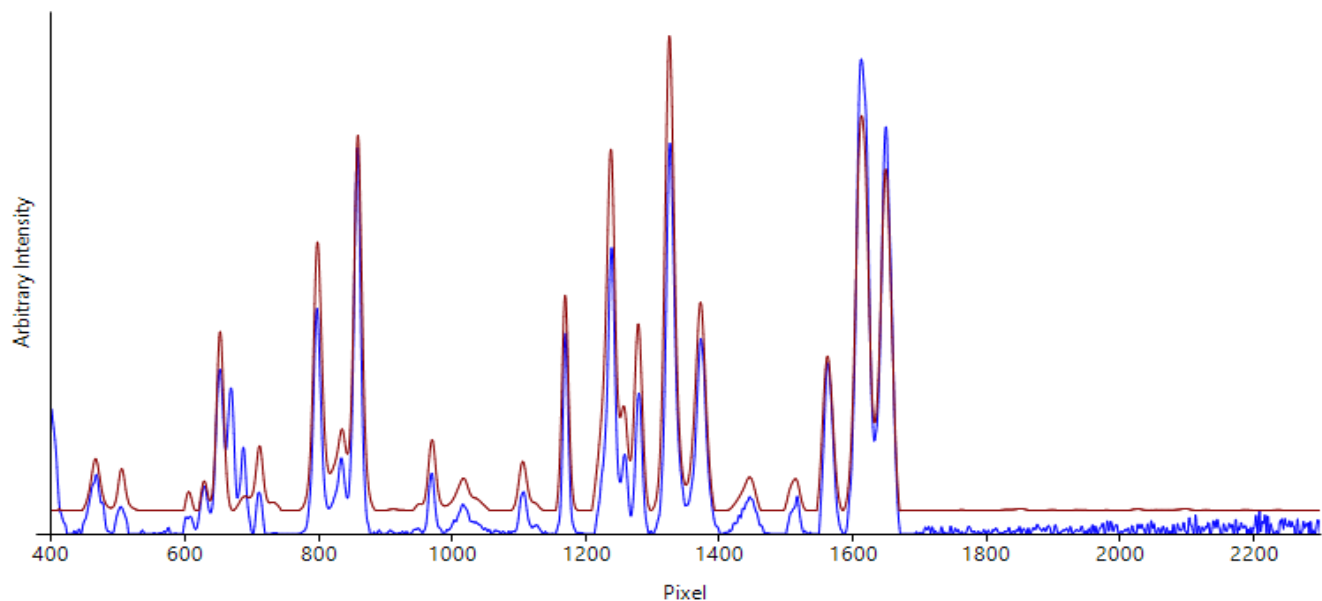

■ Scan 00039 ■ Acetaminophen

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Acetaminophen	USP/Pharmaceutical	0.91	Illicit v41, Version: 41

Mixture Identification Results

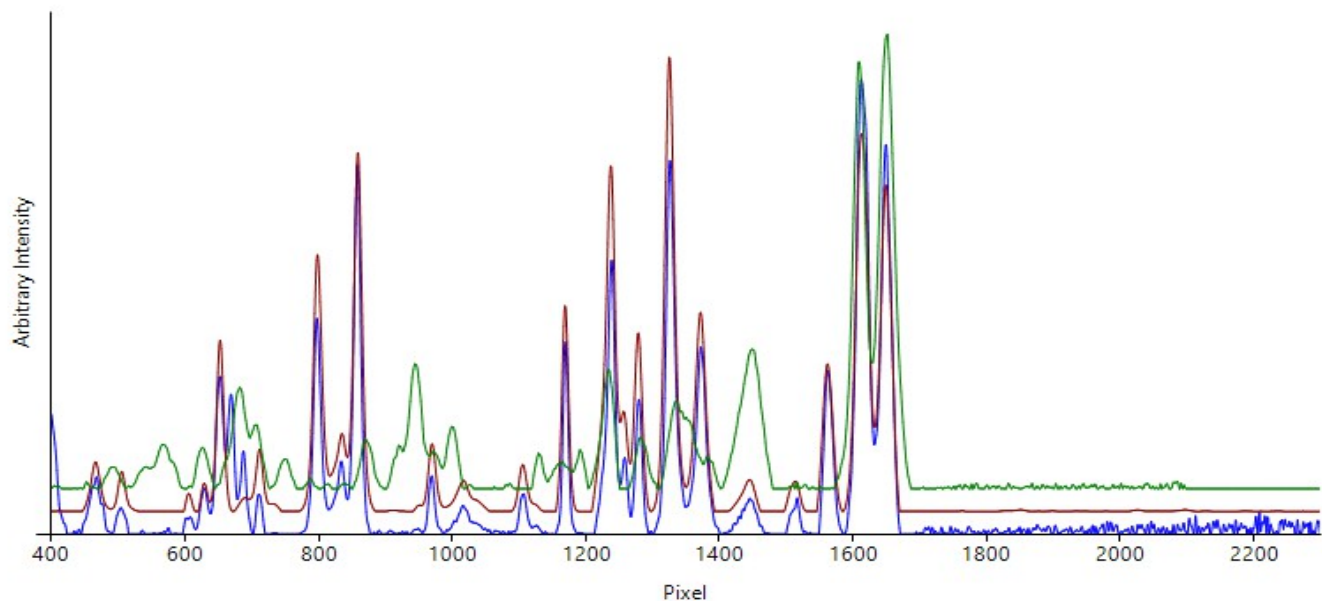

■ Scan 00039 ■ Acetaminophen ■ Methyltestosterone

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Acetaminophen	USP/Pharmaceutical	Illicit v41, Version: 41	63%
Warning	Methyltestosterone	Steroid	Illicit v41, Version: 41	14%