

Sample Report



Sample Metadata

Sample Name	Scan 00040
Hazard Level	Clear
Sample Type	USP/Pharmaceutical, Chemical
Last Modified	2024-03-06 11:50:39-05:00
Created	2024-03-06 11:50:39-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	10.00 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Bottle (Position 3)
Smart Tip Serial Number	6075060600301151

Spectral Data

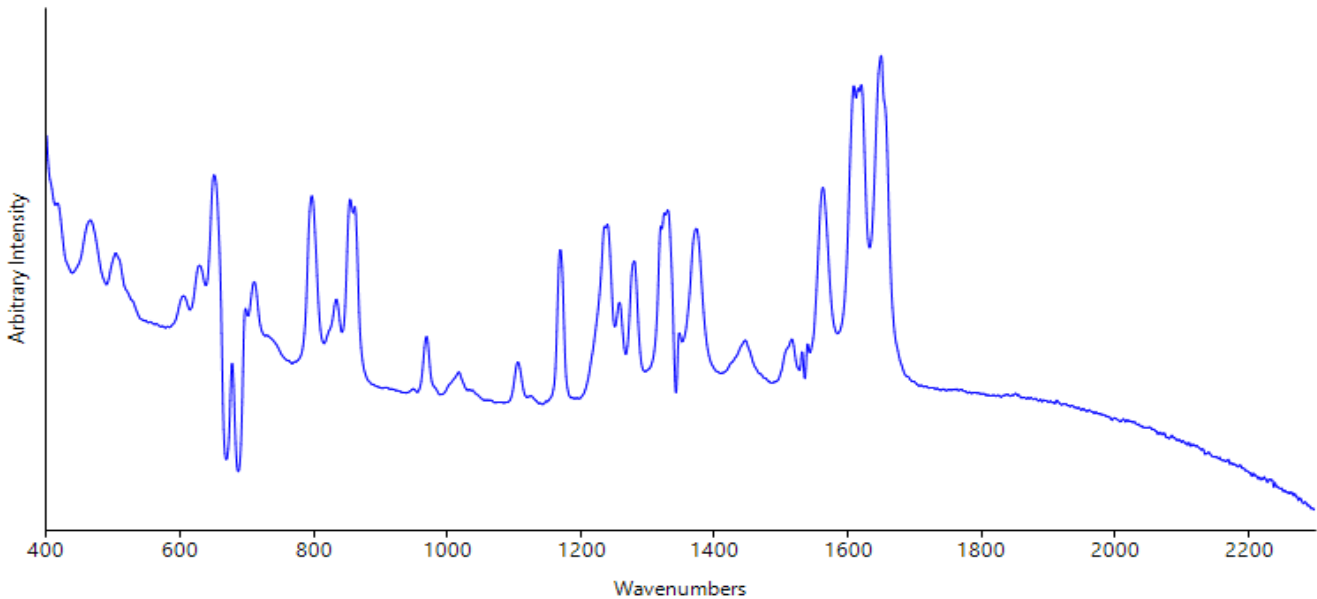


Identification Results

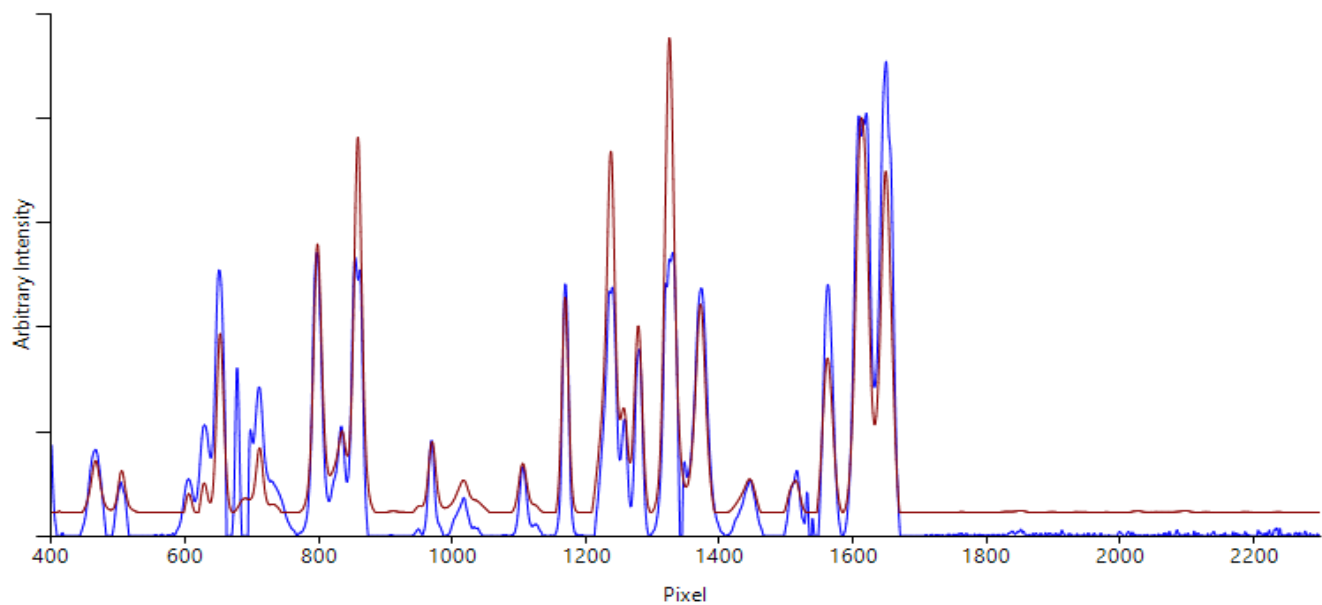

■ Scan 00040 ■ Acetaminophen

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Acetaminophen	USP/Pharmaceutical	0.85	Illicit v41, Version: 41

Mixture Identification Results

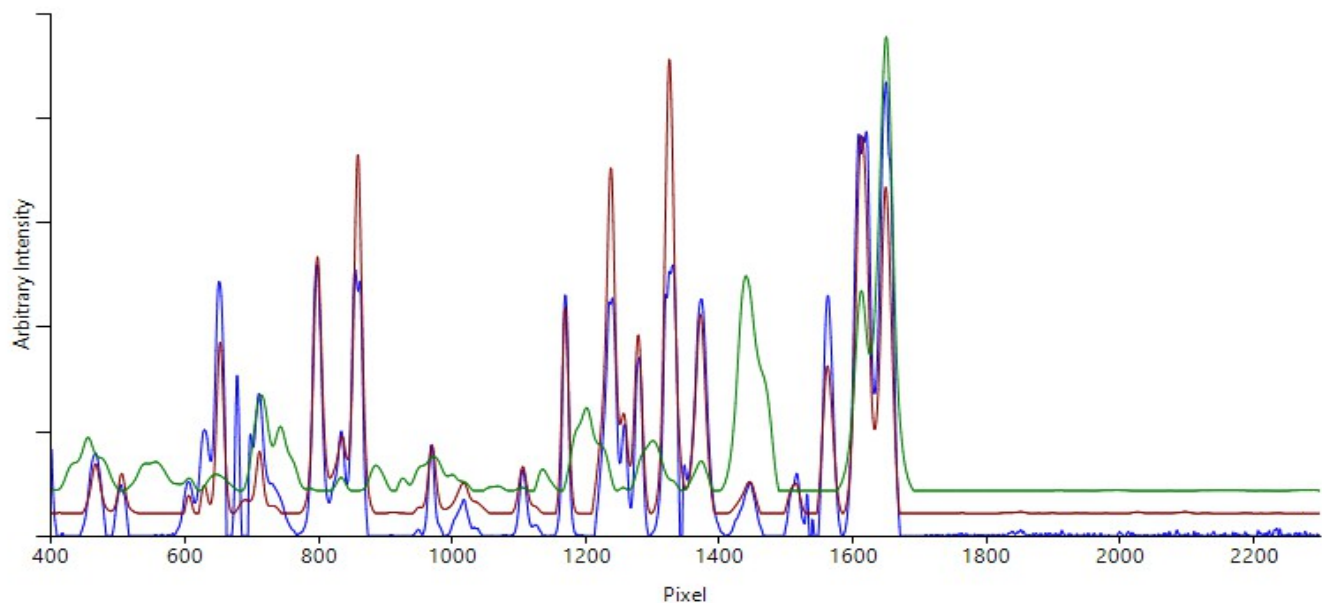

■ Scan 00040 ■ Acetaminophen ■ Gum Rosin

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Acetaminophen	USP/Pharmaceutical	Illicit v41, Version: 41	54%
Clear	Gum Rosin	Chemical	Illicit v41, Version: 41	19%