

Sample Report



Sample Metadata

Sample Name	Scan 00064
Hazard Level	Precursor
Sample Type	Illicit Drug
Last Modified	2024-03-06 14:16:28-05:00
Created	2024-03-06 14:16:28-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	3.38 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

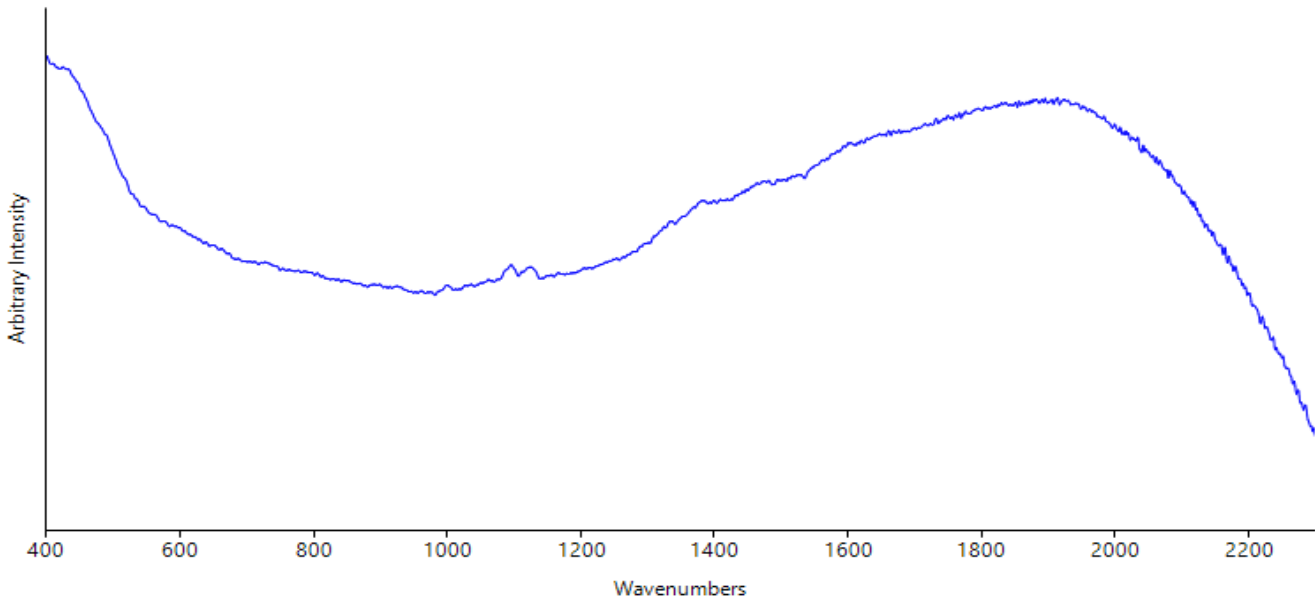

Mixture Identification Results

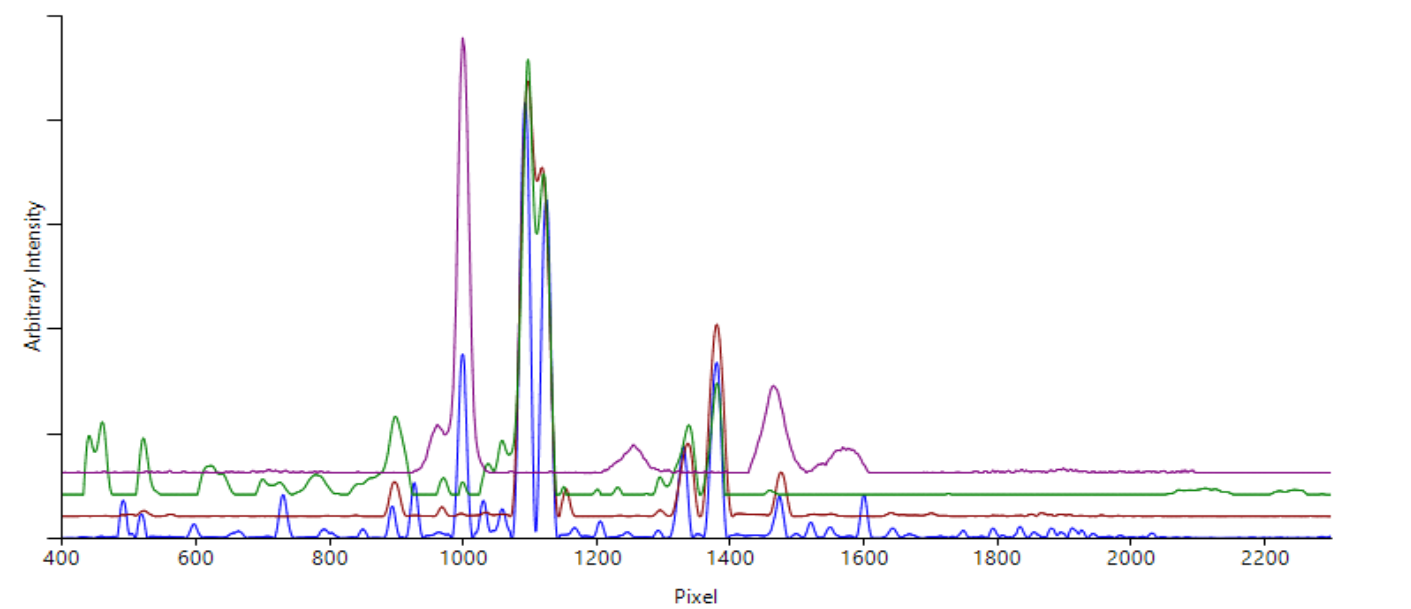

	■ Scan 00064 ■ Microcrystalline Cellulose ■ Cellulose ■ Methylamine HCl			
Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Warning	Microcrystalline Cellulose	Chemical	Illicit v41, Version: 41	33%
Warning	Cellulose	USP/Pharmaceutical	Illicit v41, Version: 41	26%
Precursor	Methylamine HCl	Illicit Drug	Illicit v41, Version: 41	25%