

Sample Report



Sample Metadata

Sample Name	Scan 00074
Hazard Level	Warning
Sample Type	Steroid
Last Modified	2024-03-06 14:35:29-05:00
Created	2024-03-06 14:35:29-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	1.61 s
Auto Integration	On
Averages	1
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

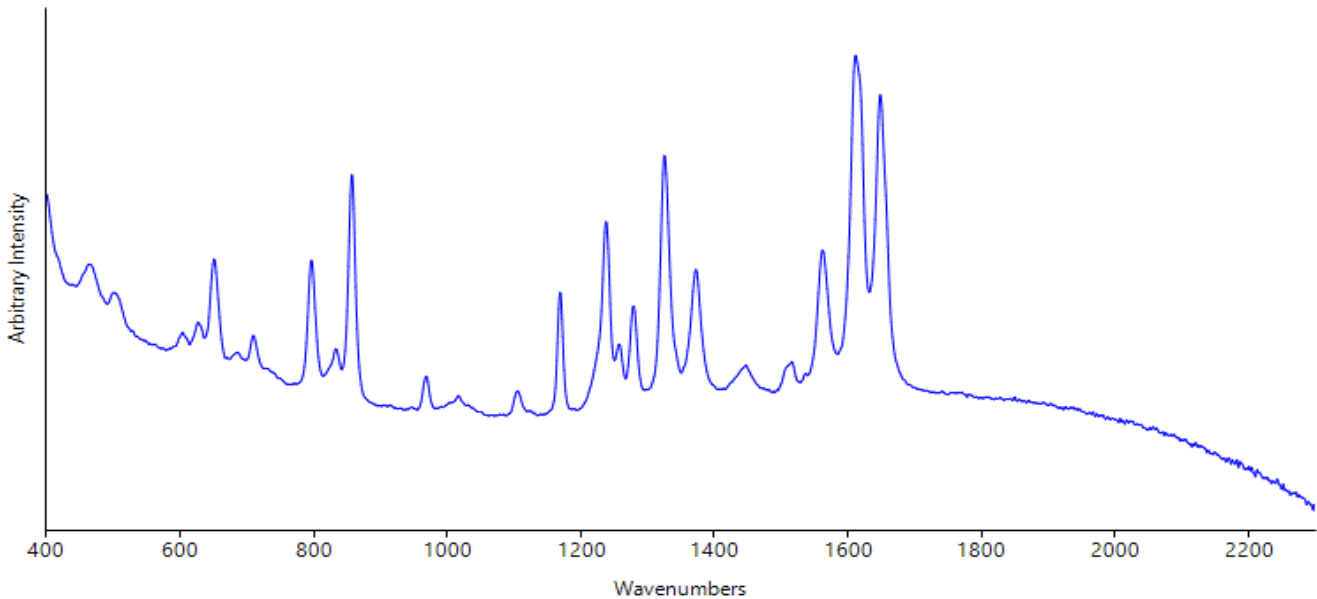


Identification Results

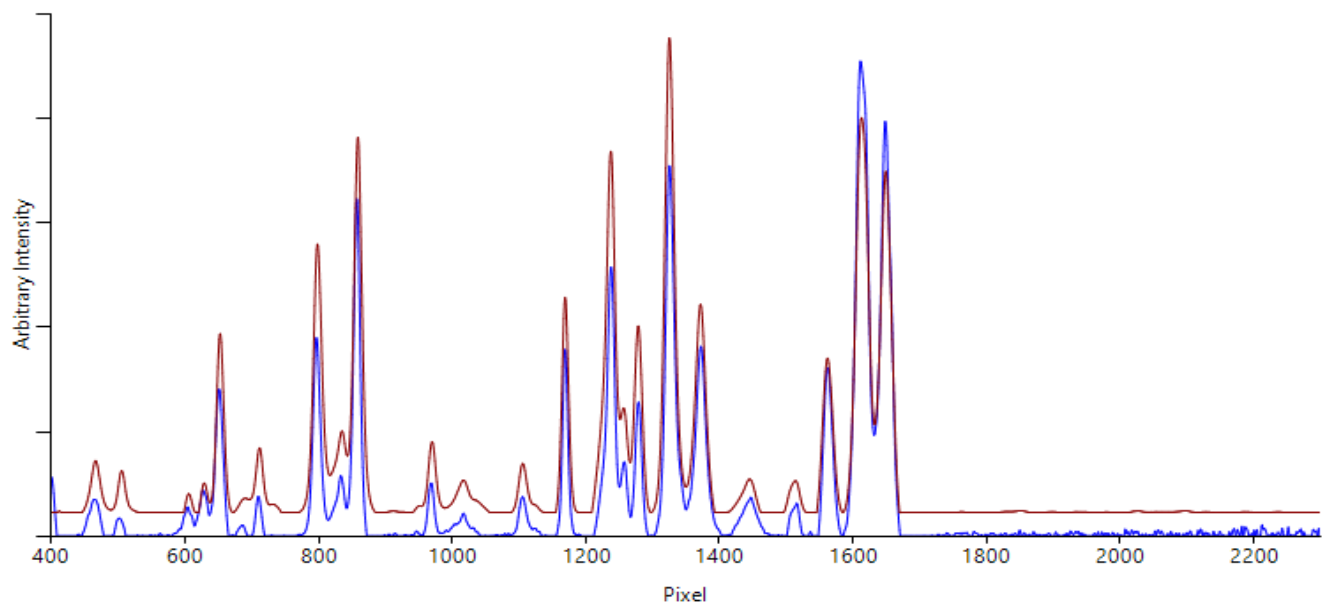

■ Scan 00074 ■ Acetaminophen

Hazard Level	Match	Sample Type	Match Score	Result Library
Clear	Acetaminophen	USP/Pharmaceutical	0.92	Illicit v41, Version: 41

Mixture Identification Results

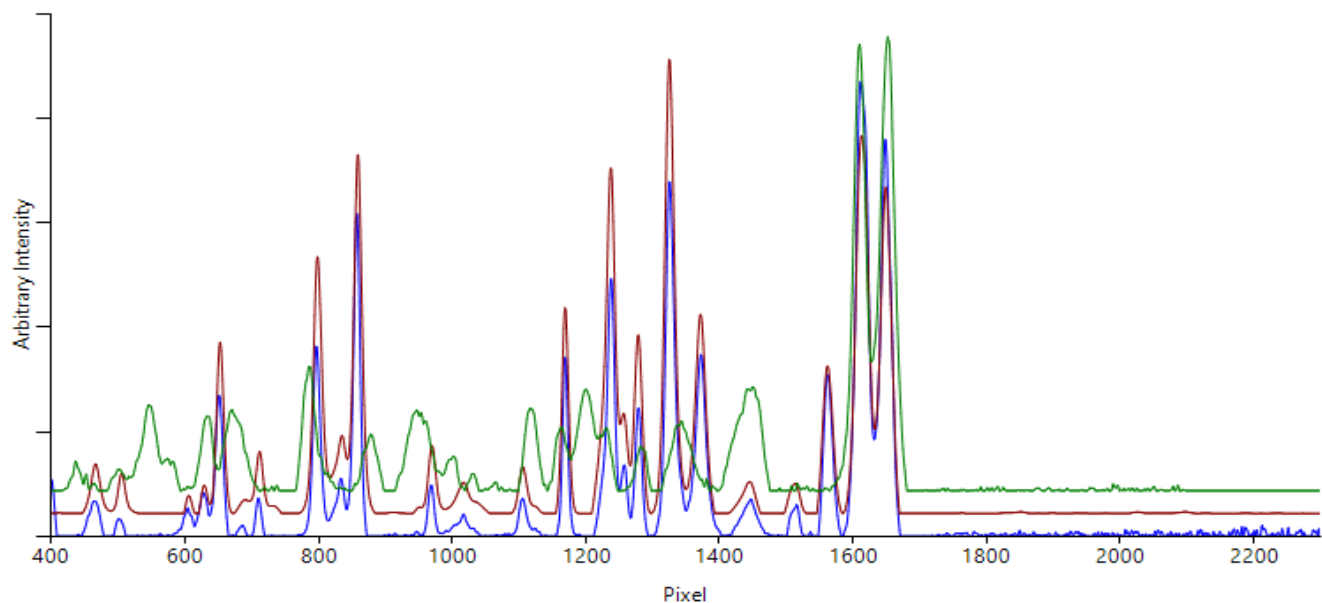

■ Scan 00074 ■ Acetaminophen ■ Isotestosterone

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Acetaminophen	USP/Pharmaceutical	Illicit v41, Version: 41	68%
Warning	Isotestosterone	Steroid	Illicit v41, Version: 41	19%