

Sample Report



Sample Metadata

Sample Name	Scan 00143
Hazard Level	Warning
Sample Type	USP/Pharmaceutical
Last Modified	2024-03-07 11:46:23-05:00
Created	2024-03-07 11:46:23-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	5.41 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

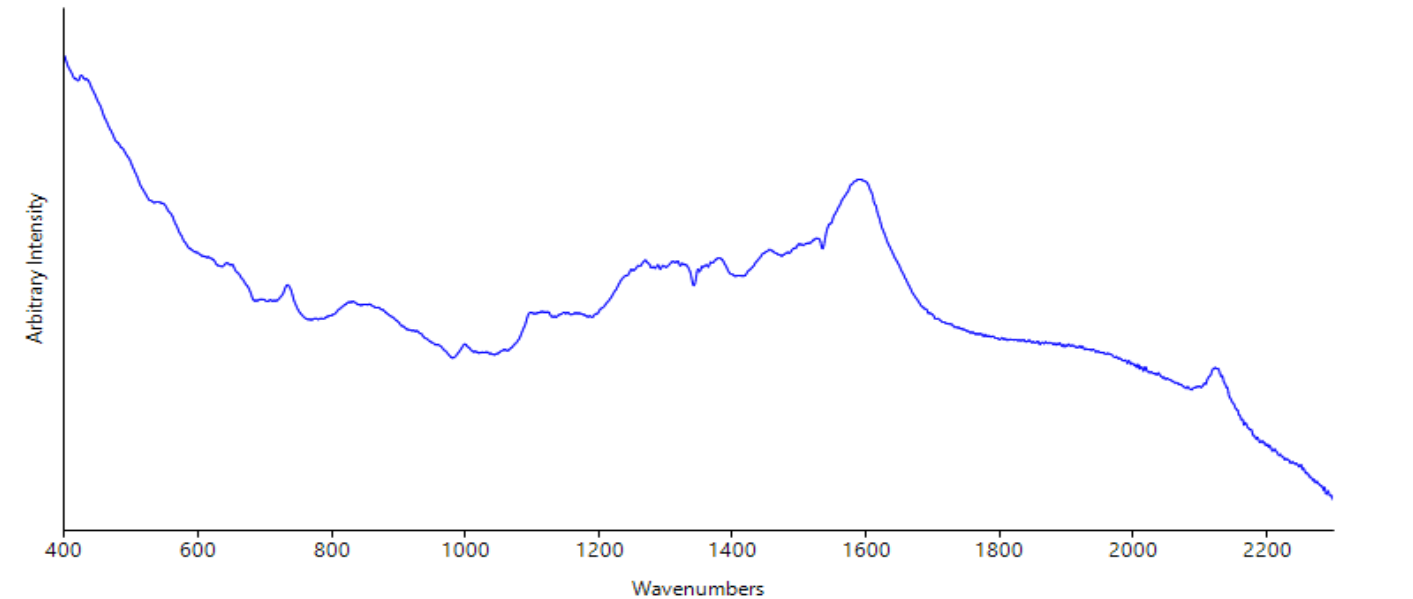

Mixture Identification Results

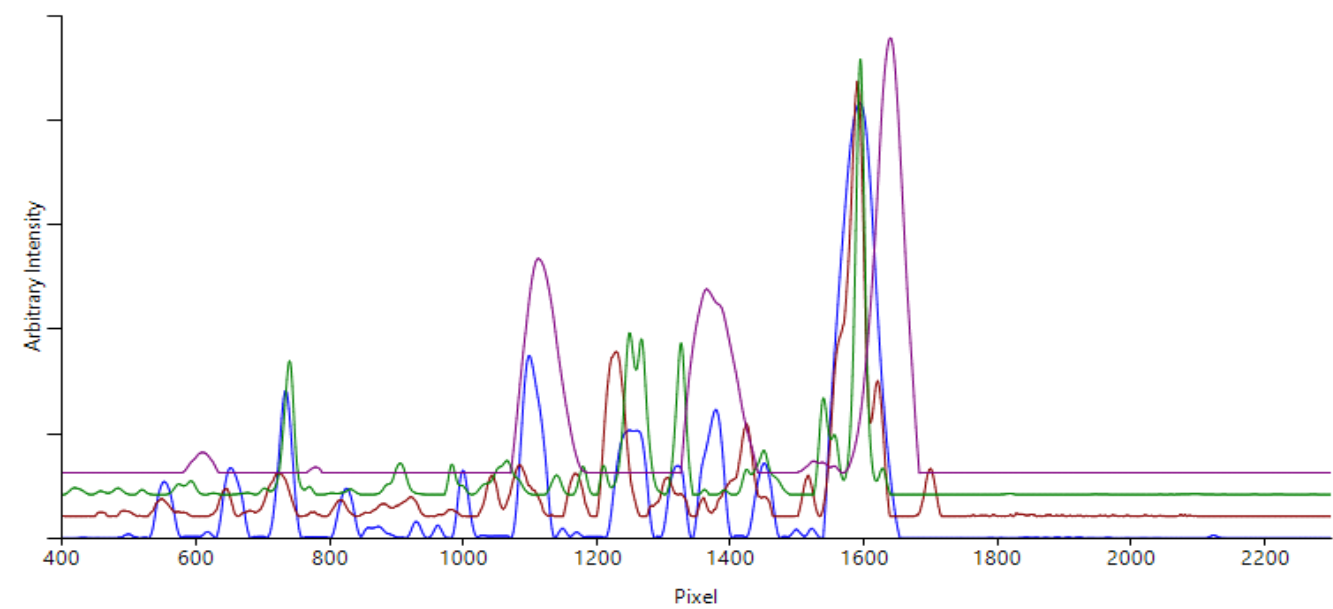

■ Scan 00143 ■ Vardenafil HCl ■ Metoclopramide HCl ■ Ammonium Hydroxide				
Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Warning	Vardenafil HCl	USP/Pharmaceutical	Illicit v41, Version: 41	54%
Clear	Metoclopramide HCl	USP/Pharmaceutical	Illicit v41, Version: 41	19%
Clear	Ammonium Hydroxide	Chemical	Illicit v41, Version: 41	12%