

Sample Report



Sample Metadata

Sample Name	Scan 00145
Hazard Level	Alarm
Sample Type	Illicit Drug
Last Modified	2024-03-07 11:49:58-05:00
Created	2024-03-07 11:49:58-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	2.64 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

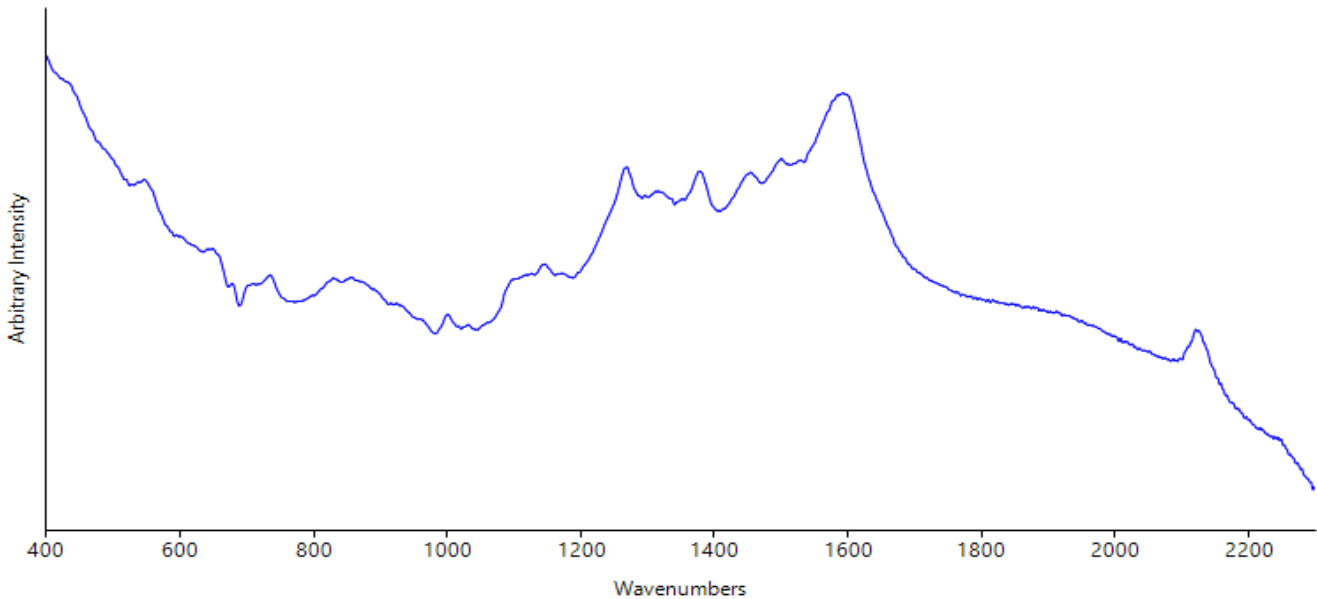

Mixture Identification Results

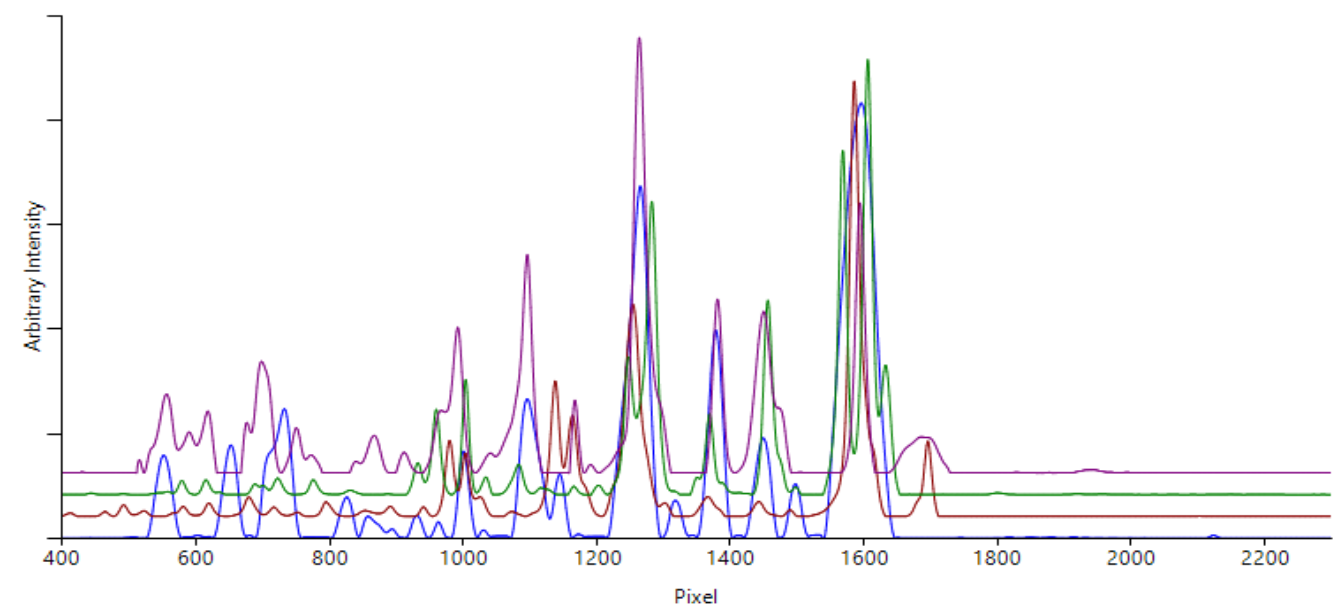

■ Scan 00145

■ BZO-HEXOXIZID

■ Ensulizole

■ Lidocaine N-oxide

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Alarm	BZO-HEXOXIZID	Illicit Drug	Illicit v41, Version: 41	40%
Clear	Ensulizole	USP/Pharmaceutical	Illicit v41, Version: 41	30%
Clear	Lidocaine N-oxide	USP/Pharmaceutical	Illicit v41, Version: 41	12%