

Sample Report



Sample Metadata

Sample Name	Scan 00148
Hazard Level	Clear
Sample Type	USP/Pharmaceutical, Chemical
Last Modified	2024-03-07 11:55:43-05:00
Created	2024-03-07 11:55:43-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	3.23 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

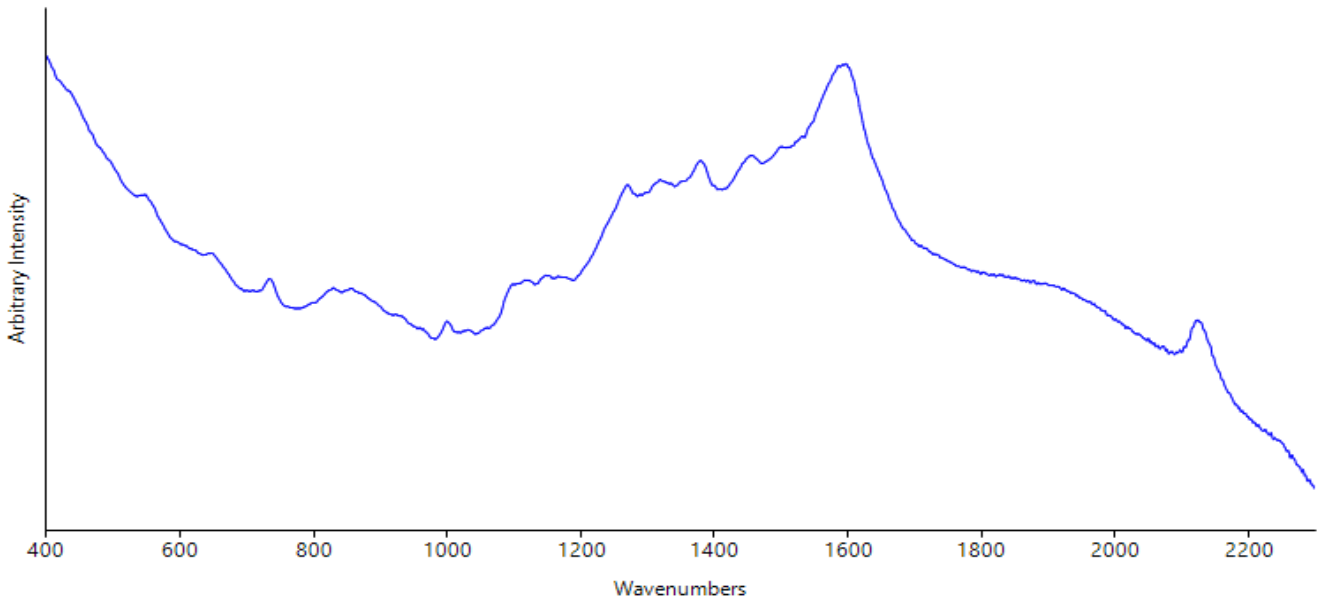

Mixture Identification Results

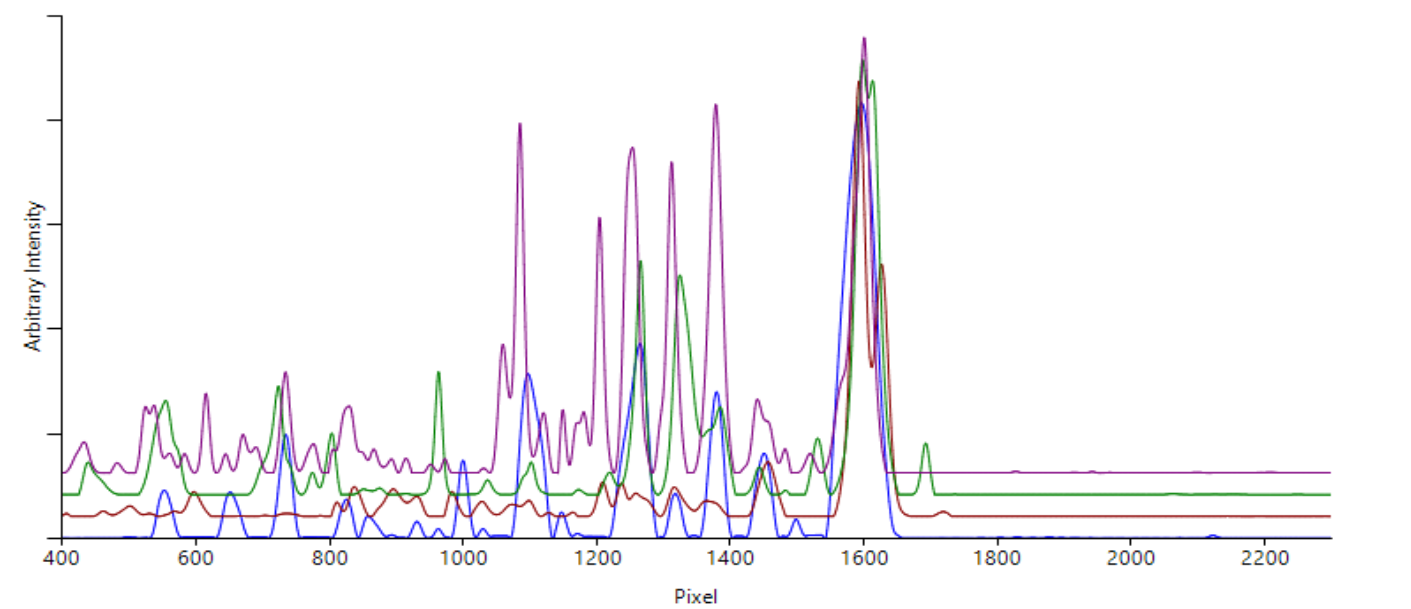

	■ Scan 00148 ■ Tylosin Tartrate ■ Gallic Acid ■ Flunixin Meglumine			
Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Clear	Tylosin Tartrate	USP/Pharmaceutical	Illicit v41, Version: 41	45%
Clear	Gallic Acid	Chemical	Illicit v41, Version: 41	23%
Clear	Flunixin Meglumine	USP/Pharmaceutical	Illicit v41, Version: 41	12%