

Sample Report



Sample Metadata

Sample Name	Scan 00160
Hazard Level	Unknown
Last Modified	2024-03-07 14:43:41-05:00
Created	2024-03-07 14:43:41-05:00


Instrument

Serial Number	192601100601640
Firmware Package	8.0.3.56
Last Calibration	2024-03-06 10:11:28-05:00
Last System Suitability Test	Pass, 2024-03-06 10:11:38-05:00


Acquisition Parameters

Operating Procedure Name	Default Procedure
Operating Procedure Version	1
Integration Time	2.71 s
Auto Integration	On
Averages	3
Laser Power	5
Smart Tip Type	Intelligent UA, Surface (Position 1)
Smart Tip Serial Number	6075060600301151

Spectral Data

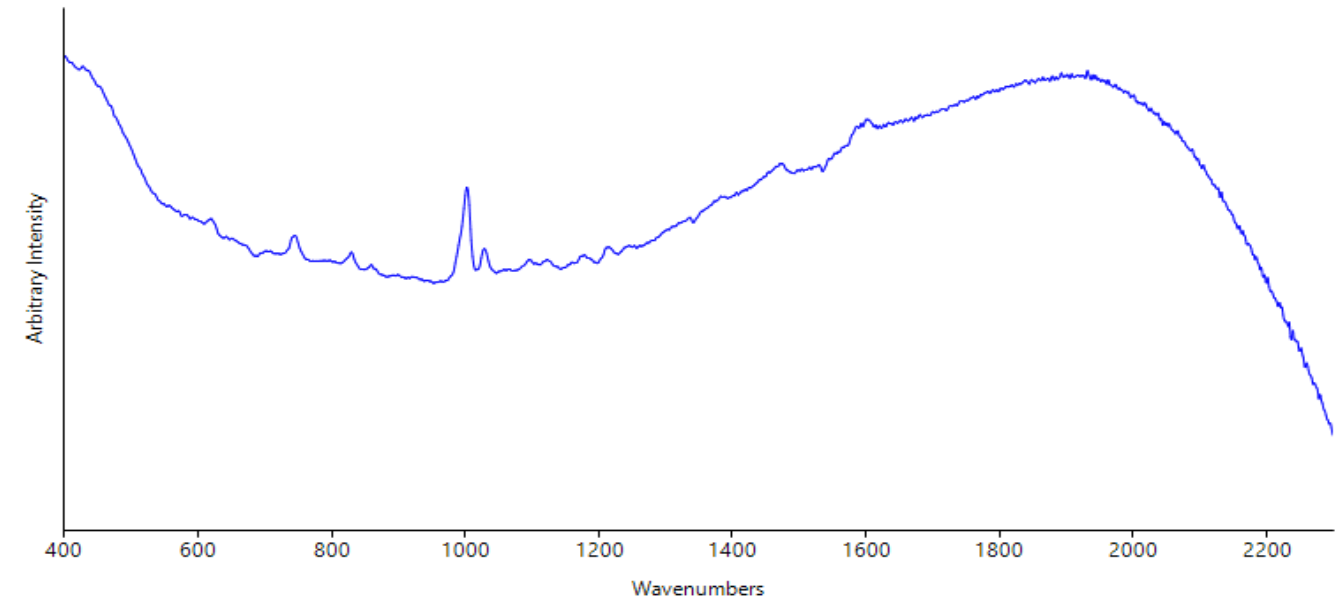


Identification Results

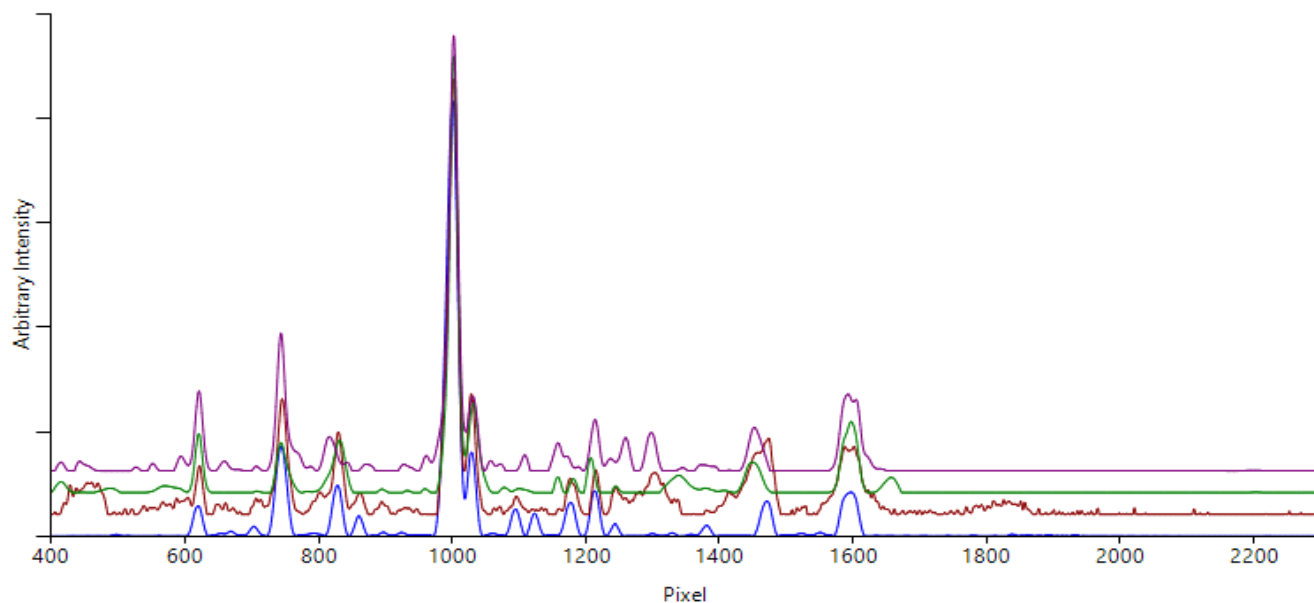

■ Scan 00160
 ■ Benzyl Fentanyl PSERS-Ag 1e-3
 ■ Diampromide (hydrochloride)
 ■ (±)-cis-Isomenthyl (hydrochloride)

Hazard Level	Match	Sample Type	Match Score	Result Library
Unknown	Benzyl Fentanyl PSERS-Ag 1e-3		0.90	NATO SERS, Version: 1
Alarm	Diampromide (hydrochloride)	Illicit Drug	0.88	Illicit v41, Version: 41
Alarm	(±)-cis-Isomenthyl (hydrochloride)	Illicit Drug	0.87	Illicit v41, Version: 41

Mixture Identification Results

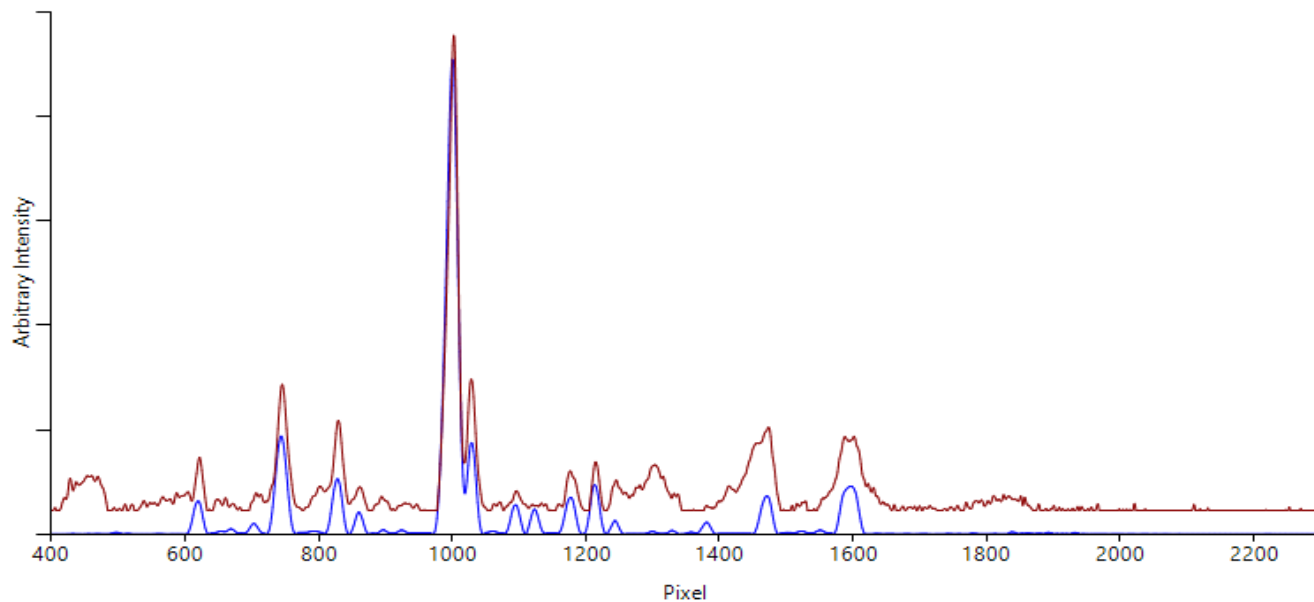

■ Scan 00160
 ■ Benzyl Fentanyl PSERS-Ag 1e-3

Hazard Level	Match	Sample Type	Source Library	Spectral Weight %
Unknown	Benzyl Fentanyl PSERS-Ag 1e-3		NATO SERS, Version: 1	95%