



Paired differences and conditional intervals

A Individual spectra

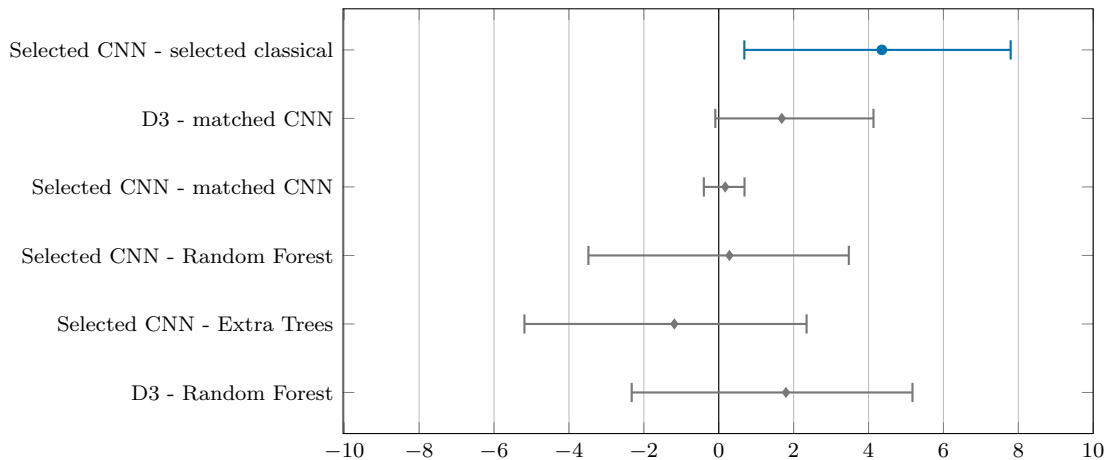

B Combined sample predictions

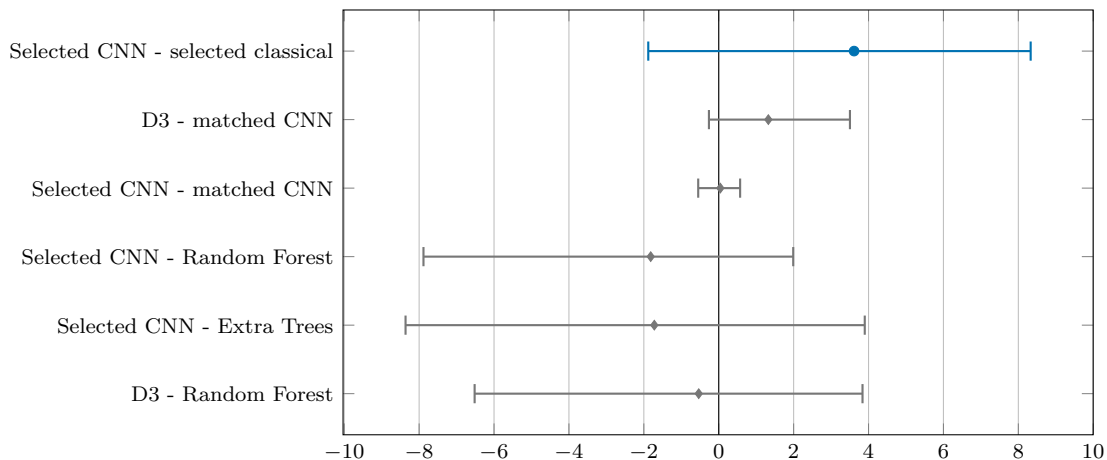

Balanced accuracy difference (percentage points)

(P: M01 selected pair; S: other contrasts). Source-only selection; 69 physical masters, 557 held spectra, 13 station-instrument domains, ten instruments. RQ-P01 primary/secondary contrasts; PP-U-MIN, 400-1800 cm^{-1} . Points are fixed balanced-accuracy differences; lines are 95% percentile intervals from 10,000 shared master/instrument weighted draws. Conditional on saved fits and observed support; secondary intervals are not multiplicity-adjusted. M01 uses individual spectra; M06 combines predictions, not spectra. Each contrast uses its own paired context support.