



Filename: 2024-03-04 - 16.09.21.D5000

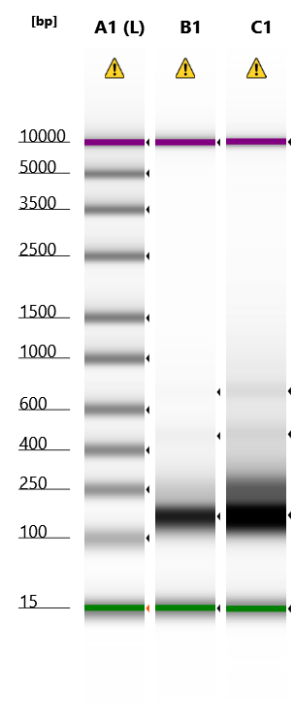

Default image (Contrast 100%)

Sample Info


Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	48.9	Ladder		Caution! Expired ScreenTape device; Ladder
B1	23.5	M60		Caution! Expired ScreenTape device
C1	71.8	M72		Caution! Expired ScreenTape device

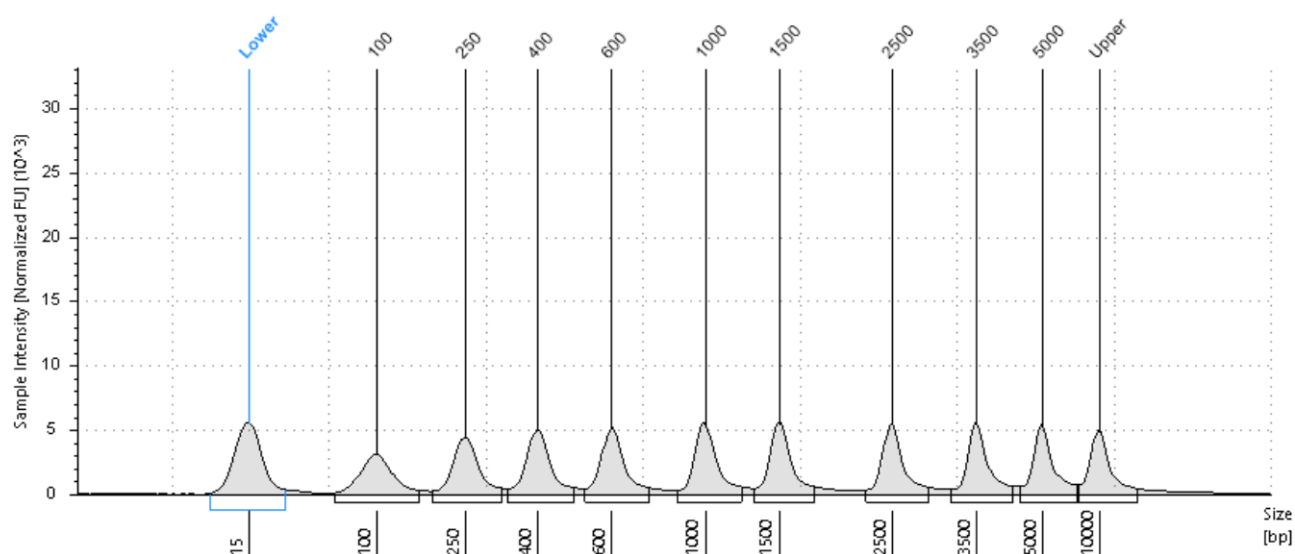A1: Ladder**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	48.9	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.61	-	678	-		Lower Marker
100	4.79	-	73.7	9.80		
250	5.35	-	32.9	10.94		
400	5.68	-	21.8	11.61		
600	5.67	-	14.5	11.60		
1000	5.82	-	8.96	11.91		
1500	5.60	-	5.74	11.46		
2500	5.38	-	3.31	11.00		
3500	5.41	-	2.38	11.08		
5000	5.18	-	1.59	10.60		
10000	3.25	3.25	0.500	-		Upper Marker

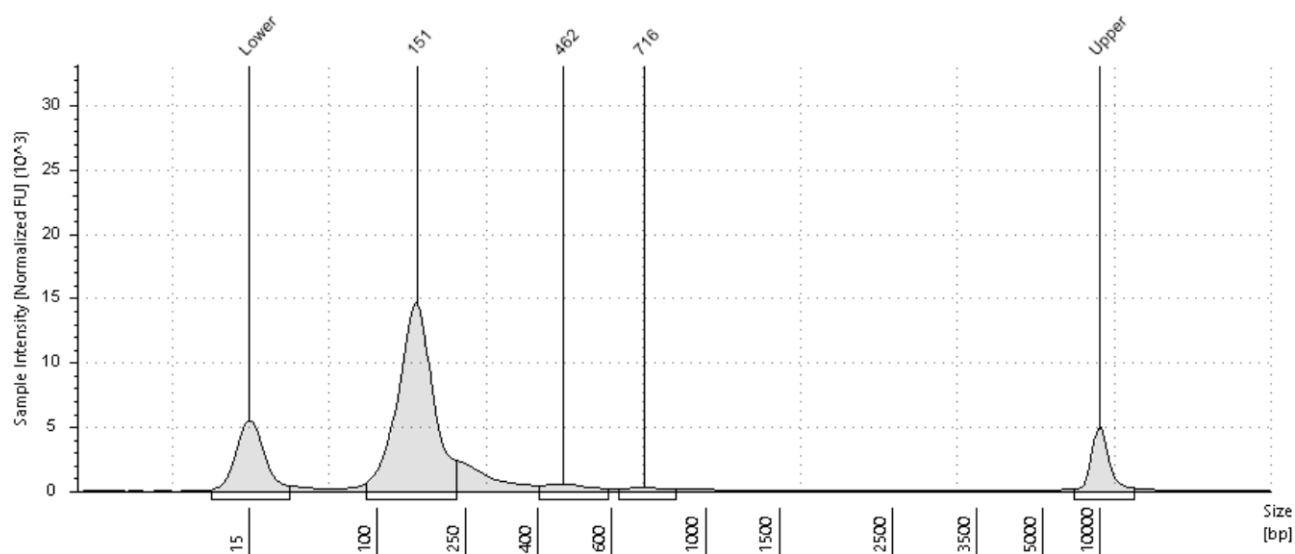
B1: M60**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	23.5	M60	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	5.84	-	599	-		Lower Marker
151	22.0	-	224	93.56		
462	1.05	-	3.48	4.45		
716	0.466	-	1.00	1.98		
10000	3.25	3.25	0.500	-		Upper Marker

C1: M72

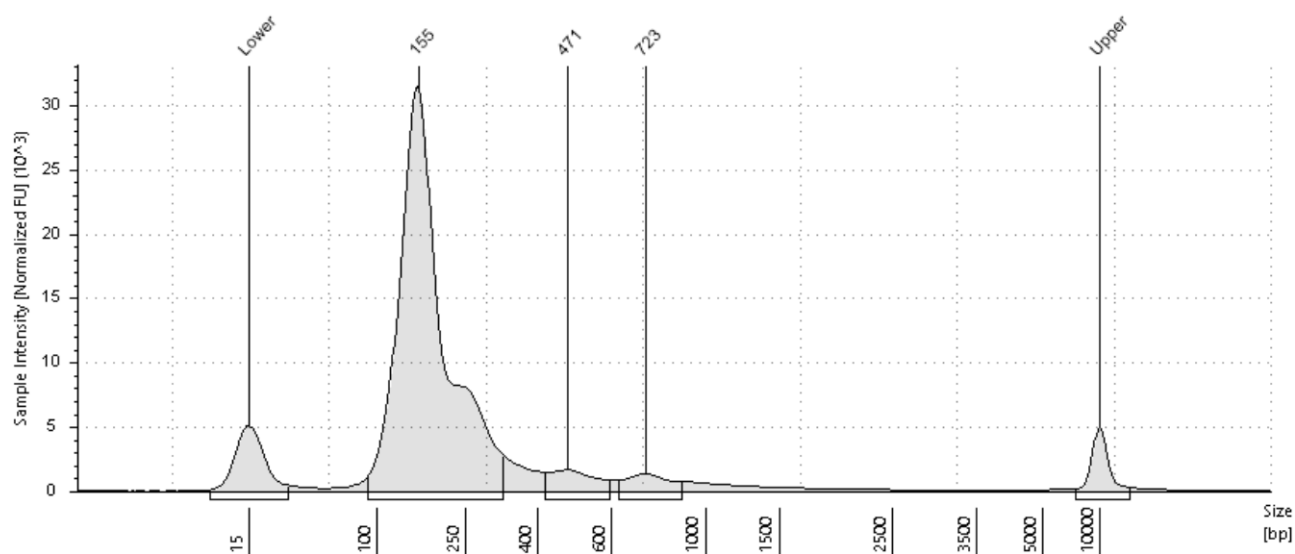

Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
C1	71.8	M72	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.20	-	636	-		Lower Marker
155	65.5	-	651	91.25		
471	3.56	-	11.6	4.95		
723	2.73	-	5.80	3.80		
10000	3.25	3.25	0.500	-		Upper Marker