


Filename: 2024-03-31 - 14.05.45.D5000

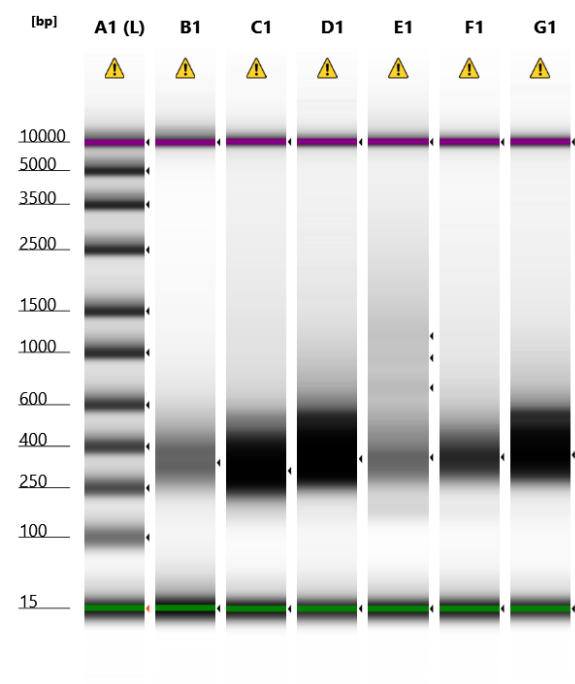


Default image (Contrast 100%)

Sample Info

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	47.2	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1	4.97	6	⚠	Caution! Expired ScreenTape device
C1	36.8	7	⚠	Caution! Expired ScreenTape device
D1	47.8	107	⚠	Caution! Expired ScreenTape device
E1	18.4	108	⚠	Caution! Expired ScreenTape device
F1	16.6	110	⚠	Caution! Expired ScreenTape device
G1	37.3	113	⚠	Caution! Expired ScreenTape device

A1: Ladder

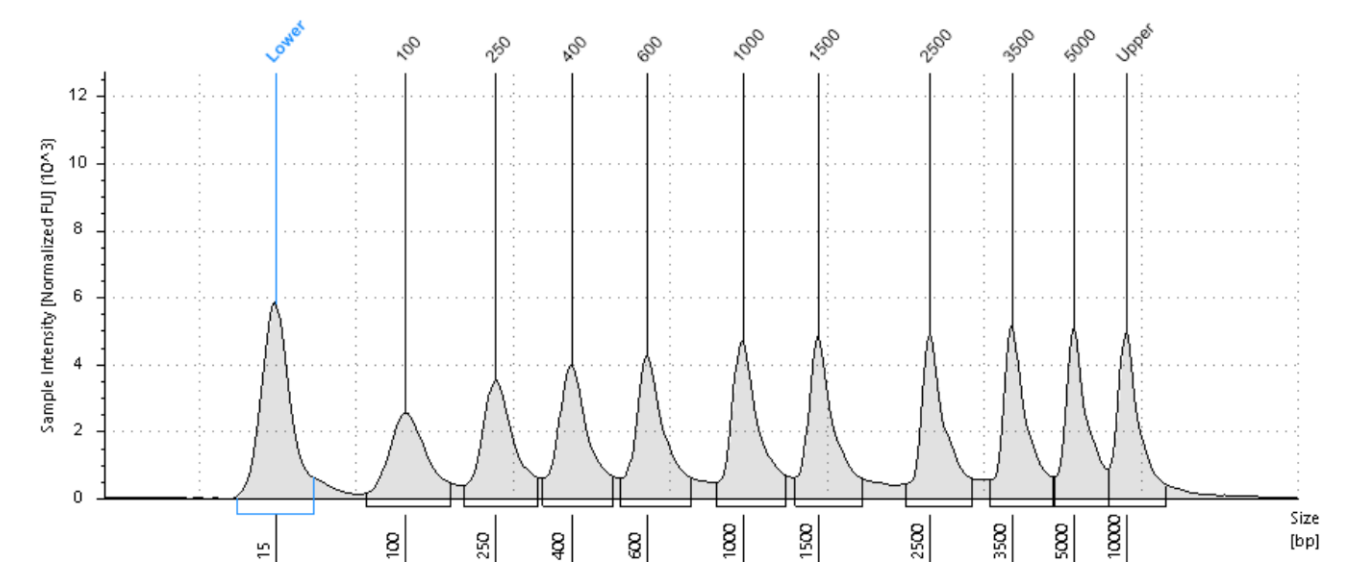


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	47.2	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.51	-	668	-		Lower Marker
100	4.31	-	66.3	9.13		
250	5.01	-	30.9	10.62		
400	5.39	-	20.7	11.43		
600	5.50	-	14.1	11.66		
1000	5.74	-	8.83	12.16		
1500	5.56	-	5.71	11.79		
2500	5.29	-	3.26	11.21		
3500	5.34	-	2.35	11.32		
5000	5.05	-	1.55	10.69		
10000	3.25	3.25	0.500	-		Upper Marker

B1: 6

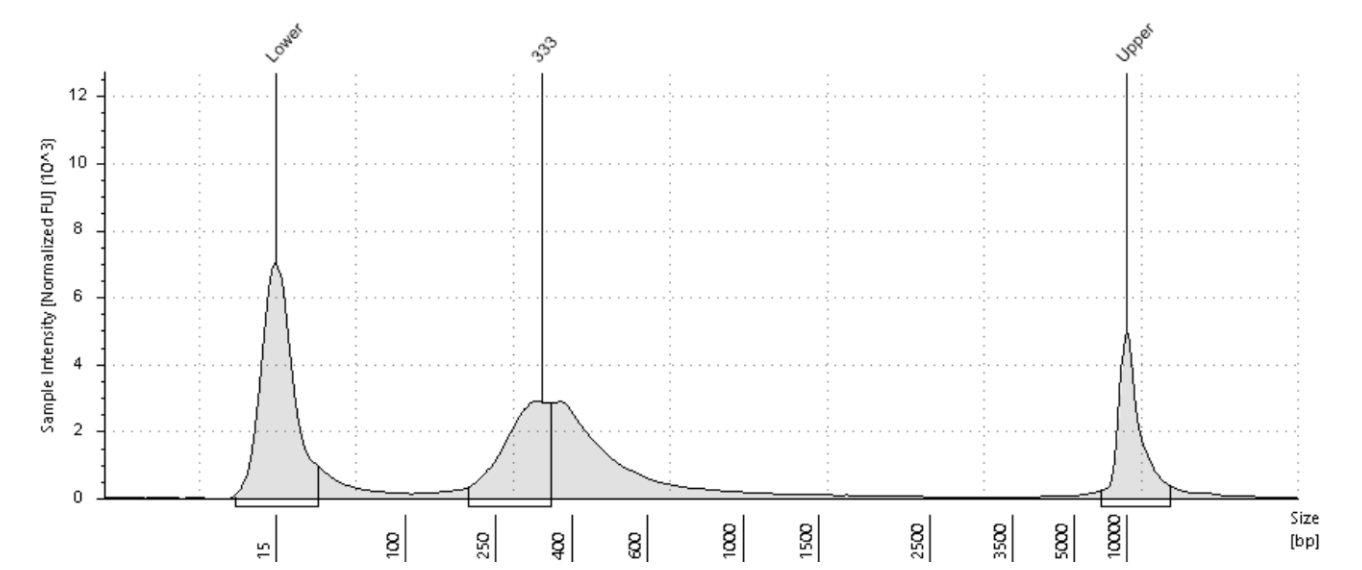


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
B1	4.97	6		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.10	-	728	-		Lower Marker
333	4.97	-	23.0	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C1: 7

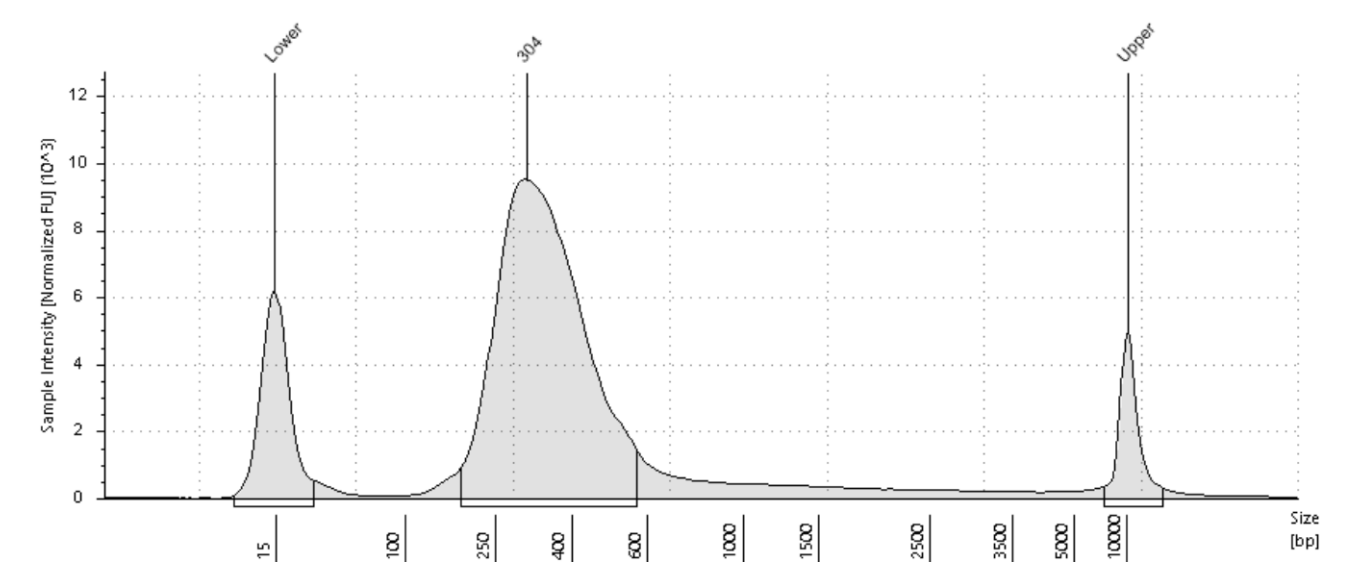


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
C1	36.8	7		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.90	-	708	-		Lower Marker
304	36.8	-	186	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

D1: 107

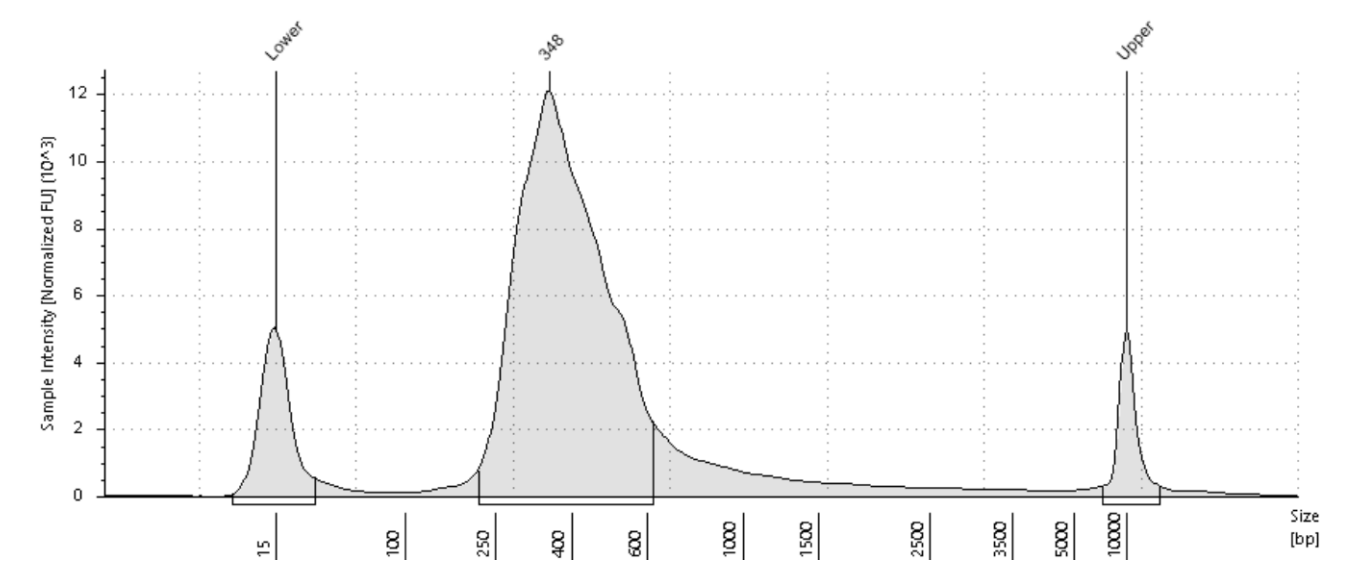


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
D1	47.8	107		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.05	-	621	-		Lower Marker
348	47.8	-	212	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

E1: 108

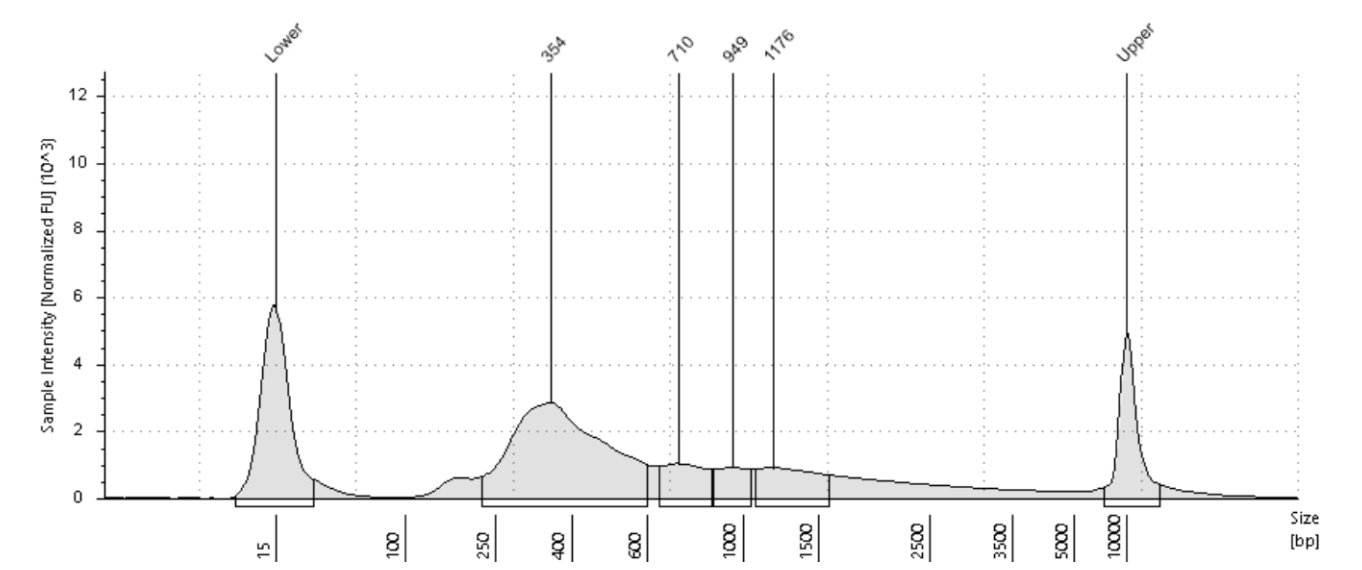


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
E1	18.4	108		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.69	-	686	-		Lower Marker
354	12.3	-	53.6	66.95		
710	2.11	-	4.58	11.47		
949	1.43	-	2.32	7.76		
1176	2.54	-	3.33	13.82		
10000	3.25	3.25	0.500	-		Upper Marker

F1: 110

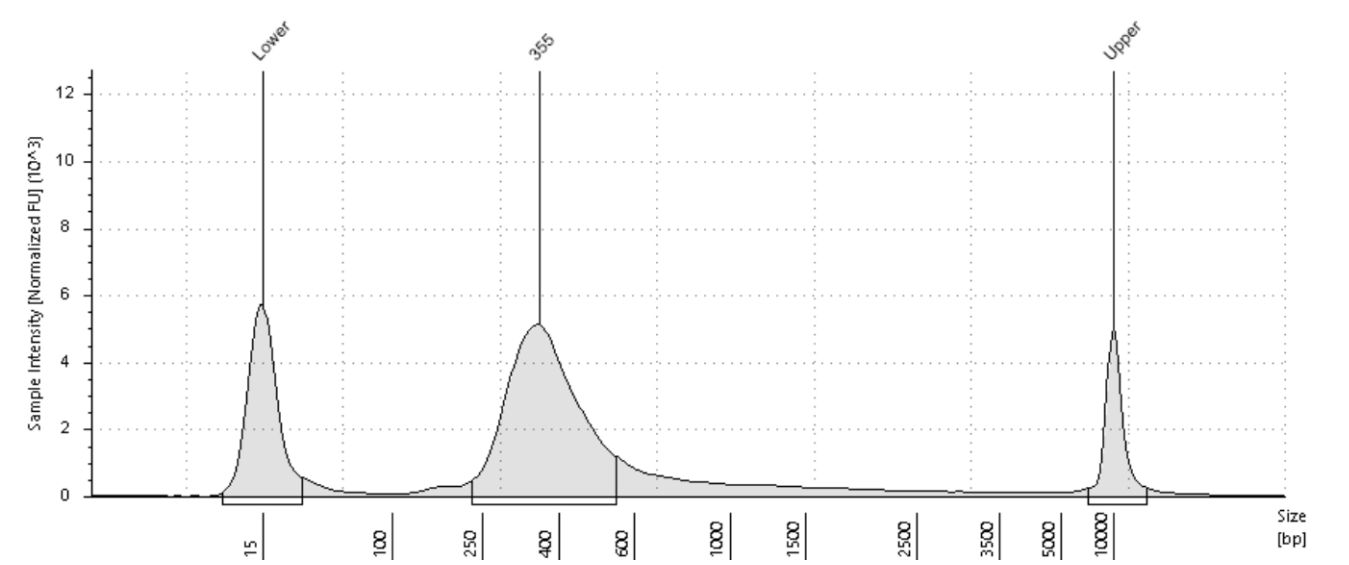


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
F1	16.6	110		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.65	-	682	-		Lower Marker
355	16.6	-	71.8	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

**G1: 113**

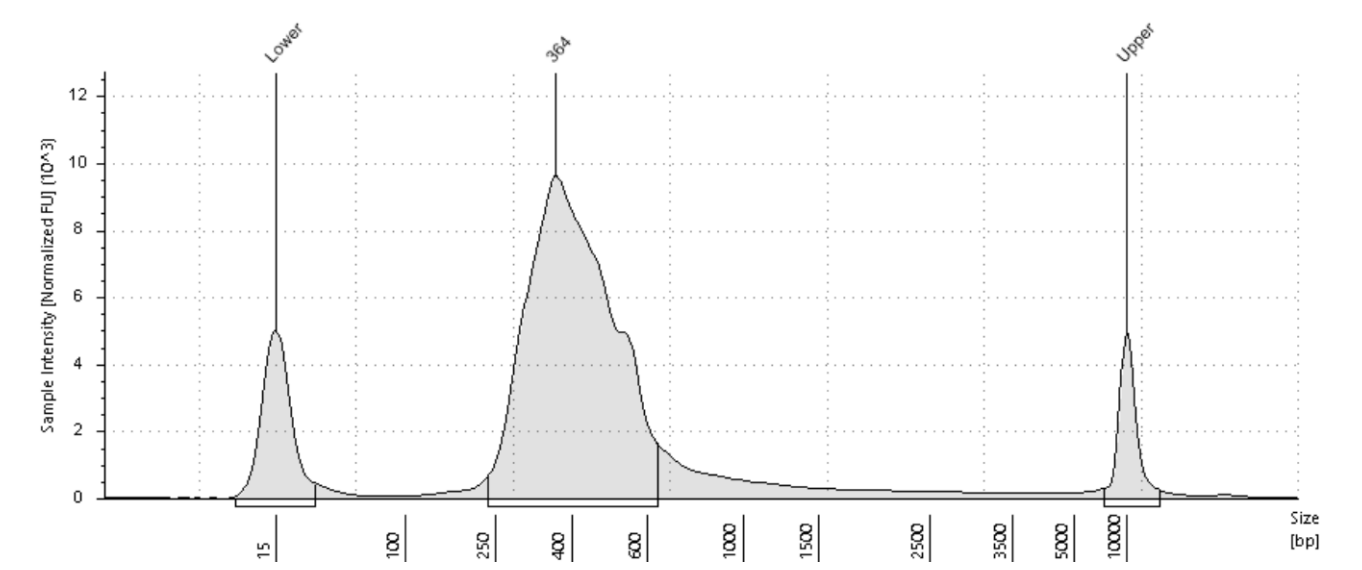

**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
G1	37.3	113		Caution! Expired ScreenTape device

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	5.87	-	602	-		Lower Marker
364	37.3	-	157	100.00		
10000	3.25	3.25	0.500	-		Upper Marker