


Filename: 2024-02-15 - 15.34.31.D5000

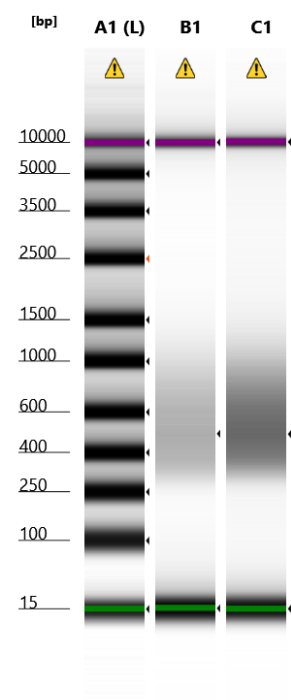


Default image (Contrast 100%)

Sample Info

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	94.3	Ladder		Caution! Expired ScreenTape device; Ladder
B1	3.99	M60		Caution! Expired ScreenTape device
C1	15.9	M72		Caution! Expired ScreenTape device

A1: Ladder

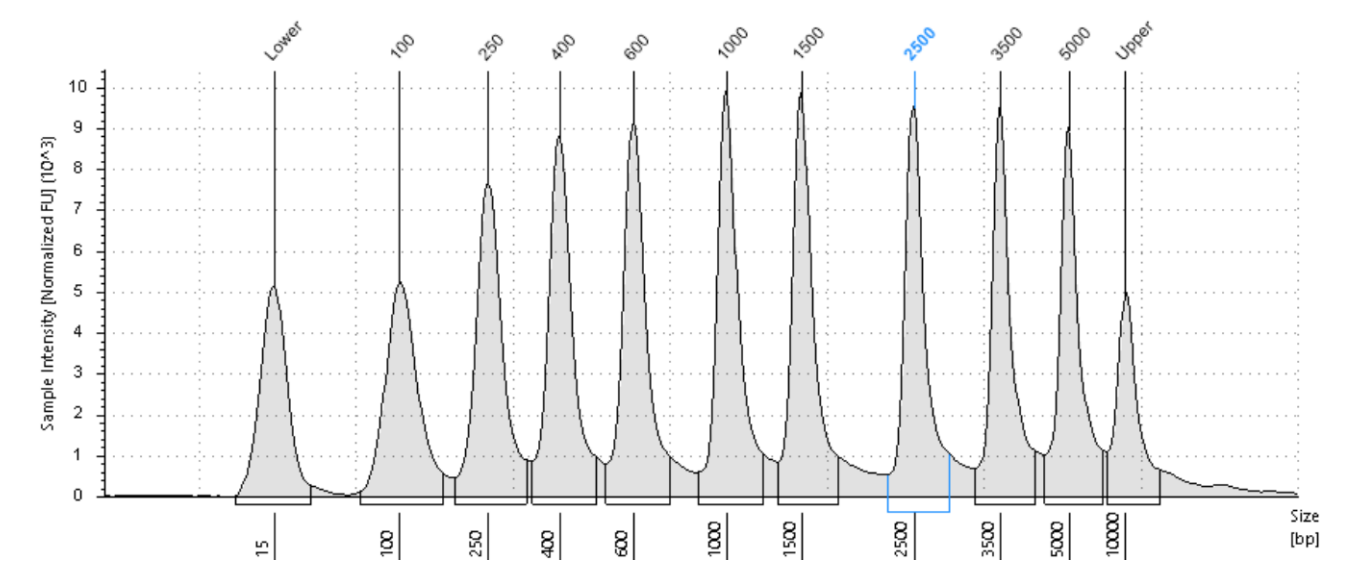


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	94.3	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.91	-	709	-		Lower Marker
100	9.01	-	139	9.56		
250	10.7	-	65.9	11.36		
400	11.0	-	42.5	11.72		
600	11.1	-	28.6	11.82		
1000	11.5	-	17.6	12.15		
1500	10.9	-	11.2	11.61		
2500	10.2	-	6.27	10.81		
3500	10.1	-	4.43	10.69		
5000	9.68	-	2.98	10.28		
10000	3.25	3.25	0.500	-		Upper Marker

B1: M60

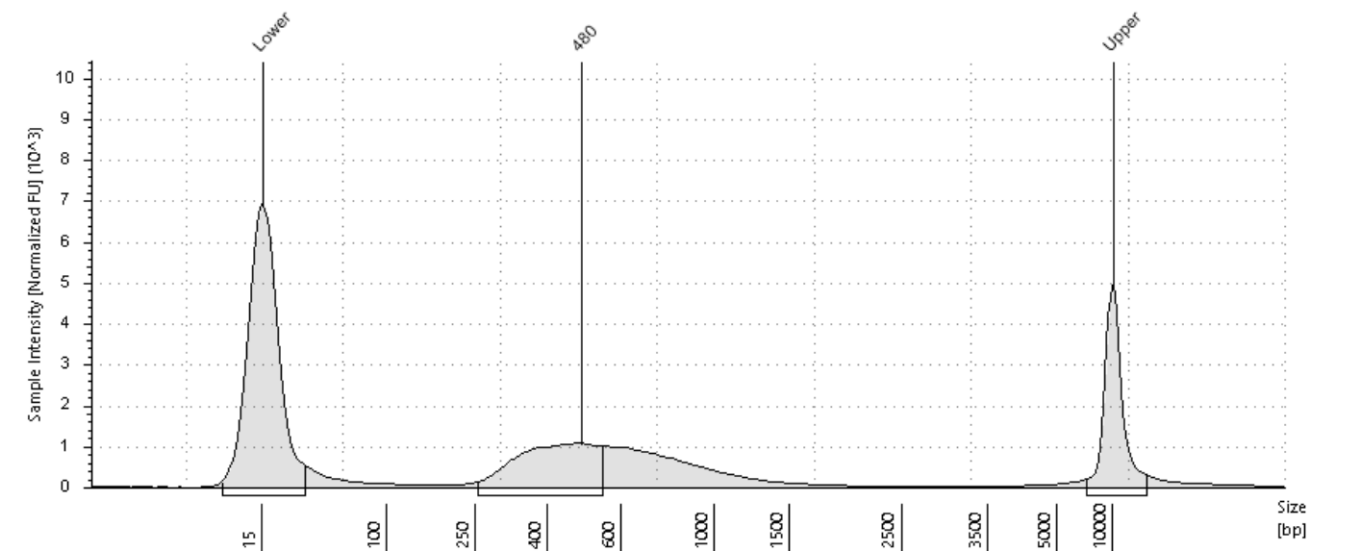


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	3.99	M60		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	8.50	-	871	-		Lower Marker
480	3.99	-	12.8	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C1: M72

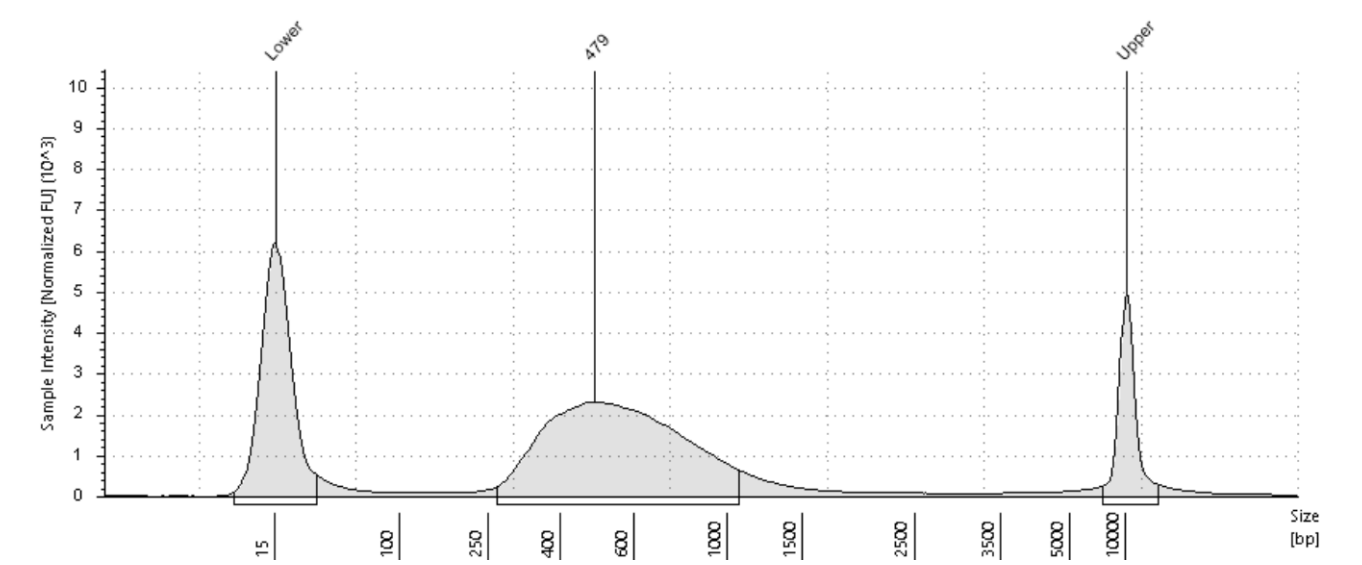

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C1	15.9	M72		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	8.00	-	820	-		Lower Marker
479	15.9	-	50.9	100.00		
10000	3.25	3.25	0.500	-		Upper Marker