



DPM X-ray calibration ($\beta_n, \beta_p = \text{fit_comparat2025 S1 MAP}$): $\beta_n = 0.244$, $\beta_p = 0.893$, $n_{e,0.3} = 3.69 \times 10^{-5} \text{ cm}^{-3}$
 Slope fix: $\alpha_{L_X} : 1.97 \rightarrow 1.81$; $\alpha_{kT} : 0.49 \rightarrow 0.65$


L_X - M_{500c} : DPM m.2 vs calibrated

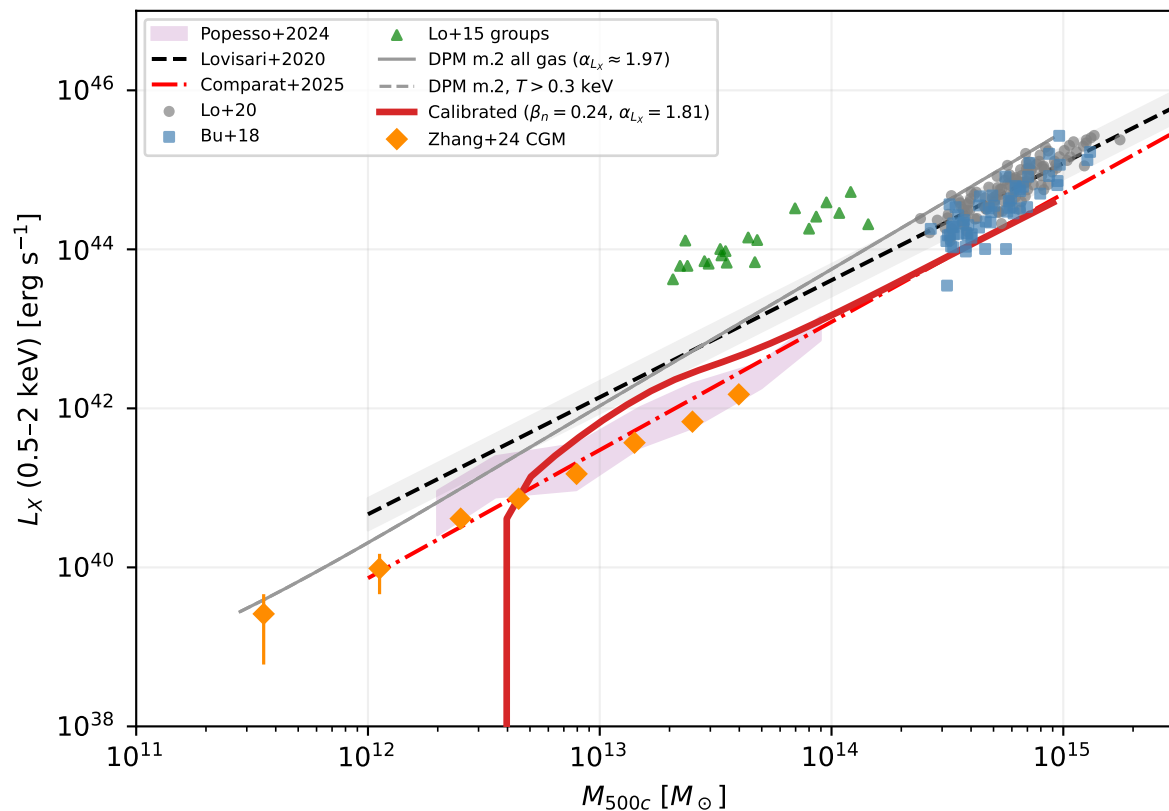

kT - M_{500c} : DPM m.2 vs calibrated

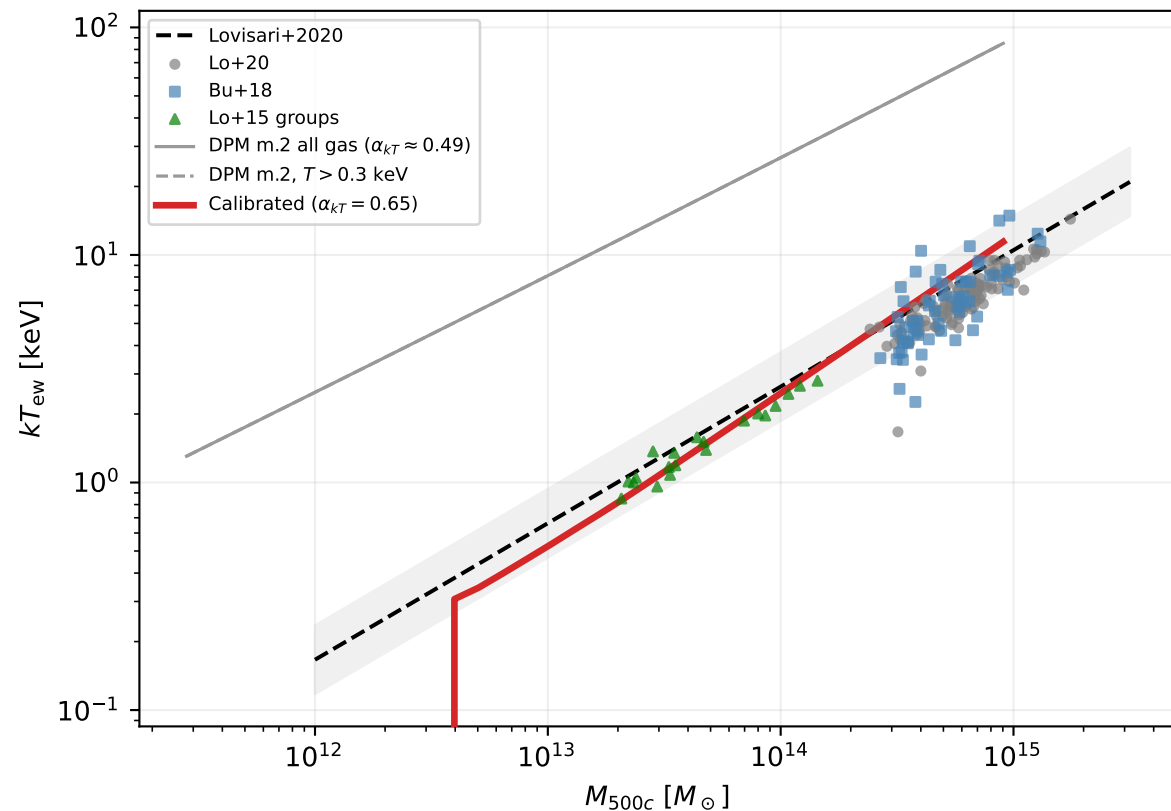

Analytical: $L_X \propto M^{1+1.5\beta_n+0.5\beta_p}$ ($\beta_p = \beta_n + 0.65$)

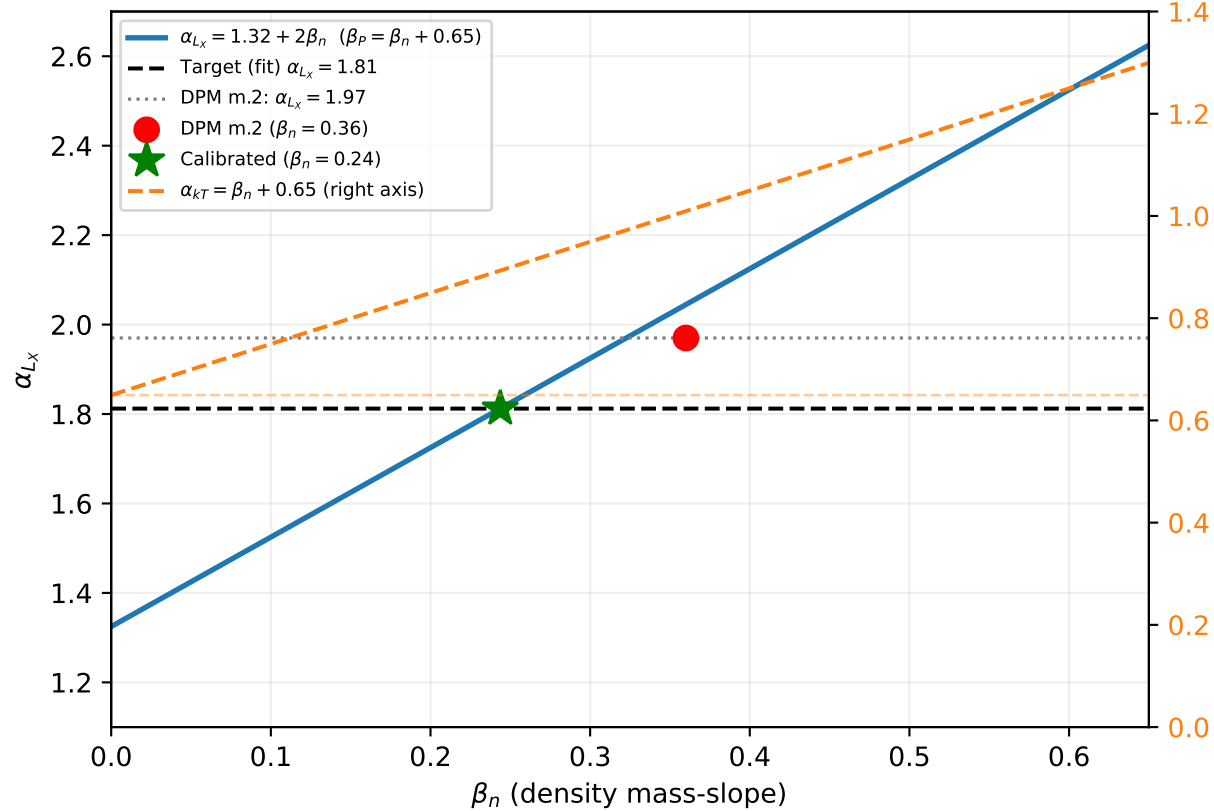

Normalization ratio vs Lovisari+2020

