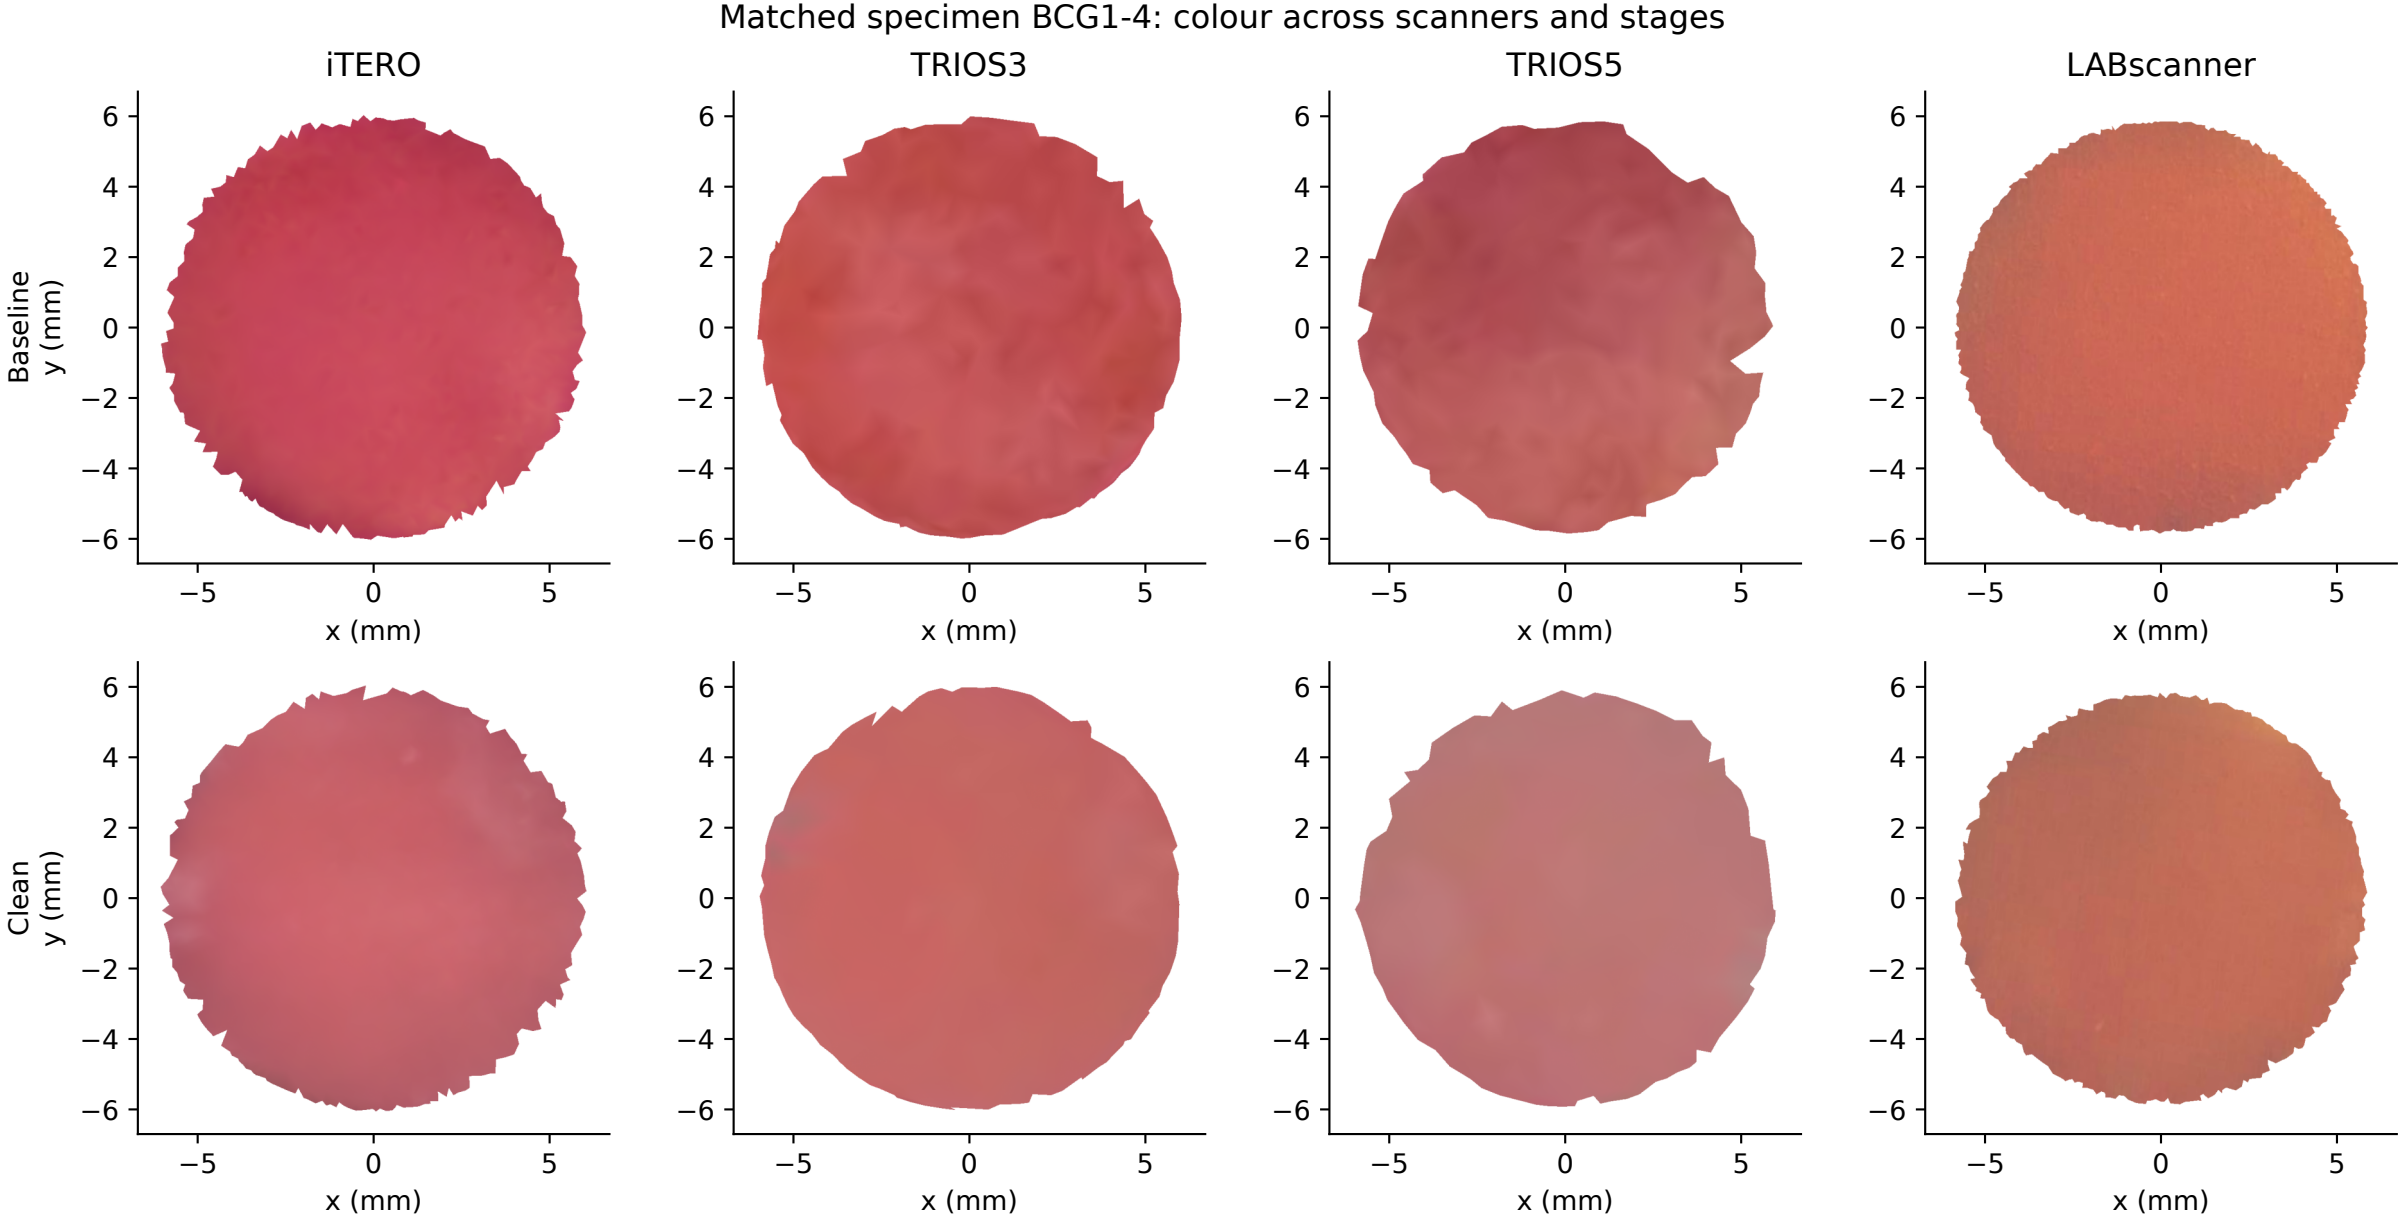

Matched specimen BCG1-4: colour across scanners and stages
iTERO
TRIOS3
TRIOS5
LABscanner
Baseline
Clean
y (mm)
x (mm)
6
4
2
0
−2
−4
−6
−5
0
5