


Scanning Tunneling Microscope Electronics

Changes to Schematic

Rev B.
Added R20 to prevent preamp oscillation
Changed C4 from 0.1uF to 1uF
Changed C1 from 10 pF to 2.2 pF
Changed R3 from 100 k to 20.0 k
Changed R5 from 2.05 k to 2.21 k
Changed R4 from 2 M to 10 M

Rev C.
Added U3, R21-32, C9-12
Added X,Y drivers to increase scan range.
Removed R14-R17, X,Y voltage dividers

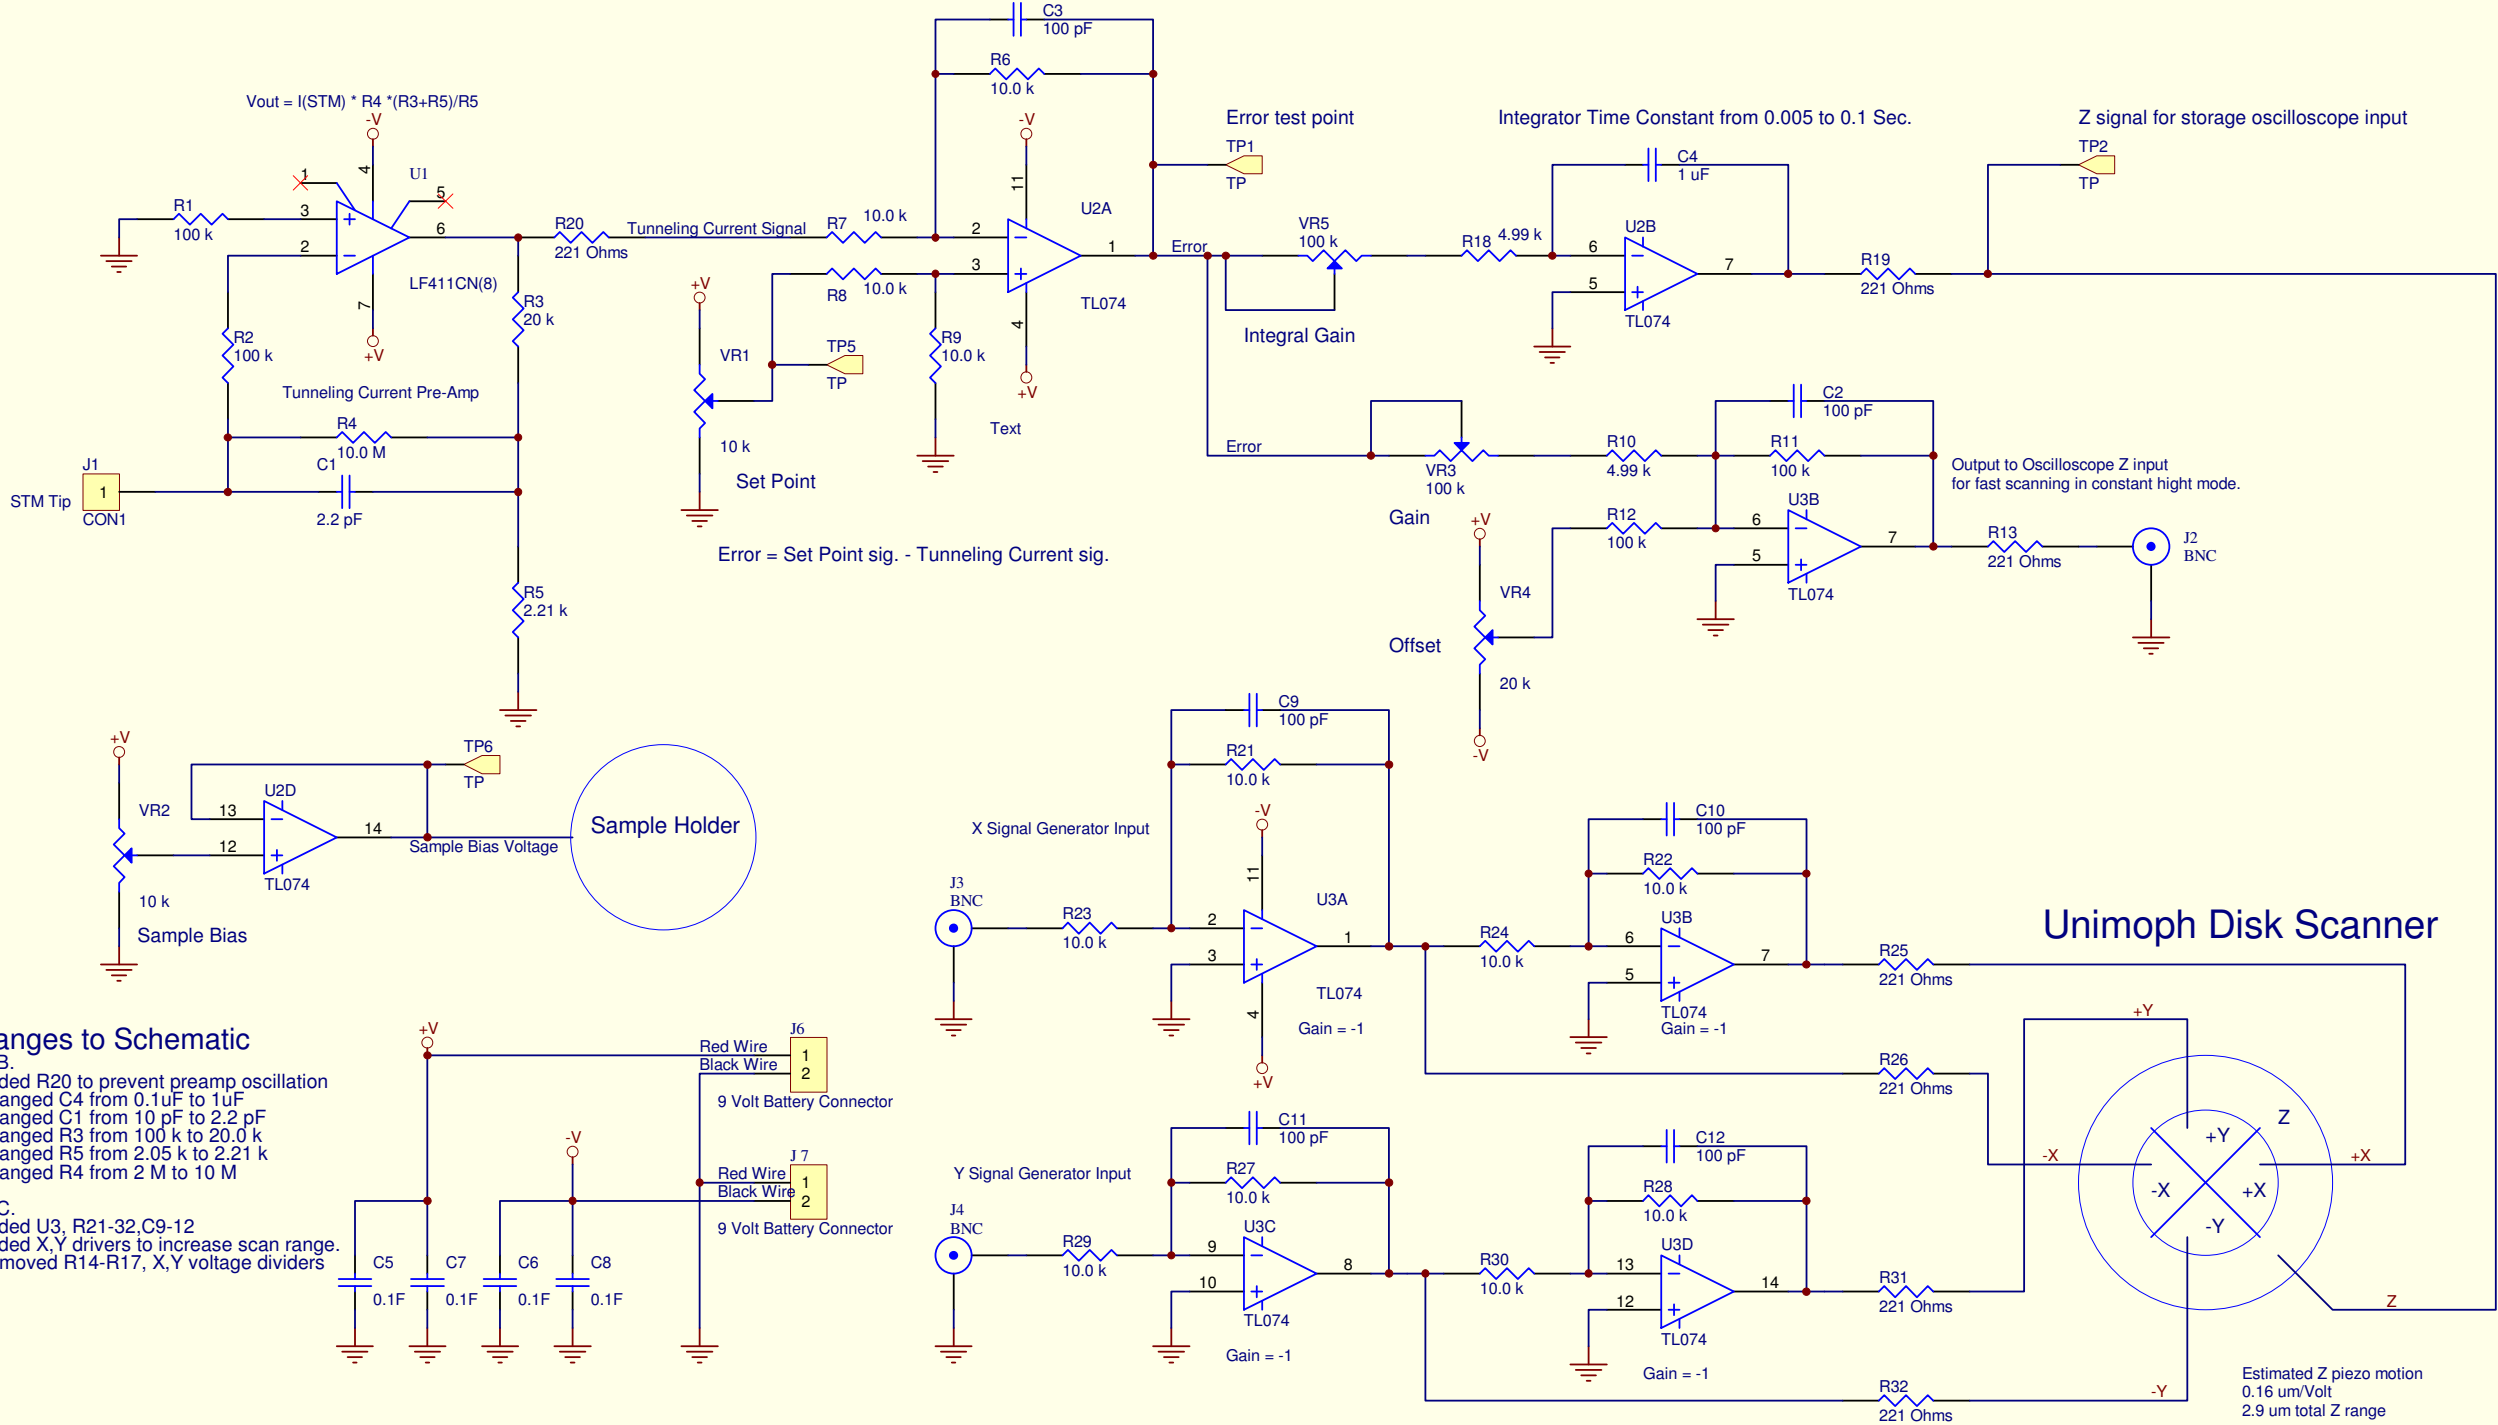

Title Simple Scanning Tunneling Microscope		
Size B	Number	Revision C
Date: 3-Dec-2003	Sheet 1 of 1	
File:	C:\Documents and Settings\John Alexander\My Documents\MyDesign.ddb	