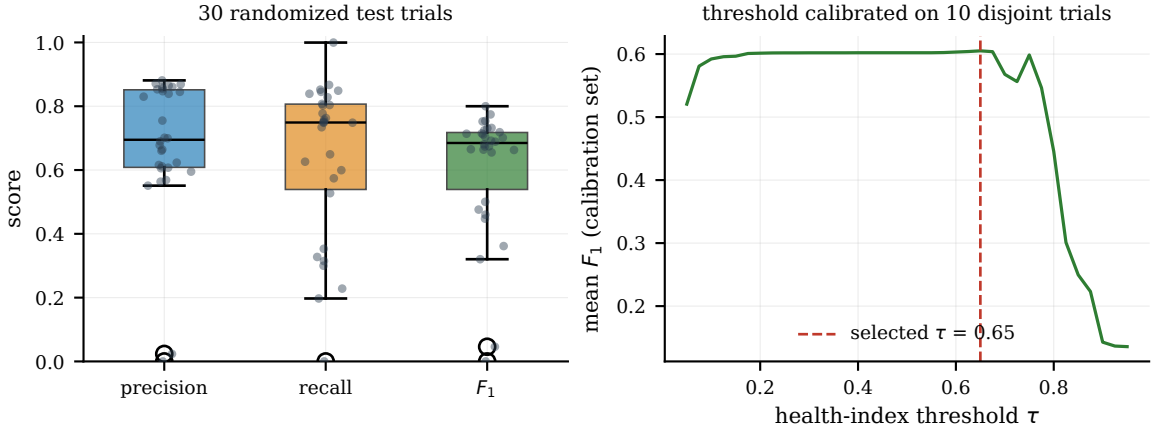
30 randomized test trials
score
1.0
0.8
0.6
0.4
0.2
0.0
precision
recall
F_1
threshold calibrated on 10 disjoint trials
mean F_1 (calibration set)
0.6
0.5
0.4
0.3
0.2
selected τ = 0.65
0.2
0.4
0.6
0.8
health-index threshold τ