20210921_Probiotics_full all @950−to−1630 dpt:sgol@2−21−0 (valid. CV 9 by C_samplename)

comps.: 5
+ RMSEC: 0.1426
+ R2C: 0.9239
● RMSECV: 0.2738
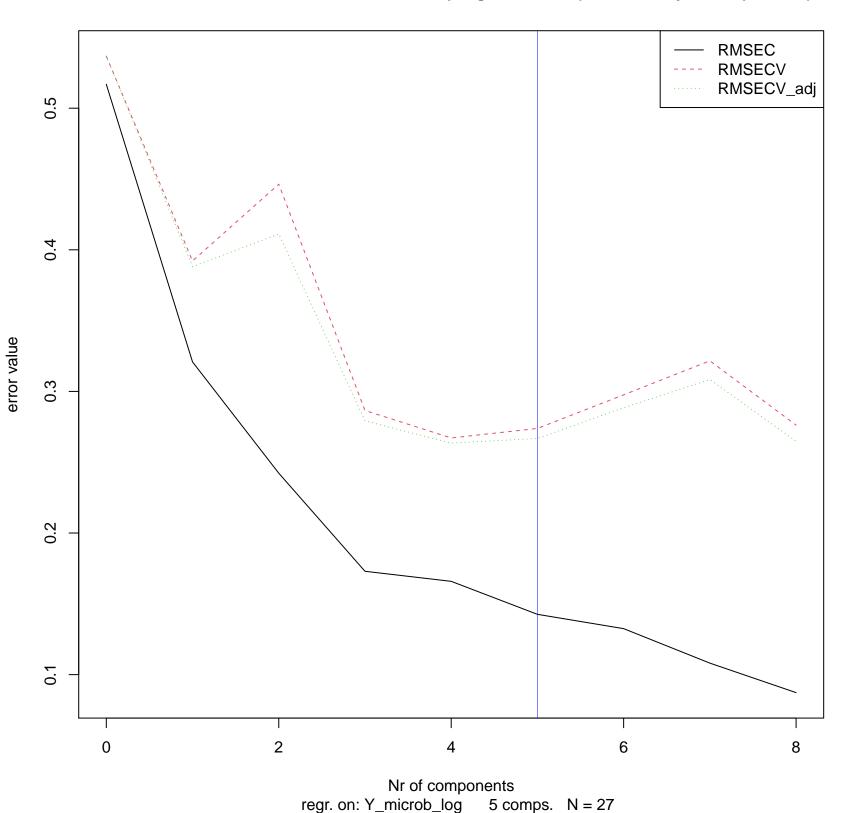● R2CV: 0.7193

predicted value

measured value

regr. on: Y_microb_log   color by: C_samplename   5 comps.   N = 27

● AC1T1 N=3
● AC1T2 N=3
● AC1T3 N=3
● AC2T1 N=3
● AC2T2 N=3
● AC2T3 N=3
● AC3T1 N=3
● AC3T2 N=3
● AC3T3 N=3

20210921_Probiotics_full all @950−to−1630 dpt:sgol@2−21−0 (valid. CV 9 by C_samplename)

error value

— RMSEC
-- RMSECV
··· RMSECV_adj

Nr of components

regr. on: Y_microb_log   5 comps.   N = 27