

Programmer Manual



RSA6100A Series Real-Time Spectrum Analyzers 071-1913-02

This document applies to firmware version 1.2
and above.

www.tektronix.com

Copyright © Tektronix. All rights reserved. Licensed software products are owned by Tektronix or its subsidiaries or suppliers, and are protected by national copyright laws and international treaty provisions.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supercedes that in all previously published material. Specifications and price change privileges reserved.

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

Contacting Tektronix

Tektronix, Inc.
14200 SW Karl Braun Drive
P.O. Box 500
Beaverton, OR 97077
USA

For product information, sales, service, and technical support:

- In North America, call 1-800-833-9200.
- Worldwide, visit www.tektronix.com to find contacts in your area.

Table of Contents

Preface	vii
Related Documentation	vii

Getting Started

Overview of the Manual	1-1
Connecting the Interface	1-3
Using the GPIB Port	1-4
Setting the GPIB Address	1-5
Using TekVISA	1-6

Syntax and Commands

Command Syntax	2-1
Backus-Naur Form Definition	2-1
SCPI Commands and Queries	2-2
IEEE 488.2 Common Commands	2-9
Constructed Mnemonics	2-9
Command Groups	2-11
Measurement Views	2-11
Functional Groups	2-13
IEEE Common Commands	2-14
ABORt Commands	2-14
CALCulate Commands	2-15
CALibration Commands	2-21
DISPlay Commands	2-21
FETCh Commands	2-28
INITiate Commands	2-33
INPut Commands	2-33
MMEMory Commands	2-34
OUTPut Commands	2-35
READ Commands	2-36
SENSe Commands	2-41
STATus Commands	2-48
SYSTem Commands	2-49
TRACe Commands	2-50
TRIGger Commands	2-53
UNIT Commands	2-53
Programming Hints	2-54
IEEE Common Commands	2-55
ABORt Commands	2-67
CALCulate Commands	2-69
CALibration Commands	2-189
DISPlay Commands	2-195
FETCh Commands	2-323

INITiate Commands	2-439
INPut Commands	2-441
MMEMory Commands	2-445
OUTPut Commands	2-469
READ Commands	2-473
SENSE Commands	2-583
STATus Commands	2-727
SYSTem Commands	2-763
TRACe Commands	2-771
TRIGger Commands	2-829
UNIT Commands	2-843
Retrieving Response Message	2-845

Status and Events

Status and Event Reporting System	3-1
Status Byte	3-4
Standard Event Status Block	3-5
Operation Status Block	3-7
Questionable Status Block	3-8
Queues	3-10
Status and Event Processing Sequence	3-11
Synchronizing Execution	3-12
Error Messages and Codes	3-15
Command Errors	3-15
Execution Errors	3-16
Device Specific Errors	3-18
Query Errors	3-19
Device Errors	3-19

Appendices

Appendix A: Character Charts	A-1
Appendix B: GPIB Interface Specification	B-1
Interface Functions	B-1
Interface Messages	B-3
Appendix C: Factory Initialization Settings	C-1
Appendix D: SCPI Conformance Information	D-1

Glossary

Index

List of Figures

Figure 1-1: Command parts	1-1
Figure 1-2: Functional groupings and an alphabetical list of commands	1-2
Figure 1-3: Event-driven program	1-2
Figure 1-4: GPIB connector (rear panel)	1-3
Figure 1-5: GPIB connection	1-4
Figure 1-6: Typical GPIB network configurations	1-4
Figure 2-1: Example of SCPI subsystem hierarchy tree	2-2
Figure 2-2: Example of abbreviating a command	2-5
Figure 2-3: Example of chaining commands and queries	2-6
Figure 2-4: Example of omitting root and lower-level nodes in a chained message	2-6
Figure 2-5: Trigger mask setting example	2-830
Figure 2-6: Retrieving response message	2-845
Figure 3-1: Status/Event reporting mechanism	3-2
Figure 3-2: Status Byte Register (SBR)	3-4
Figure 3-3: Service Request Enable Register (SRER)	3-5
Figure 3-4: Standard event status register	3-5
Figure 3-5: Operation status register	3-7
Figure 3-6: Questionable status register	3-8
Figure 3-7: Questionable frequency status register	3-9
Figure 3-8: Questionable calibration status register	3-10
Figure 3-9: Status and event processing sequence	3-11

List of Tables

Table 2-1: BNF symbols and meanings	2-1
Table 2-2: Query response examples	2-3
Table 2-3: Parameter types used in syntax descriptions	2-4
Table 2-4: Available units	2-7
Table 2-5: Available SI prefixes	2-7
Table 2-6: Constructed mnemonics	2-9
Table 2-7: Measurement views	2-12
Table 2-8: List of command groups	2-13
Table 2-9: Status and error commands	2-14
Table 2-10: ABORt commands	2-14
Table 2-11: CALCulate commands	2-15
Table 2-12: CALibration commands	2-21
Table 2-13: DISPlay commands	2-21
Table 2-14: FETCh commands	2-28
Table 2-15: INITiate commands	2-33
Table 2-16: INPut commands	2-33
Table 2-17: :MMEMory commands	2-34
Table 2-18: OUTPut commands	2-35
Table 2-19: READ commands	2-36
Table 2-20: SENSE commands	2-41
Table 2-21: STATus commands	2-48
Table 2-22: SYSTem commands	2-49
Table 2-23: TRACe commands	2-50
Table 2-24: TRIGger commands	2-53
Table 2-25: UNIT commands	2-53
Table 2-26: Instrument options	2-61
Table 2-27: CALCulate command subgroups	2-69
Table 2-28: Marker mnemonics	2-70
Table 2-29: Search condition	2-80
Table 2-30: Source data of the search operation	2-81
Table 2-31: DISPlay command subgroups	2-195
Table 2-32: Measurement views	2-197
Table 2-33: Modulation measurement views	2-218
Table 2-34: General signal viewing views	2-240
Table 2-35: Pulse results	2-296

Table 2-36: FETCh command subgroups	2-323
Table 2-37: MMEMory command subgroups	2-445
Table 2-38: Trace file extension and trace selection command	2-449
Table 2-39: READ command subgroups	2-473
Table 2-40: SENSE command subgroups	2-583
Table 2-41: Dithering status	2-592
Table 2-42: Power units	2-597
Table 2-43: Digital modulation measurement filter	2-628
Table 2-44: Modulation type	2-630
Table 2-45: Frequency tuning	2-638
Table 2-46: Color palette for DPX spectrum	2-641
Table 2-47: Color palette for spectrogram	2-705
Table 2-48: TRACe command subgroups	2-771
Table 2-49: Trigger violations	2-835
Table 2-50: Trigger event source	2-839
Table 2-51: Power units	2-844
Table 3-1: Register type	3-1
Table 3-2: SBR bit functions	3-4
Table 3-3: Standard event status register bit definition	3-6
Table 3-4: Operation status register bit definition	3-7
Table 3-5: Questionable status register bit definition	3-8
Table 3-6: Questionable frequency status register bit definition ...	3-9
Table 3-7: Questionable calibration status register bit definition ..	3-10
Table 3-8: Command errors	3-15
Table 3-9: Execution errors	3-16
Table 3-10: Device specific errors	3-18
Table 3-11: Query errors	3-19
Table 3-12: Device errors, global condition	3-19
Table 3-13: Device errors, measurement condition	3-20
Table 3-14: Device errors, source condition	3-20
Table A-1: ASCII & GPIB code chart	A-2
Table B-1: GPIB interface function implementation	B-1
Table B-2: Standard interface messages	B-3

Table C-1: Factory initialization settings, IEEE common commands	C-1
Table C-2: Factory initialization settings, CALibration commands	C-1
Table C-3: Factory initialization settings, CALCulate commands .	C-1
Table C-4: Factory initialization settings, DISPlay commands	C-2
Table C-5: Factory initialization settings, INITiate commands ...	C-6
Table C-6: Factory initialization settings, INPut commands	C-6
Table C-7: Factory initialization settings, OUTPut commands ...	C-7
Table C-8: Factory initialization settings, SENSE commands	C-7
Table C-9: Factory initialization settings, TRACe commands	C-13
Table C-10: Factory initialization settings, TRIGger commands ..	C-15
Table C-11: Factory initialization settings, UNIT commands	C-16
Table D-1: SCPI 1999.0-defined commands	D-1

Preface

This programmer manual covers the RSA6100A Series Real-Time Spectrum Analyzers. It provides information on operating your analyzer using the General Purpose Interface Bus (GPIB).

This manual is composed of the following sections:

- *Getting Started* outlines how to use the GPIB interface.
- *Syntax and Commands* defines the syntax used in command descriptions, presents a list of all command subsystems, and presents detailed descriptions of all programming commands.
- *Status and Events* describes how the status and Events Reporting system operates and presents a list of all system errors.
- *Appendices* provides additional information including character charts, GPIB interface specification, and factory initialization settings.

Related Documentation

- *RSA6100A Series Quick Start User Manual*
(Tektronix part number 071-1909-XX)
This manual contains general information about how to put your instrument into service, guides to user interface controls, and application examples.
- *RSA6100A Series Online Help*
The online help contains detailed information about how to operate the instrument.
- *TekVISA Programmer Manual*
(Tektronix part number 071-1101-XX)
This manual is available as a printable PDF file on the Tektronix web site (www.tektronix.com). The manual describes TekVISA, the Tektronix implementation of the VISA Application Programming Interface (API). TekVISA is industry-compliant software for writing interoperable instrument drivers in a variety of Application Development Environments (ADEs).



Getting Started

Getting Started

You can write computer programs that remotely set the analyzer front panel controls or that take measurements and read those measurements for further analysis or storage. To help you get started with programming the analyzer, this section includes the following subsections:

- *Overview of the Manual*
Summarizes each major section of this manual.
- *Connecting the Interface*
Describes how to physically connect the analyzer to a controller.
- *Using GPIB Ports*
Describes how to use the GPIB port.
- *Setting the GPIB Address*
Describes how to set the GPIB parameters from the front panel.
- *Using TekVISA*
Describes how to use the TekVISA communication protocol.

Overview of the Manual

The information contained in each major section of this manual is described below.

Syntax and Commands

Section 2, *Syntax and Commands*, describes the structure and content of the messages your program sends to the analyzer. Figure 1-1 shows command parts as described in the *Command Syntax* subsection.

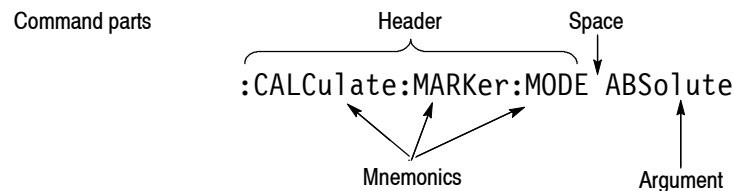


Figure 1-1: Command parts

Section 2 also describes the effect of each command and provides examples of how you might use it. The *Command Groups* subsection provides lists by functional areas. The *IEEE Common Commands* and the subsequent subsections arrange commands alphabetically (Figure 1-2).

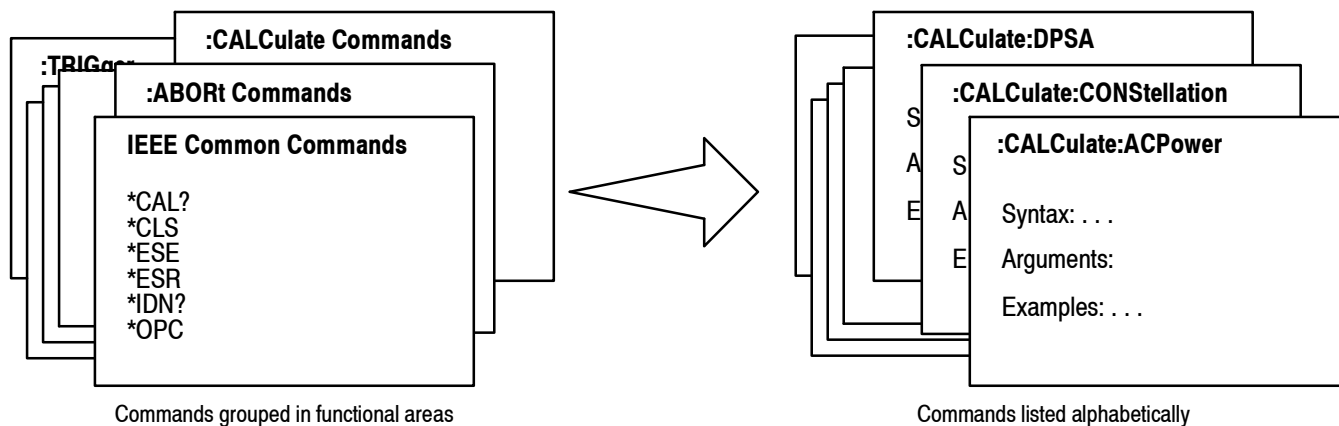


Figure 1-2: Functional groupings and an alphabetical list of commands

Status and Events

The program may request information from the instrument. The instrument provides information in the form of status and error messages. Figure 1-3 illustrates the basic operation of this system. Section 3, *Status and Events*, describes how to get status or event information from the program and details the event and error messages.

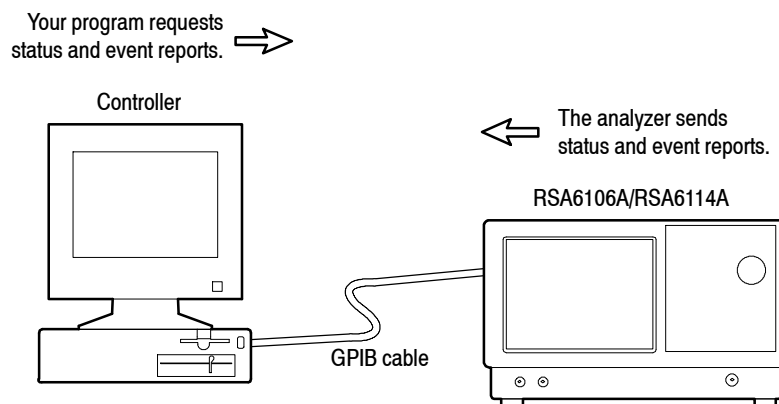


Figure 1-3: Event-driven program

Connecting the Interface

The instrument has a 24-pin GPIB connector on its rear panel, as shown in Figure 1-4. This connector has a D-type shell and conforms to IEEE Std 488.1-1987. Attach an IEEE Std 488.1-1987 GPIB cable (Tektronix part number 012-0991-00) to this connector.

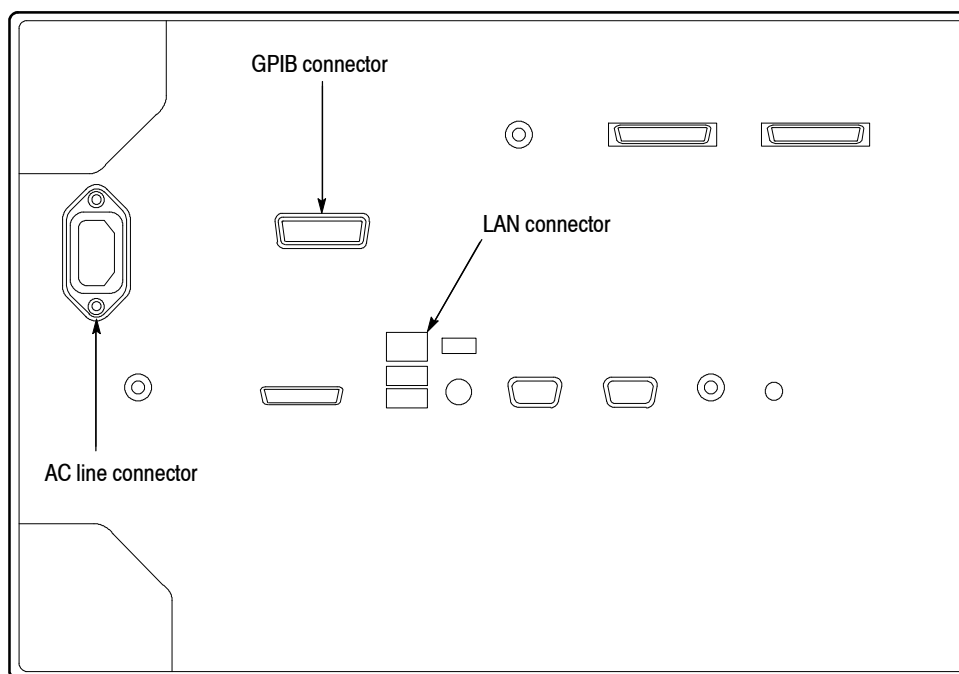


Figure 1-4: GPIB connector (rear panel)

Appendix B: GPIB Interface Specifications gives more information on the GPIB configuration of the analyzer. For the other interfaces, refer to the *RSA6100A Series Quick Start User Manual*.

Using the GPIB Port

The analyzer has Talker/Listener functions through which it can communicate with other devices, as well as the external controller, located on the bus.

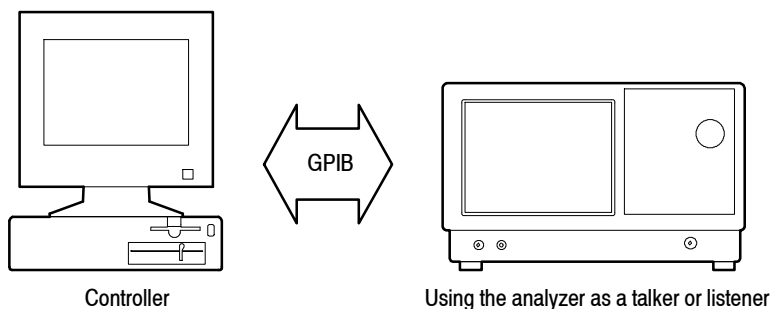


Figure 1-5: GPIB connection

GPIB Requirements

Observe the following rules when you use your analyzer with a GPIB network:

- Assign a unique device address to each device on the bus. No two devices can share the same device address.
- Do not connect more than 15 devices to any one bus.
- Connect one device for every 2 m (6 ft) of cable used.
- Do not use more than 20 m (65 ft) of cable to connect devices to a bus.
- Turn on at least 2/3 of the devices on the network while using the network.
- Connect the devices on the network in a star or linear configuration, as shown in Figure 1-6. Do not use loop or parallel configurations.


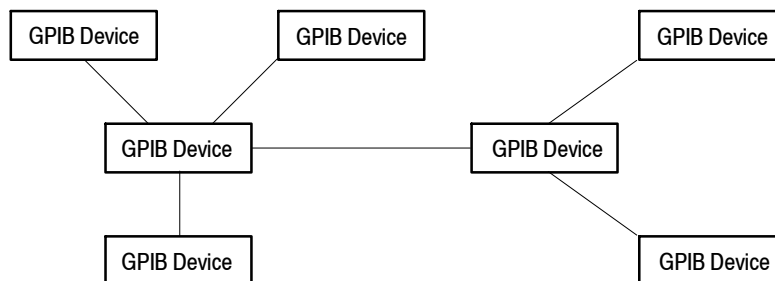


Figure 1-6: Typical GPIB network configurations


Setting the GPIB Address

When you use the GPIB port to communicate with an external controller, follow these steps to set the address of the analyzer.

1. From the **Tools** menu, select **Options** to open the Options control panel.

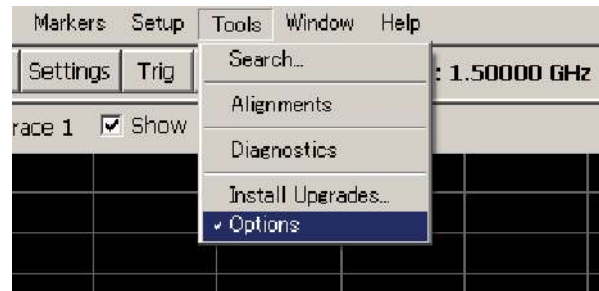

2. Click the **GPIB** tab and set the primary address. Range: 0 to 30 (default: 1)

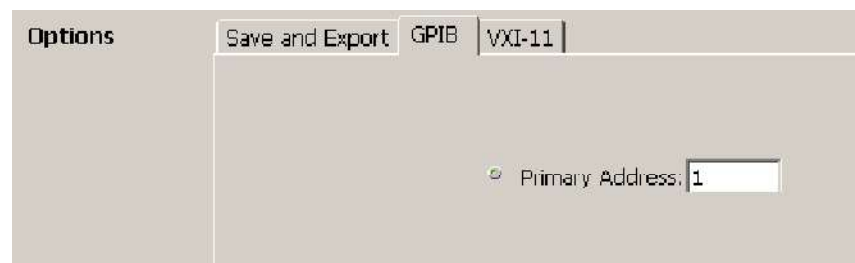

NOTE. The GPIB address cannot be initialized by the *RST command.

Using TekVISA

TekVISA is Tektronix implementation of VISA (Virtual Instrument Software Architecture), an industry-standard communication protocol. VISA provides a common standard for software developers so that software from multiple vendors, such as instrument drivers, can run on the same platform. TekVISA is industry-compliant software, available with selected Tektronix instruments. You can use this software to write (or draw) interoperable instrument drivers in a variety of Application Development Environments (ADEs). It implements a subset of Version 2.2 of the VISA specification for controlling GPIB and serial (RS-232) instrument interfaces locally or remotely via an Ethernet LAN connection.

Installation

Use an internet browser to access the Tektronix web site (www.tektronix.com) and download the current TekVISA to your PC. Unzip the downloaded file in a temporary directory of your choice and run *Setup.exe*.

NOTE. *The details on TekVISA concepts and operations are explained in the TekVISA Programmer Manual that can be also found on the Tektronix web site.*



Syntax and Commands

Command Syntax

This section contains information on the Standard Commands for Programmable Instruments (SCPI) and IEEE 488.2 Common Commands you can use to program your RSA6106A/RSA6114A analyzer. The information is organized in the following subsections:

- Backus-Naur Form Definition
- SCPI Commands and Queries
- IEEE 488.2 Common Commands
- Constructed Mnemonics

Backus-Naur Form Definition

This manual may describe commands and queries using the Backus-Naur Form (BNF) notation. Table 2-1 defines the standard BNF symbols.

Table 2- 1: BNF symbols and meanings

Symbol	Meaning
< >	Defined element
::=	Is defined as
	Exclusive OR
{ }	Group; one element is required
[]	Optional; can be omitted
. . .	Previous element(s) may be repeated
()	Comment

SCPI Commands and Queries

SCPI is a standard created by a consortium that provides guidelines for remote programming of instruments. These guidelines provide a consistent programming environment for instrument control and data transfer. This environment uses defined programming messages, instrument responses, and data format across all SCPI instruments, regardless of manufacturer. The analyzer uses a command language based on the SCPI standard.

The SCPI language is based on a hierarchical or tree structure (see Figure 2-1) that represents a subsystem. The top level of the tree is the root node; it is followed by one or more lower-level nodes.

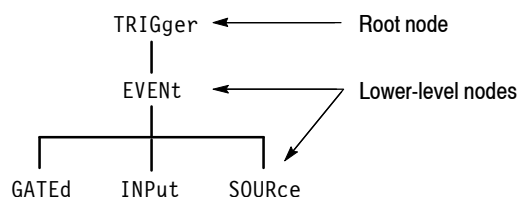


Figure 2- 1: Example of SCPI subsystem hierarchy tree

You can create commands and queries from these subsystem hierarchy trees. Commands specify actions for the instrument to perform. Queries return measurement data and information about parameter settings.

Creating Commands

SCPI commands are created by stringing together the nodes of a subsystem hierarchy and separating each node by a colon.

In Figure 2-1, TRIGger is the root node and EVENT, GATed, INPut, and SOURce are lower-level nodes. To create a SCPI command, start with the root node TRIGger and move down the tree structure adding nodes until you reach the end of a branch. Most commands and some queries have parameters; you must include a value for these parameters. If you specify a parameter value that is out of range, the parameter will be set to a default value. The command descriptions, which start on page 2-55, list the valid values for all parameters.

For example, TRIGger:EVENT:SOURce EXTRear is a valid SCPI command created from the hierarchy tree in Figure 2-1.

Creating Queries

To create a query, start at the root node of a tree structure, move down to the end of a branch, and add a question mark. TRIGger:EVENT:SOURce? is an example of a valid SCPI query using the hierarchy tree in Figure 2-1.

Query Responses

The query causes the analyzer to return information about its status or settings. When a query is sent to the analyzer, only the values are returned. When the returned value is a mnemonic, it is noted in abbreviated format, as shown in Table 2-2.

Table 2-2: Query response examples

Query	Response
:CALCulate:SPECTrum:MARKer:X?	7.50E+9
:SENSe:SPECTrum:FFT:WINDow?	BH4B

A few queries also initiate an operation action before returning information. For example, the *CAL? query runs a calibration.

Parameter Types

Every parameter in the command and query descriptions is of a specified type. The parameters are enclosed in brackets, such as <value>. The parameter type is listed after the parameter and is enclosed in parentheses, for example, (boolean). Some parameter types are defined specifically for the RSA6100A Series command set and some are defined by ANSI/IEEE 488.2-1987 (refer to Table 2-3).

Table 2-3: Parameter types used in syntax descriptions

Parameter type	Description	Example
arbitrary block ¹	A specified length of arbitrary data	#512234xxxxx . . . where 5 indicates that the following 5 digits (12234) specify the length of the data in bytes; xxxxxx ... indicates the data
boolean	Boolean numbers or values	ON or 1; OFF or 0
binary	Binary numbers	#B0110
octal	Octal numbers	#Q57, #Q3
hexadecimal ²	Hexadecimal numbers (0-9, A, B, C, D, E, F)	#HAA, #H1
NR1 ^{2,3} numeric	Integers	0, 1, 15, -1
NR2 ² numeric	Decimal numbers	1.2, 3.141516, -6.5
NR3 ² numeric	Floating point numbers	3.1415E-9, -16.1E5
NRf ² numeric	Flexible decimal number that may be type NR1, NR2 or NR3	See NR1, NR2, and NR3 examples
string ⁴	Alphanumeric characters (must be within quotation marks)	"Testing 1, 2, 3"

¹ Defined in ANSI/IEEE 488.2 as "Definite Length Arbitrary Block Response Data."

² An ANSI/IEEE 488.2-1992-defined parameter type.

³ Some commands and queries will accept an octal or hexadecimal value even though the parameter type is defined as NR1.

⁴ Defined in ANSI/IEEE 488.2 as "String Response Data."

Special Characters

The Line Feed (LF) character (ASCII 10), and all characters in the range of ASCII 127-255 are defined as special characters. These characters are used in arbitrary block arguments only; using these characters in other parts of any command yields unpredictable results.

Abbreviating Commands, Queries, and Parameters

You can abbreviate most SCPI commands, queries, and parameters to an accepted short form. This manual shows these short forms as a combination of upper and lower case letters. The upper case letters indicate the accepted short form of a command. As shown in Figure 2-2, you can create a short form by using only the upper case letters. The accepted short form and the long form are equivalent and request the same action of the instrument.

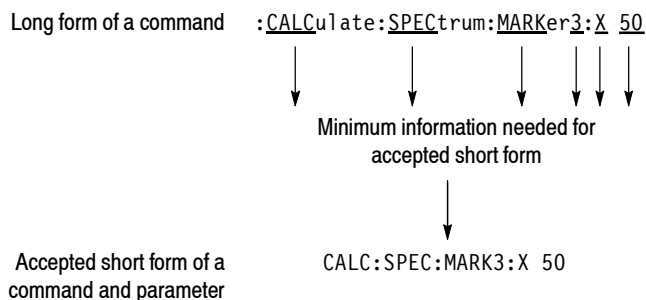


Figure 2-2: Example of abbreviating a command

NOTE. The numeric suffix of a command or query may be included in either the long form or short form; the analyzer will default to “1” if no suffix is used. In Figure 2-2, the “3” of “MARKer3” indicates that the command is directed to Marker 3.

Chaining Commands and Queries

You can chain several commands or queries together into a single message. To create a chained message, first create a command or query, add a semicolon (;), and then add more commands or queries and semicolons until the message is complete. If the command following a semicolon is a root node, precede it with a colon (:). Figure 2-3 illustrates a chained message consisting of several commands and queries. The single chained message should end in a command or query, not a semicolon. Responses to any queries in your message are separated by semicolons.

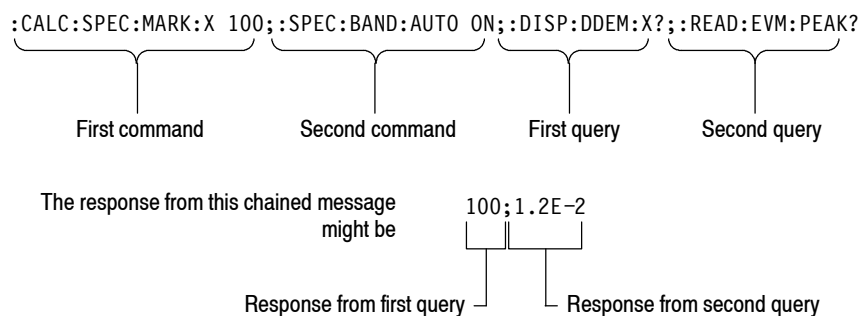


Figure 2-3: Example of chaining commands and queries

If a command or query has the same root and lower-level nodes as the previous command or query, you can omit these nodes. In Figure 2-4, the second command has the same root node (`TRIGger:EVENT`) as the first command, so these nodes can be omitted.

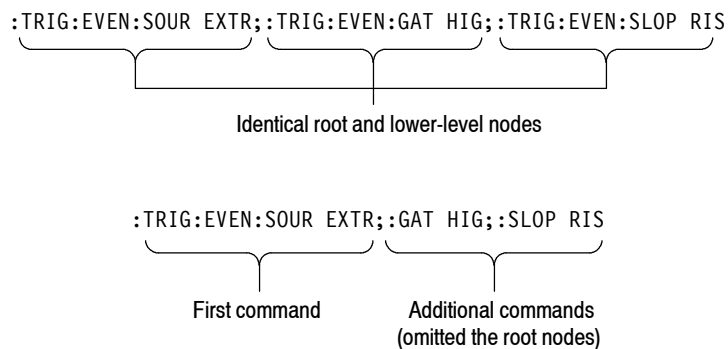


Figure 2-4: Example of omitting root and lower-level nodes in a chained message

Unit and SI Prefix

If the decimal numeric argument refers to amplitude, frequency, or time, you can express it using SI units instead of using the scaled explicit point input value format <NR3>. (SI units are units that conform to the Systeme International d'Unites standard.) For example, you can use the input format 200 mV or 1.0 MHz instead of 200.0E-3 or 1.0E+6, respectively, to specify voltage or frequency.

Table 2-4 lists the available units.

Table 2-4: Available units

Symbol	Meaning
dB	decibel (relative amplitude)
dBm	decibel (absolute amplitude)
DEG	degree (phase)
Hz	hertz (frequency)
PCT	percent (%)
s	second (time)
V	volt

The available SI prefixes are shown in Table 2-5 below.

Table 2-5: Available SI prefixes

SI prefix	Z	A	F	P	N	U	M	K	MA ¹	G	T	PE	EX
Corresponding power	10 ⁻²¹	10 ⁻¹⁸	10 ⁻¹⁵	10 ⁻¹²	10 ⁻⁹	10 ⁻⁶	10 ⁻³	10 ⁺³	10 ⁺⁶	10 ⁺⁹	10 ⁺¹²	10 ⁺¹⁵	10 ⁺¹⁸

¹ When the unit is “Hz”, “M” may be used instead of “MA” so that the frequency can be represented by “MHz”.

You can omit a unit in a command, but you must include the unit when using a SI prefix. For example, frequency of 15 MHz can be described as follows:

15.0E6, 1.5E7Hz, 15000000, 15000000Hz, 15MHz, etc.
 (“15M” is not allowed.)

Note that you can use either lower or upper case units and prefixes. The following examples have the same result, respectively.

170mhz, 170mHz, 170MHz, etc.
 250mv, 250mV, 250MV, etc.

General Rules

Here are three general rules for using SCPI commands, queries, and parameters:

- You can use single (' ') or double (" ") quotation marks for quoted strings, but you cannot use both types of quotation marks for the same string.

correct: "This string uses quotation marks correctly."

correct: 'This string also uses quotation marks correctly.'

incorrect: "This string does not use quotation marks correctly."

- You can use upper case, lower case, or a mixture of both cases for all commands, queries, and parameters.

SENSE:SPECTRUM:FFT:LENGTH 1024

is the same as

sense:spectrum:fft:length 1024

and

SENSE:spectrum:FFT:length 1024

NOTE. *Literal strings (quoted) are case sensitive, for example, file names.*

- No embedded spaces are allowed between or within nodes.

correct: SENSE:SPECTRUM:FFT:LENGTH 1024

incorrect: SENSE: SPECTRUM: FFT: LEN GTH 1024

IEEE 488.2 Common Commands

Description ANSI/IEEE Standard 488.2 defines the codes, formats, protocols, and usage of common commands and queries used on the interface between the controller and the instruments. The analyzer complies with this standard.

Command and Query Structure The syntax for an IEEE 488.2 common command is an asterisk (*) followed by a command and, optionally, a space and parameter value. The syntax for an IEEE 488.2 common query is an asterisk (*) followed by a query and a question mark. All of the common commands and queries are listed in the last part of the *Syntax and Commands* section. The following are examples of common commands:

- *ESE 16
- *CLS

The following are examples of common queries:

- *ESR?
- *IDN?

Constructed Mnemonics

Some header mnemonics specify one of a range of mnemonics. For example, a channel mnemonic can be either TRACe1, TRACe2, TRACe3, or TRACe4. You use these mnemonics in the command just as you do any other mnemonic. For example, there is a :TRACe1:SPECTrum:FUNCTion command, and there is also a :TRACe2:SPECTrum:FUNCTion command. In the command descriptions, this list of choices is abbreviated as TRACe<x>. The value of <x> is the upper range of valid suffixes. If the numeric suffix is omitted, the analyzer uses the default value of “1”.

Table 2- 6: Constructed mnemonics

Symbol	Meaning
MARKer<x>	A marker specifier where <x> = 0, 1, 2, 3, or 4. Refer to <i>Marker Mnemonics</i> on page 2-70.
TRACe<x>	A trace specifier where <x> = 0, 1, 2, 3, 4, or 5. Refer to <i>TRACe Commands</i> on page 2-771 for details.

Command Groups

This section lists the RSA6100A Series analyzer commands in two ways. It first presents them by functional groups. It then lists them alphabetically. The functional group list starts below. The alphabetical list provides more detail on each command and starts on page 2-55.

The RSA6100A Series analyzers conform to the Standard Commands for Programmable Instruments (SCPI) 1999.0 and IEEE Std 488.2-1987 except where noted.

Items followed by question marks are queries; items without question marks are commands. Some items in this section have a question mark in parentheses (?) in the command header section; this indicates that the item can be both a command and a query.

For the conventions of notation in this manual, refer to *Command Syntax* on page 2-1 and following pages.

Measurement Views

The measurement views in the RSA6100A Series analyzers are categorized into the following four groups:

- General signal viewing
- General purpose digital modulation (Option 21 only)
- RF measurements
- Pulsed RF (Option 20 only)

Each group contains the measurement views as shown in Table 2-7. Each command works in particular measurement view(s) which are specified in the **Measurement Views** item in the command descriptions.

NOTE. *If you send a command for the measurement view that is not displayed on screen, an execution error will occur.*

Table 2- 7: Measurement views

Display group	Measurement view
General signal viewing	Spectrum
	DPX (Digital Phosphor) spectrum
	Amplitude versus Time
	Frequency versus Time
	Phase versus Time
	RF I&Q versus Time
	Spectrogram
	Time overview
General purpose digital modulation (Option 21 only)	Constellation
	EVM versus Time
	Magnitude error versus Time
	Phase error versus Time
	Signal quality
	Symbol table
RF measurements	CCDF
	Channel power and ACPR (Adjacent Channel Power Ratio)
	MCPR (Multiple Carrier Power Ratio)
	Occupied Bandwidth (OBW)
Pulsed RF (Option 20 only)	Pulse statistics
	Pulse table
	Pulse trace

Functional Groups

All commands are divided into groups as show in Table 2-8.

Table 2- 8: List of command groups

Command group	Function
IEEE common	Conforms to the IEEE Std 488.2.
ABORt	Resets the trigger system and stops measurements.
CALCulate	Controls the markers and the search operations.
CALibration	Controls the external correction.
DISPlay	Controls the display of measurement results and waveforms.
FETCh	Retrieves the measurements from the last acquired data.
INITiate	Controls data acquisition.
INPut	Controls the characteristics of the signal input.
MMEMory	Provides mass storage capabilities for the analyzer.
OUTPut	Controls the characteristics of the signal output.
READ	Obtains the measurement results with acquiring data.
SENSe	Sets up detailed conditions for each measurement.
STATus	Controls the status and event registers.
SYSTem	Sets or queries system parameters for operation.
TRACe	Controls trace activation and math operations.
TRIGger	Controls triggering.
UNIT	Specifies fundamental units for measurement.

The following sections list the commands by group.

IEEE Common Commands

The IEEE 488.2 common commands have a “*” prefix.

Table 2-9: Status and error commands

Header	Description
*CAL	Performs an internal self-calibration.
*CLS	Clears status.
*ESE(?)	Sets or queries the bits in the ESER register.
*ESR?	Returns the contents of the SESR register.
*IDN?	Returns the instrument identification code.
*OPC(?)	Synchronizes commands.
*OPT?	Returns a list of options installed in your analyzer.
*RST	Returns the instrument settings to the factory defaults.
*SRE(?)	Sets or queries the bits in the SRER register.
*STB?	Returns the contents of the SBR using the MSS bit.
*TRG	Generates a trigger.
*WAI	Prevents the analyzer from executing further commands.

ABORt Commands

Use the ABORt commands to reset the trigger system and to stop measurements.

Table 2-10: ABORt commands

Header	Description
:ABORt	Resets the trigger system and stops measurements.

CALCulate Commands

Use the CALCulate commands to control the markers and the search operations.

Table 2- 11: CALCulate commands

Header	Description
:CALCulate basic command subgroup	General marker control
:CALCulate:MARKer:ADD	Adds a marker.
:CALCulate:MARKer:AOff	Turns off all markers.
:CALCulate:MARKer:DELeTe	Deletes the last marker added.
:CALCulate:MARKer:MODE(?)	Selects or queries the marker mode.
:CALCulate:MARKer:PEAK:EXCursion(?)	Sets or queries the excursion level.
:CALCulate:MARKer:PEAK:THReshold(?)	Sets or queries the threshold level to detect peaks.
:CALCulate:SEARch:LIMit:FAIl?	Queries whether the waveform cuts across the limit or not.
:CALCulate:SEARch:LIMit:MATCH:BEEp[:STATe](?)	Selects or queries whether to beep when a match occurs.
:CALCulate:SEARch:LIMit:MATCH:SACQuire[:STATe](?)	Selects or queries whether to stop acquiring data on match.
:CALCulate:SEARch:LIMit:MATCH:SDATa[:STATe](?)	Selects or queries whether to save the acquisition data automatically.
:CALCulate:SEARch:LIMit:MATCH:SPICture[:STATe](?)	Selects or queries whether to save the whole screen automatically.
:CALCulate:SEARch:LIMit:MATCH:STRace[:STATe](?)	Selects or queries whether to save the spectrum trace automatically.
:CALCulate:SEARch:LIMit:OPERation(?)	Selects or queries the limit operation in the search function.
:CALCulate:SEARch:LIMit:OPERation:FEED(?)	Sets or queries the data flow to be fed in the search operation.
:CALCulate:SEARch:LIMit:OPERation:MASK:LOAD	Loads the limit mask from a specified file for the search operation.
:CALCulate:SEARch:LIMit:OPERation:MASK:STORE	Stores the limit mask to a specified file for the search operation.
:CALCulate:SEARch:LIMit:OPERation:SLIMit(?)	Sets or queries the limit value in the search operation.
:CALCulate:SEARch:LIMit:REPort:DATA?	Returns the frequency range(s) that satisfy the search condition.
:CALCulate:SEARch:LIMit:REPort:POINts?	Returns the number of range(s) that satisfy the search condition.
:CALCulate:SEARch:LIMit:STATe(?)	Selects or queries whether to enable or disable the search function.
:CALCulate:ACPower subgroup	Channel power and ACPR measurement
:CALCulate:ACPower:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.
:CALCulate:ACPower:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:ACPower:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:ACPower:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:ACPower:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:ACPower:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:ACPower:MARKer<x>:Y?	Queries the vertical position of the marker.

Table 2- 11: CALCulate commands (Cont.)

Header	Description
:CALCulate:AVTime subgroup	Frequency versus Time measurement
:CALCulate:AVTime:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:AVTime:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:AVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:AVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:AVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:AVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:AVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:AVTime:MARKer<x>:TRACe(?)	Selects or queries the trace on which the marker is placed.
:CALCulate:AVTime:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:AVTime:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:CONSte subgroup (Option 21 only)	Constellation measurement
:CALCulate:CONSte:MARKer<x>:DELTA:X[:TIME]?	Returns the delta marker time for the selected marker.
:CALCulate:CONSte:MARKer<x>:MAGNitude?	Queries the magnitude readout of the marker.
:CALCulate:CONSte:MARKer<x>:MAXimum	Positions the marker at the symbol in the center of the time record.
:CALCulate:CONSte:MARKer<x>:PEAK:LEFT	Moves the marker in the time domain to the next lower symbol number.
:CALCulate:CONSte:MARKer<x>:PEAK:RIGHT	Moves the marker in the time domain to the next higher symbol number.
:CALCulate:CONSte:MARKer<x>:PHASe?	Queries the phase readout of the marker.
:CALCulate:CONSte:MARKer<x>:SYMBol?	Queries the symbol readout of the marker.
:CALCulate:CONSte:MARKer<x>:VALue?	Queries the value readout of the marker.
:CALCulate:CONSte:MARKer<x>:X(?)	Sets or queries the time position of the marker on the trace.
:CALCulate:DPSA subgroup	DPX spectrum measurement
:CALCulate:DPSA:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.
:CALCulate:DPSA:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:DPSA:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:DPSA:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:DPSA:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:DPSA:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:DPSA:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:DPSA:MARKer<x>[:SET]:CENTer	Sets the center frequency to the marker frequency.
:CALCulate:DPSA:MARKer<x>:TRACe(?)	Selects or queries the trace on which the marker is placed.
:CALCulate:DPSA:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:DPSA:MARKer<x>:Y?	Queries the vertical position of the marker.

Table 2- 11: CALCulate commands (Cont.)

Header	Description
:CALCulate:EVM subgroup (Option 21 only)	EVM versus Time measurement
:CALCulate:EVM:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:EVM:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:EVM:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:EVM:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:EVM:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:EVM:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:EVM:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:EVM:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:EVM:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:FVTime subgroup	Frequency versus Time measurement
:CALCulate:FVTime:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:FVTime:MARKer<x>:DELTA:Y?	Returns the delta marker frequency for the selected marker.
:CALCulate:FVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:FVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:FVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:FVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:FVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:FVTime:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:FVTime:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:IQVTime subgroup	RF I&Q versus Time measurement
:CALCulate:IQVTime:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:IQVTime:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:IQVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:IQVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:IQVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:IQVTime:MARKer<x>:TRACe(?)	Selects or queries the trace (I or Q) to place the marker.
:CALCulate:IQVTime:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:IQVTime:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:MCPower subgroup	MCPR measurement
:CALCulate:MCPower:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.
:CALCulate:MCPower:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:MCPower:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.

Table 2- 11: CALCulate commands (Cont.)

Header	Description
:CALCulate:MCPower:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:MCPower:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:MCPower:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:MCPower:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:MERRor subgroup (Option 21 only)	Magnitude error versus Time measurement
:CALCulate:MERRor:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:MERRor:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:MERRor:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:MERRor:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:MERRor:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:MERRor:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:MERRor:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:MERRor:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:MERRor:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:OBWidth subgroup	Occupied Bandwidth measurement
:CALCulate:OBWidth:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.
:CALCulate:OBWidth:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:OBWidth:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:OBWidth:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:OBWidth:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:OBWidth:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:OBWidth:MARKer<x>[:SET]:CENTer	Sets the center frequency to the value at the marker position.
:CALCulate:OBWidth:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:OBWidth:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:PERRor subgroup (Option 21 only)	Phase error versus Time measurement
:CALCulate:PERRor:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:PERRor:MARKer<x>:DELTA:Y?	Returns the delta marker phase for the selected marker.
:CALCulate:PERRor:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:PERRor:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:PERRor:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:PERRor:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:PERRor:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:PERRor:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:PERRor:MARKer<x>:Y?	Queries the vertical position of the marker.

Table 2- 11: CALCulate commands (Cont.)

Header	Description
:CALCulate:PHVTime subgroup	Phase versus Time measurement
:CALCulate:PHVTime:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:PHVTime:MARKer<x>:DELTA:Y?	Returns the delta marker phase for the selected marker.
:CALCulate:PHVTime:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:PHVTime:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:PHVTime:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:PHVTime:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:PHVTime:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:PULSe subgroup (Option 20 only)	Pulsed RF measurements
:CALCulate:PULSe:STATistics:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.
:CALCulate:PULSe:STATistics:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:PULSe:STATistics:MARKer<x>:MAXimum	Moves the marker to the highest peak on the statistics trace.
:CALCulate:PULSe:STATistics:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the statistics trace.
:CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:PULSe:STATistics:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the statistics trace.
:CALCulate:PULSe:STATistics:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:PULSe:STATistics:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:PULSe:TRACe:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:PULSe:TRACe:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:PULSe:TRACe:MARKer<x>:MAXimum	Moves the marker to the highest peak on the pulse trace.
:CALCulate:PULSe:TRACe:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the pulse trace.
:CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:PULSe:TRACe:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the pulse trace.
:CALCulate:PULSe:TRACe:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:PULSe:TRACe:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:SGRam subgroup	Spectrogram measurement
:CALCulate:SGRam:MARKer<x>:DELTA:X:FREQuency?	Returns the delta marker frequency for the selected marker.
:CALCulate:SGRam:MARKer<x>:DELTA:X[:TIME]?	Returns the delta marker time for the selected marker.
:CALCulate:SGRam:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:SGRam:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.

Table 2- 11: CALCulate commands (Cont.)

Header	Description
:CALCulate:SGRam:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:SGRam:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:SGRam:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:SGRam:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:SGRam:MARKer<x>[:SET]:CENTer	Sets the center frequency to the marker frequency.
:CALCulate:SGRam:MARKer<x>:X:FREQuency(?)	Sets or queries the marker frequency.
:CALCulate:SGRam:MARKer<x>:X:TIME](?)	Sets or queries the marker time.
:CALCulate:SGRam:MARKer<x>:Y?	Queries the marker amplitude.
:CALCulate:SPECTrum subgroup	Spectrum measurement
:CALCulate:SPECTrum:MARKer<x>:DELTA:X?	Returns the delta marker frequency for the selected marker.
:CALCulate:SPECTrum:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:SPECTrum:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:SPECTrum:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:SPECTrum:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:SPECTrum:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:SPECTrum:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:SPECTrum:MARKer<x>[:SET]:CENTer	Sets the center frequency to the marker frequency.
:CALCulate:SPECTrum:MARKer<x>:TRACe(?)	Selects or queries the trace on which the marker is placed.
:CALCulate:SPECTrum:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:SPECTrum:MARKer<x>:Y?	Queries the vertical position of the marker.
:CALCulate:TOVerview subgroup	Time overview
:CALCulate:TOVerview:MARKer<x>:DELTA:X?	Returns the delta marker time for the selected marker.
:CALCulate:TOVerview:MARKer<x>:DELTA:Y?	Returns the delta marker amplitude for the selected marker.
:CALCulate:TOVerview:MARKer<x>:MAXimum	Moves the marker to the highest peak on the trace.
:CALCulate:TOVerview:MARKer<x>:PEAK:HIGHer	Moves the marker to the next peak higher in amplitude.
:CALCulate:TOVerview:MARKer<x>:PEAK:LEFT	Moves the marker to the next peak to the left on the trace.
:CALCulate:TOVerview:MARKer<x>:PEAK:LOWer	Moves the marker to the next peak lower in amplitude.
:CALCulate:TOVerview:MARKer<x>:PEAK:RIGHT	Moves the marker to the next peak to the right on the trace.
:CALCulate:TOVerview:MARKer<x>:X(?)	Sets or queries the horizontal position of the marker.
:CALCulate:TOVerview:MARKer<x>:Y?	Queries the vertical position of the marker.

CALibration Commands

Use the CALibration commands to control the external correction.

Table 2- 12: CALibration commands

Header	Description
:CALibration:ABORt	Aborts any actions related to the alignments in progress.
:CALibration:AUTO(?)	Selects or queries whether or not to run alignments automatically.
:CALibration:CORRection:EXTErnal:EDIT<x>:LABel(?)	Sets or queries the name of the external loss table.
:CALibration:CORRection:EXTErnal:EDIT<x>:STATe(?)	Sets or queries whether to enable or disable the external loss table.
:CALibration:CORRection:EXTErnal:GAIN[:MAGNitude](?)	Sets or queries the external gain value.
:CALibration:CORRection:EXTErnal:GAIN:STATe(?)	Selects or queries whether to enable or disable the external gain value.
:CALibration:CORRection:EXTErnal:PROBE:CONNEct?	Queries whether the external probe is connected to the analyzer or not.
:CALibration:CORRection:EXTErnal:PROBE[:MAGNitude]?	Queries the external probe attenuation.
:CALibration:CORRection:EXTErnal:PROBE:STATe(?)	Determines whether to correct data for the external probe attenuation.

DISPlay Commands

Use the DISPlay commands to control the display of measurement waveforms and results on the screen.

Table 2- 13: DISPlay commands

Header	Description
:DISPlay basic command subgroup	General window control
:DISPlay:WINDow:ACTive:MEASurement?	Queries the active measurement views.
:DISPlay:WINDow:OPTimized:MEASurement?	Queries the measurement views that are optimized.
:DISPlay:ACPower subgroup	Channel power and ACPR measurement
:DISPlay:ACPower:MARKer:SHOW:STATe(?)	Determines whether to show the readout for the selected marker.
:DISPlay:ACPower:PLEVel:SHOW:STATe(?)	Determines whether to show the power levels.
:DISPlay:ACPower:RESet:SCALE	Resets the horizontal and vertical scale to the default values.
:DISPlay:ACPower:WINDow:TRACe:GRATICule:GRID:STATe(?)	Determines whether to show the graticule grid on screen.
:DISPlay:ACPower:X[:SCALE](?)	Sets or queries the horizontal range.
:DISPlay:ACPower:X[:SCALE]:AUTO	Rescales the horizontal axis automatically.
:DISPlay:ACPower:X[:SCALE]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).

Table 2- 13: DISPlay commands (Cont.)

Header	Description
:DISPlay:ACPower:Y[:SCALe](?)	Sets or queries the vertical range.
:DISPlay:ACPower:Y[:SCALe]:AUTO	Rescales the vertical axis automatically.
:DISPlay:ACPower:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset.
:DISPlay:AVTime subgroup	Amplitude versus Time measurement
:DISPlay:AVTime:MARKer:SHOW:STATe(?)	Determines whether to show the readout for the selected marker.
:DISPlay:AVTime:RESet	Resets the horizontal and vertical scale to the default values.
:DISPlay:AVTime:TRIGger:LEVel:STATe(?)	Determines whether to show the power trigger level line on screen.
:DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe(?)	Determines whether to show the graticule grid on screen.
:DISPlay:AVTime:X:RSCale	Rescales the horizontal axis automatically.
:DISPlay:AVTime:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
:DISPlay:AVTime:X[:SCALe]:AUTO:STATe(?)	Determines whether to set the horizontal scale automatically or manually.
:DISPlay:AVTime:X[:SCALe]:FULL(?)	Sets or queries the horizontal scale.
:DISPlay:AVTime:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
:DISPlay:AVTime:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
:DISPlay:AVTime:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).
:DISPlay:AVTime:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
:DISPlay:AVTime:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
:DISPlay:AVTime:Y:RSCale	Rescales the vertical axis automatically.
:DISPlay:AVTime:Y[:SCALe]:FULL(?)	Sets or queries the vertical scale.
:DISPlay:AVTime:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset.
:DISPlay:CONStellation subgroup (Option 21 only)	Constellation measurement
:DISPlay:CONStellation:WINDow:TRACe:GRATicule:GRID:STATe(?)	Selects or queries whether to show the graticule grid on the screen.
:DISPlay:DDEMod subgroup (Option 21 only)	General purpose digital modulation measurements
:DISPlay:DDEMod:MEASview:DELeTe	Deletes the measurement view.
:DISPlay:DDEMod:MEASview:NEW	Displays a new measurement view.
:DISPlay:DDEMod:MEASview:SELeCt(?)	Selects or queries the measurement view.
:DISPlay:DDEMod:RADix(?)	Selects or queries the base of symbols.
:DISPlay:DDEMod:X[:SCALe](?)	Sets or queries the horizontal scale.
:DISPlay:DDEMod:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
:DISPlay:DDEMod:X[:SCALe]:AUTO:STATe(?)	Determines whether to set the horizontal scale automatically or manually.
:DISPlay:DDEMod:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
:DISPlay:DDEMod:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
:DISPlay:DDEMod:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).

Table 2- 13: DISPlay commands (Cont.)

Header	Description
:DISPlay:DDEMod:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
:DISPlay:DDEMod:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
:DISPlay:DDEMod:X[:SCALe]:RESet	Presets the horizontal scale to the default value.
:DISPlay:DPSA subgroup	DPX spectrum measurement
:DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:STATe(?)	Selects or queries whether to show the graticule grid on the screen.
:DISPlay:DPSA:Y[:SCALe]:PDIvision(?)	Sets or queries the vertical scale (per division).
:DISPlay:EVM subgroup (Option 21 only)	EVM versus Time measurement
:DISPlay:EVM:Y[:SCALe](?)	Sets or queries the vertical scale.
:DISPlay:EVM:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
:DISPlay:EVM:Y[:SCALe]:OFFSet(?)	Sets or queries the minimum vertical value (bottom edge).
:DISPlay:FVTime subgroup	Frequency versus Time measurement
:DISPlay:FVTime:WINDow:TRACe:GRATICule:GRID:STATe(?)	Selects or queries whether to show the graticule grid on the screen.
:DISPlay:FVTime:X[:SCALe](?)	Sets or queries the horizontal scale.
:DISPlay:FVTime:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
:DISPlay:FVTime:X[:SCALe]:AUTO:STATe(?)	Determines whether to set the horizontal scale automatically or manually.
:DISPlay:FVTime:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
:DISPlay:FVTime:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
:DISPlay:FVTime:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).
:DISPlay:FVTime:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
:DISPlay:FVTime:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
:DISPlay:FVTime:Y[:SCALe](?)	Sets or queries the vertical scale.
:DISPlay:FVTime:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
:DISPlay:FVTime:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset.
:DISPlay:GENeral subgroup	General signal viewing
:DISPlay:GENeral:MEASview:DELeTe	Deletes the measurement view.
:DISPlay:GENeral:MEASview:NEW	Displays a new measurement view.
:DISPlay:GENeral:MEASview:SELeCt(?)	Selects or queries the measurement view.
:DISPlay:GPRF subgroup	General purpose RF measurements
:DISPlay:GPRF:MEASview:DELeTe	Deletes the measurement view.
:DISPlay:GPRF:MEASview:NEW	Displays a new measurement view.
:DISPlay:GPRF:MEASview:SELeCt(?)	Selects or queries the measurement view.

Table 2- 13: DISPlay commands (Cont.)

Header	Description
:DISPlay:IQVTime subgroup	RF I&Q versus Time measurement
:DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATe(?)	Selects or queries whether to show the graticule grid on the screen.
:DISPlay:IQVTime:X[:SCALe](?)	Sets or queries the horizontal scale.
:DISPlay:IQVTime:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
:DISPlay:IQVTime:X[:SCALe]:AUTO:STATe(?)	Determines whether to set the horizontal scale automatically or manually.
:DISPlay:IQVTime:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
:DISPlay:IQVTime:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
:DISPlay:IQVTime:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).
:DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
:DISPlay:IQVTime:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
:DISPlay:IQVTime:Y[:SCALe](?)	Sets or queries the vertical scale.
:DISPlay:IQVTime:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
:DISPlay:IQVTime:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset.
:DISPlay:IQVTime:Y[:SCALe]:RESCale	Rescales the vertical scale.
:DISPlay:MCPower subgroup	MCPR measurement
:DISPlay:MCPower:MARKer:SHOW:STATe(?)	Determines whether to show the readout for the selected marker.
DISPlay:MCPower:PLEVel:SHOW:STATe(?)	Determines whether to show the power levels.
:DISPlay:MCPower:RESet:SCALe	Resets the horizontal and vertical scale to the default values.
:DISPlay:MCPower:WINDow:TRACe:GRATicule:GRID:STATe(?)	Determines whether to show the graticule grid on screen.
:DISPlay:MCPower:X[:SCALe](?)	Sets or queries the horizontal range.
:DISPlay:MCPower:X[:SCALe]:AUTO	Rescales the horizontal axis automatically.
:DISPlay:MCPower:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).
:DISPlay:MCPower:Y[:SCALe](?)	Sets or queries the vertical range.
:DISPlay:MCPower:Y[:SCALe]:AUTO	Rescales the vertical axis automatically.
:DISPlay:MCPower:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset.
:DISPlay:MERRor subgroup (Option 21 only)	Magnitude error versus Time measurement
:DISPlay:MERRor:Y[:SCALe](?)	Sets or queries the vertical scale.
:DISPlay:MERRor:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
:DISPlay:MERRor:Y[:SCALe]:OFFSet(?)	Sets or queries the minimum vertical value (bottom edge).
:DISPlay:OBWidth subgroup	Occupied Bandwidth measurement
:DISPlay:OBWidth:MARKer:SHOW:STATe(?)	Determines whether to show the readout for the selected marker.
:DISPlay:OBWidth:RESet:SCALe	Resets the horizontal and vertical scale to the default values.
:DISPlay:OBWidth:SELected:BANDwidth(?)	Selects or queries the bandwidth (OBW or x dB BW) to measure.

Table 2- 13: DISPlay commands (Cont.)

Header	Description
:DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATe(?)	Determines whether to show the graticule grid on screen.
:DISPlay:OBWidth:X[:SCALe](?)	Sets or queries the horizontal range.
:DISPlay:OBWidth:X[:SCALe]:AUTO	Rescales the horizontal axis automatically.
:DISPlay:OBWidth:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).
:DISPlay:OBWidth:Y[:SCALe](?)	Sets or queries the vertical range.
:DISPlay:OBWidth:Y[:SCALe]:AUTO	Rescales the vertical axis automatically.
:DISPlay:OBWidth:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset.
:DISPlay:PERRor subgroup (Option 21 only)	Phase error versus Time measurement
:DISPlay:PERRor:Y[:SCALe](?)	Sets or queries the vertical scale.
:DISPlay:PERRor:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
:DISPlay:PERRor:Y[:SCALe]:OFFSet(?)	Sets or queries the minimum vertical value (bottom edge).
:DISPlay:PHVTime subgroup	Phase versus Time measurement
:DISPlay:PHVTime:WINDow:TRACe:GRATicule:GRID:STATe(?)	Selects or queries whether to show the graticule grid on the screen.
:DISPlay:PHVTime:X[:SCALe](?)	Sets or queries the horizontal scale.
:DISPlay:PHVTime:X[:SCALe]:AUTO	Sets the horizontal scale automatically.
:DISPlay:PHVTime:X[:SCALe]:AUTO:STATe(?)	Determines whether to set the horizontal scale automatically or manually.
:DISPlay:PHVTime:X[:SCALe]:MAXimum?	Queries the upper limit of the horizontal scale setting range.
:DISPlay:PHVTime:X[:SCALe]:MINimum?	Queries the lower limit of the horizontal scale setting range.
:DISPlay:PHVTime:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).
:DISPlay:PHVTime:X[:SCALe]:OFFSet:MAXimum?	Queries the upper limit of the horizontal offset setting range.
:DISPlay:PHVTime:X[:SCALe]:OFFSet:MINimum?	Queries the lower limit of the horizontal offset setting range.
:DISPlay:PHVTime:Y[:SCALe](?)	Sets or queries the vertical scale.
:DISPlay:PHVTime:Y[:SCALe]:AUTO	Sets the vertical scale automatically.
:DISPlay:PHVTime:Y[:SCALe]:AXIS(?)	Selects or queries the vertical axis representation.
:DISPlay:PHVTime:Y[:SCALe]:AXIS:REFerence(?)	Sets or queries the reference time for phase.
:DISPlay:PHVTime:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset.
:DISPlay:PHVTime:Y[:SCALe]:RESCale	Rescales the vertical scale.
:DISPlay:PULSe subgroup (Option 20 only)	Pulsed RF measurements
:DISPlay:PULSe:MEASview:DELeTe	Deletes the measurement view.
:DISPlay:PULSe:MEASview:NEW	Displays a new measurement view.
:DISPlay:PULSe:MEASview:SELeCt(?)	Selects or queries the measurement view.
:DISPlay:PULSe:RESult:ATX(?)	Selects or queries whether to show the average transmitted power result.
:DISPlay:PULSe:RESult:AVERAge(?)	Selects or queries whether to show the average on power result.

Table 2- 13: DISPlay commands (Cont.)

Header	Description
:DISPlay:PULSe:RESult:DROOp(?)	Selects or queries whether to show the droop in the results table.
:DISPlay:PULSe:RESult:DUTPct(?)	Selects or queries whether to show the duty factor (%) result.
:DISPlay:PULSe:RESult:DUTRatio(?)	Selects or queries whether to show the duty factor (ratio) result.
:DISPlay:PULSe:RESult:FALL(?)	Selects or queries whether to show the fall time in the results table.
:DISPlay:PULSe:RESult:FRDeviation(?)	Selects or queries whether to show the frequency deviation result.
:DISPlay:PULSe:RESult:MFRqerror(?)	Selects or queries whether to show the maximum frequency error result.
:DISPlay:PULSe:RESult:MPHerror(?)	Selects or queries whether to show the maximum phase error result.
:DISPlay:PULSe:RESult:PHDeviation(?)	Selects or queries whether to show the phase deviation result.
:DISPlay:PULSe:RESult:PPFRequency(?)	Selects or queries whether to show the pulse-pulse frequency result.
:DISPlay:PULSe:RESult:PPOWER(?)	Selects or queries whether to show the peak power in the results table.
:DISPlay:PULSe:RESult:PPPHase(?)	Selects or queries whether to show the pulse-pulse carrier phase result.
:DISPlay:PULSe:RESult:RINTerval(?)	Selects or queries whether to show the repetition interval result.
:DISPlay:PULSe:RESult:RIPple(?)	Selects or queries whether to show the ripple in the results table.
:DISPlay:PULSe:RESult:RISE(?)	Selects or queries whether to show the rise time in the results table.
:DISPlay:PULSe:RESult:RMSFRequency(?)	Selects or queries whether to show the RMS frequency error result.
:DISPlay:PULSe:RESult:RMSPherror(?)	Selects or queries whether to show the RMS phase error result.
:DISPlay:PULSe:RESult:RRATe(?)	Selects or queries whether to show the repetition rate result.
:DISPlay:PULSe:RESult:TIME(?)	Selects or queries whether to show the time in the results table.
:DISPlay:PULSe:RESult:WIDTh(?)	Selects or queries whether to show the pulse width in the results table.
:DISPlay:PULSe:SElect:NUMBer(?)	Selects or queries the pulse to measure.
:DISPlay:PULSe:SElect:RESult(?)	Selects or queries which result is shown in the trace and statistics views.
:DISPlay:PULSe:STATistics:MARKer:SHOW:STATe(?)	Selects or queries whether to show the marker readout in the graph.
:DISPlay:PULSe:STATistics:PLOT(?)	Selects or queries how to show the statistics graph.
:DISPlay:PULSe:STATistics:WINDow:TRACe:GRATICule:GRID:STATe(?)	Selects or queries whether to show the graticule grid in the statistics view.
:DISPlay:PULSe:STATistics:X:RSCale	Rescales the horizontal axis of the statistics graph.
:DISPlay:PULSe:STATistics:X[:SCALE]:NUMBer(?)	Sets or queries the horizontal scale (the number of pulses per division).
:DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet(?)	Sets or queries the minimum horizontal value in the statistics view.
:DISPlay:PULSe:STATistics:Y:RSCale	Rescales the vertical axis of the statistics graph.
:DISPlay:PULSe:STATistics:Y[:SCALE]:FULL(?)	Sets or queries the vertical full-scale in the statistics view.
:DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet(?)	Sets or queries the vertical offset in the statistics view.
:DISPlay:PULSe:STATistics:Y[:SCALE]:STOP?	Queries the minimum vertical value in the statistics view.

Table 2- 13: DISPlay commands (Cont.)

Header	Description
:DISPlay:PULSe:TRACe:MARKer:SHOW:STATe(?)	Selects or queries whether to show the marker readout in the trace view.
:DISPlay:PULSe:TRACe:POINt:SHOW(?)	Selects or queries whether to show the measurement points and lines.
:DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATe(?)	Selects or queries whether to show the graticule grid in the trace view.
:DISPlay:PULSe:TRACe:X:RSCale	Rescales the horizontal axis of the pulse trace view.
:DISPlay:PULSe:TRACe:X[:SCALe](?)	Sets or queries the horizontal full scale in the pulse trace view.
:DISPlay:PULSe:TRACe:X[:SCALe]:FULL(?)	Selects or queries the full-scale reference for the horizontal rescale.
:DISPlay:PULSe:TRACe:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value in the pulse trace view.
:DISPlay:PULSe:TRACe:X[:SCALe]:PDIVision(?)	Sets or queries the horizontal full scale in the pulse trace view.
:DISPlay:PULSe:TRACe:Y:RSCale	Rescales the vertical axis of the pulse trace view.
:DISPlay:PULSe:TRACe:Y[:SCALe]:FULL(?)	Sets or queries the vertical full scale in the pulse trace view.
:DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset in the pulse trace view.
:DISPlay:PULSe:TRACe:Y[:SCALe]:STOP?	Queries the minimum vertical value in the pulse trace view.
:DISPlay:SGRam subgroup	Spectrogram measurement
:DISPlay:SGRam:FREQUency:AUTO	Rescales the horizontal (frequency) axis automatically.
:DISPlay:SGRam:FREQUency:OFFSet(?)	Sets or queries the horizontal (frequency) offset.
:DISPlay:SGRam:FREQUency:SCALe(?)	Sets or queries the horizontal (frequency) range.
:DISPlay:SGRam:TIME:AUTO	Rescales the vertical axis automatically.
:DISPlay:SGRam:TIME:OFFSet(?)	Sets or queries the vertical axis (time) offset (bottom line number).
:DISPlay:SGRam:TIME:OVERlap(?)	Determines whether or not to allow overlap between adjacent FFT frames.
:DISPlay:SGRam:TIME:SCALe(?)	Sets or queries the vertical scale (the amount of time in each line).
:DISPlay:SPECTrum subgroup	Spectrum measurement
:DISPlay:SPECTrum:MARKer:NOISe:MODE(?)	Selects or queries whether to enable the marker noise mode.
:DISPlay:SPECTrum:WINDow:TRACe:GRATicule:GRID:STATe(?)	Selects or queries whether to show the graticule grid in the spectrum view.
:DISPlay:SPECTrum:Y[:SCALe]:PDIVision(?)	Sets or queries the vertical scale (per division).
:DISPlay:TOVerview subgroup	Time overview
:DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe(?)	Selects or queries whether to show the graticule grid in the time overview.
:DISPlay:TOVerview:X[:SCALe](?)	Sets or queries the horizontal scale.
:DISPlay:TOVerview:X[:SCALe]:AUTO	Sets the horizontal scale and offset automatically.
:DISPlay:TOVerview:X[:SCALe]:OFFSet(?)	Sets or queries the minimum horizontal value (left edge).

Table 2- 13: DISPlay commands (Cont.)

Header	Description
:DISPlay:TOVerview:Y[:SCALe](?)	Sets or queries the vertical scale.
:DISPlay:TOVerview:Y[:SCALe]:AUTO	Sets the vertical scale and offset automatically.
:DISPlay:TOVerview:Y[:SCALe]:OFFSet(?)	Sets or queries the vertical offset.
:DISPlay:TOVerview:Y[:SCALe]:RESCale	Rescales the vertical scale.

FETCh Commands

The FETCh commands retrieve the measurements from the data taken by the latest INITiate command.

To perform a FETCh operation on fresh data, use the READ commands, which acquire a new input signal and fetch the measurement results from that data.

Table 2- 14: FETCh commands

Header	Description
:FETCh basic command subgroup	General fetch control
:FETCh:RFIN:IQ?	Returns time-domain IQ data for a specific acquisition data record.
:FETCh:RFIN:IQ:HEADer?	Returns the header information for a specific acquisition data record.
:FETCh:RFIN:IQ:SCALe?	Returns the scaling factor contained in the .tiq file header.
:FETCh:RFIN:RECOrd:IDS?	Returns the beginning and end ID numbers of acquisition data.
:FETCh:ACPower subgroup	Channel power and ACPR measurement
:FETCh:ACPower?	Returns the ACPR measurement results.
:FETCh:ACPower:CHANnel:POWer?	Returns the average power of the main channel.
:FETCh:ACPower:SPECTrum?	Returns spectrum trace data of the ACPR measurement.
:FETCh:AVTime subgroup	Amplitude versus Time measurement
:FETCh:AVTime:AVERage?	Returns the RMS value.
:FETCh:AVTime:FIRSt[:SECOnd]:THIRd[:FOURth]?	Returns the trace data.
:FETCh:AVTime:MAXimum?	Returns the maximum value.
:FETCh:AVTime:MAXLocation?	Returns the time at the maximum.
:FETCh:AVTime:MINimum?	Returns the minimum value.
:FETCh:AVTime:MINLocation?	Returns the time at the minimum.
:FETCh:AVTime:RESult?	Returns the measurement results.
:FETCh:CCDF subgroup	CCDF measurement
:FETCh:CCDF?	Returns the CCDF measurement results.
:FETCh:CCDF:FIRSt[:SECOnd]:THIRd?	Returns waveform data of the specified trace.

Table 2- 14: FETCh commands (Cont.)

Header	Description
:FETCh:CONSt: subgroup (Option 21 only)	Constellation measurement
:FETCh:CONSt:RESults?	Returns the constellation measurement results.
:FETCh:CONSt:TRACe?	Returns the constellation trace data.
:FETCh:DDEMod subgroup (Option 21 only)	General purpose digital modulation measurements
:FETCh:DDEMod:STABle?	Returns the symbol table data.
:FETCh:DDEMod:SYNCh:WORD:LENGth?	Returns the length of the synch word in the symbol table.
:FETCh:DDEMod:SYNCh:WORD:POSition?	Returns the position of the synch word in the symbol table.
:FETCh:DPSA subgroup	DPX spectrum measurement
:FETCh:DPSA:TRACe:AVERage?	Returns waveform data of the average trace.
:FETCh:DPSA:TRACe:MATH?	Returns waveform data of the math trace.
:FETCh:DPSA:TRACe:MAXimum?	Returns waveform data of the maximum trace.
:FETCh:DPSA:TRACe:MINimum?	Returns waveform data of the minimum trace.
:FETCh:EVM subgroup (Option 21 only)	EVM versus Time measurement
:FETCh:EVM:FERRor?	Returns the frequency error.
:FETCh:EVM:PEAK?	Returns the peak value.
:FETCh:EVM:PINDEX?	Returns the time at the EVM peak.
:FETCh:EVM:RMS?	Returns the RMS value.
:FETCh:EVM:TRACe?	Returns the EVM versus Time trace data.
:FETCh:FVTime subgroup	Frequency versus Time measurement
:FETCh:FVTime?	Returns the Frequency versus Time trace data.
:FETCh:FVTime:MAXimum?	Returns the maximum value.
:FETCh:FVTime:MAXLocation?	Returns the time at which the frequency drift is maximum.
:FETCh:FVTime:MINimum?	Returns the minimum value.
:FETCh:FVTime:MINLocation?	Returns the time at which the frequency drift is minimum.
:FETCh:FVTime:RESult?	Returns the measurement results.
:FETCh:IQVTime subgroup	RF I&Q versus Time measurement
:FETCh:IQVTime:I?	Returns the I versus Time trace data.
:FETCh:IQVTime:MAXimum?	Returns the maximum value.
:FETCh:IQVTime:MAXLocation?	Returns the time at which the I or Q level is maximum.
:FETCh:IQVTime:MINimum?	Returns the minimum value.
:FETCh:IQVTime:MINLocation?	Returns the time at which the I or Q level is minimum.
:FETCh:IQVTime:Q?	Returns the Q versus Time trace data.
:FETCh:IQVTime:RESult?	Returns the measurement results.

Table 2- 14: FETCh commands (Cont.)

Header	Description
:FETCh:MCPower subgroup	MCPR measurement
:FETCh:MCPower:ADJacent:CHANnels?	Returns the power of adjacent channels.
:FETCh:MCPower:CHANnel:POWer?	Returns the reference power.
:FETCh:MCPower:MAIN:CHANnels?	Returns the power of main channels.
:FETCh:MCPower:SPECTrum?	Returns spectrum trace data.
:FETCh:MERRor subgroup (Option 21 only)	Magnitude error versus Time measurement
:FETCh:MERRor:FERRor?	Returns the frequency error.
:FETCh:MERRor:PEAK?	Returns the peak value.
:FETCh:MERRor:PINDEX?	Returns the time at the magnitude error peak.
:FETCh:MERRor:RMS?	Returns the RMS value.
:FETCh:MERRor:TRACe?	Returns the Magnitude error versus Time trace data.
:FETCh:OBWidth subgroup	Occupied Bandwidth measurement
:FETCh:OBWidth:FREQuency:ERRor?	Returns the frequency error.
:FETCh:OBWidth:OBWidth:BANDwidth?	Returns the occupied bandwidth.
:FETCh:OBWidth:OBWidth:LEFT:FREQuency?	Returns the left (lower) frequency of the occupied bandwidth.
:FETCh:OBWidth:OBWidth:LEFT:LEVel?	Returns the level at the left frequency of the occupied bandwidth.
:FETCh:OBWidth:OBWidth:POWer?	Returns the reference power in the Occupied Bandwidth measurement.
:FETCh:OBWidth:OBWidth:RIGHT:FREQuency?	Returns the right (higher) frequency of the occupied bandwidth.
:FETCh:OBWidth:OBWidth:RIGHT:LEVel?	Returns the level at the right frequency of the occupied bandwidth.
:FETCh:OBWidth:SPECTrum?	Returns spectrum trace data of the Occupied Bandwidth measurement.
:FETCh:OBWidth:XDBBANDwidth:BANDwidth?	Returns the x dB bandwidth.
:FETCh:OBWidth:XDBBANDwidth:LEFT:FREQuency?	Returns the left (lower) frequency of the x dB bandwidth.
:FETCh:OBWidth:XDBBANDwidth:LEFT:LEVel?	Returns the level at the left frequency of the x dB bandwidth.
:FETCh:OBWidth:XDBBANDwidth:POWer?	Returns the reference power in the x dB bandwidth measurement.
:FETCh:OBWidth:XDBBANDwidth:RIGHT:FREQuency?	Returns the right (higher) frequency of the x dB bandwidth.
:FETCh:OBWidth:XDBBANDwidth:RIGHT:LEVel?	Returns the level at the right frequency of the x dB bandwidth.
:FETCh:PERRor subgroup (Option 21 only)	Phase error versus Time measurement
:FETCh:PERRor:FERRor?	Returns the frequency error.
:FETCh:PERRor:PEAK?	Returns the peak value.
:FETCh:PERRor:PINDEX?	Returns the time at the phase error peak.
:FETCh:PERRor:RMS?	Returns the RMS value.
:FETCh:PERRor:TRACe?	Returns the Phase error versus Time trace data.

Table 2- 14: FETCh commands (Cont.)

Header	Description
:FETCh:PHVTime subgroup	Phase versus Time measurement
:FETCh:PHVTime?	Returns the Phase versus Time trace data.
:FETCh:PHVTime:MAXimum?	Returns the maximum value.
:FETCh:PHVTime:MAXLocation?	Returns the time at which the phase is maximum.
:FETCh:PHVTime:MINimum?	Returns the minimum value.
:FETCh:PHVTime:MINLocation?	Returns the time at which the phase is minimum.
:FETCh:PHVTime:RESult?	Returns the results.
:FETCh:PULSe subgroup (Option 20 only)	Pulsed RF measurements
:FETCh:PULSe[:RESult]:ATX?	Returns the average transmitted power in the results table.
:FETCh:PULSe[:RESult]:AVERage?	Returns the average on power in the results table.
:FETCh:PULSe[:RESult]:DROop?	Returns the droop in the results table.
:FETCh:PULSe[:RESult]:DUTPct?	Returns the duty factor (%) in the results table.
:FETCh:PULSe[:RESult]:DUTRatio?	Returns the duty factor (ratio) in the results table.
:FETCh:PULSe[:RESult]:FALL?	Returns the fall time in the results table.
:FETCh:PULSe[:RESult]:FRDeviation?	Returns the frequency deviation in the results table.
:FETCh:PULSe[:RESult]:MFRreqerror?	Returns the maximum frequency error in the results table.
:FETCh:PULSe[:RESult]:MPHerror?	Returns the maximum phase error in the results table.
:FETCh:PULSe[:RESult]:PHDeviation?	Returns the phase deviation in the results table.
:FETCh:PULSe[:RESult]:PPFrequency?	Returns the pulse-pulse carrier frequency in the results table.
:FETCh:PULSe[:RESult]:PPOWER?	Returns the peak power in the results table.
:FETCh:PULSe[:RESult]:PPPHase?	Returns the pulse-pulse carrier phase in the results table.
:FETCh:PULSe[:RESult]:RINTerval?	Returns the repetition interval in the results table.
:FETCh:PULSe[:RESult]:RIPPlE?	Returns the ripple in the results table.
:FETCh:PULSe[:RESult]:RISE?	Returns the rise time in the results table.
:FETCh:PULSe[:RESult]:RMSFreqerror?	Returns the RMS frequency error in the results table.
:FETCh:PULSe[:RESult]:RMSPHerror?	Returns the RMS phase error in the results table.
:FETCh:PULSe[:RESult]:RRate?	Returns the repetition rate in the results table.
:FETCh:PULSe[:RESult]:TIME?	Returns the time in the results table.
:FETCh:PULSe[:RESult]:WIDTH?	Returns the pulse width in the results table.
:FETCh:PULSe:STATistics?	Returns the trace data of the pulse statistics measurement.
:FETCh:PULSe:STATistics:ATX?	Returns the average transmitted power of the statistics.
:FETCh:PULSe:STATistics:AVERage?	Returns the average on power of the statistics.
:FETCh:PULSe:STATistics:DROOp?	Returns the droop of the statistics.
:FETCh:PULSe:STATistics:DUTPct?	Returns the duty factor (%) of the statistics.
:FETCh:PULSe:STATistics:DUTRatio?	Returns the duty factor (ratio) of the statistics.

Table 2- 14: FETCh commands (Cont.)

Header	Description
:FETCh:PULSe:STATistics:FALL?	Returns the fall time of the statistics.
:FETCh:PULSe:STATistics:FRDeviation?	Returns the frequency deviation of the statistics.
:FETCh:PULSe:STATistics:MFRqerror?	Returns the maximum frequency error of the statistics.
:FETCh:PULSe:STATistics:MPHerror?	Returns the maximum phase error of the statistics.
:FETCh:PULSe:STATistics:PHDeviation?	Returns the phase deviation of the statistics.
:FETCh:PULSe:STATistics:PPFRqfrequency?	Returns the pulse-pulse carrier frequency of the statistics.
:FETCh:PULSe:STATistics:PPOWer?	Returns the peak power of the statistics.
:FETCh:PULSe:STATistics:PPPHase?	Returns the pulse-pulse carrier phase of the statistics.
:FETCh:PULSe:STATistics:RINTerval?	Returns the repetition interval of the statistics.
:FETCh:PULSe:STATistics:RIPPLe?	Returns the ripple of the statistics.
:FETCh:PULSe:STATistics:RISE?	Returns the rise time of the statistics.
:FETCh:PULSe:STATistics:RMSFRqerror?	Returns the RMS frequency error of the statistics.
:FETCh:PULSe:STATistics:RMSPHerror?	Returns the RMS phase error of the statistics.
:FETCh:PULSe:STATistics:RRATE?	Returns the repetition rate of the statistics.
:FETCh:PULSe:STATistics:WIDTH?	Returns the pulse width of the statistics.
:FETCh:PULSe:TRACe?	Returns the waveform data of the pulse trace measurement.
:FETCh:SGRam subgroup	Spectrogram measurement
:FETCh:SGRam?	Returns the spectrogram trace data.
:FETCh:SPECTrum subgroup	Spectrum measurement
:FETCh:SPECTrum:TRACe<x>?	Returns the trace data in the Spectrum Analyzer measurement.
:FETCh:SQUality subgroup (Option 21 only)	Signal quality measurement
:FETCh:SQUality:FREQuency:ERRor?	Returns the frequency error.
:FETCh:SQUality:GAIN:IMBalance?	Returns the gain imbalance.
:FETCh:SQUality:ORIGin:OFFSet?	Returns the origin offset.
:FETCh:SQUality:PEAK:EVM?	Returns the peak EVM (%).
:FETCh:SQUality:PEAK:EVM:DB?	Returns the peak EVM (dB).
:FETCh:SQUality:PEAK:EVM:LOCation?	Returns the time at which the EVM is peak.
:FETCh:SQUality:PEAK:MERRor?	Returns the peak magnitude error (%).
:FETCh:SQUality:PEAK:MERRor:DB?	Returns the peak magnitude error (dB).
:FETCh:SQUality:PEAK:MERRor:LOCation?	Returns the time at which the magnitude error is peak.
:FETCh:SQUality:PEAK:PERRor?	Returns the peak phase error.
:FETCh:SQUality:PEAK:PERRor:LOCation?	Returns the time at which the phase error is peak.
:FETCh:SQUality:QUADrature:ERRor?	Returns the quadrature error.
:FETCh:SQUality:RHO?	Returns the ρ (waveform quality).

Table 2- 14: FETCh commands (Cont.)

Header	Description
:FETCh:SQUality:RMS:EVM?	Returns the RMS EVM (%).
:FETCh:SQUality:RMS:EVM:DB?	Returns the RMS EVM (dB).
:FETCh:SQUality:RMS:MERRor?	Returns the RMS magnitude error (%).
:FETCh:SQUality:RMS:MERRor:DB?	Returns the RMS magnitude error (dB).
:FETCh:SQUality:RMS:PERRor?	Returns the RMS phase error.
:FETCh:TOVerview subgroup	Time overview
:FETCh:TOVerview?	Returns the trace data.

INITiate Commands

Use the INITiate commands to control the acquisition of data.

Table 2- 15: INITiate commands

Header	Description
:INITiate:CONTinuous(?)	Selects or queries whether to acquire data continuously.
:INITiate[:IMMediate]	Starts data acquisition.

INPut Commands

Use the INPut commands to control the characteristics of the signal input.

Table 2- 16: INPut commands

Header	Description
:INPut[:RF]:ATTenuation(?)	Sets or queries the input attenuation.
:INPut[:RF]:ATTenuation :AUTO(?)	Selects or queries whether to set the attenuation automatically.
:INPut[:RF]:GAIN:STATe(?) (Option 01 only)	Selects or queries whether to enable the internal preamplifier.
:INPut:MLEVel[:RLEVel](?)	Sets or queries the reference level.

MMEMory Commands

Use the MMEMory commands to manipulate files on the mass memory devices.

Table 2- 17: :MMEMory commands

Header	Description
:MMEMory basic command subgroup	General file control
:MMEMory:CALibration:LOAD:CORRection:EXTernal:EDIT<x>	Loads an external loss table from a specified file.
:MMEMory:CALibration:STORe:CORRection:EXTernal:EDIT<x>	Stores an external loss table to a specified file.
:MMEMory:LOAD:IQ	Loads time-domain IQ waveform into the acquisition memory.
:MMEMory:LOAD:STATe	Loads the instrument setup from a specified file.
:MMEMory:LOAD:TRACe	Loads trace data from the specified file.
:MMEMory:STORe:IQ	Stores time-domain IQ waveform in the acquisition memory to a file.
:MMEMory:STORe:IQ:CSV	Stores time-domain IQ waveform to a file in the CSV format.
:MMEMory:STORe:IQ:MAT	Stores time-domain IQ waveform to a file in the MATLAB format.
:MMEMory:STORe:MSTate	Stores the measurement parameters in a specified file.
:MMEMory:STORe:RESults	Stores the measurement results in a specified file.
:MMEMory:STORe:STATe	Stores the instrument setup in a specified file.
:MMEMory:STORe:TRACe	Stores trace data in a specified file.
:MMEMory:AVTime subgroup	Amplitude versus Time measurement
:MMEMory:AVTime:LOAD:TRACe<x>	Loads trace data from the specified file.
:MMEMory:AVTime:STORe:TRACe<x>	Stores trace data in the specified file.
:MMEMory:CCDF subgroup	CCDF measurement
:MMEMory:CCDF:LOAD:TRACe<x>	Loads trace data from the specified file.
:MMEMory:CCDF:STORe:TRACe<x>	Stores trace data in the specified file.
:MMEMory:DPSA subgroup	DPX spectrum measurement
:MMEMory:DPSA:LOAD:TRACe<x>	Loads trace data from the specified file.
:MMEMory:DPSA:STORe:TRACe<x>	Stores trace data in the specified file.
:MMEMory:FVTime subgroup	Frequency versus Time measurement
:MMEMory:FVTime:LOAD:TRACe	Loads trace data from the specified file.
:MMEMory:FVTime:STORe:TRACe	Stores trace data in the specified file.
:MMEMory:IQVTime subgroup	RF I&Q versus Time measurement
:MMEMory:IQVTime:LOAD:TRACe:I	Loads I trace data from the specified file.
:MMEMory:IQVTime:LOAD:TRACe:Q	Loads Q trace data from the specified file.
:MMEMory:IQVTime:STORe:TRACe:I	Stores I trace data in the specified file.
:MMEMory:IQVTime:STORe:TRACe:Q	Stores Q trace data in the specified file.

Table 2- 17: :MMEMory commands (Cont.)

Header	Description
:MMEMory:PHVTime subgroup	Phase versus Time measurement
:MMEMory:PHVTime:LOAD:TRACe	Loads trace data from the specified file.
:MMEMory:PHVTime:STORe:TRACe	Stores trace data in the specified file.
:MMEMory:SPECTrum subgroup	Spectrum measurement
:MMEMory:SPECTrum:LOAD:TRACe<x>	Loads trace data from the specified file.
:MMEMory:SPECTrum:STORe:TRACe<x>	Stores trace data in the specified file.

OUTPut Commands

Use the OUTPut commands to control the characteristics of the signal output.

Table 2- 18: OUTPut commands

Header	Description
:OUTPut:IF:BANDwidth[:BWIDth(?)] (Option 05 only)	Selects or queries the IF output filter.
:OUTPut:IF[:STATe](?) (Option 05 only)	Selects or queries whether to turn on or off IF output.
:OUTPut:IQ[:STATe](?) (Option 05 only)	Selects or queries whether to turn on or off IQ output.
:OUTPut:NOISe[:STATe](?)	Selects or queries whether to turn on or off 28 V DC power.

READ Commands

The READ commands acquire an input signal once in the single mode and obtain the measurement results from that data.

To fetch the measurement results from the data currently residing in the memory without acquiring the input signal, use the FETCH commands.

Table 2- 19: READ commands

Header	Description
:READ:ACPower subgroup	ACPR measurement
:READ:ACPower?	Returns the ACPR measurement results.
:READ:ACPower:CHANnel:POWer?	Returns the average power of the main channel.
:READ:ACPower:SPECtrum?	Returns spectrum trace data of the ACPR measurement.
:READ:AVTime subgroup	Amplitude versus Time measurement
:READ:AVTime:AVERage?	Returns the RMS value.
:READ:AVTime:FIRST :SECond :THIRd :FOURth?	Returns the trace data.
:READ:AVTime:MAXimum?	Returns the maximum value.
:READ:AVTime:MAXLocation?	Returns the time at the maximum.
:READ:AVTime:MINimum?	Returns the minimum value.
:READ:AVTime:MINLocation?	Returns the time at the minimum.
:READ:AVTime:RESult?	Returns the measurement results.
:READ:CCDF subgroup	CCDF measurement
:READ:CCDF?	Returns the CCDF measurement results.
:READ:CCDF:FIRST :SECond :THIRd?	Returns waveform data of the specified trace.
:READ:CONSte subgroup (Option 21 only)	Constellation measurement
:READ:CONSte:RESults?	Returns the constellation measurement results.
:READ:CONSte:TRACe?	Returns the constellation trace data.
:READ:DDEMod subgroup (Option 21 only)	General purpose digital modulation measurements
:READ:DDEMod:STABle?	Returns the symbol table data.
:READ:DPsA subgroup	DPX spectrum measurement
:READ:DPsA:TRACe:AVERage?	Returns waveform data of the average trace.
:READ:DPsA:TRACe:MATH?	Returns waveform data of the math trace.
:READ:DPsA:TRACe:MAXimum?	Returns waveform data of the maximum trace.
:READ:DPsA:TRACe:MINimum?	Returns waveform data of the minimum trace.

Table 2- 19: READ commands (Cont.)

Header	Description
:READ:EVM subgroup (Option 21 only)	EVM versus Time measurement
:READ:EVM:FERRor?	Returns the frequency error.
:READ:EVM:PEAK?	Returns the peak value.
:READ:EVM:PINDEX?	Returns the time at the EVM peak.
:READ:EVM:RMS?	Returns the RMS value.
:READ:EVM:TRACE?	Returns the EVM versus Time trace data.
:READ:FVTime subgroup	Frequency versus Time measurement
:READ:FVTime?	Returns the Frequency versus Time trace data.
:READ:FVTime:MAXimum?	Returns the maximum value.
:READ:FVTime:MAXLocation?	Returns the time at which the frequency drift is maximum.
:READ:FVTime:MINimum?	Returns the minimum value.
:READ:FVTime:MINLocation?	Returns the time at which the frequency drift is minimum.
:READ:FVTime:RESult?	Returns the measurement results.
:READ:IQVTime subgroup	RF I&Q versus Time measurement
:READ:IQVTime:I?	Returns the I versus Time trace data.
:READ:IQVTime:MAXimum?	Returns the maximum value.
:READ:IQVTime:MAXLocation?	Returns the time at which the I or Q level is maximum.
:READ:IQVTime:MINimum?	Returns the minimum value.
:READ:IQVTime:MINLocation?	Returns the time at which the I or Q level is minimum.
:READ:IQVTime:Q?	Returns the Q versus Time trace data.
:READ:IQVTime:RESult?	Returns the measurement results.
:READ:MCPower subgroup	MCPR measurement
:READ:MCPower:ADJacent:CHANnels?	Returns the power of adjacent channels.
:READ:MCPower:CHANnel:POWer?	Returns the reference power.
:READ:MCPower:MAIN:CHANnels?	Returns the power of main channels.
:READ:MCPower:SPECTrum?	Returns spectrum trace data.
:READ:MERRor subgroup (Option 21 only)	Magnitude error versus Time measurement
:READ:MERRor:FERRor?	Returns the frequency error.
:READ:MERRor:PEAK?	Returns the peak value.
:READ:MERRor:PINDEX?	Returns the time at the magnitude error peak.
:READ:MERRor:RMS?	Returns the RMS value.
:READ:MERRor:TRACE?	Returns the Magnitude error versus Time trace data.

Table 2- 19: READ commands (Cont.)

Header	Description
:READ:PERRor subgroup (Option 21 only)	Phase error versus Time measurement
:READ:PERRor:FERRor?	Returns the frequency error.
:READ:PERRor:PEAK?	Returns the peak value.
:READ:PERRor:PINDeX?	Returns the time at the phase error peak.
:READ:PERRor:RMS?	Returns the RMS value.
:READ:PERRor:TRACe?	Returns the Phase error versus Time trace data.
:READ:OBWidth subgroup	Occupied Bandwidth measurement
:READ:OBWidth:FREQuency:ERRor?	Returns the frequency error.
:READ:OBWidth:OBWidth:BANDwidth?	Returns the occupied bandwidth.
:READ:OBWidth:OBWidth:LEFT:FREQuency?	Returns the left (lower) frequency of the occupied bandwidth.
:READ:OBWidth:OBWidth:LEFT:LEVel?	Returns the level at the left frequency of the occupied bandwidth.
:READ:OBWidth:OBWidth:POWer?	Returns the reference power in the Occupied Bandwidth measurement.
:READ:OBWidth:OBWidth:RIGHT:FREQuency?	Returns the right (higher) frequency of the occupied bandwidth.
:READ:OBWidth:OBWidth:RIGHT:LEVel?	Returns the level at the right frequency of the occupied bandwidth.
:READ:OBWidth:SPECtrum?	Returns spectrum trace data of the Occupied Bandwidth measurement.
:READ:OBWidth:XDBBbandwidth:BANDwidth?	Returns the x dB bandwidth.
:READ:OBWidth:XDBBbandwidth:LEFT:FREQuency?	Returns the left (lower) frequency of the x dB bandwidth.
:READ:OBWidth:XDBBbandwidth:LEFT:LEVel?	Returns the level at the left frequency of the x dB bandwidth.
:READ:OBWidth:XDBBbandwidth:POWer?	Returns the reference power in the x dB bandwidth measurement.
:READ:OBWidth:XDBBbandwidth:RIGHT:FREQuency?	Returns the right (higher) frequency of the x dB bandwidth.
:READ:OBWidth:XDBBbandwidth:RIGHT:LEVel?	Returns the level at the right frequency of the x dB bandwidth.
:READ:PHVTime subgroup	Phase versus Time measurement
:READ:PHVTime?	Returns the Phase versus Time trace data.
:READ:PHVTime:MAXimum?	Returns the maximum value.
:READ:PHVTime:MAXLocation?	Returns the time at which the phase is maximum.
:READ:PHVTime:MINimum?	Returns the minimum value.
:READ:PHVTime:MINLocation?	Returns the time at which the phase is minimum.
:READ:PHVTime:RESult?	Returns the results.
:READ:PULSe subgroup (Option 20 only)	Pulsed RF measurements
:READ:PULSe[:RESult]:ATX?	Returns the average transmitted power in the results table.
:READ:PULSe[:RESult]:AVERage?	Returns the average on power in the results table.
:READ:PULSe[:RESult]:DROOp?	Returns the droop in the results table.
:READ:PULSe[:RESult]:DUTPct?	Returns the duty factor (%) in the results table.
:READ:PULSe[:RESult]:DUTRatio?	Returns the duty factor (ratio) in the results table.

Table 2- 19: READ commands (Cont.)

Header	Description
:READ:PULSe[:RESult]:FALL?	Returns the fall time in the results table.
:READ:PULSe[:RESult]:FRDeviation?	Returns the frequency deviation in the results table.
:READ:PULSe[:RESult]:MFRqerror?	Returns the maximum frequency error in the results table.
:READ:PULSe[:RESult]:MPHerror?	Returns the maximum phase error in the results table.
:READ:PULSe[:RESult]:PHDeviation?	Returns the phase deviation in the results table.
:READ:PULSe[:RESult]:PPFRequency?	Returns the pulse-pulse carrier frequency in the results table.
:READ:PULSe[:RESult]:PPOwer?	Returns the peak power in the results table.
:READ:PULSe[:RESult]:PPPHase?	Returns the pulse-pulse carrier phase in the results table.
:READ:PULSe[:RESult]:RINTerval?	Returns the repetition interval in the results table.
:READ:PULSe[:RESult]:RIPple?	Returns the ripple in the results table.
:READ:PULSe[:RESult]:RISE?	Returns the rise time in the results table.
:READ:PULSe[:RESult]:RMSFRqerror?	Returns the RMS frequency error in the results table.
:READ:PULSe[:RESult]:RMSPherror?	Returns the RMS phase error in the results table.
:READ:PULSe[:RESult]:RRAtE?	Returns the repetition rate in the results table.
:READ:PULSe[:RESult]:TIME?	Returns the time in the results table.
:READ:PULSe[:RESult]:WIDTh?	Returns the pulse width in the results table.
:READ:PULSe:STATistics?	Returns the trace data of the pulse statistics measurement.
:READ:PULSe:STATistics:ATX?	Returns the average transmitted power of the statistics.
:READ:PULSe:STATistics:AVERage?	Returns the average on power of the statistics.
:READ:PULSe:STATistics:DROop?	Returns the droop of the statistics.
:READ:PULSe:STATistics:DUTPct?	Returns the duty factor (%) of the statistics.
:READ:PULSe:STATistics:DUTRatio?	Returns the duty factor (ratio) of the statistics.
:READ:PULSe:STATistics:FALL?	Returns the fall time of the statistics.
:READ:PULSe:STATistics:FRDeviation?	Returns the frequency deviation of the statistics.
:READ:PULSe:STATistics:MFRqerror?	Returns the maximum frequency error of the statistics.
:READ:PULSe:STATistics:MPHerror?	Returns the maximum phase error of the statistics.
:READ:PULSe:STATistics:PHDeviation?	Returns the phase deviation of the statistics.
:READ:PULSe:STATistics:PPFRequency?	Returns the pulse-pulse carrier frequency of the statistics.
:READ:PULSe:STATistics:PPOwer?	Returns the peak power of the statistics.
:READ:PULSe:STATistics:PPPHase?	Returns the pulse-pulse carrier phase of the statistics.
:READ:PULSe:STATistics:RINTerval?	Returns the repetition interval of the statistics.
:READ:PULSe:STATistics:RIPple?	Returns the ripple of the statistics.
:READ:PULSe:STATistics:RISE?	Returns the rise time of the statistics.
:READ:PULSe:STATistics:RMSFRqerror?	Returns the RMS frequency error of the statistics.
:READ:PULSe:STATistics:RMSPherror?	Returns the RMS phase error of the statistics.

Table 2- 19: READ commands (Cont.)

Header	Description
:READ:PULSe:STATistics:RRATe?	Returns the repetition rate of the statistics.
:READ:PULSe:STATistics:WIDTh?	Returns the pulse width of the statistics.
:READ:PULSe:TRACe?	Returns the waveform data of the pulse trace measurement.
:READ:SGRam subgroup	Spectrogram measurement
:READ:SGRam?	Returns the spectrogram trace data.
:READ:SPECtrum subgroup	Spectrum measurement
:READ:SPECtrum:TRACe<x>?	Returns the trace data in the Spectrum Analyzer measurement.
:READ:SQUality subgroup (Option 21 only)	Signal quality measurement
:READ:SQUality:FREQuency:ERRor?	Returns the frequency error.
:READ:SQUality:GAIN:IMBalance?	Returns the gain imbalance.
:READ:SQUality:ORIGin:OFFSet?	Returns the origin offset.
:READ:SQUality:PEAK:EVM?	Returns the peak EVM (%).
:READ:SQUality:PEAK:EVM:DB?	Returns the peak EVM (dB).
:READ:SQUality:PEAK:EVM:LOCation?	Returns the time at which the EVM is peak.
:READ:SQUality:PEAK:MERRor?	Returns the peak magnitude error (%).
:READ:SQUality:PEAK:MERRor:DB?	Returns the peak magnitude error (dB).
:READ:SQUality:PEAK:MERRor:LOCation?	Returns the time at which the magnitude error is peak.
:READ:SQUality:PEAK:PERRor?	Returns the peak phase error.
:READ:SQUality:PEAK:PERRor:LOCation?	Returns the time at which the phase error is peak.
:READ:SQUality:QUADrature:ERRor?	Returns the quadrature error.
:READ:SQUality:RHO?	Returns the ρ (waveform quality).
:READ:SQUality:RMS:EVM?	Returns the RMS EVM (%).
:READ:SQUality:RMS:EVM:DB?	Returns the RMS EVM (dB).
:READ:SQUality:RMS:MERRor?	Returns the RMS magnitude error (%).
:READ:SQUality:RMS:MERRor:DB?	Returns the RMS magnitude error (dB).
:READ:SQUality:RMS:PERRor?	Returns the RMS phase error.
:READ:TOVerview subgroup	Time overview
:READ:TOVerview?	Returns the trace data.

SENSe Commands

Use the SENSe commands to set up detailed measurement conditions.

Table 2- 20: SENSe commands

Header	Description
[[:SENSe]:] basic command subgroup	General analysis parameter control
[[:SENSe]:]ACQuisition:BANDwidth[:BWIDth(?)]	Sets or queries the acquisition bandwidth.
[[:SENSe]:]ACQuisition:FFRame:ACTual?	Queries the actual number of Fast Frames.
[[:SENSe]:]ACQuisition:FFRame:Limit(?]	Sets or queries the limit number of Fast Frames.
[[:SENSe]:]ACQuisition:FFRame:STATe(?]	Determines whether to enable or disable the Fast Frame.
[[:SENSe]:]ACQuisition:MEMory:AVAIlable:SAMPles?	Returns the amount of acquisition memory available in the instrument.
[[:SENSe]:]ACQuisition:MEMory:CAPacity[:TIME]?	Returns the acquisition memory capacity.
[[:SENSe]:]ACQuisition:MEMory:USED[:PERCent]?	Returns the percentage of the capacity used.
[[:SENSe]:]ACQuisition:MODE(?]	Selects or queries the acquisition mode.
[[:SENSe]:]ACQuisition:SAMPles(?]	Sets or queries the acquisition samples.
[[:SENSe]:]ACQuisition:SEConds(?]	Sets or queries the acquisition length.
[[:SENSe]:]ANALysis:ADVanced:DITHer(?]	Determines whether to enable or disable dithering.
[[:SENSe]:]ANALysis:LENGth(?]	Sets or queries the analysis length.
[[:SENSe]:]ANALysis:LENGth:ACTual?	Queries the actual analysis length.
[[:SENSe]:]ANALysis:LENGth:AUTO(?]	Selects or queries whether to set the analysis length automatically.
[[:SENSe]:]ANALysis:REFerence(?]	Selects or queries the analysis time reference.
[[:SENSe]:]ANALysis:STARt(?]	Sets or queries the analysis offset time.
[[:SENSe]:]ANALysis:STARt:AUTO(?]	Selects or queries whether to set the analysis offset automatically.
[[:SENSe]:]MEASurement:FREQuency(?]	Sets or queries the measurement frequency.
[[:SENSe]:]POWER:UNITs(?]	Selects or queries the unit of power.
[[:SENSe]:]REANalyze	Have all measurements reanalyze the current acquisition record.
[[:SENSe]:]ROSCillator:SOURce(?]	Selects or queries the reference oscillator source.
[[:SENSe]:]SPECtrum:LENGth(?]	Sets or queries the spectrum length.
[[:SENSe]:]SPECtrum:LENGth:ACTual?	Queries the actual spectrum length.
[[:SENSe]:]SPECtrum:LENGth:AUTO(?]	Selects or queries whether to set the spectrum length automatically.
[[:SENSe]:]SPECtrum:STARt(?]	Sets or queries the spectrum offset time.
[[:SENSe]:]SPECtrum:TIME:MODE(?]	Selects or queries whether to set the spectrum time automatically.

Table 2-20: SENSE commands (Cont.)

Header	Description
[[:SENSe]:ACPower subgroup	ACPR measurement
[[:SENSe]:ACPower:AVERage(?)]	Selects or queries how to average waveform.
[[:SENSe]:ACPower:AVERage:COUNt(?)]	Sets or queries the number of traces for averaging.
[[:SENSe]:ACPower:BANDwidth[:BWIDth[:RESolution]](?)]	Sets or queries the resolution bandwidth (RBW).
[[:SENSe]:ACPower:BANDwidth[:BWIDth[:RESolution]]:ACTual?]	Queries the actual resolution bandwidth (RBW).
[[:SENSe]:ACPower:BANDwidth[:BWIDth[:RESolution]]:AUTO(?)]	Selects or queries whether to set the RBW automatically.
[[:SENSe]:ACPower:CHANnel:BANDwidth[:BWIDth(?)]	Sets or queries the channel bandwidth.
[[:SENSe]:ACPower:CHANnel:FILTer(?)]	Selects or queries the adjacent channel filter.
[[:SENSe]:ACPower:CHANnel:PAIRs(?)]	Sets or queries the number of adjacent channel pairs.
[[:SENSe]:ACPower:CHANnel:SPACing(?)]	Sets or queries the channel-to-channel spacing.
[[:SENSe]:ACPower:CHIPrate(?)]	Sets or queries the chip rate.
[[:SENSe]:ACPower:CLEar:RESults]	Restarts the average trace.
[[:SENSe]:ACPower:FREQuency:STEP(?)]	Sets or queries the frequency step size.
[[:SENSe]:ACPower:FREQuency:STEP:AUTO(?)]	Selects or queries whether to set the frequency step size automatically.
[[:SENSe]:ACPower:NFLoor:STATe(?)]	Selects or queries whether to enable the correction for noise floor.
[[:SENSe]:ACPower:OPTimize:SPAN(?)]	Selects or queries the optimization method.
[[:SENSe]:ACPower:RRCRolloff(?)]	Sets or queries the filter parameter for the Root Raised Cosine filter.
[[:SENSe]:AVTime subgroup	Amplitude versus Time measurement
[[:SENSe]:AVTime:BANDwith[:BWIDth(?)]	Sets or queries the time-domain bandwidth filter.
[[:SENSe]:AVTime:BANDwidth[:BWIDth[:RESolution]]:ACTual?]	Queries the actual resolution bandwidth (RBW).
[[:SENSe]:AVTime:CLEar:RESults]	Restarts multi-trace functions (Average and Max/Min Hold).
[[:SENSe]:AVTime:MAXTracepoints(?)]	Selects or queries the maximum trace points.
[[:SENSe]:AVTime:METHod(?)]	Selects or queries the method to set the measurement bandwidth.
[[:SENSe]:AVTime:SPAN(?)]	Sets or queries the frequency span.
[[:SENSe]:CCDF subgroup	CCDF measurement
[[:SENSe]:CCDF:BANDwidth[:BWIDth(?)]	Sets or queries the CCDF measurement bandwidth.
[[:SENSe]:CCDF:CLEar]	Clears the CCDF accumulator and restarts the measurement.
[[:SENSe]:CCDF:TIME:TOTal:LENGth(?)]	Sets or queries the CCDF measurement time.
[[:SENSe]:CCDF:TIME:TYPE(?)]	Selects or queries how to repeat the CCDF measurement.

Table 2-20: SENSE commands (Cont.)

Header	Description
[[:SENSe]:DDEMod subgroup (Option 21 only)	General purpose digital modulation measurements
[[:SENSe]:DDEMod:ANALysis:LENGth(?)]	Sets or queries the analysis length.
[[:SENSe]:DDEMod:ANALysis:LENGth:ACTual?]	Queries the actual analysis length.
[[:SENSe]:DDEMod:ANALysis:LENGth:AUTO(?)]	Selects or queries whether to set the analysis length automatically.
[[:SENSe]:DDEMod:BURSt:DETEct(?)]	Selects or queries how to detect bursts.
[[:SENSe]:DDEMod:BURSt:THREShold(?)]	Sets or queries the threshold level to determine a burst.
[[:SENSe]:DDEMod:CARRier:OFFSet(?)]	Sets or queries the carrier frequency offset.
[[:SENSe]:DDEMod:FILTer:ALPHa(?)]	Sets or queries the filter factor (α /BT).
[[:SENSe]:DDEMod:FILTer:MEASurement(?)]	Selects or queries the measurement filter.
[[:SENSe]:DDEMod:FILTer:REFerence(?)]	Selects or queries the reference filter.
[[:SENSe]:DDEMod:MAGNitude:NORMalize(?)]	Selects or queries the method for the magnitude normalization.
[[:SENSe]:DDEMod:MODulation:TYPE(?)]	Selects or queries the modulation type.
[[:SENSe]:DDEMod:SRATE(?)]	Sets or queries the symbol rate.
[[:SENSe]:DDEMod:SWAP:IQ(?)]	Selects or queries whether or not to swap I and Q data.
[[:SENSe]:DDEMod:SYMBol:POINts(?)]	Sets or queries the number of points per symbol.
[[:SENSe]:DDEMod:SYNCh:WORD(?)]	Selects or queries whether to enable the synchronization word.
[[:SENSe]:DDEMod:SYNCh:WORD:SYMBol(?)]	Sets or queries the synchronization word.
[[:SENSe]:DDEMod:TIME:UNITs(?)]	Selects or queries the fundamental unit of time.
[[:SENSe]:DPSA subgroup	DPX spectrum measurement
[[:SENSe]:DPSA:AUDio:DEMod:GAIN(?)]	Sets or queries the gain for the audio demodulation.
[[:SENSe]:DPSA:AUDio:DEMod:RXBWidth(?)]	Sets or queries the receiver bandwidth for the audio demodulation.
[[:SENSe]:DPSA:AUDio:DEMod:RXFRrequency?]	Queries the receiver frequency for the audio demodulation.
[[:SENSe]:DPSA:AUDio:DEMod:STATe(?)]	Selects or queries whether to enable or disable the audio demodulation.
[[:SENSe]:DPSA:AUDio:DEMod:TUNE(?)]	Selects or queries how to determine the tuning frequency.
[[:SENSe]:DPSA:AUDio:DEMod:TYPE(?)]	Selects or queries the modulation type for the audio demodulation.
[[:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]](?)]	Sets or queries the resolution bandwidth (RBW).
[[:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]]:AUTO(?)]	Selects or queries whether to set the RBW automatically.
[[:SENSe]:DPSA:CLEar:RESults]	Restarts multi-trace functions (Average and Max/Min Hold).
[[:SENSe]:DPSA:COLor(?)]	Selects or queries the color palette of three-dimensional graphs.
[[:SENSe]:DPSA:COLor:MAXimum(?)]	Sets or queries the maximum value of the color axis.
[[:SENSe]:DPSA:COLor:MINimum(?)]	Sets or queries the minimum value of the color axis.
[[:SENSe]:DPSA:FREQuency:CENTer(?)]	Sets or queries the center frequency.
[[:SENSe]:DPSA:FREQuency:SPAN(?)]	Sets or queries the frequency span.
[[:SENSe]:DPSA:FREQuency:STARt(?)]	Sets or queries the measurement start frequency.

Table 2-20: SENSE commands (Cont.)

Header	Description
[[:SENSe]:DPSA:FREQuency:STEP(?)]	Sets or queries the frequency step size.
[[:SENSe]:DPSA:FREQuency:STEP:AUTO(?)]	Selects or queries whether to set the frequency step size automatically.
[[:SENSe]:DPSA:FREQuency:STOP(?)]	Sets or queries the measurement stop frequency.
[[:SENSe]:FVTime subgroup]	Frequency versus Time measurement
[[:SENSe]:FVTime:CLear:RESults]	Restarts multi-trace functions (Average and Max/Min Hold).
[[:SENSe]:FVTime:FREQuency:CENTer(?)]	Sets or queries the center frequency.
[[:SENSe]:FVTime:FREQuency:SPAN(?)]	Sets or queries the frequency span.
[[:SENSe]:FVTime:FREQuency:STARt(?)]	Sets or queries the measurement start frequency.
[[:SENSe]:FVTime:FREQuency:STEP(?)]	Sets or queries the frequency step size.
[[:SENSe]:FVTime:FREQuency:STEP:AUTO(?)]	Selects or queries whether to set the frequency step size automatically.
[[:SENSe]:FVTime:FREQuency:STOP(?)]	Sets or queries the measurement stop frequency.
[[:SENSe]:FVTime:MAXTracepoints(?)]	Selects or queries the maximum trace points.
[[:SENSe]:IQVTime subgroup]	RF I&Q versus Time measurement
[[:SENSe]:IQVTime:CLear:RESults]	Restarts multi-trace functions (Average and Max/Min Hold).
[[:SENSe]:IQVTime:FREQuency:CENTer(?)]	Sets or queries the center frequency.
[[:SENSe]:IQVTime:FREQuency:SPAN(?)]	Sets or queries the frequency span.
[[:SENSe]:IQVTime:FREQuency:STARt(?)]	Sets or queries the measurement start frequency.
[[:SENSe]:IQVTime:FREQuency:STEP(?)]	Sets or queries the frequency step size.
[[:SENSe]:IQVTime:FREQuency:STEP:AUTO(?)]	Selects or queries whether to set the frequency step size automatically.
[[:SENSe]:IQVTime:FREQuency:STOP(?)]	Sets or queries the measurement stop frequency.
[[:SENSe]:IQVTime:MAXTracepoints(?)]	Selects or queries the maximum trace points.
[[:SENSe]:MCPower subgroup]	MCPR measurement
[[:SENSe]:MCPower:AVERage(?)]	Selects or queries how to average waveform.
[[:SENSe]:MCPower:AVERage:COUNt(?)]	Sets or queries the number of waveforms for average.
[[:SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]](?)]	Sets or queries the resolution bandwidth (RBW).
[[:SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]]:ACTual?]	Queries the actual resolution bandwidth (RBW).
[[:SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]]:AUTO(?)]	Selects or queries whether to set the RBW automatically.
[[:SENSe]:MCPower:CHANnel:ADJacent:ADD]	Adds a pair of upper and lower adjacent channels.
[[:SENSe]:MCPower:CHANnel:ADJacent:DELeTe]	Deletes a selected adjacent channel.
[[:SENSe]:MCPower:CHANnel:FILTer(?)]	Selects or queries the measurement filter.

Table 2-20: SENSE commands (Cont.)

Header	Description
[[:SENSe]:MCPower:CHANnel:MAIN:BANDwidth]:BWIDth(?)	Sets or queries the frequency bandwidth of the main channels.
[[:SENSe]:MCPower:CHANnel:MAIN:COUNT(?)]	Sets or queries the number of main channels.
[[:SENSe]:MCPower:CHANnel:MAIN:INACTive(?)]	Makes a main channel inactive or queries the inactive main channels.
[[:SENSe]:MCPower:CHANnel:MAIN:SPACing(?)]	Sets or queries the main channel spacing.
[[:SENSe]:MCPower:CHIPrate(?)]	Sets or queries the chip rate.
[[:SENSe]:MCPower:CLEar:RESults]	Restarts the average trace.
[[:SENSe]:MCPower:FREQuency:STEP(?)]	Sets or queries the frequency step size.
[[:SENSe]:MCPower:FREQuency:STEP:AUTO(?)]	Selects or queries whether to set the frequency step size automatically.
[[:SENSe]:MCPower:NFLoor:STATe(?)]	Selects or queries whether to enable the correction for noise floor.
[[:SENSe]:MCPower:OPTimize:SPAN(?)]	Selects or queries the optimization method.
[[:SENSe]:MCPower:RCHannels?	Queries the power reference.
[[:SENSe]:MCPower:RCHannels:MAIN<x>]	Sets the power reference to the main channel with the index (<x>).
[[:SENSe]:MCPower:RCHannels:TOTal]	Sets the power reference to the total power of all the active channels.
[[:SENSe]:MCPower:RRCRolloff(?)]	Sets or queries the filter parameter for the Root Raised Cosine filter.
[[:SENSe]:OBWidth subgroup]	Occupied Bandwidth measurement
[[:SENSe]:OBWidth:AVERage?	Selects or queries whether to enable or disable averaging.
[[:SENSe]:OBWidth:AVERage:COUNT(?)]	Sets or queries the number of measurements for averaging.
[[:SENSe]:OBWidth:BANDwidth]:BWIDth:MEASurement(?)]	Sets or queries the measurement bandwidth.
[[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution](?)	Sets or queries the resolution bandwidth (RBW).
[[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution]:ACTual?	Queries the actual resolution bandwidth (RBW).
[[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution]:AUTO(?)]	Selects or queries whether to set the RBW automatically.
[[:SENSe]:OBWidth:CLEar:RESults]	Restarts the averaging.
[[:SENSe]:OBWidth:FREQuency:CENTer(?)]	Sets or queries the center frequency.
[[:SENSe]:OBWidth:FREQuency:STEP(?)]	Sets or queries the frequency step size.
[[:SENSe]:OBWidth:FREQuency:STEP:AUTO(?)]	Determines whether to set the frequency step size automatically.
[[:SENSe]:OBWidth:PERCent(?)]	Sets or queries the occupied bandwidth percent power.
[[:SENSe]:OBWidth:XDBLevel(?)]	Sets or queries the x dB level.
[[:SENSe]:PHVTime subgroup]	Phase versus Time measurement
[[:SENSe]:PHVTime:CLEar:RESults]	Restarts multi-trace functions (Average and Max/Min Hold).
[[:SENSe]:PHVTime:FREQuency:CENTer(?)]	Sets or queries the center frequency.
[[:SENSe]:PHVTime:FREQuency:SPAN(?)]	Sets or queries the frequency span.
[[:SENSe]:PHVTime:FREQuency:STARt(?)]	Sets or queries the measurement start frequency.

Table 2-20: SENSE commands (Cont.)

Header	Description
[[:SENSe]:PHVTime:FREQuency:STEP(?]	Sets or queries the frequency step size.
[[:SENSe]:PHVTime:FREQuency:STEP:AUTO(?]	Selects or queries whether to set the frequency step size automatically.
[[:SENSe]:PHVTime:FREQuency:STOP(?]	Sets or queries the measurement stop frequency.
[[:SENSe]:PHVTime:MAXTracepoints(?]	Selects or queries the maximum trace points.
[[:SENSe]:PULSe subgroup (Option 20 only)	Pulsed RF measurements
[[:SENSe]:PULSe:ANALyze:LEVel(?]	Selects or queries how to determine the 50% level.
[[:SENSe]:PULSe:ANALyze:LEVel:FIFTy(?]	Selects or queries how to determine the 50% level.
[[:SENSe]:PULSe:ANALyze:LEVel:HUNDred(?]	Selects or queries how to determine the 50% level.
[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:AUTO(?]	Selects or queries whether to set the measurement time automatically.
[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:START(?]	Sets or queries the measurement start time.
[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:STOP(?]	Sets or queries the measurement stop time.
[[:SENSe]:PULSe:ANALyze:PMLocation(?]	Sets or queries the phase measurement location.
[[:SENSe]:PULSe:ANALyze:POINT:LOCation(?]	Selects or queries the point location method.
[[:SENSe]:PULSe:ANALyze:RFALI(?]	Selects or queries the threshold levels to measure the rise/fall time.
[[:SENSe]:PULSe:ANALyze:RIPPlE(?]	Sets or queries the ripple portion of the pulse top.
[[:SENSe]:PULSe:CARRier:OFFSet(?]	Sets or queries the carrier frequency offset.
[[:SENSe]:PULSe:CARRier:SEARCh(?]	Selects or queries how to detect the carrier.
[[:SENSe]:PULSe:DETEct:MEASurement(?]	Selects or queries whether to set the maximum number of pulses.
[[:SENSe]:PULSe:DETEct:NUMBER(?]	Sets or queries the maximum number of pulses to detect.
[[:SENSe]:PULSe:DETEct:POWER[:THReshold](?]	Sets or queries the power threshold to detect pulses.
[[:SENSe]:PULSe:DETEct:TIME[:THReshold](?]	Sets or queries the minimum off-time between pulses.
[[:SENSe]:PULSe:FILTer:BANDwidth[:BWIDth](?]	Sets or queries the the filter bandwidth for the Gaussian filter.
[[:SENSe]:PULSe:FILTer:MEASurement(?]	Selects or queries the measurement filter.
[[:SENSe]:PULSe:FREFerence:AUTO(?]	Determines whether to estimate the frequency reference automatically.
[[:SENSe]:PULSe:FREFerence:CHIRpbw(?]	Sets or queries the chirp bandwidth.
[[:SENSe]:PULSe:FREFerence:OFFSet(?]	Sets or queries the frequency reference offset.
[[:SENSe]:PULSe:MODulation:TYPE(?]	Selects or queries the modulation type.
[[:SENSe]:PULSe:SIGNAL:TYPE(?]	Selects or queries the signal type.
[[:SENSe]:SGRam subgroup	Spectrogram measurement
[[:SENSe]:SGRam:BANDwidth[:BWIDth]:OPTimization(?]	Selects or queries the method of optimizing gain and input bandwidth.
[[:SENSe]:SGRam:BANDwidth[:BWIDth]:RESolution](?]	Sets or queries the resolution bandwidth (RBW).
[[:SENSe]:SGRam:BANDwidth[:BWIDth]:RESolution] :ACTual?	Queries the actual resolution bandwidth (RBW).
[[:SENSe]:SGRam:BANDwidth[:BWIDth]:RESolution] :AUTO(?]	Selects or queries whether to set the RBW automatically.

Table 2-20: SENSE commands (Cont.)

Header	Description
[[:SENSe]:SGRam:BANDwidth]:BWIDth[:RESolution]:MODE(?)	Determines whether to enable or disable the RBW processing.
[[:SENSe]:SGRam:COLor(?)]	Selects or queries the color palette of three-dimensional graphs.
[[:SENSe]:SGRam:COLor:MAXimum(?)]	Sets or queries the maximum value of the color axis.
[[:SENSe]:SGRam:COLor:MINimum(?)]	Sets or queries the minimum value of the color axis.
[[:SENSe]:SGRam:FFT:WINDow(?)]	Selects or queries the FFT window.
[[:SENSe]:SGRam:FREQuency:CENTer(?)]	Sets or queries the center frequency.
[[:SENSe]:SGRam:FREQuency:SPAN(?)]	Sets or queries the frequency span.
[[:SENSe]:SGRam:FREQuency:SPAN:BANDwidth[:RESolution]:RATio(?)]	Sets or queries the ratio of span to RBW.
[[:SENSe]:SGRam:FREQuency:SPAN:MAXimum]	Sets the frequency range to the maximum real-time span.
[[:SENSe]:SGRam:FREQuency:STARt(?)]	Sets or queries the measurement start frequency.
[[:SENSe]:SGRam:FREQuency:STEP(?)]	Sets or queries the frequency step size.
[[:SENSe]:SGRam:FREQuency:STEP:AUTO(?)]	Selects or queries whether to set the frequency step size automatically.
[[:SENSe]:SGRam:FREQuency:STOP(?)]	Sets or queries the measurement stop frequency.
[[:SENSe]:SPECTrum subgroup]	Spectrum measurement
[[:SENSe]:SPECTrum:BANDwidth]:BWIDth:OPTimization(?)]	Selects or queries the method of optimizing gain and input bandwidth.
[[:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution](?)	Sets or queries the resolution bandwidth (RBW).
[[:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution]:ACTual?	Queries the actual resolution bandwidth (RBW).
[[:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution]:AUTO(?)]	Selects or queries whether to set the RBW automatically.
[[:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution]:MODE(?)]	Selects or queries whether to enable or disable the RBW process.
[[:SENSe]:SPECTrum:CLEar:RESults]	Restarts multi-trace functions (Average and Max/Min Hold).
[[:SENSe]:SPECTrum:FFT:WINDow(?)]	Selects or queries the FFT window.
[[:SENSe]:SPECTrum:FREQuency:CENTer(?)]	Sets or queries the center frequency.
[[:SENSe]:SPECTrum:FREQuency:SPAN(?)]	Sets or queries the frequency span.
[[:SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio(?)]	Sets or queries the ratio of span to RBW.
[[:SENSe]:SPECTrum:FREQuency:STARt(?)]	Sets or queries the measurement start frequency.
[[:SENSe]:SPECTrum:FREQuency:STEP(?)]	Sets or queries the frequency step size.
[[:SENSe]:SPECTrum:FREQuency:STEP:AUTO(?)]	Selects or queries whether to set the frequency step size automatically.
[[:SENSe]:SPECTrum:FREQuency:STOP(?)]	Sets or queries the measurement stop frequency.
[[:SENSe]:SPECTrum:MAX:SPAN]	Sets the frequency span to the maximum real-time span.
[[:SENSe]:SPECTrum:POINts:COUNt(?)]	Sets or queries the number of sample points on the signal spectrum.

Table 2-20: SENSE commands (Cont.)

Header	Description
[[:SENSE]:TOVerview subgroup	Time overview
[[:SENSE]:TOVerview:FREQuency:CENTer(?)]	Sets or queries the center frequency.
[[:SENSE]:TOVerview:MAXTracepoints(?)]	Selects or queries the maximum trace points.

STATUS Commands

Use the STATUS commands to control registers defined in the SCPI status reporting structure.

Table 2-21: STATUS commands

Header	Description
:STATUS:ACPower:EVENTs?	Returns the current events for the ACPR measurement.
:STATUS:AVTime:EVENTs?	Returns the current events for the Amplitude versus Time measurement.
:STATUS:CCDF:EVENTs?	Returns the current events for the CCDF measurement.
:STATUS:CONSt:EVENTs?	Returns the current events for the Constellation measurement.
:STATUS:DPSA:EVENTs?	Returns the current events for the DPX spectrum measurement.
:STATUS:EVM:EVENTs?	Returns the current events for the EVM versus Time measurement.
:STATUS:FVTime:EVENTs?	Returns the current events for the Frequency versus Time measurement.
:STATUS:IQVTime:EVENTs?	Returns the current events for the RF I&Q versus Time measurement.
:STATUS:MCPower:EVENTs?	Returns the current events for the MCPR measurement.
:STATUS:MERRor:EVENTs?	Returns the current events for the Mag error versus Time measurement.
:STATUS:OBWidth:EVENTs?	Returns the current events for the Occupied Bandwidth measurement.
:STATUS:OPERation:CONDition?	Queries the contents of the OCR.
:STATUS:OPERation:ENABle(?)	Sets or queries the mask for the OENR.
:STATUS:OPERation[:EVENT]?	Queries the contents of the OEVR.
:STATUS:OPERation:NTRansition(?)	Sets or queries the value of the negative transition filter.
:STATUS:OPERation:PTRansition(?)	Sets or queries the value of the positive transition filter.
:STATUS:PERRor:EVENTs?	Returns the current events for the Phase error measurement.
:STATUS:PHVTime:EVENTs?	Returns the current events for the Phase versus Time measurement.
:STATUS:PRESet	Presets a status byte.
:STATUS:PULSe:RESult:EVENTs?	Returns the current events for the pulse table measurement.
:STATUS:PULSe:STATistics:EVENTs?	Returns the current events for the pulse statistics measurement.
:STATUS:PULSe:TRACe:EVENTs?	Returns the current events for the pulse trace measurement.

Table 2-21: STATus commands (Cont.)

Header	Description
:STATus:QUESTionable:CONDition?	Queries the contents of the QCR.
:STATus:QUESTionable:ENABle(?)	Sets or queries the mask for the OENR.
:STATus:QUESTionable[:EVENT]?	Queries the contents of the QER.
:STATus:QUESTionable:NTRansition(?)	Sets or queries the value of the negative transition filter.
:STATus:QUESTionable:PTRansition(?)	Sets or queries the value of the positive transition filter.
:STATus:QUESTionable:CALibration:CONDition?	Queries the contents of the questionable calibration condition register.
:STATus:QUESTionable:CALibration:ENABle(?)	Sets or queries the mask for the questionable calibration enable register.
:STATus:QUESTionable:CALibration[:EVENT]?	Queries the contents of the questionable calibration event register.
:STATus:QUESTionable:CALibration:NTRansition(?)	Sets or queries the value of the negative transition filter.
:STATus:QUESTionable:CALibration:PTRansition(?)	Sets or queries the value of the positive transition filter.
:STATus:QUESTionable:FREQuency:CONDition?	Queries the contents of the questionable frequency condition register.
:STATus:QUESTionable:FREQuency:ENABle(?)	Sets or queries the mask for the questionable frequency enable register.
:STATus:QUESTionable:FREQuency[:EVENT]?	Queries the contents of the questionable frequency event register.
:STATus:QUESTionable:FREQuency:NTRansition(?)	Sets or queries the value of the negative transition filter.
:STATus:QUESTionable:FREQuency:PTRansition(?)	Sets or queries the value of the positive transition filter.
:STATus:SGRam:EVENTs?	Returns the current events for the spectrogram measurement.
:STATus:SPECTrum:EVENTs?	Returns the current events for the spectrum measurement.
:STATus:SQUALity:EVENTs?	Returns the current events for the signal quality measurement.

SYSTem Commands

Use the SYSTem commands to set or query system parameters for operation.

Table 2-22: SYSTem commands

Header	Description
:SYSTem:COMMunicate:GPIB[:SELF]:ADDRes	Sets or queries the GPIB address of the instrument.
:SYSTem:DATE(?)	Sets or queries the current date.
:SYSTem:ERRor:ALL?	Queries all the error or event information.
:SYSTem:ERRor:CODE:ALL?	Queries all the error or event codes.
:SYSTem:ERRor:CODE[:NEXT]?	Queries the latest error or event information.
:SYSTem:ERRor:COUNt?	Queries the number of errors or events.
:SYSTem:ERRor[:NEXT]?	Queries the latest error or event information.
:SYSTem:OPTions?	Queries optional information.

Table 2-22: SYSTem commands (Cont.)

Header	Description
:SYSTem:PRESet	Presets the analyzer.
:SYSTem:TIME(?)	Sets or queries the current time.
:SYSTem:VERSion?	Queries the version of the SCPI.

TRACe Commands

Use the TRACe commands to select trace type and to control trace arithmetic.

Table 2-23: TRACe commands

Header	Description
:TRACe<x>:AVTime subgroup	Amplitude versus Time measurement
:TRACe<x>:AVTime(?)	Selects or queries whether or not to show the specified trace.
:TRACe<x>:AVTime:AVERage:COUNT(?)	Sets or queries the number of traces to combine for averaging.
:TRACe<x>:AVTime:AVERage:RESet	Clears the average data and resets the average counter.
:TRACe<x>:AVTime:COUNT(?)	Sets or queries the count for the Max or Min Hold trace.
:TRACe<x>:AVTime:COUNT:ENABle(?)	Selects or queries whether or not to enable the count for Max/Min Hold.
:TRACe<x>:AVTime:COUNT:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
:TRACe<x>:AVTime:FREeze(?)	Selects or queries whether or not to freeze the display of the trace.
:TRACe<x>:AVTime:FUNCTion(?)	Selects or queries the trace function.
:TRACe<x>:AVTime:LEFToperand(?)	Selects or queries the left operand for the math trace.
:TRACe<x>:AVTime:RIGHToperand(?)	Selects or queries the right operand for the math trace.
:TRACe<x>:AVTime:SElect(?)	Selects or queries the trace number to display the readout.
:TRACe<x>:CCDF subgroup	CCDF measurement
:TRACe<x>:CCDF:FREeze(?)	Selects or queries whether or not to freeze the display of the trace.
:TRACe<x>:CCDF:SElect(?)	Selects or queries the trace number to display the readout.
:TRACe<x>:CCDF:SHOW(?)	Selects or queries whether to show or hide the trace.
:TRACe<x>:CCDF:X(?)	Sets or queries the horizontal position of the measurement pointer.
:TRACe<x>:CCDF:Y?	Queries the vertical position (CCDF value) of the measurement pointer.
:TRACe<x>:CONStellation subgroup (Option 21 only)	Constellation measurement
:TRACe<x>:CONStellation:MODE(?)	Selects or queries how to display the constellation trace.
:TRACe<x>:DPSA subgroup	DPX spectrum measurement
:TRACe<x>:DPSA(?)	Selects or queries whether or not to show the waveform.
:TRACe<x>:DPSA:AVERage:COUNT(?)	Sets or queries the number of traces to combine for averaging.
:TRACe<x>:DPSA:COLor:INTensity(?)	Sets or queries the color intensity.

Table 2-23: TRACe commands (Cont.)

Header	Description
:TRACe<x>:DPSA:DOT:PERsistent(?)	Selects or queries whether to enable or disable the dot persistence.
:TRACe<x>:DPSA:DOT:PERsistent:TYPE(?)	Selects or queries the persistence type.
:TRACe<x>:DPSA:DOT:PERsistent:VARiable(?)	Sets or queries the length of time that data points are displayed.
:TRACe<x>:DPSA:FREeze(?)	Selects or queries whether or not to freeze the display of the trace.
:TRACe<x>:DPSA:FUNCTion(?)	Selects or queries the function.
:TRACe<x>:DPSA:LEFToperand(?)	Selects or queries the left operand for the math trace.
:TRACe<x>:DPSA:RIGHToperand(?)	Selects or queries the right operand for the math trace.
:TRACe<x>:DPSA:SElect(?)	Selects or queries the trace number to display the readout.
:TRACe:FVTime subgroup	Frequency versus Time measurement
:TRACe:FVTime(?)	Selects or queries whether or not to show the trace.
:TRACe:FVTime:AVERage:COUNt(?)	Sets or queries the number of traces to combine for averaging.
:TRACe:FVTime:COUNt(?)	Sets or queries the count for the Max or Min Hold trace.
:TRACe:FVTime:COUNt:ENABle(?)	Selects or queries whether or not to enable the count for Max/Min Hold.
:TRACe:FVTime:COUNt:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
:TRACe:FVTime:FREeze(?)	Selects or queries whether or not to freeze the display of the trace.
:TRACe:FVTime:FUNCTion(?)	Selects or queries the trace function.
:TRACe:IQVTime subgroup	RF I&Q versus Time measurement
:TRACe:IQVTime:AVERage:COUNt(?)	Sets or queries the number of traces to combine for averaging.
:TRACe:IQVTime:COUNt(?)	Sets or queries the count for the Max or Min Hold trace.
:TRACe:IQVTime:COUNt:ENABle(?)	Selects or queries whether or not to enable the count for Max/Min Hold.
:TRACe:IQVTime:COUNt:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
:TRACe:IQVTime:ENABle:I(?)	Selects or queries whether to show or hide the trace I.
:TRACe:IQVTime:ENABle:Q(?)	Selects or queries whether to show or hide the trace Q.
:TRACe:IQVTime:FREeze(?)	Selects or queries whether to freeze the IQ traces.
:TRACe:IQVTime:FUNCTion(?)	Selects or queries the trace function.
:TRACe:IQVTime:SElect:I(?)	Selects or queries whether to choose the I trace.
:TRACe:IQVTime:SElect:Q(?)	Selects or queries whether to choose the Q trace.
:TRACe:OBWidth subgroup	Occupied Bandwidth measurement
:TRACe:OBWidth:MAXHold(?)	Determines whether to enable or disable the Max Hold trace.
:TRACe:PHVTime subgroup	Frequency versus Time measurement
:TRACe:PHVTime(?)	Selects or queries whether or not to show the trace.
:TRACe:PHVTime:AVERage:COUNt(?)	Sets or queries the number of traces to combine for averaging.

Table 2-23: TRACe commands (Cont.)

Header	Description
:TRACe:PHVTime:COUNT(?)	Sets or queries the count for the Max or Min Hold trace.
:TRACe:PHVTime:COUNT:ENABLE(?)	Selects or queries whether or not to enable the count for Max/Min Hold.
:TRACe:PHVTime:COUNT:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
:TRACe:PHVTime:FREeze(?)	Selects or queries whether to freeze the trace.
:TRACe:PHVTime:FUNCTion(?)	Selects or queries the trace function.
:TRACe:SGRam subgroup	Spectrogram measurement
:TRACe:SGRam:DETEction(?)	Selects or queries the display detector.
:TRACe:SGRam:FREeze(?)	Selects or queries whether or not to freeze the spectrogram display.
:TRACe:SGRam:FUNCTion(?)	Selects or queries the trace function for the spectrogram.
:TRACe:SGRam:FUNCTion:TIME(?)	Sets or queries the number of traces to combine for the trace function.
:TRACe:SGRam:SELEct:LINE(?)	Selects or queries the number of line to send to the spectrum display.
:TRACe<x>:SPECTrum subgroup	Spectrum measurement
:TRACe<x>:SPECTrum(?)	Selects or queries whether to show or hide the specified trace.
:TRACe<x>:SPECTrum:AVERage:COUNT(?)	Sets or queries the number of traces to combine for averaging.
:TRACe<x>:SPECTrum:AVERage:RESet	Clears the average data and resets the average counter.
:TRACe<x>:SPECTrum:COUNT(?)	Sets or queries the count for the Max or Min Hold trace.
:TRACe<x>:SPECTrum:COUNT:ENABLE(?)	Selects or queries whether or not to enable the count for Max/Min Hold.
:TRACe<x>:SPECTrum:COUNT:RESet	Clears the Max or Min Hold data and counter, and restarts the process.
:TRACe<x>:SPECTrum:DETEction(?)	Selects or queries the display detector.
:TRACe<x>:SPECTrum:FREeze(?)	Selects or queries whether or not to freeze the display of the trace.
:TRACe<x>:SPECTrum:FUNCTion(?)	Selects or queries the trace function.
:TRACe<x>:SPECTrum:LEFToperand(?)	Selects or queries the left operand for the math trace.
:TRACe<x>:SPECTrum:RIGHToperand(?)	Selects or queries the right operand for the math trace.
:TRACe<x>:SPECTrum:SELEct(?)	Selects or queries the trace number to display the readout.

TRIGger Commands

Use the TRIGger commands to set up the trigger system.

Table 2-24: TRIGger commands

Header	Description
:TRIGger:MASK:NEW	Loads a new frequency mask.
:TRIGger:MASK:OPEN	Opens a trigger mask with a specified file.
:TRIGger:MASK:SAVE	Saves the current trigger mask to a specified file.
:TRIGger[:SEquence]:ADVanced:SWEep:MODE(?)	Selects or queries whether to trigger each segment in the swept mode.
:TRIGger[:SEquence]:EVENT:EXTFront:IMPedance(?)	Selects or queries the impedance of the external trigger input (front).
:TRIGger[:SEquence]:EVENT:EXTFront:LEVel(?)	Sets or queries the trigger level at the external trigger input (front).
:TRIGger[:SEquence]:EVENT:EXTFront:SLOPe(?)	Selects or queries the trigger slope of the external trigger input (front).
:TRIGger[:SEquence]:EVENT:EXTRear:SLOPe(?)	Selects or queries the trigger slope of the external trigger input (rear).
:TRIGger[:SEquence]:EVENT:GATed(?)	Selects or queries the logic for the gated trigger input.
:TRIGger[:SEquence]:EVENT:INPut:FMASk:VIOlation(?)	Selects or queries when the trigger occurs in the frequency mask trigger.
:TRIGger[:SEquence]:EVENT:INPut:LEVel(?)	Sets or queries the trigger level for the RF input level trigger.
:TRIGger[:SEquence]:EVENT:INPut:SLOPe(?)	Selects or queries the trigger slope for the RF input level trigger.
:TRIGger[:SEquence]:EVENT:INPut:TDBWidth(?)	Sets or queries the time-domain bandwidth.
:TRIGger[:SEquence]:EVENT:INPut:TDBWidth:ACTual?	Queries the actual time-domain bandwidth.
:TRIGger[:SEquence]:EVENT:INPut:TDBWidth:STATe?	Determines whether to set the time-domain bandwidth automatically.
:TRIGger[:SEquence]:EVENT:INPut:TYPE(?)	Selects or queries the trigger type for the source of RF input.
:TRIGger[:SEquence]:EVENT:SOURce(?)	Selects or queries the trigger event source.
:TRIGger[:SEquence]:FORCed(?)	Selects or queries whether to causes a manual trigger.
:TRIGger[:SEquence]:IMMediate	Causes a trigger immediately.
:TRIGger[:SEquence]:STATus(?)	Selects or queries the trigger mode (Free Run or Triggered).
:TRIGger[:SEquence]:TIME:DELay(?)	Sets or queries the trigger delay time.
:TRIGger[:SEquence]:TIME:POSition(?)	Sets or queries the trigger position.

UNIT Commands

Specify fundamental units for measurement.

Table 2-25: UNIT commands

Header	Description
:UNIT:POWer(?)	Selects or queries the unit of power.

Programming Hints

Here are some basic tips for using the RSA6100A Series GPIB commands:

- *Selecting a measurement item*
Use DISPlay commands to select or display the measurement view.
[Example] :DISPlay:GENeral:MEASview:NEW SPECTrum
Displays the spectrum view on the screen.
- *Setting measurement parameters*
Use SENSE commands to set conditions for the measurement session.
[Example] :SENSe:SPECTrum:FREQuency:CENTer 1.5GHz
Sets the center frequency to 1.5 GHz in the spectrum view.
- *Acquiring an input signal*
Use an INITiate or ABORt command to start or stop data acquisition.
[Example] :INITiate:CONTinuous ON;:INITiate:IMMediate
Starts data acquisition in the continuous mode.
- *Processing waveforms arithmetically*
Use TRACe commands for math operation on waveforms.
[Example] :TRACe1:SPECTrum:FUNCTion AVERage
Averages the spectrum waveform.
- *Measuring with the markers*
Use CALCulate commands to measure some quantity using the markers.
[Example] :CALCulate:SPECTrum:MARKer1:MAXimum
Positions the marker at the highest peak signal on the spectrum.
- *Obtaining the measurement results*
Use a FETCh or READ command to get the results.
[Example] :FETCh:SPECTrum:TRACe1?
Returns the spectrum trace data.
- *Scaling the waveform*
Use DISPlay commands to change the waveform portion on screen.
[Example] :DISPlay:IQVTime:Y:SCALe 1.5
Sets the vertical range to 1.5 V in the IQ versus Time graph.

Refer to *Appendix C* for the default settings of the commands.

IEEE Common Commands

This section details the IEEE common commands.

Command Tree

Header	Parameter
*CAL	
*CLS	
*ESE	
*ESR?	
*IDN?	
*OPC	
*OPT?	
*RST	
*SRE	
*STB?	
*TRG	
*WAI	

***CAL? (Query Only)**

Instructs the analyzer to perform an internal self-alignment and return its status.

NOTE. *The self-alignment can take several minutes to respond. No other commands will be executed until alignment is complete.*

Syntax *CAL?

Returns <NR1> = 1 indicates that the alignment was successful.
 <NR1> = 0 indicates that the alignment was unsuccessful.

Measurement Views All

Examples *CAL?
 performs an internal self-alignment and will return 1 if the alignment is successful.

***CLS (No Query Form)**

Clears the analyzer status data structures. Refer to Section 3, *Status and Events*, for the register information.

The *CLS command clears the following:

- the Event Queue
- the Standard Event Status Register (SESR)
- the Status Byte Register (except the MAV bit; see below)

If the *CLS command immediately follows an <E0I>, the Output Queue and MAV bit (Status Byte Register bit 4) are also cleared. MAV indicates information is in the output queue. The device clear (DCL) GPIB control message will clear the output queue and thus MAV. *CLS does not clear the output queue or MAV. (A complete discussion of these registers and bits, and of event handling in general, begins on page 3-1.)

*CLS can suppress a Service Request that is to be generated by an *OPC. This will happen if a hardcopy output or single sequence acquisition operation is still being processed when the *CLS command is executed.

Syntax	*CLS
Arguments	None
Measurement Views	All
Examples	*CLS clears the analyzer status data structures.
Related Commands	*ESE, *ESR, *SRE, *STB?

***ESE(?)**

Sets or queries the bits in the Event Status Enable Register (ESER). The ESER prevents events from being reported to the Status Byte Register (STB). Refer to Section 3, *Status and Events*, for the register information.

Syntax *ESE <value>
 *ESE?

Arguments <value>::=<NR1> is a value in the range from 0 through 255.
 The binary bits of the ESER are set according to this value.

Measurement Views All

Examples *ESE 145
 sets the ESER to binary 10010001, which enables the PON, EXE, and OPC bits.

 *ESE?
 might return the string *ESE 184, showing that the ESER contains the binary value 10111000.

Related Commands *CLS, *ESR, *SRE, *STB?

***ESR? (Query Only)**

Returns the contents of the Standard Event Status Register (SESR). *ESR? also clears the SESR (since reading the SESR clears it). Refer to Section 3, *Status and Events*, for the register information.

Syntax *ESR?

Arguments None

Returns <NR1> representing the contents of the SESR by a 0 to 255 decimal number.

Measurement Views All

Examples *ESR?
might return the value 213, showing that the SESR contains binary 11010101.

Related Commands *CLS, *ESE?, *SRE, *STB?

***IDN? (Query Only)**

Returns the analyzer identification code.

Syntax *IDN?

Arguments None

Measurement Views All

Returns The analyzer identification code in the following format:

TEKTRONIX,RSA61XXA,<serial_number>,<firmware_version>

Where

TEKTRONIX indicates that the manufacturer is Tektronix.

RSA61XXA is the model number (RSA6106A or RSA6114A).

<serial_number> is the serial number.

<firmware_version> is the firmware version.

Examples *IDN?
might return the response TEKTRONIX,RSA6114A,B000111,FV:1.0.1500.

***OPC(?)**

Generates the operation complete message in the Standard Event Status Register (SESR) when all pending operations finish. The *OPC? query places the ASCII character “1” into the output queue when all pending operations are finished. The *OPC? response is not available to read until all pending operations finish.

The *OPC command allows you to synchronize the operation of the analyzer with your application program. Refer to *Synchronizing Execution* on page 3-12 for the details.

Syntax *OPC

*OPC?

Arguments None

Measurement Views All

***OPT? (Query Only)**

Returns a list of options installed in your analyzer.

Syntax *OPT?

Arguments None

Returns The numbers of all the options installed in the analyzer, separated by commas. If no options have been installed, 0 is returned.

Table 2-26 lists the options for the RSA6100A Series analyzers.

Table 2-26: Instrument options

Option	Description
01	Internal preamp, 5 MHz – 3 GHz, 30 dB gain, 8 dB noise figure at 2 GHz, typical
02	256 Msample deep memory, frequency mask trigger
05	Digital IQ output and 500 MHz analog IF output
06 ¹	Removable HDD, 80 GB
07 ¹	DVD-RW
20	Advanced signal analysis (including pulse measurements)
21	General purpose modulation analysis
110	110 MHz real-time capture bandwidth
1R ¹	Rackmount

¹ These options are not returned from this query.

Measurement Views All

Examples *OPT?
might return 02,05,21, indicating that Option 02, 05, and 21 are currently installed in the analyzer.

*RST (No Query Form)

Returns the instrument settings to the factory defaults (see *Appendix C: Factory Initialization Settings*).

The *RST command does not alter the following:

- The state of the GPIB interface.
- The selected GPIB address of the analyzer.
- Alignment data that affect device specifications.
- The Output Queue.
- The Service Request Enable Register setting.
- The Standard Event Status Enable Register setting.
- The Power-on status clear flag setting.
- Stored settings.

NOTE. Execution of the *RST command is not complete until all changes from resetting the instrument are completed. Following commands and queries will not be executed until these actions are completed.

Syntax	*RST
Arguments	None
Measurement Views	All
Examples	*RST returns the instrument settings to the factory defaults.
Related Commands	*CLS

***SRE(?)**

Sets or queries the value of the Service Request Enable Register (SRER). Refer to Section 3, *Status and Events*, for the register information.

Syntax *SRE <value>
 *SRE?

Arguments <value>::=<NR1> is a value in the range from 0 to 255.
 The binary bits of the SRER are set according to this value.
 Using an out-of-range value causes an execution error.

Measurement Views All

Examples *SRE 48
 sets binary 00110000 in the SRER's bits:

 *SRE?
 might return 32, indicating that binary value 00100000 has been set in the
 SRER's bits.

Related Commands *CLS, *ESE, *ESR?, *STB?

***STB? (Query Only)**

Returns the contents of the Status Byte Register (SBR) in the status/event reporting structure using the Master Summary Status (MSS) bit. Refer to Section3, *Status and Events*, for the register information.

Syntax *STB?

Arguments None

Returns <NR1> representing the contents of the SBR as a decimal number.

Measurement Views All

Examples *STB?
might return 96, indicating that the SBR contains binary 0110 0000.

Related Commands *CLS, *ESE, *ESR?, *SRE

***TRG (No Query Form)**

Generates a trigger. It produces the same effect as the Force Trigger button on the Trigger control panel. This command is valid when the trigger mode is Triggered.

Syntax *TRG

Arguments None

Measurement Views All

Examples *TRG
generates a trigger.

Related Commands :TRIGger[:SEQuence]:STATus

***WAI (No Query Form)**

Prevents the analyzer from executing further commands or queries until all pending operations finish. This command allows you to synchronize the operation of the analyzer with your application program. For the details, refer to *Synchronizing Execution* on page 3-12.

Syntax *WAI

Arguments None

Measurement Views All

Related Commands *OPC

ABORt Commands

The ABORt command resets the trigger system and places all trigger sequences in the idle state.

Command Tree

Header	Parameter
:ABORt	

:ABORt (No Query Form)

Resets the trigger system and places all trigger sequences in the idle state. Any actions related to the trigger system that are in progress, such as a sweep or acquiring a measurement is also aborted.

To start data acquisition, use the INITiate commands.

Syntax	:ABORt
---------------	--------

Arguments	None
------------------	------

Measurement Views	All
--------------------------	-----

Examples	:ABORt resets the trigger system and stops data acquisition.
-----------------	---

Related Commands	INITiate commands
-------------------------	-------------------

CALCulate Commands

The CALCulate commands control the markers and the search operations. These commands are divided by measurement views into the subgroups listed in Table 2-27.

Table 2-27: CALCulate command subgroups

Command header	Measurement view	Refer to:
:CALCulate (basic)	All views, general marker control	page 2-71
:CALCulate:ACPower	Channel power and ACPR	page 2-86
:CALCulate:AVTime	Amplitude versus Time	page 2-91
:CALCulate:CONSte	Constellation (Option 21 only)	page 2-98
:CALCulate:DPSA	DPX (Digital Phosphor) spectrum	page 2-103
:CALCulate:EVM	EVM versus Time (Option 21 only)	page 2-110
:CALCulate:FVTime	Frequency versus Time	page 2-116
:CALCulate:IQVTime	RF I&Q versus Time	page 2-122
:CALCulate:MCPower	MCPR (Multiple Carrier Power Ratio)	page 2-129
:CALCulate:MERRor	Magnitude error versus Time (Option 21 only)	page 2-134
:CALCulate:OBWidth	OBW (Occupied Bandwidth)	page 2-140
:CALCulate:PERRor	Phase error versus Time (Option 21 only)	page 2-146
:CALCulate:PHVTime	Phase versus Time	page 2-152
:CALCulate:PULSe	Pulsed RF measurements (Option 20 only)	page 2-158
:CALCulate:SGRam	Spectrogram	page 2-169
:CALCulate:SPECtrum	Spectrum	page 2-176
:CALCulate:TOVerview	Time overview	page 2-183

Marker Mnemonics

Up to five markers can be used. In commands, these are named MARKer<x>, where <x> can be 0, 1, 2, 3, or 4 as shown in Table 2-28.

Table 2-28: Marker mnemonics

Mnemonic	Description
MARKer0	Reference marker (MR)
MARKer1	Marker 1 (M1)
MARKer2	Marker 2 (M2)
MARKer3	Marker 3 (M3)
MARKer4	Marker 4 (M4)

NOTE. *If you omit the numeric suffix, the marker control defaults to Marker 1.*

Before operating the marker, you have to enable it using the CALCulate basic commands (refer to page 2-71).

If you attempt to use a marker other than above in a :CALCulate command, the suffix error (error code -130) will occur.

:CALCulate Basic Command Subgroup

The :CALCulate basic commands globally control the markers and the search operations.

Command Tree	Header	Parameter
	:CALCulate	
	:MARKer	
	:ADD	
	:AOff	
	:DELeTe	
	:MODE	ABSolute DELTa
	:PEAK	
	:EXCursion	<numeric_value>
	:THReshold	<numeric_value>
	:SEARCh	
	:LIMit	
	:FAIL?	
	:MATCh	
	:BEEP	
	[:STATe]	<boolean>
	:SACQuire	
	[:STATe]	<boolean>
	:SDATa	
	[:STATe]	<boolean>
	:SPICture	
	[:STATe]	<boolean>
	:STRace	
	[:STATe]	<boolean>
	:OPERation	LT GT IMASK OMASK
	:FEED	<string>, <string>
	:MASK	
	:LOAD	<string>
	:STORE	<string>
	:SLIMit	<numeric_value>
	:REPort	
	:DATA?	
	:POINTs?	
	:STATe	<boolean>

:CALCulate:MARKer:ADD (No Query Form)

Adds a marker. Every execution of this command adds a marker from MR, then M1 to M4, sequentially.

NOTE. *If all markers are already turned on, the error message “Cannot add another marker” (execution error -200) is returned.*

Syntax	:CALCulate:MARKer:ADD
Arguments	None
Measurement Views	All
Examples	:CALCulate:MARKer:ADD adds a marker.
Related Commands	:CALCulate:MARKer:AOff, :CALCulate:MARKer:DELeTe

:CALCulate:MARKer:AOff (No Query Form)

Turns off all markers.

Syntax	:CALCulate:MARKer:AOff
Arguments	None
Measurement Views	All
Examples	:CALCulate:MARKer:AOff turns off all markers.
Related Commands	:CALCulate:MARKer:ADD, :CALCulate:MARKer:DELeTe

:CALCulate:MARKer:DELeTe (No Query Form)

Deletes the last marker added.

NOTE. If all markers are turned off, the error message “Cannot delete another marker” (execution error -200) is returned.

Syntax	:CALCulate:MARKer:DELeTe
Arguments	None
Measurement Views	All
Examples	:CALCulate:MARKer:DELeTe deletes the last marker added.
Related Commands	:CALCulate:MARKer:ADD, :CALCulate:MARKer:AOff

:CALCulate:MARKer:MODE(?)

Selects or queries the marker mode.

Syntax	:CALCulate:MARKer:MODE { ABSolute DELTa } :CALCulate:MARKer:MODE?
Arguments	ABSolute selects the absolute marker mode, in which the marker readout indicates the absolute value. DELTA selects the delta marker mode, in which the marker readout indicates the relative value to the reference marker.
Measurement Views	All
Examples	:CALCulate:MARKer:MODE DELTA selects the delta marker mode.

:CALCulate:MARKer:PEAK:EXCursion(?)

Sets or queries the excursion level (how far a signal must be above the surrounding noise to be detected as a peak). The signal is considered to be a peak if it exceeds the excursion level and the threshold level set by the :CALCulate :MARKer:PEAK:THReshold command.

Syntax :CALCulate:MARKer:PEAK:EXCursion <value>
 :CALCulate:MARKer:PEAK:EXCursion?

Arguments <value>::=<NRf> specifies the excursion level.
 Range: 0 to 100 dB.

Measurement Views All

Examples :CALCulate:MARKer:PEAK:EXCursion 10
 sets the excursion level to 10 dB.

Related Commands :CALCulate:MARKer:PEAK:THReshold

:CALCulate:MARKer:PEAK:THReshold(?)

Sets or queries the threshold level above which a signal is detected as a peak.

Syntax :CALCulate:MARKer:PEAK:THReshold <value>
 :CALCulate:MARKer:PEAK:THReshold?

Arguments <value>::=<NRf> specifies the threshold level for detecting peaks.
 Range: -170 to +130 dBm.

Measurement Views All

Examples :CALCulate:MARKer:PEAK:THReshold -50
 sets the threshold level to -50 dBm.

:CALCulate:SEARch:LIMit:FAIL? (Query Only)

Queries whether the waveform cuts across the limit in the search operation.

Syntax :CALCulate:SEARch:LIMit:FAIL?

Returns { 0 | 1 }

0 represents Pass, indicating that the waveform does not cut across the limit.

1 represents Fail, indicating that the waveform cuts across the limit.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:FAIL?
might return 1, indicating that the waveform cuts across the limit (Fail).

:CALCulate:SEARCh:LIMit:MATCH:BEEP[:STATe](?)

Determines whether or not to beep on match during run or replay in the search operation.

Syntax :CALCulate:SEARCh:LIMit:MATCH:BEEP[:STATe] { OFF | ON | 0 | 1 }
 :CALCulate:SEARCh:LIMit:MATCH:BEEP[:STATe]?

Arguments OFF or 0 disables to beep on match.
 ON or 1 enables to beep on match.

Measurement Views All

Examples :CALCulate:SEARCh:LIMit:MATCH:BEEP:STATe ON
 enables to beep on match.

:CALCulate:SEARCh:LIMit:MATCH:SACQuire[:STATe](?)

Determines whether or not to stop acquiring data on match during run or replay in the search operation.

Syntax :CALCulate:SEARCh:LIMit:MATCH:SACQuire[:STATe]
 { OFF | ON | 0 | 1 }
 :CALCulate:SEARCh:LIMit:MATCH:SACQuire[:STATe]?

Arguments OFF or 0 disables to stop acquiring data on match.
 ON or 1 enables to stop acquiring data on match.

Measurement Views All

Examples :CALCulate:SEARCh:LIMit:MATCH:SACQuire:STATe ON
 enables to stop acquiring data on match.

:CALCulate:SEARch:LIMit:MATCH:SDATa[:STATe](?)

Determines whether or not to save automatically (AutoSave) acquisition data on match during run in the search operation.

Syntax :CALCulate:SEARch:LIMit:MATCH:SDATa[:STATe] { OFF | ON | 0 | 1 }
:CALCulate:SEARch:LIMit:MATCH:SDATa[:STATe]?

Arguments OFF or 0 disables the AutoSave.

ON or 1 enables to save acquisition data automatically on match.
The data is saved to a file with the name:

<name>-yyyy.mm.dd.hh.mm.ss.sss.tiq

Where

<name> is the file name that was last specified.

yyyy.mm.dd and hh.mm.ss.sss represent date and 24 hour time.

The file extension is .tiq.

Example: SAVED-2007.03.20.12.34.567.tiq

For the directory of file, refer to *Specifying the File* on page 2-445 in the MMEMory command section.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:MATCH:SDATa:STATe ON
enables to save acquisition data automatically on match.

:CALCulate:SEARCh:LIMit:MATCH:SPICture[:STATe](?)

Determines whether or not to save automatically (AutoSave) the whole screen on match during run in the search operation.

Syntax :CALCulate:SEARCh:LIMit:MATCH:SPICture[:STATe]
 { OFF | ON | 0 | 1 }

 :CALCulate:SEARCh:LIMit:MATCH:SPICture[:STATe]?

Arguments OFF or 0 disables the AutoSave.

 ON or 1 enables to save the whole screen automatically on match.
 The picture is saved to a file with the name:

 <name>-yyyy.mm.dd.hh.mm.ss.sss.png

 Where
 <name> is the file name that was last specified.
 yyyy.mm.dd and hh.mm.ss.sss represent date and 24 hour time.
 The file extension is .png.
 Example: SAVED-2007.03.20.12.34.567.png

 For the directory of file, refer to *Specifying the File* on page 2-445 in the
 MMEMory command section.

Measurement Views All

Examples :CALCulate:SEARCh:LIMit:MATCH:SPICture:STATe ON
 enables to save the whole screen automatically on match.

:CALCulate:SEARch:LIMit:MATCH:STRace[:STATe](?)

Determines whether or not to save automatically (AutoSave) the spectrum trace on match during run in the search operation.

Syntax :CALCulate:SEARch:LIMit:MATCH:STRace[:STATe] { OFF | ON | 0 | 1 }
:CALCulate:SEARch:LIMit:MATCH:STRace[:STATe]?

Arguments OFF or 0 disables the AutoSave.

ON or 1 enables to save the spectrum trace automatically on match.
The trace is saved to a file with the name:

<name>-yyyy.mm.dd.hh.mm.ss.sss.Specan

Where

<name> is the file name that was last specified.

yyyy.mm.dd and hh.mm.ss.sss represent date and 24 hour time.

The file extension is .Specan.

Example: SAVED-2007.03.20.12.34.567.Specan

For the directory of file, refer to *Specifying the File* on page 2-445 in the MMEMory command section.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:MATCH:STRace:STATe ON
enables to save the spectrum trace automatically on match.

:CALCulate:SEARCh:LIMit:OPERation(?)

Selects or queries the search condition.

Syntax :CALCulate:SEARCh:LIMit:OPERation { LT | GT | IMASk | OMASk }
:CALCulate:SEARCh:LIMit:OPERation?

Arguments Table 2-29 lists the arguments.

Table 2-29: Search condition

Argument	Meaning
LT	The data is less than the limit value.
GT	The data is greater than the limit value.
IMASk	The data is inside the limit mask.
OMASk	The data is outside the limit mask.

You can select the data using the :CALCulate:SEARCh:LIMit:FEED command.

You can set the limit value using the :CALCulate:SEARCh:LIMit:OPERation :SLIMit command.

You can store or load the limit mask using the :MMEMory:LOAD|:STORE :LIMit command.

Measurement Views All

Examples :CALCulate:SEARCh:LIMit:OPERation GT
selects “the data is greater than the limit value” for the search condition.

Related Commands :CALCulate:SEARCh:LIMit:FEED,
:CALCulate:SEARCh:LIMit:OPERation:SLIMit,
:MMEMory:LOAD|:STORE:LIMit

:CALCulate:SEARch:LIMit:OPERation:FEED(?)

Sets or queries the data flow to be fed in the search operation.

Syntax :CALCulate:SEARch:LIMit:OPERation:FEED <view>,<trace>
:CALCulate:SEARch:LIMit:OPERation:FEED?

Arguments <view>::=<string> and <trace>::=<string> are listed in Table 2-30.

Table 2-30: Source data of the search operation

<view>	<trace>	Meaning
"Spectrum"	"Trace 1" ¹	Trace 1 in the Spectrum view.
	"Trace 2" ¹	Trace 2 in the Spectrum view.
	"Trace 3" ¹	Trace 3 in the Spectrum view.
	"Math Trace"	Math trace in the Spectrum view.
	"Spectrogram Trace"	Spectrogram trace in the Spectrum view.

¹ There is a space character between Trace and the number.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:OPERation:FEED "Spectrum","Trace 1"
selects the Trace 1 in the Spectrum measurement view for the search operation.

:CALCulate:SEARch:LIMit:OPERation:FEED?
might return "Spectrum","Math Trace", indicating that the math trace is used as the source data in the search operation.

:CALCulate:SEARch:LIMit:OPERation:MASK:LOAD (No Query Form)

Loads the limit mask from a specified file for the search operation.

Syntax :CALCulate:SEARch:LIMit:OPERation:MASK:LOAD <file_name>

Arguments <file_name>::=<string> specifies the file to load the limit mask from. The file extension is .lmt. You can omit the extension.

For the directory of file, refer to *Specifying the File* on page 2-445 in the MMEMory command section.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:OPERation:MASK:LOAD "Limit1"
loads the limit mask from the *Limit1.lmt* file.

:CALCulate:SEARch:LIMit:OPERation:MASK:STORE (No Query Form)

Stores the limit mask to a specified file in the search operation.

Syntax :CALCulate:SEARch:LIMit:OPERation:MASK:STORE <file_name>

Arguments <file_name>::=<string> specifies the file to store the limit mask to. The file extension is .lmt. You can omit the extension.

For the directory of file, refer to *Specifying the File* on page 2-445 in the MMEMory command section.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:OPERation:MASK:STORE "Limit1"
stores the limit mask to the *Limit1.lmt* file.

:CALCulate:SEARch:LIMit:OPERation:SLIMit(?)

Sets or queries the limit value in the search operation.

Syntax :CALCulate:SEARch:LIMit:OPERation:SLIMit <value>
 :CALCulate:SEARch:LIMit:OPERation:SLIMit?

Arguments <value>::=<NRf> specifies the limit value in the search operation.
 Range: -100 to +100 dBm.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:OPERation:SLIMit -20
 sets the limit value to -20 dBm.

Related Commands :CALCulate:SEARch:LIMit:OPERation

:CALCulate:SEARch:LIMit:REPort:DATA? (Query Only)

Returns the frequency range(s) that satisfy the search condition.

Syntax :CALCulate:SEARch:LIMit:REPort:DATA?

Arguments None

Returns <num_range>,<range(1)>,<range(2)>,...,<range(n)>

Where

<num_range>::=<NR1> is the number of ranges that satisfy the condition.

<range(n)>::="<lower_freq(n)>,<upper_freq(n)>" (string) represents the n^{th} frequency range that satisfy the search condition in ascending order.

<lower_freq(n)> and <upper_freq(n)> are the lower and upper frequencies of the range #n, respectively.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:REPort:DATA?
might return 2,"1.4800E+9, 1.5001E+9","1.5002E+9, 1.5200E+9",
indicating that the search condition is satisfied in these two ranges:
1.48 to 1.5001 GHz and 1.5002 to 1.52 GHz.

:CALCulate:SEARch:LIMit:REPort:POINTs? (Query Only)

Returns the number of frequency range(s) that satisfy the search condition.

Syntax :CALCulate:SEARch:LIMit:REPort:POINTs?

Arguments None

Returns <number>::=<NR1> represents the number of frequency range(s) that satisfy the search condition.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:REPort:POINTs?
might return 5, indicating that five ranges satisfy the search condition.

:CALCulate:SEARch:LIMit:STATe(?)

Determines whether to enable or disable the search function.

Syntax :CALCulate:SEARch:LIMit:STATe { OFF | ON | 0 | 1 }
:CALCulate:SEARch:LIMit:STATe?

Arguments OFF or 0 disables the search function.
ON or 1 enables the search function.

Measurement Views All

Examples :CALCulate:SEARch:LIMit:STATe ON
enables the search function.

:CALCulate:ACPower Subgroup

The :CALCulate:ACPower commands control the markers in the Channel power and ACPR (Adjacent Channel Power Ratio) measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:ACPower	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:LEFT	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

:CALCulate:ACPower:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker in the Channel power and ACPR measurement.

Syntax :CALCulate:ACPower:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <Nrf> Delta marker frequency for the selected marker.

Measurement Views Channel power and ACPR

Examples :CALCulate:ACPower:MARKer1:DELTA:X?
might return 1.28E+6, indicating that the delta marker frequency is 1.28 MHz.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:ACPower:MARKer<x>:DELTA:Y?

:CALCulate:ACPower:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the Channel power and ACPR measurement.

Syntax :CALCulate:ACPower:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <Nrf> Delta marker amplitude for the selected marker.

Measurement Views Channel power and ACPR

Examples :CALCulate:ACPower:MARKer1:DELTA:Y?
might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:ACPower:MARKer<x>:DELTA:X?

:CALCulate:ACPower:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Channel power and ACPR measurement.

Syntax :CALCulate:ACPower:MARKer<x>:MAXimum

Arguments None

Measurement Views Channel power and ACPR

Examples :CALCulate:ACPower:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:ACPower:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Channel power and ACPR measurement.

Syntax :CALCulate:ACPower:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Channel power and ACPR

Examples :CALCulate:ACPower:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:ACPower:MARKer<x>:PEAK:RIGHT

:CALCulate:ACPower:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Channel power and ACPR measurement.

Syntax :CALCulate:ACPower:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Channel power and ACPR

Examples :CALCulate:ACPower:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:ACPower:MARKer<x>:PEAK:LEFT

:CALCulate:ACPower:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the Channel power and ACPR measurement.

Syntax :CALCulate:ACPower:MARKer<x>:X <value>
 :CALCulate:ACPower:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
 Range: (center frequency) \pm (span)/2.

Measurement Views Channel power and ACPR

Examples :CALCulate:ACPower:MARKer1:X 800MHz
 places Marker 1 (M1) at 800 MHz on the trace.

Related Commands :CALCulate:ACPower:MARKer<x>:Y?

:CALCulate:ACPower:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the Channel power and ACPR measurement.

Syntax :CALCulate:ACPower:MARKer<x>:Y?

Arguments None

Measurement Views Channel power and ACPR

Examples :CALCulate:ACPower:MARKer1:Y?
 might return -34.28 indicating Marker 1 (M1) is at -34.28 dBm.

Related Commands :CALCulate:ACPower:MARKer<x>:X

:CALCulate:AVTime Subgroup

The :CALCulate:AVTime commands control the markers in the Amplitude versus Time measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:AVTime	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:TRACe	TRACE1 TRACE2 TRACE3 TRACE4
	:X	<numeric_value>
	:Y?	

:CALCulate:AVTime:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the Amplitude versus Time measurement.

Syntax :CALCulate:AVTime:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:DELTA:X?
might return 38.0E-9, indicating that the delta marker time is 38.0 ns.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:AVTime:MARKer<x>:DELTA:Y?

:CALCulate:AVTime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the Amplitude versus Time measurement.

Syntax :CALCulate:AVTime:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:DELTA:Y?
might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:AVTime:MARKer<x>:DELTA:X?

:CALCulate:AVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Amplitude versus Time measurement.

Syntax :CALCulate:AVTime:MARKer<x>:MAXimum

Arguments None

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:AVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Amplitude versus Time trace.

Syntax :CALCulate:AVTime:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:AVTime:MARKer<x>:PEAK:LOWer

:CALCulate:AVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Amplitude versus Time measurement.

Syntax :CALCulate:AVTime:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:AVTime:MARKer<x>:PEAK:RIGHT

:CALCulate:AVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Amplitude versus Time trace.

Syntax :CALCulate:AVTime:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:AVTime:MARKer<x>:PEAK:HIGHer

:CALCulate:AVTime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Amplitude versus Time measurement.

Syntax :CALCulate:AVTime:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:AVTime:MARKer<x>:PEAK:LEFT

:CALCulate:AVTime:MARKer<x>:TRACe(?)

Selects or queries the trace on which the specified marker is placed in the Amplitude versus Time measurement.

Syntax :CALCulate:AVTime:MARKer<x>:TRACe
 { TRACE1 | TRACE2 | TRACE3 | TRACE4 }
 :CALCulate:AVTime:MARKer<x>:TRACe?

Arguments TRACE1 places the selected marker on Trace 1.
 TRACE2 places the selected marker on Trace 2.
 TRACE3 places the selected marker on Trace 3.
 TRACE4 places the selected marker on Trace 4 (math trace).

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:TRACe TRACE1
 places Marker 1 (M1) on Trace 1.

:CALCulate:AVTime:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the Amplitude versus Time measurement.

Syntax :CALCulate:AVTime:MARKer<x>:X <value>
 :CALCulate:AVTime:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: (analysis offset) to [(analysis offset) + (analysis length)].

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:X 1.5u
 places Marker 1 (M1) at 1.5 μ s on the trace.

Related Commands :CALCulate:AVTime:MARKer<x>:Y?

:CALCulate:AVTime:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the Amplitude versus Time measurement.

Syntax :CALCulate:AVTime:MARKer<x>:Y?

Arguments None

Measurement Views Amplitude versus Time

Examples :CALCulate:AVTime:MARKer1:Y?
 might return -2.73 indicating Marker 1 (M1) is at -2.73 dBm.

Related Commands :CALCulate:AVTime:MARKer<x>:X

:CALCulate:CONSte Subgroup (Option 21 Only)

The :CALCulate:CONSte commands control the markers in the constellation measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:CONSte	
	:MARKer<x>	
	:DELTA	
	:X	
		[:TIME] ?
	:MAGNitude?	
	:MAXimum	
	:PEAK	
	:LEFT	
	:RIGHT	
	:PHASe?	
	:SYMBol?	
	:VALue?	
	:X	<numeric_value>

:CALCulate:CONSte:MARKer<x>:DELTA:X[:TIME]? (Query Only)

Returns the delta marker time for the selected marker on the constellation trace.

Syntax :CALCulate:CONSte:MARKer<x>:DELTA:X[:TIME]?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Constellation

Examples :CALCulate:CONSte:MARKer1:DELTA:X:TIME?
might return -62.75, indicating that the delta marker time is -62.75 symbols.

Related Commands :CALCulate:MARKer:ADD

:CALCulate:CONSt:MARKer<x>:MAGNitude? (Query Only)

Queries the magnitude readout of the selected marker in the constellation measurement.

Syntax :CALCulate:CONSt:MARKer<x>:MAGNitude?

Arguments None

Returns <NRf> The magnitude readout for the selected marker.

Measurement Views Constellation

Examples :CALCulate:CONSt:MARKer1:MAGNitude?
might return 0.713927 indicating the magnitude readout of Marker 1 (M1) is 0.713927.

Related Commands :CALCulate:CONSt:MARKer<x>:X

:CALCulate:CONSt:MARKer<x>:MAXimum (No Query Form)

Positions the selected marker at the symbol in the center of the time record.

Syntax :CALCulate:CONSt:MARKer<x>:MAXimum

Arguments None

Measurement Views Constellation

Examples :CALCulate:CONSt:MARKer1:MAXimum
positions Marker 1 (M1) at the symbol in the center of the time record.

:CALCulate:CONSt:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker in the time domain to the next lower symbol number, relative to the previous marker position.

Syntax :CALCulate:CONSt:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Constellation

Examples :CALCulate:CONSt:MARKer1:PEAK:LEFT
moves Marker 1 (M1) in the time domain to the next lower symbol number.

Related Commands :CALCulate:CONSt:MARKer<x>:PEAK:RIGHT

:CALCulate:CONSt:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker in the time domain to the next higher symbol number, relative to the previous marker position.

Syntax :CALCulate:CONSt:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Constellation

Examples :CALCulate:CONSt:MARKer1:PEAK:RIGHT
moves the Marker 1 (M1) in the time domain to the next higher symbol number.

Related Commands :CALCulate:CONSt:MARKer<x>:PEAK:LEFT

:CALCulate:CONSt:MARKer<x>:PHASe? (Query Only)

Queries the phase readout of the selected marker in the constellation measurement.

Syntax :CALCulate:CONSt:MARKer<x>:PHASe?

Arguments None

Returns <NRf> The phase readout for the selected marker.

Measurement Views Constellation

Examples :CALCulate:CONSt:MARKer1:PHASe?
might return 35.74 indicating the phase readout of Marker 1 (M1) is 35.74°.

Related Commands :CALCulate:CONSt:MARKer<x>:X

:CALCulate:CONSt:MARKer<x>:SYMBol? (Query Only)

Queries the symbol readout of the selected marker in the constellation measurement.

Syntax :CALCulate:CONSt:MARKer<x>:SYMBol?

Arguments None

Returns <NRf> The symbol readout for the selected marker.

Measurement Views Constellation

Examples :CALCulate:CONSt:MARKer1:SYMBol?
might return 62.00 indicating the symbol readout of Marker 1 (M1) is 62.

Related Commands :CALCulate:CONSt:MARKer<x>:X

:CALCulate:CONSt:MARKer<x>:VALue? (Query Only)

Queries the value readout of the selected marker in the constellation measurement.

Syntax :CALCulate:CONSt:MARKer<x>:VALue?

Arguments None

Returns <NRf> The value readout for the selected marker.

Measurement Views Constellation

Examples :CALCulate:CONSt:MARKer1:VALue?
might return 2.00 indicating the value readout of Marker 1 (M1) is 2.

Related Commands :CALCulate:CONSt:MARKer<x>:X

:CALCulate:CONSt:MARKer<x>:X(?)

Sets or queries the time position of the selected marker on the constellation trace.

Syntax :CALCulate:CONSt:MARKer<x>:X <value>
:CALCulate:CONSt:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the time position of the marker.
Range: (analysis offset) to [(analysis offset) + (analysis length)].

Measurement Views Constellation

Examples :CALCulate:CONSt:MARKer1:X -1.63875m
places the Marker 1 (M1) at -1.63875 ms on the constellation trace.

Related Commands :CALCulate:CONSt:MARKer<x>:MAGNitude[:PHASe[:SYMBOL]:VALue?

:CALCulate:DPSA Subgroup

The :CALCulate:DPSA commands control the markers in the DPX (Digital Phosphor) spectrum measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:DPSA	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	[:SET]	
	:CENTer	
	:TRACe	BITMAP TRACE1 TRACE2 TRACE3 TRACE4
	:X	<numeric_value>
	:Y?	

:CALCulate:DPSA:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker on the DPX spectrum trace.

Syntax :CALCulate:DPSA:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker frequency for the selected marker.

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:DELTA:X?
might return 1.28E+6, indicating that the delta marker frequency is 1.28 MHz.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:DPSA:MARKer<x>:DELTA:Y?

:CALCulate:DPSA:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the DPX spectrum trace.

Syntax :CALCulate:DPSA:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:DELTA:Y?
might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:DPSA:MARKer<x>:DELTA:X?

:CALCulate:DPSA:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the DPX spectrum trace.

Syntax :CALCulate:DPSA:MARKer<x>:MAXimum

Arguments None

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:DPSA:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the DPX spectrum trace.

Syntax :CALCulate:DPSA:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:DPSA:MARKer<x>:PEAK:LOWer

:CALCulate:DPSA:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the DPX spectrum trace.

Syntax :CALCulate:DPSA:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:DPSA:MARKer<x>:PEAK:RIGHT

:CALCulate:DPSA:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the DPX spectrum trace.

Syntax :CALCulate:DPSA:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:DPSA:MARKer<x>:PEAK:HIGHer

:CALCulate:DPSA:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the DPX spectrum trace.

Syntax :CALCulate:DPSA:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:DPSA:MARKer<x>:PEAK:LEFT

:CALCulate:DPSA:MARKer<x>[:SET]:CENTER (No Query Form)

Sets the center frequency to the marker frequency in the DPX spectrum view.

Syntax :CALCulate:DPSA:MARKer<x>[:SET]:CENTER

Arguments None

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:SET:CENTer
sets the center frequency to the marker frequency in the DPX spectrum view.

:CALCulate:DPSA:MARKer<x>:TRACe(?)

Selects or queries the trace on which the specified marker is placed in the DPX spectrum measurement.

Syntax :CALCulate:DPSA:MARKer<x>:TRACe
 { BITMAP | TRACE1 | TRACE2 | TRACE3 | TRACE4 }
:CALCulate:DPSA:MARKer<x>:TRACe?

Arguments BITMAP places the specified marker on the bitmap trace.
TRACE1 places the specified marker on the maximum trace.
TRACE2 places the specified marker on the minimum trace.
TRACE3 places the specified marker on the average trace.
TRACE4 places the specified marker on the math trace.

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:TRACe TRACE1
 places Marker 1 (M1) on the maximum trace.

:CALCulate:DPSA:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the DPX spectrum view.

Syntax :CALCulate:DPSA:MARKer<x>:X <value>
:CALCulate:DPSA:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: (center frequency) \pm (span)/2.

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:X 800MHz
places Marker 1 (M1) at 800 MHz on the trace.

Related Commands :CALCulate:DPSA:MARKer<x>:Y?

:CALCulate:DPSA:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the DPX spectrum view.

Syntax :CALCulate:DPSA:MARKer<x>:Y?

Arguments None

Measurement Views DPX spectrum

Examples :CALCulate:DPSA:MARKer1:Y?
might return -34.28 indicating Marker 1 (M1) is at -34.28 dBm.

Related Commands :CALCulate:DPSA:MARKer<x>:X

:CALCulate:EVM Subgroup (Option 21 Only)

The :CALCulate:EVM commands control the markers in the EVM versus Time measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:EVM	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

:CALCulate:EVM:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the EVM versus Time measurement.

Syntax :CALCulate:EVM:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:DELTA:X?
might return 9.52, indicating that the delta marker time is 9.52 symbols.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:EVM:MARKer<x>:DELTA:Y?

:CALCulate:EVM:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the EVM versus Time measurement.

Syntax :CALCulate:EVM:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:DELTA:Y?
might return 1.62, indicating that the delta marker amplitude is 1.62%.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:EVM:MARKer<x>:DELTA:X?

:CALCulate:EVM:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the EVM versus Time measurement.

Syntax :CALCulate:EVM:MARKer<x>:MAXimum

Arguments None

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:EVM:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the EVM versus Time trace.

Syntax :CALCulate:EVM:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:EVM:MARKer<x>:PEAK:LOWer

:CALCulate:EVM:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the EVM versus Time measurement.

Syntax :CALCulate:EVM:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:EVM:MARKer<x>:PEAK:RIGHT

:CALCulate:EVM:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the EVM versus Time trace.

Syntax :CALCulate:EVM:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:EVM:MARKer<x>:PEAK:HIGHer

:CALCulate:EVM:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the EVM versus Time measurement.

Syntax :CALCulate:EVM:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:EVM:MARKer<x>:PEAK:LEFT

:CALCulate:EVM:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the EVM versus Time measurement.

Syntax :CALCulate:EVM:MARKer<x>:X <value>
 :CALCulate:EVM:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
 Range: (analysis offset) to (analysis offset) + (analysis length).

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:X 1.5us
 places Marker 1 (M1) at 1.5 μ s on the trace.

Related Commands :CALCulate:EVM:MARKer<x>:Y?

:CALCulate:EVM:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the EVM versus Time measurement.

Syntax :CALCulate:EVM:MARKer<x>:Y?

Arguments None

Measurement Views EVM versus Time

Examples :CALCulate:EVM:MARKer1:Y?
 might return -15.34E+6 indicating Marker 1 (M1) is at -15.34 MHz.

Related Commands :CALCulate:EVM:MARKer<x>:X

:CALCulate:FVTime Subgroup

The :CALCulate:FVTime commands control the markers in the Frequency versus Time measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:FVTime	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

:CALCulate:FVTime:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the Frequency versus Time measurement.

Syntax :CALCulate:FVTime:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:DELTA:X?
might return 120.0E-9, indicating that the delta marker time is 120 ns.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:FVTime:MARKer<x>:DELTA:Y?

:CALCulate:FVTime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker frequency for the selected marker in the Frequency versus Time measurement.

Syntax :CALCulate:FVTime:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker frequency for the selected marker.

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:DELTA:Y?
might return 27.05E+3, indicating that the delta marker frequency is 27.05 kHz.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:FVTime:MARKer<x>:DELTA:X?

:CALCulate:FVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Frequency versus Time measurement.

Syntax :CALCulate:FVTime:MARKer<x>:MAXimum

Arguments None

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:FVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Frequency versus Time trace.

Syntax :CALCulate:FVTime:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:FVTime:MARKer<x>:PEAK:LOWer

:CALCulate:FVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Frequency versus Time measurement.

Syntax :CALCulate:FVTime:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:FVTime:MARKer<x>:PEAK:RIGHT

:CALCulate:FVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Frequency versus Time trace.

Syntax :CALCulate:FVTime:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:FVTime:MARKer<x>:PEAK:HIGHer

:CALCulate:FVTime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Frequency versus Time measurement.

Syntax :CALCulate:FVTime:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:FVTime:MARKer<x>:PEAK:LEFT

:CALCulate:FVTime:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the Frequency versus Time measurement.

Syntax :CALCulate:FVTime:MARKer<x>:X <value>
 :CALCulate:FVTime:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: (analysis offset) to [(analysis offset) + (analysis length)].

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:X 1.5u
 places Marker 1 (M1) at 1.5 μ s on the trace.

Related Commands :CALCulate:FVTime:MARKer<x>:Y?

:CALCulate:FVTime:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the Frequency versus Time measurement.

Syntax :CALCulate:FVTime:MARKer<x>:Y?

Arguments None

Measurement Views Frequency versus Time

Examples :CALCulate:FVTime:MARKer1:Y?
 might return -15.34E+6 indicating Marker 1 (M1) is at -15.34 MHz.

Related Commands :CALCulate:FVTime:MARKer<x>:X

:CALCulate:IQVTime Subgroup

The :CALCulate:IQVTime commands control the markers in the RF I&Q versus Time measurements.

Command Tree	Header	Parameter
	:CALCulate	
	:IQVTime	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:TRACE	TRACE1 TRACE2
	:X	<numeric_value>
	:Y?	

:CALCulate:IQVTime:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the RF I&Q versus Time measurement.

Syntax :CALCulate:IQVTime:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:DELTA:X?
might return 120.0E-9, indicating that the delta marker time is 120 ns.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:IQVTime:MARKer<x>:DELTA:Y?

:CALCulate:IQVTime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the RF I&Q versus Time measurement.

Syntax :CALCulate:IQVTime:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:DELTA:Y?
might return -3.45E-3, indicating that the delta marker amplitude is -3.45 mV.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:IQVTime:MARKer<x>:DELTA:X?

:CALCulate:IQVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the RF I&Q versus Time measurement.

Syntax :CALCulate:IQVTime:MARKer<x>:MAXimum

Arguments None

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the RF I&Q versus Time trace.

Syntax :CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

:CALCulate:IQVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the RF I&Q versus Time measurement.

Syntax :CALCulate:IQVTime:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT

:CALCulate:IQVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the RF I&Q versus Time trace.

Syntax :CALCulate:IQVTime:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer

:CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the RF I&Q versus Time measurement.

Syntax :CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:IQVTime:MARKer<x>:PEAK:LEFT

:CALCulate:IQVTime:MARKer<x>:TRACe(?)

Places the selected marker on the I or Q trace in the RF I&Q versus Time measurement.

The query command returns which trace the selected marker is placed on.

Syntax :CALCulate:IQVTime:MARKer<x>:TRACe { TRACE1 | TRACE2 }
 :CALCulate:IQVTime:MARKer<x>:TRACe?

Arguments TRACE1 places the selected marker on the I trace.
 TRACE2 places the selected marker on the Q trace.

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:TRACe TRACE1
 places Marker 1 (M1) on the I trace.

:CALCulate:IQVTime:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the RF I&Q versus Time measurement.

Syntax :CALCulate:IQVTime:MARKer<x>:X <value>
 :CALCulate:IQVTime:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
 Range: (analysis offset) to [(analysis offset) + (analysis length)].

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:X 1.5us
 places Marker 1 (M1) at 1.5 μ s on the trace.

Related Commands :CALCulate:IQVTime:MARKer<x>:Y?

:CALCulate:IQVTime:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the RF I&Q versus Time measurement.

Syntax :CALCulate:IQVTime:MARKer<x>:Y?

Arguments None

Measurement Views RF I&Q versus Time

Examples :CALCulate:IQVTime:MARKer1:Y?
 might return 25.803E-3 indicating Marker 1 (M1) is at 25.803 mV.

Related Commands :CALCulate:IQVTime:MARKer<x>:X

:CALCulate:MCPower Subgroup

The :CALCulate:MCPower commands control the markers in the MCPR (Multiple Carrier Power Ratio) measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:MCPower	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:LEFT	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

:CALCulate:MCPower:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker in the MCPR measurement.

Syntax :CALCulate:MCPower:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker frequency for the selected marker.

Measurement Views MCPR

Examples :CALCulate:MCPower:MARKer1:DELTA:X?
might return 1.28E+6, indicating that the delta marker frequency is 1.28 MHz.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:MCPower:MARKer<x>:DELTA:Y?

:CALCulate:MCPower:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the MCPR measurement.

Syntax :CALCulate:MCPower:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views MCPR

Examples :CALCulate:MCPower:MARKer1:DELTA:Y?
might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:MCPower:MARKer<x>:DELTA:X?

:CALCulate:MCPower:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the MCPR measurement.

Syntax :CALCulate:MCPower:MARKer<x>:MAXimum

Arguments None

Measurement Views MCPR

Examples :CALCulate:MCPower:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:MCPower:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the MCPR measurement.

Syntax :CALCulate:MCPower:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views MCPR

Examples :CALCulate:MCPower:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:MCPower:MARKer<x>:PEAK:RIGHT

:CALCulate:MCPower:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the MCPR measurement.

Syntax :CALCulate:MCPower:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views MCPR

Examples :CALCulate:MCPower:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:MCPower:MARKer<x>:PEAK:LEFT

:CALCulate:MCPower:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the MCPR measurement.

Syntax :CALCulate:MCPower:MARKer<x>:X <value>
:CALCulate:MCPower:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: (center frequency) \pm (span)/2.

Measurement Views MCPR

Examples :CALCulate:MCPower:MARKer1:X 800MHz
places Marker 1 (M1) at 800 MHz on the trace.

Related Commands :CALCulate:MCPower:MARKer<x>:Y?

:CALCulate:MCPower:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the MCPR measurement.

Syntax :CALCulate:MCPower:MARKer<x>:Y?

Arguments None

Measurement Views MCPR

Examples :CALCulate:MCPower:MARKer1:Y?
might return -34.28 indicating Marker 1 (M1) is at -34.28 dBm.

Related Commands :CALCulate:MCPower:MARKer<x>:X

:CALCulate:MERRor Subgroup (Option 21 Only)

The :CALCulate:MERRor commands control the markers in the Magnitude error versus Time measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:MERRor	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

:CALCulate:MERRor:MARKer<x>:DELTa:X? (Query Only)

Returns the delta marker time for the selected marker in the Magnitude error versus Time measurement.

Syntax :CALCulate:MERRor:MARKer<x>:DELTa:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:DELTa:X?
might return 9.52, indicating that the delta marker time is 9.52 symbols.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:MERRor:MARKer<x>:DELTa:Y?

:CALCulate:MERRor:MARKer<x>:DELTa:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the Magnitude error versus Time measurement.

Syntax :CALCulate:MERRor:MARKer<x>:DELTa:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:DELTa:Y?
might return 3.84, indicating that the delta marker amplitude is 3.84%.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:MERRor:MARKer<x>:DELTa:X?

:CALCulate:MERRor:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Magnitude error versus Time measurement.

Syntax :CALCulate:MERRor:MARKer<x>:MAXimum

Arguments None

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:MERRor:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Magnitude error versus Time trace.

Syntax :CALCulate:MERRor:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:MERRor:MARKer<x>:PEAK:LOWer

:CALCulate:MERRor:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Magnitude error versus Time measurement.

Syntax :CALCulate:MERRor:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:MERRor:MARKer<x>:PEAK:RIGHT

:CALCulate:MERRor:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Magnitude error versus Time trace.

Syntax :CALCulate:MERRor:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:MERRor:MARKer<x>:PEAK:HIGHer

:CALCulate:MERRor:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Magnitude error versus Time measurement.

Syntax :CALCulate:MERRor:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:MERRor:MARKer<x>:PEAK:LEFT

:CALCulate:MERRor:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the Magnitude error versus Time measurement.

Syntax :CALCulate:MERRor:MARKer<x>:X <value>
:CALCulate:MERRor:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: (analysis offset) to [(analysis offset) + (analysis length)].

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:X 1.5u
places Marker 1 (M1) at 1.5 μ s on the trace.

Related Commands :CALCulate:MERRor:MARKer<x>:Y?

:CALCulate:MERRor:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the Magnitude error versus Time measurement.

Syntax :CALCulate:MERRor:MARKer<x>:Y?

Arguments None

Measurement Views Magnitude error versus Time

Examples :CALCulate:MERRor:MARKer1:Y?
might return -15.34E+6 indicating Marker 1 (M1) is at -15.34 MHz.

Related Commands :CALCulate:MERRor:MARKer<x>:X

:CALCulate:OBWidth Subgroup

The :CALCulate:OBWidth commands control the markers in the Occupied Bandwidth (OBW) measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:OBWidth	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	[:SET]	
	:CENTer	
	:X	<numeric_value>
	:Y?	

:CALCulate:OBWidth:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker in the Occupied Bandwidth measurement.

Syntax :CALCulate:OBWidth:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker frequency for the selected marker.

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:DELTA:X?
might return 1.28E+6, indicating that the delta marker frequency is 1.28 MHz.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:OBWidth:MARKer<x>:DELTA:Y?

:CALCulate:OBWidth:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the Occupied Bandwidth measurement.

Syntax :CALCulate:OBWidth:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:DELTA:Y?
might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:OBWidth:MARKer<x>:DELTA:X?

:CALCulate:OBWidth:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Occupied Bandwidth measurement.

Syntax :CALCulate:OBWidth:MARKer<x>:MAXimum

Arguments None

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Occupied Bandwidth trace.

Syntax :CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:OBWidth:MARKer<x>:PEAK:LOWer

:CALCulate:OBWidth:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Occupied Bandwidth measurement.

Syntax :CALCulate:OBWidth:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:OBWidth:MARKer<x>:PEAK:RIGHT

:CALCulate:OBWidth:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Occupied Bandwidth trace.

Syntax :CALCulate:OBWidth:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer

:CALCulate:OBWidth:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Occupied Bandwidth measurement.

Syntax :CALCulate:OBWidth:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:OBWidth:MARKer<x>:PEAK:LEFT

:CALCulate:OBWidth:MARKer<x>[:SET]:CENTer (No Query Form)

Sets the center frequency to the value at the marker position in the Occupied Bandwidth measurement.

Syntax :CALCulate:OBWidth:MARKer<x>[:SET]:CENTer

Arguments None

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:SET:CENTer
sets the center frequency to the value at the Marker 1 position.

:CALCulate:OBWidth:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the Occupied Bandwidth measurement.

Syntax :CALCulate:OBWidth:MARKer<x>:X <value>
 :CALCulate:OBWidth:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: (center frequency) \pm (span)/2.

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:X 800MHz
 places Marker 1 (M1) at 800 MHz on the trace.

Related Commands :CALCulate:OBWidth:MARKer<x>:Y?

:CALCulate:OBWidth:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the Occupied Bandwidth measurement.

Syntax :CALCulate:OBWidth:MARKer<x>:Y?

Arguments None

Measurement Views Occupied Bandwidth

Examples :CALCulate:OBWidth:MARKer1:Y?
 might return -34.28 indicating Marker 1 (M1) is at -34.28 dBm.

Related Commands :CALCulate:OBWidth:MARKer<x>:X

:CALCulate:PERRor Subgroup (Option 21 Only)

The :CALCulate:PERRor commands control the markers in the Phase error versus Time measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:PERRor	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

:CALCulate:PERRor:MARKer<x>:DELTa:X? (Query Only)

Returns the delta marker time for the selected marker in the Phase error versus Time measurement.

Syntax :CALCulate:PERRor:MARKer<x>:DELTa:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:DELTa:X?
might return 9.52, indicating that the delta marker time is 9.52 symbols.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:PERRor:MARKer<x>:DELTa:Y?

:CALCulate:PERRor:MARKer<x>:DELTa:Y? (Query Only)

Returns the delta marker phase for the selected marker in the Phase error versus Time measurement.

Syntax :CALCulate:PERRor:MARKer<x>:DELTa:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker phase for the selected marker.

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:DELTa:Y?
might return -7.93, indicating that the delta marker phase is -7.93°.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:PERRor:MARKer<x>:DELTa:X?

:CALCulate:PERRor:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Phase error versus Time measurement.

Syntax :CALCulate:PERRor:MARKer<x>:MAXimum

Arguments None

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:PERRor:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Phase error versus Time trace.

Syntax :CALCulate:PERRor:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:PERRor:MARKer<x>:PEAK:LOWer

:CALCulate:PERRor:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Phase error versus Time measurement.

Syntax :CALCulate:PERRor:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:PERRor:MARKer<x>:PEAK:RIGHT

:CALCulate:PERRor:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Phase error versus Time trace.

Syntax :CALCulate:PERRor:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:PEAK:LOWer
moves Marker 1 (M1) lower in amplitude to the next peak on the trace.

Related Commands :CALCulate:PERRor:MARKer<x>:PEAK:HIGHer

:CALCulate:PERRor:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Phase error versus Time measurement.

Syntax :CALCulate:PERRor:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:PERRor:MARKer<x>:PEAK:LEFT

:CALCulate:PERRor:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the Phase error versus Time measurement.

Syntax :CALCulate:PERRor:MARKer<x>:X <value>
:CALCulate:PERRor:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: (analysis offset) to [(analysis offset) + (analysis length)].

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:X 1.5u
places Marker 1 (M1) at 1.5 μ s on the trace.

Related Commands :CALCulate:PERRor:MARKer<x>:Y?

:CALCulate:PERRor:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the Phase error versus Time measurement.

Syntax :CALCulate:PERRor:MARKer<x>:Y?

Arguments None

Measurement Views Phase error versus Time

Examples :CALCulate:PERRor:MARKer1:Y?
might return -15.34E+6 indicating Marker 1 (M1) is at -15.34 MHz.

Related Commands :CALCulate:PERRor:MARKer<x>:X

:CALCulate:PHVTime Subgroup

The :CALCulate:PHVTime commands control the markers in the Phase versus Time measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:PHVTime	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

:CALCulate:PHVTime:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker in the Phase versus Time measurement.

Syntax :CALCulate:PHVTime:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:DELTA:X?
might return 38.0E-9, indicating that the delta marker time is 38.0 ns.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:PHVTime:MARKer<x>:DELTA:Y?

:CALCulate:PHVTime:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker phase for the selected marker in the Phase versus Time measurement.

Syntax :CALCulate:PHVTime:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker phase for the selected marker.

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:DELTA:Y?
might return 162.38, indicating that the delta marker phase is 162.38°.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:PHVTime:MARKer<x>:DELTA:X?

:CALCulate:PHVTime:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the trace in the Phase versus Time measurement.

Syntax :CALCulate:PHVTime:MARKer<x>:MAXimum

Arguments None

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the Phase versus Time trace.

Syntax :CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:PHVTime:MARKer<x>:PEAK:LOWer

:CALCulate:PHVTime:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the trace in the Phase versus Time measurement.

Syntax :CALCulate:PHVTime:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT

:CALCulate:PHVTime:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the Phase versus Time trace.

Syntax :CALCulate:PHVTime:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer

:CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the trace in the Phase versus Time measurement.

Syntax :CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:PHVTime:MARKer<x>:PEAK:LEFT

:CALCulate:PHVTime:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the Phase versus Time measurement.

Syntax :CALCulate:PHVTime:MARKer<x>:X <value>
:CALCulate:PHVTime:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: (analysis offset) to [(analysis offset) + (analysis length)].

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:X 1.5us
places Marker 1 (M1) at 1.5 μ s on the trace.

Related Commands :CALCulate:PHVTime:MARKer<x>:Y?

:CALCulate:PHVTime:MARKer<x>:Y?

Queries the vertical position of the selected marker in the Phase versus Time measurement.

Syntax :CALCulate:PHVTime:MARKer<x>:Y?

Arguments None

Measurement Views Phase versus Time

Examples :CALCulate:PHVTime:MARKer1:Y?
might return -18.435 indicating Marker 1 (M1) is at -18.435°.

Related Commands :CALCulate:PHVTime:MARKer<x>:X

:CALCulate:PULSe Subgroup (Option 20 Only)

The :CALCulate:PULSe commands control the markers in the pulsed RF measurements.

Command Tree	Header	Parameter
	:CALCulate	
	:PULSe	
	:STATistics	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:X	<numeric_value>
	:Y?	
	:TRACe	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

NOTE. The :CALCulate:PULSe:STATistics commands are valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

For the marker mnemonics, refer to page 2-70.

:CALCulate:PULSe:STATistics:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker on the pulse trace.
This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker frequency for the selected marker.

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:DELTA:X?
might return 614.2, indicating that the delta marker frequency is 614.2 Hz.

Related Commands :CALCulate:MARKer:ADD, :DISPlay:PULSe:STATistics:PLOT,
:CALCulate:PULSe:STATistics:MARKer<x>:DELTA:Y?

:CALCulate:PULSe:STATistics:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the pulse trace.
This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:DELTA:Y?
might return 2.345, indicating that the delta marker amplitude is 2.345 dB.

Related Commands :CALCulate:MARKer:ADD, :DISPlay:PULSe:STATistics:PLOT,
:CALCulate:PULSe:STATistics:MARKer<x>:DELTA:X?

:CALCulate:PULSe:STATistics:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the pulse statistics trace. This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:MAXimum

Arguments None

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:CALCulate:PULSe:STATistics:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the pulse statistics trace. This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LOWer,
:DISPlay:PULSe:STATistics:PLOT

:CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the pulse statistics trace. This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:PULSe:STATistics:MARKer<x>:PEAK:RIGHT,
:DISPlay:PULSe:STATistics:PLOT

:CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the pulse statistics trace. This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:PULSe:STATistics:MARKer<x>:PEAK:HIGHer,
:DISPlay:PULSe:STATistics:PLOT

:CALCulate:PULSe:STATistics:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the pulse statistics trace. This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:PULSe:STATistics:MARKer<x>:PEAK:LEFT,
:DISPlay:PULSe:STATistics:PLOT

:CALCulate:PULSe:STATistics:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the pulse statistics view. This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:X <value>
:CALCulate:PULSe:STATistics:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
Range: 0 to half of the average repetition rate for all detected pulses in Hz.

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:X 12.5kHz
places Marker 1 (M1) at 12.5 kHz on the trace.

Related Commands :CALCulate:PULSe:STATistics:MARKer<x>:Y?,
:DISPlay:PULSe:STATistics:PLOT

:CALCulate:PULSe:STATistics:MARKer<x>:Y?

Queries the vertical position of the selected marker in the pulse statistics view. This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :CALCulate:PULSe:STATistics:MARKer<x>:Y?

Arguments None

Measurement Views Pulse statistics

Examples :CALCulate:PULSe:STATistics:MARKer1:Y?
might return -28.173 indicating Marker 1 (M1) is at -28.173 dB.

Related Commands :CALCulate:PULSe:STATistics:MARKer<x>:X,
:DISPlay:PULSe:STATistics:PLOT

:CALCulate:PULSe:TRACe:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker on the pulse trace.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:DELTA:X?
might return 38.0E-9, indicating that the delta marker time is 38.0 ns.

Related Commands :CALCulate:MARKer:ADD,
:CALCulate:PULSe:TRACe:MARKer<x>:DELTA:Y?

:CALCulate:PULSe:TRACe:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the pulse trace.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:DELTA:Y?
might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

Related Commands :CALCulate:MARKer:ADD,
:CALCulate:PULSe:TRACe:MARKer<x>:DELTA:X?

:CALCulate:PULSe:TRACe:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the pulse trace.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:MAXimum

Arguments None

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:PULSe:TRACe:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the pulse trace.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LOWer

:CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the pulse trace.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:PULSe:TRACe:MARKer<x>:PEAK:RIGHT

:CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the pulse trace.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:PULSe:TRACe:MARKer<x>:PEAK:HIGHer

:CALCulate:PULSe:TRACe:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the pulse trace.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:PULSe:TRACe:MARKer<x>:PEAK:LEFT

:CALCulate:PULSe:TRACe:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker in the pulse trace view.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:X <value>
 :CALCulate:PULSe:TRACe:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.

NOTE. To set the horizontal position, the marker must be on the trace of the pulse selected using the :DISPlay:PULSe:SElect:NUMBer command. You cannot put the marker out of the horizontal range of the pulse.

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:X 1.5us
 places Marker 1 (M1) at 1.5 μ s on the trace.

Related Commands :CALCulate:PULSe:TRACe:MARKer<x>:Y?
 :DISPlay:PULSe:SElect:NUMBer

:CALCulate:PULSe:TRACe:MARKer<x>:Y?

Queries the vertical position of the selected marker in the pulse trace view.

Syntax :CALCulate:PULSe:TRACe:MARKer<x>:Y?

Arguments None

Measurement Views Pulse trace

Examples :CALCulate:PULSe:TRACe:MARKer1:Y?
 might return 228.858E-3 indicating Marker 1 (M1) is at 228.858 mV.

Related Commands :CALCulate:PULSe:TRACe:MARKer<x>:X

:CALCulate:SGRam Subgroup

The :CALCulate:SGRam commands control the markers in the spectrogram.

Command Tree	Header	Parameter
	:CALCulate	
	:SGRam	
	:MARKer<x>	
	:DELTA	
	:X	
	:FREQuency?	
	[:TIME]?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	[:SET]	
	:CENTer	
	:X	
	:FREQuency	<numeric_value>
	[:TIME]	<numeric_value>
	:Y?	

:CALCulate:SGRam:MARKer<x>:DELTA:X:FREQuency? (Query Only)

Returns the delta marker frequency for the selected marker in the spectrogram.

Syntax :CALCulate:SGRam:MARKer<x>:DELTA:X:FREQuency?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker frequency for the selected marker.

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:DELTA:X:FREQuency?
might return 5.95E+6, indicating that the delta marker frequency is 5.95 MHz.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:SGRam:MARKer<x>:DELTA:Y?

:CALCulate:SGRam:MARKer<x>:DELTA:X[:TIME]? (Query Only)

Returns the delta marker time for the selected marker in the spectrogram.

Syntax :CALCulate:SGRam:MARKer<x>:DELTA:X[:TIME]?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:DELTA:X:TIME?
might return -1.84E-3, indicating that the delta marker time is -1.84 ms.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:SGRam:MARKer<x>:DELTA:Y?

:CALCulate:SGRam:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker in the spectrogram.

Syntax :CALCulate:SGRam:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:DELTA:Y?
might return -8.45, indicating that the delta marker amplitude is -8.45 dB.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:SGRam:MARKer<x>:DELTA:X?

:CALCulate:SGRam:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on a line in the spectrogram. The line is selected using the :TRACe:SGRam:SElect:LINE command.

Syntax :CALCulate:SGRam:MARKer<x>:MAXimum

Arguments None

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the line.

Related Commands :TRACe:SGRam:SElect:LINE

:CALCulate:SGRam:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on a line in the spectrogram. The line is selected using the :TRACe:SGRam:SElect:LINE command.

Syntax :CALCulate:SGRam:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the line.

Related Commands :CALCulate:SGRam:MARKer<x>:PEAK:LOWer
:TRACe:SGRam:SElect:LINE

:CALCulate:SGRam:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on a line in the spectrogram. The line is selected using the :TRACe:SGRam:SElect:LINE command.

Syntax :CALCulate:SGRam:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the line.

Related Commands :CALCulate:SGRam:MARKer<x>:PEAK:RIGHT
:TRACe:SGRam:SElect:LINE

:CALCulate:SGRam:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on a line in the spectrogram. The line is selected using the :TRACe:SGRam:SElect:LINE command.

Syntax :CALCulate:SGRam:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the line.

Related Commands :CALCulate:SGRam:MARKer<x>:PEAK:HIGHer
:TRACe:SGRam:SElect:LINE

:CALCulate:SGRam:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on a line in the spectrogram. The line is selected using the :TRACe:SGRam:SElect:LINE command.

Syntax :CALCulate:SGRam:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:SGRam:MARKer<x>:PEAK:LEFT
:TRACe:SGRam:SElect:LINE

:CALCulate:SGRam:MARKer<x>[:SET]:CENTer (No Query Form)

Sets the center frequency to the marker frequency in the spectrogram.

Syntax :CALCulate:SGRam:MARKer<x>[:SET]:CENTer

Arguments None

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:SET:CENTer
sets the center frequency to the Marker 1 frequency in the spectrogram.

:CALCulate:SGRam:MARKer<x>:X:FREQuency(?)

Sets or queries the marker frequency in the spectrogram.

Syntax :CALCulate:SGRam:MARKer<x>:X <value>
:CALCulate:SGRam:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the marker frequency.
Range: (center frequency) \pm (span)/2.

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:X 800MHz
places Marker 1 (M1) at 800 MHz on the trace.

Related Commands :CALCulate:SGRam:MARKer<x>:Y?

:CALCulate:SGRam:MARKer<x>:X[:TIME](?)

Sets or queries the marker time in the spectrogram.

Syntax :CALCulate:SGRam:MARKer<x>:X[:TIME] <value>
 :CALCulate:SGRam:MARKer<x>:X[:TIME]?

Arguments <value>::=<NRf> specifies the marker time.

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:X:TIME -234.5us
 places Marker 1 (M1) at -234.5 μ s on the trace.

Related Commands :CALCulate:SGRam:MARKer<x>:Y?

:CALCulate:SGRam:MARKer<x>:Y? (Query Only)

Queries the marker amplitude in the spectrogram.

Syntax :CALCulate:SGRam:MARKer<x>:Y?

Arguments None

Measurement Views Spectrogram

Examples :CALCulate:SGRam:MARKer1:Y?
 might return -34.28 indicating Marker 1 (M1) is at -34.28 dBm.

Related Commands :CALCulate:SGRam:MARKer<x>:X

:CALCulate:SPECTrum Subgroup

The :CALCulate:SPECTrum commands control the markers in the Spectrum measurement.

Command Tree	Header	Parameter
	:CALCulate	
	:SPECTrum	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	[:SET]	
	:CENTer	
	:TRACE	TRACE1 TRACE2 TRACE3 TRACE4 TRACE5
	:X	<numeric_value>
	:Y?	

:CALCulate:SPECTrum:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker frequency for the selected marker on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker frequency for the selected marker.

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:DELTA:X?
might return 1.28E+6, indicating that the delta marker frequency is 1.28 MHz.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:SPECTrum:MARKer<x>:DELTA:Y?

:CALCulate:SPECTrum:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:DELTA:Y?
might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:SPECTrum:MARKer<x>:DELTA:X?

:CALCulate:SPECTrum:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:MAXimum

Arguments None

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:SPECTrum:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:SPECTrum:MARKer<x>:PEAK:LOWer

:CALCulate:SPECTrum:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:SPECTrum:MARKer<x>:PEAK:RIGHT

:CALCulate:SPECTrum:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:SPECTrum:MARKer<x>:PEAK:HIGHer

:CALCulate:SPECTrum:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:SPECTrum:MARKer<x>:PEAK:LEFT

:CALCulate:SPECTrum:MARKer<x>[:SET]:CENTer (No Query Form)

Sets the center frequency to the marker frequency in the spectrum measurement.

Syntax :CALCulate:SPECTrum:MARKer<x>[:SET]:CENTer

Arguments None

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:SET:CENTer
sets the center frequency to the marker frequency in the spectrum measurement.

:CALCulate:SPECTrum:MARKer<x>:TRACe(?)

Selects or queries the trace on which the specified marker is placed in the spectrum measurement.

Syntax :CALCulate:SPECTrum:MARKer<x>:TRACe
 { TRACE1 | TRACE2 | TRACE3 | TRACE4 | TRACE5 }
 :CALCulate:SPECTrum:MARKer<x>:TRACe?

Arguments TRACE1 places the specified marker on Trace 1.
 TRACE2 places the specified marker on Trace 2.
 TRACE3 places the specified marker on n Trace 3.
 TRACE4 places the specified marker on Trace 4 (math trace).
 TRACE5 places the specified marker on Trace 5 (spectrogram).
 Trace 1 to 3 can be defined as Normal, Average, Max Hold or Min Hold using
 the :TRACe<x>:SPECTrum:FUNctIon command.

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:TRACe TRACE1
 places Marker 1 (M1) on Trace 1.

Related Commands :TRACe<x>:SPECTrum:FUNctIon

:CALCulate:SPECTrum:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:X <value>
 :CALCulate:SPECTrum:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
 Range: (center frequency) \pm (span)/2.

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:X 800MHz
 places Marker 1 (M1) at 800 MHz on the spectrum trace.

Related Commands :CALCulate:SPECTrum:MARKer<x>:Y?

:CALCulate:SPECTrum:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker on the spectrum trace.

Syntax :CALCulate:SPECTrum:MARKer<x>:Y?

Arguments None

Measurement Views Spectrum

Examples :CALCulate:SPECTrum:MARKer1:Y?
 might return -34.28 indicating Marker 1 (M1) is at -34.28 dBm.

Related Commands :CALCulate:SPECTrum:MARKer<x>:X

:CALCulate:TOVerview Subgroup

The :CALCulate:TOVerview commands control the markers in the Time Overview.

Command Tree	Header	Parameter
	:CALCulate	
	:TOVerview	
	:MARKer<x>	
	:DELTA	
	:X?	
	:Y?	
	:MAXimum	
	:PEAK	
	:HIGHer	
	:LEFT	
	:LOWer	
	:RIGHT	
	:X	<numeric_value>
	:Y?	

:CALCulate:TOVerview:MARKer<x>:DELTA:X? (Query Only)

Returns the delta marker time for the selected marker on the time overview trace.

Syntax :CALCulate:TOVerview:MARKer<x>:DELTA:X?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker time for the selected marker.

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:DELTA:X?
might return 38.0E-9, indicating that the delta marker time is 38.0 ns.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:TOVerview:MARKer<x>:DELTA:Y?

:CALCulate:TOVerview:MARKer<x>:DELTA:Y? (Query Only)

Returns the delta marker amplitude for the selected marker on the time overview trace.

Syntax :CALCulate:TOVerview:MARKer<x>:DELTA:Y?

Where <x> = 1 to 4; MARKer0 (reference marker) is invalid. The specified marker must be activated using the :CALCulate:MARKer:ADD command.

Returns <NRf> Delta marker amplitude for the selected marker.

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:DELTA:Y?
might return 23.45, indicating that the delta marker amplitude is 23.45 dB.

Related Commands :CALCulate:MARKer:ADD, :CALCulate:TOVerview:MARKer<x>:DELTA:X?

:CALCulate:TOVerview:MARKer<x>:MAXimum (No Query Form)

Moves the selected marker to the highest peak on the time overview trace.

Syntax :CALCulate:TOVerview:MARKer<x>:MAXimum

Arguments None

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:MAXimum
moves Marker 1 (M1) to the highest peak on the trace.

:CALCulate:TOVerview:MARKer<x>:PEAK:HIGHer (No Query Form)

Moves the selected marker to the next peak higher in amplitude on the time overview trace.

Syntax :CALCulate:TOVerview:MARKer<x>:PEAK:HIGHer

Arguments None

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:PEAK:HIGHer
moves Marker 1 (M1) to the next peak higher in amplitude on the trace.

Related Commands :CALCulate:TOVerview:MARKer<x>:PEAK:LOWer

:CALCulate:TOVerview:MARKer<x>:PEAK:LEFT (No Query Form)

Moves the selected marker to the next peak to the left on the time overview trace.

Syntax :CALCulate:TOVerview:MARKer<x>:PEAK:LEFT

Arguments None

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:PEAK:LEFT
moves Marker 1 (M1) to the next peak to the left on the trace.

Related Commands :CALCulate:TOVerview:MARKer<x>:PEAK:RIGHT

:CALCulate:TOVerview:MARKer<x>:PEAK:LOWer (No Query Form)

Moves the selected marker to the next peak lower in amplitude on the time overview trace.

Syntax :CALCulate:TOVerview:MARKer<x>:PEAK:LOWer

Arguments None

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:PEAK:LOWer
moves Marker 1 (M1) to the next peak lower in amplitude on the trace.

Related Commands :CALCulate:TOVerview:MARKer<x>:PEAK:HIGHer

:CALCulate:TOVerview:MARKer<x>:PEAK:RIGHT (No Query Form)

Moves the selected marker to the next peak to the right on the time overview trace.

Syntax :CALCulate:TOVerview:MARKer<x>:PEAK:RIGHT

Arguments None

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:PEAK:RIGHT
moves Marker 1 (M1) to the next peak to the right on the trace.

Related Commands :CALCulate:TOVerview:MARKer<x>:PEAK:LEFT

:CALCulate:TOVerview:MARKer<x>:X(?)

Sets or queries the horizontal position of the selected marker on the time overview trace.

Syntax :CALCulate:TOVerview:MARKer<x>:X <value>
 :CALCulate:TOVerview:MARKer<x>:X?

Arguments <value>::=<NRf> specifies the horizontal position of the marker.
 Range: (center frequency) \pm (span)/2.

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:X 800MHz
 places Marker 1 (M1) at 800 MHz on the trace.

Related Commands :CALCulate:TOVerview:MARKer<x>:Y?

:CALCulate:TOVerview:MARKer<x>:Y? (Query Only)

Queries the vertical position of the selected marker in the time overview.

Syntax :CALCulate:TOVerview:MARKer<x>:Y?

Arguments None

Measurement Views Time overview

Examples :CALCulate:TOVerview:MARKer1:Y?
 might return -34.28 indicating Marker 1 (M1) is at -34.28 dBm.

Related Commands :CALCulate:TOVerview:MARKer<x>:X

CALibration Commands

The CALibration commands perform correction for the external gain/loss and probe.

Command Tree

Header	Parameter
:CALibration	
:ABORt	
:AUTO	<boolean>
:CORRection	
:EXTeRnal	
:EDIT<x>	
:LABe1	<string>
:STATe	<boolean>
:GAIN	
[:MAGNitude]	<numeric_value>
:STATe	<boolean>
:PROBe	
:CONNeCt?	
[:MAGNitude]?	
:STATe	<boolean>

Where <x> = 1 to 3 indicates the following:

EDIT1: External Loss Table 1
EDIT2: External Loss Table 2
EDIT3: External Loss Table 3

:CALibration:ABORt (No Query Form)

Aborts any actions related to the alignments in progress.

Syntax :CALibration:ABORt

Arguments None

Measurement Views All

Examples :CALibration:ABORt
aborts any actions related to the alignments in progress.

:CALibration:AUTO(?)

Selects or queries whether or not to run alignments automatically.

Syntax :CALibration:AUTO { OFF | ON | 0 | 1 }
:CALibration:AUTO?

Arguments OFF or 0 runs alignments on user request.
Use the *CAL? command to perform alignments.
ON or 1 runs alignments as needed without user intervention.
You have to restart measurement if interrupted.

Measurement Views All

Examples :CALibration:AUTO ON
runs alignments automatically as needed.

Related Commands *CAL?

:CALibration:CORRection:EXTeRnal:EDIT<x>:LABel(?)

Sets or queries the name of the external loss table.

Syntax :CALibration:CORRection:EXTeRnal:EDIT<x>:LABel <name>
:CALibration:CORRection:EXTeRnal:EDIT<x>:LABel?

Where <x> = 1 to 3 represent the External Loss Table 1 to 3, respectively.

Arguments <name>::=<string> specifies the name of the external loss table.

Measurement Views All

Examples :CALibration:CORRection:EXTeRnal:EDIT1:LABel "Sample Table 1"
names the External Loss Table 1 "Sample Table 1".

:CALibration:CORRection:EXTeRnal:EDIT<x>:STATe(?)

Determines whether to enable or disable the external loss table.

Syntax :CALibration:CORRection:EXTeRnal:EDIT<x>:STATe
{ OFF | ON | 0 | 1 }
:CALibration:CORRection:EXTeRnal:EDIT<x>:STATe?

Where <x> = 1 to 3 represent the External Loss Table 1 to 3, respectively.

Arguments OFF or 0 disables the external loss table.
ON or 1 enables the external loss table.

NOTE. You can enable one or more tables at the same time.

Measurement Views All

Examples :CALibration:CORRection:EXTeRnal:EDIT3:STATe ON
enables the External Loss Table 3.

:CALibration:CORRection:EXTeRnal:GAIN[:MAGNitude](?)

Sets or queries the external gain value. It can be enabled or disabled using the :CALibration:CORRection:EXTeRnal:GAIN:STATe command.

Syntax :CALibration:CORRection:EXTeRnal:GAIN[:MAGNitude] <value>
:CALibration:CORRection:EXTeRnal:GAIN[:MAGNitude]?

Arguments <value>::=<NRf> specifies the external gain value. Range: -50 to +30 dB.

Measurement Views All

Examples :CALibration:CORRection:EXTeRnal:GAIN:MAGNitude -10
sets the external gain to -10 dB.

Related Commands :CALibration:CORRection:EXTeRnal:GAIN:STATe

:CALibration:CORRection:EXTeRnal:GAIN:STATe(?)

Determines whether to enable or disable the external gain value.

Syntax :CALibration:CORRection:EXTeRnal:GAIN:STATe { OFF | ON | 0 | 1 }
:CALibration:CORRection:EXTeRnal:GAIN:STATe?

Arguments OFF or 0 disables the external gain value.
ON or 1 enables the external gain value.

Measurement Views All

Examples :CALibration:CORRection:EXTeRnal:GAIN:STATe ON
enables the external gain value.

Related Commands :CALibration:CORRection:EXTeRnal:GAIN[:MAGNitude]

:CALibration:CORRection:EXTeRnal:PROBe:CONNeCt? (Query Only)

Queries whether the external probe is connected to the analyzer or not.

Syntax :CALibration:CORRection:EXTeRnal:PROBe:CONNeCt?

Arguments None

Returns { 0 | 1 }

0 indicates that the external probe is not connected to the analyzer.

1 indicates that the external probe is connected to the analyzer.

Measurement Views All

Examples :CALibration:CORRection:EXTeRnal:PROBe:CONNeCt?
might return ON, indicating that the external probe is connected to the analyzer.

:CALibration:CORRection:EXTeRnal:PROBe[:MAGNitude]? (Query Only)

Queries the external probe attenuation.

Syntax :CALibration:CORRection:EXTeRnal:PROBe[:MAGNitude]?

Arguments None

Returns <attenuation>::=<NRf> The probe attenuation value in dB.

Measurement Views All

Examples :CALibration:CORRection:EXTeRnal:PROBe:MAGNitude?
might return 10, indicating that the probe attenuation is 10 dB.

:CALibration:CORRection:EXTernal:PROBe:STATe(?)

Determines whether or not to correct data for the external probe attenuation.

Syntax :CALibration:CORRection:EXTernal:PROBe:STATe { OFF | ON | 0 | 1 }
 :CALibration:CORRection:EXTernal:PROBe:STATe?

Arguments OFF or 0 does not correct data for the external probe attenuation.
 ON or 1 corrects data for the external probe attenuation.

Measurement Views All

Examples :CALibration:CORRection:EXTernal:PROBe:STATe ON
 corrects data for the external probe attenuation.

DISPlay Commands

The DISPlay commands control the display of measurement data on the screen. These commands are divided by measurement views into the subgroups listed in Table 2-31.

Table 2-31: DISPlay command subgroups

Command header	Measurement view	Refer to:
:DISPlay (basic)	All views, general window control	page 2-196
:DISPlay:ACPower	Channel power and ACPR	page 2-199
:DISPlay:AVTime	Amplitude versus Time	page 2-205
:DISPlay:CONSte	Constellation (Option 21 only)	page 2-216
:DISPlay:DDEMod	General purpose digital modulation measurements (Option 21 only)	page 2-217
:DISPlay:DPSA	DPX (Digital Phosphor) spectrum	page 2-226
:DISPlay:EVM	EVM versus Time (Option 21 only)	page 2-228
:DISPlay:FVTime	Frequency versus Time	page 2-230
:DISPlay:GENeral	General signal viewing	page 2-239
:DISPlay:GPRF	RF measurements	page 2-243
:DISPlay:IQVTime	RF I&Q versus Time	page 2-246
:DISPlay:MCPower	MCPR (Multiple Carrier Power Ratio)	page 2-255
:DISPlay:MERRor	Magnitude error versus Time (Option 21 only)	page 2-261
:DISPlay:OBWidth	OBW (Occupied Bandwidth)	page 2-263
:DISPlay:PERRor	Phase error versus Time (Option 21 only)	page 2-269
:DISPlay:PHVTime	Phase versus Time	page 2-271
:DISPlay:PULSe	Pulsed RF measurements (Option 20 only)	page 2-281
:DISPlay:SGRam	Spectrogram	page 2-310
:DISPlay:SPECTrum	Spectrum	page 2-314
:DISPlay:TOVerview	Time overview	page 2-317

NOTE. The :DISPlay commands concern the measurement display only, and do not affect analyzer hardware settings.

:DISPlay Basic Command Subgroup

The :DISPlay basic commands control the measurement window display.

Command Tree	Header	Parameter
	:DISPlay	
	:WINDow	
	:ACTive	
	:MEASurement?	
	:OPTimized	
	:MEASurement?	

:DISPlay:WINDow:ACTive:MEASurement? (Query Only)

Queries the active measurement views.

Syntax :DISPlay:WINDow:ACTive:MEASurement?

Arguments None

Returns <view1>,<view2>,...,<view(n)>
Where <view(n)>::=<string> is the view name as shown in Table 2-32.

Table 2-32: Measurement views

Return value	Measurement view	Display group
"SPEC"	Spectrum	General signal viewing
"DPSA"	DPX (Digital Phosphor) spectrum	
"MAGVT"	Amplitude versus Time	
"FVT"	Frequency versus Time	
"PHVT"	Phase versus Time	
"IQVT"	RF I&Q versus Time	
"SGRam"	Spectrogram	
"TOV"	Time overview	
"CONS"	Constellation	General purpose digital modulation
"EVM"	EVM versus Time	
"MERR"	Magnitude error versus Time	
"PERR"	Phase error versus Time	
"SIGN"	Signal quality	
"STAB"	Symbol table	
"CCDF"	CCDF	RF measurements
"ACP"	Channel power and ACPR	
"MCP"	MCPR (Multiple Carrier Power Ratio)	
"OBW"	Occupied bandwidth	
"STAT"	Pulse statistics	Pulsed RF
"RES"	Pulse table (results table)	
"TRAC"	Pulse trace	

Measurement Views All

Examples :DISPlay:WINDow:ACTive:MEASurement?
might return "SPEC", "TRAC" indicating that the views of spectrum and pulse trace are displayed on the screen.

:DISPlay:WINDow:OPTimized:MEASurement? (Query Only)

Queries the measurement views that are optimized. “Optimized” means that there is a perfect match between the view’s settings and the actual acquisition parameters to meet the specifications. When multiple measurements are running at one time, the measurements can have different requirements for setting the acquisition hardware. You can make a measurement optimized by selecting it using the following commands:

- :DISPlay:GENeral:MEASview:SElect for the general signal viewing
- :DISPlay:DDEMod:MEASview:SElect for the digital modulation views
- :DISPlay:GPRF:MEASview:SElect for the RF measurement views
- :DISPlay:PULSe:MEASview:SElect for the pulsed RF measurement views

Syntax :DISPlay:WINDow:OPTimized:MEASurement?

Arguments None

Returns <view1>,<view2>,...,<view(n)>
Where <view(n)>::=<string> is the view name as shown in Table 2-32.

Measurement Views All

Examples :DISPlay:WINDow:OPTimized:MEASurement?
might return "SPEC", "MCP" indicating that the views of spectrum and MCPR are optimized.

Related Commands :DISPlay:DDEMod:MEASview:SElect, :DISPlay:GENeral:MEASview:SElect,
:DISPlay:GPRF:MEASview:SElect, :DISPlay:PULSe:MEASview:SElect

:DISPlay:ACPower Subgroup

The :DISPlay:ACPower commands control the Channel power and ACPR (Adjacent Channel Power Ratio) view.

Command Tree	Header	Parameter
	:DISPlay	
	:ACPower	
	:MARKer	
	:SHOW	
	:STATe	<boolean>
	:PLEVel	
	:SHOW	
	:STATe	<boolean>
	:RESet	
	:SCALE	
	:WINDow	
	:TRACe	
	:GRATicule	
	:GRID	
	:STATe	<boolean>
	:X	
	[:SCALE]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>
	:Y	
	[:SCALE]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>

:DISPlay:ACPower:MARKer:SHOW:STATe(?)

Determines whether to show or hide the readout for the selected marker in the Channel power and ACPR view.

Syntax :DISPlay:ACPower:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }
:DISPlay:ACPower:MARKer:SHOW:STATe?

Arguments OFF or 0 hides the readout for the selected marker in the graph.
ON or 1 shows the readout for the selected marker in the graph.

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:MARKer:SHOW:STATe ON
shows the readout for the selected marker in the graph.

:DISPlay:ACPower:PLEVel:SHOW:STATe(?)

Determines whether to show or hide the power levels in the Channel power and ACPR view.

Syntax :DISPlay:ACPower:PLEVel:SHOW:STATe { OFF | ON | 0 | 1 }
:DISPlay:ACPower:PLEVel:SHOW:STATe?

Arguments OFF or 0 hides the power levels in the graph.
ON or 1 shows the power levels in the graph.

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:PLEVel:SHOW:STATe ON
shows the power levels in the graph.

:DISPlay:ACPower:RESet:SCALE (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the Channel power and ACPR view.

Vertical offset = Reference level
Vertical scale = 100 dB
Horizontal offset = Center frequency
Horizontal scale = Default span

Syntax :DISPlay:ACPower:RESet:SCALE

Arguments None

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:RESet:SCALE
resets the horizontal and vertical scale to the default values.

:DISPlay:ACPower:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:ACPower:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }
 :DISPlay:ACPower:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:WINDow:TRACe:GRATicule:GRID:STATe ON
shows the graticule grid on the screen.

:DISPlay:ACPower:X[:SCALe](?)

Sets or queries the horizontal range of the Channel power and ACPR graph.

Syntax :DISPlay:ACPower:X[:SCALe] <value>
 :DISPlay:ACPower:X[:SCALe]?

Arguments <value>::=<NRf> specifies the horizontal range.
 Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:X:SCALe 10MHz
 sets the horizontal range to 10 MHz.

Related Commands :DISPlay:ACPower:X[:SCALe]:OFFSet

:DISPlay:ACPower:X[:SCALe]:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the Channel power and ACPR view.

Syntax :DISPlay:ACPower:X[:SCALe]:AUTO

Arguments None

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:X:SCALe:AUTO
 rescales the horizontal scale automatically to fit the waveform to the screen.

:DISPlay:ACPower:X[:SCALE]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) of the Channel power and ACPR graph.

Syntax :DISPlay:ACPower:X[:SCALE]:OFFSet <value>
 :DISPlay:ACPower:X[:SCALE]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum horizontal value.
 Range: [(center frequency) - (X scale) × 0.9] to
 [(center frequency) + (X scale) × 0.9]

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:X:SCALE:OFFSet 1.45GHz
 sets the minimum horizontal value to 1.45 GHz in the Channel power and ACPR graph.

Related Commands :DISPlay:ACPower:X[:SCALE]

:DISPlay:ACPower:Y[:SCALE](?)

Sets or queries the vertical range of the channel power and ACPR graph.

Syntax :DISPlay:ACPower:Y[:SCALE] <value>
 :DISPlay:ACPower:Y[:SCALE]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 0.1 to 200 dB.

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:Y:SCALE 100
 sets the vertical range to 100 dB in the Channel power and ACPR graph.

Related Commands :DISPlay:ACPower:Y[:SCALE]:OFFSet

:DISPlay:ACPower:Y[:SCALE]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the Channel power and ACPR view.

Syntax :DISPlay:ACPower:Y[:SCALE]:AUTO

Arguments None

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:Y:SCALE:AUTO
rescales the vertical scale automatically to fit the waveform to the screen.

:DISPlay:ACPower:Y[:SCALE]:OFFSet(?)

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the Channel power and ACPR graph.

Syntax :DISPlay:ACPower:Y[:SCALE]:OFFSet <value>
:DISPlay:ACPower:Y[:SCALE]:OFFSet?

Arguments <value>::=<NRf> specifies the vertical offset.
Range: -170 to +50 dBm.

Measurement Views Channel power and ACPR

Examples :DISPlay:ACPower:Y:SCALE:OFFSet -12.5
sets the vertical offset to -12.5 dBm in the Channel power and ACPR graph.

Related Commands :DISPlay:ACPower:Y[:SCALE]

:DISPlay:AVTime Subgroup

The :DISPlay:AVTime commands control the Amplitude versus Time view.

Command Tree	Header	Parameter
	:DISPlay	
	:AVTime	
	:MARKer	
	:SHOW	
	:STATE	<boolean>
	:RESet	
	:TRIGger	
	:LEVel	
	:STATE	<boolean>
	:WINDow	
	:TRACe	
	:GRATicule	
	:GRID	
	:STATE	<boolean>
	:X	
	:RSCale	
	[:SCALe]	
	:AUTO	
	:STATE	<boolean>
	:FULL	<numeric_value>
	:MAXimum?	
	:MINimum?	
	:OFFSet	<numeric_value>
	:MAXimum?	
	:MINimum?	
	:Y	
	:RSCale	
	[:SCALe]	
	:FULL	<numeric_value>
	:OFFSet	<numeric_value>

:DISPlay:AVTime:MARKer:SHOW:STATe(?)

Determines whether to show or hide the readout for the selected marker on the screen in the Amplitude versus Time measurement.

Syntax :DISPlay:AVTime:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }
:DISPlay:AVTime:MARKer:SHOW:STATe?

Arguments OFF or 0 hides the readout for the selected marker on screen.
ON or 1 shows the readout for the selected marker on screen.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:MARKer:SHOW:STATe ON
shows the readout for the selected marker on screen.

:DISPlay:AVTime:RESet (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the Amplitude versus Time view.

Vertical offset = Reference level
Vertical scale = 100 dB
Horizontal offset = Analysis offset
Horizontal scale = Analysis length

Syntax :DISPlay:AVTime:RESet

Arguments None

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:RESet
resets the horizontal and vertical scale to the default values.

:DISPlay:AVTime:TRIGger:LEVel:STATe(?)

Determines whether to show or hide the power trigger level line on the screen in the Amplitude versus Time measurement.

Syntax :DISPlay:AVTime:TRIGger:LEVel:STATe { OFF | ON | 0 | 1 }
 :DISPlay:AVTime:TRIGger:LEVel:STATe?

Arguments OFF or 0 hides the power trigger level line.
 ON or 1 shows the power trigger level line.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:TRIGger:LEVel:STATe ON
 shows the power trigger level line on the screen.

:DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }
 :DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe ON
 shows the graticule grid on the screen in the Amplitude versus Time view.

:DISPlay:AVTime:X:RSCale (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the Amplitude versus Time display.

Syntax :DISPlay:AVTime:X:RSCale

Arguments None

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:RSCale
rescales the horizontal scale automatically to fit the waveform to the screen.

:DISPlay:AVTime:X[:SCALe]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the Amplitude versus Time view. Executing this command sets :DISPlay:AVTime:X[:SCALe]:AUTO:STATe ON.

Syntax :DISPlay:AVTime:X[:SCALe]:AUTO

Arguments None

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:SCALe:AUTO
sets the horizontal scale automatically to fit the waveform to the screen.

Related Commands :DISPlay:AVTime:X[:SCALe]:AUTO:STATe

:DISPlay:AVTime:X[:SCALe]:AUTO:STATe(?)

Determines whether to set the horizontal scale automatically or manually.

Syntax :DISPlay:AVTime:X[:SCALe]:AUTO:STATe { OFF | ON | 0 | 1 }
:DISPlay:AVTime:X[:SCALe]:AUTO:STATe?

Arguments OFF or 0 specifies that the horizontal scale is set manually. To set it, use the :DISPlay:AVTime:X[:SCALe]:FULL and :DISPlay:AVTime:X[:SCALe]:OFFSet commands.

ON or 1 specifies that the horizontal scale is set automatically.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:SCALe:AUTO:STATe ON
specifies that the horizontal scale is set automatically.

Related Commands :DISPlay:AVTime:X[:SCALe]:FULL, :DISPlay:AVTime:X[:SCALe]:OFFSet

:DISPlay:AVTime:X[:SCALe]:FULL(?)

Sets or queries the horizontal scale (full-scale time) of the Amplitude versus Time graph. Programming a specified scale sets :DISPlay:AVTime:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:AVTime:X[:SCALe]:FULL <value>
 :DISPlay:AVTime:X[:SCALe]:FULL?

Arguments <value>::=<NRf> specifies the horizontal scale in full-scale time. Use the :DISPlay:AVTime:X[:SCALe]:MAXimum[:MINimum]? query to get the upper and lower limits of the setting range.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:SCALe:FULL 25.6us
 sets the horizontal scale to 25.6 μ s.

Related Commands :DISPlay:AVTime:X[:SCALe]:AUTO:STATe
 :DISPlay:AVTime:X[:SCALe]:OFFSet
 :DISPlay:AVTime:X[:SCALe]:MAXimum[:MINimum]

:DISPlay:AVTime:X[:SCALe]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Syntax :DISPlay:AVTime:X[:SCALe]:MAXimum?

Returns <NRf> The upper limit of the horizontal scale setting range.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:SCALe:MAXimum?
might return 18.135E-3, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

Related Commands :DISPlay:AVTime:X[:SCALe]:FULL

:DISPlay:AVTime:X[:SCALe]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Syntax :DISPlay:AVTime:X[:SCALe]:MINimum?

Returns <NRf> The lower limit of the horizontal scale setting range.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:SCALe:MINimum?
might return 10.0E-9, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

Related Commands :DISPlay:AVTime:X[:SCALe]:FULL

:DISPlay:AVTime:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) of the Amplitude versus Time graph. Programming a specified offset sets :DISPlay:AVTime:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:AVTime:X[:SCALe]:OFFSet <value>
 :DISPlay:AVTime:X[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum horizontal value.
 Use the :DISPlay:AVTime:X[:SCALe]:OFFSet:MAXimum|:MINimum? query to get the upper and lower limits of the setting range.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:SCALe:OFFSet 800ns
 sets the minimum horizontal value to 800 ns in the Amplitude versus Time graph.

Related Commands :DISPlay:AVTime:X[:SCALe]:AUTO:STATe
 :DISPlay:AVTime:X[:SCALe]:FULL
 :DISPlay:AVTime:X[:SCALe]:OFFSet:MAXimum|:MINimum?

:DISPlay:AVTime:X[:SCALE]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Syntax :DISPlay:AVTime:X[:SCALE]:OFFSet:MAXimum?

Returns <Nrf> The upper limit of the horizontal offset setting range.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:SCALE:OFFSet:MAXimum?
might return $-1.812\text{E}-3$, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

Related Commands :DISPlay:AVTime:X[:SCALE]:OFFSet

:DISPlay:AVTime:X[:SCALE]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Syntax :DISPlay:AVTime:X[:SCALE]:OFFSet:MINimum?

Returns <Nrf> The lower limit of the horizontal offset setting range.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:X:SCALE:OFFSet:MINimum?
might return $-16.28\text{E}-3$, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

Related Commands :DISPlay:AVTime:X[:SCALE]:OFFSet

:DISPlay:AVTime:Y:RSCale (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the Amplitude versus Time display.

Syntax :DISPlay:AVTime:Y:RSCale

Arguments None

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:Y:RSCale
rescales the vertical scale automatically to fit the waveform to the screen.

:DISPlay:AVTime:Y[:SCALe]:FULL(?)

Sets or queries the vertical range of the Amplitude versus Time graph.

Syntax :DISPlay:AVTime:Y[:SCALe]:FULL <value>
 :DISPlay:AVTime:Y[:SCALe]:FULL?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 0.1 to 200 dB.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:Y:SCALe:FULL 100
 sets the vertical range to 100 dB in the Amplitude versus Time graph.

Related Commands :DISPlay:AVTime:Y[:SCALe]:OFFSet

:DISPlay:AVTime:Y[:SCALe]:OFFSet(?)

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the Amplitude versus Time graph.

Syntax :DISPlay:AVTime:Y[:SCALe]:OFFSet <value>
 :DISPlay:AVTime:Y[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the vertical offset.
 Range: -170 to +50 dBm.

Measurement Views Amplitude versus Time

Examples :DISPlay:AVTime:Y:SCALe:OFFSet -12.5
 sets the vertical offset to -12.5 dBm in the Amplitude versus Time graph.

Related Commands :DISPlay:AVTime:Y[:SCALe]:FULL

:DISPlay:CONSte Subgroup

The :DISPlay:CONSte commands control the constellation display.

Command Tree	Header	Parameter
	:DISPlay	
	:CONSte	
	:WINDow	
	:TRACe	
	:GRATicule	
	:GRID	
	:STATe	<boolean>

:DISPlay:CONSte:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax	:DISPlay:CONSte:WINDow:TRACe:GRATicule:GRID:STATe { OFF ON 0 1 } :DISPlay:CONSte:WINDow:TRACe:GRATicule:GRID:STATe?
---------------	---

Arguments	OFF or 0 hides the graticule grid. ON or 1 shows the graticule grid.
------------------	---

Measurement Views	Constellation
--------------------------	---------------

Examples	:DISPlay:CONSte:WINDow:TRACe:GRATicule:GRID:STATe ON shows the graticule grid on the screen.
-----------------	---

:DISPlay:DDEMod Subgroup (Option 21 Only)

The :DISPlay:DDEMod commands control display in the General Purpose Digital Modulation measurements.

Command Tree	Header	Parameter
	:DISPlay	
	:DDEMod	
	:MEASview	
	:DELeTe	CONStE EVM MERRor PERRor SIGNa1qua1 STABle
	:NEW	CONStE EVM MERRor PERRor SIGNa1qua1 STABle
	:SELeCt	CONStE EVM MERRor PERRor SIGNa1qua1 STABle
	:RADix	BINary HEXadecimal
	:X	
	[:SCALE]	<numeric_value>
	:AUTO	
	:SCALE	<boolean>
	:MAXimum?	
	:MINimum?	
	:OFFSet	<numeric_value>
	:MAXimum?	
	:MINimum?	
	:RESet	

:DISPlay:DDMod:MEASview:DELeTe (No Query Form)

Deletes the measurement view in the general purpose digital modulation measurements.

Syntax :DISPlay:DDMod:MEASview:DELeTe { CONSTe | EVM | MERRor
 | PERRor | SIGNalqual | STABLe }

Arguments Table 2-33 lists the arguments. The arguments are the string type.

Table 2-33: Modulation measurement views

Argument	View
CONSTe	Constellation
EVM	EVM (Error Vector Magnitude) versus Time
MERRor	Magnitude error versus Time
PERRor	Phase error versus Time
SIGNalqual	Signal quality
STABLe	Symbol table

If you attempt to delete a view that is not displayed on screen, the error (-200, “Execution error; Measurement not running”) will be returned.

Measurement Views General purpose digital modulation

Examples :DISPlay:DDMod:MEASview:DELeTe CONSTe
 deletes the constellation view.

:DISPlay:DDEMod:MEASview:NEW (No Query Form)

Displays a new measurement view in the general purpose digital modulation measurements.

Syntax :DISPlay:DDEMod:MEASview:NEW { CONSTe | EVM | MERRor
| PERRor | SIGNalqual | STABLe }

Arguments Refer to Table 2-33 on page 2-218.

Measurement Views General purpose digital modulation

If you attempt to open a view that is currently displayed on screen, the error (-200, "Execution error; Measurement is already running") will be returned.

Examples :DISPlay:DDEMod:MEASview:NEW CONSTe
creates the constellation view.

:DISPlay:DDEMod:MEASview:SELEct(?)

Selects a measurement view in the general purpose digital modulation measurements on the screen. The query command returns the currently selected view.

Selecting a measurement optimizes it. Other measurements may be optimized as a side effect. Refer to the :DISPlay:WINDow:OPTimized:MEASurement? query.

Syntax :DISPlay:DDEMod:MEASview:SELEct { CONSTe | EVM | MERRor
| PERRor | SIGNalqual | STABLe }

Arguments Refer to Table 2-33 on page 2-218.

If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Measurement Views General purpose digital modulation

Examples :DISPlay:DDEMod:MEASview:SELEct CONSTe
selects the constellation view.

Related Commands :DISPlay:WINDow:OPTimized:MEASurement?

:DISPlay:DDEMod:RADix(?)

Selects or queries the base of symbols.
This command is effective in the symbol table.

Syntax :DISPlay:DDEMod:RADix { BINary | HEXadecimal }
 :DISPlay:DDEMod:RADix?

Arguments BINary selects binary notation.
 HEXadecimal selects hexadecimal notation.

Measurement Views Symbol table

Examples :DISPlay:DDEMod:RADix BINary
 selects binary notation for the symbol table.

:DISPlay:DDEMod:X[:SCALe](?)

Sets or queries the horizontal scale (full-scale time) for the time measurements in the general purpose digital modulation analysis. Programming a specified scale sets :DISPlay:DDEMod:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:DDEMod:X[:SCALe] <value>
 :DISPlay:DDEMod:X[:SCALe]?

Arguments <value>::=<NRf> specifies the horizontal scale in full-scale time.
 Use the :DISPlay:DDEMod:X[:SCALe]:MAXimum[:MINimum]? query to get the upper and lower limits of the setting range.

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALe 1.5us
 sets the horizontal scale to 1.5 μ s.

Related Commands :DISPlay:DDEMod:X[:SCALe]:AUTO:STATe
 :DISPlay:DDEMod:X[:SCALe]:OFFSet,
 :DISPlay:DDEMod:X[:SCALe]:MAXimum[:MINimum]

:DISPlay:DDEMod:X[:SCALe]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the general purpose digital modulation analysis. Executing this command sets :DISPlay:DDEMod:X[:SCALe]:AUTO:STATe ON.

Syntax :DISPlay:DDEMod:X[:SCALe]:AUTO

Arguments None

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALe:AUTO
sets the horizontal scale automatically to fit the waveform to the screen.

Related Commands :DISPlay:DDEMod:X[:SCALe]:AUTO:STATe

:DISPlay:DDEMod:X[:SCALe]:AUTO:STATe(?)

Determines whether to set the horizontal scale automatically or manually.

Syntax :DISPlay:DDEMod:X[:SCALe]:AUTO:STATe { OFF | ON | 0 | 1 }
:DISPlay:DDEMod:X[:SCALe]:AUTO:STATe?

Arguments OFF or 0 specifies that the horizontal scale is set manually. To set it, use the :DISPlay:DDEMod:X[:SCALe] and :DISPlay:DDEMod:X[:SCALe]:OFFSet commands.

ON or 1 specifies that the horizontal scale is set automatically.

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALe:AUTO:STATe ON
specifies that the horizontal scale is set automatically.

Related Commands :DISPlay:DDEMod:X[:SCALe], :DISPlay:DDEMod:X[:SCALe]:OFFSet

:DISPlay:DDEMod:X[:SCALe]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Syntax :DISPlay:DDEMod:X[:SCALe]:MAXimum?

Returns <NRf> The upper limit of the horizontal scale setting range.

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALe:MAXimum?
might return 18.135E-3, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

Related Commands :DISPlay:DDEMod:X[:SCALe]

:DISPlay:DDEMod:X[:SCALe]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Syntax :DISPlay:DDEMod:X[:SCALe]:MINimum?

Returns <NRf> The lower limit of the horizontal scale setting range.

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALe:MINimum?
might return 10.0E-9, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

Related Commands :DISPlay:DDEMod:X[:SCALe]

:DISPlay:DDEMod:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) for the time measurements in the general purpose digital modulation analysis. Programming a specified offset sets :DISPlay:DDEMod:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:DDEMod:X[:SCALe]:OFFSet <value>
 :DISPlay:DDEMod:X[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum horizontal value.
 Use the :DISPlay:DDEMod:X[:SCALe]:OFFSet:MAXimum|:MINimum? query to get the upper and lower limits of the setting range.

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALe:OFFSet 20.075us
 sets the minimum horizontal value to 20.075 μ s.

Related Commands :DISPlay:DDEMod:X[:SCALe]:AUTO:STATe
 :DISPlay:DDEMod:X[:SCALe]
 :DISPlay:DDEMod:X[:SCALe]:OFFSet:MAXimum|:MINimum?

:DISPlay:DDEMod:X[:SCALe]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Syntax :DISPlay:DDEMod:X[:SCALe]:OFFSet:MAXimum?

Returns <NRf> The upper limit of the horizontal offset setting range.

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALe:OFFSet:MAXimum?
might return $-1.812\text{E}-3$, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

Related Commands :DISPlay:DDEMod:X[:SCALe]:OFFSet

:DISPlay:DDEMod:X[:SCALe]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Syntax :DISPlay:DDEMod:X[:SCALe]:OFFSet:MINimum?

Returns <NRf> The lower limit of the horizontal offset setting range.

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALe:OFFSet:MINimum?
might return $-16.28\text{E}-3$, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

Related Commands :DISPlay:DDEMod:X[:SCALe]:OFFSet

:DISPlay:DDEMod:X[:SCALE]:RESet (No Query Form)

Presets the horizontal scale to the default value for the time measurements in the general purpose digital modulation analysis.

Syntax :DISPlay:DDEMod:X[:SCALE]:RESet

Arguments None

Measurement Views EVM versus Time, Magnitude error versus Time, Phase error versus Time

Examples :DISPlay:DDEMod:X:SCALE:RESet
presets the horizontal scale to the default value.

:DISPlay:DPSA Subgroup

The :DISPlay:DPSA commands control the DPX (Digital Phosphor) spectrum view.

Command Tree	Header	Parameter
	:DISPlay	
	:DPSA	
	:WINDow	
	:TRACe	
	:GRATICule	
	:GRID	
	:STATe	<boolean>
	:Y	
	[:SCALe]	
	:PDIVision	<numeric_value>

:DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:STATe
 { OFF | ON | 0 | 1 }

 :DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views DPX spectrum

Examples :DISPlay:DPSA:WINDow:TRACe:GRATICule:GRID:STATe ON
 shows the graticule grid on the screen in the DPX spectrum view.

:DISPlay:DPSA:Y[:SCALe]:PDIVision(?)

Sets or queries the vertical scale (per division) in the DPX spectrum view.

Syntax :DISPlay:DPSA:Y[:SCALe]:PDIVision <value>
 :DISPlay:DPSA:Y[:SCALe]:PDIVision?

Arguments <value>::=<NRf> specifies the vertical scale (per division).
 Range: 2 to 20 dB/div.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:Y:SCALe:PDIVision 0.5
 sets the vertical scale to 0.5 dB/div.

Related Commands [:SENSe]:POWeR:UNITs

:DISPlay:EVM Subgroup (Option 21 Only)

The :DISPlay:EVM commands control the EVM (Error Vector Magnitude) versus Time view.

Command Tree	Header	Parameter
	:DISPlay	
	:EVM	
	:Y	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>

:DISPlay:EVM:Y[:SCALe](?)

Sets or queries the vertical range of the EVM versus Time graph.

Syntax :DISPlay:EVM:Y[:SCALe] <value>
 :DISPlay:EVM:Y[:SCALe]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 1 to 100%.

Measurement Views EVM versus Time

Examples :DISPlay:EVM:Y:SCALe 50
 sets the vertical range to 50% in the EVM versus Time graph.

Related Commands :DISPlay:EVM:Y[:SCALe]:OFFSet

:DISPlay:EVM:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the EVM versus Time display.

Syntax :DISPlay:EVM:Y[:SCALe]:AUTO

Arguments None

Measurement Views EVM versus Time

Examples :DISPlay:EVM:Y:SCALe:AUTO
sets the vertical scale automatically to fit the waveform to the screen.

:DISPlay:EVM:Y[:SCALe]:OFFSet(?)

Sets or queries the minimum vertical value (bottom edge) of the EVM versus Time graph.

Syntax :DISPlay:EVM:Y[:SCALe]:OFFSet <value>
:DISPlay:EVM:Y[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum vertical value.
Range: -100 to 100%.

Measurement Views EVM versus Time

Examples :DISPlay:EVM:Y:SCALe:OFFSet -9.5
sets the minimum vertical value to -9.5% in the EVM versus Time graph.

Related Commands :DISPlay:EVM:Y[:SCALe]

:DISPlay:FVTime Subgroup

The :DISPlay:FVTime commands control the Frequency versus Time view.

Command Tree	Header	Parameter
	:DISPlay	
	:FVTime	
	:WINDow	
	:TRACe	
	:GRATICule	
	:GRID	
	:STATe	<boolean>
	:X	
	[:SCALe]	<numeric_value>
	:AUTO	
	:STATe	<boolean>
	:MAXimum?	
	:MINimum?	
	:OFFSet	<numeric_value>
	:MAXimum?	
	:MINimum?	
	:Y	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>

:DISPlay:FVTime:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:FVTime:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }

 :DISPlay:FVTime:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:WINDow:TRACe:GRATicule:GRID:STATe ON
 shows the graticule grid on the Frequency versus Time view.

:DISPlay:FVTime:X[:SCALe](?)

Sets or queries the horizontal scale (full-scale time) of the Frequency versus Time graph. Programming a specified scale sets :DISPlay:FVTime:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:FVTime:X[:SCALe] <value>
 :DISPlay:FVTime:X[:SCALe]?

Arguments <value>::={ <NRf> | MAXimum | MINimum } specifies the horizontal scale in full-scale time. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively.

Use the :DISPlay:FVTime:X[:SCALe]:MAXimum|:MINimum? query to get the upper and lower limit values of the setting range.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:X:SCALe 25.6us
 sets the horizontal scale to 25.6 μ s.

Related Commands :DISPlay:FVTime:X[:SCALe]:AUTO:STATe
 :DISPlay:FVTime:X[:SCALe]:OFFSet
 :DISPlay:FVTime:X[:SCALe]:MAXimum|:MINimum

:DISPlay:FVTime:X[:SCALE]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the Frequency versus Time view. Executing this command sets :DISPlay:FVTime:X[:SCALE]:AUTO:STATe ON.

Syntax :DISPlay:FVTime:X[:SCALE]:AUTO

Arguments None

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:X:SCALE:AUTO
sets the horizontal scale automatically to fit the waveform to the screen.

Related Commands :DISPlay:FVTime:X[:SCALE]:AUTO:STATe

:DISPlay:FVTime:X[:SCALE]:AUTO:STATe(?)

Determines whether to set the horizontal scale automatically or manually.

Syntax :DISPlay:FVTime:X[:SCALE]:AUTO:STATe { OFF | ON | 0 | 1 }
:DISPlay:FVTime:X[:SCALE]:AUTO:STATe?

Arguments OFF or 0 specifies that the horizontal scale is set manually. To set it, use the :DISPlay:FVTime:X[:SCALE] and :DISPlay:FVTime:X[:SCALE]:OFFSet commands.

ON or 1 specifies that the horizontal scale is set automatically.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:X:SCALE:AUTO:STATe ON
specifies that the horizontal scale is set automatically.

Related Commands :DISPlay:FVTime:X[:SCALE], :DISPlay:FVTime:X[:SCALE]:OFFSet

:DISPlay:FVTime:X[:SCALE]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Syntax :DISPlay:FVTime:X[:SCALE]:MAXimum?

Returns <NRf> The upper limit of the horizontal scale setting range.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:X:SCALE:MAXimum?
might return 18.135E-3, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

Related Commands :DISPlay:FVTime:X[:SCALE]

:DISPlay:FVTime:X[:SCALE]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Syntax :DISPlay:FVTime:X[:SCALE]:MINimum?

Returns <NRf> The lower limit of the horizontal scale setting range.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:X:SCALE:MINimum?
might return 10.0E-9, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

Related Commands :DISPlay:FVTime:X[:SCALE]

:DISPlay:FVTime:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) of the Frequency versus Time graph. Programming a specified offset sets :DISPlay:FVTime:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:FVTime:X[:SCALe]:OFFSet <value>
:DISPlay:FVTime:X[:SCALe]:OFFSet?

Arguments <value>::={ <NRf> | MAXimum | MINimum } specifies the horizontal offset. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively.

Use the :DISPlay:FVTime:X[:SCALe]:OFFSet:MAXimum|:MINimum? query to get the upper and lower limit values of the setting range.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:X:SCALe:OFFSet 800ns
sets the minimum horizontal value to 800 ns in the Frequency versus Time graph.

Related Commands :DISPlay:FVTime:X[:SCALe]:AUTO:STATe
:DISPlay:FVTime:X[:SCALe]
:DISPlay:FVTime:X[:SCALe]:OFFSet:MAXimum|:MINimum?

:DISPlay:FVTime:X[:SCALE]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Syntax :DISPlay:FVTime:X[:SCALE]:OFFSet:MAXimum?

Returns <NRf> The upper limit of the horizontal offset setting range.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:X:SCALE:OFFSet:MAXimum?
might return $-1.812\text{E}-3$, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

Related Commands :DISPlay:FVTime:X[:SCALE]:OFFSet

:DISPlay:FVTime:X[:SCALE]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Syntax :DISPlay:FVTime:X[:SCALE]:OFFSet:MINimum?

Returns <NRf> The lower limit of the horizontal offset setting range.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:X:SCALE:OFFSet:MINimum?
might return $-16.28\text{E}-3$, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

Related Commands :DISPlay:FVTime:X[:SCALE]:OFFSet

:DISPlay:FVTime:Y[:SCALe](?)

Sets or queries the vertical range of the Frequency versus Time graph.

Syntax :DISPlay:FVTime:Y[:SCALe] <value>
 :DISPlay:FVTime:Y[:SCALe]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 10 Hz to 120 MHz.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:Y:SCALe 30MHz
 sets the vertical range to 30 MHz in the Frequency versus Time graph.

Related Commands :DISPlay:FVTime:Y[:SCALe]:OFFSet

:DISPlay:FVTime:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Frequency versus Time view.

Syntax :DISPlay:FVTime:Y[:SCALe]:AUTO

Arguments None

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:Y:SCALe:AUTO
 sets the vertical scale automatically to fit the waveform to the screen.

:DISPlay:FVTime:Y[:SCALE]:OFFSet(?)

Sets or queries the vertical offset (the value at the center of the vertical axis) in the Frequency versus Time graph.

Syntax :DISPlay:FVTime:Y[:SCALE]:OFFSet <value>
 :DISPlay:FVTime:Y[:SCALE]:OFFSet?

Arguments <value>::=<NRf> specifies the vertical offset.
 Range: -60 MHz to +60 MHz.

Measurement Views Frequency versus Time

Examples :DISPlay:FVTime:Y:SCALE:OFFSet -14.5MHz
 sets the vertical offset to -14.5 MHz in the Frequency versus Time graph.

Related Commands :DISPlay:FVTime:Y[:SCALE]

:DISPlay:GENeral Subgroup

The :DISPlay:GENeral commands control display in the general signal viewing.

Command Tree	Header	Parameter
	:DISPlay	
	:GENeral	
	:MEASview	
	:DELeTe	SPECTrum DPSA AVTime FVTime PHVTime IQVTime SGRam TOVerview
	:NEW	SPECTrum DPSA AVTime FVTime PHVTime IQVTime SGRam TOVerview
	:SELeCt	SPECTrum DPSA AVTime FVTime PHVTime IQVTime SGRam TOVerview

:DISPlay:GENeral:MEASview:DELeTe (No Query Form)

Deletes a measurement view in the general signal viewing.

Syntax :DISPlay:GENeral:MEASview:DELeTe { SPECTrum | DPSA | AVTime
 | FVTime | PHVTime | IQVTime | SGRam | TOVerview }

Arguments Table 2-34 shows the arguments. The arguments are the string type.

Table 2-34: General signal viewing views

Argument	View
SPECTrum	Spectrum
DPSA	DPX (Digital Phosphor) spectrum
AVTime	Amplitude versus Time
FVTime	Frequency versus Time
PHVTime	Phase versus Time
IQVTime	IQ versus Time
SGRam	Spectrogram
TOVerview	Time overview

If you attempt to delete a view that is not displayed on screen, the error (-200, “Execution error; Measurement not running”) will be returned.

Measurement Views General signal viewing

Examples :DISPlay:GENeral:MEASview:DELeTe DPSA
 deletes the DPX spectrum view.

:DISPlay:GENeral:MEASview:NEW (No Query Form)

Displays a new measurement view in the general signal viewing.

Syntax :DISPlay:GENeral:MEASview:NEW { SPECTrum | DPSA | AVTime
 | FVTime | PHVTime | IQVTime | SGRam | TOVerview }

Arguments Refer to Table 2-34 on page 2-240.

If you attempt to open a view that is currently displayed on screen, the error (-200, “Execution error; Measurement is already running”) will be returned.

Measurement Views General signal viewing

Examples :DISPlay:GENeral:MEASview:NEW DPSA
 creates the DPX spectrum view.

:DISPlay:GENeral:MEASview:SElect(?)

Selects a measurement view in the general signal viewing on the screen.

The query command returns the currently selected view.

Selecting a measurement optimizes it. Other measurements may be optimized as a side effect. Refer to the :DISPlay:WINDow:OPTimized:MEASurement? query.

Syntax :DISPlay:GENeral:MEASview:SElect { SPECTrum | DPStA | AVTime
 | FVTime | PHVTime | IQVTime | SGRam | TOVerview }

Arguments Refer to Table 2-34 on page 2-240.

If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

The time overview (TOVerview) cannot be selected as the primary measurement. If you select it, the error (-200, "Execution error; Time Overview cannot be Primary measurement") will be returned. If you use the :DISPlay:GENeral:MEASview:SElect? query with the time overview as the only measurement active, the error (-200, "Execution error; Analysis selected is not running") will be returned.

Measurement Views General signal viewing

Examples :DISPlay:GENeral:MEASview:SElect DPStA
 selects the DPX spectrum view.

Related Commands :DISPlay:WINDow:OPTimized:MEASurement?

:DISPlay:GPRF Subgroup

The :DISPlay:GPRF commands control display for the RF measurements.

Command Tree	Header	Parameter
	:DISPlay	
	:GPRF	
	:MEASview	
	:DELeTe	CCDF ACPower MCPower OBW
	:NEW	CCDF ACPower MCPower OBW
	:SELeT	CCDF ACPower MCPower OBW

:DISPlay:GPRF:MEASview:DELeTe (No Query Form)

Deletes a selected measurement view in the RF measurements.

Syntax :DISPlay:GPRF:MEASview:DELeTe { CCDF | ACPower | MCPower | OBW }

Arguments CCDF deletes the CCDF view.
 ACPower deletes the Channel power and ACPR view.
 MCPower deletes the MCPR view.
 OBW deletes the Occupied Bandwidth view.
 If you attempt to delete a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Measurement Views RF measurements

Examples :DISPlay:GPRF:MEASview:DELeTe ACPower
 deletes the Channel power and ACPR view.

:DISPlay:GPRF:MEASview:NEW (No Query Form)

Displays a new measurement view in the RF measurements.

Syntax :DISPlay:GPRF:MEASview:NEW { CCDF | ACPower | MCPower | OBW }

Arguments CCDF opens the CCDF view.

ACPower opens the Channel power and ACPR view.

MCPower opens the MCPR view.

OBW opens the Occupied Bandwidth view.

If you attempt to open a view that is currently displayed on screen, the error (-200, "Execution error; Measurement is already running") will be returned.

Measurement Views RF measurements

Examples :DISPlay:GPRF:MEASview:NEW ACPower
creates the Channel power and ACPR view.

:DISPlay:GPRF:MEASview:SElect(?)

Selects a measurement view in the RF measurements on the screen.

The query command returns the currently selected view.

Selecting a measurement optimizes it. Other measurements may be optimized as a side effect. Refer to the :DISPlay:WINDow:OPTimized:MEASurement? query.

Syntax :DISPlay:GPRF:MEASview:SElect { CCDF | ACPower | MCPower | OBW }
 :DISPlay:GPRF:MEASview:SElect?

Arguments CCDF selects the CCDF view.

 ACPower selects the Channel power and ACPR view.

 MCPower selects the MCPR view.

 OBW selects the Occupied Bandwidth view.

 If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Measurement Views RF measurements

Examples :DISPlay:GPRF:MEASview:SElect ACPower
 selects the Channel power and ACPR view.

Related Commands :DISPlay:WINDow:OPTimized:MEASurement?

:DISPlay:IQVTime Subgroup

The :DISPlay:IQVTime commands control the RF I&Q versus Time view.

Command Tree	Header	Parameter
	:DISPlay	
	:IQVTime	
	:WINDow	
	:TRACe	
	:GRATICule	
	:GRID	
	:STATe	<boolean>
	:X	
	[:SCALe]	<numeric_value>
	:AUTO	
	:STATe	<boolean>
	:MAXimum?	
	:MINimum?	
	:OFFSet	<numeric_value>
	:MAXimum?	
	:MINimum?	
	:Y	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>
	:RESCale	

:DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }
 :DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATe ON
 shows the graticule grid on the RF I&Q versus Time view.

:DISPlay:IQVTime:X[:SCALe](?)

Sets or queries the horizontal scale (full-scale time) of the RF I&Q versus Time graph. Programming a specified scale sets :DISPlay:IQVTime:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:IQVTime:X[:SCALe] <value>
 :DISPlay:IQVTime:X[:SCALe]?

Arguments <value>::={ <NRf> | MAXimum | MINimum } specifies the horizontal scale in full-scale time. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively.

Use the :DISPlay:IQVTime:X[:SCALe]:MAXimum|:MINimum? query to get the upper and lower limit values of the setting range.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:X:SCALe 100us
 sets the horizontal scale to 100 μ s.

Related Commands :DISPlay:IQVTime:X[:SCALe]:AUTO:STATe
 :DISPlay:IQVTime:X[:SCALe]:OFFSet
 :DISPlay:IQVTime:X[:SCALe]:MAXimum|:MINimum

:DISPlay:IQVTime:X[:SCALe]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the RF I&Q versus Time view. Executing this command sets :DISPlay:IQVTime:X[:SCALe]:AUTO:STATe ON.

Syntax :DISPlay:IQVTime:X[:SCALe]:AUTO

Arguments None

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:X:SCALe:AUTO
sets the horizontal scale automatically to fit the waveform to the screen.

Related Commands :DISPlay:IQVTime:X[:SCALe],:AUTO:STATe

:DISPlay:IQVTime:X[:SCALe]:AUTO:STATe(?)

Determines whether to set the horizontal scale automatically or manually.

Syntax :DISPlay:IQVTime:X[:SCALe]:AUTO:STATe { OFF | ON | 0 | 1 }
:DISPlay:IQVTime:X[:SCALe]:AUTO:STATe?

Arguments OFF or 0 specifies that the horizontal scale is set manually. To set it, use the :DISPlay:IQVTime:X[:SCALe] and :DISPlay:IQVTime:X[:SCALe]:OFFSet commands.

ON or 1 specifies that the horizontal scale is set automatically.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:X:SCALe:AUTO:STATe ON
specifies that the horizontal scale is set automatically.

Related Commands :DISPlay:IQVTime:X[:SCALe], :DISPlay:IQVTime:X[:SCALe]:OFFSet

:DISPlay:IQVTime:X[:SCALe]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Syntax :DISPlay:IQVTime:X[:SCALe]:MAXimum?

Returns <NRf> The upper limit of the horizontal scale setting range.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:X:SCALe:MAXimum?
might return 18.135E-3, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

Related Commands :DISPlay:IQVTime:X[:SCALe]

:DISPlay:IQVTime:X[:SCALe]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Syntax :DISPlay:IQVTime:X[:SCALe]:MINimum?

Returns <NRf> The lower limit of the horizontal scale setting range.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:X:SCALe:MINimum?
might return 10.0E-9, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

Related Commands :DISPlay:IQVTime:X[:SCALe]

:DISPlay:IQVTime:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) of the RF I&Q versus Time graph. Programming a specified offset sets :DISPlay:IQVTime:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:IQVTime:X[:SCALe]:OFFSet <value>
:DISPlay:IQVTime:X[:SCALe]:OFFSet?

Arguments <value>::={ <NRf> | MAXimum | MINimum } specifies the horizontal offset. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively.

Use the :DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum|MINimum? query to get the upper and lower limit values of the setting range.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:X:SCALe:OFFSet 800ns
sets the minimum horizontal value to 800 ns in the RF I&Q versus Time graph.

Related Commands :DISPlay:IQVTime:X[:SCALe]:AUTO:STATe
:DISPlay:IQVTime:X[:SCALe]
:DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum|MINimum?

:DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Syntax :DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum?

Returns <NRf> The upper limit of the horizontal offset setting range.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:X:SCALe:OFFSet:MAXimum?
might return $-1.812\text{E}-3$, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

Related Commands :DISPlay:IQVTime:X[:SCALe]:OFFSet

:DISPlay:IQVTime:X[:SCALe]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Syntax :DISPlay:IQVTime:X[:SCALe]:OFFSet:MINimum?

Returns <NRf> The lower limit of the horizontal offset setting range.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:X:SCALe:OFFSet:MINimum?
might return $-16.28\text{E}-3$, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

Related Commands :DISPlay:IQVTime:X[:SCALe]:OFFSet

:DISPlay:IQVTime:Y[:SCALe](?)

Sets or queries the vertical range of the RF I&Q versus Time graph.

Syntax :DISPlay:IQVTime:Y[:SCALe] <value>
 :DISPlay:IQVTime:Y[:SCALe]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 1 μ to 10 V.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:Y:SCALe 1.5
 sets the vertical range to 1.5 V in the RF I&Q versus Time graph.

Related Commands :DISPlay:IQVTime:Y[:SCALe]:OFFSet

:DISPlay:IQVTime:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the RF I&Q versus Time view.

Syntax :DISPlay:IQVTime:Y[:SCALe]:AUTO

Arguments None

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:Y:SCALe:AUTO
 sets the vertical scale automatically to fit the waveform to the screen.

:DISPlay:IQVTime:Y[:SCALe]:OFFSet(?)

Sets or queries the vertical offset (the value at the center of the vertical axis) in the RF I&Q versus Time graph.

Syntax :DISPlay:IQVTime:Y[:SCALe]:OFFSet <value>
 :DISPlay:IQVTime:Y[:SCALe]:OFFSet

Arguments <value>::=<NRf> specifies the vertical offset.
 Range: -5 to +5 V.

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:Y:SCALe:OFFSet -82.75mV
 sets the vertical offset to -82.75 mV in the RF I&Q versus Time graph.

Related Commands :DISPlay:IQVTime:Y[:SCALe]

:DISPlay:IQVTime:Y[:SCALe]:RESCale (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen.

Syntax :DISPlay:IQVTime:Y[:SCALe]:RESCale

Arguments None

Measurement Views RF I&Q versus Time

Examples :DISPlay:IQVTime:Y:SCALe:RESCale
 rescales the vertical axis automatically to fit the waveform to the screen.

:DISPlay:MCPower Subgroup

The :DISPlay:MCPower commands control the MCPR (Multiple Carrier Power Ratio) view.

Command Tree	Header	Parameter
	:DISPlay	
	:MCPower	
	:MARKer	
	:SHOW	
	:STATe	<boolean>
	:PLEVel	
	:SHOW	
	:STATe	<boolean>
	:RESet	
	:SCALE	
	:WINDow	
	:TRACe	
	:GRATicule	
	:GRID	
	:STATe	<boolean>
	:X	
	[:SCALE]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>
	:Y	
	[:SCALE]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>

:DISPlay:MCPower:MARKer:SHOW:STATe(?)

Determines whether to show or hide the readout for the selected marker in the MCPR view.

Syntax :DISPlay:MCPower:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }
:DISPlay:MCPower:MARKer:SHOW:STATe?

Arguments OFF or 0 hides the readout for the selected marker in the graph.
ON or 1 shows the readout for the selected marker in the graph.

Measurement Views MCPR

Examples :DISPlay:MCPower:MARKer:SHOW:STATe ON
shows the readout for the selected marker in the graph.

:DISPlay:MCPower:PLEVel:SHOW:STATe(?)

Determines whether to show or hide the power levels in the MCPR view.

Syntax :DISPlay:MCPower:PLEVel:SHOW:STATe { OFF | ON | 0 | 1 }
:DISPlay:MCPower:PLEVel:SHOW:STATe?

Arguments OFF or 0 hides the power levels in the graph.
ON or 1 shows the power levels in the graph.

Measurement Views MCPR

Examples :DISPlay:MCPower:PLEVel:SHOW:STATe ON
shows the power levels in the graph.

:DISPlay:MCPower:RESet:SCALE (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the MCPR view.

Vertical offset = Reference level
Vertical scale = 100 dB
Horizontal offset = Center frequency
Horizontal scale = Default span

Syntax :DISPlay:MCPower:RESet:SCALE

Arguments None

Measurement Views MCPR

Examples :DISPlay:MCPower:RESet:SCALE
resets the horizontal and vertical scale to the default values.

:DISPlay:MCPower:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:MCPower:WINDow:TRACe:GRATicule:GRID:STATe
{ OFF | ON | 0 | 1 }
:DISPlay:MCPower:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
ON or 1 shows the graticule grid.

Measurement Views MCPR

Examples :DISPlay:MCPower:WINDow:TRACe:GRATicule:GRID:STATe ON
shows the graticule grid on the screen.

:DISPlay:MCPower:X[:SCALe](?)

Sets or queries the horizontal range of the MCPR graph.

Syntax :DISPlay:MCPower:X[:SCALe] <value>
 :DISPlay:MCPower:X[:SCALe]?

Arguments <value>::=<NRf> specifies the horizontal range.
 Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views MCPR

Examples :DISPlay:MCPower:X:SCALe 10MHz
 sets the horizontal range to 10 MHz.

Related Commands :DISPlay:MCPower:X[:SCALe]:OFFSet

:DISPlay:MCPower:X[:SCALe]:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the MCPR view.

Syntax :DISPlay:MCPower:X[:SCALe]:AUTO

Arguments None

Measurement Views MCPR

Examples :DISPlay:MCPower:X:SCALe:AUTO
 rescales the horizontal scale automatically to fit the waveform to the screen.

:DISPlay:MCPower:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) of the MCPR graph.

Syntax :DISPlay:MCPower:X[:SCALe]:OFFSet <value>
 :DISPlay:MCPower:X[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum horizontal value.
 Range: $[(\text{center frequency}) - (\text{X scale}) \times 0.9]$ to $[(\text{center frequency}) + (\text{X scale}) \times 0.9]$

Measurement Views MCPR

Examples :DISPlay:MCPower:X:SCALe:OFFSet 1.45GHz
 sets the minimum horizontal value to 1.45 GHz in the MCPR graph.

Related Commands :DISPlay:MCPower:X[:SCALe]

:DISPlay:MCPower:Y[:SCALe](?)

Sets or queries the vertical range of the MCPR graph.

Syntax :DISPlay:MCPower:Y[:SCALe] <value>
 :DISPlay:MCPower:Y[:SCALe]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 0.1 to 200 dB.

Measurement Views MCPR

Examples :DISPlay:MCPower:Y:SCALe 100
 sets the vertical range to 100 dB in the MCPR graph.

Related Commands :DISPlay:MCPower:Y[:SCALe]:OFFSet

:DISPlay:MCPower:Y[:SCALE]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the MCPR view.

Syntax :DISPlay:MCPower:Y[:SCALE]:AUTO

Arguments None

Measurement Views MCPR

Examples :DISPlay:MCPower:Y:SCALE:AUTO
rescales the vertical scale automatically to fit the waveform to the screen.

:DISPlay:MCPower:Y[:SCALE]:OFFSet(?)

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the MCPR graph.

Syntax :DISPlay:MCPower:Y[:SCALE]:OFFSet <value>
:DISPlay:MCPower:Y[:SCALE]:OFFSet?

Arguments <value>::=<NRf> specifies the vertical offset.
Range: -170 to +50 dBm.

Measurement Views MCPR

Examples :DISPlay:MCPower:Y:SCALE:OFFSet -12.5
sets the vertical offset to -12.5 dBm in the MCPR graph.

Related Commands :DISPlay:MCPower:Y[:SCALE]

:DISPlay:MERRor Subgroup (Option 21 Only)

The :DISPlay:MERRor commands set up the Magnitude error versus Time view.

Command Tree	Header	Parameter
	:DISPlay	
	:MERRor	
	:Y	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>

:DISPlay:MERRor:Y[:SCALe](?)

Sets or queries the vertical range of the Magnitude error versus Time graph.

Syntax :DISPlay:MERRor:Y[:SCALe] <value>
 :DISPlay:MERRor:Y[:SCALe]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 1 to 100%.

Measurement Views Magnitude error versus Time

Examples :DISPlay:MERRor:Y:SCALe 50
 sets the vertical range to 50% in the Magnitude error versus Time graph.

Related Commands :DISPlay:MERRor:Y[:SCALe]:OFFSet

:DISPlay:MERRor:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Magnitude error versus Time view.

Syntax :DISPlay:MERRor:Y[:SCALe]:AUTO

Arguments None

Measurement Views Magnitude error versus Time

Examples :DISPlay:MERRor:Y:SCALe:AUTO
sets the vertical scale automatically to fit the waveform to the screen.

:DISPlay:MERRor:Y[:SCALe]:OFFSet(?)

Sets or queries the minimum vertical value (bottom edge) of the Magnitude error versus Time graph.

Syntax :DISPlay:MERRor:Y[:SCALe]:OFFSet <value>
:DISPlay:MERRor:Y[:SCALe]:OFFSet

Arguments <value>::=<NRf> specifies the minimum vertical value.
Range: -100 to +100%.

Measurement Views Magnitude error versus Time

Examples :DISPlay:MERRor:Y:SCALe:OFFSet -9.5
sets the minimum vertical value to -9.5% in the Magnitude error versus Time graph.

Related Commands :DISPlay:MERRor:Y[:SCALe]

:DISPlay:OBWidth Subgroup

The :DISPlay:OBWidth commands control the Occupied Bandwidth (OBW) view.

Command Tree	Header	Parameter
	:DISPlay	
	:OBWidth	
	:MARKer	
	:SHOW	
	:STATe	<boolean>
	:RESet	
	:SCALe	
	:SELected	
	:BANDwidth	OBWidth XDBbandwidth
	:WINDow	
	:TRACe	
	:GRATicule	
	:GRID	
	:STATe	<boolean>
	:X	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>
	:Y	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>

:DISPlay:OBWidth:MARKer:SHOW:STATe(?)

Determines whether to show or hide the readout for the selected marker in the Occupied Bandwidth view.

Syntax :DISPlay:OBWidth:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }
:DISPlay:OBWidth:MARKer:SHOW:STATe?

Arguments OFF or 0 hides the readout for the selected marker in the view.
ON or 1 shows the readout for the selected marker in the view.

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:MARKer:SHOW:STATe ON
shows the readout for the selected marker in the view.

:DISPlay:OBWidth:RESet:SCALE (No Query Form)

Resets the horizontal and vertical scale to the default values described below in the Occupied Bandwidth view.

Vertical offset = Reference level
Vertical scale = 100 dB
Horizontal offset = Center frequency
Horizontal scale = Default span

Syntax :DISPlay:OBWidth:RESet:SCALE

Arguments None

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:RESet:SCALE
resets the horizontal and vertical scale to the default values.

:DISPlay:OBWidth:SElected:BANDwidth(?)

Selects or queries the bandwidth (OBW or x dB BW) to measure in the Occupied Bandwidth view.

Syntax :DISPlay:OBWidth:SElected:BANDwidth { OBWidth | XDBbandwidth }
:DISPlay:OBWidth:SElected:BANDwidth?

Arguments OBWidth selects the occupied bandwidth to measure.
XDBbandwidth selects the x dB bandwidth to measure.

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:SElected:BANDwidth OBWidth
selects the occupied bandwidth to measure.

:DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATe
{ OFF | ON | 0 | 1 }
:DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
ON or 1 shows the graticule grid.

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATe ON
shows the graticule grid on the screen.

:DISPlay:OBWidth:X[:SCALe](?)

Sets or queries the horizontal range of the Occupied Bandwidth view.

Syntax :DISPlay:OBWidth:X[:SCALe] <value>
 :DISPlay:OBWidth:X[:SCALe]?

Arguments <value>::=<NRf> specifies the horizontal range.
 Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:X:SCALe 10MHz
 sets the horizontal range to 10 MHz.

Related Commands :DISPlay:OBWidth:X[:SCALe]:OFFSet

:DISPlay:OBWidth:X[:SCALe]:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the Occupied Bandwidth view.

Syntax :DISPlay:OBWidth:X[:SCALe]:AUTO

Arguments None

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:X:SCALe:AUTO
 rescales the horizontal scale automatically to fit the waveform to the screen.

:DISPlay:OBWidth:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) of the Occupied Bandwidth view.

Syntax :DISPlay:OBWidth:X[:SCALe]:OFFSet <value>
 :DISPlay:OBWidth:X[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum horizontal value.
 Range: [(center frequency) - (X scale) × 0.9] to
 [(center frequency) + (X scale) × 0.9]

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:X:SCALe:OFFSet 1.45GHz
 sets the minimum horizontal value to 1.45 GHz in the Occupied Bandwidth view.

Related Commands :DISPlay:OBWidth:X[:SCALe]

:DISPlay:OBWidth:Y[:SCALe](?)

Sets or queries the vertical range of the Occupied Bandwidth view.

Syntax :DISPlay:OBWidth:Y[:SCALe] <value>
 :DISPlay:OBWidth:Y[:SCALe]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 0.1 to 200 dB.

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:Y:SCALe 100
 sets the vertical range to 100 dB in the Occupied Bandwidth view.

Related Commands :DISPlay:OBWidth:Y[:SCALe]:OFFSet

:DISPlay:OBWidth:Y[:SCALe]:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the waveform to the screen in the Occupied Bandwidth view.

Syntax :DISPlay:OBWidth:Y[:SCALe]:AUTO

Arguments None

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:Y:SCALe:AUTO
rescales the vertical scale automatically to fit the waveform to the screen.

:DISPlay:OBWidth:Y[:SCALe]:OFFSet(?)

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the Occupied Bandwidth view.

Syntax :DISPlay:OBWidth:Y[:SCALe]:OFFSet <value>
:DISPlay:OBWidth:Y[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the vertical offset.
Range: -170 to +50 dBm.

Measurement Views Occupied Bandwidth

Examples :DISPlay:OBWidth:Y:SCALe:OFFSet -12.5
sets the vertical offset to -12.5 dBm in the Occupied Bandwidth view.

Related Commands :DISPlay:OBWidth:Y[:SCALe]

:DISPlay:PERRor Subgroup (Option 21 Only)

The :DISPlay:PERRor commands set up the Phase error versus Time view.

Command Tree	Header	Parameter
	:DISPlay	
	:PERRor	
	:Y	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>

:DISPlay:PERRor:Y[:SCALe](?)

Sets or queries the vertical range of the Phase error versus Time graph.

Syntax :DISPlay:PERRor:Y[:SCALe] <value>
 :DISPlay:PERRor:Y[:SCALe]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 1 to 360°.

Measurement Views Phase error versus Time

Examples :DISPlay:PERRor:Y:SCALe 30
 sets the vertical range to 30° in the Phase error versus Time graph.

Related Commands :DISPlay:PERRor:Y[:SCALe]:OFFSet

:DISPlay:PERRor:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Phase error versus Time view.

Syntax :DISPlay:PERRor:Y[:SCALe]:AUTO

Arguments None

Measurement Views Phase error versus Time

Examples :DISPlay:PERRor:Y:SCALe:AUTO
sets the vertical scale automatically to fit the waveform to the screen.

:DISPlay:PERRor:Y[:SCALe]:OFFSet(?)

Sets or queries the minimum vertical value (bottom edge) of the Phase error versus Time graph.

Syntax :DISPlay:PERRor:Y[:SCALe]:OFFSet <value>
:DISPlay:PERRor:Y[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum vertical value.
Range: -360 to +360°.

Measurement Views Phase error versus Time

Examples :DISPlay:PERRor:Y:SCALe:OFFSet -14.5
sets the minimum vertical value to -14.5° in the Phase Error versus Time graph.

Related Commands :DISPlay:PERRor:Y[:SCALe]

:DISPlay:PHVTime Subgroup

The :DISPlay:PHVTime commands control display in the Phase versus Time measurement.

Command Tree	Header	Parameter
	:DISPlay	
	:PHVTime	
	:WINDow	
	:TRACe	
	:GRATicule	
	:GRID	
	:STATe	<boolean>
	:X	
	[:SCALe]	<numeric_value>
	:AUTO	
	:STATe	<boolean>
	:MAXimum?	
	:MINimum?	
	:OFFSet	<numeric_value>
	:MAXimum?	
	:MINimum?	
	:Y	
	[:SCALe]	<numeric_value>
	:AUTO	
	:AXIS	MODulopi CONTinuous
	:REFerence	<numeric_value>
	:OFFSet	<numeric_value>
	:RESCale	

:DISPlay:PHVTime:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:PHVTime:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }

 :DISPlay:PHVTime:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:WINDow:TRACe:GRATicule:GRID:STATe ON
 shows the graticule grid on the Frequency versus Time view.

:DISPlay:PHVTime:X[:SCALe](?)

Sets or queries the horizontal scale (full-scale time) of the Phase versus Time graph. Programming a specified scale sets :DISPlay:PHVTime:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:PHVTime:X[:SCALe] <value>
 :DISPlay:PHVTime:X[:SCALe]?

Arguments <value>::={ <NRf> | MAXimum | MINimum } specifies the horizontal scale in full-scale time. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively.

Use the :DISPlay:PHVTime:X[:SCALe]:MAXimum|:MINimum? query to get the upper and lower limit values of the setting range.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:X:SCALe 1.5ms
 sets the horizontal scale to 1.5 ms.

Related Commands :DISPlay:PHVTime:X[:SCALe]:AUTO:STATe
 :DISPlay:PHVTime:X[:SCALe]:OFFSet
 :DISPlay:PHVTime:X[:SCALe]:MAXimum|:MINimum

:DISPlay:PHVTime:X[:SCALe]:AUTO (No Query Form)

Sets the horizontal scale automatically to fit the waveform to the screen in the Phase versus Time view. Executing this command sets :DISPlay:PHVTime:X[:SCALe]:AUTO:STATe ON.

Syntax :DISPlay:PHVTime:X[:SCALe]:AUTO

Arguments None

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:X:SCALe:AUTO
sets the horizontal scale automatically to fit the waveform to the screen.

Related Commands :DISPlay:PHVTime:X[:SCALe]:AUTO:STATe

:DISPlay:PHVTime:X[:SCALe]:AUTO:STATe(?)

Determines whether to set the horizontal scale automatically or manually.

Syntax :DISPlay:PHVTime:X[:SCALe]:AUTO:STATe { OFF | ON | 0 | 1 }
:DISPlay:PHVTime:X[:SCALe]:AUTO:STATe?

Arguments OFF or 0 specifies that the horizontal scale is set manually. To set it, use the :DISPlay:PHVTime:X[:SCALe] and :DISPlay:PHVTime:X[:SCALe]:OFFSet commands.

ON or 1 specifies that the horizontal scale is set automatically.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:X:SCALe:AUTO:STATe ON
specifies that the horizontal scale is set automatically.

Related Commands :DISPlay:PHVTime:X[:SCALe], :DISPlay:PHVTime:X[:SCALe]:OFFSet

:DISPlay:PHVTime:X[:SCALe]:MAXimum? (Query Only)

Queries the upper limit of the horizontal scale setting range.

Syntax :DISPlay:PHVTime:X[:SCALe]:MAXimum?

Returns <NRf> The upper limit of the horizontal scale setting range.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:X:SCALe:MAXimum?
might return 18.135E-3, indicating that the upper limit of the horizontal scale setting range is 18.135 ms.

Related Commands :DISPlay:PHVTime:X[:SCALe]

:DISPlay:PHVTime:X[:SCALe]:MINimum? (Query Only)

Queries the lower limit of the horizontal scale setting range.

Syntax :DISPlay:PHVTime:X[:SCALe]:MINimum?

Returns <NRf> The lower limit of the horizontal scale setting range.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:X:SCALe:MINimum?
might return 10.0E-9, indicating that the lower limit of the horizontal scale setting range is 10.0 ns.

Related Commands :DISPlay:PHVTime:X[:SCALe]

:DISPlay:PHVTime:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) of the Phase versus Time graph. Programming a specified offset sets :DISPlay:PHVTime:X[:SCALe]:AUTO:STATe OFF.

Syntax :DISPlay:PHVTime:X[:SCALe]:OFFSet
 :DISPlay:PHVTime:X[:SCALe]:OFFSet?

Arguments <value>::={ <NRf> | MAXimum | MINimum } specifies the horizontal offset. MAXimum and MINimum represent the upper and lower limits of the setting range, respectively.

Use the :DISPlay:PHVTime:X[:SCALe]:OFFSet:MAXimum|MINimum? query to get the upper and lower limit values of the setting range.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:X:SCALe:OFFSet 800ns
 sets the minimum horizontal value to 800 ns in the Phase versus Time graph.

Related Commands :DISPlay:PHVTime:X[:SCALe]:AUTO:STATe
 :DISPlay:PHVTime:X[:SCALe]
 :DISPlay:PHVTime:X[:SCALe]:OFFSet:MAXimum|MINimum?

:DISPlay:PHVTime:X[:SCALe]:OFFSet:MAXimum? (Query Only)

Queries the upper limit of the horizontal offset setting range.

Syntax :DISPlay:PHVTime:X[:SCALe]:OFFSet:MAXimum?

Returns <NRf> The upper limit of the horizontal offset setting range.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:X:SCALe:OFFSet:MAXimum?
might return -1.812E-3, indicating that the upper limit of the horizontal offset setting range is -1.812 ms.

Related Commands :DISPlay:PHVTime:X[:SCALe]:OFFSet

:DISPlay:PHVTime:X[:SCALe]:OFFSet:MINimum? (Query Only)

Queries the lower limit of the horizontal offset setting range.

Syntax :DISPlay:PHVTime:X[:SCALe]:OFFSet:MINimum?

Returns <NRf> The lower limit of the horizontal offset setting range.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:X:SCALe:OFFSet:MINimum?
might return -16.28E-3, indicating that the lower limit of the horizontal offset setting range is -16.28 ms.

Related Commands :DISPlay:PHVTime:X[:SCALe]:OFFSet

:DISPlay:PHVTime:Y[:SCALe](?)

Sets or queries the vertical range of the Phase versus Time graph.

Syntax :DISPlay:PHVTime:Y[:SCALe] <value>
 :DISPlay:PHVTime:Y[:SCALe]

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 1 to 1T°.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:Y:SCALe 180
 sets the vertical range to 180° in the Phase versus Time graph.

Related Commands :DISPlay:PHVTime:Y[:SCALe]:OFFSet

:DISPlay:PHVTime:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the Phase versus Time view.

Syntax :DISPlay:PHVTime:Y[:SCALe]:AUTO

Arguments None

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:Y:SCALe:AUTO
 sets the vertical scale automatically to fit the waveform to the screen.

:DISPlay:PHVTime:Y[:SCALe]:AXIS(?)

Selects or queries the vertical axis representation.

Syntax :DISPlay:PHVTime:Y[:SCALe]:AXIS { MODulo π | CONTinuous }
 :DISPlay:PHVTime:Y[:SCALe]:AXIS?

Arguments MODulo π (modulo π) shows the phase constrained within $\pm 180^\circ$ along the vertical axis.
 CONTinuous shows the phase as continuous quantity along the vertical axis.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:Y:SCALe:AXIS MODulo π
 selects modulo π representation for the vertical axis.

:DISPlay:PHVTime:Y[:SCALe]:AXIS:REFeRence(?)

Selects or queries which time point in the analysis period to use as the zero-phase-value reference.

Syntax :DISPlay:PHVTime:Y[:SCALe]:AXIS:REFeRence <value>
 :DISPlay:PHVTime:Y[:SCALe]:AXIS:REFeRence?

Arguments <value>::=<NRf> specifies the phase reference time.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:Y:SCALe:AXIS:REFeRence 1.5us
 sets the phase reference time to 1.5 μ s.

:DISPlay:PHVTime:Y[:SCALe]:OFFSet(?)

Sets or queries the vertical offset (the value at the center of the vertical axis) in the Phase versus Time graph.

Syntax :DISPlay:PHVTime:Y[:SCALe]:OFFSet <value>
 :DISPlay:PHVTime:Y[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the vertical offset.
 Range: $-0.5T$ to $+0.5T^\circ$.

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:Y:SCALe:OFFSet -158.5
 sets the vertical offset to -158.5° in the Phase versus Time graph.

Related Commands :DISPlay:PHVTime:Y[:SCALe]

:DISPlay:PHVTime:Y[:SCALe]:RESCale (No Query Form)

Rescales the vertical axis automatically to fit the Phase versus Time waveform to the screen.

Syntax :DISPlay:PHVTime:Y[:SCALe]:RESCale

Arguments None

Measurement Views Phase versus Time

Examples :DISPlay:PHVTime:Y:SCALe:RESCale
 rescales the vertical axis automatically to fit the Phase versus Time waveform to the screen.

:DISPlay:PULSe Subgroup (Option 20 Only)

The :DISPlay:PULSe commands control display in the Pulsed RF measurements.

Command Tree	Header	Parameter
	:DISPlay	
	:PULSe	
	:MEASview	
	:DELeTe	RESult TRACe STATistics
	:NEW	RESult TRACe STATistics
	:SELeCt	RESult TRACe STATistics
	:RESult	
	:ATX	<boolean>
	:AVERage	<boolean>
	:DROop	<boolean>
	:DUTPct	<boolean>
	:DUTRatio	<boolean>
	:FALL	<boolean>
	:FRDeviation	<boolean>
	:MFReqerror	<boolean>
	:MPHerror	<boolean>
	:PHDeviation	<boolean>
	:PPFRequency	<boolean>
	:PPOWer	<boolean>
	:PPPHase	<boolean>
	:RINTerval	<boolean>
	:RIPPlE	<boolean>
	:RISE	<boolean>
	:RMSFreqerror	<boolean>
	:RMSPherror	<boolean>
	:RRATe	<boolean>
	:TIME	<boolean>
	:WIDTh	<boolean>
	:SELeCt	
	:NUMBer	<numeric_value>
	:RESult	AVERage PPOWer ATX WIDTh RISE FALL RINTerval RRATe DUTPct DUTRatio RIPPlE DROop PPPHase PPFRequency RMSFreqerror MFReqerror RMSPherror MPHerror FRDeviation PHDeviation

```
:STATistics
:MARKer
:SHOW
:STATe <boolean>
:PLOT TREND | FFT
:WINDow
:TRACe
:GRATICule
:GRID
:STATe <boolean>

:X
:RSCale
[:SCALE]
:NUMBER <numeric_value>
:OFFSET <numeric_value>

:Y
:RSCale
[:SCALE]
:FULL <numeric_value>
:OFFSET <numeric_value>
:STOP? <numeric_value>

:TRACe
:MARKer
:SHOW
:STATe <boolean>
:POINT
:SHOW <boolean>
:WINDow
:TRACe
:GRATICule
:GRID
:STATe <boolean>

:X
:RSCale
[:SCALE] <numeric_value>
:FULL SElected | MAXimum
:OFFSET <numeric_value>
:PDIVision <numeric_value>

:Y
:RSCale
[:SCALE]
:FULL <numeric_value>
:OFFSET <numeric_value>
:STOP? <numeric_value>
```

:DISPlay:PULSe:MEASview:DELeTe (No Query Form)

Deletes the measurement view in the pulsed RF measurements.

Syntax :DISPlay:PULSe:MEASview:DELeTe { RESult | TRACe | STATistics }

Arguments RESult deletes the pulse table view.

TRACe deletes the pulse trace view.

STATistics deletes the pulse statistics view.

If you attempt to delete a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Measurement Views Pulsed RF measurements

Examples :DISPlay:PULSe:MEASview:DELeTe TRACe
deletes the pulse trace view.

:DISPlay:PULSe:MEASview:NEW (No Query Form)

Displays a new measurement view in the pulsed RF measurements.

Syntax :DISPlay:PULSe:MEASview:NEW { RESult | TRACe | STATistics }

Arguments RESult opens the pulse table view.

TRACe opens the pulse trace view.

STATistics opens the pulse statistics view.

If you attempt to open a view that is currently displayed on screen, the error (-200, "Execution error; Measurement is already running") will be returned.

Measurement Views Pulsed RF measurements

Examples :DISPlay:PULSe:MEASview:NEW STATistics
creates the pulse statistics view.

:DISPlay:PULSe:MEASview:SElect(?)

Selects a measurement view in the pulsed RF measurements on the screen.
The query command returns the currently selected view.

Syntax :DISPlay:PULSe:MEASview:SElect { RESult | TRACe | STATistics }

Arguments RESult selects the pulse table view.

TRACe selects the pulse trace view.

STATistics selects the pulse statistics view.

If you attempt to select a view that is not displayed on screen, the error (-200, "Execution error; Measurement not running") will be returned.

Measurement Views Pulsed RF measurements

Examples :DISPlay:PULSe:MEASview:SElect TRACe
selects the pulse trace view.

:DISPlay:PULSe:RESult:ATX(?)

Determines whether or not to show the average transmitted power measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:ATX { OFF | ON | 0 | 1 }
:DISPlay:PULSe:RESult:ATX?

Arguments OFF or 0 does not show the average transmitted power measurement result.

ON or 1 shows the average transmitted power measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:ATX ON
shows the average transmitted power measurement result in the pulse table.

:DISPlay:PULSe:RESult:AVERage(?)

Determines whether or not to show the average on power measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:AVERage { OFF | ON | 0 | 1 }
:DISPlay:PULSe:RESult:AVERage?

Arguments OFF or 0 does not show the average on power measurement result.
ON or 1 shows the average on power measurement result in the results table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:AVERage ON
shows the average on power measurement result in the pulse table.

:DISPlay:PULSe:RESult:DR0op(?)

Determines whether or not to show the droop measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:DR0op { OFF | ON | 0 | 1 }
:DISPlay:PULSe:RESult:DR0op?

Arguments OFF or 0 does not show the droop measurement result.
ON or 1 shows the droop measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:DR0op ON
shows the droop measurement result in the pulse table.

:DISPlay:PULSe:RESult:DUTPct(?)

Determines whether or not to show the duty factor (%) measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:DUTPct { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:DUTPct?

Arguments OFF or 0 does not show the duty factor measurement result.
 ON or 1 shows the duty factor measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:DUTPct ON
 shows the duty factor (%) measurement result in the pulse table.

:DISPlay:PULSe:RESult:DUTRatio(?)

Determines whether or not to show the duty factor (ratio) measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:DUTRatio { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:DUTRatio?

Arguments OFF or 0 does not show the duty factor measurement result.
 ON or 1 shows the duty factor measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:DUTRatio ON
 shows the duty factor (ratio) measurement result in the pulse table.

:DISPlay:PULSe:RESult:FALL(?)

Determines whether or not to show the fall time measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:FALL { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:FALL?

Arguments OFF or 0 does not show the fall time measurement result.
 ON or 1 shows the fall time measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:FALL ON
 shows the fall time measurement result in the pulse table.

:DISPlay:PULSe:RESult:FRDeviation(?)

Determines whether or not to show the frequency deviation measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:FRDeviation { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:FRDeviation?

Arguments OFF or 0 does not show the frequency deviation measurement result.
 ON or 1 shows the frequency deviation measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:FRDeviation ON
 shows the frequency deviation measurement result in the pulse table.

:DISPlay:PULSe:RESult:MFRerror(?)

Determines whether or not to show the maximum frequency error measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:MFRerror { OFF | ON | 0 | 1 }
:DISPlay:PULSe:RESult:MFRerror?

Arguments OFF or 0 does not show the maximum frequency error measurement result.
ON or 1 shows the maximum frequency error measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:MFRerror ON
shows the maximum frequency error measurement result in the pulse table.

:DISPlay:PULSe:RESult:MPHerror(?)

Determines whether or not to show the maximum phase error measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:MPHerror { OFF | ON | 0 | 1 }
:DISPlay:PULSe:RESult:MPHerror?

Arguments OFF or 0 does not show the maximum phase error measurement result.
ON or 1 shows the maximum phase error measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:MPHerror ON
shows the maximum phase error measurement result in the pulse table.

:DISPlay:PULSe:RESult:PHDeviation(?)

Determines whether or not to show the phase deviation measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:PHDeviation { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:PHDeviation?

Arguments OFF or 0 does not show the phase deviation measurement result.
 ON or 1 shows the phase deviation measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:PHDeviation ON
 shows the phase deviation measurement result in the pulse table.

:DISPlay:PULSe:RESult:PPFRequency(?)

Determines whether or not to show the pulse-pulse carrier frequency measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:PPFRequency { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:PPFRequency?

Arguments OFF or 0 does not show the pulse-pulse carrier frequency measurement result.
 ON or 1 shows the pulse-pulse carrier frequency measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:PPFRequency ON
 shows the pulse-pulse carrier frequency measurement result in the pulse table.

:DISPlay:PULSe:RESult:PPOWer(?)

Determines whether or not to show the peak power measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:PPOWer { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:PPOWer?

Arguments OFF or 0 does not show the peak power measurement result.
 ON or 1 shows the peak power measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:PPOWer ON
 shows the peak power measurement result in the pulse table.

:DISPlay:PULSe:RESult:PPPHase(?)

Determines whether or not to show the pulse-pulse carrier phase measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:PPPHase { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:PPPHase?

Arguments OFF or 0 does not show the pulse-pulse carrier phase measurement result.
 ON or 1 shows the pulse-pulse carrier phase measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:PPPHase ON
 shows the pulse-pulse carrier phase measurement result in the pulse table.

:DISPlay:PULSe:RESult:RINTerval(?)

Determines whether or not to show the repetition interval measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:RINTerval { OFF | ON | 0 | 1 }
:DISPlay:PULSe:RESult:RINTerval?

Arguments OFF or 0 does not show the repetition interval measurement result.
ON or 1 shows the repetition interval measurement result in the results table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:RINTerval ON
shows the repetition interval measurement result in the pulse table.

:DISPlay:PULSe:RESult:RIPPlE(?)

Determines whether or not to show the ripple measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:RIPPlE { OFF | ON | 0 | 1 }
:DISPlay:PULSe:RESult:RIPPlE?

Arguments OFF or 0 does not show the ripple measurement result.
ON or 1 shows the ripple measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:RIPPlE ON
shows the ripple measurement result in the pulse table.

:DISPlay:PULSe:RESult:RISE(?)

Determines whether or not to show the rise time measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:RISE { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:RISE?

Arguments OFF or 0 does not show the rise time measurement result.
 ON or 1 shows the rise time measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:RISE ON
 shows the rise time measurement result in the pulse table.

:DISPlay:PULSe:RESult:RMSFreqerror(?)

Determines whether or not to show the RMS frequency error measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:RMSFreqerror { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:RMSFreqerror?

Arguments OFF or 0 does not show the RMS frequency error measurement result.
 ON or 1 shows the RMS frequency error measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:RMSFreqerror ON
 shows the RMS frequency error measurement result in the pulse table.

:DISPlay:PULSe:RESult:RMSPherror(?)

Determines whether or not to show the RMS phase error measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:RMSPherror { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:RMSPherror?

Arguments OFF or 0 does not show the RMS phase error measurement result.
 ON or 1 shows the RMS phase error measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:RMSPherror ON
 shows the RMS phase error measurement result in the pulse table.

:DISPlay:PULSe:RESult:RRATe(?)

Determines whether or not to show the repetition rate measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:RRATe { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:RRATe?

Arguments OFF or 0 does not show the repetition rate measurement result.
 ON or 1 shows the repetition rate measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:RRATe ON
 shows the repetition rate measurement result in the pulse table.

:DISPlay:PULSe:RESult:TIME(?)

Determines whether or not to show the time measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:TIME { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:TIME?

Arguments OFF or 0 does not show the time measurement result.
 ON or 1 shows the time measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:TIME ON
 shows the time measurement result in the pulse table.

:DISPlay:PULSe:RESult:WIDTh(?)

Determines whether or not to show the pulse width measurement result in the pulse table.

Syntax :DISPlay:PULSe:RESult:WIDTh { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:RESult:WIDTh?

Arguments OFF or 0 does not show the pulse width measurement result.
 ON or 1 shows the pulse width measurement result in the pulse table.

Measurement Views Pulse table

Examples :DISPlay:PULSe:RESult:WIDTh ON
 shows the pulse width measurement result in the pulse table.

:DISPlay:PULSe:SElect:NUMBer(?)

Selects or queries a pulse to measure. For the selected pulse, the statistics view indicates the measurement result while the table view highlights it, and the trace view displays the waveform.

Syntax :DISPlay:PULSe:SElect:NUMBer <number>
 :DISPlay:PULSe:SElect:NUMBer?

Arguments <number>::=<NR1> specifies the number of pulse to measure.
 Range: -(the number of acquired pulses before the time reference) to
 +(the number of acquired pulses after the time reference)

Zero (0) represents the pulse at the analysis time reference specified using the [:SENSe]:ANALysis:REference command.
The number of acquired pulses depends on the analysis range.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :DISPlay:WINDow:SElect:NUMBer -28
 measures the pulse #-28.

Related Commands [:SENSe]:ANALysis:REference

:DISPlay:PULSe:SElect:RESult(?)

Selects or queries which result is shown in the pulse trace and statistics views.

Syntax :DISPlay:PULSe:SElect:RESult { AVERage | PPOWer | ATX | WIDTH
 | RISE | FALL | RINTerval | RRATe | DUTPct | DUTRatio | RIPPlE
 | DROop | PPPHase | PPFRequency | RMSFRequerror | MFRequerror
 | RMSPherror | MPHerror | FRDeviatiOn | PHDeviatiOn }

Arguments Table 2-35 lists the arguments.

Table 2-35: Pulse results

Argument	Result
AVERage	Average on power
PPOWer	Peak power
ATX	Average transmitted power
WIDTH	Pulse width
RISE	Rise time
FALL	Fall time
RINTerval	Repetition interval
RRATe	Repetition rate
DUTPct	Duty factor (%)
DUTRatio	Duty factor (ratio)
RIPPlE	Ripple
DROop	Droop
PPPHase	Pulse-pulse carrier phase
PPFRequency	Pulse-pulse carrier frequency
RMSFRequerror	RMS frequency error
MFRequerror	Maximum frequency error
RMSPherror	RMS phase error
MPHerror	Maximum phase error
FRDeviatiOn	Frequency deviation
PHDeviatiOn	Phase deviation

Measurement Views Pulse statistics, Pulse trace

Examples :DISPlay:PULSe:SElect:RESult AVERage
shows the average on power result in the pulse trace and statistics views.

:DISPlay:PULSe:STATistics:MARKer:SHOW:STATe(?)

Determines whether to show or hide the marker readout in the statistics graph.
This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to FFT.

Syntax :DISPlay:PULSe:STATistics:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }
:DISPlay:PULSe:STATistics:MARKer:SHOW:STATe?

Arguments OFF or 0 hides the marker readout.
ON or 1 shows the marker readout.

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:MARKer:SHOW:STATe ON
shows the marker readout in the statistics graph.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:DISPlay:PULSe:STATistics:PLOT(?)

Selects or queries how to show the statistics graph.

Syntax :DISPlay:PULSe:STATistics:PLOT { TREND | FFT }
 :DISPlay:PULSe:STATistics:PLOT?

Arguments TREND shows the statistics result along with the pulse number.
 FFT shows the statistics result transformed into the frequency domain by FFT.

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:PLOT TREND
 shows the statistics result along with the pulse number.

:DISPlay:PULSe:STATistics:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid in the statistics view.

Syntax :DISPlay:PULSe:STATistics:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:STATistics:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:WINDow:TRACe:GRATicule:GRID:STATe ON
 shows the graticule grid on the statistics view.

:DISPlay:PULSe:STATistics:X:RSCale (No Query Form)

Rescales the horizontal axis to fit the waveform to the screen in the statistics graph.

Syntax :DISPlay:PULSe:STATistics:X:RSCale

Arguments None

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:X:RSCale
rescales the horizontal axis of the statistics graph.

:DISPlay:PULSe:STATistics:X[:SCALE]:NUMBer(?)

Sets or queries the horizontal full scale in the statistics graph.

Syntax :DISPlay:PULSe:STATistics:X[:SCALE]:NUMBer <value>
:DISPlay:PULSe:STATistics:X[:SCALE]:NUMBer?

Arguments <value>::=<Nrf> specifies the horizontal full scale.

The setting range depends on the :DISPlay:PULSe:STATistics:PLOT command parameters as shown in the table below.

:DISPlay:PULSe:STATistics:PLOT	Setting range
TREND	1 to 1000
FFT	1 Hz to 120 MHz

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:X:SCALE:NUMBer 50
sets the horizontal full scale to 50 pulses when the plot is trend.

Related Commands :DISPlay:PULSe:STATistics:PLOT
:DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet

:DISPlay:PULSe:STATistics:X[:SCALe]:OFFSet(?)

Selects or queries the minimum horizontal value (the first pulse to show) in the statistics graph.

Syntax :DISPlay:PULSe:STATistics:X[:SCALe]:OFFSet <value>
 :DISPlay:PULSe:STATistics:X[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the number of the first pulse.
 Range: $-(X - X/10)$ to $+(X - X/10)$
 where X is the horizontal scale set by the :DISPlay:PULSe:STATistics
 :X[:SCALe]:NUMBer command

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:X:SCALe:OFFSet 120
 sets the first pulse number to #120.

Related Commands :DISPlay:PULSe:STATistics:X[:SCALe]:NUMBer

:DISPlay:PULSe:STATistics:Y:RSCale (No Query Form)

Rescales the vertical axis to fit the waveform to the screen in the statistics graph.

Syntax :DISPlay:PULSe:STATistics:Y:RSCale

Arguments None

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:X:RSCale
 rescales the vertical axis of the statistics graph.

:DISPlay:PULSe:STATistics:Y[:SCALe]:FULL(?)

Sets or queries the vertical full scale in the statistics graph.

Syntax :DISPlay:PULSe:STATistics:Y[:SCALe]:FULL <value>
 :DISPlay:PULSe:STATistics:Y[:SCALe]:FULL?

Arguments <value>::=<NRf> specifies the vertical full scale.
 The setting range depends on the :DISPlay:PULSe:STATistics:PLOT command parameters and the measurement items as shown in the table below.

:DISPlay:PULSe:STATistics:PLOT	Measurement item	Setting range
TREND	Average on power Peak power Average transmitted power	0.1 to 200 dB
	Pulse width Rise time Fall time Repetition interval	1 n to 5 Ms
	Repetition rate	100 m to 100 MHz
	Duty factor Ripple	1 to 100%
	Droop	1 to 200%
	Pulse-pulse carrier phase	1 to 360°
FFT	All	10 to 200 dB

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:Y:SCALe:FULL 100
 sets the vertical full scale to 100 dB.

Related Commands :DISPlay:PULSe:STATistics:PLOT
 :DISPlay:PULSe:STATistics:X[:SCALe]:OFFSet

:DISPlay:PULSe:STATistics:Y[:SCALe]:OFFSet(?)

Sets or queries the vertical offset in the statistics graph.

Syntax :DISPlay:PULSe:STATistics:Y[:SCALe]:OFFSet <value>
 :DISPlay:PULSe:STATistics:Y[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the vertical offset.

The vertical offset is the value at the top or the bottom edge of the graph depending on measurement items. The setting range depends on the :DISPlay:PULSe:STATistics:PLOT command parameters and the measurement items as shown in the table below.

:DISPlay:PULSe:STATistics:PLOT	Measurement item	Setting range	Offset position ¹
TRENd	Average on power Peak power Average transmitted power	-170 to +50 dBm	Top (Bottom for the unit of Volts or Watts)
	Pulse width Rise time Fall time Repetition interval	0 to 5 Ms	Bottom
	Repetition rate	0 to 100 MHz	Bottom
	Duty factor Ripple	0 to 100%	Bottom
	Droop	0 to +100%	Bottom
	Pulse-pulse carrier phase	-180 to +180°	Bottom
FFT	All	-400 to +100 dB	Top

¹ Indicates whether the offset is the value at the top or the bottom edge of the graph.

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:Y:SCALe:OFFSet 24.8
 sets the maximum vertical value to 24.8 dBm in the statistics graph.

Related Commands :DISPlay:PULSe:STATistics:PLOT,
 :DISPlay:PULSe:STATistics:X[:SCALe]:PDIVision

:DISPlay:PULSe:STATistics:Y[:SCALe]:STOP? (Query Only)

Queries the minimum vertical value (bottom edge) in the statistics graph.

Syntax :DISPlay:PULSe:STATistics:Y[:SCALe]:STOP?

Returns <y_stop>::=<NRf> is the minimum vertical value (bottom edge).

Measurement Views Pulse statistics

Examples :DISPlay:PULSe:STATistics:Y:SCALe:STOP?
might return -150.0 indicating that the minimum vertical value is -150 dBm in the pulse statistics graph.

Related Commands :DISPlay:PULSe:STATistics:X[:SCALe]:OFFSet

:DISPlay:PULSe:TRACe:MARKer:SHOW:STATe(?)

Determines whether to show or hide the marker readout in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:MARKer:SHOW:STATe { OFF | ON | 0 | 1 }
:DISPlay:PULSe:TRACe:MARKer:SHOW:STATe?

Arguments OFF or 0 hides the marker readout.
ON or 1 shows the marker readout.

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:MARKer:SHOW:STATe ON
shows the marker readout on the pulse trace view.

:DISPlay:PULSe:TRACe:POINt:SHOW(?)

Determines whether to show or hide the measurement points and lines in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:POINt:SHOW { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:TRACe:POINt:SHOW?

Arguments OFF or 0 hides the measurement points and lines.
 ON or 1 shows the measurement points and lines.

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:POINt:SHOW ON
 shows the measurement points and lines in the pulse trace view.

:DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }
 :DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATe ON
 shows the graticule grid on the pulse trace view.

:DISPlay:PULSe:TRACe:X:RSCale (No Query Form)

Rescales the horizontal axis to fit the waveform to the screen in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:X[:SCALe]:RSCale

Arguments None

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:X:SCALe:RSCale
rescales the horizontal axis in the pulse trace view.

:DISPlay:PULSe:TRACe:X[:SCALe](?)

Sets or queries the horizontal full scale in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:X[:SCALe] <value>
:DISPlay:PULSe:TRACe:X[:SCALe]?

Arguments <value>::=<NRf> specifies the horizontal full scale.
Range: 10 ns to acquisition memory capacity.

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:X:SCALe 5.5E-6
sets the horizontal scale to 5.5 μ s.

:DISPlay:PULSe:TRACe:X[:SCALe]:FULL(?)

Selects or queries the full-scale reference for the horizontal rescale.

Syntax :DISPlay:PULSe:TRACe:X[:SCALe]:FULL { SElecteD | MAXimum }
 :DISPlay:PULSe:TRACe:X[:SCALe]:FULL?

Arguments SElecteD uses the selected pulse for the full-scale reference.
 MAXimum uses the maximum pulse for the full-scale reference.

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:X:SCALe:FULL SElecteD
 uses the selected pulse for the full-scale reference.

:DISPlay:PULSe:TRACe:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:X[:SCALe]:OFFSet <value>
 :DISPlay:PULSe:TRACe:X[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum horizontal value.
 Range: $[(\text{analysis offset}) - (\text{X scale}) \times 0.9]$ to $[(\text{analysis offset}) + (\text{analysis length}) - (\text{X scale}) \times 0.1]$

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:X:SCALe:OFFSet 937.5E-9
 sets the minimum horizontal value to 937.5 ns.

Related Commands :DISPlay:PULSe:TRACe:X[:SCALe]:PDIVision

:DISPlay:PULSe:TRACe:X[:SCALe]:PDIVision(?)

Sets or queries the horizontal full scale in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:X[:SCALe]:PDIVision <value>
 :DISPlay:PULSe:TRACe:X[:SCALe]:PDIVision?

Arguments <value>::=<NRf> specifies the horizontal full scale.
 Range: 10 ns to acquisition memory capacity.

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:X:SCALe:PDIVision 5.5E-6
 sets the horizontal scale to 5.5 μ s.

:DISPlay:PULSe:TRACe:Y:RSCale (No Query Form)

Rescales the vertical axis to fit the waveform to the screen in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:Y[:SCALe]:RSCale

Arguments None

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:Y:SCALe:RSCale
rescales the vertical axis in the pulse trace view.

:DISPlay:PULSe:TRACe:Y[:SCALe]:FULL(?)

Sets or queries the vertical full scale in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:Y[:SCALe]:FULL <value>
:DISPlay:PULSe:TRACe:Y[:SCALe]:FULL?

Arguments <value>::=<NRf> specifies the vertical full scale.
Range: 0.1 to 200 dB.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:Y:SCALe:FULL 100
sets the vertical full scale to 100 dB.

Related Commands [:SENSe]:POWer:UNITs, :DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet

:DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet(?)

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet <value>
 :DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the vertical offset.
 Range: -170 to +50 dBm.

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:Y:SCALe:OFFSet 23.5
 sets the vertical offset to 23.5 dBm.

Related Commands :DISPlay:PULSe:TRACe:Y[:SCALe]:STOP?

:DISPlay:PULSe:TRACe:Y[:SCALe]:STOP? (Query Only)

Queries the minimum vertical value (bottom edge) in the pulse trace view.

Syntax :DISPlay:PULSe:TRACe:Y[:SCALe]:STOP?

Returns <y_stop>::=<NRf> is the minimum vertical value (bottom edge).

Measurement Views Pulse trace

Examples :DISPlay:PULSe:TRACe:Y:SCALe:STOP?
 might return -150.0 indicating that the minimum vertical value is -150 dBm in the pulse trace view.

Related Commands :DISPlay:PULSe:TRACe:Y[:SCALe]:OFFSet

:DISPlay:SGRam Subgroup

The :DISPlay:SGRam commands control the spectrogram view.

Command Tree	Header	Parameter
	:DISPlay:SGRam	
	:FREQuency	
	:AUTO	
	:OFFSet	<numeric_value>
	:SCALE	<numeric_value>
	:TIME	
	:AUTO	
	:OFFSet	<numeric_value>
	:OVERlap	<boolean>
	:SCALE	<numeric_value>

:DISPlay:SGRam:FREQuency:AUTO (No Query Form)

Rescales the horizontal axis automatically to fit the waveform to the screen in the spectrogram view.

Syntax :DISPlay:SGRam:FREQuency:AUTO

Arguments None

Measurement Views Spectrogram

Examples :DISPlay:SGRam:FREQuency:AUTO
rescales the horizontal scale automatically to fit the waveform to the screen.

:DISPlay:SGRam:FREQuency:OFFSet(?)

Sets or queries the frequency offset (the value at the center of the horizontal axis) in the spectrogram.

Syntax :DISPlay:SGRam:FREQuency:OFFSet <value>
 :DISPlay:SGRam:FREQuency:OFFSet?

Arguments <value>::=<NRf> specifies the frequency offset.
 Range: [(center frequency) - (X scale) × 0.9] to
 [(center frequency) + (X scale) × 0.9]

Measurement Views Spectrogram

Examples :DISPlay:SGRam:FREQuency:OFFSet 1.45GHz
 sets the frequency offset to 1.45 GHz in the spectrogram.

Related Commands :DISPlay:SGRam:FREQuency:SCAlE

:DISPlay:SGRam:FREQuency:SCAlE(?)

Sets or queries the horizontal range of the spectrogram.

Syntax :DISPlay:SGRam:FREQuency:SCAlE <value>
 :DISPlay:SGRam:FREQuency:SCAlE?

Arguments <value>::=<NRf> specifies the horizontal range.
 Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Spectrogram

Examples :DISPlay:SGRam:FREQuency:SCAlE 10MHz
 sets the horizontal range to 10 MHz.

Related Commands :DISPlay:SGRam:FREQuency:OFFSet

:DISPlay:SGRam:TIME:AUTO (No Query Form)

Rescales the vertical axis automatically to fit the graph to the screen in the spectrogram view.

Syntax :DISPlay:SGRam:TIME:AUTO

Arguments None

Measurement Views Spectrogram

Examples :DISPlay:SGRam:TIME:AUTO
rescales the vertical scale automatically to fit the waveform to the screen.

:DISPlay:SGRam:TIME:OFFSet(?)

Sets or queries the vertical axis (time) offset (bottom line number) in the spectrogram.

Syntax :DISPlay:SGRam:TIME:OFFSet <value>
:DISPlay:SGRam:TIME:OFFSet?

Arguments <value>::=<NRf> specifies the time offset.
Range: Line #0 to 125000. Zero (0) represents the latest line.

Measurement Views Spectrogram

Examples :DISPlay:SGRam:TIME:OFFSet 15
sets the time offset to Line #15.

Related Commands :DISPlay:SGRam:TIME:SCAlc

:DISPlay:SGRam:TIME:OVERlap(?)

Determines whether or not to allow overlap between adjacent FFT frames on the time axis in the spectrogram.

Syntax :DISPlay:SGRam:TIME:OVERlap { OFF | ON | 0 | 1 }
 :DISPlay:SGRam:TIME:OVERlap?

Arguments OFF or 0 inhibits overlap between adjacent FFT frames on the time axis.
 ON or 1 allows overlap between adjacent FFT frames on the time axis.

Measurement Views Spectrogram

Examples :DISPlay:SGRam:TIME:OVERlap ON
 allows overlap between adjacent FFT frames on the time axis in the spectrogram.

:DISPlay:SGRam:TIME:SCAle(?)

Sets or queries the vertical scale (the amount of time in each line) in the spectrogram. The vertical axis is composed of successive spectral displays. The new spectra can be added at a timed rate specified by this command. For example, if you set the scale to -5, one line is displayed every 5 spectra.

Syntax :DISPlay:SGRam:TIME:SCAle <value>
 :DISPlay:SGRam:TIME:SCAle?

Arguments <value>::=<NR1> specifies the vertical scale.
 Range: -1023 to 0. Zero (0) displays every spectrum.

Measurement Views Spectrogram

Examples :DISPlay:SGRam:TIME:SCAle -5
 displays one line every 5 spectra in the spectrogram.

Related Commands :DISPlay:SGRam:TIME:OFFSet

:DISPlay:SPECTrum Subgroup

The :DISPlay:SPECTrum commands control display of the spectrum view.

Command Tree	Header	Parameter
	:DISPlay	
	:SPECTrum	
	:MARKer	
	:NOISe	
	:MODE	<boolean>
	:WINDow	
	:TRACe	
	:GRATicule	
	:GRID	
	:STATe	<boolean>
	:Y	
	[:SCAlE]	
	:PDIVision	<numeric_value>

:DISPlay:SPECTrum:MARKer:NOISe:MODE(?)

Determines whether to enable or disable the marker noise mode in the spectrum view. In this mode, the marker readout indicates amplitude in dBm/Hz. It is valid for all markers except for the reference marker.

NOTE. To use the marker noise mode, select dBm as the power unit by the [:SENSe]:POWer:UNITs command.

Syntax :DISPlay:SPECTrum:MARKer:NOISe:MODE { OFF | ON | 0 | 1 }

:DISPlay:SPECTrum:MARKer:NOISe:MODE?

Arguments OFF or 0 disables the marker noise mode.

ON or 1 enables the marker noise mode.

Measurement Views Spectrum

Examples :DISPlay:SPECTrum:MARKer:NOISe:MODE ON
enables the marker noise mode.

Related Commands [:SENSe]:POWer:UNITs

:DISPlay:SPECTrum:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:SPECTrum:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }
 :DISPlay:SPECTrum:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views Spectrum

Examples :DISPlay:SPECTrum:WINDow:TRACe:GRATicule:GRID:STATe ON
 shows the graticule grid on the screen in the spectrum view.

:DISPlay:SPECTrum:Y[:SCALe]:PDIVision(?)

Sets or queries the vertical scale (per division) in the spectrum view.

Syntax :DISPlay:SPECTrum:Y[:SCALe]:PDIVision <value>
 :DISPlay:SPECTrum:Y[:SCALe]:PDIVision?

Arguments <value>::=<NRf> specifies the vertical scale (per division).
 Range: 0.01 to 20 dB/div.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:Y:SCALe:PDIVision 0.5
 sets the vertical scale to 0.5 dB/div.

Related Commands [:SENSe]:POWeR:UNITs

:DISPlay:TOVerview Subgroup

The :DISPlay:TOVerview commands control display of the time overview.

Command Tree	Header	Parameter
	:DISPlay	
	:TOVerview	
	:WINDow	
	:TRACe	
	:GRATicule	
	:GRID	
	:STATe	<boolean>
	:X	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>
	:Y	
	[:SCALe]	<numeric_value>
	:AUTO	
	:OFFSet	<numeric_value>
	:RESCale	

:DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe(?)

Determines whether to show or hide the graticule grid on the screen.

Syntax :DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe
 { OFF | ON | 0 | 1 }
 :DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe?

Arguments OFF or 0 hides the graticule grid.
 ON or 1 shows the graticule grid.

Measurement Views Time overview

Examples :DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe ON
 shows the graticule grid on the screen in the time overview.

:DISPlay:TOVerview:X[:SCALe](?)

Sets or queries the horizontal scale (full-scale time) of the time overview.

Syntax :DISPlay:TOVerview:X[:SCALe] <value>
 :DISPlay:TOVerview:X[:SCALe]?

Arguments <value>::=<NRf> specifies the horizontal scale in full-scale time.
 Range: 10 ns to the acquisition memory capacity.

 You can see the acquisition memory capacity using the [:SENSe]:ACQuisition
 :MEMory:CAPacity[:TIME]? query.

Measurement Views Time overview

Examples :DISPlay:TOVerview:X:SCALe 12.5us
 sets the horizontal scale to 12.5 μ s.

Related Commands :DISPlay:TOVerview:X[:SCALe]:OFFSet,
 [:SENSe]:ACQuisition:MEMory:CAPacity[:TIME]?

:DISPlay:TOVerview:X[:SCALe]:AUTO (No Query Form)

Sets the horizontal scale and offset automatically to fit the waveform to the screen in the time overview.

Syntax :DISPlay:TOVerview:X[:SCALe]:AUTO

Arguments None

Measurement Views Time overview

Examples :DISPlay:TOVerview:X:SCALe:AUTO
sets the horizontal scale and offset automatically to fit the waveform to the screen.

:DISPlay:TOVerview:X[:SCALe]:OFFSet(?)

Sets or queries the minimum horizontal value (left edge) of the time overview.

Syntax :DISPlay:TOVerview:X[:SCALe]:OFFSet <value>
:DISPlay:TOVerview:X[:SCALe]:OFFSet?

Arguments <value>::=<NRf> specifies the minimum horizontal value.
Range: [(analysis offset) - (X scale) × 0.9] to
[(analysis offset) + (analysis length) - (X scale) × 0.1]

Measurement Views Time overview

Examples :DISPlay:TOVerview:X:SCALe:OFFSet 800ns
sets the minimum horizontal value to 800 ns in the time overview.

Related Commands :DISPlay:TOVerview:X[:SCALe]

:DISPlay:TOVerview:Y[:SCALe](?)

Sets or queries the vertical range of the time overview.

Syntax :DISPlay:TOVerview:Y[:SCALe] <value>
 :DISPlay:TOVerview:Y[:SCALe]?

Arguments <value>::=<NRf> specifies the vertical range.
 Range: 0.1 to 200 dB.

Measurement Views Time overview

Examples :DISPlay:TOVerview:Y:SCALe 50
 sets the vertical range to 50 dBm in the time overview.

Related Commands :DISPlay:TOVerview:Y[:SCALe]:OFFSet

:DISPlay:TOVerview:Y[:SCALe]:AUTO (No Query Form)

Sets the vertical scale and offset automatically to fit the waveform to the screen in the time overview.

Syntax :DISPlay:TOVerview:Y[:SCALe]:AUTO

Arguments None

Measurement Views Time overview

Examples :DISPlay:TOVerview:Y:SCALe:AUTO
 sets the vertical scale and offset automatically to fit the waveform to the screen.

:DISPlay:TOVerview:Y[:SCALe]:OFFSet(?)

Sets or queries the vertical offset (the value at the top edge of the vertical axis) in the time overview.

Syntax :DISPlay:TOVerview:Y[:SCALe]:OFFSet <value>
 :DISPlay:TOVerview:Y[:SCALe]:OFFSet

Arguments <value>::=<NRf> specifies the vertical offset.
 Range: -170 to +50 dBm.

Measurement Views Time overview

Examples :DISPlay:TOVerview:Y:SCALe:OFFSet -80
 sets the vertical offset to -80 dBm in the time overview.

Related Commands :DISPlay:TOVerview:Y[:SCALe]

:DISPlay:TOVerview:Y[:SCALe]:RESCale (No Query Form)

Sets the vertical scale automatically to fit the waveform to the screen in the time overview.

Syntax :DISPlay:TOVerview:Y[:SCALe]:RESCale

Arguments None

Measurement Views Time overview

Examples :DISPlay:TOVerview:Y:SCALe:RESCale
 sets the vertical scale automatically to fit the waveform to the screen.

FETCh Commands

The FETCh commands retrieve the measurements from the data taken by the latest INITiate command.

To perform a FETCh operation on fresh data, use the :READ commands on page 2-473. The :READ commands acquire a new input signal and fetch the measurement results from that data.

The FETCh commands are divided by measurement views into the subgroups listed in Table 2-36.

Table 2-36: FETCh command subgroups

Command header	Measurement view	Refer to:
:FETCh (basic)	All views, general fetch control	page 2-324
:FETCh:ACPower	Channel power and ACPR	page 2-329
:FETCh:AVTime	Amplitude versus Time	page 2-332
:FETCh:CCDF	CCDF	page 2-337
:FETCh:CONSte	Constellation (Option 21 only)	page 2-340
:FETCh:DDEMod	General purpose digital modulation measurements (Option 21 only)	page 2-342
:FETCh:DPSA	DPX (Digital Phosphor) spectrum	page 2-344
:FETCh:EVM	EVM versus Time (Option 21 only)	page 2-348
:FETCh:FVTime	Frequency versus Time	page 2-351
:FETCh:IQVTime	RF I&Q versus Time	page 2-355
:FETCh:MCPower	MCPR (Multiple Carrier Power Ratio)	page 2-360
:FETCh:MERRor	Magnitude error versus Time (Option 21 only)	page 2-365
:FETCh:OBW	OBW (Occupied Bandwidth)	page 2-368
:FETCh:PERRor	Phase error versus Time (Option 21 only)	page 2-377
:FETCh:PHVTime	Phase versus Time	page 2-380
:FETCh:PULSe	Pulsed RF measurements (Option 20 only)	page 2-384
:FETCh:SGRam	Spectrogram	page 2-423
:FETCh:SPECTrum	Spectrum	page 2-424
:FETCh:SQUality	Signal quality (Option 21 only)	page 2-426
:FETCh:TOVerview	Time overview	page 2-437

:FETCh Basic Command Subgroup

The :FETCh basic commands returns information on acquisition data.

Command Tree	Header	Parameter
	:FETCh	
	:RFIN?	
	:IQ?	<RecordID>,[<NumericDT0>,<NumericDT0>]
	:HEADer?	<RecordID>
	:SCALe?	
	:Record	
	:IDS?	

:FETCh:RFIN:IQ? (Query Only)

Returns time-domain IQ data for a specific acquisition data record. You can set a range of IQ pairs optionally. The instrument needs to be in stopped mode. If not in stopped mode, it returns the execution error (-200).

Syntax :FETCh:RFIN:IQ? <rec_ID>[,<begin_num>,<end_num>]

Arguments <rec_ID> specifies the acquisition data record ID number.
 <begin_num> specifies the beginning number of IQ pairs.
 <end_num> specifies the end number of IQ pairs.

Use the :FETCh:RFIN:RECOrd:IDS? query to get the beginning and end ID's of acquisition data records.

Returns #<num_digit><num_byte><I(1)><Q(1)><I(2)><Q(2)>...<I(n)><Q(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<I(n)> and <Q(n)> are the time-domain IQ data pair.

4-byte little endian floating-point format specified in IEEE 488.2.

To find out the range of IQ pairs, use the :FETCh:RFIN:IQ:HEADer? query. The returned value of <num_sample> is the number of IQ pairs.

NOTE. Do not fetch a large number of IQ pairs because of memory limitation.

Measurement Views All

Examples :FETCh:RFIN:IQ? 10,25,350
 might return #43848xxxx... (3848-byte data) for the record #10, ranging from 25th to 350th IQ pair.

Related Commands :FETCh:RFIN:IQ:HEADer?, :FETCh:RFIN:RECOrd:IDS?

:FETCh:RFIN:IQ:HEADer? (Query Only)

Returns the header information for a specific acquisition data record.
The instrument needs to be in stopped mode. If not in stopped mode, it returns the execution error (-200).

Syntax :FETCh:RFIN:IQ:HEADer? <rec_ID>

Arguments <rec_ID> specifies the acquisition data record ID number.

Use the :FETCh:RFIN:RECORD:IDS? query to get the beginning and end ID's of acquisition data records.

Returns ,<sampling_freq>,<num_sample>,<center_freq>,<acq_BW>,
 <ref_level>,<trig_pos>,<time_stamp>,<FastFrame_ID>

Where

::=<NR3> is the span in Hz.

<sampling_freq>::=<NR3> is the sampling frequency in Hz.

<num_sample>::=<NR3> is the number of samples.

<center_freq>::=<NR3> is the center frequency in Hz.

<acq_BW>::=<NR3> is the acquisition bandwidth in Hz.

<ref_level>::=<NR3> is the reference level in dBm.

<trig_pos>::=<NR3> is the trigger position in seconds.

<time_stamp>::=<string> is the time stamp.

<FastFrame_ID>::=<NR1> is the Fast Frame ID: Zero or positive number.

If the Fast Frame is disabled, the ID will be negative.

Measurement Views All

Examples :FETCh:RFIN:IQ:HEADer? 10
might return 40.0E+6,50.0E+6,4.027E+3,1.5E+9,40.0E+6,0.0,20.242E-6,
"10/31/2007 11:18:32 AM",-1, indicating
 Span: 40 MHz
 Sampling frequency: 50 MHz
 Number of samples: 4027
 Center frequency: 1.5 GHz
 Acquisition bandwidth: 40 MHz
 Reference level: 0 dBm
 Trigger position: 20.242 μ s
 Time stamp: 10/31/2007 11:18:32 AM
 Fast Frame ID: -1

Related Commands :FETCh:RFIN:RECORD:IDS?

:FETCh:RFIN:IQ:SCALE? (Query Only)

Returns the internal RF linear data scaling factor contained in the .tiq file header. The scaling factor can be used to convert digital IQ output (Option 05) values into real IQ values.

Syntax :FETCh:RFIN:IQ:SCALE?

Arguments None

Returns <NR3> The RF linear data scaling factor.

Measurement Views All

Examples : FETCh:RFIN:IQ:SCALE?
might return 19.553E-6 for the scaling factor.

Related Commands :FETCh:RFIN:RECOrd:IDS?

:FETCh:RFIN:RECORD:IDS? (Query Only)

Returns the beginning and end ID numbers of acquisition data.
The instrument needs to be in stopped mode. If not in stopped mode, it returns the execution error (-200).

Syntax :FETCh:RFIN:RECORD:IDS?

Arguments None

Returns <begin_ID>,<end_ID>

Where
<begin_ID>::=<NR1> is the beginning ID of acquisition data.
<end_ID>::=<NR1> is the end ID of acquisition data.

Measurement Views All

Examples :FETCh:RFIN:RECORD:IDS?
might return 1,147 indicating the beginning and end ID's of acquisition data are 1 and 147, respectively.

:FETCh:ACPower Subgroup

The :FETCh:ACPower commands returns the results of the Channel power and ACPR (Adjacent Channel Power Ratio) measurement.

Command Tree	Header	Parameter
	:FETCh	
	:ACPower?	
	:CHANnel	
	:POWer?	
	:SPECTrum?	

:FETCh:ACPower? (Query Only)

Returns the Channel power and ACPR measurement results for all available channels.

Syntax :FETCh:ACPower?

Arguments None

Returns <chan_power>,<acpr_lower(1)>,<acpr_upper(1)>,
 <acpr_lower(2)>,<acpr_upper(2)>,...
 <acpr_lower(n)>,<acpr_upper(n)>

Where

<chan_power> is the average power of the main channel as the power reference in dBm.

<acpr_lower(n)> is the ACPR for the lower channel #n in dB.

<acpr_upper(n)> is the ACPR for the upper channel #n in dB.

The number of n depends on the setting of the [:SENSe]:ACPower:CHANnel:PAIRs command.

Measurement Views Channel power and ACPR

Examples :FETCh:ACPower?
might return 4.227,-28.420,-23.847,-22.316,-29.225 indicating
(average power of the main channel) = 4.227 dBm,
(ACPR for the lower channel 1) = -28.420 dB,
(ACPR for the upper channel 1) = -23.847 dB,
(ACPR for the lower channel 2) = -22.316 dB, and
(ACPR for the upper channel 2) = -29.225 dB.

Related Commands [:SENSe]:ACPower:CHANnel:PAIRs

:FETCh:ACPower:CHANnel:POWer? (Query Only)

Returns the average power of the main channel (power reference) in the Channel power and ACPR measurement.

Syntax :FETCh:ACPower:CHANnel:POWer?

Arguments None

Returns <chan_power>::=<NRf> is the average power of the main channel in dBm.

Measurement Views Channel power and ACPR

Examples :FETCh:ACPower:CHANnel:POWer?
might return 4.227 indicating that the average power of the main channel is 4.227 dBm.

:FETCh:ACPower:SPECTrum? (Query Only)

Returns spectrum trace data of the Channel power and ACPR measurement.

Syntax :FETCh:ACPower:SPECTrum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Channel power and ACPR

Examples :FETCh:ACPower:SPECTrum?
might return #43204xxxx... (3204-byte data) for the spectrum trace data of the Channel power and ACPR measurement.

:FETCh:AVTime Subgroup

The :FETCh:AVTime commands returns the results of the Amplitude versus Time measurement.

Command Tree	Header	Parameter
	:FETCh	
	:AVTime	
	:AVERage?	
	:FIRSt :SECond :THIRd :FOURth	
	:MAXimum?	
	:MAXLocation?	
	:MINimum?	
	:MINLocation?	
	:RESult?	

NOTE. Except for the :FETCh:AVTime:FIRSt|:SECond|:THIRd|:FOURth command, select the trace using the :TRACe<x>:AVTime:SElect command.

The unit of amplitude is defaulted to dBm. It can be changed by the [:SENSe]:POWer:UNITs command.

:FETCh:AVTime:AVERage? (Query Only)

Returns the RMS (root-mean-square) value for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax	:FETCh:AVTime:AVERage?
Arguments	None
Returns	<avg>::=<NRf> is the RMS amplitude in dBm.
Measurement Views	Amplitude versus Time
Examples	:FETCh:AVTime:AVERage? might return -2.53 indicating the RMS amplitude is -2.53 dBm.
Related Commands	:TRACe<x>:AVTime:SElect

:FETCh:AVTime:FIRSt|:SECond|:THIRd|:FOURth? (Query Only)

Returns the trace data in the Amplitude versus Time measurement.

Syntax :FETCh:AVTime:FIRSt|:SECond|:THIRd|:FOURth?

Where FIRSt, SECond, THIRd, and FOURth represent Trace 1 to 4, respectively. Each trace is defined as follows:

FIRSt: Trace 1
 SECond: Trace 2
 THIRd: Trace 3
 FOURth: Math trace

The traces can be specified by the :TRACe<x>:AVTime command subgroup.

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where
 <num_digit> is the number of digits in <num_byte>.
 <num_byte> is the number of bytes of data that follow.
 <data(n)> is the amplitude in dBm for the point #n,
 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Amplitude versus Time

Examples :FETCh:AVTime:FIRSt?
 might return #3156xxxx... (156-byte data) for Trace 1.

Related Commands :TRACe<x>:AVTime command subgroup

:FETCh:AVTime:MAXimum? (Query Only)

Returns the maximum value for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :FETCh:AVTime:MAXimum?

Arguments None

Returns <max>::=<NRf> is the maximum Amplitude in dBm.

Measurement Views Amplitude versus Time

Examples :FETCh:AVTime:MAXimum?
might return -2.84 indicating the maximum amplitude is -2.84 dBm.

Related Commands :FETCh:AVTime:MAXLocation?, :TRACe<x>:AVTime:SElect

:FETCh:AVTime:MAXLocation? (Query Only)

Returns the time at which the amplitude is maximum for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :FETCh:AVTime:MAXLocation?

Arguments None

Returns <max_time>::=<NRf> is the time at the maximum in seconds.

Measurement Views Amplitude versus Time

Examples :FETCh:AVTime:MAXLocation?
might return 25.03E-9 indicating the amplitude is maximum at 25.03 ns.

Related Commands :FETCh:AVTime:MAX?, :TRACe<x>:AVTime:SElect

:FETCh:AVTime:MINimum? (Query Only)

Returns the minimum value for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :FETCh:AVTime:MINimum?

Arguments None

Returns <min>::=<NRf> is the minimum amplitude in dBm.

Measurement Views Amplitude versus Time

Examples :FETCh:AVTime:MINimum?
might return -57.64 indicating the minimum amplitude is -57.64 dBm.

Related Commands :FETCh:AVTime:MINLocation?, :TRACe<x>:AVTime:SElect

:FETCh:AVTime:MINLocation? (Query Only)

Returns the time at which the amplitude is minimum for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :FETCh:AVTime:MINLocation?

Arguments None

Returns <min_time>::=<NRf> is the time at the minimum in seconds.

Measurement Views Amplitude versus Time

Examples :FETCh:AVTime:MINLocation?
might return 450.7E-9 indicating the amplitude is minimum at 450.7 ns.

Related Commands :FETCh:AVTime:MIN?, :TRACe<x>:AVTime:SElect

:FETCh:AVTime:RESult? (Query Only)

Returns the measurement results for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :FETCh:AVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>,<rms>

Where

<max>::=<NRf> is the maximum amplitude in dBm.

<max_time>::=<NRf> is the time at the maximum in seconds.

<min>::=<NRf> is the minimum amplitude in dBm.

<min_time>::=<NRf> is the time at the minimum in seconds.

<rms>::=<NRf> is the RMS amplitude in dBm.

Measurement Views Amplitude versus Time

Examples :FETCh:AVTime:RESult?
might return -2.68,48.62E-6,-82.47,22.11E-6,-8.24 indicating that
the maximum amplitude is -2.68 dBm at 48.62 μ s,
the minimum amplitude is -82.47 dBm at 22.11 μ s, and
the RMS amplitude is -8.24 dBm

Related Commands :TRACe:AVTime:SElect

:FETCh:CCDF Subgroup

The :FETCh:CCDF commands returns the results of the CCDF (Complementary Cumulative Distribution Function) measurement.

Command Tree	Header	Parameter
	:FETCh	
	:CCDF?	
	:FIRSt :SECond :THIRd?	

:FETCh:CCDF? (Query Only)

Returns the CCDF measurement results.

Syntax :FETCh:CCDF?

Arguments None

Returns <avg_amp1>,<avg_ccdf>,<crest_factor>,<amp1_10>,<amp1_1>,<amp1_p1>,<amp1_p01>,<amp1_p001>,<amp1_p0001>

Where

<avg_amp1> is the average amplitude in dBm.

(The unit can be changed by the [:SENSe]:POWer:UNITs command.)

<avg_ccdf> is the average CCDF in percent.

<crest_factor> is the crest factor in dB.

<amp1_10> is the amplitude at CCDF of 10% in dB.

<amp1_1> is the amplitude at CCDF of 1% in dB.

<amp1_p1> is the amplitude at CCDF of 0.1% in dB.

<amp1_p01> is the amplitude at CCDF of 0.01% in dB.

<amp1_p001> is the amplitude at CCDF of 0.001% in dB.

<amp1_p0001> is the amplitude at CCDF of 0.0001% in dB.

Measurement Views CCDF

Examples :FETCh:CCDF?
might return -33.35,35.8,9.75,3.88,7.07,8.50,9.25,9.72,9.74
indicating
(average amplitude) = -33.35 dBm,
(average CCDF) = 35.8%,
(crest factor) = 9.75 dB,
(amplitude at CCDF of 10%) = 3.88 dB,
(amplitude at CCDF of 1%) = 7.07 dB,
(amplitude at CCDF of 0.1%) = 8.50 dB,
(amplitude at CCDF of 0.01%) = 9.25 dB,
(amplitude at CCDF of 0.001%) = 9.72 dB, and
(amplitude at CCDF of 0.0001%) = 9.74 dB.

Related Commands [:SENSe]:POWer:UNITs

:FETCh:CCDF:FIRSt|:SECond|:THIRd? (Query Only)

Returns waveform data of the specified trace in the CCDF measurement.

Syntax :FETCh:CCDF:FIRSt|:SECond|:THIRd?

Where FIRSt, SECond, and THIRd represent Trace 1 to 3, respectively.
Each trace is defined as follows:

FIRSt:	Trace 1
SECond:	Trace 2
THIRd:	Gaussian reference curve

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the CCDF value of the specified trace for the point #n in percent,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views CCDF

Examples :FETCh:CCDF:FIRSt?
might return #41024xxxx... (1024-byte data) for the waveform data of Trace 1.

Related Commands [:SENSe]:CCDF:TIME:TYPE

:FETCh:CONSte Subgroup (Option 21 Only)

The :FETCh:CONSte commands returns the results of the Constellation measurement.

Command Tree	Header	Parameter
	:FETCh	
	:CONSte	
	:RESuLts?	
	:TRACe?	

:FETCh:CONSte:RESuLts? (Query Only)

Returns the constellation measurement results of EVM RMS, peak and location displayed on the bottom of the screen.

Syntax :FETCh:CONSte:RESuLts?

Arguments None

Returns <EVM_RMS>,<EVM_peak>,<location>

Where
<EVM_RMS>::=<NRf> is the RMS EVM in percent (%).
<EVM_peak>::=<NRf> is the peak EVM in percent (%).
<location>::=<NRf> is the peak location in symbol number.

Measurement Views Constellation

Examples :FETCh:CONSte:RESuLts?
might return 2.841,3.227,68.000, indicating that the RMS EVM is 2.841% and the peak EVM is 3.227% at symbol #68.

:FETCh:CONSt:TRACe? (Query Only)

Returns the constellation trace data.

Syntax :FETCh:CONSt:TRACe?

Arguments None

Returns #<num_digit><num_byte><I(1)><Q(1)><I(2)><Q(2)>...<I(n)><Q(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<I(n)> and <Q(n)> are the normalized I- and Q-coordinate values at the n^{th} data point. 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Constellation

Examples :FETCh:CONSt:TRACe?
might return #43848xxxx... (3848-byte data) for the constellation trace data.

:FETCh:DDEMod Subgroup (Option 21 Only)

The :FETCh:DDEMod commands returns the results of the General Purpose Digital Modulation measurements.

Command Tree	Header	Parameter
	:FETCh	
	:DDEMod	
	:STABLe?	
	:SYNCh	
	:WORD	
	:LENGth?	
	:POSition?	

:FETCh:DDEMod:STABLe? (Query Only)

Returns the symbol table data.

Syntax :FETCh:DDEMod:STABLe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where
<num_digit> is the number of digits in <num_byte>.
<num_byte> is the number of bytes of data that follow.
<data(n)> is the symbol table data for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Symbol table

Examples :FETCh:DDEMod:STABLe?
might return #3512xxxx... (512-byte data) for the symbol table.

:FETCh:DDEMod:SYNCh:WORD:LENGth? (Query Only)

Returns the length of the synch word in the symbol table.

Syntax :FETCh:DDEMod:SYNCh:WORD:LENGth?

Arguments None

Returns <NR1> indicates the length of the synch word in symbols.

Measurement Views Symbol table

Examples :FETCh:DDEMod:SYNCh:WORD:LENGth?
might return 3, indicating the length of the synch word is three symbols.

Related Commands :FETCh:DDEMod:SYNCh:WORD:POSition?

:FETCh:DDEMod:SYNCh:WORD:POSition? (Query Only)

Returns the position of the synch word in the symbol table.

Syntax :FETCh:DDEMod:SYNCh:WORD:POSition?

Arguments None

Returns <NR1> indicates what symbol number the synch word begins at in the table.
Zero (0) represents the first symbol in the table.

Measurement Views Symbol table

Examples :FETCh:DDEMod:SYNCh:WORD:POSition?
might return 10, indicating the synch word begins at 11th symbol in the table.

Related Commands :FETCh:DDEMod:SYNCh:WORD:LENGth?

:FETCh:DPSA Subgroup

The :FETCh:DPSA commands returns the results of the DPX (Digital Phosphor) Spectrum measurement.

Command Tree	Header	Parameter
	:FETCh	
	:DPSA	
	:TRACe	
	:AVERage?	
	:MATH?	
	:MAXimum?	
	:MINimum?	

:FETCh:DPSA:TRACe:AVERage? (Query Only)

Returns waveform data of the average trace in the DPX spectrum measurement.

Syntax :FETCh:DPSA:TRACe:AVERage?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude of the average trace for the point #n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views DPX spectrum

Examples :FETCh:DPSA:TRACe:AVERage?
might return #42004xxxx... (2004-byte data) for the waveform data of the average trace.

:FETCh:DPSA:TRACe:MATH? (Query Only)

Returns waveform data of the math trace in the DPX spectrum measurement.

Syntax :FETCh:DPSA:TRACe:MATH?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude of the math trace for the point #n in dBm,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views DPX spectrum

Examples :FETCh:DPSA:TRACe:MATH?
might return #42004xxxx... (2004-byte data) for the waveform data of the math trace.

:FETCh:DPSA:TRACe:MAXimum? (Query Only)

Returns waveform data of the maximum trace in the DPX spectrum measurement.

Syntax :FETCh:DPSA:TRACe:MAXimum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude of the maximum trace for the point #n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views DPX spectrum

Examples :FETCh:DPSA:TRACe:MAXimum?
might return #42004xxxx... (2004-byte data) for the waveform data of the maximum trace.

:FETCh:DPSA:TRACe:MINimum? (Query Only)

Returns waveform data of the minimum trace in the DPX spectrum measurement.

Syntax :FETCh:DPSA:TRACe:MINimum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude data of the minimum trace for the point #n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views DPX spectrum

Examples :FETCh:DPSA:TRACe:MINimum?
might return #42004xxxx... (2004-byte data) for the waveform data of the minimum trace.

:FETCh:EVM Subgroup (Option 21 Only)

The :FETCh:EVM commands returns the results of the EVM (Error Vector Magnitude) versus Time measurement.

Command Tree	Header	Parameter
	:FETCh	
	:EVM	
		:FERRor?
		:PEAK?
		:PINDeX?
		:RMS?
		:TRACe?

:FETCh:EVM:FERRor? (Query Only)

Returns the frequency error in the EVM versus Time measurement.

Syntax :FETCh:EVM:FERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Measurement Views EVM versus Time

Examples :FETCh:EVM:FERRor?
might return -10.7E+3 indicating the frequency error is -10.7 kHz.

:FETCh:EVM:PEAK? (Query Only)

Returns the peak value in the EVM versus Time measurement.

Syntax :FETCh:EVM:PEAK?

Arguments None

Returns <peak>::=<NRf> is the peak EVM value in percent (%).

Measurement Views EVM versus Time

Examples :FETCh:EVM:PEAK?
might return 1.32 indicating the peak EVM value is 1.32%.

Related Commands :FETCh:EVM:PINDeX?

:FETCh:EVM:PINDeX? (Query Only)

Returns the time at the EVM peak.

Syntax :FETCh:EVM:PINDeX?

Arguments None

Returns <peak_time>::=<NRf> is the time at the EVM peak in seconds.

You can select the time unit using the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views EVM versus Time

Examples :FETCh:EVM:PINDeX?
might return 28.912E-6 indicating the time at the EVM peak is 28.912 μ s.

Related Commands :FETCh:EVM:PEAK?, [:SENSe]:DDEMod:TIME:UNITs

:FETCh:EVM:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the EVM versus Time measurement.

Syntax :FETCh:EVM:RMS?

Arguments None

Returns <rms>::=<NRf> is the RMS EVM value in percent (%).

Measurement Views EVM versus Time

Examples :FETCh:EVM:RMS?
might return 0.582 indicating the RMS EVM value is 0.582%.

:FETCh:EVM:TRACe? (Query Only)

Returns the EVM versus Time trace data.

Syntax :FETCh:EVM:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the EVM value for the point #n in percent (%),

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views EVM versus Time

Examples :FETCh:EVM:TRACe?
might return #42036xxxx... (2036-byte data) for the EVM versus Time trace.

:FETCh:FVTime Subgroup

The :FETCh:EVM commands returns the results of the Frequency versus Time measurement.

Command Tree	Header	Parameter
	:FETCh	
	:FVTime?	
	:MAXimum?	
	:MAXLocation?	
	:MINimum?	
	:MINLocation?	
	:RESult?	

:FETCh:FVTime? (Query Only)

Returns the Frequency versus Time trace data.

Syntax :FETCh:FVTime?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the frequency in Hz for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Frequency versus Time

Examples :FETCh:FVTime?
might return #3156xxxx... (156-byte data) for the Frequency versus Time trace.

:FETCh:FVTime:MAXimum? (Query Only)

Returns the maximum value in the Frequency versus Time measurement.

Syntax :FETCh:FVTime:MAXimum?

Arguments None

Returns <max>::=<NRf> is the maximum frequency drift in Hz.

Measurement Views Frequency versus Time

Examples :FETCh:FVTime:MAXimum?
might return 2.625E+6 indicating the maximum frequency drift is 2.625 MHz.

Related Commands :FETCh:FVTime:MAXLocation?

:FETCh:FVTime:MAXLocation? (Query Only)

Returns the time at which the frequency drift is maximum.

Syntax :FETCh:FVTime:MAXLocation?

Arguments None

Returns <max_time>::=<NRf> is the time in seconds at which the frequency drift is maximum.

Measurement Views Frequency versus Time

Examples :FETCh:FVTime:MAXLocation?
might return 25.03E-9 indicating the frequency drift is maximum at 25.03 ns.

Related Commands :FETCh:FVTime:MAXimum?

:FETCh:FVTime:MINimum? (Query Only)

Returns the minimum value in the Frequency versus Time measurement.

Syntax :FETCh:FVTime:MINimum?

Arguments None

Returns <min>::=<NRf> is the minimum frequency drift in Hz.

Measurement Views Frequency versus Time

Examples :FETCh:FVTime:MINimum?
might return -6.618E+6 indicating the minimum frequency drift is -6.618 MHz.

Related Commands :FETCh:FVTime:MINLocation?

:FETCh:FVTime:MINLocation? (Query Only)

Returns the time at which the frequency drift is minimum.

Syntax :FETCh:FVTime:MINLocation?

Arguments None

Returns <min_time>::=<NRf> is the time in seconds at which the frequency drift is minimum.

Measurement Views Frequency versus Time

Examples :FETCh:FVTime:MAXLocation?
might return 450.7E-9 indicating the frequency drift is minimum at 450.7 ns.

Related Commands :FETCh:FVTime:MINimum?

:FETCh:FVTime:RESult? (Query Only)

Returns the Frequency versus Time measurement results.

Syntax :FETCh:FVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>

Where

<max>::=<NRf> is the maximum frequency drift in Hz.

<max_time>::=<NRf> is the time in seconds at which the frequency drift is maximum.

<min>::=<NRf> is the minimum frequency drift in Hz.

<min_time>::=<NRf> is the time in seconds at which the frequency drift is minimum.

Measurement Views Frequency versus Time

Examples :FETCh:FVTime:RESult?
might return 2.625E+6,25.03E-9,-6.618E+6,450.7E-9 indicating:
the maximum frequency drift is 2.625 MHz at 25.03 ns and
the minimum frequency drift is -6.618 MHz at 450.7 ns.

:FETCh:IQVTime Subgroup

The :FETCh:IQVTime commands returns the results of the RF I&Q versus Time measurement.

Command Tree	Header	Parameter
	:FETCh	
	:IQVTime	
	:I?	
	:MAXimum?	
	:MAXLocation?	
	:MINimum?	
	:MINLocation?	
	:Q?	
	:RESult?	

:FETCh:IQVTime:I? (Query Only)

Returns the I versus Time trace data.

Syntax :FETCh:IQVTime:I?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the I level in volts for the point #n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views RF I&Q versus Time

Examples :FETCh:IQVTime:I?
might return #3160xxxx... (160-byte data) for the I versus Time trace.

:FETCh:IQVTime:MAXimum? (Query Only)

Returns the maximum value in the RF I&Q versus Time measurement.

Syntax :FETCh:IQVTime:MAXimum?

Arguments None

Returns <max>::=<NRf> is the maximum I or Q level in volts.
Use the [:SENSe]:IQVTime:TRACe:SElect:I or Q command to select the trace.

Measurement Views RF I&Q versus Time

Examples :FETCh:IQVTime:MAXimum?
might return 1.214 indicating the maximum I or Q level is 1.214 V.

Related Commands :FETCh:IQVTime:MAXLocation?,
[:SENSe]:IQVTime:TRACe:SElect:I, [:SENSe]:IQVTime:TRACe:SElect:Q

:FETCh:IQVTime:MAXLocation? (Query Only)

Returns the time at which the I or Q level is maximum.

Syntax :FETCh:IQVTime:MAXLocation?

Arguments None

Returns <max_time>::=<NRf> is the time in seconds at which the I or Q level is maximum.

Measurement Views RF I&Q versus Time

Examples :FETCh:IQVTime:MAXLocation?
might return 175.3E-9 indicating the I or Q level is maximum at 175.3 ns.

Related Commands :FETCh:IQVTime:MAXimum?

:FETCh:IQVTime:MINimum? (Query Only)

Returns the minimum value in the RF I&Q versus Time measurement.

Syntax :FETCh:IQVTime:MINimum?

Arguments None

Returns <min>::=<NRf> is the minimum I or Q level in volts.
Use the [:SENSe]:IQVTime:TRACe:SElect:I or Q command to select the trace.

Measurement Views RF I&Q versus Time

Examples :FETCh:IQVTime:MINimum?
might return -370.5E-3 indicating the minimum I or Q level is -370.5 mV.

Related Commands :FETCh:IQVTime:MINLocation?,
[:SENSe]:IQVTime:TRACe:SElect:I, [:SENSe]:IQVTime:TRACe:SElect:Q

:FETCh:IQVTime:MINLocation? (Query Only)

Returns the time at which the I or Q level is minimum.

Syntax :FETCh:IQVTime:MINLocation?

Arguments None

Returns <min_time>::=<NRf> is the time in seconds at which the I or Q level is minimum.

Measurement Views RF I&Q versus Time

Examples :FETCh:IQVTime:MAXLocation?
might return 450.7E-9 indicating the I or Q level is minimum at 450.7 ns.

Related Commands :FETCh:IQVTime:MINimum?

:FETCh:IQVTime:Q? (Query Only)

Returns the Q versus Time trace data.

Syntax :FETCh:IQVTime:Q?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the Q level in volts for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views RF I&Q versus Time

Examples :FETCh:IQVTime:Q?
might return #3160xxxx... (160-byte data) for the Q versus Time trace.

:FETCh:IQVTime:RESult? (Query Only)

Returns the RF I&Q versus Time measurement results.

Syntax :FETCh:IQVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>

Where

<max>::=<NRf> is the maximum I or Q level in volts.

<max_time>::=<NRf> is the time in seconds at which the I or Q level is maximum.

<min>::=<NRf> is the minimum I or Q level in volts.

<min_time>::=<NRf> is the time in seconds at which the I or Q level is minimum.

Use the [:SENSe]:IQVTime:TRACe:SElect:I or Q command to select the trace.

Measurement Views RF I&Q versus Time

Examples :FETCh:IQVTime:RESult?
might return 1.214,175.3E-9,-370.5E-3,450.7E-9 indicating:
the maximum I or Q level is 1.214 V at 175.3 ns and
the minimum I or Q level is -370.5 mV at 450.7 ns.

Related Commands [:SENSe]:IQVTime:TRACe:SElect:I, [:SENSe]:IQVTime:TRACe:SElect:Q

:FETCh:MCPower Subgroup

The :FETCh:MCPower commands returns the results of the MCPR (Multiple Carrier Power Ratio) measurement.

Command Tree	Header	Parameter
	:FETCh	
	:MCPower	
	:ADJacent	
	:CHANnels?	
	:CHANnel	
	:POWer?	
	:MAIN	
	:CHANnels?	
	:SPECTrum?	

:FETCh:MCPower:ADJacent:CHANnels? (Query Only)

Returns the power of adjacent channels in order of increasing frequency.

Syntax :FETCh:MCPower:ADJacent:CHANnels?

Arguments None

Returns <acpr_lower(n)>,...<acpr_lower(2)>,<acpr_lower(1)>,
<acpr_upper(1)>,<acpr_upper(2)>,...<acpr_upper(n)>

Where

<acpr_lower(n)> is the ACPR for the lower channel #n in dB.

<acpr_upper(n)> is the ACPR for the upper channel #n in dB.

To add a pair of upper and lower adjacent channels, use the [:SENSe]
:MCPower:CHANnel:ADD:ADJacent command.

Measurement Views MCPR

Examples :FETCh:MCPower:ADJacent:CHANnels?
might return -4.420,-4.847,-4.316,-4.225 indicating
(ACPR for the lower channel 2) = -4.420 dB,
(ACPR for the lower channel 1) = -4.847 dB,
(ACPR for the upper channel 1) = -4.316 dB, and
(ACPR for the upper channel 2) = -4.225 dB.

Related Commands [:SENSe]:MCPower:CHANnel:ADD:ADJacent

:FETCh:MCPower:CHANnel:POWer? (Query Only)

Returns the reference power in the MCPR measurement.

Syntax :FETCh:MCPower:CHANnel:POWer?

Arguments None

Returns <ref_power>::<NRf> is the reference power in dBm.
To select the power reference, use the [:SENSe]:MCPower:RCHannels commands.

Measurement Views MCPR

Examples :FETCh:MCPower:CHANnel:POWer?
might return 4.227 indicating that the reference power is 4.227 dBm.

Related Commands [:SENSe]:MCPower:RCHannels commands

:FETCh:MCPower:MAIN:CHANnels? (Query Only)

Returns the power of main channels in order of increasing frequency.

Syntax :FETCh:MCPower:MAIN:CHANnels?

Arguments None

Returns <power_main(1)>,<power_main(2)>,...<power_main(n)>

Where

<power_main(n)> is the power of main channel #n in dBm.

To specify the main channels, use the [:SENSe]:MCPower:CHANnel:MAIN commands.

Measurement Views MCPR

Examples :FETCh:MCPower:MAIN:CHANnels?
might return -2.420,-2.847,-2.316,-2.225 indicating
(power of the main channel 1) = -2.420 dBm,
(power of the main channel 2) = -2.847 dBm,
(power of the main channel 3) = -2.316 dBm, and
(power of the main channel 4) = -2.225 dBm.

Related Commands [:SENSe]:MCPower:CHANnel:MAIN commands

:FETCh:MCPower:SPECTrum? (Query Only)

Returns spectrum trace data of the MCPR measurement.

Syntax :FETCh:MCPower:SPECTrum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views MCPR

Examples :FETCh:MCPower:SPECTrum?
might return #43204xxxx... (3204-byte data) for the spectrum trace data of the MCPR measurement.

:FETCh:MERRor Subgroup (Option 21 Only)

The :FETCh:MERRor commands returns the results of the Magnitude error versus Time measurement.

Command Tree	Header	Parameter
	:FETCh	
	:MERRor	
	:FERRor?	
	:PEAK?	
	:PINdex?	
	:RMS?	
	:TRACe?	

:FETCh:MERRor:FERRor? (Query Only)

Returns the frequency error in the Magnitude error versus Time measurement.

Syntax :FETCh:MERRor:FERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Measurement Views Magnitude error versus Time

Examples :FETCh:MERRor:FERRor?
might return -10.7E+3 indicating the frequency error is -10.7 kHz.

:FETCh:MERRor:PEAK? (Query Only)

Returns the peak value in the Magnitude error versus Time measurement.

Syntax :FETCh:MERRor:PEAK?

Arguments None

Returns <peak>::=<NRf> is the peak magnitude error in percent (%).

Measurement Views Magnitude error versus Time

Examples :FETCh:MERRor:PEAK?
might return 1.57 indicating the peak magnitude error is 1.57%.

Related Commands :FETCh:MERRor:PINDeX?

:FETCh:MERRor:PINDeX? (Query Only)

Returns the time at the magnitude error peak.

Syntax :FETCh:MERRor:PINDeX?

Arguments None

Returns <peak_time>::=<NRf> is the time at the magnitude error peak in seconds.
You can select the time unit using the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Magnitude error versus Time

Examples :FETCh:MERRor:PINDeX?
might return 28.912E-6 indicating the time at the magnitude error peak is 28.912 μ s.

Related Commands :FETCh:MERRor:PEAK?, [:SENSe]:DDEMod:TIME:UNITs

:FETCh:MERRor:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the Magnitude error versus Time measurement.

Syntax :FETCh:MERRor:RMS?

Arguments None

Returns <rms>::=<NRf> is the RMS magnitude error in percent (%).

Measurement Views Magnitude error versus Time

Examples :FETCh:MERRor:RMS?
might return 0.382 indicating the magnitude error is 0.382% RMS.

:FETCh:MERRor:TRACe? (Query Only)

Returns the Magnitude error versus Time trace data.

Syntax :FETCh:MERRor:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the magnitude error in percent (%) for the point #n, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Magnitude error versus Time

Examples :FETCh:MERRor:TRACe?
might return #42036xxxx... (2036-byte data) for the Magnitude error versus Time trace.

:FETCh:OBWidth Subgroup

The :FETCh:OBWidth commands returns the results of the Occupied Bandwidth (OBW) measurement.

Command Tree	Header	Parameter
	:FETCh	
	:OBWidth	
	:FREQuency	
	:ERRor?	
	:OBWidth	
	:BANDwidth?	
	:LEFT	
	:FREQuency?	
	:LEVe1?	
	:POWer?	
	:RIGHT	
	:FREQuency?	
	:LEVe1?	
	:SPECTrum?	
	:XDBBbandwidth	
	:BANDwidth?	
	:LEFT	
	:FREQuency?	
	:LEVe1?	
	:POWer?	
	:RIGHT	
	:FREQuency?	
	:LEVe1?	

:FETCh:OBWidth:FREQuency:ERRor? (Query Only)

Returns the frequency error in the Occupied Bandwidth measurement.

Syntax :FETCh:OBWidth:FREQuency:ERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Measurement Views Occupied Bandwidth

Examples :FETCh:MERRor:FERRor?
might return -10.7E+3 indicating the frequency error is -10.7 kHz.

:FETCh:OBWidth:OBWidth:BANDwidth? (Query Only)

Returns the occupied bandwidth in the Occupied Bandwidth measurement.

Syntax :FETCh:OBWidth:OBWidth:BANDwidth?

Arguments None

Returns <OBW>::=<NRf> is the occupied bandwidth in Hz.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:OBWidth:BANDwidth?
might return 4.0E+6 indicating the occupied bandwidth is 4 MHz.

:FETCh:OBWidth:OBWidth:LEFT:FREQuency? (Query Only)

Returns the left (lower) frequency of the occupied bandwidth.

Syntax :FETCh:OBWidth:OBWidth:LEFT:FREQuency?

Arguments None

Returns <OBW_left_freq>::=<NRf> is the left frequency in Hz.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:OBWidth:LEFT:FREQuency?
might return 1.498E+9 indicating the left frequency is 1.498 GHz.

Related Commands :FETCh:OBWidth:OBWidth:RIGHT:FREQuency?

:FETCh:OBWidth:OBWidth:LEFT:LEVel? (Query Only)

Returns the level at the left frequency of the occupied bandwidth.

Syntax :FETCh:OBWidth:OBWidth:LEFT:LEVel?

Arguments None

Returns <OBW_left_level>::=<NRf> is the level at the left frequency in dB.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:OBWidth:LEFT:LEVel?
might return -23.5 indicating the level at the left frequency is -23.5 dB.

Related Commands :FETCh:OBWidth:OBWidth:RIGHT:LEVel?

:FETCh:OBWidth:OBWidth:POWer? (Query Only)

Returns the reference power in the Occupied Bandwidth measurement.

Syntax :FETCh:OBWidth:OBWidth:POWer?

Arguments None

Returns <OBW_ref_power>::=<NRf> is the reference power in dBm.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:OBWidth:POWer?
might return -10.0 indicating the reference power is -10 dBm.

:FETCh:OBWidth:OBWidth:RIGHT:FREQuency? (Query Only)

Returns the right (higher) frequency of the occupied bandwidth.

Syntax :FETCh:OBWidth:OBWidth:RIGHT:FREQuency?

Arguments None

Returns <OBW_right_freq>::=<NRf> is the right frequency in Hz.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:OBWidth:RIGHT:FREQuency?
might return 1.502E+9 indicating the right frequency is 1.502 GHz.

Related Commands :FETCh:OBWidth:OBWidth:LEFT:FREQuency?

:FETCh:OBWidth:OBWidth:RIGHT:LEVel? (Query Only)

Returns the level at the right frequency of the occupied bandwidth.

Syntax :FETCh:OBWidth:OBWidth:RIGHT:LEVel?

Arguments None

Returns <OBW_right_level>::=<NRf> is the level at the right frequency in dB.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:OBWidth:RIGHT:LEVel?
might return -23.5 indicating the level at the right frequency is -23.5 dB.

Related Commands :FETCh:OBWidth:OBWidth:LEFT:LEVel?

:FETCh:OBWidth:SPECTrum? (Query Only)

Returns spectrum trace data of the Occupied Bandwidth measurement.

Syntax :FETCh:OBWidth:SPECTrum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:SPECTrum?
might return #43204xxxx... (3204-byte data) for the spectrum trace data of the Occupied Bandwidth measurement.

:FETCh:OBWidth:XDBBandwidth:BANDwidth? (Query Only)

Returns the x dB bandwidth in the Occupied Bandwidth measurement.

Syntax :FETCh:OBWidth:XDBBandwidth:BANDwidth?

Arguments None

Returns <xdbBW>::=<NRf> is the x dB bandwidth in Hz.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:XDBBandwidth:BANDwidth?
might return 2.0E+6 indicating the x dB bandwidth is 2 MHz.

:FETCh:OBWidth:XDBBandwidth:LEFT:FREQuency? (Query Only)

Returns the left (lower) frequency of the x dB bandwidth.

Syntax :FETCh:OBWidth:XDBBandwidth:LEFT:FREQuency?

Arguments None

Returns <xdbBW_left_freq>::=<NRf> is the left frequency in Hz.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:XDBBandwidth:LEFT:FREQuency?
might return 1.498E+9 indicating the left frequency is 1.498 GHz.

Related Commands :FETCh:OBWidth:XDBBandwidth:RIGHT:FREQuency?

:FETCh:OBWidth:XDBBandwidth:LEFT:LEVel? (Query Only)

Returns the level at the left frequency of the x dB bandwidth.

Syntax :FETCh:OBWidth:XDBBandwidth:LEFT:LEVel?

Arguments None

Returns <xdbBW_left_level>::=<NRf> is the level at the left frequency in dB.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:XDBBandwidth:LEFT:LEVel?
might return -23.5 indicating the level at the left frequency is -23.5 dB.

Related Commands :FETCh:OBWidth:XDBBandwidth:RIGHT:LEVel?

:FETCh:OBWidth:XDBBandwidth:POWer? (Query Only)

Returns the reference power in the x dB bandwidth measurement.

Syntax :FETCh:OBWidth:XDBBandwidth:POWer?

Arguments None

Returns <xdbBW_ref_power>::=<NRf> is the reference power in dBm.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:XDBBandwidth:POWer?
might return -10.0 indicating the reference power is -10 dBm.

:FETCh:OBWidth:XDBBandwidth:RIGHT:FREQuency? (Query Only)

Returns the right (higher) frequency of the x dB bandwidth.

Syntax :FETCh:OBWidth:XDBBandwidth:RIGHT:FREQuency?

Arguments None

Returns <xdBBW_right_freq>::=<NRf> is the right frequency in Hz.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:XDBBandwidth:RIGHT:FREQuency?
might return 1.502E+9 indicating the right frequency is 1.502 GHz.

Related Commands :FETCh:OBWidth:XDBBandwidth:LEFT:FREQuency?

:FETCh:OBWidth:XDBBandwidth:RIGHT:LEVel? (Query Only)

Returns the level at the right frequency of the x dB bandwidth.

Syntax :FETCh:OBWidth:XDBBandwidth:RIGHT:LEVel?

Arguments None

Returns <xdBBW_right_level>::=<NRf> is the level at the right frequency in dB.

Measurement Views Occupied Bandwidth

Examples :FETCh:OBWidth:XDBBandwidth:RIGHT:LEVel?
might return -23.5 indicating the level at the right frequency is -23.5 dB.

Related Commands :FETCh:OBWidth:XDBBandwidth:LEFT:LEVel?

:FETCh:PERRor Subgroup (Option 21 Only)

The :FETCh:PERRor commands returns the results of the Phase error versus Time measurement.

Command Tree	Header	Parameter
	:FETCh	
	:PERRor	
	:FERRor?	
	:PEAK?	
	:PINdex?	
	:RMS?	
	:TRACe?	

:FETCh:PERRor:FERRor? (Query Only)

Returns the frequency error in the Phase error versus Time measurement.

Syntax :FETCh:PERRor:FERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Measurement Views Phase error versus Time

Examples :FETCh:PERRor:FERRor?
might return -10.7E+3 indicating the frequency error is -10.7 kHz.

:FETCh:PERRor:PEAK? (Query Only)

Returns the peak value in the Phase error versus Time measurement.

Syntax :FETCh:PERRor:PEAK?

Arguments None

Returns <peak>::=<NRf> is the peak phase error in degrees.

Measurement Views Phase error versus Time

Examples :FETCh:PERRor:PEAK?
might return 0.683 indicating the peak phase error is 0.683°.

Related Commands :FETCh:PERRor:PINDex?

:FETCh:PERRor:PINDex? (Query Only)

Returns the time at the phase error peak.

Syntax :FETCh:PERRor:PINDex?

Arguments None

Returns <peak_time>::=<NRf> is the time at the phase error peak in seconds.
You can select the time unit using the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Phase error versus Time

Examples :FETCh:PERRor:PINDex?
might return 28.912E-6 indicating the time at the phase error peak is 28.912 µs.

Related Commands :FETCh:PERRor:PEAK?, [:SENSe]:DDEMod:TIME:UNITs

:FETCh:PERRor:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the Phase error versus Time measurement.

Syntax :FETCh:PERRor:RMS?

Arguments None

Returns <rms>::=<NRf> is the RMS phase error in degrees.

Measurement Views Phase error versus Time

Examples :FETCh:PERRor:RMS?
might return 0.746 indicating the phase error is 0.746° RMS.

:FETCh:PERRor:TRACe? (Query Only)

Returns the Phase error versus Time trace data.

Syntax :FETCh:PERRor:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the phase error in degrees for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Phase error versus Time

Examples :FETCh:PERRor:TRACe?
might return #42036xxxx... (2036-byte data) for the Phase error versus Time trace.

:FETCh:PHVTime Subgroup

The :FETCh:PHVTime commands returns the results of the Phase versus Time measurement.

Command Tree	Header	Parameter
	:FETCh	
	:PHVTime?	
	:MAXimum?	
	:MAXLocation?	
	:MINimum?	
	:MINLocation?	
	:RESult?	

:FETCh:PHVTime? (Query Only)

Returns the Phase versus Time trace data.

Syntax :FETCh:PHVTime?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the phase in degrees for the point #n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Phase versus Time

Examples :FETCh:PHVTime?
might return #3160xxxx... (160-byte data) for the Phase versus Time trace.

:FETCh:PHVTime:MAXimum? (Query Only)

Returns the maximum value in the Phase versus Time measurement.

Syntax :FETCh:PHVTime:MAXimum?

Arguments None

Returns <max>::=<NRf> is the maximum phase in degrees.

Measurement Views Phase versus Time

Examples :FETCh:PHVTime:MAXimum?
might return 153.8 indicating the maximum phase is 153.8°.

Related Commands :FETCh:PHVTime:MAXLocation?

:FETCh:PHVTime:MAXLocation? (Query Only)

Returns the time at which the phase is maximum.

Syntax :FETCh:PHVTime:MAXLocation?

Arguments None

Returns <max_time>::=<NRf> is the time in seconds at which the phase is maximum.

Measurement Views Phase versus Time

Examples :FETCh:PHVTime:MAXLocation?
might return 175.3E-9 indicating the I or Q level is maximum at 175.3 ns.

Related Commands :FETCh:PHVTime:MAXimum?

:FETCh:PHVTime:MINimum? (Query Only)

Returns the minimum value in the Phase versus Time measurement.

Syntax :FETCh:PHVTime:MINimum?

Arguments None

Returns <min>::=<NRf> is the minimum phase in degrees.

Measurement Views Phase versus Time

Examples :FETCh:PHVTime:MINimum?
might return -176.3 indicating the minimum phase is -176.3°.

Related Commands :FETCh:PHVTime:MINLocation?

:FETCh:PHVTime:MINLocation? (Query Only)

Returns the time at which the phase is minimum.

Syntax :FETCh:PHVTime:MINLocation?

Arguments None

Returns <min_time>::=<NRf> is the time in seconds at which the phase is minimum.

Measurement Views Phase versus Time

Examples :FETCh:PHVTime:MAXLocation?
might return 450.7E-9 indicating the phase is minimum at 450.7 ns.

Related Commands :FETCh:PHVTime:MINimum?

:FETCh:PHVTime:RESult? (Query Only)

Returns the Phase versus Time measurement results.

Syntax :FETCh:PHVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>

Where

<max>::=<NRf> is the maximum phase in degrees.

<max_time>::=<NRf> is the time in seconds at which the phase is maximum.

<min>::=<NRf> is the minimum phase in degrees.

<min_time>::=<NRf> is the time in seconds at which the phase is minimum.

Measurement Views Phase versus Time

Examples :FETCh:PHVTime:RESult?
might return 153.8,175.3E-9,-176.3,450.7E-9 indicating:
the maximum phase is 153.8° at 175.3 ns and
the minimum phase is -176.3° at 450.7 ns.

:FETCh:PULSe Subgroup (Option 20 Only)

The :FETCh:PULSe commands returns the results of the Pulse Measurements.

Command Tree	Header	Parameter
	:FETCh	
	:PULSe	
	[:RESuLt]	
		:ATX?
		:AVERage?
		:DROop?
		:DUTPct?
		:DUTRatio?
		:FALL?
		:FRDeviation?
		:MFReqerror?
		:MPHerror?
		:PHDeviation?
		:PPFRequency?
		:PPOWer?
		:PPPHase?
		:RINTerval?
		:RIPPlE?
		:RISE?
		:RMSFreqerror?
		:RMSPHerror?
		:RRATe?
		:TIME?
		:WIDTh?
	:STATistics?	
		:ATX?
		:AVERage?
		:DROop?
		:DUTPct?
		:DUTRatio?
		:FALL?
		:FRDeviation?
		:MFReqerror?
		:MPHerror?
		:PHDeviation?
		:PPFRequency?
		:PPOWer?
		:PPPHase?
		:RINTerval?
		:RIPPlE?
		:RISE?

```

:RMSFreqerror?
:RMSPherror?
:RRATe?
:WIDTh?
:TRACe?

```

:FETCh:PULSe[:RESult]:ATX? (Query Only)

Returns the average transmitted power in the pulse table.

Syntax :FETCh:PULSe[:RESult]:ATX?

Arguments None

Returns <first_pulse_num>,<ATX(1)>,<ATX(2)>,...<ATX(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<ATX(n)>::=<NRf> is the average transmitted power for the pulse with the number of [first_pulse_num + n - 1] in dBm.

The unit can be changed to watts by the [:SENSe]:POWer:UNITs command. Volt is invalid in the average transmitted power measurement.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:ATX?
might return 0,-18.57,-18.73,-18.20,-18.53 for Pulse 0 to 3.

Related Commands [:SENSe]:POWer:UNITs

:FETCh:PULSe[:RESult]:AVERage? (Query Only)

Returns the average on power in the pulse table.

Syntax :FETCh:PULSe[:RESult]:AVERage?

Arguments None

Returns <first_pulse_num>,<avg(1)>,<avg(2)>,...<avg(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<avg(n)>::=<NRf> is the average on power for the pulse with the number of [first_pulse_num + n - 1] in dBm.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:AVERage?
might return 0,-2.354,-2.368,-2.343,-2.358 for Pulse 0 to 3.

Related Commands [:SENSe]:POWer:UNITs

:FETCh:PULSe[:RESult]:DROOp? (Query Only)

Returns the droop in the pulse table.

Syntax :FETCh:PULSe[:RESult]:DROOp?

Arguments None

Returns <first_pulse_num>,<droop(1)>,<droop(2)>,...<droop(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<droop(n)>::=<NRf> is the wattage droop for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:DROOp?
might return 0,-270.9E-3,-193.0E-3,-242.7E-3,-177.5E-3 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:DUTPct? (Query Only)

Returns the duty factor (%) in the pulse table.

Syntax :FETCh:PULSe[:RESult]:DUTPct?

Arguments None

Returns <first_pulse_num>,<duty_pct(1)>,<duty_pct(2)>,...
<duty_pct(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<duty_pct(n)>::=<NRf> is the duty factor for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:DUTPct?
might return 0,28.94,28.96,29.00,29.01 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:DUTRatio? (Query Only)

Returns the duty factor (ratio) in the pulse table.

Syntax :FETCh:PULSe[:RESult]:DUTRatio?

Arguments None

Returns <first_pulse_num>,<duty_ratio(1)>,<duty_ratio(2)>,...
<duty_ratio(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<duty_ratio(n)>::=<NRf> is the duty factor for the pulse with the number of
[first_pulse_num + n - 1] (no unit).

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:DUTRatio?
might return 0,289.4E-3,289.6E-3,290.0E-3,290.1E-3 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:FALL? (Query Only)

Returns the fall time in the pulse table.

Syntax :FETCh:PULSe[:RESult]:FALL?

Arguments None

Returns <first_pulse_num>,<fall(1)>,<fall(2)>,...<fall(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<fall(n)>::=<NRf> is the fall time for the pulse with the number of
[first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:FALL?
might return 0,110.3E-9,90.45E-9,95.03E-9,111.9E-9 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:FRDeviation? (Query Only)

Returns the frequency deviation in the pulse table.

Syntax :FETCh:PULSe[:RESult]:FRDeviation?

Arguments None

Returns <first_pulse_num>,<freq_dev(1)>,<freq_dev(2)>,...
<freq_dev(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<freq_dev(n)>::=<NRf> is the frequency deviation for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:FRDeviation?
might return 1,740.6E+3,736.5E+3,718.3E+3,672.2E+3 for Pulse 1 to 4.

:FETCh:PULSe[:RESult]:MFRerror? (Query Only)

Returns the maximum frequency error in the pulse table.

Syntax :FETCh:PULSe[:RESult]:MFRerror?

Arguments None

Returns <first_pulse_num>,<max_freq_err(1)>,<max_freq_err(2)>,...
<max_freq_err(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<max_freq_err(n)>::=<NRf> is the maximum frequency error for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:MFRerror?
might return 1,597.5E+3,675.8E+3,642.8E+3,598.2E+3 for Pulse 1 to 4.

:FETCh:PULSe[:RESult]:MPHerror? (Query Only)

Returns the maximum phase error in the pulse table.

Syntax :FETCh:PULSe[:RESult]:MPHerror?

Arguments None

Returns <first_pulse_num>,<max_phase_err(1)>,<max_phase_err(2)>,...
<max_phase_err(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<max_phase_err(n)>::=<NRf> is the maximum phase error for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:MPHerror?
might return 1,-9.221,-8.413,-11.853,-10.258 for Pulse 1 to 4.

:FETCh:PULSe[:RESult]:PHDeviation? (Query Only)

Returns the phase deviation in the pulse table.

Syntax :FETCh:PULSe[:RESult]:PHDeviation?

Arguments None

Returns <first_pulse_num>,<phase_dev(1)>,<phase_dev(2)>,...
<phase_dev(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<phase_dev(n)>::=<NRf> is the phase deviation for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:PHDeviation?
might return 1,11.658,9.640,10.509,8.272 for Pulse 1 to 4.

:FETCh:PULSe[:RESult]:PPFrequency? (Query Only)

Returns the pulse-pulse carrier frequency in the pulse table.

Syntax :FETCh:PULSe[:RESult]:PPFrequency?

Arguments None

Returns <first_pulse_num>,<pp_freq(1)>,<pp_freq(2)>,...<pp_freq(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<pp_freq(n)>::=<NRf> is the pulse-pulse carrier frequency for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:PPFrequency?
might return 0,0.000,1.258E+3,-3.121E+3,1.862E+3 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:PPOWer? (Query Only)

Returns the peak power in the pulse table.

Syntax :FETCh:PULSe[:RESult]:PPOWer?

Arguments None

Returns <first_pulse_num>,<pk_power(1)>,<pk_power(2)>,...
 <pk_power(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<pk_power(n)>::=<NRf> is the peak power for the pulse with the number of
[first_pulse_num + n - 1] in dBm.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:PPOWer?
 might return 0,-2.26,-2.27,-2.23,-2.25 for Pulse 0 to 3.

Related Commands [:SENSe]:POWer:UNITs

:FETCh:PULSe[:RESult]:PPPHase? (Query Only)

Returns the pulse-pulse carrier phase in the pulse table.

Syntax :FETCh:PULSe[:RESult]:PPPHase?

Arguments None

Returns <first_pulse_num>,<pp_phase(1)>,<pp_phase(2)>,...
<pp_phase(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<pp_phase(n)>::=<NRf> is the pulse-pulse carrier phase for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:PPPHase?
might return 0,0.000,21.66,46.76,57.56 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:RINterval? (Query Only)

Returns the repetition interval in the pulse table.

Syntax :FETCh:PULSe[:RESult]:RINterval?

Arguments None

Returns <first_pulse_num>,<rep_int(1)>,<rep_int(2)>,...<rep_int(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<rep_int(n)>::=<NRf> is the repetition interval for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:RINterval?
might return 0,16.03E-6,16.08E-6,16.07E-6,16.02E-6 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:RIPple? (Query Only)

Returns the ripple in the pulse table.

Syntax :FETCh:PULSe[:RESult]:RIPple?

Arguments None

Returns <first_pulse_num>,<ripple(1)>,<ripple(2)>,...<ripple(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<ripple(n)>::=<NRf> is the voltage ripple for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:RIPple?
might return 0,106.5E-3,177.6E-3,148.3E-3,148.5E-3 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:RISE? (Query Only)

Returns the rise time in the pulse table.

Syntax :FETCh:PULSe[:RESult]:RISE?

Arguments None

Returns <first_pulse_num>,<rise(1)>,<rise(2)>,...<rise(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<rise(n)>::=<NRf> is the rise time for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:RISE?
might return 0,92.94E-9,115.9E-9,115.1E-9,97.45E-9 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:RMSFreqerror? (Query Only)

Returns the RMS frequency error in the pulse table.

Syntax :FETCh:PULSe[:RESult]:RMSFreqerror?

Arguments None

Returns <first_pulse_num>,<RMS_freq_err(1)>,<RMS_freq_err(2)>,...
<RMS_freq_err(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<RMS_freq_err(n)>::=<NRf> is the RMS frequency error for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:RMSFreqerror?
might return 1,51.54E+3,69.20E+3,64.21E+3,51.02E+3 for Pulse 1 to 4.

:FETCh:PULSe[:RESult]:RMSPherror? (Query Only)

Returns the RMS phase error in the pulse table.

Syntax :FETCh:PULSe[:RESult]:RMSPherror?

Arguments None

Returns <first_pulse_num>,<RMS_phase_err(1)>,<RMS_phase_err(2)>,...
<RMS_phase_err(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<RMS_phase_err(n)>::=<NRf> is the RMS phase error for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:RMSPherror?
might return 1,908.4E-3,752.8E-3,981.7E-3,886.4E-3 for Pulse 1 to 4.

:FETCh:PULSe[:RESult]:RRATe? (Query Only)

Returns the repetition rate in the pulse table.

Syntax :FETCh:PULSe[:RESult]:RRATe?

Arguments None

Returns <first_pulse_num>,<rep_rate(1)>,<rep_rate(2)>,...
<rep_rate(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<rep_rate(n)>::=<NRf> is the repetition rate for the pulse with the number of
[first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:RRATe?
might return 0,62.50E+3,62.52E+3,62.51E+3,62.49E+3 for Pulse 0 to 3.

:FETCh:PULSe[:RESult]:TIME? (Query Only)

Returns the time in the pulse table.

Syntax :FETCh:PULSe[:RESult]:TIME?

Arguments None

Returns <first_pulse_num>,<time(1)>,<time(2)>,...<time(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<time(n)>::=<NRf> is the time for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:TIME?
might return 1,7.937E-3,8.436E-3,6.504E-3,9.876E-3 for Pulse 1 to 4.

:FETCh:PULSe[:RESult]:WIDTh? (Query Only)

Returns the pulse width in the pulse table.

Syntax :FETCh:PULSe[:RESult]:WIDTh?

Arguments None

Returns <first_pulse_num>,<width(1)>,<width(2)>,...<width(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<width(n)>::=<NRf> is the pulse width for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :FETCh:PULSe:RESult:WIDTh?
might return 0,4.630E-6,4.632E-6,4.639E-6,4.642E-6 for Pulse 0 to 3.

:FETCh:PULSe:STATistics? (Query Only)

Returns the trace data of the pulse statistics measurement selected by the :DISPlay:PULSe:SElect:RESult command.

NOTE. Select the plot type (Trend or FFT) using the :DISPlay:PULSe:STATistics:PLOT command before executing this query.

Syntax :FETCh:PULSe:STATistics?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude for the point #n.

The unit is dBm (Plot = Trend) or dB (Plot = FFT).

4-byte little endian floating-point format specified in IEEE 488.2.

The unit of power is selected by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics?
might return #264xxxx... (64-byte data) for the statistics trace of the pulse width measurement when :DISPlay:PULSe:SElect:RESult is set to WIDTh.

Related Commands :DISPlay:PULSe:SElect:RESult, :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:ATX? (Query Only)

Returns the average transmitted power in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:ATX?

Arguments None

Returns <ATX_avg>,<ATX_min>,<ATX_max>

Where

<ATX_avg>::=<NRf> is the average of the average transmitted power.

<ATX_min>::=<NRf> is the minimum of the average transmitted power.

<ATX_max>::=<NRf> is the maximum of the average transmitted power.

Unit: dBm.

The unit can be changed to watts by the [:SENSe]:POWer:UNITs command.

Volt is invalid in the average transmitted power measurement.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:ATX?
might return -18.51,-18.74,-18.12 for the average transmitted power in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT, [:SENSe]:POWer:UNITs

:FETCh:PULSe:STATistics:AVERage? (Query Only)

Returns the average on power in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:AVERage?

Arguments None

Returns <avg_avg>,<avg_min>,<avg_max>

Where

<avg_avg>::=<NRf> is the average of the average on power.

<avg_min>::=<NRf> is the minimum of the average on power.

<avg_max>::=<NRf> is the maximum of the average on power.

Unit: dBm.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:AVERage?
might return -2.35,-2.36,-2.34 for the average on power in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT, [:SENSe]:POWer:UNITs

:FETCh:PULSe:STATistics:DR0op? (Query Only)

Returns the droop in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:DR0op?

Arguments None

Returns <droop_avg>,<droop_min>,<droop_max>

Where

<droop_avg>::=<NRf> is the average droop.

<droop_min>::=<NRf> is the minimum droop.

<droop_max>::=<NRf> is the maximum droop.

Unit: Percent (%) by watts.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:DR0op?
might return 22.67E-3,-613.5E-3,633.8E-3 for the droop in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:DUTPct? (Query Only)

Returns the duty factor (%) in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:DUTPct?

Arguments None

Returns <duty_pct_avg>,<duty_pct_min>,<duty_pct_max>

Where

<duty_pct_avg>::=<NRf> is the average duty factor.

<duty_pct_min>::=<NRf> is the minimum duty factor.

<duty_pct_max>::=<NRf> is the maximum duty factor.

Unit: Percent (%).

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:DUTPct?
might return 2.437,2.310,2.657 for the duty factor (%) in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:DUTRatio? (Query Only)

Returns the duty factor (ratio) in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:DUTRatio?

Arguments None

Returns <duty_ratio_avg>,<duty_ratio_min>,<duty_ratio_max>

Where

<duty_ratio_avg>::=<NRf> is the average duty factor.

<duty_ratio_min>::=<NRf> is the minimum duty factor.

<duty_ratio_max>::=<NRf> is the maximum duty factor.

Unit: None.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:DUTRatio?
might return 24.37E-3,23.11E-3,26.57E-3 for the duty factor (ratio) in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:FALL? (Query Only)

Returns the fall time in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:FALL?

Arguments None

Returns <fall_avg>,<fall_min>,<fall_max>

Where

<fall_avg>::=<NRf> is the average fall time.

<fall_min>::=<NRf> is the minimum fall time.

<fall_max>::=<NRf> is the maximum fall time.

Unit: Seconds.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:FALL?
might return 70.27E-9,69.62E-9,71.27E-9 for the fall time in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:FRDeviation? (Query Only)

Returns the frequency deviation in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:FRDeviation?

Arguments None

Returns <freq_dev_avg>,<freq_dev_min>,<freq_dev_max>

Where

<freq_dev_avg>::=<NRf> is the average frequency deviation.

<freq_dev_min>::=<NRf> is the minimum frequency deviation.

<freq_dev_max>::=<NRf> is the maximum frequency deviation.

Unit: Hz.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:FRDeviation?
might return 754.1E+3,660.5E+3,835.2E+3 for the frequency deviation in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:MFRReqerror? (Query Only)

Returns the maximum frequency error in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:MFRReqerror?

Arguments None

Returns <max_freq_err_avg>,<max_freq_err_min>,<max_freq_err_max>

Where

<max_freq_err_avg>::=<NRf> is the average of maximum frequency error.

<max_freq_err_min>::=<NRf> is the minimum of maximum frequency error.

<max_freq_err_max>::=<NRf> is the maximum of maximum frequency error.

Unit: Hz.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:MFRReqerror?
might return 645.0E+3,555.6E+3,738.8E+3 for the maximum frequency error in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:MPHerror? (Query Only)

Returns the maximum phase error in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:MPHerror?

Arguments None

Returns <max_phase_err_avg>,<max_phase_err_min>,<max_phase_err_max>

Where

<max_phase_err_avg>::=<NRf> is the average of maximum phase error.

<max_phase_err_min>::=<NRf> is the minimum of maximum phase error.

<max_phase_err_max>::=<NRf> is the maximum of maximum phase error.

Unit: Degrees.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:MPHerror?
might return -11.47,-17.18,-7.61 for the maximum phase error in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:PHDeviation? (Query Only)

Returns the phase deviation in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:PHDeviation?

Arguments None

Returns <phase_dev_avg>,<phase_dev_min>,<phase_dev_max>

Where

<phase_dev_avg>::=<NRf> is the average phase deviation.

<phase_dev_min>::=<NRf> is the minimum phase deviation.

<phase_dev_max>::=<NRf> is the maximum phase deviation.

Unit: Degrees.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:PHDeviation?
might return 11.678,7.694,17.374 for the phase deviation in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:PPFrequency? (Query Only)

Returns the pulse-pulse carrier frequency in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:PPFrequency?

Arguments None

Returns <pp_freq_avg>,<pp_freq_min>,<pp_freq_max>

Where

<pp_freq_avg>::=<NRf> is the average pulse-pulse carrier frequency.

<pp_freq_min>::=<NRf> is the minimum pulse-pulse carrier frequency.

<pp_freq_max>::=<NRf> is the maximum pulse-pulse carrier frequency.

Unit: Hz.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:PPFrequency?
might return 1.135E+3,311.3E+3,-262.8E+3 for the pulse-pulse carrier frequency in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:PPOWer? (Query Only)

Returns the peak power in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:PPOWer?

Arguments None

Returns <pk_power_avg>,<pk_power_min>,<pk_power_max>

Where

<pk_power_avg>::=<NRf> is the average peak power.

<pk_power_min>::=<NRf> is the minimum peak power.

<pk_power_max>::=<NRf> is the maximum peak power.

Unit: dBm.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:PPOWer?
might return -2.273,-2.313,-2.235 for the peak power in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT, [:SENSe]:POWer:UNITs

:FETCh:PULSe:STATistics:PPPHase? (Query Only)

Returns the pulse-pulse carrier phase in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:PPPHase?

Arguments None

Returns <pp_phase_avg>,<pp_phase_min>,<pp_phase_max>

Where

<pp_phase_avg>::=<NRf> is the average pulse-pulse carrier phase.

<pp_phase_min>::=<NRf> is the minimum pulse-pulse carrier phase.

<pp_phase_max>::=<NRf> is the maximum pulse-pulse carrier phase.

Unit: Degrees.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:PPPHase?
might return -9.298E-3,-254.3E-3,311.7E-3 for the pulse-pulse carrier phase in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:RINterval? (Query Only)

Returns the repetition interval in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:RINterval?

Arguments None

Returns <rep_int_avg>,<rep_int_min>,<rep_int_max>

Where

<rep_int_avg>::=<NRf> is the average repetition interval.

<rep_int_min>::=<NRf> is the minimum repetition interval.

<rep_int_max>::=<NRf> is the maximum repetition interval.

Unit: Seconds.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:RINterval?
might return 240.5E-6,217.9E-6,281.2E-6 for the repetition interval in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:RIPPlE? (Query Only)

Returns the ripple in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:RIPPlE?

Arguments None

Returns <ripple_avg>,<ripple_min>,<ripple_max>

Where

<ripple_avg>::=<NRf> is the average ripple.

<ripple_min>::=<NRf> is the minimum ripple.

<ripple_max>::=<NRf> is the maximum ripple.

Unit: Percent (%) by volts.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:RIPPlE?
might return 160.4E-3,83.78E-3,287.7E-3 for the ripple in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:RISE? (Query Only)

Returns the rise time in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:RISE?

Arguments None

Returns <rise_avg>,<rise_min>,<rise_max>

Where

<rise_avg>::=<NRf> is the average rise time.

<rise_min>::=<NRf> is the minimum rise time.

<rise_max>::=<NRf> is the maximum rise time.

Unit: Seconds.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:RISE?
might return 105.4E-9,91.65E-9,116.2E-9 for the rise time in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:RMSFreqerror? (Query Only)

Returns the RMS frequency error in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:RMSFreqerror?

Arguments None

Returns <RMS_freq_err_avg>,<RMS_freq_err_min>,<RMS_freq_err_max>

Where

<RMS_freq_err_avg>::=<NRf> is the average of RMS frequency error.

<RMS_freq_err_min>::=<NRf> is the minimum of RMS frequency error.

<RMS_freq_err_max>::=<NRf> is the maximum of RMS frequency error.

Unit: Hz.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:RMSFreqerror?
might return 63.67E+3,45.49E+3,81.28E+3 for the RMS frequency error in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:RMSPherror? (Query Only)

Returns the RMS phase error in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:RMSPherror?

Arguments None

Returns <RMS_phase_err_avg>,<RMS_phase_err_min>,<RMS_phase_err_max>

Where

<RMS_phase_err_avg>::=<NRf> is the average of RMS phase error.

<RMS_phase_err_min>::=<NRf> is the minimum of RMS phase error.

<RMS_phase_err_max>::=<NRf> is the maximum of RMS phase error.

Unit: Degrees.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:RMSPherror?
might return 1.032,604.5E-3,1.606 for the RMS phase error in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:RRATe? (Query Only)

Returns the repetition rate in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:RRATe?

Arguments None

Returns <rep_rate_avg>,<rep_rate_min>,<rep_rate_max>

Where

<rep_rate_avg>::=<NRf> is the average repetition rate.

<rep_rate_min>::=<NRf> is the minimum repetition rate.

<rep_rate_max>::=<NRf> is the maximum repetition rate.

Unit: Hz.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:RRATe?
might return 62.50E+3,62.49E+3,62.52E+3 for the repetition rate in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:STATistics:WIDTh? (Query Only)

Returns the pulse width in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :FETCh:PULSe:STATistics:WIDTh?

Arguments None

Returns <width_avg>,<width_min>,<width_max>

Where

<width_avg>::=<NRf> is the average pulse width.

<width_min>::=<NRf> is the minimum pulse width.

<width_max>::=<NRf> is the maximum pulse width.

Unit: Seconds.

Measurement Views Pulse statistics

Examples :FETCh:PULSe:STATistics:WIDTh?
might return 4.636E-6,4.630E-6,4.643E-6 for the pulse width in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:FETCh:PULSe:TRACe? (Query Only)

Returns the waveform data in the pulse trace measurement selected by the :DISPlay:PULSe:SElect:RESult command.

Syntax :FETCh:PULSe:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

The unit of power is selected by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse trace

Examples :FETCh:PULSe:TRACe?
might return #43204xxxx... (3204-byte data) for the trace of the pulse width measurement when :DISPlay:PULSe:SElect:RESult is set to WIDTh.

Related Commands :DISPlay:PULSe:SElect:RESult

:FETCh:SGRam Subgroup

The :FETCh:SGRam commands returns the results of the spectrogram measurement.

Command Tree	Header	Parameter
	:FETCh	
	:SGRam?	

:FETCh:SGRam? (Query Only)

Returns trace data of a line in the spectrogram.
The line is selected using the :TRACe:SGRam:SElect:LINE command.

Syntax :FETCh:SGRam?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where
 <num_digit> is the number of digits in <num_byte>.
 <num_byte> is the number of bytes of data that follow.
 <data(n)> is the amplitude in dBm for the point #n,
 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Spectrogram

Examples :FETCh:SGRam?
 might return #43204xxxx... (3204-byte data) for the line in the spectrogram.

Related Commands :TRACe:SGRam:SElect:LINE

:FETCh:SPECtrum Subgroup

The :FETCh:SPECtrum commands returns results of the Spectrum measurement.

Command Tree	Header	Parameter
	:FETCh	
	:SPECtrum	
	:TRACe<x>?	

Where <x> = 1 to 5. Each trace is defined as follows:

TRACe1: Trace 1
TRACe2: Trace 2
TRACe3: Trace 3
TRACe4: Math trace
TRACe5: Spectrogram

The traces can be specified by the :TRACe<x>:SPECtrum command subgroup.

:FETCh:SPECTrum:TRACe<x>? (Query Only)

Returns the trace data in the Spectrum measurement.

Syntax :FETCh:SPECTrum:TRACe<x>?

Where <x> = 1 to 5.

NOTE. TRACe5 (spectrogram) is valid when the spectrum and spectrogram measurements are running.

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Spectrum

Examples :FETCh:SPECTrum:TRACe1?
might return #43204xxxx... (3204-byte data) for Trace 1 in the spectrum measurement.

Related Commands :TRACe<x>:SPECTrum command subgroup

:FETCh:SQQuality Subgroup (Option 21 Only)

The :FETCh:SQQuality commands return the results of the signal quality measurement.

Command Tree	Header	Parameter
	:FETCh	
	:SQQuality	
	:FREQuency	
	:ERRor?	
	:GAIN	
	:IMBalance?	
	:ORIGin	
	:OFFSet?	
	:PEAK	
	:EVM?	
	:DB?	
	:LOCation?	
	:MERRor?	
	:DB?	
	:LOCation?	
	:PERRor?	
	:LOCation?	
	:QUADrature	
	:ERRor?	
	:RHO	
	:RMS	
	:EVM?	
	:DB?	
	:MERRor?	
	:DB?	
	:PERRor?	

:FETCh:SQQuality:FREQuency:ERRor? (Query Only)

Returns the frequency error in the signal quality measurement.

Syntax :FETCh:SQQuality:FREQuency:ERRor?

Arguments None

Returns <NRf> Frequency error in Hz.

Measurement Views Signal quality

Examples :FETCh:SQQuality:FREQuency:ERRor?
might return 612.043E+3, indicating that the frequency error is 612.043 kHz.

:FETCh:SQQuality:GAIN:IMBalance? (Query Only)

Returns the gain imbalance in the signal quality measurement.

Syntax :FETCh:SQQuality:GAIN:IMBalance?

Arguments None

Returns <NRf> Gain imbalance in dB.

Measurement Views Signal quality

Examples :FETCh:SQQuality:GAIN:IMBalance?
might return -57.746E-3, indicating that the gain imbalance is -0.057746 dB.

:FETCh:SQUality:ORIGin:OFFSet? (Query Only)

Returns the origin offset in the signal quality measurement.

Syntax :FETCh:SQUality:ORIGin:OFFSet?

Arguments None

Returns <NRf> Origin offset in dB.

Measurement Views Signal quality

Examples :FETCh:SQUality:ORIGin:OFFSet?
might return -44.968, indicating that the origin offset is -44.968 dB.

:FETCh:SQUality:PEAK:EVM? (Query Only)

Returns the peak EVM (%) in the signal quality measurement.

Syntax :FETCh:SQUality:PEAK:EVM?

Arguments None

Returns <NRf> Peak EVM in percent (%).

Measurement Views Signal quality

Examples :FETCh:SQUality:PEAK:EVM?
might return 4.276, indicating that the peak EVM is 4.276%.

:FETCh:SQUality:PEAK:EVM:DB? (Query Only)

Returns the peak EVM (dB) in the signal quality measurement.

Syntax :FETCh:SQUality:PEAK:EVM:DB?

Arguments None

Returns <NRf> Peak EVM in dB.

Measurement Views Signal quality

Examples :FETCh:SQUality:PEAK:EVM:DB?
might return -27.358, indicating that the peak EVM is -27.358 dB.

:FETCh:SQUality:PEAK:EVM:LOCation? (Query Only)

Returns the time at which the EVM is peak.

Syntax :FETCh:SQUality:PEAK:EVM:LOCation?

Arguments None

Returns <NRf> The time in seconds at which the EVM is peak.
The unit can be changed by the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Signal quality

Examples :FETCh:SQUality:PEAK:EVM:LOCation?
might return 36.018E-6, indicating that the EVM is peak at 36.018 μ s.

Related Commands [:SENSe]:DDEMod:TIME:UNITs

:FETCh:SQUality:PEAK:MERRor? (Query Only)

Returns the peak magnitude error (%) in the signal quality measurement.

Syntax :FETCh:SQUality:PEAK:MERRor?

Arguments None

Returns <NRf> Peak magnitude error in percent (%).

Measurement Views Signal quality

Examples :FETCh:SQUality:PEAK:MERRor?
might return 3.595, indicating that the peak magnitude error is 3.595%.

:FETCh:SQUality:PEAK:MERRor:DB? (Query Only)

Returns the peak magnitude error (dB) in the signal quality measurement.

Syntax :FETCh:SQUality:PEAK:MERRor:DB?

Arguments None

Returns <NRf> Peak magnitude error in dB.

Measurement Views Signal quality

Examples :FETCh:SQUality:PEAK:MERRor:DB?
might return -28.583, indicating that the magnitude error is -28.583 dB.

:FETCh:SQuality:PEAK:MERRor:LOCation? (Query Only)

Returns the time at which the magnitude error is peak.

Syntax :FETCh:SQuality:PEAK:MERRor:LOCation?

Arguments None

Returns <NRf> The time in seconds at which the magnitude error is peak.
The unit can be changed by the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Signal quality

Examples :FETCh:SQuality:PEAK:MERRor:LOCation?
might return 42.127E-6, indicating that the magnitude error is peak at
42.127 μ s.

Related Commands [:SENSe]:DDEMod:TIME:UNITs

:FETCh:SQUality:PEAK:PERRor? (Query Only)

Returns the peak phase error in the signal quality measurement.

Syntax :FETCh:SQUality:PEAK:PERRor?

Arguments None

Returns <NRf> Peak phase error in degrees.

Measurement Views Signal quality

Examples :FETCh:SQUality:PEAK:PERRor?
might return 1.907, indicating that the peak phase error is 1.907°.

:FETCh:SQUality:PEAK:PERRor:LOCation? (Query Only)

Returns the time at which the phase error is peak.

Syntax :FETCh:SQUality:PEAK:PERRor:LOCation?

Arguments None

Returns <NRf> The time in seconds at which the phase error is peak.
The unit can be changed by the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Signal quality

Examples :FETCh:SQUality:PEAK:PERRor:LOCation?
might return 41.825E-6, indicating that the phase error is peak at 41.825 μs.

Related Commands [:SENSe]:DDEMod:TIME:UNITs

:FETCh:SQQuality:QUADrature:ERRor? (Query Only)

Returns the quadrature error in the signal quality measurement.

Syntax :FETCh:SQQuality:QUADrature:ERRor?

Arguments None

Returns <NRf> Quadrature error in degrees.

Measurement Views Signal quality

Examples :FETCh:SQQuality:QUADrature:ERRor?
might return -14.264E-3, indicating that the quadrature error is -0.014264°.

:FETCh:SQQuality:RH0? (Query Only)

Returns the ρ (waveform quality) value in the signal quality measurement.

Syntax :FETCh:SQQuality:RH0?

Arguments None

Returns <NRf> ρ value.

Measurement Views Signal quality

Examples :FETCh:SQQuality:RH0?
might return 998.703E-3, indicating that ρ is 0.998703.

:FETCh:SQUality:RMS:EVM? (Query Only)

Returns the RMS EVM (%) in the signal quality measurement.

Syntax :FETCh:SQUality:RMS:EVM?

Arguments None

Returns <NRf> RMS EVM in percent (%).

Measurement Views Signal quality

Examples :FETCh:SQUality:RMS:EVM?
might return 2.417, indicating that the RMS EVM is 2.417%.

:FETCh:SQUality:RMS:EVM:DB? (Query Only)

Returns the RMS EVM (dB) in the signal quality measurement.

Syntax :FETCh:SQUality:RMS:EVM:DB?

Arguments None

Returns <NRf> RMS EVM in dB.

Measurement Views Signal quality

Examples :FETCh:SQUality:RMS:EVM:DB?
might return -32.356, indicating that the RMS EVM is -32.356 dB.

:FETCh:SQQuality:RMS:MERRor? (Query Only)

Returns the RMS magnitude error (%) in the signal quality measurement.

Syntax :FETCh:SQQuality:RMS:MERRor?

Arguments None

Returns <NRf> RMS magnitude error in percent (%).

Measurement Views Signal quality

Examples :FETCh:SQQuality:RMS:MERRor?
might return 1.837, indicating that the RMS magnitude error is 1.837%.

:FETCh:SQQuality:RMS:MERRor:DB? (Query Only)

Returns the RMS magnitude error (dB) in the signal quality measurement.

Syntax :FETCh:SQQuality:RMS:MERRor:DB?

Arguments None

Returns <NRf> RMS MERRor in dB.

Measurement Views Signal quality

Examples :FETCh:SQQuality:RMS:MERRor:DB?
might return -34.706, indicating that the magnitude error is -34.706 dB.

:FEtCh:SQUality:RMS:PErRor? (Query Only)

Returns the RMS phase error in the signal quality measurement.

Syntax :FEtCh:SQUality:RMS:PErRor?

Arguments None

Returns <NRf> RMS phase error in degrees.

Measurement Views Signal quality

Examples :FEtCh:SQUality:RMS:PErRor?
might return 893.472E-3, indicating that the RMS phase error is 0.893472°.

:FETCh:TOVerview Subgroup

The :FETCh:TOVerview commands returns the results of the time overview measurement.

Command Tree	Header	Parameter
	:FETCh	
	:TOVerview?	

:FETCh:TOVerview? (Query Only)

Returns the trace data in the time overview.

Syntax :FETCh:TOVerview?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Time overview

Examples :FETCh:TOVerview?
might return #43204xxxx... (3204-byte data) for the trace in the time overview.

INITiate Commands

The INITiate commands control data acquisition.

Command Tree

Header	Parameter
:INITiate	
:CONTinuous	<boolean>
[:IMMediate]	

:INITiate:CONTinuous(?)

Determines whether to place the analyzer in the single or the continuous acquisition mode.

Syntax :INITiate:CONTinuous { OFF | ON | 0 | 1 }
 :INITiate:CONTinuous?

Arguments OFF or 0 places the analyzer in the single acquisition mode.
 To initiate the acquisition, use the :INITiate[:IMMediate] command.
 To stop the acquisition because the trigger does not occur in the single mode, send the following command: :INITiate:CONTinuous OFF

 ON or 1 places the analyzer in the continuous acquisition mode.
 To initiate the acquisition, use the :INITiate[:IMMediate] command.
 To stop the acquisition in the continuous mode, send the following command: :INITiate:CONTinuous OFF

Measurement Views All

Examples :INITiate:CONTinuous ON
 places the analyzer in the continuous acquisition mode.

Related Commands :INITiate[:IMMediate]

:INITiate[:IMMediate] (No Query Form)

Starts input signal acquisition.

NOTE. It is an overlapped command, which does not finish executing before the next command starts executing. Use the *OPC(?) and *WAI commands to synchronize all pending operations to the execution of this command.

Syntax :INITiate[:IMMediate]

Arguments None

Measurement Views All

Examples :INITiate:IMMediate
starts input signal acquisition.

Related Commands *OPC, *TRG, *WAI, :INITiate:CONTinuous

INPut Commands

The INPut commands control the characteristics of the signal input.

Command Tree

Header	Parameter
:INPut	
[:RF]	
:ATTenuation	<numeric_value>
:AUTO	<boolean>
:GAIN	
:STATe	<boolean>
:MLEVel :RLEVel	<numeric_value>

:INPut[:RF]:ATTenuation(?)

Sets or queries the input attenuation. Programming a specified attenuation sets :INPut[:RF]:ATTenuation:AUTO OFF.

Syntax :INPut[:RF]:ATTenuation <value>
 :INPut[:RF]:ATTenuation?

Arguments <value>::=<NR1> specifies the input attenuation.
 Range: 0 to 75 dB in 5 dB steps.

Measurement Views All

Examples :INPut:RF:ATTenuation 20
 sets the input attenuation to 20 dB.

Related Commands :INPut[:RF]:ATTenuation:AUTO

:INPut[:RF]:ATTenuation:AUTO(?)

Determines whether to set the input attenuation automatically or manually.

Syntax :INPut[:RF]:ATTenuation:AUTO { OFF | ON | 0 | 1 }
 :INPut[:RF]:ATTenuation:AUTO?

Arguments OFF or 0 specifies that the input attenuation is set manually.
 To set it, use the :INPut[:RF]:ATTenuation command.

 ON or 1 specifies that the input attenuation is set automatically according to the reference level.

Measurement Views All

Examples :INPut:RF:ATTenuation:AUTO ON
 specifies that the input attenuation is set automatically.

Related Commands :INPut[:RF]:ATTenuation

:INPut[:RF]:GAIN:STATe(?)***Option 01 Only***

Determines whether to enable or disable the internal pre-amp.

Syntax :INPut[:RF]:GAIN:STATe { OFF | ON | 0 | 1 }
 :INPut[:RF]:GAIN:STATe?

Arguments OFF or 0 disables the internal pre-amp.
 ON or 1 enables the internal pre-amp.

Measurement Views All

Examples :INPut:RF:GAIN:STATe ON
 enables the internal pre-amp.

:INPut:MLEVel|:RLEVel(?)

Sets or queries the reference level.

Syntax :INPut:MLEVel|:RLEVel <value>
 :INPut:MLEVel|:RLEVel?

Arguments <value>::=<NRf> specifies the reference level.
 Range: -170 to +50 dBm.

Measurement Views All

Examples :INPut:RLEVel -10
 sets the reference level to -10 dBm.

MMEMory Commands

The :MMEMory commands allow you to manipulate files on the mass memory devices. For handling files, refer to the *RSA6100A Series Quick Reference User Manual*. These commands are divided by measurement views into the subgroups listed in Table 2-37.

Table 2-37: MMEMory command subgroups

Command header	Measurement view	Refer to:
:MMEMory (basic)	All views, general file control	page 2-446
:MMEMory:AVTime	Amplitude versus Time	page 2-454
:MMEMory:CCDF	CCDF	page 2-456
:MMEMory:DPSA	DPX (Digital Phosphor) spectrum	page 2-458
:MMEMory:FVTime	Frequency versus Time	page 2-460
:MMEMory:IQVTime	RF I&Q versus Time	page 2-462
:MMEMory:PHVTime	Phase versus Time	page 2-465
:MMEMory:SPECTrum	Spectrum	page 2-467

NOTE. For the data file formats, refer to the RSA6100A Series Online Help.

Specifying the File

For loading and storing a file, specify the file following these rules:

- You can omit the file extension to load and store data. The measurement-specific extension is automatically added.
- You can use the absolute path to specify the file name. For example, specify the *SAMPLE1* file in the *My Documents* folder on the C drive as "C:\My Documents\SAMPLE1".
- If you omit the directory path, the default path is used, which is C:\Program Files\Tektronix\RSA6100A initially.

Once a file is saved to a different directory, the new directory will be used as the default for all load and store operations.

:MMEMory Basic Command Subgroup

The :MMEMory basic commands control loading and storing files.

Command Tree	Header	Parameter
	:MMEMory	
	:CALibration	
	:LOAD	
	:CORRection	
	:EXternal	
	:EDIT<x>	<file_name>
	:STORe	
	:CORRection	
	:EXternal	
	:EDIT<x>	<file_name>
	:LOAD	
	:IQ	<file_name>
	:STATe	<file_name>
	:TRACe	<file_name>
	:STORe	
	:IQ	<file_name>
	:CSV	<file_name>
	:MAT	<file_name>
	:MSTate	<file_name>
	:RESuIts	<file_name>
	:STATe	<file_name>
	:TRACe	<file_name>

:MMEMory:CALibration:LOAD:CORRection:EXternal:EDIT<x> (No Query Form)

Loads the external loss table from a specified file.

Syntax :MMEMory:CALibration:LOAD:CORRection:EXternal:EDIT<x>
<file_name>

Where <x> = 1 to 3 represent External Loss Table 1 to 3, respectively.

Arguments <file_name>::=<string> specifies the file to load the external loss table from. The file extension is .csv. You can omit the extension.

Measurement Views All

Examples :MMEMory:CALibration:LOAD:CORRection:EXternal:EDIT1 "Table1"
loads the External Loss Table 1 from the *Table1.csv* file.

:MMEMory:CALibration:STORe:CORRection:EXternal:EDIT<x> (No Query Form)

Stores the external loss table to a specified file.

Syntax :MMEMory:CALibration:STORe:CORRection:EXternal:EDIT<x>
<file_name>

Where <x> = 1 to 3 represent External Loss Table 1 to 3, respectively.

Arguments <file_name>::=<string> specifies the file to store the external loss table to. The file extension is .csv. You can omit the extension.

Measurement Views All

Examples :MMEMory:CALibration:STORe:CORRection:EXternal:EDIT1 "Table1"
stores the External Loss Table 1 to the *Table1.csv* file.

:MMEMory:LOAD:IQ (No Query Form)

Loads time-domain IQ waveform into the acquisition memory from a file.

Syntax :MMEMory:LOAD:IQ <file_name>

Arguments <file_name>::=<string> specifies the file to load IQ data from.
The file extension is .tiq. You can omit the extension.

Measurement Views All

Examples :MMEMory:LOAD:IQ "IQ1"
loads IQ data from the *IQ1.tiq* file.

:MMEMory:LOAD:STATe (No Query Form)

Loads the instrument setup from a specified file for the currently selected view.

Syntax :MMEMory:LOAD:STATe <file_name>

Arguments <file_name>::=<string> specifies the file to load the instrument setup from.
The file extension is .setup. You can omit the extension.

Measurement Views All

Examples :MMEMory:LOAD:STATe "STATE1"
loads the instrument setup from the *STATE1.setup* file.

:MMEMory:LOAD:TRACe (No Query Form)

Loads the trace data from a specified file for the currently selected view.

Syntax :MMEMory:LOAD:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file to load the trace data from. The file extension is named for the measurement view as shown in Table 2-38. The trace file is not available in some views which are indicated by “NA” in the file extension column.

For the views that allow multiple-trace display, select the trace to load or store using the command listed in the trace selection column in Table 2-38. You can load the specified trace with any trace data that you saved in the view if the traces have the same units. For example, you can load Trace 2 with Trace 1 data that you saved.

Table 2-38: Trace file extension and trace selection command

Display group	Measurement view	File extension	Trace selection
General signal viewing	Spectrum	Specan	:TRACe<x>:SPECtrum:SElect
	DPX spectrum	dpt	:TRACe<x>:DPSA:SElect
	Amplitude versus Time	AmplVsTime	:TRACe<x>:AVTime:SElect
	Frequency versus Time	FreqVsTime	NA
	Phase versus Time	PhaseVsTime	NA
	RF I&Q versus Time	RFIQVsTime	NA
	Spectrogram	Sogram	NA
	Time overview	NA	NA
General purpose digital modulation (Option 21 only)	Constellation	NA	NA
	EVM versus Time	NA	NA
	Magnitude error versus Time	NA	NA
	Phase error versus Time	NA	NA
	Signal quality	NA	NA
	Symbol table	NA	NA
RF measurements	CCDF	CCDF	:TRACe<x>:CCDF:SElect
	Channel power and ACPR	NA	NA
	MCPR	NA	NA
	Occupied Bandwidth	NA	NA

Table 2-38: Trace file extension and trace selection command (Cont.)

Display group	Measurement view	File extension	Trace selection
Pulsed RF (Option 20 only)	Pulse statistics	NA	NA
	Pulse table	NA	NA
	Pulse trace	NA	NA

Measurement Views Refer to Table 2-38.

Examples :MMEMory:LOAD:TRACe "TRACE1"
loads the trace data from the *TRACE1.Specan* file when the spectrum view is selected.

Related Commands :TRACe<x>:AVTime:SElect, :TRACe<x>:CCDF:SElect,
:TRACe<x>:DPSA:SElect, :TRACe<x>:SPECtrum:SElect

:MMEMory:STORe:IQ (No Query Form)

Saves time-domain IQ waveform in the acquisition memory to a specified file.

Syntax :MMEMory:STORe:IQ <file_name>

Arguments <file_name>::=<string> specifies the file to save IQ data.
The file extension is .tiq. You can omit the extension.

Measurement Views All

Examples :MMEMory:STORe:IQ "IQ1"
saves IQ data to the *IQ1.tiq* file.

:MMEMory:STORe:IQ:CSV (No Query Form)

Saves time-domain IQ waveform in the acquisition memory to a specified file in the CSV (Comma Separated Values) format, allowing you to export the file into Microsoft Excel or other database systems.

Syntax :MMEMory:STORe:IQ:CSV <file_name>

Arguments <file_name>::=<string> specifies the file to save IQ data.
The file extension is .csv. You can omit the extension.

Measurement Views All

Examples :MMEMory:STORe:IQ:CSV "IQ2"
saves IQ data to the *IQ2.csv* file.

:MMEMory:STORe:IQ:MAT (No Query Form)

Saves time-domain IQ waveform in the acquisition memory to a specified file in the MATLAB format, allowing you to export the file into the MATLAB technical computing environment.

Syntax :MMEMory:STORe:IQ:MAT <file_name>

Arguments <file_name>::=<string> specifies the file to save IQ data.
The file extension is .mat. You can omit the extension.

Measurement Views All

Examples :MMEMory:STORe:IQ:MAT "IQ3"
saves IQ data to the *IQ3.mat* file.

:MMEMory:STORe:MSTate (No Query Form)

Stores the measurement parameters to a specified file in the ASCII text format for the currently selected view, allowing you to export the file into other applications.

Syntax :MMEMory:STORe:MSTate <file_name>

Arguments <file_name>::=<string> specifies the file to store the measurement parameters. The file extension is .txt. You can omit the extension.

Measurement Views All

Examples :MMEMory:STORe:MSTate "MSTATE1"
stores the measurement parameters to the *MSTATE1.txt* file.

:MMEMory:STORe:RESults (No Query Form)

Stores the measurement results including measurement parameters and trace data to a specified file in the CSV (Comma Separated Values) format for the currently selected view, allowing you to export the file into Microsoft Excel or other database systems.

Syntax :MMEMory:STORe:RESults <file_name>

Arguments <file_name>::=<string> specifies the file to store the measurement results. The file extension is .csv. You can omit the extension.

Measurement Views All

Examples :MMEMory:STORe:RESults "RESULT1"
stores the measurement results to the *RESULT1.csv* file.

:MMEMory:STORe:STATe (No Query Form)

Stores the instrument setup to a specified file for the currently selected view.

Syntax :MMEMory:STORe:STATe <file_name>

Arguments <file_name>::=<string> specifies the file to store the instrument setup. The file extension is .setup. You can omit the extension.

Measurement Views All

Examples :MMEMory:STORe:STATe "STATE1"
stores the instrument setup in the *STATE1.setup* file.

:MMEMory:STORe:TRACe (No Query Form)

Stores the trace data in a specified file for the currently selected view.

Syntax :MMEMory:STORe:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file to store the trace data in. The file extension is named for the measurement view as shown in Table 2-38 on page 2-449. The trace file is not available in some views which are indicated by “NA” in the file extension column. For the views that allow multiple-trace display, select the trace to load or store using the command listed in the trace selection column.

Measurement Views Refer to Table 2-38 on page 2-449.

Examples :MMEMory:STORe:TRACe "TRACE1"
stores the trace data in the *TRACE1.Specan* file when the spectrum view is selected.

:MMEMory:AVTime Subgroup

The :MMEMory:AVTime commands control the mass storage in the Amplitude versus Time measurement.

Command Tree	Header	Parameter
	:MMEMory	
	:AVTime	
	:LOAD	
	:TRACe<x>	<file_name>
	:STORe	
	:TRACe<x>	<file_name>

Where <x> = 1 to 4.

TRACe1: Trace 1

TRACe2: Trace 2

TRACe3: Trace 3

TRACe4: Math trace (for store only)

:MMEMory:AVTime:LOAD:TRACe<x> (No Query Form)

Loads the Amplitude versus Time trace data from the specified file.

Syntax :MMEMory:AVTime:LOAD:TRACe<x> <file_name>

Where <x> = 1 to 3; Trace 4 (math trace) is invalid.

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .AmplVsTime. You can omit the extension.

Measurement Views Amplitude versus Time

Examples :MMEMory:AVTime:LOAD:TRACe1 "Sample1"
loads Trace 1 data from the *Sample1.AmplVsTime* file.

:MMEMory:AVTime:STORE:TRACe<x> (No Query Form)

Stores the Amplitude versus Time trace data in the specified file.

Syntax :MMEMory:AVTime:STORE:TRACe<x> <file_name>

Where <x> = 1 to 4; All traces are valid.

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .AmplVsTime. You can omit the extension.

Measurement Views Amplitude versus Time

Examples :MMEMory:AVTime:STORE:TRACe1 "Sample1"
stores Trace 1 data in the *Sample1.AmplVsTime* file.

:MMEMory:CCDF Subgroup

The :MMEMory:CCDF commands control the mass storage in the CCDF measurement.

Command Tree	Header	Parameter
	:MMEMory	
	:CCDF	
	:LOAD	
	:TRACe<x>	<file_name>
	:STORe	
	:TRACe<x>	<file_name>

Where <x> = 1 or 2.
TRACe1: Trace 1
TRACe2: Trace 2
TRACe3 (Gaussian reference curve) is invalid.

:MMEMory:CCDF:LOAD:TRACe<x> (No Query Form)

Loads the CCDF trace data from the specified file.

Syntax :MMEMory:CCDF:LOAD:TRACe<x> <file_name>

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .CCDF. You can omit the extension.

Measurement Views CCDF

Examples :MMEMory:CCDF:LOAD:TRACe1 "Sample1"
loads Trace 1 data from the *Sample1.CCDF* file.

:MMEMory:CCDF:STORe:TRACe<x> (No Query Form)

Stores the CCDF trace data in the specified file.

Syntax :MMEMory:CCDF:STORe:TRACe<x> <file_name>

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .CCDF. You can omit the extension.

Measurement Views CCDF

Examples :MMEMory:CCDF:STORe:TRACe1 "Sample1"
stores Trace 1 data in the *Sample1.CCDF* file.

:MMEMory:DPSA Subgroup

The :MMEMory:DPSA commands control the mass storage in the DPX (Digital Phosphor) spectrum measurement.

Command Tree	Header	Parameter
	:MMEMory	
	:DPSA	
	:LOAD	
	:TRACe<x>	<file_name>
	:STORe	
	:TRACe<x>	<file_name>

Where <x> = 1 to 5. Each trace is defined as follows:

TRACe1: Maximum trace
TRACe2: Minimum trace
TRACe3: Average trace
TRACe4: Math trace (for store only)
TRACe5: Bitmap trace

:MMEMory:DPSA:LOAD:TRACe<x> (No Query Form)

Loads the DPX spectrum trace data from the specified file.

Syntax :MMEMory:DPSA:LOAD:TRACe<x> <file_name>

Where <x> = 1, 2, 3, or 5; TRACe4 (math trace) is invalid.

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .dpt. You can omit the extension.

Measurement Views DPX spectrum

Examples :MMEMory:DPSA:LOAD:TRACe1 "Sample1"
loads Trace 1 data from the *Sample1.dpt* file.

:MMEMory:DPSA:STORe:TRACe<x> (No Query Form)

Stores the DPX spectrum trace data in the specified file.

Syntax :MMEMory:DPSA:STORe:TRACe<x> <file_name>

Where <x> = 1 to 5; All traces are valid.

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .dpt. You can omit the extension.

Measurement Views DPX spectrum

Examples :MMEMory:DPSA:STORe:TRACe1 "Sample1"
stores Trace 1 data in the *Sample1.dpt* file.

:MMEMory:FVTime Subgroup

The :MMEMory:FVTime commands control the mass storage in the Frequency versus Time measurement.

Command Tree	Header	Parameter
	:MMEMory	
	:FVTime	
	:LOAD	
	:TRACe	<file_name>
	:STORe	
	:TRACe	<file_name>

:MMEMory:FVTime:LOAD:TRACe (No Query Form)

Loads the Frequency versus Time trace data from the specified file.

Syntax :MMEMory:FVTime:LOAD:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .FreqVsTime. You can omit the extension.

Measurement Views Frequency versus Time

Examples :MMEMory:FVTime:LOAD:TRACe "Sample1"
loads the Frequency versus Time trace data from the *Sample1.FreqVsTime* file.

:MMEMory:FVTime:STORe:TRACe (No Query Form)

Stores the Frequency versus Time trace data in the specified file.

Syntax :MMEMory:FVTime:STORe:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .FreqVsTime. You can omit the extension.

Measurement Views Frequency versus Time

Examples :MMEMory:FVTime:STORe:TRACe "Sample1"
stores the Frequency versus Time trace data in the *Sample1.FreqVsTime* file.

:MMEMory:IQVTime Subgroup

The :MMEMory:IQVTime commands control the mass storage in the RF I&Q versus Time measurement.

Command Tree	Header	Parameter
	:MMEMory	
	:IQVTime	
	:LOAD	
	:TRACe	
	:I	<file_name>
	:Q	<file_name>
	:STORe	
	:TRACe	
	:I	<file_name>
	:Q	<file_name>

:MMEMory:IQVTime:LOAD:TRACe:I (No Query Form)

Loads I trace data from the specified file.

Syntax :MMEMory:IQVTime:LOAD:TRACe:I <file_name>

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .RFIQVsTime. You can omit the extension.

Measurement Views RF I&Q versus Time

Examples :MMEMory:IQVTime:LOAD:TRACe:I "Sample1"
loads the I trace data from the *Sample1.RFIQVsTime* file.

:MMEMory:IQVTime:LOAD:TRACe:Q (No Query Form)

Loads Q trace data from the specified file.

Syntax :MMEMory:IQVTime:LOAD:TRACe:Q <file_name>

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .RFIQVsTime. You can omit the extension.

Measurement Views RF I&Q versus Time

Examples :MMEMory:IQVTime:LOAD:TRACe:I "Sample2"
loads the I trace data from the *Sample2.RFIQVsTime* file.

:MMEMory:IQVTime:STORe:TRACe:I (No Query Form)

Stores I trace data in the specified file.

Syntax :MMEMory:IQVTime:STORe:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .RFIQVsTime. You can omit the extension.

Measurement Views RF I&Q versus Time

Examples :MMEMory:IQVTime:STORe:TRACe "Sample1"
stores the I trace data in the *Sample1.RFIQVsTime* file.

:MMEMory:IQVTime:STORe:TRACe:Q (No Query Form)

Stores Q trace data in the specified file.

Syntax :MMEMory:IQVTime:STORe:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .RFIQVsTime. You can omit the extension.

Measurement Views RF I&Q versus Time

Examples :MMEMory:IQVTime:STORe:TRACe "Sample2"
stores the Q trace data in the *Sample2.RFIQVsTime* file.

:MMEMory:PHVTime Subgroup

The :MMEMory:PHVTime commands control the mass storage in the Phase versus Time measurement.

Command Tree	Header	Parameter
	:MMEMory	
	:PHVTime	
	:LOAD	
	:TRACe	<file_name>
	:STORe	
	:TRACe	<file_name>

:MMEMory:PHVTime:LOAD:TRACe (No Query Form)

Loads the Phase versus Time trace data from the specified file.

Syntax :MMEMory:PHVTime:LOAD:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .PhaseVsTime. You can omit the extension.

Measurement Views Phase versus Time

Examples :MMEMory:PHVTime:LOAD:TRACe "Sample1"
loads the Phase versus Time trace data from the *Sample1.PhaseVsTime* file.

:MMEMory:PHVTime:STORe:TRACe (No Query Form)

Stores the Phase versus Time trace data in the specified file.

Syntax :MMEMory:PHVTime:STORe:TRACe <file_name>

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .PhaseVsTime. You can omit the extension.

Measurement Views Phase versus Time

Examples :MMEMory:PHVTime:STORe:TRACe "Sample1"
stores the Phase versus Time trace data in the *Sample1.PhaseVsTime* file.

:MMEMory:SPECTrum Subgroup

The :MMEMory:SPECTrum commands control the mass storage in the Spectrum measurement.

Command Tree	Header	Parameter
	:MMEMory	
	:SPECTrum	
	:LOAD	
	:TRACe<x>	<file_name>
	:STORe	
	:TRACe<x>	<file_name>

Where <x> = 1 to 5. Each trace is defined as follows:

TRACe1: Trace 1
TRACe2: Trace 2
TRACe3: Trace 3
TRACe4: Math trace (for store only)
TRACe5: Spectrogram (for store only)

:MMEMory:SPECTrum:LOAD:TRACe<x> (No Query Form)

Loads the spectrum trace data from the specified file.

Syntax :MMEMory:SPECTrum:LOAD:TRACe<x> <file_name>

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Arguments <file_name>::=<string> specifies the file from which to load trace data. The file extension is .Specan. You can omit the extension.

Measurement Views Spectrum

Examples :MMEMory:SPECTrum:LOAD:TRACe1 "Sample1"
loads Trace 1 data from the *Sample1.Specan* file.

:MMEMory:SPECTrum:STORe:TRACe<x> (No Query Form)

Stores the spectrum trace data in the specified file.

Syntax :MMEMory:SPECTrum:STORe:TRACe<x> <file_name>

Where <x> = 1 to 5; All traces are valid.

NOTE. TRACe5 (spectrogram) is valid when the spectrum and spectrogram measurements are running.

Arguments <file_name>::=<string> specifies the file in which to store trace data. The file extension is .Specan. You can omit the extension.

Measurement Views Spectrum

Examples :MMEMory:SPECTrum:STORe:TRACe1 "Sample1"
stores Trace 1 data in the *Sample1.Specan* file.

OUTPut Commands

The :OUTPut commands control the characteristics of the signal output.

Command Tree

Header	Parameter
:OUTPut	
:IF	<boolean>
:BANDwidth	
:BWIDth	FLATtop GAUSSian
[:STATe]	<boolean>
:IQ	<boolean>
:NOISe	
[:STATe]	<boolean>

:OUTPut:IF:BANDwidth|:BWIDth(?)**Option 05 Only**

Selects or queries the IF output filter when :OUTPut:IF[:STATe] is set to ON.

Syntax :OUTPut:IF:BANDwidth|:BWIDth { FLATtop | GAUSSian }
:OUTPut:IF:BANDwidth|:BWIDth?

Arguments FLATtop selects the flattop filter.
GAUSSian selects the Gaussian filter.

Measurement Views All

Examples :OUTPut:IF:BANDwidth GAUSSian
selects the Gaussian filter for the IF output.

Related Commands :OUTPut:IF[:STATe]

:OUTPut:IF[:STATe](?)**Option 05 Only**

Determines whether to turn on or off the 500 MHz IF Out on the rear panel.

Syntax :OUTPut:IF[:STATe] { OFF | ON | 0 | 1 }
:OUTPut:IF[:STATe]?

Arguments OFF or 0 turns off IF Out.
ON or 1 turns on IF Out.

Measurement Views All

Examples :OUTPut:IF:STATe ON
turns on IF Out.

Related Commands :OUTPut:IF:BANDwidth|:BWIDth

:OUTPut:IQ[:STATe](?)*Option 05 Only*

Determines whether to enable or disable the digital IQ output data stream from the rear panel connectors.

Syntax :OUTPut:IQ[:STATe] { 0 | 1 | OFF | ON }
:OUTPut:IQ[:STATe]?

Arguments OFF or 0 disables the digital IQ output.
ON or 1 enables the digital IQ output.
At *RST, this value is set to OFF.

Measurement Modes All

Examples :OUTPut:IQ:STATe ON
enables the digital IQ output.

:OUTPut:NOISe[:STATe](?)

Determines whether to turn on or off the +28 V DC Out on the rear panel.

Syntax :OUTPut:NOISe[:STATe] { OFF | ON | 0 | 1 }
:OUTPut:NOISe[:STATe]?

Arguments OFF or 0 turns off +28 V DC Out.
ON or 1 turns on +28 V DC Out.

Measurement Views All

Examples :OUTPut:NOISe:STATe ON
turns on +28 V DC Out.

READ Commands

The READ commands acquire an input signal once in the single mode and obtain the measurement results from that data.

To fetch the measurement results from the data currently residing in the memory without acquiring the input signal, use the :FETCh commands.

The READ commands are divided by measurement views into the subgroups listed in Table 2-39.

Table 2-39: READ command subgroups

Command header	Measurement view	Refer to:
:READ:ACPower	Channel power and ACPR	page 2-474
:READ:AVTime	Amplitude versus Time	page 2-477
:READ:CCDF	CCDF	page 2-482
:READ:CONSt	Constellation (Option 21 only)	page 2-485
:READ:DDEMod	General purpose digital modulation measurements (Option 21 only)	page 2-487
:READ:DPSA	DPX (Digital Phosphor) spectrum	page 2-488
:READ:EVM	EVM versus Time (Option 21 only)	page 2-492
:READ:FVTime	Frequency versus Time	page 2-495
:READ:IQVTime	RF I&Q versus Time	page 2-499
:READ:MCPower	MCPR (Multiple Carrier Power Ratio)	page 2-504
:READ:MERRor	Magnitude error versus Time (Option 21 only)	page 2-509
:READ:OBW	OBW (Occupied Bandwidth)	page 2-512
:READ:PERRor	Phase error versus Time (Option 21 only)	page 2-521
:READ:PHVTime	Phase versus Time	page 2-524
:READ:PULSe	Pulsed RF measurements (Option 20 only)	page 2-528
:READ:SGRam	Spectrogram	page 2-567
:READ:SPECtrum	Spectrum	page 2-568
:READ:SQUality	Signal quality (Option 21 only)	page 2-570
:READ:TOVerview	Time overview	page 2-581

:READ:ACPower Subgroup

The :READ:ACPower commands returns the results of the Channel power and ACPR (Adjacent Channel Power Ratio) measurement.

Command Tree	Header	Parameter
	:READ	
	:ACPower?	
	:CHANnel	
	:POWer?	
	:SPECTrum?	

:READ:ACPower? (Query Only)

Returns the Channel power and ACPR measurement results for all available channels.

Syntax :READ:ACPower?

Arguments None

Returns <chan_power>,<acpr_lower(1)>,<acpr_upper(1)>,
<acpr_lower(2)>,<acpr_upper(2)>,...
<acpr_lower(n)>,<acpr_upper(n)>

Where

<chan_power> is the average power of the main channel as the power reference in dBm.

<acpr_lower(n)> is the ACPR for the lower channel #n in dB.

<acpr_upper(n)> is the ACPR for the upper channel #n in dB.

The number of n depends on the setting of the [:SENSe]:ACPower:CHANnel:PAIRs command.

Measurement Views Channel power and ACPR

Examples :READ:ACPower?
might return 4.227,-28.420,-23.847,-22.316,-29.225 indicating
(average power of the main channel) = 4.227 dBm,
(ACPR for the lower channel 1) = -28.420 dB,
(ACPR for the upper channel 1) = -23.847 dB,
(ACPR for the lower channel 2) = -22.316 dB, and
(ACPR for the upper channel 2) = -29.225 dB.

Related Commands [:SENSe]:ACPower:CHANnel:PAIRs

:READ:ACPower:CHANnel:POWer? (Query Only)

Returns the average power of the main channel (power reference) in the Channel power and ACPR measurement.

Syntax :READ:ACPower:CHANnel:POWer?

Arguments None

Returns <chan_power>::=<NRf> is the average power of the main channel in dBm.

Measurement Views Channel power and ACPR

Examples :READ:ACPower:CHANnel:POWer?
might return 4.227 indicating that the average power of the main channel is 4.227 dBm.

:READ:ACPower:SPECTrum? (Query Only)

Returns spectrum trace data of the Channel power and ACPR measurement.

Syntax :READ:ACPower:SPECTrum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the spectrum trace data in dBm for the point n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Channel power and ACPR

Examples :READ:ACPower:SPECTrum?
might return #43204xxxx... (3204-byte data) for the spectrum trace data of the Channel power and ACPR measurement.

:READ:AVTime Subgroup

The :READ:AVTime commands returns the results of the Amplitude versus Time measurement.

Command Tree	Header	Parameter
	:READ	
	:AVTime	
	:AVERage	
	:FIRSt :SECond :THIRd :FOURth	
	:MAXimum	
	:MAXLocation	
	:MINimum	
	:MINLocation	
	:RESult	

NOTE. Except for the :READ:AVTime:FIRSt|:SECond|:THIRd|:FOURth command, select the trace using the :TRACe<x>:AVTime:SElect command.

The unit of amplitude is defaulted to dBm. It can be changed by the [:SENSe]:POWer:UNITs command.

:READ:AVTime:AVERage? (Query Only)

Returns the RMS (root-mean-square) value for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax	:READ:AVTime:AVERage?
Arguments	None
Returns	<avg>::=<NRf> is the RMS amplitude in dBm.
Measurement Views	Amplitude versus Time
Examples	:READ:AVTime:AVERage? might return -2.53 indicating the RMS amplitude is -2.53 dBm.
Related Commands	:TRACe<x>:AVTime:SElect

:READ:AVTime:FIRSt|:SECond|:THIRd|:FOURth? (Query Only)

Returns the trace data in the Amplitude versus Time measurement.

Syntax :READ:AVTime:FIRSt|:SECond|:THIRd|:FOURth?

Where FIRSt, SECond, THIRd, and FOURth represent Trace 1 to 4, respectively. Each trace is defined as follows:

FIRSt:	Trace 1
SECond:	Trace 2
THIRd:	Trace 3
FOURth:	Math trace

The traces can be specified by the :TRACe<x>:AVTime command subgroup.

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Amplitude versus Time

Examples :READ:AVTime:FIRSt?
might return #3156xxxx... (156-byte data) for Trace 1.

Related Commands :TRACe<x>:AVTime command subgroup

:READ:AVTime:MAXimum? (Query Only)

Returns the maximum value for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :READ:AVTime:MAXimum?

Arguments None

Returns <max>::=<NRf> is the maximum Amplitude in dBm.

Measurement Views Amplitude versus Time

Examples :READ:AVTime:MAXimum?
might return -2.84 indicating the maximum amplitude is -2.84 dBm.

Related Commands :READ:AVTime:MAXLocation?, :TRACe<x>:AVTime:SElect

:READ:AVTime:MAXLocation? (Query Only)

Returns the time at which the amplitude is maximum for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElec command.

Syntax :READ:AVTime:MAXLocation?

Arguments None

Returns <max_time>::=<NRf> is the time at the maximum in seconds.

Measurement Views Amplitude versus Time

Examples :READ:AVTime:MAXLocation?
might return 25.03E-9 indicating the amplitude is maximum at 25.03 ns.

Related Commands :READ:AVTime:MAXimum?, :TRACe<x>:AVTime:SElect

:READ:AVTime:MINimum? (Query Only)

Returns the minimum value for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :READ:AVTime:MINimum?

Arguments None

Returns <min>::=<NRf> is the minimum amplitude in dBm.

Measurement Views Amplitude versus Time

Examples :READ:AVTime:MINimum?
might return -57.64 indicating the minimum amplitude is -57.64 dBm.

Related Commands :READ:AVTime:MINLocation?, :TRACe<x>:AVTime:SElect

:READ:AVTime:MINLocation? (Query Only)

Returns the time at which the amplitude is minimum for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :READ:AVTime:MINLocation?

Arguments None

Returns <min_time>::=<NRf> is the time at the minimum in seconds.

Measurement Views Amplitude versus Time

Examples :READ:AVTime:MINLocation?
might return 450.7E-9 indicating the amplitude is minimum at 450.7 ns.

Related Commands :READ:AVTime:MINimum?, :TRACe:AVTime:SElect

:READ:AVTime:RESult? (Query Only)

Returns the measurement results for the selected trace in the Amplitude versus Time measurement. Select the trace using the :TRACe<x>:AVTime:SElect command.

Syntax :READ:AVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>,<rms>

Where

<max>::=<NRf> is the maximum amplitude in dBm.

<max_time>::=<NRf> is the time at the maximum in seconds.

<min>::=<NRf> is the minimum amplitude in dBm.

<min_time>::=<NRf> is the time at the minimum in seconds.

<rms>::=<NRf> is the RMS amplitude in dBm.

Measurement Views Amplitude versus Time

Examples :READ:AVTime:RESult?
might return -2.68,48.62E-6,-82.47,22.11E-6,-8.24 indicating that the maximum amplitude is -2.68 dBm at 48.62 μ s, the minimum amplitude is -82.47 dBm at 22.11 μ s, and the RMS amplitude is -8.24 dBm

Related Commands :TRACe<x>:AVTime:SElect

:READ:CCDF Subgroup

The :READ:CCDF commands returns the results of the CCDF (Complementary Cumulative Distribution Function) measurement.

Command Tree	Header	Parameter
	:READ	
	:CCDF?	
	:FIRSt? :SECond? :THIRd?	

:READ:CCDF? (Query Only)

Returns the CCDF measurement results.

Syntax :READ:CCDF?

Arguments None

Returns <avg_amp1>,<avg_ccdf>,<crest_factor>,<aml_10>,<aml_1>,<aml_p1>,<aml_p01>,<aml_p001>,,<aml_p0001>

Where

<avg_amp1> is the average amplitude in dBm.

(The unit can be changed by the [:SENSe]:POWer:UNITs command.)

<avg_ccdf> is the average CCDF in percent.

<crest_factor> is the crest factor in dB.

<aml_10> is the amplitude at CCDF of 10% in dB.

<aml_1> is the amplitude at CCDF of 1% in dB.

<aml_p1> is the amplitude at CCDF of 0.1% in dB.

<aml_p01> is the amplitude at CCDF of 0.01% in dB.

<aml_p001> is the amplitude at CCDF of 0.001% in dB.

<aml_p0001> is the amplitude at CCDF of 0.0001% in dB.

Measurement Views CCDF

Examples :READ:CCDF?
might return -33.35,35.8,9.75,3.88,7.07,8.50,9.25,9.72,9.74
indicating
(average amplitude) = -33.35 dBm,
(average CCDF) = 35.8%,
(crest factor) = 9.75 dB,
(amplitude at CCDF of 10%) = 3.88 dB,
(amplitude at CCDF of 1%) = 7.07 dB,
(amplitude at CCDF of 0.1%) = 8.50 dB,
(amplitude at CCDF of 0.01%) = 9.25 dB,
(amplitude at CCDF of 0.001%) = 9.72 dB, and
(amplitude at CCDF of 0.0001%) = 9.74 dB.

Related Commands [:SENSe]:POWer:UNITs

:READ:CCDF:FIRSt|:SECond|:THIRd? (Query Only)

Returns waveform data of the specified trace in the CCDF measurement.

NOTE. This query is invalid when [:SENSe]:CCDF:TIME:TYPE is set to CONTinuous or TOTal.

Syntax :READ:CCDF:FIRSt|:SECond|:THIRd?

Where FIRSt, SECond, and THIRd represent Trace 1 to 3, respectively.
Each trace is defined as follows:

FIRSt:	Trace 1
SECond:	Trace 2
THIRd:	Gaussian reference curve

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the waveform data of the specified trace for the point n in percent, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views CCDF

Examples :READ:CCDF:FIRSt?
might return #41024xxxx... (1024-byte data) for the waveform data of Trace 1.

Related Commands [:SENSe]:CCDF:TIME:TYPE

:READ:CONSte Subgroup (Option 21 Only)

The :READ:CONSte commands returns the results of the Constellation measurement.

Command Tree	Header	Parameter
	:READ	
	:CONSte	
	:RESuLts?	
	:TRACe?	

:READ:CONSte:RESuLts? (Query Only)

Returns the constellation measurement results of EVM RMS, peak and location displayed on the bottom of the screen.

Syntax :READ:CONSte:RESuLts?

Arguments None

Returns <EVM_RMS>,<EVM_peak>,<location>

Where

<EVM_RMS>::=<NRf> is the RMS EVM in percent (%).

<EVM_peak>::=<NRf> is the peak EVM in percent (%).

<location>::=<NRf> is the peak location in symbol number.

Measurement Views Constellation

Examples :READ:CONSte:RESuLts?

might return 2.841,3.227,68.000, indicating that the RMS EVM is 2.841% and the peak EVM is 3.227% at symbol #68.

:READ:CONStE:TRACe? (Query Only)

Returns the constellation trace data.

Syntax :READ:CONStE:TRACe?

Arguments None

Returns #<num_digit><num_byte><I(1)><Q(1)><I(2)><Q(2)>...<I(n)><Q(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<I(n)> and <Q(n)> are the normalized I- and Q-coordinate values at the nth data point. 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Constellation

Examples :READ:CONStE:TRACe?
might return #43848xxxx... (3848-byte data) for the constellation trace data.

:READ:DDEMod Subgroup (Option 21 Only)

The :READ:DDEMod commands returns the results of the General Purpose Digital Modulation measurements.

Command Tree	Header	Parameter
	:READ	
	:DDEMod	
	:STABLe?	

:READ:DDEMod:STABLe? (Query Only)

Returns the symbol table data.

Syntax :READ:DDEMod:STABLe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

- <num_digit> is the number of digits in <num_byte>.
- <num_byte> is the number of bytes of data that follow.
- <data(n)> is the symbol table data for the point n, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Symbol table

Examples :READ:DDEMod:STABLe?
might return #3512xxxx... (512-byte data) for the symbol table.

:READ:DPSA Subgroup

The :READ:DPSA commands returns the results of the DPX (Digital Phosphor) Spectrum measurement.

Command Tree	Header	Parameter
	:READ	
	:DPSA	
	:TRACe	
	:AVERage?	
	:MATH?	
	:MAXimum?	
	:MINimum?	

:READ:DPSA:TRACe:AVERage? (Query Only)

Returns waveform data of the average trace in the DPX spectrum measurement.

Syntax :READ:DPSA:TRACe:AVERage?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the waveform data of the average trace for the point n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views DPX spectrum

Examples :READ:DPSA:TRACe:AVERage?
might return #42004xxxx... (2004-byte data) for the waveform data of the average trace.

:READ:DPSA:TRACe:MATH? (Query Only)

Returns waveform data of the math trace in the DPX spectrum measurement.

Syntax :READ:DPSA:TRACe:MATH?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the waveform data of the math trace for the point n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views DPX spectrum

Examples :READ:DPSA:TRACe:MATH?
might return #42004xxxx... (2004-byte data) for the waveform data of the math trace.

:READ:DPSA:TRACe:MAXimum? (Query Only)

Returns waveform data of the maximum trace in the DPX spectrum measurement.

Syntax :READ:DPSA:TRACe:MAXimum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the waveform data of the maximum trace for the point n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views DPX spectrum

Examples :READ:DPSA:TRACe:MAXimum?
might return #42004xxxx... (2004-byte data) for the waveform data of the maximum trace.

:READ:DPSA:TRACe:MINimum? (Query Only)

Returns waveform data of the minimum trace in the DPX spectrum measurement.

Syntax :READ:DPSA:TRACe:MINimum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the waveform data of the minimum trace for the point n in dBm, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views DPX spectrum

Examples :READ:DPSA:TRACe:MINimum?
might return #42004xxxx... (2004-byte data) for the waveform data of the minimum trace.

:READ:EVM Subgroup (Option 21)

The :READ:EVM commands returns the results of the EVM (Error Vector Magnitude) versus Time measurement.

Command Tree	Header	Parameter
	:READ	
	:EVM	
	:FERRor?	
	:PEAK?	
	:PINDeX?	
	:RMS?	
	:TRACe?	

:READ:EVM:FERRor? (Query Only)

Returns the frequency error in the EVM versus Time measurement.

Syntax :READ:EVM:FERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Measurement Views EVM versus Time

Examples :READ:EVM:FERRor?
might return -10.7E+3 indicating the frequency error is -10.7 kHz.

:READ:EVM:PEAK? (Query Only)

Returns the peak value in the EVM versus Time measurement.

Syntax :READ:EVM:PEAK?

Arguments None

Returns <peak>::=<NRf> is the peak EVM value in percent (%).

Measurement Views EVM versus Time

Examples :READ:EVM:PEAK?
might return 1.32 indicating the peak EVM value is 1.32%.

Related Commands :READ:EVM:PINDEX?

:READ:EVM:PINDEX? (Query Only)

Returns the time at the EVM peak.

Syntax :READ:EVM:PINDEX?

Arguments None

Returns <peak_time>::=<NRf> is the time at the EVM peak in seconds.

You can select the time unit using the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views EVM versus Time

Examples :READ:EVM:PINDEX?
might return 28.912E-6 indicating the time at the EVM peak is 28.912 μ s.

Related Commands :READ:EVM:PEAK?, [:SENSe]:DDEMod:TIME:UNITs

:READ:EVM:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the EVM versus Time measurement.

Syntax :READ:EVM:RMS?

Arguments None

Returns <rms>::=<NRf> is the RMS EVM value in percent (%).

Measurement Views EVM versus Time

Examples :READ:EVM:RMS?
might return 0.582 indicating the RMS EVM value is 0.582%.

:READ:EVM:TRACe? (Query Only)

Returns the EVM versus Time trace data.

Syntax :READ:EVM:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the EVM versus Time trace data for the point n in percent (%), 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views EVM versus Time

Examples :READ:EVM:TRACe?
might return #42036xxxx... (2036-byte data) for the EVM versus Time trace.

:READ:FVTime Subgroup

The :READ:EVM commands returns the results of the Frequency versus Time measurement.

Command Tree	Header	Parameter
	:READ	
	:FVTime?	
	:MAXimum?	
	:MAXLocation?	
	:MINimum?	
	:MINLocation?	
	:RESult?	

:READ:FVTime? (Query Only)

Returns the Frequency versus Time trace data.

Syntax :READ:FVTime?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the frequency drift data for the point n in Hz,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Frequency versus Time

Examples :READ:FVTime?
might return #3156xxxx... (156-byte data) for the Frequency versus Time trace.

:READ:FVTime:MAXimum? (Query Only)

Returns the maximum value in the Frequency versus Time measurement.

Syntax :READ:FVTime:MAXimum?

Arguments None

Returns <max>::=<NRf> is the maximum frequency drift in Hz.

Measurement Views Frequency versus Time

Examples :READ:FVTime:MAXimum?
might return 2.625E+6 indicating the maximum frequency drift is 2.625 MHz.

Related Commands :READ:FVTime:MAXLocation?

:READ:FVTime:MAXLocation? (Query Only)

Returns the time at which the frequency drift is maximum.

Syntax :READ:FVTime:MAXLocation?

Arguments None

Returns <max_time>::=<NRf> is the time in seconds at which the frequency drift is maximum.

Measurement Views Frequency versus Time

Examples :READ:FVTime:MAXLocation?
might return 25.03E-9 indicating the frequency drift is maximum at 25.03 ns.

Related Commands :READ:FVTime:MAXimum?

:READ:FVTime:MINimum? (Query Only)

Returns the minimum value in the Frequency versus Time measurement.

Syntax :READ:FVTime:MINimum?

Arguments None

Returns <min>::=<NRf> is the minimum frequency drift in Hz.

Measurement Views Frequency versus Time

Examples :READ:FVTime:MINimum?
might return -6.618E+6 indicating the minimum frequency drift is -6.618 MHz.

Related Commands :READ:FVTime:MINLocation?

:READ:FVTime:MINLocation? (Query Only)

Returns the time at which the frequency drift is minimum.

Syntax :READ:FVTime:MINLocation?

Arguments None

Returns <min_time>::=<NRf> is the time in seconds at which the frequency drift is minimum.

Measurement Views Frequency versus Time

Examples :READ:FVTime:MAXLocation?
might return 450.7E-9 indicating the frequency drift is minimum at 450.7 ns.

Related Commands :READ:FVTime:MINimum?

:READ:FVTime:RESult? (Query Only)

Returns the Frequency versus Time measurement results.

Syntax :READ:FVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>

Where

<max>::=<NRf> is the maximum frequency drift in Hz.

<max_time>::=<NRf> is the time in seconds at which the frequency drift is maximum.

<min>::=<NRf> is the minimum frequency drift in Hz.

<min_time>::=<NRf> is the time in seconds at which the frequency drift is minimum.

Measurement Views Frequency versus Time

Examples :READ:FVTime:RESult?
might return 2.625E+6,25.03E-9,-6.618E+6,450.7E-9 indicating:
the maximum frequency drift is 2.625 MHz at 25.03 ns and
the minimum frequency drift is -6.618 MHz at 450.7 ns.

:READ:IQVTime Subgroup

The :READ:IQVTime commands returns the results of the RF I&Q versus Time measurement.

Command Tree	Header	Parameter
	:READ	
	:IQVTime?	
	:I?	
	:MAXimum?	
	:MAXLocation?	
	:MINimum?	
	:MINLocation?	
	:Q?	
	:RESult?	

:READ:IQVTime:I? (Query Only)

Returns the I versus Time trace data.

Syntax :READ:IQVTime:I?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the I level data for the point n in volts, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views RF I&Q versus Time

Examples :READ:IQVTime:I?
might return #3160xxxx... (160-byte data) for the I versus Time trace.

:READ:IQVTime:MAXimum? (Query Only)

Returns the maximum value in the RF I&Q versus Time measurement.

Syntax :READ:IQVTime:MAXimum?

Arguments None

Returns <max>::=<NRf> is the maximum I or Q level in volts.

Measurement Views RF I&Q versus Time

Examples :READ:IQVTime:MAXimum?
might return 1.214 indicating the maximum I or Q level is 1.214 V.

Related Commands :READ:IQVTime:MAXLocation?

:READ:IQVTime:MAXLocation? (Query Only)

Returns the time at which the I or Q level is maximum.

Syntax :READ:IQVTime:MAXLocation?

Arguments None

Returns <max_time>::=<NRf> is the time in seconds at which the I or Q level is maximum.

Measurement Views RF I&Q versus Time

Examples :READ:IQVTime:MAXLocation?
might return 175.3E-9 indicating the I or Q level is maximum at 175.3 ns.

Related Commands :READ:IQVTime:MAXimum?

:READ:IQVTime:MINimum? (Query Only)

Returns the minimum value in the RF I&Q versus Time measurement.

Syntax :READ:IQVTime:MINimum?

Arguments None

Returns <min>::=<NRf> is the minimum I or Q level in volts.

Measurement Views RF I&Q versus Time

Examples :READ:IQVTime:MINimum?
might return -370.5E-3 indicating the minimum I or Q level is -370.5 mV.

Related Commands :READ:IQVTime:MINLocation?

:READ:IQVTime:MINLocation? (Query Only)

Returns the time at which the I or Q level is minimum.

Syntax :READ:IQVTime:MINLocation?

Arguments None

Returns <min_time>::=<NRf> is the time in seconds at which the I or Q level is minimum.

Measurement Views RF I&Q versus Time

Examples :READ:IQVTime:MAXLocation?
might return 450.7E-9 indicating the I or Q level is minimum at 450.7 ns.

Related Commands :READ:IQVTime:MINimum?

:READ:IQVTime:Q? (Query Only)

Returns the Q versus Time trace data.

Syntax :READ:IQVTime:Q?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the Q level data for the point n in volts,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views IQ versus Time

Examples :READ:IQVTime:Q?
might return #3160xxxx... (160-byte data) for the Q versus Time trace.

:READ:IQVTime:RESult? (Query Only)

Returns the RF I&Q versus Time measurement results.

Syntax :READ:IQVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>

Where

<max>::=<NRf> is the maximum I or Q level in volts.

<max_time>::=<NRf> is the time in seconds at which the I or Q level is maximum.

<min>::=<NRf> is the minimum I or Q level in volts.

<min_time>::=<NRf> is the time in seconds at which the I or Q level is minimum.

Use the [:SENSe]:IQVTime:TRACe:SElect:I or Q command to select the trace.

Measurement Views RF I&Q versus Time

Examples :READ:IQVTime:RESult?
might return 1.214,175.3E-9,-370.5E-3,450.7E-9 indicating:
the maximum I or Q level is 1.214 V at 175.3 ns and
the minimum I or Q level is -370.5 mV at 450.7 ns.

Related Commands [:SENSe]:IQVTime:TRACe:SElect:I, [:SENSe]:IQVTime:TRACe:SElect:Q

:READ:MCPower Subgroup

The :READ:MCPower commands returns the results of the MCPR (Multiple Carrier Power Ratio) measurement.

Command Tree	Header	Parameter
	:READ	
	:MCPower?	
	:ADJacent	
	:CHANnels	
	:CHANnel	
	:POWer?	
	:MAIN	
	:CHANnels	
	:SPECTrum?	

:READ:MCPower:ADJacent:CHANnels? (Query Only)

Returns the power of adjacent channels in order of increasing frequency.

Syntax :READ:MCPower:ADJacent:CHANnels?

Arguments None

Returns <acpr_lower(n)>,...<acpr_lower(2)>,<acpr_lower(1)>,
 <acpr_upper(1)>,<acpr_upper(2)>,...<acpr_upper(n)>

Where

<acpr_lower(n)> is the ACPR for the lower channel #n in dB.

<acpr_upper(n)> is the ACPR for the upper channel #n in dB.

To add a pair of upper and lower adjacent channels, use the [:SENSe]
:MCPower:CHANnel:ADD:ADJacent command.

Measurement Views MCPR

Examples :READ:MCPower:ADJacent:CHANnels?
might return -4.420,-4.847,-4.316,-4.225 indicating
(ACPR for the lower channel 2) = -4.420 dB,
(ACPR for the lower channel 1) = -4.847 dB,
(ACPR for the upper channel 1) = -4.316 dB, and
(ACPR for the upper channel 2) = -4.225 dB.

Related Commands [:SENSe]:MCPower:CHANnel:ADD:ADJacent

:READ:MCPower:CHANnel:POWer? (Query Only)

Returns the reference power in the MCPR measurement.

Syntax :READ:MCPower:CHANnel:POWer?

Arguments None

Returns <ref_power>::<NRf> is the reference power in dBm.
To select the power reference, use the [:SENSe]:MCPower:RCHannels commands.

Measurement Views MCPR

Examples :READ:MCPower:CHANnel:POWer?
might return 4.227 indicating that the reference power is 4.227 dBm.

Related Commands [:SENSe]:MCPower:RCHannels commands

:READ:MCPower:MAIN:CHANnels? (Query Only)

Returns the power of main channels in order of increasing frequency.

Syntax :READ:MCPower:MAIN:CHANnels?

Arguments None

Returns <power_main(1)>,<power_main(2)>,...<power_main(n)>

Where

<power_main(n)> is the power of main channel #n in dBm.

To specify the main channels, use the [:SENSe]:MCPower:CHANnel:MAIN commands.

Measurement Views MCPR

Examples :READ:MCPower:MAIN:CHANnels?
might return -2.420,-2.847,-2.316,-2.225 indicating
(power of the main channel 1) = -2.420 dBm,
(power of the main channel 2) = -2.847 dBm,
(power of the main channel 3) = -2.316 dBm, and
(power of the main channel 4) = -2.225 dBm.

Related Commands [:SENSe]:MCPower:CHANnel:MAIN commands

:READ:MCPower:SPECTrum? (Query Only)

Returns spectrum trace data of the MCPR measurement.

Syntax :READ:MCPower:SPECTrum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the spectrum trace data in dBm for the point n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views MCPR

Examples :READ:MCPower:SPECTrum?
might return #43204xxxx... (3204-byte data) for the spectrum trace data of the MCPR measurement.

:READ:MERRor Subgroup (Option 21)

The :READ:MERRor commands returns the results of the Magnitude error versus Time measurement.

Command Tree	Header	Parameter
	:READ	
	:MERRor	
	:FERRor?	
	:PEAK?	
	:PINdex?	
	:RMS?	
	:TRACe?	

:READ:MERRor:FERRor? (Query Only)

Returns the frequency error in the Magnitude error versus Time measurement.

Syntax :READ:MERRor:FERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Measurement Views Magnitude error versus Time

Examples :READ:MERRor:FERRor?
might return -10.7E+3 indicating the frequency error is -10.7 kHz.

:READ:MERRor:PEAK? (Query Only)

Returns the peak value in the Magnitude error versus Time measurement.

Syntax :READ:MERRor:PEAK?

Arguments None

Returns <peak>::=<NRf> is the peak magnitude error in percent (%).

Measurement Views Magnitude error versus Time

Examples :READ:MERRor:PEAK?
might return 1.57 indicating the peak magnitude error is 1.57%.

Related Commands :READ:MERRor:PINDex?

:READ:MERRor:PINDex? (Query Only)

Returns the time at the magnitude error peak.

Syntax :READ:MERRor:PINDex?

Arguments None

Returns <peak_time>::=<NRf> is the time at the magnitude error peak in seconds.

You can select the time unit using the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Magnitude error versus Time

Examples :READ:MERRor:PINDex?
might return 28.912E-6 indicating the time at the magnitude error peak is 28.912 μ s.

Related Commands :READ:MERRor:PEAK?, [:SENSe]:DDEMod:TIME:UNITs

:READ:MERRor:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the Magnitude error versus Time measurement.

Syntax :READ:MERRor:RMS?

Arguments None

Returns <rms>::=<NRf> is the RMS magnitude error in percent (%).

Measurement Views Magnitude error versus Time

Examples :READ:MERRor:RMS?
might return 0.382 indicating the magnitude error is 0.382% RMS.

:READ:MERRor:TRACe? (Query Only)

Returns the Magnitude error versus Time trace data.

Syntax :READ:MERRor:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the magnitude error data for the point n in percent (%),
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Magnitude error versus Time

Examples :READ:MERRor:TRACe?
might return #42036xxxx... (2036-byte data) for the Magnitude error versus Time trace.

:READ:OBWidth Subgroup

The :READ:OBWidth commands returns the results of the Occupied Bandwidth (OBW) measurement.

Command Tree	Header	Parameter
	:READ	
	:OBWidth	
	:FREQuency	
	:ERRor?	
	:OBWidth	
	:BANDwidth?	
	:LEFT	
	:FREQuency?	
	:LEVe1?	
	:POWeR?	
	:RIGHT	
	:FREQuency?	
	:LEVe1?	
	:SPECTrum?	
	:XDBBbandwidth	
	:BANDwidth?	
	:LEFT	
	:FREQuency?	
	:LEVe1?	
	:POWeR?	
	:RIGHT	
	:FREQuency?	
	:LEVe1?	

:READ:OBWidth:FREQuency:ERRor? (Query Only)

Returns the frequency error in the Occupied Bandwidth measurement.

Syntax :READ:OBWidth:FREQuency:ERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Measurement Views Occupied Bandwidth

Examples :READ:MERRor:FERRor?
might return -10.7E+3 indicating the frequency error is -10.7 kHz.

:READ:OBWidth:OBWidth:BANDwidth? (Query Only)

Returns the occupied bandwidth in the Occupied Bandwidth measurement.

Syntax :READ:OBWidth:OBWidth:BANDwidth?

Arguments None

Returns <OBW>::=<NRf> is the occupied bandwidth in Hz.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:OBWidth:BANDwidth?
might return 4.0E+6 indicating the occupied bandwidth is 4 MHz.

:READ:OBWidth:OBWidth:LEFT:FREQuency? (Query Only)

Returns the left (lower) frequency of the occupied bandwidth.

Syntax :READ:OBWidth:OBWidth:LEFT:FREQuency?

Arguments None

Returns <OBW_left_freq>::=<NRf> is the left frequency in Hz.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:OBWidth:LEFT:FREQuency?
might return 1.498E+9 indicating the left frequency is 1.498 GHz.

Related Commands :READ:OBWidth:OBWidth:RIGHT:FREQuency?

:READ:OBWidth:OBWidth:LEFT:LEVel? (Query Only)

Returns the level at the left frequency of the occupied bandwidth.

Syntax :READ:OBWidth:OBWidth:LEFT:LEVel?

Arguments None

Returns <OBW_left_level>::=<NRf> is the level at the left frequency in dB.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:OBWidth:LEFT:LEVel?
might return -23.5 indicating the level at the left frequency is -23.5 dB.

Related Commands :READ:OBWidth:OBWidth:RIGHT:LEVel?

:READ:OBWidth:OBWidth:POWer? (Query Only)

Returns the reference power in the Occupied Bandwidth measurement.

Syntax :READ:OBWidth:OBWidth:POWer?

Arguments None

Returns <OBW_ref_power>::=<NRf> is the reference power in dBm.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:OBWidth:POWer?
might return -10.0 indicating the reference power is -10 dBm.

:READ:OBWidth:OBWidth:RIGHT:FREQuency? (Query Only)

Returns the right (higher) frequency of the occupied bandwidth.

Syntax :READ:OBWidth:OBWidth:RIGHT:FREQuency?

Arguments None

Returns <OBW_right_freq>::=<NRf> is the right frequency in Hz.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:OBWidth:RIGHT:FREQuency?
might return 1.502E+9 indicating the right frequency is 1.502 GHz.

Related Commands :READ:OBWidth:OBWidth:LEFT:FREQuency?

:READ:OBWidth:OBWidth:RIGHT:LEVel? (Query Only)

Returns the level at the right frequency of the occupied bandwidth.

Syntax :READ:OBWidth:OBWidth:RIGHT:LEVel?

Arguments None

Returns <OBW_right_level>::=<NRf> is the level at the right frequency in dB.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:OBWidth:RIGHT:LEVel?
might return -23.5 indicating the level at the right frequency is -23.5 dB.

Related Commands :READ:OBWidth:OBWidth:LEFT:LEVel?

:READ:OBWidth:SPECTrum? (Query Only)

Returns spectrum trace data of the Occupied Bandwidth measurement.

Syntax :READ:OBWidth:SPECTrum?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:SPECTrum?
might return #43204xxxx... (3204-byte data) for the spectrum trace data of the Occupied Bandwidth measurement.

:READ:OBWidth:XDBBandwidth:BANDwidth? (Query Only)

Returns the x dB bandwidth in the Occupied Bandwidth measurement.

Syntax :READ:OBWidth:XDBBandwidth:BANDwidth?

Arguments None

Returns <xdbBW>::=<NRf> is the x dB bandwidth in Hz.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:XDBBandwidth:BANDwidth?
might return 2.0E+6 indicating the x dB bandwidth is 2 MHz.

:READ:OBWidth:XDBBandwidth:LEFT:FREQUENCY? (Query Only)

Returns the left (lower) frequency of the x dB bandwidth.

Syntax :READ:OBWidth:XDBBandwidth:LEFT:FREQUENCY?

Arguments None

Returns <xdbBW_left_freq>::=<NRf> is the left frequency in Hz.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:XDBBandwidth:LEFT:FREQUENCY?
might return 1.498E+9 indicating the left frequency is 1.498 GHz.

Related Commands :READ:OBWidth:XDBBandwidth:RIGHT:FREQUENCY?

:READ:OBWidth:XDBBandwidth:LEFT:LEVEL? (Query Only)

Returns the level at the left frequency of the x dB bandwidth.

Syntax :READ:OBWidth:XDBBandwidth:LEFT:LEVEL?

Arguments None

Returns <xdbBW_left_level>::=<NRf> is the level at the left frequency in dB.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:XDBBandwidth:LEFT:LEVEL?
might return -23.5 indicating the level at the left frequency is -23.5 dB.

Related Commands :READ:OBWidth:XDBBandwidth:RIGHT:LEVEL?

:READ:OBWidth:XDBBandwidth:POWer? (Query Only)

Returns the reference power in the x dB bandwidth measurement.

Syntax :READ:OBWidth:XDBBandwidth:POWer?

Arguments None

Returns <xdbBW_ref_power>::=<NRf> is the reference power in dBm.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:XDBBandwidth:POWer?
might return -10.0 indicating the reference power is -10 dBm.

:READ:OBWidth:XDBBandwidth:RIGHT:FREQUENCY? (Query Only)

Returns the right (higher) frequency of the x dB bandwidth.

Syntax :READ:OBWidth:XDBBandwidth:RIGHT:FREQUENCY?

Arguments None

Returns <xdbBW_right_freq>::=<NRf> is the right frequency in Hz.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:XDBBandwidth:RIGHT:FREQUENCY?
might return 1.502E+9 indicating the right frequency is 1.502 GHz.

Related Commands :READ:OBWidth:XDBBandwidth:LEFT:FREQUENCY?

:READ:OBWidth:XDBBandwidth:RIGHT:LEVEL? (Query Only)

Returns the level at the right frequency of the x dB bandwidth.

Syntax :READ:OBWidth:XDBBandwidth:RIGHT:LEVEL?

Arguments None

Returns <xdbBW_right_level>::=<NRf> is the level at the right frequency in dB.

Measurement Views Occupied Bandwidth

Examples :READ:OBWidth:XDBBandwidth:RIGHT:LEVEL?
might return -23.5 indicating the level at the right frequency is -23.5 dB.

Related Commands :READ:OBWidth:XDBBandwidth:LEFT:LEVEL?

:READ:PERRor Subgroup (Option 21)

The :READ:PERRor commands returns the results of the Phase error versus Time measurement.

Command Tree	Header	Parameter
	:READ	
	:PERRor	
	:FERRor?	
	:PEAK?	
	:PINdex?	
	:RMS?	
	:TRACe?	

:READ:PERRor:FERRor? (Query Only)

Returns the frequency error in the Phase error versus Time measurement.

Syntax :READ:PERRor:FERRor?

Arguments None

Returns <freq_error>::=<NRf> is the frequency error in Hz.

Measurement Views Phase error versus Time

Examples :READ:PERRor:FERRor?
might return -10.7E+3 indicating the frequency error is -10.7 kHz.

:READ:PERRor:PEAK? (Query Only)

Returns the peak value in the Phase error versus Time measurement.

Syntax :READ:PERRor:PEAK?

Arguments None

Returns <peak>::=<NRf> is the peak phase error in degrees.

Measurement Views Phase error versus Time

Examples :READ:PERRor:PEAK?
might return 0.683 indicating the peak phase error is 0.683°.

Related Commands :READ:PERRor:PINDEX?

:READ:PERRor:PINDEX? (Query Only)

Returns the time at the phase error peak.

Syntax :READ:PERRor:PINDEX?

Arguments None

Returns <peak_time>::=<NRf> is the time at the phase error peak in seconds.
You can select the time unit using the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Phase error versus Time

Examples :READ:PERRor:PINDEX?
might return 28.912E-6 indicating the time at the phase error peak is 28.912 μs.

Related Commands :READ:PERRor:PEAK?, [:SENSe]:DDEMod:TIME:UNITs

:READ:PERRor:RMS? (Query Only)

Returns the RMS (Root-Mean-Square) value in the Phase error versus Time measurement.

Syntax :READ:PERRor:RMS?

Arguments None

Returns <rms>::=<NRf> is the RMS phase error in degrees.

Measurement Views Phase error versus Time

Examples :READ:PERRor:RMS?
might return 0.746 indicating the phase error is 0.746° RMS.

:READ:PERRor:TRACe? (Query Only)

Returns the Phase error versus Time trace data.

Syntax :READ:PERRor:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the phase error data for the point n in degrees, 4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Phase error versus Time

Examples :READ:PERRor:TRACe?
might return #42036xxxx... (2036-byte data) for the Phase error versus Time trace.

:READ:PHVTime Subgroup

The :READ:PHVTime commands returns the results of the Phase versus Time measurement.

Command Tree	Header	Parameter
	:READ	
	:PHVTime?	
	:MAXimum?	
	:MAXLocation?	
	:MINimum?	
	:MINLocation?	
	:RESult?	

:READ:PHVTime? (Query Only)

Returns the Phase versus Time trace data.

Syntax :READ:PHVTime?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the phase in degrees for the point #n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Phase versus Time

Examples :READ:PHVTime?
might return #3160xxxx... (160-byte data) for the Phase versus Time trace.

:READ:PHVTime:MAXimum? (Query Only)

Returns the maximum value in the Phase versus Time measurement.

Syntax :READ:PHVTime:MAXimum?

Arguments None

Returns <max>::=<NRf> is the maximum phase in degrees.

Measurement Views Phase versus Time

Examples :READ:PHVTime:MAXimum?
might return 153.8 indicating the maximum phase is 153.8°.

Related Commands :READ:PHVTime:MAXLocation?

:READ:PHVTime:MAXLocation? (Query Only)

Returns the time at which the phase is maximum.

Syntax :READ:PHVTime:MAXLocation?

Arguments None

Returns <max_time>::=<NRf> is the time in seconds at which the phase is maximum.

Measurement Views Phase versus Time

Examples :READ:PHVTime:MAXLocation?
might return 175.3E-9 indicating the I or Q level is maximum at 175.3 ns.

Related Commands :READ:PHVTime:MAXimum?

:READ:PHVTime:MINimum? (Query Only)

Returns the minimum value in the Phase versus Time measurement.

Syntax :READ:PHVTime:MINimum?

Arguments None

Returns <min>::=<NRf> is the minimum phase in degrees.

Measurement Views Phase versus Time

Examples :READ:PHVTime:MINimum?
might return -176.3 indicating the minimum phase is -176.3°.

Related Commands :READ:PHVTime:MINLocation?

:READ:PHVTime:MINLocation? (Query Only)

Returns the time at which the phase is minimum.

Syntax :READ:PHVTime:MINLocation?

Arguments None

Returns <min_time>::=<NRf> is the time in seconds at which the phase is minimum.

Measurement Views Phase versus Time

Examples :READ:PHVTime:MAXLocation?
might return 450.7E-9 indicating the phase is minimum at 450.7 ns.

Related Commands :READ:PHVTime:MINimum?

:READ:PHVTime:RESult? (Query Only)

Returns the Phase versus Time measurement results.

Syntax :READ:PHVTime:RESult?

Arguments None

Returns <max>,<max_time>,<min>,<min_time>

Where

<max>::=<NRf> is the maximum phase in degrees.

<max_time>::=<NRf> is the time in seconds at which the phase is maximum.

<min>::=<NRf> is the minimum phase in degrees.

<min_time>::=<NRf> is the time in seconds at which the phase is minimum.

Measurement Views Phase versus Time

Examples :READ:PHVTime:RESult?
might return 153.8,175.3E-9,-176.3,450.7E-9 indicating:
the maximum phase is 153.8° at 175.3 ns and
the minimum phase is -176.3° at 450.7 ns.

:READ:PULSe Subgroup (Option 20 Only)

The :READ:PULSe commands returns the results of the Pulse Measurements.

Command Tree	Header	Parameter
	:READ	
	:PULSe	
	[:RESult]	
		:ATX?
		:AVERage?
		:DROop?
		:DUTPct?
		:DUTRatio?
		:FALL?
		:FRDeviation?
		:MFReqerror?
		:MPHerror?
		:PHDeviation?
		:PPFRequency?
		:PPOWer?
		:PPPHase?
		:RINTerval?
		:RIPPlE?
		:RISE?
		:RMSFreqerror?
		:RMSPHerror?
		:RRATe?
		:TIME?
		:WIDTh?
	:STATistics?	
		:ATX?
		:AVERage?
		:DROop?
		:DUTPct?
		:DUTRatio?
		:FALL?
		:FRDeviation?
		:MFReqerror?
		:MPHerror?
		:PHDeviation?
		:PPFRequency?
		:PPOWer?
		:PPPHase?
		:RINTerval?
		:RIPPlE?
		:RISE?

```

:RMSFreqerror?
:RMSPherror?
:RRATe?
:WIDTh?
:TRACe?

```

:READ:PULSe[:RESult]:ATX? (Query Only)

Returns the average transmitted power in the pulse table.

Syntax :READ:PULSe[:RESult]:ATX?

Arguments None

Returns <first_pulse_num>,<ATX(1)>,<ATX(2)>,...<ATX(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<ATX(n)>::=<NRf> is the average transmitted power for the pulse with the number of [first_pulse_num + n - 1] in dBm.

The unit can be changed to watts by the [:SENSe]:POWer:UNITs command. Volt is invalid in the average transmitted power measurement.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:ATX?
might return 0,-18.57,-18.73,-18.20,-18.53 for Pulse 0 to 3.

Related Commands [:SENSe]:POWer:UNITs

:READ:PULSe[:RESult]:AVERage? (Query Only)

Returns the average on power in the pulse table.

Syntax :READ:PULSe[:RESult]:AVERage?

Arguments None

Returns <first_pulse_num>,<avg(1)>,<avg(2)>,...<avg(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<avg(n)>::=<NRf> is the average on power for the pulse with the number of [first_pulse_num + n - 1] in dBm.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:AVERage?
might return 0,-2.354,-2.368,-2.343,-2.358 for Pulse 0 to 3.

Related Commands [:SENSe]:POWer:UNITs

:READ:PULSe[:RESult]:DROop? (Query Only)

Returns the average on power in the pulse table.

Syntax :READ:PULSe[:RESult]:DROop?

Arguments None

Returns <first_pulse_num>,<droop(1)>,<droop(2)>,...<droop(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<droop(n)>::=<NRf> is the wattage droop for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Measurement Views Pulse table

Examples :READ:PULSe:RESult:DROop?
might return 0,-270.9E-3,-193.0E-3,-242.7E-3,-177.5E-3 for Pulse 0 to 3.

:READ:PULSe[:RESult]:DUTPct? (Query Only)

Returns the duty factor (%) in the pulse table.

Syntax :READ:PULSe[:RESult]:DUTPct?

Arguments None

Returns <first_pulse_num>,<duty_pct(1)>,<duty_pct(2)>,...
<duty_pct(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<duty_pct(n)>::=<NRf> is the duty factor for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Measurement Views Pulse table

Examples :READ:PULSe:RESult:DUTPct?
might return 0,28.94,28.96,29.00,29.01 for Pulse 0 to 3.

:READ:PULSe[:RESult]:DUTRatio? (Query Only)

Returns the duty factor (ratio) in the pulse table.

Syntax :READ:PULSe[:RESult]:DUTRatio?

Arguments None

Returns <first_pulse_num>,<duty_ratio(1)>,<duty_ratio(2)>,...
<duty_ratio(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<duty_ratio(n)>::=<NRf> is the duty factor for the pulse with the number of
[first_pulse_num + n - 1] (no unit).

Measurement Views Pulse table

Examples :READ:PULSe:RESult:DUTRatio?
might return 0,289.4E-3,289.6E-3,290.0E-3,290.1E-3 for Pulse 0 to 3.

:READ:PULSe[:RESult]:FALL? (Query Only)

Returns the fall time in the pulse table.

Syntax :READ:PULSe[:RESult]:FALL?

Arguments None

Returns <first_pulse_num>,<fall(1)>,<fall(2)>,...<fall(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<fall(n)>::=<NRf> is the fall time for the pulse with the number of
[first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:FALL?
might return 0,110.3E-9,90.45E-9,95.03E-9,111.9E-9 for Pulse 0 to 3.

:READ:PULSe[:RESult]:FRDeviation? (Query Only)

Returns the frequency deviation in the pulse table.

Syntax :READ:PULSe[:RESult]:FRDeviation?

Arguments None

Returns <first_pulse_num>,<freq_dev(1)>,<freq_dev(2)>,...
<freq_dev(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<freq_dev(n)>::=<NRf> is the frequency deviation for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:FRDeviation?
might return 1,740.6E+3,736.5E+3,718.3E+3,672.2E+3 for Pulse 1 to 4.

:READ:PULSe[:RESult]:MFRerror? (Query Only)

Returns the maximum frequency error in the pulse table.

Syntax :READ:PULSe[:RESult]:MFRerror?

Arguments None

Returns <first_pulse_num>,<max_freq_err(1)>,<max_freq_err(2)>,...
 <max_freq_err(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<max_freq_err(n)>::=<NRf> is the maximum frequency error for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:MFRerror?
 might return 1,597.5E+3,675.8E+3,642.8E+3,598.2E+3 for Pulse 1 to 4.

:READ:PULSe[:RESult]:MPHerror? (Query Only)

Returns the maximum phase error in the pulse table.

Syntax :READ:PULSe[:RESult]:MPHerror?

Arguments None

Returns <first_pulse_num>,<max_phase_err(1)>,<max_phase_err(2)>,...
 <max_phase_err(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<max_phase_err(n)>::=<NRf> is the maximum phase error for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:MPHerror?
 might return 1,-9.221,-8.413,-11.853,-10.258 for Pulse 1 to 4.

:READ:PULSe[:RESult]:PHDeviation? (Query Only)

Returns the phase deviation in the pulse table.

Syntax :READ:PULSe[:RESult]:PHDeviation?

Arguments None

Returns <first_pulse_num>,<phase_dev(1)>,<phase_dev(2)>,...
 <phase_dev(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<phase_dev(n)>::=<NRf> is the phase deviation for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:PHDeviation?
 might return 1,11.658,9.640,10.509,8.272 for Pulse 1 to 4.

:READ:PULSe[:RESult]:PPFrequency? (Query Only)

Returns the pulse-pulse carrier frequency in the pulse table.

Syntax :READ:PULSe[:RESult]:PPFrequency?

Arguments None

Returns <first_pulse_num>,<pp_freq(1)>,<pp_freq(2)>,...<pp_freq(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<pp_freq(n)>::=<NRf> is the pulse-pulse carrier frequency for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:PPFrequency?
might return 0,0.000,1.258E+3,-3.121E+3,1.862E+3 for Pulse 0 to 3.

:READ:PULSe[:RESult]:PPOWer? (Query Only)

Returns the peak power in the pulse table.

Syntax :READ:PULSe[:RESult]:PPOWer?

Arguments None

Returns <first_pulse_num>,<pk_power(1)>,<pk_power(2)>,...
 <pk_power(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<pk_power(n)>::=<NRf> is the peak power for the pulse with the number of
 [first_pulse_num + n - 1] in dBm.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:PPOWer?
 might return 0,-2.26,-2.27,-2.23,-2.25 for Pulse 0 to 3.

Related Commands [:SENSe]:POWer:UNITs

:READ:PULSe[:RESult]:PPPHase? (Query Only)

Returns the pulse-pulse carrier phase in the pulse table.

Syntax :READ:PULSe[:RESult]:PPPHase?

Arguments None

Returns <first_pulse_num>,<pp_phase(1)>,<pp_phase(2)>,...
<pp_phase(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<pp_phase(n)>::=<NRf> is the pulse-pulse carrier phase for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:PPPHase?
might return 0,0.000,21.66,46.76,57.56 for Pulse 0 to 3.

:READ:PULSe[:RESult]:RINterval? (Query Only)

Returns the repetition interval in the pulse table.

Syntax :READ:PULSe[:RESult]:RINterval?

Arguments None

Returns <first_pulse_num>,<rep_int(1)>,<rep_int(2)>,...<rep_int(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<rep_int(n)>::=<NRf> is the repetition interval for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:RINterval?
might return 0,16.03E-6,16.08E-6,16.07E-6,16.02E-6 for Pulse 0 to 3.

:READ:PULSe[:RESult]:RIPple? (Query Only)

Returns the ripple in the pulse table.

Syntax :READ:PULSe[:RESult]:RIPple?

Arguments None

Returns <first_pulse_num>,<ripple(1)>,<ripple(2)>,...<ripple(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<ripple(n)>::=<NRf> is the voltage ripple for the pulse with the number of [first_pulse_num + n - 1] in percent (%).

Measurement Views Pulse table

Examples :READ:PULSe:RESult:RIPple?
might return 0,106.5E-3,177.6E-3,148.3E-3,148.5E-3 for Pulse 0 to 3.

:READ:PULSe[:RESult]:RISE? (Query Only)

Returns the rise time in the pulse table.

Syntax :READ:PULSe[:RESult]:RISE?

Arguments None

Returns <first_pulse_num>,<rise(1)>,<rise(2)>,...<rise(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<rise(n)>::=<NRf> is the rise time for the pulse with the number of [first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:RISE?
might return 0,92.94E-9,115.9E-9,115.1E-9,97.45E-9 for Pulse 0 to 3.

:READ:PULSe[:RESult]:RMSFreqerror? (Query Only)

Returns the RMS frequency error in the pulse table.

Syntax :READ:PULSe[:RESult]:RMSFreqerror?

Arguments None

Returns <first_pulse_num>,<RMS_freq_err(1)>,<RMS_freq_err(2)>,...
<RMS_freq_err(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<RMS_freq_err(n)>::=<NRf> is the RMS frequency error for the pulse with the number of [first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:RMSFreqerror?
might return 1,51.54E+3,69.20E+3,64.21E+3,51.02E+3 for Pulse 1 to 4.

:READ:PULSe[:RESult]:RMSPherror? (Query Only)

Returns the RMS phase error in the pulse table.

Syntax :READ:PULSe[:RESult]:RMSPherror?

Arguments None

Returns <first_pulse_num>,<RMS_phase_err(1)>,<RMS_phase_err(2)>,...
 <RMS_phase_err(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<RMS_phase_err(n)>::=<NRf> is the RMS phase error for the pulse with the number of [first_pulse_num + n - 1] in degrees.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:RMSPherror?
 might return 1,908.4E-3,752.8E-3,981.7E-3,886.4E-3 for Pulse 1 to 4.

:READ:PULSe[:RESult]:RRATe? (Query Only)

Returns the repetition rate in the pulse table.

Syntax :READ:PULSe[:RESult]:RRATe?

Arguments None

Returns <first_pulse_num>,<rep_rate(1)>,<rep_rate(2)>,...
<rep_rate(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<rep_rate(n)>::=<NRf> is the repetition rate for the pulse with the number of
[first_pulse_num + n - 1] in Hz.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:RRATe?
might return 0,62.50E+3,62.52E+3,62.51E+3,62.49E+3 for Pulse 0 to 3.

:READ:PULSe[:RESult]:TIME? (Query Only)

Returns the time in the pulse table.

Syntax :READ:PULSe[:RESult]:TIME?

Arguments None

Returns <first_pulse_num>,<time(1)>,<time(2)>,...<time(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<time(n)>::=<NRf> is the time for the pulse with the number of
[first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:TIME?
might return 1,7.937E-3,8.436E-3,6.504E-3,9.876E-3 for Pulse 1 to 4.

:READ:PULSe[:RESult]:WIDTh? (Query Only)

Returns the pulse width in the pulse table.

Syntax :READ:PULSe[:RESult]:WIDTh?

Arguments None

Returns <first_pulse_num>,<width(1)>,<width(2)>,...<width(n)>

Where

<first_pulse_num>::=<NR1> is the first pulse number.

<width(n)>::=<NRf> is the pulse width for the pulse with the number of
[first_pulse_num + n - 1] in seconds.

Measurement Views Pulse table

Examples :READ:PULSe:RESult:WIDTh?
might return 0,4.630E-6,4.632E-6,4.639E-6,4.642E-6 for Pulse 0 to 3.

:READ:PULSe:STATistics? (Query Only)

Returns the trace data of the pulse statistics measurement selected by the :DISPlay:PULSe:SElect:RESult command.

NOTE. Select the plot type (Trend or FFT) using the :DISPlay:PULSe:STATistics :PLOT command before executing this query.

Syntax :READ:PULSe:STATistics?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude for the point #n.

The unit is dBm (Plot = Trend) or dB (Plot = FFT).

4-byte little endian floating-point format specified in IEEE 488.2.

The unit of power is selected by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics?
might return #264xxxx... (64-byte data) for the statistics trace of the pulse width measurement when :DISPlay:PULSe:SElect:RESult is set to WIDTH.

Related Commands :DISPlay:PULSe:SElect:RESult, :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:ATX? (Query Only)

Returns the average transmitted power in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:ATX?

Arguments None

Returns <ATX_avg>,<ATX_min>,<ATX_max>

Where

<ATX_avg>::=<NRf> is the average of the average transmitted power.

<ATX_min>::=<NRf> is the minimum of the average transmitted power.

<ATX_max>::=<NRf> is the maximum of the average transmitted power.

Unit: dBm.

The unit can be changed to watts by the [:SENSe]:POWer:UNITs command.

Volt is invalid in the average transmitted power measurement.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:ATX?
might return -18.51,-18.74,-18.12 for the average transmitted power in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT, [:SENSe]:POWer:UNITs

:READ:PULSe:STATistics:AVERage? (Query Only)

Returns the average on power in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:AVERage?

Arguments None

Returns <avg_avg>,<avg_min>,<avg_max>

Where

<avg_avg>::=<NRf> is the average of the average on power.

<avg_min>::=<NRf> is the minimum of the average on power.

<avg_max>::=<NRf> is the maximum of the average on power.

Unit: dBm.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:AVERage?
might return -2.35,-2.36,-2.34 for the average on power in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT, [:SENSe]:POWer:UNITs

:READ:PULSe:STATistics:DROop? (Query Only)

Returns the droop in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:DROop?

Arguments None

Returns <droop_avg>,<droop_min>,<droop_max>

Where

<droop_avg>::=<NRf> is the average droop.

<droop_min>::=<NRf> is the minimum droop.

<droop_max>::=<NRf> is the maximum droop.

Unit: Percent (%) by watts.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:DROop?
might return 22.67E-3,-613.5E-3,633.8E-3 for the droop in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:DUTPct? (Query Only)

Returns the duty factor (%) in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:DUTPct?

Arguments None

Returns <duty_pct_avg>,<duty_pct_min>,<duty_pct_max>

Where

<duty_pct_avg>::=<NRf> is the average duty factor.

<duty_pct_min>::=<NRf> is the minimum duty factor.

<duty_pct_max>::=<NRf> is the maximum duty factor.

Unit: Percent (%).

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:DUTPct?
might return 2.437,2.310,2.657 for the duty factor (%) in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:DUTRatio? (Query Only)

Returns the duty factor (ratio) in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:DUTRatio?

Arguments None

Returns <duty_ratio_avg>,<duty_ratio_min>,<duty_ratio_max>

Where

<duty_ratio_avg>::=<NRf> is the average duty factor.

<duty_ratio_min>::=<NRf> is the minimum duty factor.

<duty_ratio_max>::=<NRf> is the maximum duty factor.

Unit: None.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:DUTRatio?
might return 24.37E-3,23.11E-3,26.57E-3 for the duty factor (ratio) in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:FALL? (Query Only)

Returns the fall time in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:FALL?

Arguments None

Returns <fall_avg>,<fall_min>,<fall_max>

Where

<fall_avg>::=<NRf> is the average fall time.

<fall_min>::=<NRf> is the minimum fall time.

<fall_max>::=<NRf> is the maximum fall time.

Unit: Seconds.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:FALL?
might return 70.27E-9,69.62E-9,71.27E-9 for the fall time in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:FRDeviation? (Query Only)

Returns the frequency deviation in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:FRDeviation?

Arguments None

Returns <freq_dev_avg>,<freq_dev_min>,<freq_dev_max>

Where

<freq_dev_avg>::=<NRf> is the average frequency deviation.

<freq_dev_min>::=<NRf> is the minimum frequency deviation.

<freq_dev_max>::=<NRf> is the maximum frequency deviation.

Unit: Hz.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:FRDeviation?
might return 754.1E+3,660.5E+3,835.2E+3 for the frequency deviation in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:MFRqerror? (Query Only)

Returns the maximum frequency error in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:MFRqerror?

Arguments None

Returns <max_freq_err_avg>,<max_freq_err_min>,<max_freq_err_max>

Where

<max_freq_err_avg>::=<NRf> is the average of maximum frequency error.

<max_freq_err_min>::=<NRf> is the minimum of maximum frequency error.

<max_freq_err_max>::=<NRf> is the maximum of maximum frequency error.

Unit: Hz.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:MFRqerror?
might return 645.0E+3,555.6E+3,738.8E+3 for the maximum frequency error in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:MPHerror? (Query Only)

Returns the maximum phase error in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:MPHerror?

Arguments None

Returns <max_phase_err_avg>,<max_phase_err_min>,<max_phase_err_max>

Where

<max_phase_err_avg>::=<NRf> is the average of maximum phase error.

<max_phase_err_min>::=<NRf> is the minimum of maximum phase error.

<max_phase_err_max>::=<NRf> is the maximum of maximum phase error.

Unit: Degrees.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:MPHerror?
might return -11.47,-17.18,-7.61 for the maximum phase error in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:PHDeviation? (Query Only)

Returns the phase deviation in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:PHDeviation?

Arguments None

Returns <phase_dev_avg>,<phase_dev_min>,<phase_dev_max>

Where

<phase_dev_avg>::=<NRf> is the average phase deviation.

<phase_dev_min>::=<NRf> is the minimum phase deviation.

<phase_dev_max>::=<NRf> is the maximum phase deviation.

Unit: Degrees.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:PHDeviation?
might return 11.678,7.694,17.374 for the phase deviation in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:PPFrequency? (Query Only)

Returns the pulse-pulse carrier frequency in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:PPFrequency?

Arguments None

Returns <pp_freq_avg>,<pp_freq_min>,<pp_freq_max>

Where

<pp_freq_avg>::=<NRf> is the average pulse-pulse carrier frequency.

<pp_freq_min>::=<NRf> is the minimum pulse-pulse carrier frequency.

<pp_freq_max>::=<NRf> is the maximum pulse-pulse carrier frequency.

Unit: Hz.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:PPFrequency?
might return 1.135E+3,311.3E+3,-262.8E+3 for the pulse-pulse carrier frequency in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:PPower? (Query Only)

Returns the peak power in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:PPower?

Arguments None

Returns <pk_power_avg>,<pk_power_min>,<pk_power_max>

Where

<pk_power_avg>::=<NRf> is the average peak power.

<pk_power_min>::=<NRf> is the minimum peak power.

<pk_power_max>::=<NRf> is the maximum peak power.

Unit: dBm.

The unit can be changed by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:PPower?
might return -2.273,-2.313,-2.235 for the peak power in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT, [:SENSe]:POWer:UNITs

:READ:PULSe:STATistics:PPPHase? (Query Only)

Returns the pulse-pulse carrier phase in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:PPPHase?

Arguments None

Returns <pp_phase_avg>,<pp_phase_min>,<pp_phase_max>

Where

<pp_phase_avg>::=<NRf> is the average pulse-pulse carrier phase.

<pp_phase_min>::=<NRf> is the minimum pulse-pulse carrier phase.

<pp_phase_max>::=<NRf> is the maximum pulse-pulse carrier phase.

Unit: Degrees.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:PPPHase?
might return -9.298E-3,-254.3E-3,311.7E-3 for the pulse-pulse carrier phase in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:RINteRval? (Query Only)

Returns the repetition interval in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:RINteRval?

Arguments None

Returns <rep_int_avg>,<rep_int_min>,<rep_int_max>

Where

<rep_int_avg>::=<NRf> is the average repetition interval.

<rep_int_min>::=<NRf> is the minimum repetition interval.

<rep_int_max>::=<NRf> is the maximum repetition interval.

Unit: Seconds.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:RINteRval?
might return 240.5E-6,217.9E-6,281.2E-6 for the repetition interval in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:RIPPlE? (Query Only)

Returns the ripple in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:RIPPlE?

Arguments None

Returns <ripple_avg>,<ripple_min>,<ripple_max>

Where

<ripple_avg>::=<NRf> is the average ripple.

<ripple_min>::=<NRf> is the minimum ripple.

<ripple_max>::=<NRf> is the maximum ripple.

Unit: Percent (%) by volts.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:RIPPlE?
might return 160.4E-3,83.78E-3,287.7E-3 for the ripple in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:RISE? (Query Only)

Returns the rise time in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:RISE?

Arguments None

Returns <rise_avg>,<rise_min>,<rise_max>

Where

<rise_avg>::=<NRf> is the average rise time.

<rise_min>::=<NRf> is the minimum rise time.

<rise_max>::=<NRf> is the maximum rise time.

Unit: Seconds.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:RISE?
might return 105.4E-9,91.65E-9,116.2E-9 for the rise time in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:RMSFreqerror? (Query Only)

Returns the RMS frequency error in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:RMSFreqerror?

Arguments None

Returns <RMS_freq_err_avg>,<RMS_freq_err_min>,<RMS_freq_err_max>

Where

<RMS_freq_err_avg>::=<NRf> is the average of RMS frequency error.

<RMS_freq_err_min>::=<NRf> is the minimum of RMS frequency error.

<RMS_freq_err_max>::=<NRf> is the maximum of RMS frequency error.

Unit: Hz.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:RMSFreqerror?
might return 63.67E+3,45.49E+3,81.28E+3 for the RMS frequency error in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:RMSPherror? (Query Only)

Returns the RMS phase error in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:RMSPherror?

Arguments None

Returns <RMS_phase_err_avg>,<RMS_phase_err_min>,<RMS_phase_err_max>

Where

<RMS_phase_err_avg>::=<NRf> is the average of RMS phase error.

<RMS_phase_err_min>::=<NRf> is the minimum of RMS phase error.

<RMS_phase_err_max>::=<NRf> is the maximum of RMS phase error.

Unit: Degrees.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:RMSPherror?
might return 1.032,604.5E-3,1.606 for the RMS phase error in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:RRATe? (Query Only)

Returns the repetition rate in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:RRATe?

Arguments None

Returns <rep_rate_avg>,<rep_rate_min>,<rep_rate_max>

Where

<rep_rate_avg>::=<NRf> is the average repetition rate.

<rep_rate_min>::=<NRf> is the minimum repetition rate.

<rep_rate_max>::=<NRf> is the maximum repetition rate.

Unit: Hz.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:RRATe?
might return 62.50E+3,62.49E+3,62.52E+3 for the repetition rate in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:STATistics:WIDTh? (Query Only)

Returns the pulse width in the pulse statistics.

This command is valid when :DISPlay:PULSe:STATistics:PLOT is set to TREND.

Syntax :READ:PULSe:STATistics:WIDTh?

Arguments None

Returns <width_avg>,<width_min>,<width_max>

Where

<width_avg>::=<NRf> is the average pulse width.

<width_min>::=<NRf> is the minimum pulse width.

<width_max>::=<NRf> is the maximum pulse width.

Unit: Seconds.

Measurement Views Pulse statistics

Examples :READ:PULSe:STATistics:WIDTh?
might return 4.636E-6,4.630E-6,4.643E-6 for the pulse width in the pulse statistics.

Related Commands :DISPlay:PULSe:STATistics:PLOT

:READ:PULSe:TRACe? (Query Only)

Returns the waveform data in the pulse trace measurement selected by the :DISPlay:PULSe:SElect:RESult command.

Syntax :READ:PULSe:TRACe?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the amplitude in dBm for the point #n,
4-byte little endian floating-point format specified in IEEE 488.2.

The unit of power is selected by the [:SENSe]:POWer:UNITs command.

Measurement Views Pulse trace

Examples :READ:PULSe:TRACe?
might return #43204xxxx... (3204-byte data) for the trace of the pulse width measurement when :DISPlay:PULSe:SElect:RESult is set to WIDTh.

Related Commands :DISPlay:PULSe:SElect:RESult

:READ:SGRam Subgroup

The :READ:SGRam commands returns the results of the spectrogram measurement.

Command Tree	Header	Parameter
	:READ	
	:SGRam?	

:READ:SGRam? (Query Only)

Returns the spectrogram trace data.

Syntax :READ:SGRam?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the trace data in dBm for the point n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Spectrogram

Examples :READ:SGRam:TRACe1?
might return #43204xxxx... (3204-byte data) for the spectrogram trace.

:READ:SPECTrum Subgroup

The :READ:SPECTrum commands returns results of the Spectrum measurement.

Command Tree	Header	Parameter
	:READ	
	:SPECTrum	
	:TRACe<x>?	

Where <x> = 1 to 5. Each trace is defined as follows:

- TRACe1: Trace 1
- TRACe2: Trace 2
- TRACe3: Trace 3
- TRACe4: Math trace
- TRACe5: Spectrogram

The traces can be specified by the :TRACe<x>:SPECTrum command subgroup.

:READ:SPECTrum:TRACe<x>? (Query Only)

Returns the trace data in the Spectrum measurement.

Syntax :READ:SPECTrum:TRACe<x>?

Where <x> = 1 to 5.

NOTE. TRACe5 (spectrogram) is valid when the spectrum and spectrogram measurements are running.

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the trace data in dBm for the point n,
4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Spectrum

Examples :READ:SPECTrum:TRACe1?
might return #43204xxxx... (3204-byte data) for Trace 1 in the Spectrum measurement.

Related Commands :TRACe<x>:SPECTrum command subgroup

:READ:SQQuality Subgroup (Option 21)

The :READ:SQQuality commands return the results of the signal quality measurement.

Command Tree	Header	Parameter
	:READ	
	:SQQuality	
	:FREQuency	
	:ERRor?	
	:GAIN	
	:IMBalance?	
	:ORIGin	
	:OFFSet?	
	:PEAK	
	:EVM?	
	:DB?	
	:LOCation?	
	:MERRor?	
	:DB?	
	:LOCation?	
	:PERRor?	
	:LOCation?	
	:QUADrature	
	:ERRor?	
	:RHO	
	:RMS	
	:EVM?	
	:DB?	
	:MERRor?	
	:DB?	
	:PERRor?	

:READ:SQQuality:FREQuency:ERRor? (Query Only)

Returns the frequency error in the signal quality measurement.

Syntax :READ:SQQuality:FREQuency:ERRor?

Arguments None

Returns <NRf> Frequency error in Hz.

Measurement Views Signal quality

Examples :READ:SQQuality:FREQuency:ERRor?
might return 612.043E+3, indicating that the frequency error is 612.043 kHz.

:READ:SQQuality:GAIN:IMBalance? (Query Only)

Returns the gain imbalance in the signal quality measurement.

Syntax :READ:SQQuality:GAIN:IMBalance?

Arguments None

Returns <NRf> Gain imbalance in dB.

Measurement Views Signal quality

Examples :READ:SQQuality:GAIN:IMBalance?
might return -57.746E-3, indicating that the gain imbalance is -0.057746 dB.

:READ:SQUality:ORIGin:OFFSet? (Query Only)

Returns the origin offset in the signal quality measurement.

Syntax :READ:SQUality:ORIGin:OFFSet?

Arguments None

Returns <NRf> Origin offset in dB.

Measurement Views Signal quality

Examples :READ:SQUality:ORIGin:OFFSet?
might return -44.968, indicating that the origin offset is -44.968 dB.

:READ:SQUality:PEAK:EVM? (Query Only)

Returns the peak EVM (%) in the signal quality measurement.

Syntax :READ:SQUality:PEAK:EVM?

Arguments None

Returns <NRf> Peak EVM in percent (%).

Measurement Views Signal quality

Examples :READ:SQUality:PEAK:EVM?
might return 4.276, indicating that the peak EVM is 4.276%.

:READ:SQUality:PEAK:EVM:DB? (Query Only)

Returns the peak EVM (dB) in the signal quality measurement.

Syntax :READ:SQUality:PEAK:EVM:DB?

Arguments None

Returns <NRf> Peak EVM in dB.

Measurement Views Signal quality

Examples :READ:SQUality:PEAK:EVM:DB?
might return -27.358, indicating that the peak EVM is -27.358 dB.

:READ:SQUality:PEAK:EVM:LOCation? (Query Only)

Returns the time at which the EVM is peak.

Syntax :READ:SQUality:PEAK:EVM:LOCation?

Arguments None

Returns <NRf> The time in seconds at which the EVM is peak.
The unit can be changed by the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Signal quality

Examples :READ:SQUality:PEAK:EVM:LOCation?
might return 36.018E-6, indicating that the EVM is peak at 36.018 μ s.

:READ:SQUality:PEAK:MERRor? (Query Only)

Returns the peak magnitude error (%) in the signal quality measurement.

Syntax :READ:SQUality:PEAK:MERRor?

Arguments None

Returns <NRf> Peak magnitude error in percent (%).

Measurement Views Signal quality

Examples :READ:SQUality:PEAK:MERRor?
might return 3.595, indicating that the peak magnitude error is 3.595%.

:READ:SQUality:PEAK:MERRor:DB? (Query Only)

Returns the peak magnitude error (dB) in the signal quality measurement.

Syntax :READ:SQUality:PEAK:MERRor:DB?

Arguments None

Returns <NRf> Peak magnitude error in dB.

Measurement Views Signal quality

Examples :READ:SQUality:PEAK:MERRor:DB?
might return -28.583, indicating that the magnitude error is -28.583 dB.

:READ:SQuality:PEAK:MERRor:LOCation? (Query Only)

Returns the time at which the magnitude error is peak.

Syntax :READ:SQuality:PEAK:MERRor:LOCation?

Arguments None

Returns <NRf> The time in seconds at which the magnitude error is peak.
The unit can be changed by the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Signal quality

Examples :READ:SQuality:PEAK:MERRor:LOCation?
might return 42.127E-6, indicating that the magnitude error is peak at
42.127 μ s.

:READ:SQUality:PEAK:PERRor? (Query Only)

Returns the peak phase error in the signal quality measurement.

Syntax :READ:SQUality:PEAK:PERRor?

Arguments None

Returns <NRf> Peak phase error in degrees.

Measurement Views Signal quality

Examples :READ:SQUality:PEAK:PERRor?
might return 1.907, indicating that the peak phase error is 1.907°.

:READ:SQUality:PEAK:PERRor:LOCation? (Query Only)

Returns the time at which the phase error is peak.

Syntax :READ:SQUality:PEAK:PERRor:LOCation?

Arguments None

Returns <NRf> The time in seconds at which the phase error is peak.
The unit can be changed by the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views Signal quality

Examples :READ:SQUality:PEAK:PERRor:LOCation?
might return 41.825E-6, indicating that the phase error is peak at 41.825 μs.

:READ:SQuality:QUADrature:ERRor? (Query Only)

Returns the quadrature error in the signal quality measurement.

Syntax :READ:SQuality:QUADrature:ERRor?

Arguments None

Returns <NRf> Quadrature error in degrees.

Measurement Views Signal quality

Examples :READ:SQuality:QUADrature:ERRor?
might return -14.264E-3, indicating that the quadrature error is -0.014264°.

:READ:SQuality:RHO? (Query Only)

Returns the ρ (waveform quality) value in the signal quality measurement.

Syntax :READ:SQuality:RHO?

Arguments None

Returns <NRf> ρ value.

Measurement Views Signal quality

Examples :READ:SQuality:RHO?
might return 998.703E-3, indicating that ρ is 0.998703.

:READ:SQUality:RMS:EVM? (Query Only)

Returns the RMS EVM (%) in the signal quality measurement.

Syntax :READ:SQUality:RMS:EVM?

Arguments None

Returns <NRf> RMS EVM in percent (%).

Measurement Views Signal quality

Examples :READ:SQUality:RMS:EVM?
might return 2.417, indicating that the RMS EVM is 2.417%.

:READ:SQUality:RMS:EVM:DB? (Query Only)

Returns the RMS EVM (dB) in the signal quality measurement.

Syntax :READ:SQUality:RMS:EVM:DB?

Arguments None

Returns <NRf> RMS EVM in dB.

Measurement Views Signal quality

Examples :READ:SQUality:RMS:EVM:DB?
might return -32.356, indicating that the RMS EVM is -32.356 dB.

:READ:SQuality:RMS:MERRor? (Query Only)

Returns the RMS magnitude error (%) in the signal quality measurement.

Syntax :READ:SQuality:RMS:MERRor?

Arguments None

Returns <NRf> RMS magnitude error in percent (%).

Measurement Views Signal quality

Examples :READ:SQuality:RMS:MERRor?
might return 1.837, indicating that the RMS magnitude error is 1.837%.

:READ:SQuality:RMS:MERRor:DB? (Query Only)

Returns the RMS magnitude error (dB) in the signal quality measurement.

Syntax :READ:SQuality:RMS:MERRor:DB?

Arguments None

Returns <NRf> RMS magnitude error in dB.

Measurement Views Signal quality

Examples :READ:SQuality:RMS:MERRor:DB?
might return -34.706, indicating that the magnitude error is -34.706 dB.

:READ:SQUality:RMS:PError? (Query Only)

Returns the RMS phase error in the signal quality measurement.

Syntax :READ:SQUality:RMS:PError?

Arguments None

Returns <NRf> RMS phase error in degrees.

Measurement Views Signal quality

Examples :READ:SQUality:RMS:PError?
might return 893.472E-3, indicating that the RMS phase error is 0.893472°.

:READ:TOVerview Subgroup

The :READ:TOVerview commands returns the results of the time overview measurement.

Command Tree	Header	Parameter
	:READ	
	:TOVerview?	

:READ:TOVerview? (Query Only)

Returns the trace data in the time overview.

Syntax :READ:TOVerview?

Arguments None

Returns #<num_digit><num_byte><data(1)><data(2)>...<data(n)>

Where

<num_digit> is the number of digits in <num_byte>.

<num_byte> is the number of bytes of data that follow.

<data(n)> is the trace data in dBm for the point n,

4-byte little endian floating-point format specified in IEEE 488.2.

Measurement Views Time overview

Examples :READ:TOVerview?
might return #43204xxxx... (3204-byte data) for the trace in the time overview.

SENSe Commands

The SENSe commands set the details for each of the measurement sessions. They are divided by measurement views into the subgroups listed in Table 2-40.

Table 2-40: SENSe command subgroups

Command header	Measurement view	Refer to:
[[:SENSe]] (basic)	All views, general analysis parameter control	page 2-584
[[:SENSe]]:ACPower	Channel power and ACPR	page 2-604
[[:SENSe]]:AVTime	Amplitude versus Time	page 2-614
[[:SENSe]]:CCDF	CCDF	page 2-619
[[:SENSe]]:DDEMod	General purpose digital modulation measurements (Option 21 only)	page 2-622
[[:SENSe]]:DPSA	DPX (Digital Phosphor) spectrum	page 2-635
[[:SENSe]]:FVTime	Frequency versus Time	page 2-647
[[:SENSe]]:IQVTime	IQ level versus Time	page 2-653
[[:SENSe]]:MCPower	MCPR (Multiple Carrier Power Ratio)	page 2-659
[[:SENSe]]:OBWidth	Occupied Bandwidth (OBW)	page 2-672
[[:SENSe]]:PHVTime	Phase versus Time	page 2-679
[[:SENSe]]:PULSe	Pulsed RF measurements (Option 20 only)	page 2-685
[[:SENSe]]:SGRam	Spectrogram	page 2-701
[[:SENSe]]:SPECtrum	Spectrum	page 2-713
[[:SENSe]]:TOVerview	Time overview	page 2-724

[[:SENSe] Basic Command Subgroup

The [[:SENSe] basic commands globally set up the analysis parameters.

Command Tree	Header	Parameter
	[[:SENSe]	
	:ACQuisition	
	:BANDwidth :BWIDth	<numeric_value>
	:FFRame	
	:ACTual?	
	:LIMit	<numeric_value>
	:STATe	<boolean>
	:MEMory	
	:AVAIlable	
	:SAMPles?	
	:CAPacity	
	:[:TIME]?	
	:USED	
	:[:PERCent]?	
	:MODE	AUTO SAMPles LENGth
	:SAMPles	<numeric_value>
	:SEConds	<numeric_value>
	:ANALysis	
	:ADVanced	
	:DITHer	<boolean>
	:HWARE	
	:STATus?	
	:LENGth	<numeric_value>
	:ACTual?	
	:AUTO	<boolean>
	:REFerence	ACQSTART TRIGGER
	:START	<numeric_value>
	:AUTO	<boolean>
	:MEASurement	
	:FREQuency	<numeric_value>
	:POWer	
	:UNITs	DBM DBV VOLTs WATTs DBUW DBW DBUV DBMV DBUA DBUV_M DBUA_M AMPS
	:REANalyze	
	:ROSCillator	
	SOURce	INTernal EXTernal

:SPECTrum	
:LENGth	<numeric_value>
:ACTual?	
:AUTO	<boolean>
:STARt	<numeric_value>
:TIMe	
:MODE	INDependent COMMon

[[:SENSe]:ACQuisition:BANDwidth]:BWIDth(?)

Sets or queries the acquisition bandwidth (frequency range of the acquisition) when [[:SENSe]:ACQuisition:MODE is set to SAMPlEs or LENGth.

Syntax [[:SENSe]:ACQuisition:BANDwidth]:BWIDth <value>
[[:SENSe]:ACQuisition:BANDwidth]:BWIDth?

Arguments <value>::=<NRf> specifies the acquisition bandwidth.
Range: 1 MHz to 40 MHz (Standard) / 110 MHz (Option 110).

Measurement Views All

Examples :SENSe:ACQuisition:BANDwidth 30MHz
sets the acquisition bandwidth to 30 MHz.

Related Commands [[:SENSe]:ACQuisition:MODE

[[:SENSe]:ACQuisition:FFRame:ACTual? (Query Only)

Queries the actual number of Fast Frames.

Syntax [[:SENSe]:ACQuisition:FFRame:ACTual?

Arguments None

Returns <NR1> The actual number of Fast Frames.

Measurement Views All

Examples :SENSe:ACQuisition:FFRame:ACTual?
might return 178 indicating that the actual number of Fast Frames is 178.

[:SENSe]:ACQuisition:FFRame:LiMit(?)

Sets or queries the limit number of Fast Frames.

Syntax [:SENSe]:ACQuisition:FFRame:Limit <value>
 [:SENSe]:ACQuisition:FFRame:Limit?

Arguments <value>::=<NR1> specifies the fast frame limit.
 Range: 1 to 65535 frames.

Measurement Views All

Examples :SENSe:ACQuisition:FFRame:Limit 500
 sets the Fast Frame limit to 500.

[:SENSe]:ACQuisition:FFRame:STATe(?)

Determines whether to enable or disable the Fast Frame.

Syntax [:SENSe]:ACQuisition:FFRame:STATe { OFF | ON | 0 | 1 }
 [:SENSe]:ACQuisition:FFRame:STATe?

Arguments OFF or 0 disables the Fast Frame.
 ON or 1 enables the Fast Frame.

Measurement Views All

Examples :SENSe:ACQuisition:FFRame:STATe ON
 enables the Fast Frame.

[[:SENSe]:ACQuisition:MEMory:AVAIlable:SAMPles? (Query Only)

Returns the amount of acquisition memory available in the instrument.

Syntax [:SENSe]:ACQuisition:MEMory:AVAIlable:SAMPles?

Arguments None

Returns <NRf> The amount of acquisition memory available in samples.

Measurement Views All

Examples :SENSe:ACQuisition:MEMory:AVAIlable:SAMPles?
might return 999.424E+3, indicating that 999424 samples are available.

[[:SENSe]:ACQuisition:MEMory:CAPacity[:TIME]? (Query Only)

Returns the acquisition memory capacity (maximum period of time that can be acquired with the acquisition memory).

Syntax [:SENSe]:ACQuisition:MEMory:CAPacity[:TIME]?

Arguments None

Returns <NRf> The acquisition memory capacity in seconds.

Measurement Views All

Examples :SENSe:ACQuisition:MEMory:CAPacity:TIME?
might return 26.651E-3, indicating that 26.651 ms can be acquired.

[[:SENSe]:ACQuisition:MEMory:USED[:PERCent]]? (Query Only)

Returns the percentage of the capacity used based on the current settings.

Syntax [:SENSe]:ACQuisition:MEMory:USED[:PERCent]?

Arguments None

Returns <NRf> The percentage of the capacity used.

Measurement Views All

Examples :SENSe:ACQuisition:MEMory:USED:PERCent?
might return 50.0, indicating that 50% is used.

[[:SENSe]:ACQuisition:MODE(?)]

Selects or queries the acquisition mode (how to determine the sampling parameters of acquisition bandwidth, samples, and length).

Syntax [:SENSe]:ACQuisition:MODE { AUTO | SAMPlEs | LENGth }
[:SENSe]:ACQuisition:MODE?

Arguments AUTO sets the all sampling parameters automatically.

SAMPlEs sets the acquisition bandwidth and samples manually, using the [:SENSe]:ACQuisition:BANDwidth[:BWIDth] and :SAMPlEs commands.

LENGth sets the acquisition bandwidth and length manually, using the [:SENSe]:ACQuisition:BANDwidth[:BWIDth] and :SEConds commands.

Measurement Views All

Examples :SENSe:ACQuisition:MODE AUTO
sets the all sampling parameters automatically.

Related Commands [:SENSe]:ACQuisition:BANDwidth[:BWIDth],
[:SENSe]:ACQuisition:SAMPlEs, [:SENSe]:ACQuisition:SEConds

[[:SENSe]:ACQuisition:SAMPles(?)]

Sets or queries the acquisition samples (number of samples acquired over the acquisition time) when [[:SENSe]:ACQuisition:MODE] is set to SAMPles.

Syntax [[:SENSe]:ACQuisition:SAMPles <value>
 [[:SENSe]:ACQuisition:SAMPles?

Arguments <value>::=<NR1> specifies the acquisition samples.
 Range: 2 to 1 G samples.

Measurement Views All

Examples :SENSe:ACQuisition:SAMPles 1114
 sets the acquisition samples to 1114.

Related Commands [[:SENSe]:ACQuisition:MODE]

[[:SENSe]:ACQuisition:SEConds(?)]

Sets or queries the acquisition length (time over which the acquisition occurs) when [[:SENSe]:ACQuisition:MODE] is set to LENGth.

Syntax [[:SENSe]:ACQuisition:SEConds <value>
 [[:SENSe]:ACQuisition:SEConds?

Arguments <value>::=<NRf> specifies the acquisition length.

Measurement Views All

Examples :SENSe:ACQuisition:SAMPles 12.5ms
 sets the acquisition length to 12.5 ms.

Related Commands [[:SENSe]:ACQuisition:MODE]

[[:SENSe]:ANALysis:ADVanced:DITHer(?)]

Determines whether to enable or disable dithering, or set it automatically.

Dither is a random low-level signal consisting of white noise of one quantizing level peak-to-peak amplitude which may be added to an analog signal prior to sampling for the purpose of minimizing quantization error.

Syntax [:SENSe]:ANALysis:ADVanced:DITHer { AUTO | ON | OFF }
[:SENSe]:ANALysis:ADVanced:DITHer?

Arguments AUTO specifies that the dither is set automatically.
ON enables dithering.
OFF disables dithering.

Measurement Views All

Examples :SENSe:ANALysis:ADVanced:DITHer ON
enables dithering.

[:SENSe]:ANALysis:ADVanced:DITHer:HWARe:STATus? (Query Only)

Queries the dithering hardware status.

Syntax [:SENSe]:ANALysis:ADVanced:DITHer:HWARe:STATus?

Arguments None

Returns One of the following status information.

Table 2-41: Dithering status

Status	Description
DUNaligned	Dithering is disabled and unaligned.
ON	Dithering is enabled
OFF	Dithering is disabled.

Measurement Views All

Examples :SENSe:ANALysis:ADVanced:DITHer:HWARe:STATus?
might return OFF, indicating that the dithering is disabled.

[[:SENSe]:ANALysis:LENGth(?)]

Sets or queries the analysis length. Programming a specified length sets [[:SENSe]:ANALysis:AUTO OFF.

Syntax [[:SENSe]:ANALysis:LENGth <value>
 [[:SENSe]:ANALysis:LENGth?

Arguments <value>::=<NRf> specifies the analysis length.
 Range: 10 ns to [(acquisition length) - 400 ns].

 If [(analysis start) + (analysis length)] > [(acquisition length) - 400 ns], the
 actual analysis length is reduced to [(acquisition length) - 200 ns].

 The unit of time is specified by the [[:SENSe]:TIME:UNITs command.

Measurement Views All

Examples :SENSe:ANALysis:LENGth 25.625us
 sets the analysis length to 25.625 μ s.

Related Commands [[:SENSe]:ANALysis:AUTO, [[:SENSe]:TIME:UNITs

[:SENSe]:ANALysis:LENGth:ACTual? (Query Only)

Queries the actual analysis length.

Syntax [:SENSe]:ANALysis:LENGth:ACTual?

Arguments None

Returns <NRF> Actual analysis length in seconds or symbols.
The unit of time is specified by the [:SENSe]:TIME:UNITs command.

Measurement Views All

Examples :SENSe:ANALysis:LENGth:ACTual?
might return 25.625E-6, indicating that the actual analysis length is 25.625 μ s.

Related Commands [:SENSe]:TIME:UNITs

[:SENSe]:ANALysis:LENGth:AUTO(?)

Determines whether to set the analysis length automatically or manually.

Syntax [:SENSe]:ANALysis:LENGth:AUTO { OFF | ON | 0 | 1 }
[:SENSe]:ANALysis:LENGth:AUTO?

Arguments OFF or 0 sets the analysis length manually, using the [:SENSe]:ANALysis:LENGth command.
ON or 1 sets the analysis length automatically.

Measurement Views All

Examples :SENSe:ANALysis:LENGth:AUTO ON
sets the analysis length automatically.

Related Commands [:SENSe]:ANALysis:LENGth

[[:SENSe]:ANALysis:REFeRence(?)]

Selects or queries the analysis time reference.

Syntax [:SENSe]:ANALysis:REFeRence { ACQSTART | TRIGGER }
 [:SENSe]:ANALysis:REFeRence?

Arguments ACQSTART specifies the acquisition start as the time zero reference.
 TRIGGER specifies the trigger point as the time zero reference.

Measurement Views All

Examples :SENSe:ANALysis:REFeRence ACQSTART
 specifies the acquisition start as the analysis time reference.

[[:SENSe]:ANALysis:STARt(?)]

Sets or queries the analysis offset time. Programming a specified offset time sets [:SENSe]:ANALysis:STARt:AUTO OFF.

Syntax [:SENSe]:ANALysis:STARt <value>
 [:SENSe]:ANALysis:STARt?

Arguments <value>::=<NRf> specifies the analysis offset time.
 Range: 0 to [(acquisition length) - 200 ns].
 If [(analysis start) + (analysis length)] > [(acquisition length) - 400 ns], the
 actual analysis length is reduced to [(acquisition length) - 200 ns].
 The unit of time is specified by the [:SENSe]:TiMe:UNITs command.

Measurement Views All

Examples :SENSe:ANALysis:STARt 23.5us
 sets the analysis offset to 23.5 μ s.

Related Commands [:SENSe]:ANALysis:LENGth, [:SENSe]:ANALysis:STARt:AUTO,
 [:SENSe]:TiMe:UNITs

[[:SENSe]:ANALysis:START:AUTO(?)]

Determines whether to set the analysis offset automatically or manually.

Syntax [:SENSe]:ANALysis:START:AUTO { OFF | ON | 0 | 1 }
 [:SENSe]:ANALysis:START:AUTO?

Arguments OFF or 0 sets the analysis offset manually, using the [:SENSe]:ANALysis:START command.
 ON or 1 sets the analysis offset automatically.

Measurement Views All

Examples :SENSe:ANALysis:START:AUTO ON
 sets the analysis offset automatically.

Related Commands [:SENSe]:ANALysis:START

[[:SENSe]:MEASurement:FREQuency(?)]

Sets or queries the measurement frequency.

Syntax [:SENSe]:MEASurement:FREQuency <value>
 [:SENSe]:MEASurement:FREQuency?

Arguments <value>::=<NRf> specifies the measurement frequency.
 Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views All

Examples :SENSe:MEASurement:FREQuency 7.5GHz
 sets the measurement frequency to 7.5 GHz.

[[:SENSe]:POWer:UNITs(?)]

Selects or queries the fundamental unit of power.

Syntax [:SENSe]:POWer:UNITs { DBM | DBV | VOLTs | WATTs | DBUW | DBW
| DBUV | DBMV | DBUA | DBUV_M | DBUA_M | AMPS }

[:SENSe]:POWer:UNITs?

Arguments Table 2-42 lists the arguments.

Table 2-42: Power units

Argument	Power unit
DBM	dBm
DBV	dBV
VOLTs	Volts
WATTs	Watts
DBUW	dB μ W
DBW	dBW
DBUV	dB μ V
DBMV	dBmV
DBUA	dB μ A
DBUV_M	dB μ V/m
DBUA_M	dB μ A/m
AMPS	Amps

NOTE. Select dB μ V/m or dB μ A/m unit when using an antenna table.

Measurement Views All

Examples :SENSe:POWer:UNITs DBM
specifies the fundamental unit of power as dBm.

[:SENSe]:REANalyze (No Query Form)

Have all measurements reanalyze the current acquisition record.

NOTE. *It is an overlapped command, which does not finish executing before the next command starts executing. Use the *OPC(?) and *WAI commands to synchronize all pending operations to the execution of this command.*

Syntax [:SENSe]:REANalyze

Arguments None

Measurement Views All

Examples :SENSe:REANalyze
have all measurements reanalyze the current acquisition record.

Related Commands *OPC, *WAI

[:SENSe]:ROSCillator:SOURce(?)

Selects or queries the frequency reference oscillator source.

Syntax [:SENSe]:ROSCillator:SOURce { INTernal | EXTernal }
 [:SENSe]:ROSCillator:SOURce?

Arguments INTernal specifies that the analyzer uses the 10 MHz internal oscillator.

 EXTernal specifies that the analyzer uses the external reference signal. Use the Ref In connector on the rear panel to input the signal.

 Selecting EXTernal initiates an attempt to lock the internal reference oscillator to the external reference signal. If the signal is not connected or is at an invalid frequency or amplitude, an error (2028, “External frequency reference signal not valid. Using internal reference”) is returned. If not able to lock to the external reference, an error (2029, “Unable to lock to external frequency reference. Using internal reference.”) is returned.

Measurement Views All

Examples :SENSe:ROSCillator:SOURce INTernal
 uses the 10 MHz internal oscillator for the frequency reference.

[[:SENSe]:SPECTrum:LENGth(?]

Sets or queries the spectrum length when [[:SENSe]:SPECTrum:TIME:MODE is INDepeNdeNt. Programming a specified length sets [[:SENSe]:SPECTrum:AUTO OFF.

Syntax [[:SENSe]:SPECTrum:LENGth <value>
[[:SENSe]:SPECTrum:LENGth?

Arguments <value>::=<NRf> specifies the spectrum length.
Range: 0 to [(acquisition length) - (spectrum start)].

If [(spectrum start) + (spectrum length)] > (acquisition length), the actual spectrum length is reduced to the acquisition length.

The unit of time is set by the [[:SENSe]:TIME:UNITs command.

Measurement Views All

Examples :SENSe:SPECTrum:LENGth 38.5us
sets the SPECTrum length to 38.5 μ s.

Related Commands [[:SENSe]:SPECTrum:AUTO, [[:SENSe]:SPECTrum:START,
[[:SENSe]:SPECTrum:TIME:MODE, [[:SENSe]:TIME:UNITs

[[:SENSe]:SPECTrum:LENGth:ACTual? (Query Only)

Queries the actual spectrum length.

Syntax [:SENSe]:SPECTrum:LENGth:ACTual?

Arguments None

Returns <NRf> Actual spectrum length in seconds or symbols.
The unit of time is specified by the [:SENSe]:TIME:UNITs command.

Measurement Views All

Examples :SENSe:SPECTrum:LENGth:ACTual?
might return 6.337E-6, indicating that the actual spectrum length is 6.337 μ s.

Related Commands [:SENSe]:TIME:UNITs

[[:SENSe]:SPECTrum:LENGth:AUTO(?)]

Determines whether to set the spectrum length automatically or manually when [:SENSe]:SPECTrum:TIME:MODE is INDependent.

Syntax [:SENSe]:SPECTrum:LENGth:AUTO { OFF | ON | 0 | 1 }
[:SENSe]:SPECTrum:LENGth:AUTO?

Arguments OFF or 0 sets the spectrum length manually, using the [:SENSe]:SPECTrum:LENGth command.
ON or 1 sets the spectrum length automatically.

Measurement Views All

Examples :SENSe:SPECTrum:LENGth:AUTO ON
sets the spectrum length automatically.

Related Commands [:SENSe]:SPECTrum:LENGth, [:SENSe]:SPECTrum:TIME:MODE

[[:SENSe]:SPECTrum:START(?)]

Sets or queries the spectrum offset time when [[:SENSe]:SPECTrum:TIME:MODE] is INDependent.

Syntax [[:SENSe]:SPECTrum:START <value>
[[:SENSe]:SPECTrum:START?

Arguments <value>::=<NRf> specifies the spectrum offset time.
Range: 0 to the acquisition length.

If [(spectrum start) + (spectrum length)] > (acquisition length), the actual spectrum length is reduced to the acquisition length.

The unit of time is set by the [[:SENSe]:TIME:UNITs] command.

Measurement Views All

Examples :SENSe:SPECTrum:START 23.5us
sets the analysis offset to 23.5 μ s.

Related Commands [[:SENSe]:SPECTrum:LENGth, [[:SENSe]:SPECTrum:TIME:MODE,
[[:SENSe]:TIME:UNITs]

[[:SENSe]:SPECTrum:TIME:MODE(?)]

Determines whether to set the spectrum time parameters automatically or manually.

Syntax [:SENSe]:SPECTrum:TIME:MODE { INDepeNdeNt | COMMon }
[:SENSe]:SPECTrum:TIME:MODE?

Arguments INDepeNdeNt sets the spectrum time parameters manually, using the [:SENSe]:SPECTrum:STARt and [:SENSe]:SPECTrum:LENGth commands.

COMMon sets the spectrum time parameters automatically using the analysis time settings.

Measurement Views All

Examples :SENSe:SPECTrum:TIME:MODE COMMon
sets the spectrum time parameters automatically.

Related Commands [:SENSe]:ANALysis commands
[:SENSe]:SPECTrum:STARt, [:SENSe]:SPECTrum:LENGth

[[:SENSe]:ACPower Subgroup

The [[:SENSe]:ACPower commands set up the conditions related to the Channel power and ACPR (Adjacent Channel Power Ratio) measurement.

Command Tree	Header	Parameter
	[SENSe]	
	:ACPower	
	:AVERage	OFF TIME FREQuency
	:COUNT	<numeric_value>
	:BANDwidth :BWIDth	
	[:RESolution]	<numeric_value>
	:ACTual?	
	:AUTO	<boolean>
	:CHANnel	
	:BANDwidth	
	:BWIDth	<numeric_value>
	:FILTer	RRCosine NONE
	:PAIRs	<numeric_value>
	:SPACing	<numeric_value>
	:CHIPrate	<numeric_value>
	:CLEar	
	:RESults	
	:FREQuency	
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:NFFloor	
	:STATe	<boolean>
	:OPTimize	
	:SPAN	RTBandwidth DRANge
	:RRCRolloff	<numeric_value>

[[:SENSe]:ACPower:AVERage(?)]

Selects or queries how to average waveform in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:AVERage { OFF | TIME | FREQuency }
 [:SENSe]:ACPower:AVERage?

Arguments OFF disables averaging.
 TIME averages waveform using time samples.
 FREQuency averages waveform using frequency samples.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:AVERage TIME
 averages waveform using time samples.

[[:SENSe]:ACPower:AVERage:COUNT(?)]

Sets or queries the number of traces for averaging in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:AVERage:COUNT <number>
 [:SENSe]:ACPower:AVERage:COUNT?

Arguments <number>::=<NR1> specifies the average count. Range: 2 to 10000.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:AVERage:COUNT 64
 sets the average count to 64.

[[:SENSe]:ACPower:BANDwidth|:BWIDth[:RESolution]](?)

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets [:SENSe]:ACPower:BANDwidth|:BWIDth[:RESolution]:AUTO OFF.

Syntax [:SENSe]:ACPower:BANDwidth|:BWIDth[:RESolution] <value>
[:SENSe]:ACPower:BANDwidth|:BWIDth[:RESolution]?

Arguments <value>::=<NRf> specifies the RBW.
Range: 100 Hz to 5 MHz.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:BANDwidth:RESolution 200kHz
sets the RBW to 200 kHz.

Related Commands [:SENSe]:ACPower:BANDwidth[:RESolution]:AUTO

[[:SENSe]:ACPower:BANDwidth|:BWIDth[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:BANDwidth|:BWIDth[:RESolution]:ACTual?

Arguments None

Returns <NRf> The actual RBW in Hz.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:BANDwidth:RESolution:ACTual?
might return 299.624E+3, indicating that the actual RBW is 299.624 kHz.

[[:SENSe]:ACPower:BANDwidth[:BWIDth[:RESolution]:AUTO(?]

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:BANDwidth[:BWIDth[:RESolution]:AUTO
 { OFF | ON | 0 | 1 }

 [:SENSe]:ACPower:BANDwidth[:BWIDth[:RESolution]:AUTO?

Arguments OFF or 0 specifies that the RBW is set manually using the [:SENSe]:ACPower:
 :BANDwidth[:BWIDth[:RESolution] command.

 ON or 1 specifies that the RBW is set automatically.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:BANDwidth:AUTO ON
 sets the RBW automatically.

Related Commands [:SENSe]:ACPower:BANDwidth[:BWIDth[:RESolution]

[[:SENSe]:ACPower:CHANnel:BANDwidth]:BWIDth(?)

Sets or queries frequency bandwidth of each channel (all share the same value) in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:CHANnel:BANDwidth|:BWIDth <value>
[:SENSe]:ACPower:CHANnel:BANDwidth|:BWIDth?

Arguments <value>::=<NRf> specifies the channel bandwidth.
Range: 1 Hz to full span.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:CHANnel:BANDwidth 1.5MHz
sets the channel bandwidth to 1.5 MHz.

[[:SENSe]:ACPower:CHANnel:FILTer(?)

Selects or queries the adjacent channel filter in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:CHANnel:FILTer { RRCosine | NONE }
[:SENSe]:ACPower:CHANnel:FILTer?

Arguments RRCosine uses the Root-Raised Cosine filter.
NONE uses no filter.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:CHANnel:FILTer RRCosine
uses the Root-Raised Cosine filter for the Channel power and ACPR measurement.

[[:SENSe]:ACPower:CHANnel:PAIRs(?)]

Sets or queries the number of adjacent channel pairs (upper and lower) in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:CHANnel:PAIRs <number>
 [:SENSe]:ACPower:CHANnel:PAIRs?

Arguments <number>::=<NR1> specifies the number of adjacent pairs.
 Range: 0 to 99.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:CHANnel:PAIRs 5
 sets five adjacent channel pairs.

[[:SENSe]:ACPower:CHANnel:SPACing(?)]

Sets or queries frequency difference between centers of each channel in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:CHANnel:SPACing <value>
 [:SENSe]:ACPower:CHANnel:SPACing?

Arguments <value>::=<NRf> specifies the channel-to-channel spacing.
 Range: 1 Hz to 1 GHz.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:CHANnel:SPACing 5MHz
 sets the channel-to-channel spacing to 5 MHz.

[[:SENSe]:ACPower:CHIPrate(?)]

Sets or queries the chip rate when [[:SENSe]:ACPower:CHANnel:FILTer] is set to RRCosine (Root Raised Cosine).

Syntax [[:SENSe]:ACPower:CHIPrate <value>
 [[:SENSe]:ACPower:CHIPrate?

Arguments <value>::=<NRf> specifies the chip rate.
 Range: 100 Hz to 105 MHz.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:CHIPrate 5kHz
 sets the chip rate to 5 kHz.

Related Commands [[:SENSe]:ACPower:CHANnel:FILTer]

[[:SENSe]:ACPower:CLEar:RESults (No Query Form)]

Restarts the average trace.

Syntax [[:SENSe]:ACPower:CLEar:RESults]

Arguments None

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:CLEar:RESults
 restarts the average trace.

[[:SENSe]:ACPower:FREQuency:STEP(?)]

Sets or queries the frequency step size in the Channel power and ACPR measurement. Programming a specified step size sets [:SENSe]:ACPower:FREQuency:STEP:AUTO OFF.

Syntax [:SENSe]:ACPower:FREQuency:STEP <value>
 [:SENSe]:ACPower:FREQuency:STEP?

Arguments <value>::=<NRf> specifies the frequency step size.
 Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:FREQuency:STEP 1kHz
 sets the frequency step size to 1 kHz.

Related Commands [:SENSe]:ACPower:FREQuency:STEP:AUTO

[[:SENSe]:ACPower:FREQuency:STEP:AUTO(?)]

Determines whether to set the frequency step size automatically or manually in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
 [:SENSe]:ACPower:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the [:SENSe]:ACPower:FREQuency:STEP command.
 ON or 1 specifies that the frequency step size is set automatically.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:FREQuency:STEP:AUTO ON
 specifies that the frequency step size is set automatically.

Related Commands [:SENSe]:ACPower:FREQuency:STEP

[[:SENSe]:ACPower:NFLoor:STATe(?)]

Determines whether to enable or disable the correction for noise floor.

Syntax [:SENSe]:ACPower:NFLoor:STATe { OFF | ON | 0 | 1 }
[:SENSe]:ACPower:NFLoor:STATe?

Arguments OFF or 0 disables the correction for noise floor.
ON or 1 enables the correction for noise floor.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:NFLoor:STATe ON
enables the correction for noise floor.

[[:SENSe]:ACPower:OPTimize:SPAN(?)]

Selects or queries the optimization method in the Channel power and ACPR measurement.

Syntax [:SENSe]:ACPower:OPTimize:SPAN { RTBandwidth | DRANge }
[:SENSe]:ACPower:OPTimize:SPAN?

Arguments RTBandwidth optimizes the measurement for real-time bandwidth.
DRANge optimizes the measurement for dynamic range.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:OPTimize:SPAN RTBandwidth
optimizes the measurement for real-time bandwidth.

[[:SENSe]:ACPower:RRCRolloff(?)]

Sets or queries the filter parameter (roll-off ratio) for the Root Raised Cosine filter.

Syntax [:SENSe]:ACPower:RRCRolloff <value>
 [:SENSe]:ACPower:RRCRolloff?

Arguments <value>::=<NRf> specifies the filter parameter.
 Range: 0.0001 to 1 in 0.0001 steps.

Measurement Views Channel power and ACPR

Examples :SENSe:ACPower:RRCRolloff 0.3
 sets the filter parameter to 0.3.

Related Commands [:SENSe]:ACPower:CHANnel:FILTer

[[:SENSe]:AVTime Subgroup

The [[:SENSe]:AVTime commands set up the conditions related to the Amplitude versus Time measurement.

Command Tree	Header	Parameter
	[[:SENSe]	
	:AVTime	
	:BANDwith :BWIDth	<numeric_value>
	:ACTual?	
	:CLEar	
	:RESults	
	:MAXTracepoints	ONEK TENK HUNDredk NEVerdecimate
	:METHod	SPAN TDBW
	:SPAN	<numeric_value>

[[:SENSe]:AVTime:BANDwith|:BWIDth(?]

Sets or queries the time-domain bandwidth filter in the Amplitude versus Time measurement. Programming a specified bandwidth disables the [[:SENSe]:AVTime:SPAN setting.

Syntax [[:SENSe]:AVTime:BANDwith|:BWIDth <value>
[[:SENSe]:AVTime:BANDwith|:BWIDth?

Arguments <value>::=<NRf> specifies the filter bandwidth.
Range: 1 Hz to 20 MHz (Standard) / 60 MHz (Option 110).

Measurement Views Amplitude versus Time

Examples :SENSe:AVTime:BANDwith 10MHz
sets the filter bandwidth to 10 MHz.

Related Commands [[:SENSe]:AVTime:SPAN

[[:SENSe]:AVTime:BANDwidth|:BWIDth:ACTual? (Query Only]

Queries the actual time-domain bandwidth in the Amplitude versus Time measurement.

Syntax [[:SENSe]:AVTime:BANDwidth|:BWIDth:ACTual?

Arguments None

Returns <NRf> The actual time-domain bandwidth in Hz.

Measurement Views Amplitude versus Time

Examples :SENSe:AVTime:BANDwidth:ACTual?
might return 20E+6, indicating that the actual time-domain bandwidth is 20 MHz.

[:SENSe]:AVTime:CLEar:RESults (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Syntax [:SENSe]:AVTime:CLEar:RESults

Arguments None

Measurement Views Amplitude versus Time

Examples :SENSe:AVTime:CLEar:RESults
restarts multi-trace functions.

[:SENSe]:AVTime:MAXTracepoints(?)

Selects or queries the maximum trace points in the Amplitude versus Time measurement.

Syntax [:SENSe]:AVTime:MAXTracepoints
 { ONEK | TENK | HUNDredk | NEVerdecimate }
[:SENSe]:AVTime:MAXTracepoints?

Arguments ONEK sets the maximum trace points to 1 k.
TENK sets the maximum trace points to 10 k.
HUNDredk sets the maximum trace points to 100 k.
NEVerdecimate never decimates the trace points.

Measurement Views Amplitude versus Time

Examples :SENSe:AVTime:MAXTracepoints TENK
sets the maximum trace points to 10 k.

[[:SENSe]:AVTime:METHod(?]

Selects or queries the method to set the measurement bandwidth in the Amplitude versus Time measurement.

Syntax [:SENSe]:AVTime:METHod { SPAN | TDBW }
 [:SENSe]:AVTime:METHod?

Arguments SPAN specifies that the measurement bandwidth is set by the frequency span, using the [:SENSe]:AVTime:SPAN command.

 TDBW specifies that the measurement bandwidth is set by the time-domain bandwidth, using the [:SENSe]:AVTime:BANDwidth|:BWIDth command.

Measurement Views Amplitude versus Time

Examples :SENSe:AVTime:METHod SPAN
 specifies that the measurement bandwidth is set by the frequency span.

Related Commands [:SENSe]:AVTime:BANDwidth|:BWIDth, [:SENSe]:AVTime:SPAN

[:SENSe]:AVTime:SPAN(?)

Sets or queries the frequency span in the Amplitude versus Time measurement. Programming a specified span disables the [:SENSe]:AVTime:BANDwidth [:BWIDth setting.

Syntax [:SENSe]:AVTime:SPAN <value>
[:SENSe]:AVTime:SPAN?

Arguments <value>::=<NRf> specifies the frequency span.
Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)

Measurement Views Amplitude versus Time

Examples :SENSe:AVTime:SPAN 5MHz
sets the frequency span to 5 MHz.

Related Commands [:SENSe]:AVTime:BANDwidth [:BWIDth

[[:SENSe]:CCDF Subgroup

The [[:SENSe]:CCDF commands set up the conditions related to the CCDF (Complementary Cumulative Distribution Function) measurement.

Command Tree	Header	Parameter
	[SENSe]	
	:CCDF	
	:BANDwidth :BWIDth	
	:CLEar	
	:TIME	
	:TOTal	
	:LENGth	<numeric_value>
	:TYPE	SINGLE TOTal CONTinuous

[[:SENSe]:CCDF:BANDwidth|:BWIDth(?)

Sets or queries the CCDF measurement bandwidth (frequency span).

Syntax [[:SENSe]:CCDF:BANDwidth|:BWIDth <value>
 [[:SENSe]:CCDF:BANDwidth|:BWIDth?

Arguments <value>::=<NRf> is the CCDF measurement bandwidth.
 Range: 10 Hz to 40 MHz (Standard) / 60 MHz (Option 110).

Measurement Views CCDF

Examples :SENSe:CCDF:BANDwidth 1MHz
 sets the CCDF measurement bandwidth to 1 MHz.

[[:SENSe]:CCDF:CLEAr (No Query Form)

Clears the CCDF accumulator and restarts the measurement.

Syntax [:SENSe]:CCDF:CLEAr

Arguments None

Measurement Views CCDF

Examples :SENSe:CCDF:CLEAr
clears the CCDF accumulator and restarts the measurement.

[[:SENSe]:CCDF:TIME:TOTal:LENGth(?]

Sets or queries the CCDF measurement time when [:SENSe]:CCDF:TIME:TYPE is set to TOTal.

Syntax [:SENSe]:CCDF:TIME:TOTal:LENGth <value>
[:SENSe]:CCDF:TIME:TOTal:LENGth?

Arguments <value>::=<NRf> specifies the CCDF measurement time.
Range: 20 ms to 100 s.

Measurement Views CCDF

Examples :SENSe:CCDF:TIME:TOTal:LENGth 10
sets the CCDF measurement time to 10 s.

Related Commands [:SENSe]:CCDF:TIME:TYPE

[[:SENSe]:CCDF:TIME:TYPE(?)]

Determines how to repeat the CCDF measurement.

Syntax [:SENSe]:CCDF:TIME:TYPE { SINGLE | TOTa1 | CONTinuous }
[:SENSe]:CCDF:TIME:TYPE?

Arguments SINGLE specifies that the analyzer sets the analysis length to 1 ms and then acquire data once to calculate CCDF.

TOTa1 specifies that the analyzer sets the analysis length to 20 ms and then repeats data acquisition and CCDF calculation for the time specified by the [:SENSe]:CCDF:TIME:LENGth command.

CONTinuous specifies that the analyzer sets the analysis length to 1 ms and then repeats data acquisition and CCDF calculation continuously. To reset the process, use the [:SENSe]:CCDF:CLEar command or the INITiate commands.

Measurement Views CCDF

Examples :SENSe:CCDF:TIME:TYPE ON
sets the CCDF measurement time automatically.

Related Commands INITiate commands, [:SENSe]:CCDF:CLEar, [:SENSe]:CCDF:TIME:LENGth

[[:SENSe]:DDEMod Subgroup (Option 21 Only)

The [[:SENSe]:DDEMod commands set up conditions related to the General Purpose Digital Modulation measurements.

Command Tree	Header	Parameter
	[[:SENSe]	
	:DDEMod	
	:ANALysis	
	:LENGth	<numeric_value>
	:ACTual?	
	:AUTO	<boolean>
	:BURSt	
	:DETEct	ON OFF
	:THREshold	<numeric_value>
	:CARRier	
	:OFFSet	<numeric_value>
	:FILTer	
	:ALPHa	<numeric_value>
	:MEASurement	OFF RRCosine RCOSine GAUSSian RECTangular IS95TXEQ_MEA IS95TX_MEA IS95REF
	:REFerence	OFF RRCosine RCOSine GAUSSian RECTangular IS95TXEQ_MEA IS95TX_MEA IS95REF
	:MAGNitude	
	:NORMalize	RSYMBOL MSYMBOL
	:MODulation	
	:TYPE	QPSK PSK8 D8PSK DQPSK PIOVER4DQPSK BPSK QAM16 QAM64 QAM256 MSK
	:SRATE	<numeric_value>
	:SWAP	
	:IQ	<boolean>
	:SYMBOL	
	:POINTs	ONE TWO FOUR EIGHT
	:SYNCh	
	:WORD	<boolean>
	:SYMBOL	<binary_block>
	:TIME	
	:UNITs	SECONDS SYMBOLs

[[:SENSe]:DDEMod:ANALysis:LENGth(?)]

Sets or queries the analysis length. Programming a specified length sets [[:SENSe]:DDEMod:ANALysis:AUTO OFF.

Syntax [[:SENSe]:DDEMod:ANALysis:LENGth <value>
[[:SENSe]:DDEMod:ANALysis:LENGth?

Arguments <value>::=<NRf> specifies the analysis length.
Range: 200ns to [(acquisition length) - 400 ns].

If [(analysis start) + (analysis length)] > [(acquisition length) - 400 ns], the actual analysis length is reduced to [(acquisition length) - 200 ns].

The unit of time is specified by the [[:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:ANALysis:LENGth 25.625us
sets the analysis length to 25.625 μ s.

Related Commands [[:SENSe]:DDEMod:ANALysis:AUTO, [[:SENSe]:DDEMod:TIME:UNITs

[[:SENSe]:DDEMod:ANALysis:LENGth:ACTual? (Query Only)

Queries the actual analysis length.

Syntax [:SENSe]:DDEMod:ANALysis:LENGth:ACTual?

Arguments None

Returns <Nrf> Actual analysis length in seconds or symbols.
The unit of time is specified by the [:SENSe]:DDEMod:TIME:UNITs command.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:ANALysis:LENGth:ACTual?
might return 25.625E-6, indicating that the actual analysis length is 25.625 μ s.

Related Commands [:SENSe]:DDEMod:TIME:UNITs

[[:SENSe]:DDEMod:ANALysis:LENGth:AUTO(?)]

Determines whether to set the analysis length automatically or manually.

Syntax [:SENSe]:DDEMod:ANALysis:LENGth:AUTO { OFF | ON | 0 | 1 }
[:SENSe]:DDEMod:ANALysis:LENGth:AUTO?

Arguments OFF or 0 sets the analysis length manually, using the [:SENSe]:DDEMod:ANALysis:LENGth command.
ON or 1 sets the analysis length automatically.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:ANALysis:LENGth:AUTO ON
sets the analysis length automatically.

Related Commands [:SENSe]:DDEMod:ANALysis:LENGth

[[:SENSe]:DDEMod:BURSt:DETECT(?)]

Determines how to detect bursts.

Syntax [:SENSe]:DDEMod:BURSt:DETECT { ON | OFF }
[:SENSe]:DDEMod:BURSt:DETECT?

Arguments ON analyzes just that burst period if a burst is found.
If a burst is not found, does not analyze but displays an error message.

OFF analyzes the whole analysis length.

NOTE. When selecting On and if the signal is not adequate for the demodulation, the measurement will fail and show an error message.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:BURSt:DETECT OFF
analyzes the whole analysis length.

Related Commands [:SENSe]:DDEMod:BURSt:THRESHOLD

[[:SENSe]:DDEMod:BURSt:THReshold(?)]

Sets or queries the threshold level above which the input signal is determined to be a burst.

Syntax [:SENSe]:DDEMod:BURSt:THReshold <value>
[:SENSe]:DDEMod:BURSt:THReshold?

Arguments <value>::=<NRf> specifies the threshold level for detecting bursts.
Range: -100 to -10 dBc.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:BURSt:THReshold -25
sets the threshold level to -25 dBc.

Related Commands [:SENSe]:DDEMod:BURSt:DETECT

[[:SENSe]:DDEMod:CARRier:OFFSet(?)]

Sets or queries the carrier frequency offset in the digital modulation analysis.

Syntax [:SENSe]:DDEMod:CARRier:OFFSet <value>
[:SENSe]:DDEMod:CARRier:OFFSet?

Arguments <value>::=<NRf> specifies the carrier frequency offset.
Range: -50 kHz to +50 kHz.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:CARRier:OFFSet 2kHz
sets the carrier frequency offset to 2 kHz.

[:SENSe]:DDEMod:FILTer:ALPHa(?)

Sets or queries the filter factor (α/BT) in the digital modulation analysis.

Syntax [:SENSe]:DDEMod:FILTer:ALPHa <value>
 [:SENSe]:DDEMod:FILTer:ALPHa?

Arguments <value>::=<NRf> specifies the filter factor.
 Range: 0.0001 to 1.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:FILTer:ALPHa 0.5
 sets the filter factor to 0.5.

[**:SENSe**]:DDEMod:FILTer:MEASurement(?)

Selects or queries the measurement filter in the digital modulation analysis.

Syntax [**:SENSe**]:DDEMod:FILTer:MEASurement
 { OFF | RRCosine | RCOSine | GAUSSian | RECTangular
 | IS95TXEQ_MEA | IS95TX_MEA | IS95REF }
 [**:SENSe**]:DDEMod:FILTer:MEASurement?

Arguments Table 2-43 lists the arguments.

Table 2-43: Digital modulation measurement filter

Argument	Measurement filter
OFF	No filter
RRCosine	Root Raised Cosine
RCOSine	Raised Cosine
GAUSSian	Gaussian
RECTangular	Rectangular
IS95TXEQ_MEA	IS95 receive filter for the transmitter configured with both the transmit filter and the phase equalizer.
IS95TX_MEA	IS95 receive filter for the transmitter configured with only the transmit filter.
IS95REF	IS95 reference filter including the response of the transmit filter and phase equalizer as well as the receive (complementary) filter.

Measurement Views General purpose digital modulation

Examples **:SENSe**:DDEMod:FILTer:MEASurement RRCosine
 selects the Root Raised Cosine filter as the measurement filter.

[[:SENSe]:DDEMod:FILTer:REFeRence(?)]

Selects or queries the reference filter in the digital modulation analysis.

Syntax [:SENSe]:DDEMod:FILTer:REFeRence
 { OFF | RRCosine | RCOSine | GAUSSian | RECTangular
 | IS95TXEQ_MEA | IS95TX_MEA | IS95REF }
 [:SENSe]:DDEMod:FILTer:REFeRence?

Arguments Refer to Table 2-30 on page 2-81.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:FILTer:REFeRence RCOSine
 selects the Raised Cosine filter as the reference filter.

[[:SENSe]:DDEMod:MAGNitude:NORMalize(?)]

Selects or queries the method for the magnitude normalization.

Syntax [:SENSe]:DDEMod:MAGNitude:NORMalize { RSYMBOL | MSYMBOL }
 [:SENSe]:DDEMod:MAGNitude:NORMalize?

Arguments RSYMBOL normalizes the magnitude with the RMS symbol magnitude.
 MSYMBOL normalizes the magnitude with the maximum symbol magnitude.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:MAGNitude:NORMalize RSYMBOL
 normalizes the magnitude with the RMS symbol magnitude.

[[:SENSe]:DDEMod:MODulation:TYPE(?]

Selects or queries the modulation type in the digital modulation analysis.

Syntax [:SENSe]:DDEMod:MODulation:TYPE { QPSK | PSK8 | D8PSK | DQPSK
 | PIOVER4DQPSK | BPSK | QAM16 | QAM64 | QAM256 | MSK }

[:SENSe]:DDEMod:MODulation:TYPE?

Arguments Table 2-44 lists the arguments and corresponding modulation type.

Table 2-44: Modulation type

Argument	Modulation type
QPSK	QPSK
PSK8	8PSK
D8PSK	D8PSK
DQPSK	DQPSK
PIOVER4DQPSK	$\pi/4$ QPSK
BPSK	BPSK
QAM16	16QAM
QAM64	64QAM
QAM256	256QAM
MSK	MSK

Measurement Views General purpose digital modulation

Examples :SENSe]:DDEMod:MODulation:TYPE QPSK
 selects QPSK modulation system.

[:SENSe]:DDEMod:SRATe(?)

Sets or queries the symbol rate in the digital modulation analysis.

Syntax [:SENSe]:DDEMod:SRATe <value>
 [:SENSe]:DDEMod:SRATe?

Arguments <value>::=<NRf> specifies the symbol rate.
 Range: 100 Hz to 122.9 MHz.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:SRATe 21.0E3
 sets the symbol rate to 21 kHz.

[:SENSe]:DDEMod:SWAP:IQ(?)

Determines whether or not to exchange I and Q data before demodulating.

Syntax [:SENSe]:DDEMod:SWAP:IQ { OFF | ON | 0 | 1 }
 [:SENSe]:DDEMod:SWAP:IQ?

Arguments OFF or 0 uses I and Q data as they are.
 ON or 1 exchanges I and Q data.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:SWAP:IQ ON
 exchanges I and Q data before demodulating.

[[:SENSe]:DDEMod:SYMBol:POINTs(?]

Selects or queries the number of points per symbol (how many points to use between symbols when connecting the dots).

NOTE. 1 is not valid for the GMSK modulation.

In the constellation view, select VECTors using the :TRACe<x>:CONSt:MODE command first to change Points/Symbol.

Syntax [:SENSe]:DDEMod:SYMBol:POINTs { ONE | TWO | FOUR | EIGHT }
[:SENSe]:DDEMod:SYMBol:POINTs?

Arguments ONE, TWO, FOUR, and EIGHT represent the number of points per symbol .

Measurement Views Constellation, EVM versus Time, Magnitude error versus Time,
Phase error versus Time

Examples :SENSe:DDEMod:SYMBol:POINTs FOUR
sets the number of points per symbol to four.

Related Commands :TRACe<x>:CONSt:MODE

[[:SENSe]:DDEMod:SYNCh:WORD(?]

Determines whether to enable or disable the synchronization word.

Syntax [:SENSe]:DDEMod:SYNCh:WORD { OFF | ON | 0 | 1 }
 [:SENSe]:DDEMod:SYNCh:WORD?

Arguments OFF or 0 disables the synchronization word.
 ON or 1 enables the synchronization word.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:SYNCh:WORD ON
 enables the synchronization word.

Related Commands [:SENSe]:DDEMod:SYNCh:WORD:SYMBol

[:SENSe]:DDEMod:SYNCh:WORD:SYMBol(?)

Sets or queries the synchronization word when [:SENSe]:DDEMod:SYNCh:WORD is ON. The word depends on the modulation type selected by the [:SENSe]:DDEMod:MODulation:TYPE command.

Syntax [:SENSe]:DDEMod:SYNCh:WORD:SYMBol <block>
[:SENSe]:DDEMod:SYNCh:WORD:SYMBol?

Arguments <block> ::= #<num_digit><num_byte><sym(1)><sym(2)>...<sym(n)>
Where
<num_digit> is the number of digits in <num_byte>.
<num_byte> is the number of bytes of data that follow.
<sym(n)> is the ⁿth symbol value of the sync word. 32-bit integer. n: Max 256.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:SYNCh:WORD:SYMBol #216xxxx (4 symbols)
sets a sync word composed of four symbols.

Related Commands [:SENSe]:DDEMod:MODulation:TYPE, [:SENSe]:DDEMod:SYNCh:WORD

[:SENSe]:DDEMod:Time:UNITs(?)

Selects or queries the fundamental unit of time.

Syntax [:SENSe]:DDEMod:Time:UNITs { SEConds | SYMBolS }
[:SENSe]:DDEMod:Time:UNITs?

Arguments SEConds specifies the fundamental unit of time as seconds.
SYMBolS specifies the fundamental unit of time as symbols.

Measurement Views General purpose digital modulation

Examples :SENSe:DDEMod:Time:UNITs SEConds
specifies the fundamental unit of time as seconds.

[[:SENSe]:DPSA Subgroup

The [[:SENSe]:DPSA commands set up the conditions related to the DPX (Digital Phosphor) Spectrum measurement.

Command Tree	Header	Parameter
	[[:SENSe]	
	:DPSA	
	:AUDio	
	:DEMod	
	:GAIN	<numeric_value>
	:RXBWidth	<numeric_value>
	:RXFrequency?	
	:STATe	<boolean>
	:TUNE	MR MARK1 MARK2 MARK3 MARK4 SMARker FREQcontrol
	:TYPE	AM FM
	:BANDwidth :BWIDth	
	[[:RESolution]	<numeric_value>
	:AUTO	<boolean>
	:CLEar	
	:RESults	
	:COLor	RED GREen BLUE CYAN BCYan YELLOW MAGenta GRAY TEMPerature SPECTral
	:MAXimum	<numeric_value>
	:MINimum	<numeric_value>
	:FREQuency	
	:CENTer	<numeric_value>
	:SPAN	<numeric_value>
	:START	<numeric_value>
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:STOP	<numeric_value>

[[:SENSe]:DPSA:AUDio:DEMod:GAIN(?)]

Sets or queries the audio gain.

NOTE. *The sound level is also affected by the Windows volume control.*

Syntax [:SENSe]:DPSA:AUDio:DEMod:GAIN <value>
 [:SENSe]:DPSA:AUDio:DEMod:GAIN?

Arguments <value>::=<NR1> specifies the audio gain.
 Range: 0 to 15 (integer).

Measurement Views DPX spectrum

Examples :SENSe:DPSA:AUDio:DEMod:GAIN 7
 sets the audio gain to 7.

[[:SENSe]:DPSA:AUDio:DEMod:RXBWidth(?)]

Sets or queries the receiver bandwidth in the audio demodulation.

Syntax [:SENSe]:DPSA:AUDio:DEMod:RXBWidth <value>
 [:SENSe]:DPSA:AUDio:DEMod:RXBWidth?

Arguments <value>::=<NRf> specifies the receiver bandwidth in the audio demodulation.
 Range: 1 kHz to 500 kHz.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:AUDio:DEMod:RXBWidth 30kHz
 sets the receiver bandwidth to 30 kHz.

[[:SENSe]:DPSA:AUDio:DEMod:RXFrequency? (Query Only)

Returns the receiver frequency in the audio demodulation.

The frequency depends on the setting of the [[:SENSe]:DPSA:AUDio:DEMod:TUNE command.

Syntax [[:SENSe]:DPSA:AUDio:DEMod:RXFrequency?

Returns <frequency>::=<NRf> is the receiver frequency in the audio demodulation.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:AUDio:DEMod:RXFrequency?
might return 80.3E+6, indicating that the receiver frequency is 80.3 MHz.

Related Commands [[:SENSe]:DPSA:AUDio:DEMod:TUNE

[[:SENSe]:DPSA:AUDio:DEMod:STATe(?)

Determines whether to enable or disable the audio demodulation.

Syntax [[:SENSe]:DPSA:AUDio:DEMod:STATe { OFF | ON | 0 | 1 }
[[:SENSe]:DPSA:AUDio:DEMod:STATe?

Arguments OFF or 0 disables the audio demodulation.
ON or 1 enables the audio demodulation.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:AUDio:DEMod:STATe ON
enables the audio demodulation.

[[:SENSe]:DPSA:AUDio:DEMod:TUNE(?]

Selects or queries how to determine the tuning frequency in the audio demodulation.

Syntax [:SENSe]:DPSA:AUDio:DEMod:TUNE { MR | MARK1 | MARK2 | MARK3
 | MARK4 | SMARker | FREQcontrol }

 [:SENSe]:DPSA:AUDio:DEMod:TUNE?

Arguments Table 2-45 lists the arguments.

Table 2-45: Frequency tuning

Argument	Tune with:
MR	Reference marker (MR)
MARK1	Marker 1 (M1)
MARK2	Marker 2 (M2)
MARK3	Marker 3 (M3)
MARK4	Marker 4 (M4)
SMARker	Selected marker
FREQcontrol	Center frequency setting

Measurement Views DPX spectrum

Examples :SENSe:DPSA:AUDio:DEMod:TUNE MARK1
 sets the tuning frequency to the value at Marker 1.

[[:SENSe]:DPSA:AUDio:DEMod:TYPE(?]

Selects or queries the modulation type in the audio demodulation.

Syntax [:SENSe]:DPSA:AUDio:DEMod:TYPE { AM | FM }
 [:SENSe]:DPSA:AUDio:DEMod:TYPE?

Arguments AM selects the AM (Amplitude Modulation).
 FM selects the FM (Frequency Modulation).

Measurement Views DPX spectrum

Examples :SENSe:DPSA:AUDio:DEMod:TYPE FM
 selects FM in the audio demodulation.

[[:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]](?)

Sets or queries the resolution bandwidth (RBW) in the DPX spectrum measurement. Programming a specified RBW sets [:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]:AUTO OFF.

Syntax [:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution] <value>
 [:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]?

Arguments <value>::=<NRf> is the resolution bandwidth.
 Range: 1 Hz to 5 MHz.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:BANDwidth:RESolution 200kHz
 sets the resolution bandwidth to 200 kHz.

Related Commands [:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]:AUTO

[[:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]:AUTO(?]

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the DPX spectrum measurement.

Syntax [:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]:AUTO
 { OFF | ON | 0 | 1 }

 [:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]:AUTO?

Arguments OFF or 0 specifies that the resolution bandwidth is set manually using the [:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution] command.

 ON or 1 specifies that the resolution bandwidth is set automatically.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:BANDwidth:AUTO ON
 sets the resolution bandwidth automatically.

Related Commands [:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]

[[:SENSe]:DPSA:CLEar:RESults (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Syntax [:SENSe]:DPSA:CLEar:RESults

Arguments None

Measurement Views DPX spectrum

Examples :SENSe:DPSA:CLEar:RESults
 restarts multi-trace functions.

[**:SENSe**]:DPSA:COLor(?)

Selects or queries the color palette of three-dimensional graphs.

Syntax [**:SENSe**]:DPSA:COLor { RED | GREen | BLUe | CYAN | BCYan
 | YELLow | MAGenta | GRAY | TEMPerature | SPECtral }
 [**:SENSe**]:DPSA:COLor?

Arguments Table 2-46 lists the arguments.

Table 2-46: Color palette for DPX spectrum

Argument	Palette
RED	Red
GREen	Green
BLUe	Blue
CYAN	Cyan
BCYan	Binary cyan
YELLow	Yellow
MAGenta	Magenta
GRAY	Gray
TEMPerature	Temperature
SPECtral	Spectral

Measurement Views DPX spectrum

Examples :SENSe:DPSA:COLor TEMPerature
 selects the temperature color palette.

[[:SENSe]:DPSA:COLor:MAXimum(?)]

Sets or queries the maximum value of the color axis in the DPX spectrum measurement.

Syntax [:SENSe]:DPSA:COLor:MAXimum <value>
[:SENSe]:DPSA:COLor:MAXimum?

Arguments <value>::=<NRf> specifies the maximum value of the color axis.
Range: The minimum value to 100%.
The minimum value is set using the [:SENSe]:DPSA:COLor:MIN command.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:COLor:MAXimum 90
sets the maximum value of the color axis to 90%.

Related Commands [:SENSe]:DPSA:COLor:MINimum

[[:SENSe]:DPSA:COLor:MINimum(?)]

Sets or queries the minimum value of the color axis in the DPX spectrum measurement.

Syntax [:SENSe]:DPSA:COLor:MINimum <value>
[:SENSe]:DPSA:COLor:MINimum?

Arguments <value>::=<NRf> specifies the minimum value of the color axis.
Range: 0% to the maximum value.
The maximum value is set using the [:SENSe]:DPSA:COLor:MAX command.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:COLor:MINimum 10
sets the minimum value of the color axis to 10%.

Related Commands [:SENSe]:DPSA:COLor:MAXimum

[**:SENSe**]:DPSA:FREQuency:CENTer(?)

Sets or queries the center frequency in the DPX spectrum measurement.

NOTE. The center, start and stop frequencies are set interlocking each other with the following relationships:

$$(start\ frequency) = (center\ frequency) - (span)/2$$

$$(stop\ frequency) = (center\ frequency) + (span)/2$$

Syntax [**:SENSe**]:DPSA:FREQuency:CENTer <value>

[**:SENSe**]:DPSA:FREQuency:CENTer?

Arguments <value>::=<NRf> specifies the center frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views DPX spectrum

Examples :SENSe:DPSA:FREQuency:CENTer 7.5GHz
sets the center frequency to 7.5 GHz.

Related Commands [**:SENSe**]:DPSA:FREQuency:START, [**:SENSe**]:DPSA:FREQuency:STOP

[**:SENSe**]:DPSA:FREQuency:SPAN(?)

Sets or queries the frequency span in the DPX spectrum measurement.

Syntax [**:SENSe**]:DPSA:FREQuency:SPAN <value>

[**:SENSe**]:DPSA:FREQuency:SPAN?

Arguments <value>::=<NRf> is the frequency span.
Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)

Measurement Views DPX spectrum

Examples :SENSe:DPSA:FREQuency:SPAN 20MHz
sets the span to 20 MHz.

[[:SENSe]:DPSA:FREQuency:STARt(?)]

Sets or queries the measurement start frequency (left edge on the graph) in the DPX spectrum measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [[:SENSe]:DPSA:FREQuency:CENTer] command.

Syntax [[:SENSe]:DPSA:FREQuency:STARt <value>
[[:SENSe]:DPSA:FREQuency:STARt?

Arguments <value>::=<NRf> is the measurement start frequency.
Range: (center frequency) \pm (span)/2.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:FREQuency:STARt 6.95GHz
sets the start frequency to 6.95 GHz.

Related Commands [[:SENSe]:DPSA:FREQuency:CENTer, [[:SENSe]:DPSA:FREQuency:STOP

[**:SENSe**]:DPSA:FREQuency:STEP(?)

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [**:SENSe**]:DPSA:FREQuency:STEP:AUTO OFF.

Syntax [**:SENSe**]:DPSA:FREQuency:STEP <value>
 [**:SENSe**]:DPSA:FREQuency:STEP?

Arguments <value>::=<NRf> specifies the frequency step size.
 Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views DPX spectrum

Examples :SENSe:DPSA:FREQuency:STEP 1.5kHz
 sets the step size to 1.5 kHz.

Related Commands [**:SENSe**]:DPSA:FREQuency:STEP:AUTO

[**:SENSe**]:DPSA:FREQuency:STEP:AUTO(?)

Determines whether to set the frequency step size automatically or manually.

Syntax [**:SENSe**]:DPSA:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
 [**:SENSe**]:DPSA:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the
 [**:SENSe**]:DPSA:FREQuency:STEP command.
 ON or 1 specifies that the frequency step size is set automatically.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:BANDwidth:AUTO ON
 sets the frequency step size automatically.

Related Commands [**:SENSe**]:DPSA:FREQuency:STEP

[[:SENSe]:DPSA:FREQuency:STOP(?)]

Sets or queries the measurement stop frequency (right edge of the graph) in the DPX spectrum measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [[:SENSe]:DPSA:FREQuency:CENTer] command.

Syntax [[:SENSe]:DPSA:FREQuency:STOP <value>
 [[:SENSe]:DPSA:FREQuency:STOP?

Arguments <value>::=<NRf> is the measurement stop frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views DPX spectrum

Examples :SENSe:DPSA:FREQuency:STOP 7.05GHz
 sets the stop frequency to 7.05 GHz.

Related Commands [[:SENSe]:DPSA:FREQuency:CENTer, [[:SENSe]:DPSA:FREQuency:START

[[:SENSe]:FVTime Subgroup

The [[:SENSe]:FVTime commands set up the conditions related to the Frequency versus Time measurement.

Command Tree	Header	Parameter
	[[:SENSe]	
	:FVTime	
	:CLEar	
	:RESults	
	:FREQuency	
	:CENTer	<numeric_value>
	:SPAN	<numeric_value>
	:START	<numeric_value>
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:STOP	<numeric_value>
	:MAXTracepoints	ONEK TENK HUNDredk NEVerdecimate

[[:SENSe]:FVTime:CLEar:RESults (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Syntax [[:SENSe]:FVTime:CLEar:RESults

Arguments None

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:CLEar:RESults
restarts multi-trace functions.

[[:SENSe]:FVTime:FREQuency:CENTer(?]

Sets or queries the center frequency in the Frequency versus Time measurement.

NOTE. The center, start and stop frequencies are set interlocking each other with the following relationships:

$$(start\ frequency) = (center\ frequency) - (span)/2$$

$$(stop\ frequency) = (center\ frequency) + (span)/2$$

Syntax [:SENSe]:FVTime:FREQuency:CENTer <value>

[:SENSe]:FVTime:FREQuency:CENTer?

Arguments <value>::=<NRf> specifies the center frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:FREQuency:CENTer 7.5GHz
sets the center frequency to 7.5 GHz.

Related Commands [:SENSe]:FVTime:FREQuency:START, [:SENSe]:FVTime:FREQuency:STOP

[[:SENSe]:FVTime:FREQuency:SPAN(?)]

Sets or queries the frequency span in the Frequency versus Time measurement.

Syntax [:SENSe]:FVTime:FREQuency:SPAN <value>
 [:SENSe]:FVTime:FREQuency:SPAN?

Arguments <value>::=<NRf> is the frequency span.
 Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:FREQuency:SPAN 20MHz
 sets the span to 20 MHz.

[[:SENSe]:FVTime:FREQuency:START(?)]

Sets or queries the measurement start frequency (left edge on the graph) in the Frequency versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [:SENSe]:FVTime:FREQuency:CENTer command.

Syntax [:SENSe]:FVTime:FREQuency:START <value>
 [:SENSe]:FVTime:FREQuency:START?

Arguments <value>::=<NRf> is the measurement start frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:FREQuency:START 6.95GHz
 sets the start frequency to 6.95 GHz.

Related Commands [:SENSe]:FVTime:FREQuency:CENTer, [:SENSe]:FVTime:FREQuency:STOP

[[:SENSe]:FVTime:FREQuency:STEP(?]

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [:SENSe]:FVTime:FREQuency:STEP:AUTO OFF.

Syntax [:SENSe]:FVTime:FREQuency:STEP <value>
[:SENSe]:FVTime:FREQuency:STEP?

Arguments <value>::=<NRf> specifies the frequency step size.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:FREQuency:STEP 1.5kHz
sets the step size to 1.5 kHz.

Related Commands [:SENSe]:FVTime:FREQuency:STEP:AUTO

[[:SENSe]:FVTime:FREQuency:STEP:AUTO(?]

Determines whether to set the frequency step size automatically or manually.

Syntax [:SENSe]:FVTime:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[:SENSe]:FVTime:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the
[:SENSe]:FVTime:FREQuency:STEP command.
ON or 1 specifies that the frequency step size is set automatically.

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:BANDwidth:AUTO ON
sets the frequency step size automatically.

Related Commands [:SENSe]:FVTime:FREQuency:STEP

[[:SENSe]:FVTime:FREQuency:STOP(?)]

Sets or queries the measurement stop frequency (right edge of the graph) in the Frequency versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [[:SENSe]:FVTime:FREQuency:CENTer] command.

Syntax [[:SENSe]:FVTime:FREQuency:STOP <value>
 [[:SENSe]:FVTime:FREQuency:STOP?

Arguments <value>::=<NRf> is the measurement stop frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:FREQuency:STOP 7.05GHz
 sets the stop frequency to 7.05 GHz.

Related Commands [[:SENSe]:FVTime:FREQuency:CENTer, [[:SENSe]:FVTime:FREQuency:START

[[:SENSe]:FVTime:MAXTracepoints(?)]

Selects or queries the maximum trace points in the Frequency versus Time measurement.

Syntax [:SENSe]:FVTime:MAXTracepoints
 { ONEK | TENK | HUNDredk | NEVerdecimate }

[:SENSe]:FVTime:MAXTracepoints?

Arguments ONEK sets the maximum trace points to 1 k.
 TENK sets the maximum trace points to 10 k.
 HUNDredk sets the maximum trace points to 100 k.
 NEVerdecimate never decimates the trace points.

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:MAXTracepoints TENK
 sets the maximum trace points to 10 k.

[:SENSe]:IQVTime Subgroup

The [:SENSe]:IQVTime commands set up the conditions related to the RF I&Q versus Time measurement.

Command Tree	Header	Parameter
	[:SENSe]	
	:IQVTime	
	:CLEar	
	:RESults	
	:FREQuency	
	:CENTer	<numeric_value>
	:SPAN	<numeric_value>
	:START	<numeric_value>
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:STOP	<numeric_value>
	MAXTracepoints	ONEK TENK HUNDredk NEVerdecimate

[:SENSe]:IQVTime:CLEar:RESults (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Syntax [:SENSe]:IQVTime:CLEar:RESults

Arguments None

Measurement Views RF I&Q versus Time

Examples :SENSe:IQVTime:CLEar:RESults
restarts multi-trace functions.

[[:SENSe]:IQVTime:FREQuency:CENTer(?]

Sets or queries the center frequency in the RF I&Q versus Time measurement.

NOTE. The center, start and stop frequencies are set interlocking each other with the following relationships:

$$(start\ frequency) = (center\ frequency) - (span)/2$$

$$(stop\ frequency) = (center\ frequency) + (span)/2$$

Syntax [[:SENSe]:IQVTime:FREQuency:CENTer <value>

[[:SENSe]:IQVTime:FREQuency:CENTer?

Arguments <value>::=<NRf> specifies the center frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views RF I&Q versus Time

Examples :SENSe:IQVTime:FREQuency:CENTer 7.5GHz
sets the center frequency to 7.5 GHz.

Related Commands [[:SENSe]:IQVTime:FREQuency:START, [[:SENSe]:IQVTime:FREQuency:STOP

[::SENSe]:IQVTime:FREQuency:SPAN(?)

Sets or queries the frequency span in the RF I&Q versus Time measurement.

Syntax [::SENSe]:IQVTime:FREQuency:SPAN <value>
 [::SENSe]:IQVTime:FREQuency:SPAN?

Arguments <value>::=<NRf> is the frequency span.
 Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)

Measurement Views RF I&Q versus Time

Examples :SENSe:IQVTime:FREQuency:SPAN 20MHz
 sets the span to 20 MHz.

[::SENSe]:IQVTime:FREQuency:START(?)

Sets or queries the measurement start frequency (left edge on the graph) in the RF I&Q versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [::SENSe]:IQVTime:FREQuency:CENTer command.

Syntax [::SENSe]:IQVTime:FREQuency:START <value>
 [::SENSe]:IQVTime:FREQuency:START?

Arguments <value>::=<NRf> is the measurement start frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views RF I&Q versus Time

Examples :SENSe:IQVTime:FREQuency:START 6.95GHz
 sets the start frequency to 6.95 GHz.

Related Commands [::SENSe]:IQVTime:FREQuency:CENTer,
 [::SENSe]:IQVTime:FREQuency:STOP

[:SENSe] :IQVTime:FREQuency:STEP(?)

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [:SENSe] :IQVTime:FREQuency:STEP:AUTO OFF.

Syntax [:SENSe] :IQVTime:FREQuency:STEP <value>
[:SENSe] :IQVTime:FREQuency:STEP?

Arguments <value> : :=<NRf> specifies the frequency step size.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views RF I&Q versus Time

Examples :SENSe:IQVTime:FREQuency:STEP 1.5kHz
sets the step size to 1.5 kHz.

Related Commands [:SENSe] :IQVTime:FREQuency:STEP:AUTO

[:SENSe] :IQVTime:FREQuency:STEP:AUTO(?)

Determines whether to set the frequency step size automatically or manually.

Syntax [:SENSe] :IQVTime:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[:SENSe] :IQVTime:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the [:SENSe] :IQVTime:FREQuency:STEP command.
ON or 1 specifies that the frequency step size is set automatically.

Measurement Views RF I&Q versus Time

Examples :SENSe:IQVTime:BANDwidth:AUTO ON
sets the frequency step size automatically.

Related Commands [:SENSe] :IQVTime:FREQuency:STEP

[[:SENSe]:IQVTime:FREQuency:STOP(?)]

Sets or queries the measurement stop frequency (right edge of the graph) in the RF I&Q versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [[:SENSe]:IQVTime:FREQuency:CENTer] command.

Syntax [[:SENSe]:IQVTime:FREQuency:STOP <value>
 [[:SENSe]:IQVTime:FREQuency:STOP?

Arguments <value>::=<NRf> is the measurement stop frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views RF I&Q versus Time

Examples :SENSe:IQVTime:FREQuency:STOP 7.05GHz
 sets the stop frequency to 7.05 GHz.

Related Commands [[:SENSe]:IQVTime:FREQuency:CENTer,
 [[:SENSe]:IQVTime:FREQuency:START

[[:SENSe]:IQVTime:MAXTracepoints(?)]

Selects or queries the maximum trace points in the RF I&Q versus Time measurement.

Syntax [:SENSe]:IQVTime:MAXTracepoints
 { ONEK | TENK | HUNDredk | NEVerdecimate }

 [:SENSe]:IQVTime:MAXTracepoints?

Arguments ONEK sets the maximum trace points to 1 k.
 TENK sets the maximum trace points to 10 k.
 HUNDredk sets the maximum trace points to 100 k.
 NEVerdecimate never decimates the trace points.

Measurement Views RF I&Q versus Time

Examples :SENSe:IQVTime:MAXTracepoints TENK
 sets the maximum trace points to 10 k.

[[:SENSe]:MCPower Subgroup

The [[:SENSe]:MCPower commands set up the conditions related to the MCPR (Multiple Carrier Power Ratio) measurement.

Command Tree	Header	Parameter
	[[:SENSe]	
	:MCPower	
	:AVERage	OFF TIME FREQuency
	:COUNT	<numeric_value>
	:BANDwidth :BWIDth	
	[[:RESolution]	<numeric_value>
	:ACTual?	
	:AUTO	<boolean>
	:CHANnel	
	:ADJacent	
	:ADD	<numeric_value>,<numeric_value>
	:DELeTe	<string>
	:FILTer	RRCosine NONE
	:MAIN	
	:BANDwidth	
	:BWIDth	<numeric_value>
	:COUNT	<numeric_value>
	:INACTive	<string>,<boolean>
	:SPACing	<numeric_value>
	:CHIPrate	<numeric_value>
	:CLEar	
	:RESults	
	:FREQuency	
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:NFLoor	
	:STATe	<boolean>
	:OPTimize	
	:SPAN	RTBandwidth DRANge
	:RCHannels?	
	:MAIN<x>	
	:TOTal	
	:RRCRolloff	<numeric_value>

[[:SENSe]:MCPower:AVERage(?)]

Selects or queries the average method in the MCPR measurement.

Syntax [:SENSe]:MCPower:AVERage { OFF | TIME | FREQuency }
[:SENSe]:MCPower:AVERage?

Arguments OFF disables averaging.
TIME performs averaging for time samples.
FREQuency performs averaging for frequency samples.

Measurement Views MCPR

Examples :SENSe:MCPower:AVERage TIME
performs averaging for time samples.

[[:SENSe]:MCPower:AVERage:COUNT(?)]

Sets or queries the average count in the MCPR measurement.

Syntax [:SENSe]:MCPower:AVERage:COUNT <value>
[:SENSe]:MCPower:AVERage:COUNT?

Arguments <value>::=<NR1> specifies the average count.
Range: 2 to 10000.

Measurement Views MCPR

Examples :SENSe:MCPower:AVERage:COUNT 256
sets the average count to 256.

[[:SENSe]:MCPower:BANDwidth|:BWIDth[:RESolution]](?)

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets [:SENSe]:MCPower:BANDwidth|:BWIDth[:RESolution]:AUTO OFF.

Syntax [:SENSe]:MCPower:BANDwidth|:BWIDth[:RESolution] <value>
 [:SENSe]:MCPower:BANDwidth|:BWIDth[:RESolution]?

Arguments <value>::=<NRf> specifies the RBW.
 Range: 100 Hz to 5 MHz.

Measurement Views MCPR

Examples :SENSe:MCPower:BANDwidth:RESolution 200kHz
 sets the RBW to 200 kHz.

Related Commands [:SENSe]:MCPower:BANDwidth|:BWIDth[:RESolution]:AUTO

[[:SENSe]:MCPower:BANDwidth|:BWIDth[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the MCPR measurement.

Syntax [:SENSe]:MCPower:BANDwidth|:BWIDth[:RESolution]:ACTual?

Arguments None

Returns <NRf> The actual RBW in Hz.

Measurement Views MCPR

Examples :SENSe:MCPower:BANDwidth:RESolution:ACTual?
 might return 299.624E+3, indicating that the actual RBW is 299.624 kHz.

[[:SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]:AUTO(?)]

Determines whether to set the resolution bandwidth (RBW) automatically or manually.

Syntax [:SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]:AUTO
 { OFF | ON | 0 | 1 }

[:SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]:AUTO?

Arguments OFF or 0 specifies that the resolution bandwidth is set manually using the
[:SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution] command.

ON or 1 specifies that the resolution bandwidth is set automatically.

Measurement Views MCPR

Examples :SENSe:MCPower:BANDwidth:AUTO ON
 sets the resolution bandwidth automatically.

Related Commands [:SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]

[:SENSe]:MCPower:CHANnel:ADJacent:ADD (No Query Form)

Adds a pair of upper and lower adjacent channels in the MCPR measurement.

Syntax [:SENSe]:MCPower:CHANnel:ADJacent:ADD <offset>,<bandwidth>

Arguments <offset>::=<NRf> specifies the offset from the center frequency for the adjacent channel. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).
 <bandwidth>::=<NRf> specifies the bandwidth of the adjacent channel. Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views MCPR

Examples :SENSe:MCPower:CHANnel:ADJacent:ADD 200kHz,80kHz
 adds a pair of upper and lower adjacent channels with the offset of ± 200 kHz and the bandwidth of 80 kHz.

[:SENSe]:MCPower:CHANnel:ADJacent:DELeTe (No Query Form)

Deletes a selected adjacent channel in the MCPR measurement.

Syntax [:SENSe]:MCPower:CHANnel:ADJacent:DELeTe <channel>

Arguments <channel>::=<string> specifies the channel to be deleted.
 Specify the channel with "A<n>" for the adjacent channel where <n> represents the channel number (<n> = 1, 2, 3,...). See the example below.

Measurement Views MCPR

Examples :SENSe:MCPower:CHANnel:DELeTe "A2"
 deletes A2 (the adjacent channel 2).

[:SENSe]:MCPower:CHANnel:FILTer(?)

Selects or queries the adjacent channel filter in the MCPR measurement.

Syntax [:SENSe]:MCPower:CHANnel:FILTer { RRCosine | NONE }
[:SENSe]:MCPower:CHANnel:FILTer?

Arguments RRCosine selects the Root-Raised-Cosine filter.
NONE uses no filter.

Measurement Views MCPR

Examples :SENSe:MCPower:CHANnel:FILTer RRCosine
selects Root-Raised-Cosine for the adjacent channel filter.

[:SENSe]:MCPower:CHANnel:MAIN:BANDwidth|:BWIDth(?)

Sets or queries the frequency bandwidth of the main channels (all share the same value) in the MCPR measurement.

Syntax [:SENSe]:MCPower:CHANnel:MAIN:BANDwidth|:BWIDth <value>
[:SENSe]:MCPower:CHANnel:MAIN:BANDwidth|:BWIDth?

Arguments <value>::=<NRf> specifies the main channel bandwidth.
Range: 1 Hz to full span.

Measurement Views MCPR

Examples :SENSe:MCPower:CHANnel:MAIN:BANDwidth 4.5MHz
sets the main channel bandwidth to 4.5 MHz.

[[:SENSe]:MCPower:CHANnel:MAIN:COUNT(?)]

Sets or queries the number of main channels in the MCPR measurement.
You can use this command to add and remove main channels.

Syntax [:SENSe]:MCPower:CHANnel:MAIN:COUNT <value>
 [:SENSe]:MCPower:CHANnel:MAIN:COUNT?

Arguments <value>::=<NRf> specifies the number of main channels.
Range: 1 to 99.

Measurement Views MCPR

Examples :SENSe:MCPower:CHANnel:MAIN:COUNT 3
 sets the the number of main channels to 3.

[[:SENSe]:MCPower:CHANnel:MAIN:INACTive(?)]

Makes a specified main channel inactive. You can set it on or off.
The query returns all inactive main channels.

Syntax [:SENSe]:MCPower:CHANnel:MAIN:INACTive <channel>,<boolean>
 [:SENSe]:MCPower:CHANnel:MAIN:INACTive?

Arguments <channel>::=<string> specifies the channel to be inactive.
Specify the channel with "M<n>" for the main channel where <n> represents the
channel number (<n> = 1, 2, 3,...). See the example below.

<boolean>::={ OFF | ON | 0 | 1 } specifies that the specified channel is
inactive (On) or not (Off).

Measurement Views MCPR

Examples :SENSe:MCPower:CHANnel:MAIN:INACTive "M2",ON
 makes the main channel 2 inactive.

[[:SENSe]:MCPower:CHANnel:MAIN:SPACing(?]

Sets or queries frequency difference between centers of each main channel in the MCPR measurement.

Syntax [:SENSe]:MCPower:CHANnel:MAIN:SPACing <value>
[:SENSe]:MCPower:CHANnel:MAIN:SPACing?

Arguments <value>::=<NRf> specifies the spacing between two adjacent main channels.
Range: 1 Hz to 1 GHz.

Measurement Views MCPR

Examples :SENSe:MCPower:CHANnel:MAIN:SPACing 5MHz
sets the main channel spacing to 5 MHz.

[[:SENSe]:MCPower:CHIPrate(?]

Sets or queries the chip rate in the MCPR measurement.
This command is valid when [:SENSe]:MCPower:CHANnel:FILTer is set to RRCosine (Root-Raised-Cosine).

Syntax [:SENSe]:MCPower:CHIPrate <value>
[:SENSe]:MCPower:CHIPrate?

Arguments <value>::=<NRf> specifies the chip rate.
Range: 100 Hz to 105 MHz.

Measurement Views MCPR

Examples :SENSe:MCPower:CHIPrate 1kHz
sets the chip rate to 1 kHz.

Related Commands [:SENSe]:MCPower:CHANnel:FILTer

[:SENSe]:MCPower:CLEar:RESults (No Query Form)

Restarts the average trace.

Syntax [:SENSe]:MCPower:CLEar:RESults

Arguments None

Measurement Views MCPR

Examples :SENSe:MCPower:CLEar:RESults
restarts the average trace.

[:SENSe]:MCPower:FREQuency:STEP(?)

Sets or queries the frequency step size. Programming a specified step size sets [:SENSe]:MCPower:FREQuency:STEP:AUTO OFF.

Syntax [:SENSe]:MCPower:FREQuency:STEP <value>
[:SENSe]:MCPower:FREQuency:STEP?

Arguments <value>::=<NRf> specifies the frequency step size.
Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views MCPR

Examples :SENSe:MCPower:FREQuency:STEP 50kHz
sets the frequency step size to 50 kHz.

Related Commands [:SENSe]:MCPower:FREQuency:STEP:AUTO

[:SENSe]:MCPower:FREQuency:STEP:AUTO(?)

Determines whether to set the frequency step size automatically or manually in the MCPR measurement.

Syntax [:SENSe]:MCPower:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[:SENSe]:MCPower:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the
[:SENSe]:MCPower:FREQuency:STEP command.
ON or 1 specifies that the frequency step size is set automatically.

Measurement Views MCPR

Examples :SENSe:MCPower:FREQuency:STEP:AUTO ON
specifies that the frequency step size is set automatically.

Related Commands [:SENSe]:MCPower:FREQuency:STEP

[:SENSe]:MCPower:NFLoor:STATE(?)

Determines whether to enable or disable correction for noise floor.

Syntax [:SENSe]:MCPower:NFLoor:STATE { OFF | ON | 0 | 1 }
[:SENSe]:MCPower:NFLoor:STATE?

Arguments OFF or 0 disables correction for noise floor.
ON or 1 enables correction for noise floor.

Measurement Views MCPR

Examples :SENSe:MCPower:NFLoor:STATE ON
enables correction for noise floor.

[:SENSe]:MCPower:OPTimize(?)

Selects or queries the optimization method in the MCPR measurement.

Syntax [:SENSe]:MCPower:OPTimize:SPAN { RTBandwidth | DRANge }
[:SENSe]:MCPower:OPTimize:SPAN?

Arguments RTBandwidth optimizes the measurement for real-time bandwidth.
DRANge optimizes the measurement for dynamic range.

Measurement Views MCPR

Examples :SENSe:MCPower:OPTimize:SPAN RTBandwidth
optimizes the measurement for real-time bandwidth.

[:SENSe]:MCPower:RChannels? (Query Only)

Queries the power reference in the MCPR measurement.

Syntax [:SENSe]:MCPower:RChannels?

Arguments None

Returns <power_ref>::={ Total | M<x> } where <x> = 1 to 99.

Total indicates that the power reference is the total power of all the active channels.

M<x> indicates that the power reference is the main channel with the index (<x>).

Measurement Views MCPR

Examples :SENSe:MCPower:RChannels?
might return M3, indicating that the power reference is the main channel 3.

[:SENSe]:MCPower:RChannels:MAIN<x> (No Query Form)

Sets the power reference to the main channel with the index (<x>) in the MCPR measurement.

Syntax [:SENSe]:MCPower:RChannels:MAIN<x>

Where <x> = 1 to 99, representing the main channel 1 to 99, respectively. The main channel must be defined using the [:SENSe]:MCPower:CHANnel:MAIN commands.

Arguments None

Measurement Views MCPR

Examples :SENSe:MCPower:RChannels:MAIN3
selects Main 3 for the power reference channel.

Related Commands [:SENSe]:MCPower:CHANnel:MAIN commands

[[:SENSe]:MCPower:RCHannels:TOTal (No Query Form)

Sets the power reference to the total power of all the active channels in the MCPR measurement.

Syntax [[:SENSe]:MCPower:RCHannels:TOTal

Arguments None

Measurement Views MCPR

Examples :SENSe:MCPower:RCHannels:TOTal
sets the power reference to the total power of all the active channels.

[[:SENSe]:MCPower:RRCRolloff(?]

Sets or queries the filter parameter (roll-off ratio) for the Root Raised Cosine filter.

Syntax [[:SENSe]:MCPower:RRCRolloff <value>
[[:SENSe]:MCPower:RRCRolloff?

Arguments <value>::=<NRf> specifies the filter parameter.
Range: 0.001 to 1, 0.0001 step.

Measurement Views MCPR

Examples :SENSe:MCPower:RRCRolloff 0.3
sets the filter parameter to 0.3.

Related Commands [[:SENSe]:MCPower:CHANnel:FILTer

[[:SENSe]:OBWidth Subgroup

The [[:SENSe]:OBWidth commands set up the conditions related to the Occupied Bandwidth (OBW) measurement.

Command Tree	Header	Parameter
	[SENSe]	
	:OBWidth	
	:AVERage	<boolean>
	:COUNT	<numeric_value>
	:BANDwidth :BWIDTH	
	:MEASurement	<numeric_value>
	[:RESolution]	<numeric_value>
	:ACTual?	
	:AUTO	<boolean>
	:CLEar	
	:RESults	
	:FREQuency	
	:CENTer	<numeric_value>
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:PERCent	<numeric_value>
	:XDBLevel	<numeric_value>

[[:SENSe]:OBWidth:AVERage(?)]

Selects or queries whether to enable or disable averaging in the Occupied Bandwidth measurement.

Syntax [:SENSe]:OBWidth:AVERage { OFF | ON | 0 | 1 }
[:SENSe]:OBWidth:AVERage?

Arguments OFF or 0 disables averaging.
ON or 1 enables averaging.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:AVERage ON
enables averaging.

[[:SENSe]:OBWidth:AVERage:COUNT(?)]

Sets or queries the number of measurements for averaging in the Occupied Bandwidth measurement.

Syntax [:SENSe]:OBWidth:AVERage:COUNT <number>
[:SENSe]:OBWidth:AVERage:COUNT?

Arguments <number>::=<NR1> specifies the average count. Range: 2 to 10000.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:AVERage:COUNT 64
sets the average count to 64.

[[:SENSe]:OBWidth:BANDwidth[:BWIDth:MEASurement(?)]

Sets or queries the measurement bandwidth to determine the total power in the Occupied Bandwidth measurement.

Syntax [:SENSe]:OBWidth:BANDwidth[:BWIDth:MEASurement <value>
[:SENSe]:OBWidth:BANDwidth[:BWIDth:MEASurement?

Arguments <value>::=<NRf> specifies the measurement bandwidth.
Range: 100 Hz to 109 MHz.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:BANDwidth:MEASurement 10MHz
sets the measurement bandwidth to 10 MHz.

[[:SENSe]:OBWidth:BANDwidth[:BWIDth[:RESolution](?)]

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets [:SENSe]:OBWidth:BANDwidth[:BWIDth[:RESolution]:AUTO OFF.

Syntax [:SENSe]:OBWidth:BANDwidth[:BWIDth[:RESolution] <value>
[:SENSe]:OBWidth:BANDwidth[:BWIDth[:RESolution]?

Arguments <value>::=<NRf> specifies the RBW.
Range: 100 Hz to 5 MHz.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:BANDwidth:RESolution 200kHz
sets the RBW to 200 kHz.

Related Commands [:SENSe]:OBWidth:BANDwidth[:RESolution]:AUTO

[[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the Occupied Bandwidth measurement.

Syntax [[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution]:ACTual?

Arguments None

Returns <NRf> The actual RBW in Hz.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:BANDwidth:RESolution:ACTual?
might return 299.624E+3, indicating that the actual RBW is 299.624 kHz.

[[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution]:AUTO(?)

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the Occupied Bandwidth measurement.

Syntax [[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution]:AUTO
{ OFF | ON | 0 | 1 }
[[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution]:AUTO?

Arguments OFF or 0 specifies that the RBW is set manually using the [[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution] command.
ON or 1 specifies that the RBW is set automatically.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:BANDwidth:AUTO ON
sets the RBW automatically.

Related Commands [[:SENSe]:OBWidth:BANDwidth]:BWIDth[:RESolution]

[:SENSe]:OBWidth:CLEar:RESults (No Query Form)

Restarts the average trace.

This command is valid when [:SENSe]:OBWidth:AVERage is set to ON.

Syntax [:SENSe]:OBWidth:CLEar:RESults

Arguments None

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:CLEar:RESults
restarts the average trace.

Related Commands [:SENSe]:OBWidth:AVERage

[:SENSe]:OBWidth:FREQuency:CENTer(?)

Sets or queries the center frequency in the Occupied Bandwidth measurement.

Syntax [:SENSe]:OBWidth:FREQuency:CENTer <value>
[:SENSe]:OBWidth:FREQuency:CENTer?

Arguments <value>::=<NRf> specifies the center frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:FREQuency:CENTer 7.5GHz
sets the center frequency to 7.5 GHz.

[[:SENSe]:OBWidth:FREQuency:STEP(?)]

Sets or queries the frequency step size in the Occupied Bandwidth measurement. Programming a specified step size sets [:SENSe]:OBWidth:FREQuency:STEP :AUTO OFF.

Syntax [:SENSe]:OBWidth:FREQuency:STEP <value>
[:SENSe]:OBWidth:FREQuency:STEP?

Arguments <value>::=<NRf> specifies the frequency step size.
Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:FREQuency:STEP 1kHz
sets the frequency step size to 1 kHz.

Related Commands [:SENSe]:OBWidth:FREQuency:STEP:AUTO

[[:SENSe]:OBWidth:FREQuency:STEP:AUTO(?)]

Determines whether to set the frequency step size automatically or manually in the Occupied Bandwidth measurement.

Syntax [:SENSe]:OBWidth:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[:SENSe]:OBWidth:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the [:SENSe]:OBWidth:FREQuency:STEP command.
ON or 1 specifies that the frequency step size is set automatically.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:FREQuency:STEP:AUTO ON
specifies that the frequency step size is set automatically.

Related Commands [:SENSe]:OBWidth:FREQuency:STEP

[[:SENSe]:OBWidth:PERCent(?)]

Sets or queries the occupied bandwidth percent power (power ratio of the occupied bandwidth to the measurement bandwidth).

Syntax [:SENSe]:OBWidth:PERCent <value>
 [:SENSe]:OBWidth:PERCent?

Arguments <value>::=<NRf> specifies the occupied bandwidth percent power.
 Range: 50 to 99.9%.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:PERCent 98
 sets the occupied bandwidth percent power to 98%.

[[:SENSe]:OBWidth:XDBLevel(?)]

Sets or queries the x dB level (how far down from the peak level the bandwidth is measured) in the x dB bandwidth measurement.

Syntax [:SENSe]:OBWidth:XDBLevel <value>
 [:SENSe]:OBWidth:XDBLevel?

Arguments <value>::=<NRf> specifies the x dB level.
 Range: -80 to -1 dB.

Measurement Views Occupied Bandwidth

Examples :SENSe:OBWidth:XDBLevel -10
 sets the x dB level to -10 dB.

[[:SENSe]:PHVTime Subgroup

The [[:SENSe]:PHVTime commands set up the conditions related to the Phase versus Time measurement.

Command Tree	Header	Parameter
	[[:SENSe]	
	:PHVTime	
	:CLEar	
	:RESults	
	:FREQuency	
	:CENTer	<numeric_value>
	:SPAN	<numeric_value>
	:START	<numeric_value>
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:STOP	<numeric_value>
	:MAXTracepoints	ONEK TENK HUNDredk NEVerdecimate

[[:SENSe]:PHVTime:CLEar:RESults (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Syntax [[:SENSe]:PHVTime:CLEar:RESults

Arguments None

Measurement Views Phase versus Time

Examples :SENSe:PHVTime:CLEar:RESults
restarts multi-trace functions.

[:SENSe]:PHVTime:FREQuency:CENTer(?)

Sets or queries the center frequency in the Phase versus Time measurement.

NOTE. The center, start and stop frequencies are set interlocking each other with the following relationships:

$$(start\ frequency) = (center\ frequency) - (span)/2$$

$$(stop\ frequency) = (center\ frequency) + (span)/2$$

Syntax [:SENSe]:PHVTime:FREQuency:CENTer <value>

[:SENSe]:PHVTime:FREQuency:CENTer?

Arguments <value>: :=<NRf> specifies the center frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Phase versus Time

Examples :SENSe:PHVTime:FREQuency:CENTer 7.5GHz
sets the center frequency to 7.5 GHz.

Related Commands [:SENSe]:PHVTime:FREQuency:START,
[:SENSe]:PHVTime:FREQuency:STOP

[::SENSe]:PHVTime:FREQuency:SPAN(?)

Sets or queries the frequency span in the Phase versus Time measurement.

Syntax [::SENSe]:PHVTime:FREQuency:SPAN <value>
 [::SENSe]:PHVTime:FREQuency:SPAN?

Arguments <value>::=<NRf> is the frequency span.
 Range: 10 Hz to 40 MHz (Standard) / 110 MHz (Option 110)

Measurement Views Phase versus Time

Examples :SENSe:PHVTime:FREQuency:SPAN 20MHz
 sets the span to 20 MHz.

[::SENSe]:PHVTime:FREQuency:START(?)

Sets or queries the measurement start frequency (left edge on the graph) in the Phase versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [::SENSe]:PHVTime:FREQuency:CENTer command.

Syntax [::SENSe]:PHVTime:FREQuency:START <value>
 [::SENSe]:PHVTime:FREQuency:START?

Arguments <value>::=<NRf> is the measurement start frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views Phase versus Time

Examples :SENSe:PHVTime:FREQuency:START 6.95GHz
 sets the start frequency to 6.95 GHz.

Related Commands [::SENSe]:PHVTime:FREQuency:CENTer,
 [::SENSe]:PHVTime:FREQuency:STOP

[:SENSe]:PHVTime:FREQuency:STEP(?)

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [:SENSe]:PHVTime:FREQuency:STEP:AUTO OFF.

Syntax [:SENSe]:PHVTime:FREQuency:STEP <value>
[:SENSe]:PHVTime:FREQuency:STEP?

Arguments <value>::=<NRf> specifies the frequency step size.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Phase versus Time

Examples :SENSe:PHVTime:FREQuency:STEP 1.5kHz
sets the step size to 1.5 kHz.

Related Commands [:SENSe]:PHVTime:FREQuency:STEP:AUTO

[:SENSe]:PHVTime:FREQuency:STEP:AUTO(?)

Determines whether to set the frequency step size automatically or manually.

Syntax [:SENSe]:PHVTime:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[:SENSe]:PHVTime:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the
[:SENSe]:PHVTime:FREQuency:STEP command.
ON or 1 specifies that the frequency step size is set automatically.

Measurement Views Phase versus Time

Examples :SENSe:PHVTime:BANDwidth:AUTO ON
sets the frequency step size automatically.

Related Commands [:SENSe]:PHVTime:FREQuency:STEP

[[:SENSe]:PHVTime:FREQuency:STOP(?)]

Sets or queries the measurement stop frequency (right edge of the graph) in the Phase versus Time measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [[:SENSe]:PHVTime:FREQuency:CENTer] command.

Syntax [[:SENSe]:PHVTime:FREQuency:STOP <value>
 [[:SENSe]:PHVTime:FREQuency:STOP?

Arguments <value>::=<NRf> is the measurement stop frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views Phase versus Time

Examples :SENSe:PHVTime:FREQuency:STOP 7.05GHz
 sets the stop frequency to 7.05 GHz.

Related Commands [[:SENSe]:PHVTime:FREQuency:CENTer,
 [[:SENSe]:PHVTime:FREQuency:START

[[:SENSe]:PHVTime:MAXTracepoints(?)]

Selects or queries the maximum trace points in the Phase versus Time measurement.

Syntax [:SENSe]:PHVTime:MAXTracepoints
 { ONEK | TENK | HUNDredk | NEVerdecimate }

[:SENSe]:PHVTime:MAXTracepoints?

Arguments ONEK sets the maximum trace points to 1 k.
 TENK sets the maximum trace points to 10 k.
 HUNDredk sets the maximum trace points to 100 k.
 NEVerdecimate never decimates the trace points.

Measurement Views Phase versus Time

Examples :SENSe:PHVTime:MAXTracepoints TENK
 sets the maximum trace points to 10 k.

[:SENSe]:PULSe Subgroup (Option 20 Only)

The [:SENSe]:PULSe commands set up the conditions related to the pulsed RF measurements.

Command Tree	Header	Parameter
	[:SENSe]	
	:PULSe	
	:ANALyze	
	:LEVel	VOLTage POWer
	:FIFTy	VOLTage POWer
	:HUNDred	AVERage INDEpendent
	:MEASurement	
	:TIME	
	:AUTO	<boolean>
	:START	<numeric_value>
	:STOP	<numeric_value>
	:PMLOCation	<numeric_value>
	:POINT	
	:LOCation	AVERage INDEpendent
	:RFALL	WIDE NARRow
	:RIPple	<numeric_value>
	:CARRier	
	:OFFSet	<numeric_value>
	:SEARch	AUTO MANual
	:DETECT	
	:MEASurement	<boolean>
	:NUMBER	<numeric_value>
	:POWER	
	[:THReshold]	<numeric_value>
	:TIME	
	[:THReshold]	<numeric_value>
	:FILTer	
	:BANDwidth :BWIDth	<numeric_value>
	:MEASurement	GAUSSian NONE MAXRtbw
	:FREFeRence	
	:AUTO	<boolean>
	:CHIRpbw	<numeric_value>
	:OFFSet	<numeric_value>
	:MODulation	
	:TYPE	CWConst CWCHange LCHirp
	:SIGNal	
	:TYPE	CWConst CWCHange LCHirp

[:SENSe]:PULSe:ANALyze:LEVel(?)

Selects or queries how to determine the 50% level for the pulsed RF measurements.

Syntax [:SENSe]:PULSe:ANALyze:LEVel { VOLTage | POWer }
[:SENSe]:PULSe:ANALyze:LEVel?

Arguments VOLTage uses -6 dB to determine the 50% level.
POWer uses -3 dB to determine the 50% level.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:LEVel POWer
uses -3 dB to determine the 50% level.

[:SENSe]:PULSe:ANALyze:LEVel:FIFTy(?)

Selects or queries how to determine the 50% level for the pulsed RF measurements. This command is equivalent to the [:SENSe]:PULSe:ANALyze:LEVel command.

Syntax [:SENSe]:PULSe:ANALyze:LEVel:FIFTy { VOLTage | POWer }
[:SENSe]:PULSe:ANALyze:LEVel:FIFTy?

Arguments VOLTage uses -6 dB to determine the 50% level.
POWer uses -3 dB to determine the 50% level.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:LEVel:FIFTy POWer
uses -3 dB to determine the 50% level.

Related Commands [:SENSe]:PULSe:ANALyze:LEVel

[:SENSe]:PULSe:ANALyze:LEVel:HUNDred(?)

Selects or queries how to determine the 100% level in the pulsed RF measurements. This command is equivalent to the [:SENSe]:PULSe:ANALyze:POINt:LOCation command.

Syntax [:SENSe]:PULSe:ANALyze:LEVel:HUNDred { AVERage | INDepeNdeNt }
[:SENSe]:PULSe:ANALyze:LEVel:HUNDred?

Arguments AVERage uses the average amplitude calculated for the pulse-on as the 100% reference to measure the rise and fall times.

INDepeNdeNt uses the amplitudes at the beginning and end of the pulse-on as the 100% references to measure the rise and fall times, respectively.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:LEVel:HUNDred AVERage
uses pulse average amplitude to set the 100% level.

Related Commands [:SENSe]:PULSe:ANALyze:POINt:LOCation

[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:AUTO(?)]

Determines whether to set the measurement time for frequency and phase results automatically or manually in the pulsed RF measurements.

Syntax `[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:AUTO { OFF | ON | 0 | 1 }
[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:AUTO?`

Arguments OFF or 0 sets the measurement time manually.
Use the `[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:START` and
`[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:STOP` commands
to set the measurement start and stop time.

ON or 1 sets the measurement time automatically.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples `:SENSe:PULSe:ANALyze:MEASurement:TIME:AUTO ON`
sets the measurement time for frequency and phase results automatically.

Related Commands `[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:START,`
`[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:STOP`

[:SENSe]:PULSe:ANALyze:MEASurement:TIME:START(?)

Sets or queries the measurement start time for frequency and phase results in the pulsed RF measurements.

Syntax [:SENSe]:PULSe:ANALyze:MEASurement:TIME:START <value>
 [:SENSe]:PULSe:ANALyze:MEASurement:TIME:START?

Arguments <value>::=<NRf> specifies the measurement start time from the 50% level of the pulse rising edge. Range: -100 to 100 ms.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:MEASurement:TIME:AUTO 2.8us
 sets the start time to 2.8 μ s from the 50% level of the pulse rising edge.

Related Commands [:SENSe]:PULSe:ANALyze:MEASurement:TIME:STOP

[:SENSe]:PULSe:ANALyze:MEASurement:TIME:STOP(?)

Sets or queries the measurement stop time for frequency and phase results in the pulsed RF measurements.

Syntax [:SENSe]:PULSe:ANALyze:MEASurement:TIME:STOP <value>
 [:SENSe]:PULSe:ANALyze:MEASurement:TIME:STOP?

Arguments <value>::=<NRf> specifies the measurement stop time from the 50% level of the pulse falling edge. Range: -100 to 100 ms.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:MEASurement:TIME:STOP 1.2us
 sets the stop time to 1.2 μ s from the 50% level of the pulse falling edge.

Related Commands [:SENSe]:PULSe:ANALyze:MEASurement:TIME:START

[:SENSe] :PULSe:ANALyze:PMLOCation(?)

Sets or queries the phase measurement location (the position along the pulse tops where the phase is measured) in the pulse-pulse phase measurement.

Syntax [:SENSe] :PULSe:ANALyze:PMLOCation <value>
 [:SENSe] :PULSe:ANALyze:PMLOCation?

Arguments <value>::=<NRf> specifies the pulse-pulse phase measurement location.
Range: 5 ns to 100 ms.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:PMLOCation 1.5ms
 sets the phase measurement location to 1.5 ms.

[:SENSe] :PULSe:ANALyze:POINt:LOCation(?)

Selects or queries the point location method in the pulsed RF measurements.

Syntax [:SENSe] :PULSe:ANALyze:POINt:LOCation { AVERage | INDePendent }
 [:SENSe] :PULSe:ANALyze:POINt:LOCation?

Arguments AVERage uses the average amplitude calculated for the pulse-on as the 100% reference to measure the rise and fall times.

 INDePendent uses the amplitudes at the beginning and end of the pulse-on as the 100% references to measure the rise and fall times, respectively.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:POINt:LOCation AVERage
 uses pulse average amplitude to locate points.

[:SENSe]:PULSe:ANALyze:RFALl(?)

Selects or queries the threshold levels to measure the rise/fall time.

Syntax [:SENSe]:PULSe:ANALyze:RFALl { WIDE | NARRow }
 [:SENSe]:PULSe:ANALyze:RFALl?

Arguments WIDE selects 10 – 90% to measure the rise/fall time.
 NARRow selects 20 – 80% to measure the rise/fall time.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:RFALl WIDE
 selects 10 – 90% to measure the rise/fall time.

[:SENSe]:PULSe:ANALyze:RIPPlE(?)

Sets or queries the ripple portion of the pulse top (that is, how much of the beginning and end of the pulse top is excluded from the ripple calculation).

Syntax [:SENSe]:PULSe:ANALyze:RIPPlE <value>
 [:SENSe]:PULSe:ANALyze:RIPPlE?

Arguments <value>::=<NRf> specifies the ripple portion of the pulse top.
 Range: 10 to 100% in 1% steps.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:ANALyze:RIPPlE 30
 sets the ripple portion to 30% of the pulse top.

[:SENSe]:PULSe:CARRier:OFFSet(?)

Sets or queries the carrier frequency offset.

Syntax [:SENSe]:PULSe:CARRier:OFFSet <value>
 [:SENSe]:PULSe:CARRier:OFFSet?

Arguments <value>::=<NRf> specifies the carrier frequency offset.
 Range: -50 kHz to +50 kHz.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:CARRier:OFFSet 2.5kHz
 sets the offset frequency to 2.5 kHz to the carrier.

Related Commands [:SENSe]:PULSe:CARRier:SEARch

[:SENSe]:PULSe:CARRier:SEARch(?)

Selects or queries how to detect the carrier in the pulsed RF measurements.

Syntax [:SENSe]:PULSe:CARRier:SEARch { AUTO | MANua1 }
 [:SENSe]:PULSe:CARRier:SEARch?

Arguments AUTO specifies that the carrier is detected automatically.
 MANua1 specifies that the carrier frequency offset is set manually, using the
 [:SENSe]:PULSe:CARRier:OFFSet command.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:CARRier:SEARch AUTO
 specifies that the carrier is detected automatically.

Related Commands [:SENSe]:PULSe:CARRier:OFFSet

[[:SENSe]:PULSe:DETECT:MEASurement(?)]

Determines whether or not to set the maximum number of pulses to measure within the analysis time.

Syntax [:SENSe]:PULSe:DETECT:MEASurement { OFF | ON | 0 | 1 }
[:SENSe]:PULSe:DETECT:MEASurement?

Arguments OFF or 0 measures all pulses (max. 1000) in the analysis time.
ON or 1 specifies that the maximum number of pulses is set manually, using the [:SENSe]:PULSe:DETECT:NUMBER command.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:DETECT:MEASurement ON
specifies that the maximum number of pulses is set manually.

Related Commands [:SENSe]:PULSe:DETECT:NUMBER

[[:SENSe]:PULSe:DETECT:NUMBer(?)]

Sets or queries the maximum number of pulses to measure within the analysis time when [[:SENSe]:PULSe:DETECT:MEASurement] is On.

Syntax [[:SENSe]:PULSe:DETECT:NUMBer <value>
 [[:SENSe]:PULSe:DETECT:NUMBer?

Arguments <value>::=<NRf> specifies the maximum number of pulses to measure within the analysis time. Range: 1 to 1000.

If the analysis time contains fewer pulses than this number, all of these are measured.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:DETECT:MEASurement 850
 sets the maximum number of pulses to 850.

Related Commands [[:SENSe]:PULSe:DETECT:MEASurement]

[[:SENSe]:PULSe:DETECT:POWer[:THReshold](?)

Sets or queries the power threshold to detect pulses.

Syntax [:SENSe]:PULSe:DETECT:POWer[:THReshold] <value>
[:SENSe]:PULSe:DETECT:POWer[:THReshold]?

Arguments <value>::=<NRf> specifies the power threshold to detect pulses.
Range: -70 to 0 dB.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:DETECT:POWer:THReshold -20
sets the power threshold to -20 dB.

[[:SENSe]:PULSe:DETECT:TIME[:THReshold](?)

Sets or queries the minimum off-time between pulses.

Syntax [:SENSe]:PULSe:DETECT:TIME[:THReshold] <value>
[:SENSe]:PULSe:DETECT:TIME[:THReshold]?

Arguments <value>::=<NRf> specifies the minimum off-time between pulses.
Range: 1 ns to 100 ms.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:DETECT:TIME:THReshold 1.5ms
sets the time threshold to 1.5 ms.

[[:SENSe]:PULSe:FILTer:BANDwidth|:BWiDth(?]

Sets or queries the filter or acquisition bandwidth when [[:SENSe]:PULSe:FILTer:MEASurement is set to GAUSSian or NONE (No filter), respectively.

Syntax [[:SENSe]:PULSe:FILTer:BANDwidth|:BWiDth <value>
[[:SENSe]:PULSe:FILTer:BANDwidth|:BWiDth?

Arguments <value>::=<NRf> specifies the filter/acquisition bandwidth depending the [[:SENSe]:PULSe:FILTer:MEASurement setting. The table below shows the setting range.

[[:SENSe]:PULSe:FILTer:MEASurement	Range
GAUSSian	100 Hz to 20 MHz (Standard) / 100 Hz to 55 MHz (Option 110) in 1-2-3-5 sequence.
NONE	152, 305, 610, 1.22 k, 2.44 k, 4.88 k, 9.76 k, 19.3 k, 39 k, 78 k, 156 k, 312 k, 625 k, 1.25 M, 2.5 M, 5 M, 10 M, 20 M, 40 MHz, and optionally 60 M and 110 MHz (Option 110).

You can enter any value, but it is rounded up to the next valid number.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:FILTer:MEASurement 10MHz
sets the filter bandwidth to 10 MHz.

Related Commands [[:SENSe]:PULSe:FILTer:MEASurement

[[:SENSe]:PULSe:FILTer:MEASurement(?)]

Selects or queries the measurement filter in the pulsed RF measurements.

Syntax [:SENSe]:PULSe:FILTer:MEASurement { GAUSSian | NONE | MAXRtbw }
[:SENSe]:PULSe:FILTer:MEASurement?

Arguments GAUSSian uses the Gaussian filter in the pulsed RF measurements.
Use the [:SENSe]:PULSe:FILTer:BANDwidth[:BWIDth] command to set the filter bandwidth.

NONE uses no filter.
Use the [:SENSe]:PULSe:FILTer:BANDwidth[:BWIDth] command to set the acquisition bandwidth.

MAXRtbw uses no filter. The acquisition bandwidth is fixed to the maximum real-time bandwidth: 40 MHz (Standard) or 110 MHz (Option 110).

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:FILTer:MEASurement GAUSSian
uses the Gaussian filter in the pulsed RF measurements.

Related Commands [:SENSe]:PULSe:FILTer:BANDwidth[:BWIDth]

[[:SENSe]:PULSe:FREference:AUTO(?)]

Determines whether to estimate the pulse frequency reference automatically or manually in the pulsed RF measurements.

Syntax [:SENSe]:PULSe:FREference:AUTO { OFF | ON | 0 | 1 }
[:SENSe]:PULSe:FREference:AUTO?

Measurement Views Pulse statistics, Pulse table, Pulse trace

Arguments OFF or 0 estimates the frequency reference manually.
Use the [:SENSe]:PULSe:FREference:OFFSet command to set the frequency offset.
Use the [:SENSe]:PULSe:FREference:CHIRpbw command to set the chirp bandwidth.

ON or 1 estimates the frequency reference automatically.

Examples :SENSe:PULSe:FREference:AUTO ON
specifies that the frequency reference is estimated automatically.

Related Commands [:SENSe]:PULSe:FREference:CHIRpbw
[:SENSe]:PULSe:FREference:OFFSet

[[:SENSe]:PULSe:FREference:CHIRpbw(?]

Sets or queries the chirp bandwidth. This command is valid when
[:SENSe]:PULSe:MODulation:TYPE is set to LCHirp and
[:SENSe]:PULSe:FREference:AUTO is set to OFF.

Syntax [:SENSe]:PULSe:FREference:CHIRpbw <value>
 [:SENSe]:PULSe:FREference:CHIRpbw?

Arguments <value>::=<NRf> specifies the chirp bandwidth.
Range: 100 Hz to 40 MHz (Standard) / 110 MHz (Option 110).

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:FREference:CHIRpbw 1.5MHz
sets the chirp bandwidth to 1.5 MHz.

Related Commands [:SENSe]:PULSe:FREference:AUTO, [:SENSe]:PULSe:MODulation:TYPE

[[:SENSe]:PULSe:FREference:OFFSet(?]

Sets or queries the frequency reference offset. This command is valid when
[:SENSe]:PULSe:FREference:AUTO is set to OFF.

Syntax [:SENSe]:PULSe:FREference:OFFSet <value>
 [:SENSe]:PULSe:FREference:OFFSet?

Arguments <value>::=<NRf> specifies the frequency reference offset.
Range: -50 kHz to +50 kHz.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:FREference:OFFSet 2.5kHz
sets the frequency offset to 2.5 kHz to the reference.

Related Commands [:SENSe]:PULSe:FREference:AUTO

[[:SENSe]:PULSe:MODulation:TYPE(?]

Selects or queries the modulation type in the pulsed RF measurements.
This command is equivalent to the [[:SENSe]:PULSe:SIGNal:TYPE command.

Syntax [[:SENSe]:PULSe:MODulation:TYPE { CWConst | CWCHange | LCHirp }
[[:SENSe]:PULSe:MODulation:TYPE?

Arguments CWConst selects the CW (continuous wave) with constant phase.
CWCHange selects the CW (continuous wave) with changing phase.
LCHirp selects the linear chirp.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:MODulation:TYPE CWCHange
selects the CW with changing phase as the modulation type.

Related Commands [[:SENSe]:PULSe:SIGNal:TYPE

[[:SENSe]:PULSe:SIGNal:TYPE(?]

Selects or queries the signal type in the pulsed RF measurements.

Syntax [[:SENSe]:PULSe:SIGNal:TYPE { CWConst | CWCHange | LCHirp }
[[:SENSe]:PULSe:SIGNal:TYPE?

Arguments CWConst selects the CW (continuous wave) with constant phase.
CWCHange selects the CW (continuous wave) with changing phase.
LCHirp selects the linear chirp.

Measurement Views Pulse statistics, Pulse table, Pulse trace

Examples :SENSe:PULSe:SIGNal:TYPE CWCHange
selects the CW with changing phase as the signal type.

[[:SENSe]:SGRam Subgroup

The [[:SENSe]:SGRam commands set up conditions related to the spectrogram.

Command Tree	Header	Parameter
	[[:SENSe]	
	:SGRam	
	:BANDwidth :BWIDth	
	:OPTimization	AUTO MAXDynrange MINNoise
	[[:RESolution]	<numeric_value>
	:ACTual?	
	:AUTO	<boolean>
	:MODE	<boolean>
	:COLor	RED GREen BLUe CYAN BCYan YELLow MAGenta GRAY TEMPerature SPECTral
	:MAXimum	
	:MINimum	
	:FFT	
	:WINDow	UNIForm BH4B FLATtop HANNing KAISer
	:FREQuency	
	:CENTer	<numeric_value>
	:SPAN	<numeric_value>
	:BANDwidth	
	[[:RESolution]	
	:RATio	<numeric_value>
	:MAXimum	
	:START	<numeric_value>
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:STOP	<numeric_value>

[[:SENSe]:SGRam:BANDwidth]:BWIDth:OPTimization(?)

Selects or queries the method of optimizing the gain and input bandwidth in the spectrogram.

Syntax [:SENSe]:SGRam:BANDwidth]:BWIDth:OPTimization
 { AUTO | MAXDynrange | MINNoise }

 [:SENSe]:SGRam:BANDwidth]:BWIDth:OPTimization?

Arguments AUTO optimizes automatically the gain and input bandwidth.

 MAXDynrange optimizes the gain and input bandwidth to maximize the dynamic range.

 MINNoise optimizes the gain and input bandwidth to minimize noise.

Measurement Views Spectrogram

Examples :SENSe:SGRam:BANDwidth:OPTimization AUTO
 optimizes automatically the gain and input bandwidth.

[[:SENSe]:SGRam:BANDwidth]:BWIDth[:RESolution](?)

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets [:SENSe]:SGRam:BANDwidth]:BWIDth:RESolution:AUTO OFF.

Syntax [:SENSe]:SGRam:BANDwidth]:BWIDth[:RESolution] <value>

 [:SENSe]:SGRam:BANDwidth]:BWIDth[:RESolution]?

Arguments <value>::=<NRf> specifies the RBW.
 Range: 1 Hz to 10 MHz.

Measurement Views Spectrogram

Examples :SENSe:SGRam:BANDwidth:RESolution 200kHz
 sets the RBW to 200 kHz.

Related Commands [:SENSe]:SGRam:BANDwidth]:BWIDth[:RESolution]:AUTO

[[:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the spectrogram.

Syntax [[:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:ACTual?

Arguments None

Returns <NRf> The actual RBW in Hz.

Measurement Views Spectrogram

Examples :SENSe:SGRam:BANDwidth:RESolution:ACTual?
might return 299.624E+3, indicating that the actual RBW is 299.624 kHz.

[[:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:AUTO(?]

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the spectrogram.

Syntax [[:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:AUTO
{ OFF | ON | 0 | 1 }
[[:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:AUTO?

Arguments OFF or 0 specifies that the resolution bandwidth is set manually using the [[:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution] command.

ON or 1 specifies that the resolution bandwidth is set automatically.

Measurement Views Spectrogram

Examples :SENSe:SGRam:BANDwidth:AUTO ON
sets the resolution bandwidth automatically.

Related Commands [[:SENSe]:DPSA:BANDwidth[:RESolution]

[[:SENSe]:SGRam:BANDwidth]:BWIDth[:RESolution]:MODE(?)

Determines whether to enable or disable the RBW processing in the spectrogram.

Syntax [:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:MODE
 { OFF | ON | 0 | 1 }

 [:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:MODE?

Arguments OFF or 0 disables the RBW processing. You can select the FFT window using the [:SENSe]:SGRam:FFT:WINDow command.

 ON or 1 enables the RBW processing. Refer to the [:SENSe]:SGRam:BANDwidth[:BWIDth:RESolution command to set the RBW.

Measurement Views Spectrogram

Examples :SENSe:SGRam:BANDwidth:MODE ON
 enables the RBW processing.

Related Commands [:SENSe]:SGRam:BANDwidth[:BWIDth:RESolution,
 [:SENSe]:SGRam:FFT:WINDow

[**:SENSe**]:**SGRam:COLor(?)**

Selects or queries the color palette of three-dimensional graphs.

Syntax [**:SENSe**]:**SGRam:COLor** { RED | GREen | BLUe | CYAN | BCYan
 | YELLow | MAGenta | GRAY | TEMPerature | SPECtral }
 [**:SENSe**]:**SGRam:COLor**?

Arguments Table 2-47 lists the arguments.

Table 2-47: Color palette for spectrogram

Argument	Palette
RED	Red
GREen	Green
BLUe	Blue
CYAN	Cyan
BCYan	Binary cyan
YELLow	Yellow
MAGenta	Magenta
GRAY	Gray
TEMPerature	Temperature
SPECtral	Spectral

Measurement Views Spectrogram

Examples :SENSe:SGRam:COLor TEMPerature
 selects the temperature color palette.

[[:SENSe]:SGRam:COLor:MAXimum(?)]

Sets or queries the maximum value of the color axis in the spectrogram.

Syntax [:SENSe]:SGRam:COLor:MAXimum <value>
 [:SENSe]:SGRam:COLor:MAXimum?

Arguments <value>::=<NRf> specifies the maximum value of the color axis.
 Range: -100 to +100 dBm.

Measurement Views Spectrogram

Examples :SENSe:SGRam:COLor:MAXimum 10
 sets the maximum value of the color axis to 10 dBm.

Related Commands [:SENSe]:SGRam:COLor:MINimum

[[:SENSe]:SGRam:COLor:MINimum(?)]

Sets or queries the minimum value of the color axis in the spectrogram.

Syntax [:SENSe]:SGRam:COLor:MINimum <value>
 [:SENSe]:SGRam:COLor:MINimum?

Arguments <value>::=<NRf> specifies the minimum value of the color axis.
 Range: -100 to +100 dBm.

Measurement Views Spectrogram

Examples :SENSe:SGRam:COLor:MINimum 10
 sets the minimum value of the color axis to 10 dBm.

Related Commands [:SENSe]:SGRam:COLor:MAXimum

[:SENSe] :SGRam :FFT :WINDow (?)

Selects or queries the FFT window in the Spectrum Analyzer mode.

Syntax [:SENSe] :SGRam :FFT :WINDow
 { UNIFORM | BH4B | FLATtop | HANNing | KAISer }
[:SENSe] :SGRam :FFT :WINDow?

Arguments UNIFORM selects the uniform window.
 BH4B selects the Blackman-Harris 4B type window.
 FLATtop selects the flat-top window.
 HANNing selects the Hanning window.
 KAISer selects the Kaiser window.

Measurement Views Spectrogram

Examples :SENSe :SGRam :FFT :WINDow HANNing
 selects the Hanning window.

[[:SENSe]:SGRam:FREQuency:CENTer(?]

Sets or queries the center frequency in the spectrogram.

NOTE. The center, start and stop frequencies are set interlocking each other with the following relationships:

$$(start\ frequency) = (center\ frequency) - (span)/2$$

$$(stop\ frequency) = (center\ frequency) + (span)/2$$

Syntax [:SENSe]:SGRam:FREQuency:CENTer <value>

[:SENSe]:SGRam:FREQuency:CENTer?

Arguments <value>::=<NRf> specifies the center frequency.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Spectrogram

Examples :SENSe:SGRam:FREQuency:CENTer 7.5GHz
sets the center frequency to 7.5 GHz.

Related Commands [:SENSe]:SGRam:FREQuency:STARt, [:SENSe]:SGRam:FREQuency:STOP

[[:SENSe]:SGRam:FREQuency:SPAN(?]

Sets or queries the frequency span in the spectrogram.

Syntax [[:SENSe]:SGRam:FREQuency:SPAN <value>

[[:SENSe]:SGRam:FREQuency:SPAN?

Arguments <value>::=<Nrf> specifies the frequency span.
Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Spectrogram

Examples :SENSe:SGRam:FREQuency:SPAN 20MHz
sets the span to 20 MHz.

[[:SENSe]:SGRam:FREQuency:SPAN:BANDwidth[:RESolution]:RATio(?]

Sets or queries the ratio of span to RBW (Resolution Bandwidth) in the spectrogram. This command is valid when [[:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:AUTO is set to On.

Syntax [[:SENSe]:SGRam:FREQuency:SPAN:BANDwidth[:RESolution]:RATio
<value>

[[:SENSe]:SGRam:FREQuency:SPAN:BANDwidth[:RESolution]:RATio?

Arguments <value>::=<Nrf> specifies the ratio of span to RBW.
Range: 20 to 1000.

Programming a specified ratio sets the RBW (= span/ratio), which is rounded down to the nearest valid value.

Measurement Views Spectrogram

Examples :SENSe:SGRam:FREQuency:SPAN:BANDwidth:RESolution:RATio 200
sets the ratio to 200, setting the RBW to 200 kHz for the span of 40 MHz.

Related Commands [[:SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:AUTO

[[:SENSe]:SGRam:FREQuency:SPAN:MAXimum (No Query Form)

Sets the frequency range to the maximum real-time span in the spectrogram.

Syntax `[[:SENSe]:SGRam:FREQuency:SPAN:MAXimum <value>`

Arguments None

Measurement Views Spectrogram

Examples `:SENSe:SGRam:FREQuency:SPAN:MAXimum`
sets the frequency range to the maximum real-time span.

[[:SENSe]:SGRam:FREQuency:STARt(?]

Sets or queries the measurement start frequency (left edge of the graph) in the spectrogram.

The center, start and stop frequencies are set interlocking each other. Refer to the `[[:SENSe]:SGRam:FREQuency:CENTer` command.

Syntax `[[:SENSe]:SGRam:FREQuency:STARt <value>`
`[[:SENSe]:SGRam:FREQuency:STARt?`

Arguments `<value>::=<NRf>` is the measurement start frequency.
Range: $(\text{center frequency}) \pm (\text{span})/2$.

Measurement Views Spectrogram

Examples `:SENSe:SGRam:FREQuency:STARt 6.95GHz`
sets the start frequency to 6.95 GHz.

Related Commands `[[:SENSe]:SGRam:FREQuency:CENTer`, `[[:SENSe]:SGRam:FREQuency:STOP`

[[:SENSe]:SGRam:FREQuency:STEP(?)]

Sets or queries the frequency step size. Programming a specified step size sets [[:SENSe]:SGRam:FREQuency:STEP:AUTO OFF.

Syntax [[:SENSe]:SGRam:FREQuency:STEP <value>
[[:SENSe]:SGRam:FREQuency:STEP?

Arguments <value>::=<NRf> specifies the frequency step size.
Range: 0 to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Spectrogram

Examples :SENSe:SGRam:FREQuency:STEP 1kHz
sets the frequency step size to 1 kHz.

Related Commands [[:SENSe]:SGRam:FREQuency:STEP:AUTO

[[:SENSe]:SGRam:FREQuency:STEP:AUTO(?)]

Determines whether to set the frequency step size automatically or manually in the spectrogram.

Syntax [[:SENSe]:SGRam:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[[:SENSe]:SGRam:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the [[:SENSe]:SGRam:FREQuency:STEP command.
ON or 1 specifies that the frequency step size is set automatically.

Measurement Views Spectrogram

Examples :SENSe:SGRam:FREQuency:STEP:AUTO ON
specifies that the frequency step size is set automatically.

Related Commands [[:SENSe]:SGRam:FREQuency:STEP

[[:SENSe]:SGRam:FREQuency:STOP(?)]

Sets or queries the measurement stop frequency (right edge of the graph) in the spectrogram.

The center, start and stop frequencies are set interlocking each other. Refer to the [[:SENSe]:SGRam:FREQuency:CENTer] command.

Syntax [[:SENSe]:SGRam:FREQuency:STOP <value>
 [[:SENSe]:SGRam:FREQuency:STOP?

Arguments <value>::=<NRf> is the measurement start frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views Spectrogram

Examples :SENSe:SGRam:FREQuency:STOP 7.05GHz
 sets the stop frequency to 7.05 GHz.

Related Commands [[:SENSe]:SGRam:FREQuency:CENTer,
 [[:SENSe]:SGRam:FREQuency:START

[[:SENSe]:SPECTrum Subgroup

The [[:SENSe]:SPECTrum commands set up the conditions related to the Spectrum measurement.

Command Tree	Header	Parameter
	[[:SENSe]	
	:SPECTrum	
	:BANDwidth :BWIDth	
	:OPTimization	AUTO MAXDynrange MINNoise
	[[:RESolution]	<numeric_value>
	:ACTual?	
	:AUTO	<boolean>
	:MODE	<boolean>
	:CLEar	
	:RESults	
	:FFT	
	:WINDow	UNIFORM BH4B FLATtop HANNing KAISer
	:FREQuency	
	:CENTer	<numeric_value>
	:SPAN	<numeric_value>
	:BANDwidth	
	[[:RESolution]	
	:RATio	<numeric_value>
	:START	<numeric_value>
	:STEP	<numeric_value>
	:AUTO	<boolean>
	:STOP	<numeric_value>
	:MAX	
	:SPAN	
	:POINTs	
	:COUNT	P801 P2401 P4001 P8001 P10401

[[:SENSe]:SPECTrum:BANDwidth]:BWIDth:OPTimization(?)

Selects or queries the method of optimizing the gain and input bandwidth in the spectrum measurement.

Syntax [:SENSe]:SPECTrum:BANDwidth]:BWIDth:OPTimization
 { AUTO | MAXDynrange | MINNoise }

 [:SENSe]:SPECTrum:BANDwidth]:BWIDth:OPTimization?

Arguments AUTO optimizes automatically the gain and input bandwidth.

 MAXDynrange optimizes the gain and input bandwidth to maximize the dynamic range.

 MINNoise optimizes the gain and input bandwidth to minimize noise.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:BANDwidth:OPTimization AUTO
 optimizes automatically the gain and input bandwidth.

[[:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution](?)

Sets or queries the resolution bandwidth (RBW). Programming a specified RBW sets [:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution]:AUTO OFF.

Syntax [:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution] <value>

 [:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution]?

Arguments <value>::=<NRf> specifies the RBW.
 Range: 1 Hz to 10 MHz.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:BANDwidth:RESolution 200kHz
 sets the RBW to 200 kHz.

Related Commands [:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution]:AUTO

[[:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:ACTual? (Query Only)

Queries the actual resolution bandwidth (RBW) in the spectrum measurement.

Syntax `[[:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:ACTual?`

Arguments None

Returns <NRf> The actual RBW in Hz.

Measurement Views Spectrum

Examples `:SENSe:SPECTrum:BANDwidth:RESolution:ACTual?`
might return 299.624E+3, indicating that the actual RBW is 299.624 kHz.

[[:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:AUTO(?]

Determines whether to set the resolution bandwidth (RBW) automatically or manually in the spectrum measurement.

Syntax `[[:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:AUTO
{ OFF | ON | 0 | 1 }
[[:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:AUTO?`

Arguments OFF or 0 specifies that the resolution bandwidth is set manually using the `[[:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]` command.
ON or 1 specifies that the resolution bandwidth is set automatically.

Measurement Views Spectrum

Examples `:SENSe:SPECTrum:BANDwidth:AUTO ON`
sets the resolution bandwidth automatically.

Related Commands `[[:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]`

[[:SENSe]:SPECTrum:BANDwidth]:BWIDth[:RESolution]:MODE(?)

Determines whether to enable or disable the RBW process.

Syntax [:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:MODE
 { OFF | ON | 0 | 1 }

 [:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:MODE?

Arguments OFF or 0 disables the RBW process. You can select the FFT window using the [:SENSe]:SPECTrum:FFT:WINDow command.

 ON or 1 enables the RBW process. You can set the RBW using the [:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution] and :AUTO commands.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:BANDwidth:MODE ON
 enables the RBW process.

Related Commands [:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution],
 [:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:AUTO,
 [:SENSe]:SPECTrum:FFT:WINDow

[[:SENSe]:SPECTrum:CLEAr:RESults (No Query Form)

Restarts multi-trace functions (Average and Max/Min Hold).

Syntax [:SENSe]:SPECTrum:CLEAr:RESults

Arguments None

Measurement Views Spectrum

Examples :SENSe:SPECTrum:CLEAr:RESults
 restarts multi-trace functions.

[:SENSe]:SPECTrum:FFT:WINDow(?)

Selects or queries the FFT window in the spectrum measurement.

Syntax [:SENSe]:SPECTrum:FFT:WINDow
 { UNIFORM | BH4B | FLATtop | HANNing | KAISer }
[:SENSe]:SPECTrum:FFT:WINDow?

Arguments UNIFORM selects the uniform window.
 BH4B selects the Blackman-Harris 4B type window.
 FLATtop selects the flat-top window.
 HANNing selects the Hanning window.
 KAISer selects the Kaiser window.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:FFT:WINDow HANNing
 selects the Hanning window.

[:SENSe]:SPECTrum:FREQuency:CENTer(?)

Sets or queries the center frequency in the spectrum measurement.

NOTE. The center, start and stop frequencies are set interlocking each other with the following relationships:

$$(start\ frequency) = (center\ frequency) - (span)/2$$

$$(stop\ frequency) = (center\ frequency) + (span)/2$$

Syntax [:SENSe]:SPECTrum:FREQuency:CENTer <value>
 [:SENSe]:SPECTrum:FREQuency:CENTer?

Arguments <value>::=<NRf> specifies the center frequency.
 Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Spectrum

Examples :SENSe:SPECTrum:FREQuency:CENTer 7.5GHz
 sets the center frequency to 7.5 GHz.

Related Commands [:SENSe]:SPECTrum:FREQuency:START
 [:SENSe]:SPECTrum:FREQuency:STOP

[[:SENSe]:SPECTrum:FREQuency:SPAN(?)]

Sets or queries the frequency span in the spectrum measurement.

Syntax [:SENSe]:SPECTrum:FREQuency:SPAN <value>
 [:SENSe]:SPECTrum:FREQuency:SPAN?

Arguments <value>::=<NRf> specifies the frequency span.
 Range: 10 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Spectrum

Examples :SENSe:SPECTrum:FREQuency:SPAN 20MHz
 sets the span to 20 MHz.

[[:SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio(?)]

Sets or queries the ratio of span to RBW (Resolution Bandwidth) in the spectrum measurement. This command is valid when [:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:AUTO] is set to On.

Syntax [:SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio
 <value>
 [:SENSe]:SPECTrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio?

Arguments <value>::=<NRf> specifies the ratio of span to RBW.
 Range: 20 to 1000.
 Programming a specified ratio sets the RBW (= span/ratio), which is rounded down to the nearest valid value.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:FREQuency:SPAN:BANDwidth:RESolution:RATio
 200
 sets the ratio to 200, setting the RBW to 200 kHz for the span of 40 MHz.

Related Commands [:SENSe]:SPECTrum:BANDwidth[:BWIDth[:RESolution]:AUTO]

[[:SENSe]:SPECTrum:FREQuency:STARt(?)]

Sets or queries the measurement start frequency (left edge on the graph) in the spectrum measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [[:SENSe]:SPECTrum:FREQuency:CENTer] command.

Syntax [[:SENSe]:SPECTrum:FREQuency:STARt <value>
 [[:SENSe]:SPECTrum:FREQuency:STARt?

Arguments <value>::=<NRf> is the measurement start frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:FREQuency:STARt 6.95GHz
 sets the start frequency to 6.95 GHz.

Related Commands [[:SENSe]:SPECTrum:FREQuency:CENTer
 [[:SENSe]:SPECTrum:FREQuency:STOP

[[:SENSe]:SPECTrum:FREQuency:STEP(?]

Sets or queries the frequency step size (the amount per press by which the up or down key changes the setting value). Programming a specified step size sets [[:SENSe]:SPECTrum:FREQuency:STEP:AUTO OFF.

Syntax [[:SENSe]:SPECTrum:FREQuency:STEP <value>
[[:SENSe]:SPECTrum:FREQuency:STEP?

Arguments <value>::=<NRf> specifies the frequency step size.
Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Spectrum

Examples :SENSe:SPECTrum:FREQuency:STEP 1.5kHz
sets the step size to 1.5 kHz.

Related Commands [[:SENSe]:SPECTrum:FREQuency:STEP:AUTO

[[:SENSe]:SPECTrum:FREQuency:STEP:AUTO(?]

Determines whether to set the frequency step size automatically or manually.

Syntax [[:SENSe]:SPECTrum:FREQuency:STEP:AUTO { OFF | ON | 0 | 1 }
[[:SENSe]:SPECTrum:FREQuency:STEP:AUTO?

Arguments OFF or 0 specifies that the frequency step size is set manually using the [[:SENSe]:SPECTrum:FREQuency:STEP command.
ON or 1 specifies that the frequency step size is set automatically.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:BANDwidth:AUTO ON
sets the frequency step size automatically.

Related Commands [[:SENSe]:SPECTrum:FREQuency:STEP

[[:SENSe]:SPECTrum:FREQuency:STOP(?)]

Sets or queries the measurement stop frequency (right edge on the graph) in the spectrum measurement.

The center, start and stop frequencies are set interlocking each other. Refer to the [[:SENSe]:SPECTrum:FREQuency:CENTer] command.

Syntax [[:SENSe]:SPECTrum:FREQuency:STOP <value>
 [[:SENSe]:SPECTrum:FREQuency:STOP?

Arguments <value>::=<NRf> is the measurement start frequency.
 Range: (center frequency) \pm (span)/2.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:FREQuency:STOP 7.05GHz
 sets the stop frequency to 7.05 GHz.

Related Commands [[:SENSe]:SPECTrum:FREQuency:CENTer
 [[:SENSe]:SPECTrum:FREQuency:START

[[:SENSe]:SPECTrum:MAX:SPAN (No Query Form)

Sets the frequency span to the maximum real-time span.

Syntax [:SENSe]:SPECTrum:MAX:SPAN

Arguments None

Measurement Views Spectrum

Examples :SENSe:SPECTrum::MAX:SPAN
sets the frequency span to the maximum real-time span.

[[:SENSe]:SPECTrum:POINts:COUNT(?]

Sets or queries the number of sample points on the signal spectrum.

Syntax [:SENSe]:SPECTrum:POINts:COUNT
 { P801 | P2401 | P4001 | P8001 | P10401 }
[:SENSe]:SPECTrum:POINts:COUNT?

Arguments P801 sets the number of sample points to 801.
P2401 sets the number of sample points to 2401.
P4001 sets the number of sample points to 4001.
P8001 sets the number of sample points to 8001.
P10401 sets the number of sample points to 10401.

Measurement Views Spectrum

Examples :SENSe:SPECTrum:POINts:COUNT P801
sets the number of sample points to 801.

[[:SENSe]:TOVerview Subgroup

The [[:SENSe]:TOVerview commands set up conditions for the Time Overview.

Command Tree	Header	Parameter
	[[:SENSe]	
	:TOVerview	
	:FREQuency	
	:CENTer	<numeric_value>
	:MAXTracepoints	ONEK TĒNK HUNDredk NEVerdecimate

[[:SENSe]:TOVerview:FREQuency:CENTer(?)]

Sets or queries the center frequency in the time overview.

Syntax [:SENSe]:TOVerview:FREQuency:CENTer <value>
 [:SENSe]:TOVerview:FREQuency:CENTer?

Arguments <value>::=<NRf> specifies the center frequency.
 Range: 0 Hz to 6.2 GHz (RSA6106A) / 14 GHz (RSA6114A).

Measurement Views Time overview

Examples :SENSe:TOVerview:FREQuency:CENTer 7.5GHz
 sets the center frequency to 7.5 GHz.

[[:SENSe]:TOVerview:MAXTracepoints(?)]

Selects or queries the maximum trace points in the time overview.

Syntax [:SENSe]:TOVerview:MAXTracepoints
 { ONEK | TENK | HUNDredk | NEVerdecimate }
 [:SENSe]:TOVerview:MAXTracepoints?

Arguments ONEK sets the maximum trace points to 1 k.
 TENK sets the maximum trace points to 10 k.
 HUNDredk sets the maximum trace points to 100 k.
 NEVerdecimate never decimates the trace points.

Measurement Views Time overview

Examples :SENSe:TOVerview:MAXTracepoints TENK
 sets the maximum trace points to 10 k.

STATus Commands

The STATus commands control the SCPI-defined status reporting structures. In addition to those in IEEE 488.2, the analyzer has questionable and operation registers defined in SCPI. These registers conform to the IEEE 488.2 specification and each is comprised of a condition register, an event register, an enable register, and negative and positive transition filters.

NOTE. For details on the registers, refer to Status and Events beginning on page 3-1.

Command Tree

Header	Parameter
:STATus	
:ACPower	
:EVENTs?	
:AVTime	
:EVENTs?	
:CCDF	
:EVENTs?	
:CONSte	
:EVENTs?	
:DPSA	
:EVENTs?	
:EVM	
:EVENTs?	
:FVTime	
:EVENTs?	
:IQVTime	
:EVENTs?	
:MCPower	
:EVENTs?	
:MERRor	
:EVENTs?	
:OBWidth	
:EVENTs?	

```

:OPERation
  :CONDition?
  :ENABle          <bit_value>
  [:EVENT]?
  :NTRansition     <bit_value>
  :PTRansition     <bit_value>
:PERRor
  :EVENTs?
:PHVTime
  :EVENTs?
:PRESet
:PULSe
  :RESult
  :EVENTs?
  :STATistics
  :EVENTs?
  :TRACe
  :EVENTs?
:QUEStionable
  :CONDition?
  :ENABle          <bit_value>
  [:EVENT]?
  :NTRansition     <bit_value>
  :PTRansition     <bit_value>
  :CALibration
    :CONDition?
    :ENABle        <bit_value>
    [:EVENT]?
    :NTRansition   <bit_value>
    :PTRansition   <bit_value>
  :FREquency
    :CONDition?
    :ENABle        <bit_value>
    [:EVENT]?
    :NTRansition   <bit_value>
    :PTRansition   <bit_value>
:SGRam
  :EVENTs?
:SPECTrum
  :EVENTs?
:SQUALity
  :EVENTs?

```

:STATus:ACPower:EVENTs? (Query Only)

Returns the current events for the Channel power and ACPR measurement.

Syntax :STATus:ACPower:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Channel power and ACPR

Examples STATus:ACPower:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:AVTime:EVENTs? (Query Only)

Returns the current events for the Amplitude versus Time measurement.

Syntax :STATus:AVTime:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Amplitude versus Time

Examples STATus:AVTime:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:CCDF:EVENTs? (Query Only)

Returns the current events for the CCDF measurement.

Syntax :STATus:CCDF:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views CCDF

Examples STATus:CCDF:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:CONStE:EVENTs? (Query Only)

Returns the current events for the constellation measurement.

Syntax :STATus:CONStE:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Constellation

Examples STATus:CONStE:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:DPSA:EVENTs? (Query Only)

Returns the current events for the DPX spectrum measurement.

Syntax :STATus:CCDF:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views DPX spectrum

Examples STATus:DPSA:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:EVM:EVENTs? (Query Only)

Returns the current events for the EVM versus Time measurement.

Syntax :STATus:EVM:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views EVM versus Time

Examples STATus:EVM:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:FVTime:EVENTs? (Query Only)

Returns the current events for the Frequency versus Time measurement.

Syntax :STATus:FVTime:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Frequency versus Time

Examples STATus:FVTime:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:IQVTime:EVENTs? (Query Only)

Returns the current events for the RF I&Q versus Time measurement.

Syntax :STATus:IQVTime:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views RF I&Q versus Time

Examples STATus:IQVTime:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:MCPower:EVENTs? (Query Only)

Returns the current events for the MCPR (multi-carrier ACPR) measurement.

Syntax :STATus:MCPower:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views MCPR

Examples STATus:MCPower:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:MERRor:EVENTs? (Query Only)

Returns the current events for the Magnitude error versus Time measurement.

Syntax :STATus:MERRor:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Magnitude error versus Time

Examples STATus:MERRor:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:OBWidth:EVENTs? (Query Only)

Returns the current events for the Occupied Bandwidth (OBW) measurement.

Syntax :STATus:OBWidth:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Occupied Bandwidth

Examples STATus:OBW:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:OPERation:CONDition? (Query Only)

Returns the contents of the Operation Condition Register (OCR).

Syntax :STATus:OPERation:CONDition?

Arguments None

Returns <NR1> is a decimal number showing the contents of the OCR.

Measurement Views All

Examples :STATus:OPERation:CONDition?
might return 16, showing that the bits in the OCR have the binary value 0000000000010000, which means the analyzer is in measurement.

:STATus:OPERation:ENABle(?)

Sets or queries the enable mask of the Operation Enable Register (OENR) which allows true conditions in the Operation Event Register to be reported in the summary bit.

Syntax :STATus:OPERation:ENABle <bit_value>
:STATus:OPERation:ENABle?

Arguments <bit_value>::=<NR1> is the enable mask of the OENR. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the OENR.
Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:OPERation:ENABle 1
enables the ALIGning bit.

:STATus:OPERation:ENABle?
might return 1, showing that the bits in the OENR have the binary value 00000000 00000001, which means that the ALIGning bit is valid.

:STATus:OPERation[:EVENT]? (Query Only)

Returns the contents of the Operation Event Register (OEVR).
Reading the OEVR clears it.

Syntax :STATus:OPERation[:EVENT]?

Arguments None

Returns <NR1> is a decimal number showing the contents of the OEVR.

Measurement Views All

Examples STATus:OPERation:EVENT?
might return 1, showing that the bits in the OEVR have the binary value
00000000 00000001, which means that the ALIGNing bit is set.

:STATus:OPERation:NTRansition(?)

Sets or queries the negative transition filter value of the Operation Transition Register (OTR).

Syntax :STATus:OPERation:NTRansition <bit_value>
:STATus:OPERation:NTRansition?

Arguments <bit_value>::=<NR1> is the negative transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the OTR.
Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:OPERation:NTRansition #H0011
sets the negative transition filter value to #H0011.

:STATus:OPERation:NTRansition?
might return 17.

:STATus:OPERation:PTRansition(?)

Sets or queries the positive transition filter value of the Operation Transition Register (OTR).

Syntax :STATus:OPERation:PTRansition <bit_value>
 :STATus:OPERation:PTRansition?

Arguments <bit_value>::=<NR1> is the positive transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the OTR.
 Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:OPERation:PTRansition 0
 sets the positive transition filter value to 0.
 :STATus:OPERation:PTRansition?
 might return 0.

:STATus:PERRor:EVENTs? (Query Only)

Returns the current events for the Phase error versus Time measurement.

Syntax :STATus:PERRor:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Phase error versus Time

Examples STATus:PERRor:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:PHVTime:EVENTs? (Query Only)

Returns the current events for the Phase versus Time measurement.

Syntax :STATus:PHVTime:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>"] "{,<ecode>,"<edesc>[:<einfo>"]}"

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Phase versus Time

Examples STATus:PHVTime:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:PRESet (No Query Form)

Presets the SCPI enable registers and transition registers.

Syntax :STATus:PRESet

Arguments None

Measurement Views All

Examples :STATus:PRESet
presets the SCPI enable registers and transition registers.

:STATus:PULSe:RESult:EVENTs? (Query Only)

Returns the current events for the pulse table measurement.

Syntax :STATus:PULSe:RESult:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Pulse table

Examples STATus:PULSe:RESult:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:PULSe:STATistics:EVENTs? (Query Only)

Returns the current events for the pulse statistics measurement.

Syntax :STATus:PULSe:STATistics:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Pulse statistics

Examples STATus:PULSe:STATistics:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:PULSe:TRACe:EVENTs? (Query Only)

Returns the current events for the pulse trace measurement.

Syntax :STATus:PULSe:TRACe:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Pulse trace

Examples STATus:PULSe:TRACe:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:QUESTionable:CONDition? (Query Only)

Returns the contents of the Questionable Condition Register (QCR).

Syntax :STATus:QUESTionable:CONDition?

Arguments None

Returns <NR1> is a decimal number showing the contents of the QCR.

Measurement Views All

Examples :STATus:QUESTionable:CONDition?
might return 256, showing that the bits in the QCR have the binary value 00000001 00000000, which means the Calibration Summary bit is set.

:STATus:QUESTionable:ENABle(?)

Sets or queries the enable mask of the Questionable Enable Register (QENR) which allows true conditions in the Questionable Event Register to be reported in the summary bit.

Syntax :STATus:QUESTionable:ENABle <bit_value>
:STATus:QUESTionable:ENABle?

Arguments <bit_value>::=<NR1> is the enable mask of QENR. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the QENR.
Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUESTionable:ENABle 256
enables the Calibration Summary bit.

:STATus:QUESTionable:ENABle?
might return 256, showing that the bits in the QENR have the binary value 00000001 00000000, which means that the Calibration Summary bit is valid.

:STATus:QUESTionable[:EVENT]? (Query Only)

Returns the contents of the Questionable Event Register (QEVr).
Reading the QEVr clears it.

Syntax :STATus:QUESTionable[:EVENT]?

Arguments None

Returns <NR1> is a decimal number showing the contents of the QEVr.

Measurement Views All

Examples STATus:QUESTionable:EVENT?
might return 256, showing that the bits in the QEVr have the binary value 00000001 00000000, which means that the Calibration Summary bit is set.

:STATus:QUESTionable:NTRansition(?)

Sets or queries the negative transition filter value of the Questionable Transition Register (QTR).

Syntax :STATus:QUESTionable:NTRansition <bit_value>
:STATus:QUESTionable:NTRansition?

Arguments <bit_value>::=<NR1> is the negative transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the QTR.
Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUESTionable:NTRansition #H0020
sets the negative transition filter value to #H0020.

:STATus:QUESTionable:NTRansition?
might return 32.

:STATus:QUEStionable:PTRansition(?)

Sets or queries the positive transition filter value of the Questionable Transition Register (QTR).

Syntax :STATus:QUEStionable:PTRansition <bit_value>
 :STATus:QUEStionable:PTRansition?

Arguments <bit_value>::=<NR1> is the positive transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the QTR.
 Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUEStionable:PTRansition 0
 sets the positive transition filter value to 0.
 :STATus:QUEStionable:PTRansition?
 might return 0.

:STATus:QUEStionable:CALibration:CONDition? (Query Only)

Returns the contents of the questionable calibration condition register.

Syntax :STATus:QUEStionable:CALibration:CONDition?

Arguments None

Returns <NR1> is a decimal number showing the contents of the questionable calibration condition register.

Measurement Views All

Examples :STATus:QUEStionable:CALibration:CONDition?
 might return 16384, showing that the bits in the questionable calibration condition register have the binary value 01000000 00000000, which means the Alignment Needed bit is set.

:STATus:QUESTionable:CALibration:ENABLE(?)

Sets or queries the enable mask of the questionable calibration enable register which allows true conditions in the questionable calibration event register to be reported in the summary bit.

Syntax :STATus:QUESTionable:CALibration:ENABLE <bit_value>
 :STATus:QUESTionable:CALibration:ENABLE?

Arguments <bit_value>::=<NR1> is the enable mask of the questionable calibration enable register. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the questionable calibration enable register. Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUESTionable:CALibration:ENABLE 16384
 enables the Alignment Needed bit.

 :STATus:QUESTionable:CALibration:ENABLE?
 might return 16384, showing that the bits in the questionable calibration enable register have the binary value 01000000 00000000, which means that the Calibration Summary bit is valid.

:STATus:QUESTionable:CALibration[:EVENT]? (Query Only)

Returns the contents of the questionable calibration event register.
Reading the register clears it.

Syntax :STATus:QUESTionable:CALibration[:EVENT]?

Arguments None

Returns <NR1> is a decimal number showing the contents of the questionable calibration event register.

Measurement Views All

Examples STATus:QUESTionable:CALibration:EVENT?
might return 16384, showing that the bits in the questionable calibration event register have the binary value 01000000 00000000, which means that the Calibration Summary bit is set.

:STATus:QUEStionable:CALibration:NTRansition(?)

Sets or queries the negative transition filter value of the questionable calibration transition register.

Syntax :STATus:QUEStionable:CALibration:NTRansition <bit_value>
 :STATus:QUEStionable:CALibration:NTRansition?

Arguments <bit_value>::=<NR1> is the negative transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the questionable calibration transition register.
 Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUEStionable:CALibration:NTRansition #H4000
 sets the negative transition filter value to #H4000.
 :STATus:QUEStionable:CALibration:NTRansition?
 might return 16384.

:STATus:QUESTionable:CALibration:PTRansition(?)

Sets or queries the positive transition filter value of the questionable calibration transition register.

Syntax :STATus:QUESTionable:CALibration:PTRansition <bit_value>
:STATus:QUESTionable:CALibration:PTRansition?

Arguments <bit_value>::=<NR1> is the positive transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the questionable calibration transition register.
Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUESTionable:CALibration:PTRansition 0
sets the positive transition filter value to 0.

:STATus:QUESTionable:CALibration:PTRansition?
might return 0.

:STATus:QUESTionable:FREQuency:CONDition? (Query Only)

Returns the contents of the questionable frequency condition register.

Syntax :STATus:QUESTionable:FREQuency:CONDition?

Arguments None

Returns <NR1> is a decimal number showing the contents of the questionable frequency condition register.

Measurement Views All

Examples :STATus:QUESTionable:FREQuency:CONDition?
might return 512, showing that the bits in the questionable frequency condition register have the binary value 00000010 00000000, which means the Locked To External Ref bit is set.

:STATus:QUESTionable:FREQuency:ENABle(?)

Sets or queries the enable mask of the questionable frequency enable register which allows true conditions in the questionable frequency event register to be reported in the summary bit.

Syntax :STATus:QUESTionable:FREQuency:ENABle <bit_value>
:STATus:QUESTionable:FREQuency:ENABle?

Arguments <bit_value>::=<NR1> is the enable mask of the questionable frequency enable register. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the questionable frequency enable register. Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUESTionable:FREQuency:ENABle 512
enables the Locked To External Ref bit.

:STATus:QUESTionable:FREQuency:ENABle?
might return 512, showing that the bits in the questionable calibration enable register have the binary value 00000010 00000000, which means that the Locked To External Ref bit is valid.

:STATus:QUESTionable:FREQuency[:EVENT]? (Query Only)

Returns the contents of the questionable frequency event register.
Reading the register clears it.

Syntax :STATus:QUESTionable:FREQuency[:EVENT]?

Arguments None

Returns <NR1> is a decimal number showing the contents of the questionable frequency event register.

Measurement Views All

Examples STATus:QUESTionable:FREQuency:EVENT?
might return 512, showing that the bits in the questionable frequency event register have the binary value 00000010 00000000, which means that the Locked To External Ref bit is set.

:STATus:QUEStionable:FREQuency:NTRansition(?)

Sets or queries the negative transition filter value of the questionable frequency transition register.

Syntax :STATus:QUEStionable:FREQuency:NTRansition <bit_value>
 :STATus:QUEStionable:FREQuency:NTRansition?

Arguments <bit_value>::=<NR1> is the negative transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the questionable frequency transition register.
 Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUEStionable:FREQuency:NTRansition #H0200
 sets the negative transition filter value to #H0200.
 :STATus:QUEStionable:FREQuency:NTRansition?
 might return 512.

:STATus:QUESTionable:FREQuency:PTRansition(?)

Sets or queries the positive transition filter value of the questionable frequency transition register.

Syntax :STATus:QUESTionable:FREQuency:PTRansition <bit_value>
 :STATus:QUESTionable:FREQuency:PTRansition?

Arguments <bit_value>::=<NR1> is the positive transition filter value. Range: 0 to 65535.

Returns <NR1> is a decimal number showing the contents of the questionable frequency transition register.
 Range: 0 to 32767 (The most-significant bit cannot be set true.)

Measurement Views All

Examples :STATus:QUESTionable:FREQuency:PTRansition 0
 sets the positive transition filter value to 0.
 :STATus:QUESTionable:FREQuency:PTRansition?
 might return 0.

:STATus:SGRam:EVENTs? (Query Only)

Returns the current events for the spectrogram measurement.

Syntax :STATus:SGRam:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Spectrogram

Examples STATus:SGRam:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that
the sampling parameters are controlled manually.

:STATus:SPECTrum:EVENTs? (Query Only)

Returns the current events for the spectrum measurement.

Syntax :STATus:SPECTrum:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Spectrum

Examples STATus:SPECTrum:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

:STATus:SQUALity:EVENTs? (Query Only)

Returns the current events for the signal quality measurement.

Syntax :STATus:SQUALity:EVENTs?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"{"<ecode>,"<edesc>[:<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

If there is no error, the response is 0,"No error".

Measurement Views Signal quality

Examples STATus:SQUALity:EVENTs?
might return 2026,"Acq Sampling Params: manual control", indicating that the sampling parameters are controlled manually.

SYSTem Commands

The SYSTem commands control system-related conditions.

Command Tree

Header	Parameter
:SYSTem	
:COMMunicate	
:GPIB	
[:SELF]	
:ADDRes	<numeric_value>
:DATE	<year>,<month>,<day>
:ERRor	
:ALL?	
:CODE	
:ALL?	
[:NEXT]?	
:COUNT?	
[:NEXT]?	
:OPTions?	
:PRESet	
:TIME	<hour>,<minute>,<second>
:VERSion?	

:SYSTem:COMMunicate:GPIB[:SELF]:ADDRess(?)

Sets or queries the GPIB address of the instrument.

Syntax :SYSTem:COMMunicate:GPIB[:SELF]:ADDRess <value>
 :SYSTem:COMMunicate:GPIB[:SELF]:ADDRess?

Arguments <value>::=<NR1> specifies the GPIB address of the instrument.
 *RST has no effect on the value.

Measurement Views All

Examples :SYSTem:COMMunicate:GPIB:SELF:ADDRess 18
 sets the GPIB address to 18.

:SYSTem:DATE(?)

Sets or queries the date (year, month, and day). This command is equivalent to the date setting through the Windows Control Panel.

Syntax :SYSTem:DATE <year>,<month>,<day>
 :SYSTem:DATE?

Arguments <year>::=<NRf> specifies the year (4 digits). Range: 2000 to 2099
 <month>::=<NRf> specifies the month. Range: 1 (January) to 12 (December)
 <day>::=<NRf> specifies the day. Range: 1 to 31
 These values are rounded to the nearest integer.
 *RST has no effect on the settings.

Measurement Views All

Examples :SYSTem:DATE 2002,3,19
 sets the internal calendar to March 19, 2002.

Related Commands :SYSTem:TIME

:SYSTem:ERRor:ALL? (Query Only)

Queries the error/event queue for all the unread items and removes them from the queue. The response is a comma separated list of number, string pairs in FIFO order. For details of the error messages, refer to page 3-15.

Syntax :SYSTem:ERRor:ALL?

Arguments None

Returns <ecode>,"<edesc>[;<einfo>]"{"<ecode>,"<edesc>[;<einfo>]"}

Where

<ecode>::=<NR1> is the error/event code (-32768 to 32767).

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the detail of the error/event.

If the queue is empty, the response is 0, "No error; Queue empty - No events to report".

Measurement Views All

Examples :SYSTem:ERRor:ALL?
might return
-130, "Suffix error; Unrecognized suffix, INPut:MLEVel -10dB",
indicating that the unit of the reference level is improper.

:SYSTem:ERRor:CODE:ALL? (Query Only)

Queries the error/event queue for all the unread items and removes them from the queue. The response returns a comma separated list of only the error/event code numbers in FIFO order. For details of the error messages, refer to page 3-15.

Syntax :SYSTem:ERRor:CODE:ALL?

Arguments None

Returns <ecode>{,<ecode>}

Where

<ecode>: :=<NR1> is the error/event code, ranging from -32768 to 32767.

If the queue is empty, the response is 0.

Measurement Views All

Examples :SYSTem:ERRor:CODE:ALL?
might return -101,-108 of the error codes.

:SYSTem:ERRor:CODE[:NEXT]? (Query Only)

Queries the error/event queue for the next item and removes it from the queue. The response returns only the error/event code number omitting the string. Except for the shortened response, the query operates identically to :SYSTem:ERRor[:NEXT]? For details of the error messages, refer to page 3-15.

Syntax :SYSTem:ERRor:CODE[:NEXT]?

Arguments None

Returns <ecode>::=<NR1> is the error/event code, ranging from -32768 to 32767.

Measurement Views All

Examples :SYSTem:ERRor:CODE:NEXT?
might return -101 of the error code.

Related Commands :SYSTem:ERRor[:NEXT]?

:SYSTem:ERRor:COUNt? (Query Only)

Queries the error/event queue for the number of unread items. As errors and events may occur at any time, more items may be present in the queue at the time it is actually read.

Syntax :SYSTem:ERRor:COUNt?

Arguments None

Returns <enum>::=<NR1> is the number of errors/events.
If the queue is empty, the response is 0.

Measurement Views All

Examples :SYSTem:ERRor:COUNt?
might return 2, indicating that the error/event queue contains two of unread errors/events.

:SYSTem:ERRor[:NEXT]? (Query Only)

Queries the error/event queue for the next item and removes it from the queue. The response returns the full queue item consisting of an integer and a string. For details of the error messages, refer to page 3-15.

Syntax :SYSTem:ERRor[:NEXT]?

Arguments None

Returns <ecode>,"<edesc>[:<einfo>]"

Where

<ecode>::=<NR1> is the error/event code, ranging from -32768 to 32767.

<edesc>::=<string> is the description on the error/event.

<einfo>::=<string> is the additional information on the error/event.

Measurement Views All

Examples :SYSTem:ERRor:NEXT?
might return
-130, "Suffix error; Unrecognized suffix, INPut:MLEVel -10dB",
indicating that the unit is improper.

:SYSTem:OPTions? (Query Only)

Queries the options installed in the analyzer.

This command is equivalent to the IEEE common command *OPT?.

Syntax :SYSTem:OPTions?

Arguments None

Returns <option>::=<string> contains the comma-separated option numbers.

Measurement Modes All

Examples :SYSTem:OPTions?
might return "01,02,20", indicating that Option 01, 02, and 20 are currently installed in the analyzer.

Related Commands *OPT?, :INSTrument[:SElect]

:SYSTem:PRESet (No Query Form)

Restores the analyzer to the defaults.

This command is equivalent to the PRESET key on the front panel.

Syntax :SYSTem:PRESet

Arguments None

Measurement Modes All

Examples :SYSTem:PRESet
restores the analyzer to the defaults.

:SYSTem:TIME(?)

Sets or queries the time (hours, minutes, and seconds). This command is equivalent to the time setting through the Windows Control Panel.

Syntax :SYSTem:TIME <hour>,<minute>,<second>
 :SYSTem:TIME?

Arguments <hour>::= <NRf> specifies the hours. Range: 0 to 23.
 <minute>::=<NRf> specifies the minutes. Range: 0 to 59.
 <second>::=<NRf> specifies the seconds. Range: 0 to 59.

 These values are rounded to the nearest integer.
 *RST has no effect on the settings.

Measurement Modes All

Examples :SYSTem:TIME 10,15,30
 sets the time to 10:15:30.

Related Commands :SYSTem:DATE

:SYSTem:VERSion? (Query Only)

Returns the SCPI version number for which the analyzer complies.

Syntax :SYSTem:VERSion?

Arguments None

Returns <NR2> has the form YYYY.V where the Ys represent the year-version (for example, 1999) and the V represents an approved revision number for that year.

Measurement Modes All

Examples :SYSTem:VERSion?
 might return 1999.0 for the SCPI version.

TRACe Commands

The TRACe commands select trace type and control trace arithmetic. These commands are divided by measurement views into the subgroups listed in Table 2-48.

Table 2-48: TRACe command subgroups

Command header	Measurement view	Refer to:
:TRACe<x>:AVTime	Amplitude versus Time	page 2-772
:TRACe<x>:CCDF	CCDF	page 2-782
:TRACe<x>:CONSte	Constellation	page 2-787
:TRACe<x>:DPsA	DPX (Digital Phosphor) spectrum	page 2-788
:TRACe:FVTime	Frequency versus Time	page 2-798
:TRACe:IQVTime	RF I&Q versus Time	page 2-802
:TRACe:OBWidth	Occupied Bandwidth (OBW)	page 2-809
:TRACe:PHVTime	Phase versus Time	page 2-810
:TRACe:SGRam	Spectrogram	page 2-814
:TRACe<x>:SPECtrum	Spectrum	page 2-817

:TRACe<x>:AVTime Subgroup

The :TRACe:AVTime commands control traces in the Amplitude versus Time measurement.

Command Tree	Header	Parameter
	:TRACe<x>	
	:AVTime	<boolean>
	:AVERage	
	:COUNT	<numeric_value>
	:RESet	
	:COUNT	<numeric_value>
	:ENABle	<boolean>
	:RESet	
	:FREeze	<boolean>
	:FUNCTion	NORMa1 AVERage MAXHold MINHold
	:LEFToperand	TRACE1 TRACE2 TRACE3
	:RIGHToperand	TRACE1 TRACE2 TRACE3
	:SElect	

Where <x> = 1 to 4. Each trace is defined as follows:

- TRACe1: Trace 1
- TRACe2: Trace 2
- TRACe3: Trace 3
- TRACe4: Math trace

NOTE. Valid traces depend on commands. Refer to each command syntax.

:TRACe<x>:AVTime(?)

Determines whether or not to show the specified trace in the Amplitude versus Time view.

Syntax :TRACe<x>:AVTime { OFF | ON | 0 | 1 }
:TRACe<x>:AVTime?

Where <x> = 1 to 4; All traces are valid.

Arguments OFF or 0 hides the specified trace in the Amplitude versus Time view.
ON or 1 shows the specified trace in the Amplitude versus Time view.

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime ON
shows Trace 1 in the Amplitude versus Time view.

:TRACe<x>:AVTime:AVERage:COUNT(?)

Sets or queries the number of traces to combine. This command is effective when you select AVERage with the :TRACe<x>:AVTime:FUNCTION command.

Syntax :TRACe<x>:AVTime:AVERage:COUNT <number>
:TRACe<x>:AVTime:AVERage:COUNT?

Where <x> = 1 to 3; Trace 4 (math trace) is invalid.

Arguments <number>::=<NR1> specifies the number of traces to combine for averaging.
Range: 1 to 10000.

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime:AVERage:COUNT 64
sets the average count to 64 for Trace 1.

Related Commands :TRACe<x>:AVTime:FUNCTION

:TRACe<x>:AVTime:AVERage:RESet (No Query Form)

Restarts acquisition and display of waveforms for the specified trace. For an Average, Max Hold, or Min Hold trace, it restarts the sequence, discarding accumulated data and resetting the counter.

Syntax :TRACe<x>:AVTime:AVERage:RESet

Where <x> = 1 to 3; Trace 4 (math trace) is invalid.

Arguments None

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime:AVERage:RESet
restarts acquisition and display of waveforms for Trace 1.

Related Commands :TRACe<x>:AVTime:FUNctIon

:TRACe<x>:AVTime:COUNT(?)

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the Amplitude versus Time measurement. This command is effective when :TRACe<x>:AVTime:FUNCTION is set to MAXHold or MINHold and :INITiate:CONTInuous is set to OFF.

Syntax :TRACe<x>:AVTime:COUNT <number>

:TRACe<x>:AVTime:COUNT?

Where <x> = 1 to 3; Trace 4 (math trace) is invalid.

Arguments <number>::=<NR1> specifies the count for Max/Min Hold.
Range: 1 to 10000.

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime:COUNT 32
sets the count to 32 for Trace 1.

Related Commands :INITiate:CONTInuous, :TRACe<x>:AVTime:FUNCTION

:TRACe<x>:AVTime:COUNT:ENABLE(?)

Determines whether to enable or disable the count for the Max or Min Hold trace in the Amplitude versus Time view. This command is effective when :TRACe<x>:AVTime:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe<x>:AVTime:COUNT:ENABLE { OFF | ON | 0 | 1 }
:TRACe<x>:AVTime:COUNT:ENABLE?

Where <x> = 1 to 3; Trace 4 (math trace) is invalid.

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
ON or 1 enables the count for the Max/Min Hold trace.

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime:COUNT:ENABLE ON
enables the Max/Min Hold count for Trace 1.

Related Commands :TRACe<x>:AVTime:FUNCTION

:TRACe<x>:AVTime:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process for the specified trace in the Amplitude versus Time view. This command is effective when :TRACe<x>:AVTime:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe<x>:AVTime:COUNT:RESet

Where <x> = 1 to 3; Trace 4 (math trace) is invalid.

Arguments None

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime:COUNT:RESet
clears the Max/Min Hold data and counter, and restarts the process for Trace 1.

Related Commands :TRACe<x>:AVTime:FUNCTION

:TRACe<x>:AVTime:FREEze(?)

Determines whether or not to freeze the display of the specified trace in the Amplitude versus Time view.

Syntax :TRACe<x>:AVTime:FREEze { OFF | ON | 0 | 1 }
:TRACe<x>:AVTime:FREEze?

Where <x> = 1 to 4; All traces are valid.

Arguments OFF or 0 updates the display of the specified trace normally.
ON or 1 stops updating the display of the specified trace.

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime:FREEze ON
freezes the display for Trace 1.

:TRACe<x>:AVTime:FUNction(?)

Selects or queries the function for the specified trace in the Amplitude versus Time view.

Syntax :TRACe<x>:AVTime:FUNction
 { NORMa1 | AVERage | MAXHold | MINHold }

 :TRACe<x>:AVTime:FUNction?

Where <x> = 1 to 3; Trace 4 (math trace) is invalid.

Arguments NORMa1 selects the normal display.

AVERage selects the Average display that indicates the average amplitude at each time point.

MAXHold selects the Max Hold display that indicates the maximum amplitude at each time point.

MINHold selects the Min Hold display that indicates the minimum amplitude at each time point.

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime:FUNction MAXHold
 selects Max Hold for Trace 1 in the Amplitude versus Time view.

:TRACe<x>:AVTime:LEFToperand(?)

Selects or queries the left operand for the math trace (Trace 4) in the Amplitude versus Time view.

Syntax :TRACe<x>:AVTime:LEFToperand { TRACE1 | TRACE2 | TRACE3 }
 :TRACe<x>:AVTime:LEFToperand?

Where <x> = 4; Only Trace 4 (math trace) is valid.

Arguments TRACE1 selects Trace 1 as the left operand for the math trace.
 TRACE2 selects Trace 2 as the left operand for the math trace.
 TRACE3 selects Trace 3 as the left operand for the math trace.

Measurement Views Amplitude versus Time

Examples :TRACe4:AVTime:LEFToperand TRACE2
 selects Trace 2 as the left operand for the math trace.

Related Commands :TRACe<x>:AVTime:RIGHToperand

:TRACe<x>:AVTime:RIGHtooperand(?)

Selects or queries the right operand for the math trace (Trace 4) in the Amplitude versus Time view.

Syntax :TRACe<x>:AVTime:RIGHtooperand { TRACE1 | TRACE2 | TRACE3 }
 :TRACe<x>:AVTime:RIGHtooperand?

Where <x> = 4; Only Trace 4 (math trace) is valid.

Arguments TRACE1 selects Trace 1 as the right operand for the math trace.
 TRACE2 selects Trace 2 as the right operand for the math trace.
 TRACE3 selects Trace 3 as the right operand for the math trace.

Measurement Views Amplitude versus Time

Examples :TRACe4:AVTime:RIGHtooperand TRACE1
 selects Trace 1 as the right operand for the math trace.

Related Commands :TRACe<x>:AVTime:LEFTooperand

:TRACe<x>:AVTime:SElect(?)

Selects or queries the trace whose measurement results are being displayed in the readout on the top and bottom of the view.

Syntax :TRACe<x>:AVTime:SElect
 :TRACe<x>:AVTime:SElect?

Where <x> = 1 to 4; All traces are valid.

Arguments None

Returns { 0 | 1 }

0 indicates that the results are not being displayed in the readout for the trace.

1 indicates that the results are being displayed in the readout for the trace.

Measurement Views Amplitude versus Time

Examples :TRACe1:AVTime:SElect
 selects Trace 1 to display the measurement results in the readout.

 :TRACe1:AVTime:SElect?
 might return 1, indicating that the results are being displayed in the readout for Trace 1.

:TRACe<x>:CCDF Subgroup

The :TRACe:CCDF commands control traces in the CCDF measurement.

Command Tree	Header	Parameter
	:TRACe<x>	
	:CCDF	
	:FREeze	<boolean>
	:SElect	
	:SHOW	<boolean>
	:X	<numeric_value>
	:Y?	

Where <x> = 1 to 3. Each trace is defined as follows:

TRACe1: Trace 1
TRACe2: Trace 2
TRACe3: Gaussian reference curve

NOTE. Valid traces depend on commands. Refer to each command syntax.

:TRACe<x>:CCDF:FREeze(?)

Determines whether or not to freeze the display of the specified trace (Trace 1 or 2) in the CCDF view.

Syntax :TRACe<x>:CCDF:FREeze { OFF | ON | 0 | 1 }
:TRACe<x>:CCDF:FREeze?

Where <x> = 1 or 2; Trace 3 (Gaussian curve) is invalid.

Arguments OFF or 0 updates the display of the specified trace normally.
ON or 1 stops updating the display of the specified trace.

Measurement Views CCDF

Examples :TRACe1:CCDF:FREeze ON
freezes the display for Trace 1.

:TRACe<x>:CCDF:SElect(?)

Selects or queries the trace whose measurement results are being displayed in the readout on the top of the view. The selected trace is indicated by the measurement pointer (pink triangle) on the waveform.

Syntax :TRACe<x>:CCDF:SElect
:TRACe<x>:CCDF:SElect?

Where <x> = 1 to 3; All traces are valid.

Arguments None

Returns { 0 | 1 }

0 indicates that the results are not being displayed in the readout for the trace.

1 indicates that the results are being displayed in the readout for the trace.

Measurement Views CCDF

Examples :TRACe1:CCDF:SElect
selects Trace 1 to display the measurement results in the readout.

:TRACe1:CCDF:SElect?
might return 1, indicating that the results are being displayed in the readout for Trace 1.

:TRACe<x>:CCDF:SHOW(?)

Determines whether to show or hide the specified trace in the CCDF view.

Syntax :TRACe<x>:CCDF:SHOW { OFF | ON | 0 | 1 }
 :TRACe<x>:CCDF:SHOW?

Where <x> = 1 to 3; All traces are valid.

Arguments OFF or 0 hides the specified trace.
 ON or 1 shows the specified trace.

Measurement Views CCDF

Examples :TRACe1:CCDF:SHOW ON
 shows Trace 1 in the CCDF view.

:TRACe<x>:CCDF:X(?)

Sets or queries the horizontal position of the measurement pointer (pink triangle) to measure the CCDF. Use the :TRACe<x>:CCDF:Y? query to read the value.

NOTE. Use the :TRACe<x>:CCDF:SHOW command to show the specified trace and the :TRACe<x>:CCDF:SElect command to select the trace before running the :TRACe<x>:CCDF:X command.

Syntax :TRACe<x>:CCDF:X <value>

:TRACe<x>:CCDF:X?

Where <x> = 1 to 3; All traces are valid.

Arguments <value>::=<NRf> specifies the horizontal position of the measurement pointer. Range: 0 to 20 dB.

Measurement Views CCDF

Examples :TRACe1:CCDF:X 5
puts the measurement pointer at 5 dB on Trace 1.

Related Commands :TRACe<x>:CCDF:SElect, :TRACe<x>:CCDF:SHOW,
:TRACe<x>:CCDF:Y?

:TRACe<x>:CCDF:Y? (Query Only)

Queries the vertical position (CCDF value) of the measurement pointer (displayed as a pink triangle). Use the :TRACe<x>:CCDF:X command to set the horizontal position of the pointer.

NOTE. Use the :TRACe<x>:CCDF:SHOW command to show the specified trace and the :TRACe<x>:CCDF:SElect command to select the trace before running the :TRACe<x>:CCDF:Y? query.

Syntax :TRACe<x>:CCDF:Y?

Where <x> = 1 to 3; All traces are valid.

Arguments None

Returns <value>::=<NRf> is the vertical position (CCDF) of the measurement pointer. Range: 0 to 100%.

The value of 99.0999953003E+36 is returned if the trace is not available.

Measurement Views CCDF

Examples :TRACe1:CCDF:Y?
might return 14.72, indicating the CCDF is 14.72% at the measurement pointer on Trace 1.

Related Commands :TRACe<x>:CCDF:SElect, :TRACe<x>:CCDF:SHOW, :TRACe<x>:CCDF:X

:TRACe<x>:CONSte Subgroup

The :TRACe<x>:CONSte commands control traces in the Constellation measurement.

Command Tree	Header	Parameter
	:TRACe<x>	
	:CONSte	
	:MODE	VECTors SYMBols

Where <x> = 0 or 1. TRACe0 or TRACe1 represents the constellation trace.

:TRACe<x>:CONSte:MODE(?)

Selects or queries how to display the constellation trace.

Syntax :TRACe<x>:CONSte:MODE { VECTors | SYMBols }
:TRACe<x>:CONSte:MODE?

Arguments VECTors connects adjacent symbol points with the signal locus.
SYMBols displays individual symbol points.

Measurement Views Constellation

Examples :TRACe1:CONSte:MODE VECTors
shows the constellation connecting adjacent symbol points with the signal locus.

:TRACe<x>:DPSA Subgroup

The :TRACe<x>:DPSA commands control traces in the DPX (Digital Phosphor) Spectrum measurement.

Command Tree	Header	Parameter
	:TRACe<x>	
	:DPSA	<boolean>
	:AVERage	
	:COUNT	<numeric_value>
	:COLor	
	:INTensity	<numeric_value>
	:DOT	
	:PERSistent	<boolean>
	:TYPE	VARIable INFinite
	:VARIable	<numeric_value>
	:FREeze	<boolean>
	:FUNCTion	NORMal HOLD AVERage
	:LEFToperand	TRACE1 TRACE2 TRACE3
	:RIGHToperand	TRACE1 TRACE2 TRACE3
	:SElect	

Where <x> = 1 to 5. Each trace is defined as follows:

- TRACe1: +Peak trace
- TRACe2: -Peak trace
- TRACe3: Average trace
- TRACe4: Math trace
- TRACe5: Bitmap trace

NOTE. Valid traces depend on commands. Refer to each command syntax.

:TRACe<x>:DPSA(?)

Determines whether or not to show the specified trace in the DPX spectrum view.

Syntax :TRACe<x>:DPSA { OFF | ON | 0 | 1 }

:TRACe<x>:DPSA?

Where <x> = 1 to 5; All traces are valid.

Arguments OFF or 0 hides the specified trace in the DPX spectrum view.

ON or 1 shows the specified trace in the DPX spectrum view.

Measurement Views DPX spectrum

Examples :TRACe1:DPSA ON
shows Trace 1 (the maximum trace) in the DPX spectrum view.

:TRACe<x>:DPSA:AVERAge:COUNT(?)

Sets or queries the number of traces to combine for averaging in the DPX spectrum view.

Syntax :TRACe<x>:DPSA:AVERAge:COUNT <number>

:TRACe<x>:DPSA:AVERAge:COUNT?

Where <x> = 3; Only Trace 3 (average trace) is valid.

Arguments <number>::=<NR1> specifies the number of traces to combine for averaging.
Range: 1 to 10000.

Measurement Views DPX spectrum

Examples :TRACe3:DPSA:AVERAge:COUNT 32
sets the average count to 32.

:TRACe<x>:DPSA:COLor:INTensity(?)

Sets or queries the color intensity in the DPX spectrum view.
The value is common to all traces.

Syntax :TRACe<x>:DPSA:COLor:INTensity <value>

:TRACe<x>:DPSA:COLor:INTensity?

Where <x> = 1 to 5; All traces are valid.

Arguments <value>::=<NRf> specifies color intensity. Range: 1 to 100%.

Measurement Views DPX spectrum

Examples :TRACe1:DPSA:COLor:INTensity 30
sets the color intensity to 30%.

:TRACe<x>:DPSA:DOT:PERSistent(?)

Determines whether to enable or disable the dot persistence for the bitmap trace (Trace 5) in the DPX spectrum view.

Syntax :TRACe<x>:DPSA:DOT:PERSistent { OFF | ON | 0 | 1 }

:TRACe<x>:DPSA:DOT:PERSistent?

Where <x> = 5; Only Trace 5 (bitmap trace) is valid.

Arguments OFF or 0 disables the dot persistence.

ON or 1 enables the dot persistence.

Measurement Views DPX spectrum

Examples :TRACe5:DPSA:DOT:PERSistent ON
enables the dot persistence in the DPX spectrum view.

:TRACe<x>:DPSA:DOT:PERsistent:TYPE(?)

Selects or queries the persistence type for the bitmap trace (Trace 5) in the DPX spectrum view.

Syntax :TRACe<x>:DPSA:DOT:PERsistent:TYPE { VARIable | INFinite }

:TRACe<x>:DPSA:DOT:PERsistent:TYPE?

Where <x> = 5; Only Trace 5 (bitmap trace) is valid.

Arguments VARIable selects the variable persistence display which leaves acquired data points on the display for a period of time specified by the :TRACe<x>:DPSA:DOT:PERsistent:VARIable command.

INFinite selects the infinite persistence display which accumulates data points on the display indefinitely.

Measurement Views DPX spectrum

Examples :TRACe5:DPSA:DOT:PERsistent:TYPE VARIable
selects the variable persistence display.

Related Commands :TRACe<x>:DPSA:DOT:PERsistent:VARIable

:TRACe<x>:DPSA:DOT:PERsistent:VARiable(?)

Sets or queries how long data points are displayed. This command is effective when :TRACe<x>:DPSA:DOT:PERsistent:TYPE is set to VARiable. This affects the display only.

Syntax :TRACe<x>:DPSA:DOT:PERsistent:VARiable <number>

:TRACe<x>:DPSA:DOT:PERsistent:VARiable?

Where <x> = 5; Only Trace 5 (bitmap trace) is valid.

Arguments <number>: :=<NR1> specifies the number that the waveform points are displayed on the screen. Range: 1 to 1000 (unitless; the default value is 10).

Measurement Views DPX spectrum

Examples :TRACe5:DPSA:DOT:PERsistent:VARiable 20
specifies that the waveform points are displayed on the screen for a period of 20 before they disappear.

Related Commands :TRACe<x>:DPSA:DOT:PERsistent:TYPE

:TRACe<x>:DPSA:FREEze(?)

Determines whether or not to freeze the display of the specified trace in the DPX spectrum view.

Syntax :TRACe<x>:DPSA:FREEze { OFF | ON | 0 | 1 }
 :TRACe<x>:DPSA:FREEze?

Where <x> = 1 to 5; All traces are valid.

Arguments OFF or 0 updates the display of the specified trace normally.
 ON or 1 stops updating the display of the specified trace.

Measurement Views DPX spectrum

Examples :TRACe1:DPSA:FREEze ON
 freezes the display for the +peak trace.

:TRACe<x>:DPSA:FUNCTION(?)

Selects or queries the trace function for the +Peak, -Peak, or Average trace (Trace 1, 2, or 3, respectively) in the DPX spectrum view.

Syntax :TRACe<x>:DPSA:FUNCTION { NORMal | HOLD | AVERage }
 :TRACe<x>:DPSA:FUNCTION?

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (bitmap trace) are invalid.

Arguments The table below shows the trace function and display.

Function	Trace1 (+Peak trace)	Trace2 (- Peak trace)	Trace3 (Average trace)
NORMal	Normal spectrum (Detection: +Peak)	Normal spectrum (Detection: -Peak)	Normal spectrum (Detection: Average)
HOLD	Max-hold spectrum	Min-hold spectrum	NA
AVERage	NA	NA	Average spectrum

For the average trace, use the :TRACe<x>:DPSA:AVERage:COUNt command to set the average count.

Measurement Views DPX spectrum

Examples :TRACe1:DPSA:FUNCTION HOLD
 selects the max hold waveform for Trace 1.

Related Commands :TRACe<x>:DPSA:AVERage:COUNt

:TRACe<x>:DPSA:LEFToperand(?)

Selects or queries the left operand for the math trace (Trace 4) in the DPX spectrum view.

Syntax :TRACe<x>:DPSA:LEFToperand { TRACE1 | TRACE2 | TRACE3 }
 :TRACe<x>:DPSA:LEFToperand?

Where <x> = 4; Only Trace 4 (math trace) is valid.

Arguments TRACE1 selects Trace 1 as the left operand for the math trace.
 TRACE2 selects Trace 2 as the left operand for the math trace.
 TRACE3 selects Trace 3 as the left operand for the math trace.

Measurement Views DPX spectrum

Examples :TRACe4:DPSA:LEFToperand TRACE2
 selects Trace 2 as the left operand for the math trace.

Related Commands :TRACe<x>:DPSA:RIGHToperand

:TRACe<x>:DPSA:RIGHtooperand(?)

Selects or queries the right operand for the math trace (Trace 4) in the DPX spectrum view.

Syntax :TRACe<x>:DPSA:RIGHtooperand { TRACE1 | TRACE2 | TRACE3 }
 :TRACe<x>:DPSA:RIGHtooperand?

Where <x> = 4; Only Trace 4 (math trace) is valid.

Arguments TRACE1 selects Trace 1 as the right operand for the math trace.
 TRACE2 selects Trace 2 as the right operand for the math trace.
 TRACE3 selects Trace 3 as the right operand for the math trace.

Measurement Views DPX spectrum

Examples :TRACe4:DPSA:RIGHtooperand TRACE1
 selects Trace 1 as the right operand for the math trace.

Related Commands :TRACe<x>:DPSA:LEFTooperand

:TRACe<x>:DPSA:SElect(?)

Selects or queries the trace to display the readout at the upper left of the DPX spectrum view.

Syntax :TRACe<x>:DPSA:SElect

:TRACe<x>:DPSA:SElect?

Where <x> = 1 to 5; All traces are valid.

Arguments None

Returns { 0 | 1 }

0 indicates that the readout is not being displayed for the specified trace.

1 indicates that the readout is being displayed for the specified trace.

Measurement Views DPX spectrum

Examples :TRACe1:DPSA:SElect
selects Trace 1 (+Peak trace) to display the readout.

:TRACe1:DPSA:SElect?
might return 1, indicating that the readout is being displayed for Trace 1.

:TRACe:FVTime Subgroup

The :TRACe:FVTime commands control traces in the Frequency versus Time measurement.

Command Tree	Header	Parameter
	:TRACe	
	:FVTime	<boolean>
	:AVERage	
	:COUNt	<numeric_value>
	:COUNt	<numeric_value>
	:ENABle	<boolean>
	:RESet	
	:FREeze	<boolean>
	:FUNCTion	NORMal AVERage MAXHold MINHold

:TRACe:FVTime(?)

Determines whether or not to show the trace in the Frequency versus Time view.

Syntax :TRACe:FVTime { OFF | ON | 0 | 1 }
:TRACe:FVTime?

Arguments OFF or 0 hides the trace in the Frequency versus Time view.
ON or 1 shows the trace in the Frequency versus Time view.

Measurement Views Frequency versus Time

Examples :TRACe:FVTime ON
shows the trace in the Frequency versus Time view.

:TRACe:FVTime:AVERage:COUNT(?)

Sets or queries the number of traces to combine. This command is effective when you select AVERage with the :TRACe:FVTime:FUNCTION command.

Syntax :TRACe:FVTime:AVERage:COUNT <number>
:TRACe:FVTime:AVERage:COUNT?

Arguments <number>::=<NR1> specifies the number of traces to combine for averaging.
Range: 1 to 10000.

Measurement Views Frequency versus Time

Examples :TRACe:FVTime:AVERage:COUNT 64
sets the average count to 64.

Related Commands :TRACe:FVTime:FUNCTION

:TRACe:FVTime:COUNT(?)

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the Frequency versus Time measurement. This command is effective when :TRACe<x>:FVTime:FUNCTION is set to MAXHold or MINHold and :INITiate:CONTinuous is set to OFF.

Syntax :TRACe:FVTime:COUNT <number>
:TRACe:FVTime:COUNT?

Arguments <number>::=<NR1> specifies the count for Max/Min Hold.
Range: 1 to 10000.

Measurement Views Frequency versus Time

Examples :TRACe:FVTime:COUNT 32
sets the count to 32 for the Max/Min Hold trace.

Related Commands :INITiate:CONTinuous, :TRACe:FVTime:FUNCTION

:TRACe:FVTime:COUNT:ENABLE(?)

Determines whether to enable or disable the count for the Max or Min Hold trace in the Frequency versus Time view. This command is effective when :TRACe:FVTime:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe:FVTime:COUNT:ENABLE { OFF | ON | 0 | 1 }
:TRACe:FVTime:COUNT:ENABLE?

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
ON or 1 enables the count for the Max/Min Hold trace.

Measurement Views Frequency versus Time

Examples :TRACe:FVTime:COUNT:ENABLE ON
enables the Max/Min Hold count.

Related Commands :TRACe:FVTime:FUNCTION

:TRACe:FVTime:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process in the Frequency versus Time view. This command is effective when :TRACe:FVTime:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe:FVTime:COUNT:RESet

Arguments None

Measurement Views Frequency versus Time

Examples :TRACe:FVTime:COUNT:RESet
clears the Max/Min Hold data and counter, and restarts the process.

Related Commands :TRACe:FVTime:FUNCTION

:TRACe:FVTime:FREeze(?)

Determines whether or not to freeze the display of the trace in the Frequency versus Time measurement.

Syntax :TRACe:FVTime:FREeze { OFF | ON | 0 | 1 }
:TRACe:FVTime:FREeze?

Arguments OFF or 0 updates the display of the trace normally.
ON or 1 stops updating the display of the trace.

Measurement Views Frequency versus Time

Examples :TRACe:FVTime:FREeze ON
stops updating the display of the trace.

:TRACe:FVTime:FUNCTion(?)

Selects or queries the trace function in the Frequency versus Time measurement.

Syntax :TRACe:FVTime:FUNCTion { NORMa1 | AVERage | MAXHold | MINHold }
:TRACe:FVTime:TRACe:FUNCTion?

Arguments NORMa1 selects the normal waveform display.
AVERage selects the Average display that indicates the average frequency drift at each time point.
MAXHold selects the Max Hold display that indicates the maximum frequency drift at each time point.
MINHold selects the Min Hold display that indicates the minimum frequency drift at each time point.

Measurement Views Frequency versus Time

Examples :SENSe:FVTime:FUNCTion MAXHold
displays the Max Hold trace in the Frequency versus Time measurement.

:TRACe:IQVTime Subgroup

The :TRACe:IQVTime commands control traces in the RF I&Q versus Time measurement.

Command Tree	Header	Parameter
	:TRACe	
	:IQVTime	
	:AVERage	
	:COUNT	<numeric_value>
	:COUNT	<numeric_value>
	:ENABLe	<boolean>
	:RESet	
	:ENABLe	
	:I	<boolean>
	:Q	<boolean>
	:FREeze	<boolean>
	:FUNCTion	NORMal AVERage MAXHold MINHold
	:SElect	
	:I	<boolean>
	:Q	<boolean>

:TRACe:IQVTime:AVERAge:COUNT(?)

Sets or queries the number of traces to combine. This command works for both I and Q traces when you select AVERAge in the :TRACe:IQVTime:FUNCTion command.

Syntax :TRACe:IQVTime:AVERAge:COUNT <number>
:TRACe:IQVTime:AVERAge:COUNT?

Arguments <number>::=<NR1> specifies the number of traces to combine for averaging. Range: 1 to 10000.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:AVERAge:COUNT 64
sets the average count to 64.

Related Commands :TRACe:IQVTime:FUNCTion

:TRACe:IQVTime:COUNT(?)

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the RF I&Q versus Time measurement. This command is effective when :TRACe<x>:IQVTime:FUNCTion is set to MAXHold or MINHold and :INITiate:CONTinuous is set to OFF.

Syntax :TRACe:IQVTime:COUNT <number>
:TRACe:IQVTime:COUNT?

Arguments <number>::=<NR1> specifies the count for Max/Min Hold. Range: 1 to 10000.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:COUNT 32
sets the count to 32 for the Max/Min Hold trace.

Related Commands :INITiate:CONTinuous, :TRACe:IQVTime:FUNCTion

:TRACe:IQVTime:COUNT:ENABLE(?)

Determines whether to enable or disable the count for the Max or Min Hold trace in the RF I&Q versus Time view. This command is effective when :TRACe:IQVTime:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe:IQVTime:COUNT:ENABLE { OFF | ON | 0 | 1 }
:TRACe:IQVTime:COUNT:ENABLE?

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
ON or 1 enables the count for the Max/Min Hold trace.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:COUNT:ENABLE ON
enables the Max/Min Hold count.

Related Commands :TRACe:IQVTime:FUNCTION

:TRACe:IQVTime:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process in the RF I&Q versus Time view. This command is effective when :TRACe:IQVTime:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe:IQVTime:COUNT:RESet

Arguments None

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:COUNT:RESet
clears the Max/Min Hold data and counter, and restarts the process.

Related Commands :TRACe:IQVTime:FUNCTION

:TRACe:IQVTime:ENABle:I(?)

Determines whether to show or hide the I trace in the RF I&Q versus Time measurement.

Syntax :TRACe:IQVTime:ENABle:I { OFF | ON | 0 | 1 }
:TRACe:IQVTime:ENABle:I?

Arguments OFF or 0 hides the I trace.
ON or 1 shows the I trace.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:ENABle:I ON
shows the I trace in the RF I&Q versus Time measurement.

:TRACe:IQVTime:ENABle:Q(?)

Determines whether to show or hide the Q trace in the RF I&Q versus Time measurement.

Syntax :TRACe:IQVTime:ENABle:Q { OFF | ON | 0 | 1 }
:TRACe:IQVTime:ENABle:Q?

Arguments OFF or 0 hides the Q trace.
ON or 1 shows the Q trace.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:ENABle:Q ON
shows the Q trace in the IQ level versus Time measurement.

:TRACe:IQVTime:FREEze(?)

Determines whether to freeze the IQ traces in the RF I&Q versus Time measurement.

Syntax :TRACe:IQVTime:FREEze { OFF | ON | 0 | 1 }
:TRACe:IQVTime:FREEze?

Arguments OFF or 0 updates IQ trace display normally.
ON or 1 stops updating IQ trace display.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:FREEze ON
freezes the IQ traces.

:TRACe:IQVTime:FUNction(?)

Selects or queries the trace function in the RF I&Q versus Time measurement.

Syntax :TRACe:IQVTime:FUNction { NORMa1 | AVERage | MAXHold | MINHold }
:TRACe:IQVTime:FUNction?

Arguments NORMa1 selects the normal waveform display.
AVERage selects the Average display that indicates the average signal level at each time point.
MAXHold selects the Max Hold display that indicates the maximum signal level at each time point.
MINHold selects the Min Hold display that indicates the minimum signal level at each time point.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:FUNction MAXHold
displays the Max Hold trace in the IQ level versus Time measurement.

:TRACe:IQVTime:SElect:I(?)

Determines whether or not to select the I trace to obtain the maximum and minimum measurement results.

Syntax :TRACe:IQVTime:SElect:I { OFF | ON | 0 | 1 }
:TRACe:IQVTime:SElect:I?

Arguments OFF or 0 deselects the I trace.
ON or 1 selects the I trace.
Executing :TRACe:IQVTime:SElect:I ON sets :TRACe:IQVTime:SElect:Q OFF.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:SElect:I ON
selects the I trace in the RF I&Q versus Time measurement.

Related Commands :TRACe:IQVTime:SElect:Q

:TRACe:IQVTime:SElect:Q(?)

Determines whether or not to select the Q trace to obtain the maximum and minimum measurement results.

Syntax :TRACe:IQVTime:SElect:Q { OFF | ON | 0 | 1 }
:TRACe:IQVTime:SElect:Q?

Arguments OFF or 0 deselects the Q trace.
ON or 1 selects the Q trace.
Executing :TRACe:IQVTime:SElect:Q ON sets :TRACe:IQVTime:SElect:I OFF.

Measurement Views RF I&Q versus Time

Examples :TRACe:IQVTime:SElect:Q ON
selects the Q trace in the RF I&Q versus Time measurement.

Related Commands :TRACe:IQVTime:SElect:I

:TRACe:OBWidth Subgroup

The :TRACe:OBW commands control traces in the Occupied Bandwidth (OBW) measurement.

Command Tree	Header	Parameter
	:TRACe	
	:OBWidth	
	:MAXHold	<boolean>

:TRACe:OBWidth:MAXHold(?)

Determines whether or not to perform a Max Hold on the spectrum data for the Occupied Bandwidth trace.

Syntax :TRACe:OBWidth:MAXHold { OFF | ON | 0 | 1 }
:TRACe:OBWidth:MAXHold?

Arguments OFF or 0 does not perform a Max Hold on the spectrum data.
ON or 1 performs a Max Hold on the spectrum data.

Measurement Views Occupied Bandwidth

Examples :TRACe:OBWidth:MAXHold ON
performs a Max Hold on the spectrum data for the Occupied Bandwidth trace.

:TRACe:PHVTime Subgroup

The :TRACe:PHVTime commands control traces in the Phase versus Time measurement.

Command Tree	Header	Parameter
	:TRACe	
	:PHVTime	<boolean>
	:AVERage	
	:COUNt	<numeric_value>
	:COUNt	<numeric_value>
	:ENABle	<boolean>
	:RESet	
	:FREeze	<boolean>
	:FUNCTion	NORMal AVERage MAXHold MINHold

:TRACe:PHVTime(?)

Determines whether or not to show the trace in the Phase versus Time view.

Syntax :TRACe:PHVTime { OFF | ON | 0 | 1 }
:TRACe:PHVTime?

Arguments OFF or 0 hides the trace in the Phase versus Time view.
ON or 1 shows the trace in the Phase versus Time view.

Measurement Views Phase versus Time

Examples :TRACe:PHVTime ON
shows the trace in the Phase versus Time view.

:TRACe:PHVTime:AVERAge:COUNT(?)

Sets or queries the number of traces to combine. This command is effective when you select AVERAge with the :TRACe:PHVTime:FUNCTION command.

Syntax :TRACe:PHVTime:AVERAge:COUNT <number>
:TRACe:PHVTime:AVERAge:COUNT?

Arguments <number>::=<NR1> specifies the number of traces to combine for averaging.
Range: 1 to 10000.

Measurement Views Phase versus Time

Examples :TRACe:PHVTime:AVERAge:COUNT 64
sets the average count to 64.

Related Commands :TRACe:PHVTime:FUNCTION

:TRACe:PHVTime:COUNt(?)

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the Phase versus Time measurement.
This command is effective when :TRACe<x>:PHVTime:FUNCTION is set to MAXHold or MINHold and :INITiate:CONTinuous is set to OFF.

Syntax :TRACe:PHVTime:COUNt <number>
:TRACe:PHVTime:COUNt?

Arguments <number>::=<NR1> specifies the count for Max/Min Hold.
Range: 1 to 10000.

Measurement Views Phase versus Time

Examples :TRACe:PHVTime:COUNt 32
sets the count to 32 for the Max/Min Hold trace.

Related Commands :INITiate:CONTinuous, :TRACe:PHVTime:FUNCTION

:TRACe:PHVTime:COUNT:ENABLE(?)

Determines whether to enable or disable the count for the Max or Min Hold trace in the Phase versus Time view. This command is effective when :TRACe:PHVTime:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe:PHVTime:COUNT:ENABLE { OFF | ON | 0 | 1 }
:TRACe:PHVTime:COUNT:ENABLE?

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
ON or 1 enables the count for the Max/Min Hold trace.

Measurement Views Phase versus Time

Examples :TRACe:PHVTime:COUNT:ENABLE ON
enables the Max/Min Hold count.

Related Commands :TRACe:PHVTime:FUNCTION

:TRACe:PHVTime:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process in the Phase versus Time view. This command is effective when :TRACe:PHVTime:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe:PHVTime:COUNT:RESet

Arguments None

Measurement Views Phase versus Time

Examples :TRACe:PHVTime:COUNT:RESet
clears the Max/Min Hold data and counter, and restarts the process.

Related Commands :TRACe:PHVTime:FUNCTION

:TRACe:PHVTime:FReeze(?)

Determines whether to freeze the trace display in the Phase versus Time measurement.

Syntax :TRACe:PHVTime:FReeze { OFF | ON | 0 | 1 }
:TRACe:PHVTime:FReeze?

Arguments OFF or 0 updates the trace display normally.
ON or 1 stops updating trace display.

Measurement Views Phase versus Time

Examples :TRACe:PHVTime:FReeze ON
stops updating trace display.

:TRACe:PHVTime:FUNCTion(?)

Selects or queries the trace function in the Phase versus Time measurement.

Syntax :TRACe:PHVTime:FUNCTion
{ NORMa1 | AVERage | MAXHold | MINHold }
[:SENSe]:PHVTime:TRACe:FUNCTion?

Arguments NORMa1 selects the normal waveform display.
AVERage selects the Average display that indicates the average phase drift at each time point.
MAXHold selects the Max Hold display that indicates the maximum phase drift at each time point.
MINHold selects the Min Hold display that indicates the minimum phase drift at each time point.

Measurement Views Phase versus Time

Examples :TRACe:PHVTime:FUNCTion MAXHold
displays the Max Hold trace in the Phase versus Time measurement.

:TRACe:SGRam Subgroup

The :TRACe:SGRam commands control traces in the spectrogram.

Command Tree	Header	Parameter
	:TRACe	
	:SGRam	
	:DETection	AVERage POSitive NEGative
	:FREeze	<boolean>
	:FUNction	NONE AVERage MAXHold MINHold
	:TIME	<numeric_value>
	:SElect	
	:LINE	<numeric_value>

:TRACe:SGRam:DETection(?)

Selects or queries the display detector (method to be used for decimating traces to fit the available horizontal space on screen). The number of horizontal pixels on screen is generally smaller than that of waveform data points. When actually displayed, the waveform data is therefore thinned out, according to the number of pixels, for being compressed.

Syntax :TRACe:SGRam:DETection { AVERage | POSitive | NEGative }
 :TRACe:SGRam:DETection?

Arguments AVERage displays the average data value for each pixel.
 POSitive displays the maximum data value for each pixel.
 NEGative displays the minimum data value for each pixel.

Measurement Views Spectrogram

Examples :TRACe:SGRam:DETection POSitive
 displays the maximum data value for each pixel.

:TRACe:SGRam:FReeze(?)

Determines whether or not to freeze the spectrogram display.

Syntax :TRACe:SGRam:FReeze { OFF | ON | 0 | 1 }
:TRACe:SGRam:FReeze?

Arguments OFF or 0 updates the display of the spectrogram normally.
ON or 1 stops updating the display of the spectrogram.

Measurement Views Spectrogram

Examples :TRACe:SGRam:FReeze ON
freezes the spectrogram display.

:TRACe:SGRam:FUNCTion(?)

Selects or queries the trace function for the specified trace in the spectrogram.

Syntax :TRACe:SGRam:FUNCTion { NONE | AVERage | MAXHold | MINHold }
:TRACe:SGRam:FUNCTion?

Arguments NONE selects the normal spectrogram display.
AVERage selects the Average display that indicates the average signal level at each frequency point.
MAXHold selects the Max Hold display that indicates the maximum signal level at each frequency point.
MINHold selects the Min Hold display that indicates the minimum signal level at each frequency point.

Measurement Views Spectrogram

Examples :TRACe:SGRam:FUNCTion MAXHold
selects the Max Hold display for the spectrogram.

:TRACe:SGRam:FUNction:TIME(?)

Sets or queries the time length to combine traces for averaging in the spectrogram. This command is effective when :TRACe:SGRam:FUNction is set to AVERage, MAXHold or MINHold.

Syntax :TRACe:SGRam:FUNction:TIME <value>
 :TRACe:SGRam:FUNction:TIME?

Arguments <value>::=<NR1> specifies the time length to combine traces for averaging.
 Range: 0.02 to 60 minutes.

Measurement Views Spectrogram

Examples :TRACe1:SGRam:FUNction:TIME 1.5
 sets the time length to 1.5 minutes to combine traces for averaging.

Related Commands :TRACe:SGRam:FUNction

:TRACe:SGRam:SElect:LINE(?)

Selects or queries the number of line to send to the spectrum display.

Syntax :TRACe:SGRam:SElect:LINE <number>
 :TRACe:SGRam:SElect:LINE?

Arguments <number>::=<NR1> specifies the number of line to send to the spectrum display.
 Range: 0 to the maximum line number of the spectrogram displayed on screen.

Measurement Views Spectrogram

Examples :TRACe:SGRam:SElect:LINE 75
 selects Line #75 in the spectrogram to send to the spectrum display.

Related Commands :TRACe<x>:SPECTrum

:TRACe<x>:SPECTrum Subgroup

The :TRACe<x>:SPECTrum commands control traces in the Spectrum measurement.

Command Tree	Header	Parameter
	:TRACe<x>	
	:SPECTrum	<boolean>
	:AVERage	
	:COUNT	<numeric_value>
	:RESet	
	:COUNT	<numeric_value>
	:ENABle	<boolean>
	:RESet	
	:DETEction	AVERage POSitive NEGative
	:FREeze	<boolean>
	:FUNction	NONE AVERage MAXHold MINHold
	:LEFToperand	TRACE1 TRACE2 TRACE3
	:RIGHToperand	TRACE1 TRACE2 TRACE3
	:SElect	

Where <x> = 1 to 5. Each trace is defined as follows:

TRACe1: Trace 1
 TRACe2: Trace 2
 TRACe3: Trace 3
 TRACe4: Math trace
 TRACe5: Spectrogram

NOTE. Valid traces depend on commands. Refer to each command syntax.

:TRACe<x>:SPECTrum(?)

Determines whether to show or hide the specified trace in the Spectrum view.

Syntax :TRACe<x>:SPECTrum { OFF | ON | 0 | 1 }
 :TRACe<x>:SPECTrum?

Where <x> = 1 to 5; All traces are valid.

Arguments OFF or 0 hides the specified trace.
 ON or 1 shows the specified trace.
 For Trace 5 (spectrogram), use the :TRACe:SGRam:SElect:LINE command to
 select the number of line to send to the spectrum display.

Measurement Views Spectrum

Examples :TRACe1:SPECTrum ON
 shows Trace 1 in the Spectrum Analyzer view.

Related Commands :TRACe:SGRam:SElect:LINE

:TRACe<x>:SPECTrum:AVERage:COUNT(?)

Sets or queries the number of traces to combine. This command is effective when :TRACe<x>:SPECTrum:FUNCTION is AVERage, MAXHold or MINHold.

Syntax :TRACe<x>:SPECTrum:AVERage:COUNT <number>

:TRACe<x>:SPECTrum:AVERage:COUNT?

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Arguments <number>::=<NR1> specifies the number of traces to combine for averaging. Range: 1 to 10000.

Measurement Views Spectrum

Examples :TRACe1:SPECTrum:AVERage:COUNT 64
sets the average count to 64 for Trace 1.

Related Commands :TRACe<x>:SPECTrum:FUNCTION

:TRACe<x>:SPECTrum:AVERage:RESet (No Query Form)

Clears average data and counter, and restarts the average process for the specified trace in the Spectrum view. This command is effective when :TRACe<x>:SPECTrum:FUNCTION is set to AVERage, MAXHold or MINHold.

Syntax :TRACe<x>:SPECTrum:AVERage:RESet

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Arguments None

Measurement Views Spectrum

Examples :TRACe1:SPECTrum:AVERage:RESet
clears average data and counter, and restarts the average process for Trace 1.

Related Commands :TRACe<x>:SPECTrum:FUNCTION

:TRACe<x>:SPECTrum:COUNT(?)

Sets or queries how many acquisitions run in the single acquisition mode for the Max or Min Hold trace in the Spectrum measurement. This command is effective when :TRACe<x>:SPECTrum:FUNCTION is set to MAXHold or MINHold and :INITiate:CONTInuous is set to OFF.

Syntax :TRACe<x>:SPECTrum:COUNT <number>

:TRACe<x>:SPECTrum:COUNT?

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Arguments <number>::=<NR1> specifies the count for Max/Min Hold.
Range: 1 to 10000.

Measurement Views Spectrum

Examples :TRACe1:SPECTrum:COUNT 32
sets the count to 32 for Trace 1.

Related Commands :INITiate:CONTInuous, :TRACe<x>:SPECTrum:FUNCTION

:TRACe<x>:SPECTrum:COUNT:ENABLE(?)

Determines whether to enable or disable the count for the Max or Min Hold trace in the Spectrum view. This command is effective when :TRACe<x>:SPECTrum:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe<x>:SPECTrum:COUNT:ENABLE { OFF | ON | 0 | 1 }
:TRACe<x>:SPECTrum:COUNT:ENABLE?

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Arguments OFF or 0 disables the count for the Max/Min Hold trace.
ON or 1 enables the count for the Max/Min Hold trace.

Measurement Views Spectrum

Examples :TRACe1:SPECTrum:COUNT:ENABLE ON
enables the Max/Min Hold count for Trace 1.

Related Commands :TRACe<x>:SPECTrum:FUNCTION

:TRACe<x>:SPECtrum:COUNT:RESet (No Query Form)

Clears the Max or Min Hold data and counter, and restarts the process for the specified trace in the Spectrum view. This command is effective when :TRACe<x>:SPECtrum:FUNCTION is set to MAXHold or MINHold.

Syntax :TRACe<x>:SPECtrum:COUNT:RESet

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Arguments None

Measurement Views Spectrum

Examples :TRACe1:SPECtrum:COUNT:RESet
clears the Max/Min Hold data and counter, and restarts the process for Trace 1.

Related Commands :TRACe<x>:SPECtrum:FUNCTION

:TRACe<x>:SPECTrum:DETection(?)

Selects or queries the display detector (method to be used for decimating traces to fit the available horizontal space on screen). The number of horizontal pixels on screen is generally smaller than that of waveform data points. When actually displayed, the waveform data is therefore thinned out, according to the number of pixels, for being compressed.

Syntax :TRACe<x>:SPECTrum:DETection { AVERage | POSitive | NEGative }
:TRACe<x>:SPECTrum:DETection?

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Arguments AVERage displays the average data value for each pixel.
POSitive displays the maximum data value for each pixel.
NEGative displays the minimum data value for each pixel.

Measurement Views Spectrum

Examples :TRACe1:SPECTrum:DETection POSitive
displays the maximum data value for each pixel on Trace 1.

:TRACe<x>:SPECTrum:FREEze(?)

Determines whether or not to freeze the display of the specified trace in the Spectrum view.

Syntax :TRACe<x>:SPECTrum:FREEze { OFF | ON | 0 | 1 }

:TRACe<x>:SPECTrum:FREEze?

Where <x> = 1 to 5; All traces are valid.

Arguments OFF or 0 updates the display of the specified trace normally.

ON or 1 stops updating the display of the specified trace.

Measurement Views Spectrum

Examples :TRACe1:SPECTrum:FREEze ON
freezes Trace 1 in the Spectrum Analysis display.

:TRACe<x>:SPECTrum:FUNCTION(?)

Selects or queries the function for the specified trace in the Spectrum view.

Syntax :TRACe<x>:SPECTrum:FUNCTION
 { NONE | AVERage | MAXHold | MINHold }

 :TRACe<x>:SPECTrum:FUNCTION?

Where <x> = 1 to 3; Trace 4 (math trace) and Trace 5 (spectrogram) are invalid.

Arguments NONE selects the normal spectrum display.

AVERage selects the Average display that indicates the average signal level at each frequency point.

MAXHold selects the Max Hold display that indicates the maximum signal level at each frequency point.

MINHold selects the Min Hold display that indicates the minimum signal level at each frequency point.

Measurement Views Spectrum

Examples :TRACe1:SPECTrum:FUNCTION MAXHold
 selects Max Hold for Trace 1 in the Spectrum view.

:TRACe<x>:SPECTrum:LEFToperand(?)

Selects or queries the left operand for the math trace (Trace 4) in the Spectrum view.

Syntax :TRACe<x>:SPECTrum:LEFToperand { TRACE1 | TRACE2 | TRACE3 }
:TRACe<x>:SPECTrum:LEFToperand?

Where <x> = 4; Only Trace 4 (math trace) is valid.

Arguments TRACE1 selects Trace 1 as the left operand for the math trace.
TRACE2 selects Trace 2 as the left operand for the math trace.
TRACE3 selects Trace 3 as the left operand for the math trace.

Measurement Views Spectrum

Examples :TRACe4:SPECTrum:LEFToperand TRACE1
selects Trace 1 as the left operand for the math trace.

Related Commands :TRACe<x>:SPECTrum:RIGHToperand

:TRACe<x>:SPECTrum:RIGHtooperand(?)

Selects or queries the right operand for the math trace (Trace 4) in the Spectrum view.

Syntax :TRACe<x>:SPECTrum:RIGHtooperand { TRACE1 | TRACE2 | TRACE3 }
 :TRACe<x>:SPECTrum:RIGHtooperand?

Where <x> = 4; Only Trace 4 (math trace) is valid.

Arguments TRACE1 selects Trace 1 as the right operand for the math trace.
 TRACE2 selects Trace 2 as the right operand for the math trace.
 TRACE3 selects Trace 3 as the right operand for the math trace.

Measurement Views Spectrum

Examples :TRACe4:SPECTrum:RIGHtooperand TRACE1
 selects Trace 1 as the right operand for the math trace.

Related Commands :TRACe<x>:SPECTrum:LEFTooperand

:TRACe<x>:SPECTrum:SElect(?)

Selects or queries the trace to display the readout at the upper left of the Spectrum view.

Syntax :TRACe<x>:SPECTrum:SElect

:TRACe<x>:SPECTrum:SElect?

Where <x> = 1 to 5; All traces are valid.

NOTE. TRACe5 (spectrogram) is valid when the spectrum and spectrogram measurements are running.

Arguments None

Returns { 0 | 1 }

0 indicates that the readout is not being displayed for the specified trace.

1 indicates that the readout is being displayed for the specified trace.

Measurement Views Spectrum

Examples :TRACe1:SPECTrum:SElect
selects Trace 1 to display the readout.

:TRACe1:SPECTrum:SElect?
might return 1, indicating that the readout is being displayed for Trace 1.

TRIGger Commands

The TRIGger commands control triggering.

Command Tree

Header	Parameter
:TRIGger	
:MASK	
:NEW	<freq(1)>,<amp1(1)>, <freq(2)>,<amp1(2)>, ...,<freq(n)>,<amp1(n)>
:OPEN	<file_name>
:SAVE	<file_name>
[:SEQUence]	
:ADVanced	
:SWEep	
:MODE	<boolean>
:EVENT	
:EXTFront	
:IMPedance	OHM50 OHM5K
:LEVel	<numeric_value>
:SLOPe	RISe FALL
:EXTRear	
:SLOPe	RISe FALL
:GATed	HIGH LOW
:INPut	
:FMAsk	
:VIOLation	T F TF FT TFT FTF
:LEVel	<numeric_value>
:SLOPe	RISe FALL
:TDBWidth	<numeric_value>
ACTual?	
STATe	<boolean>
:TYPE	POWER FMAK
:SOURce	INPut EXTFront EXTRear EXTGated LINE
:FORCed	<boolean>
:IMMediate	
:STATus	<boolean>
:TIME	
:DELay	<numeric_value>
:POSition	<numeric_value>

:TRIGger:MASK:NEW (No Query Form)

Loads a new frequency mask.

Syntax :TRIGger:MASK:NEW <freq(1)>,<ampl(1)>,<freq(2)>,<ampl(2)>,
...,<freq(n)>,<ampl(n)> (n = 100 maximum)

Arguments <freq(n)>,<ampl(n)> is a frequency (Hz) and amplitude (dBm) pair to specify a point of the mask. Up to 100 pairs can be specified with zero frequency being the center screen.

The mask is visible in the spectrum view with the following trigger conditions:

- Trigger mode: Triggered
(:TRIGger[:SEquence]:STATus is set to ON or 1.)
- Trigger type: Frequency Mask
(:TRIGger[:SEquence]:EVENT:INPut:TYPE is set to FMASK.)

Measurement Views All

Examples :TRIGger:MASK:NEW -8E6,-80,0,-10,8E6,-80
loads the mask with the points A (-8 MHz, -80 dBm), B (0 Hz, -10 dBm), and C (8 MHz, -80 dBm), as shown in Figure 2-5.

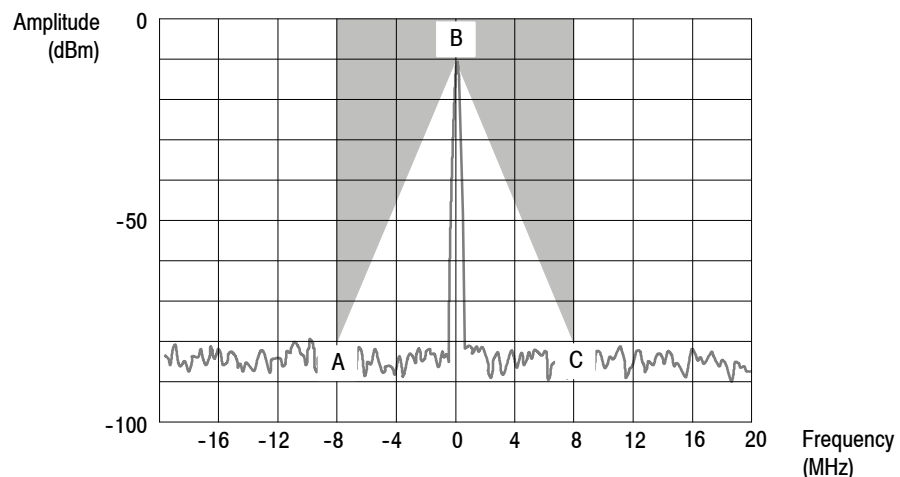


Figure 2-5: Trigger mask setting example

Related Commands :TRIGger[:SEquence]:EVENT:INPut:TYPE, :TRIGger[:SEquence]:STATus

:TRIGger:MASK:OPEN (No Query Form)

Opens a trigger mask with a specified file.

To save a trigger mask, use the :TRIGger:MASK:SAVE command.

Syntax :TRIGger:MASK:OPEN <file_name>

Arguments <file_name>::=<string> specifies the trigger mask file to open.
The file extension is .msk. You can omit the extension.

For the directory of file, refer to *Specifying the File* on page 2-445 in the MMEMory command section.

Measurement Views All

Examples :TRIGger:MASK:OPEN "C:\My Documents\Mask1"
opens the trigger mask with the *Mask1* file in the *My Document* directory.

Related Commands :TRIGger:MASK:SAVE

:TRIGger:MASK:SAVE (No Query Form)

Saves the current trigger mask to a specified file.

To open the trigger mask, use the :TRIGger:MASK:OPEN command.

Syntax :TRIGger:MASK:SAVE <file_name>

Arguments <file_name>::=<string> specifies the file to save the trigger mask.
The file extension is .msk. You can omit the extension.

For the directory of file, refer to *Specifying the File* on page 2-445 in the MMEMory command section.

Measurement Views All

Examples :TRIGger:MASK:SAVE "C:\My Documents\Mask1"
saves the trigger mask to the *Mask1* file in the *My Document* directory.

Related Commands :TRIGger:MASK:OPEN

:TRIGger[:SEquence]:ADVanced:SWEep:MODE(?)

Determines whether or not to trigger each segment in the swept acquisition mode.

Syntax :TRIGger[:SEquence]:ADVanced:SWEep:MODE { OFF | ON | 0 | 1 }
:TRIGger[:SEquence]:ADVanced:SWEep:MODE?

Arguments OFF or 0 does not trigger each segment in the swept acquisition mode.
ON or 1 triggers each segment in the swept acquisition mode.

Measurement Views All

Examples :TRIGger:SEquence:ADVanced:SWEep:MODE ON
triggers each segment in the swept acquisition mode.

:TRIGger[:SEquence]:EVENT:EXTFront:IMPedance(?)

Selects or queries the impedance of the external trigger input on the front panel.

Syntax :TRIGger[:SEquence]:EVENT:EXTFront:IMPedance { OHM50 | OHM5K }
:TRIGger[:SEquence]:EVENT:EXTFront:IMPedance?

Arguments OHM50 selects 50 Ω impedance.
OHM5K selects 5 k Ω impedance.

Measurement Views All

Examples :TRIGger:SEquence:EVENT:EXTFront:IMPedance OHM50
selects 50 Ω impedance for the external trigger input on the front panel.

:TRIGger[:SEQuence]:EVENT:EXTFront:LEVel(?)

Sets or queries the trigger level at the external trigger input on the front panel.

Syntax :TRIGger[:SEQuence]:EVENT:EXTFront:LEVel <value>
 :TRIGger[:SEQuence]:EVENT:EXTFront:LEVel?

Arguments <value>::=<NRf> specifies the trigger level.
 Range: -2.5 to +2.5 V.

Measurement Views All

Examples :TRIGger:SEQuence:EVENT:EXTFront:LEVel 1.5
 sets the trigger level to 1.5 V at the external trigger input on the front panel.

:TRIGger[:SEQuence]:EVENT:EXTFront:SLOPe(?)

Selects or queries the trigger slope of the external trigger input on the front panel.

Syntax :TRIGger[:SEQuence]:EVENT:EXTFront:SLOPe { RISE | FALL }
 :TRIGger[:SEQuence]:EVENT:EXTFront:SLOPe?

Arguments RISE causes the trigger event on the rising edge.
 FALL causes the trigger event on the falling edge.

Measurement Views All

Examples :TRIGger:SEQuence:EVENT:EXTFront:SLOPe RISE
 causes the trigger event on the rising edge of the external input signal.

:TRIGger[:SEquence]:EVENT:EXTRear:SLOPe(?)

Selects or queries the trigger slope of the external trigger input on the rear panel.
The trigger level is fixed to the TTL threshold.

Syntax :TRIGger[:SEquence]:EVENT:EXTRear:SLOPe { RISE | FALL }
 :TRIGger[:SEquence]:EVENT:EXTRear:SLOPe?

Arguments RISE causes the trigger event on the rising edge.
 FALL causes the trigger event on the falling edge.

Measurement Views All

Examples :TRIGger:SEquence:EVENT:EXTRear:SLOPe RISE
 causes the trigger event on the rising edge of the external input signal.

:TRIGger[:SEquence]:EVENT:GATed(?)

Selects or queries the positive or negative logic for the gated trigger input on the rear panel.

Syntax :TRIGger[:SEquence]:EVENT:GATed { HIGH | LOW }
 :TRIGger[:SEquence]:EVENT:GATed?

Arguments HIGH specifies that the gated trigger input is high active.
 LOW specifies that the gated trigger input is low active.

Measurement Views All

Examples :TRIGger:SEquence:EVENT:GATed HIGH
 specifies that the gated trigger input is high active.

:TRIGger[:SEQuence]:EVENT:INPut:FMASk:VIOLation(?)

Selects or queries when the analyzer triggers in the frequency mask trigger.

Syntax :TRIGger[:SEQuence]:EVENT:INPut:FMASk:VIOLation
 { T | F | TF | FT | TFT | FTF }
 :TRIGger[:SEQuence]:EVENT:INPut:FMASk:VIOLation?

Arguments Table 2-49 lists the arguments which represent the trigger violations.

Table 2-49: Trigger violations

Violation	Description
T	Only one state is required to initiate a trigger event. The signal has at least one data point inside the mask. The trigger event occurs at the first point that appears inside the mask. A trigger event could occur on the first acquisition.
F	Only one state change is required to initiate a trigger event. The signal has at least one data point outside the mask. The trigger event occurs at the first point that appears outside the mask. A trigger event could occur on the first acquisition.
TF	Two states are required to initiate a trigger event. The signal must be inside the mask and then passes out of the mask. The trigger event occurs at the first transition where the signal passes out of the mask.
FT	Two states are required to initiate a trigger event. The signal must be outside the mask and then passes into the mask. The trigger event occurs at the first transition where the signal passes into the mask.
TFT	Three states are required to initiate a trigger event. The signal starts inside the mask and then passes out of the mask. Next, the signal must pass into the mask. The trigger event occurs at the second transition where the signal passes back into the mask.
FTF	Three states are required to initiate a trigger event. The signal starts outside the mask and then passes into the mask. Next, the signal must pass back outside the mask. The trigger event occurs at the second transition where the signal passes back out of the mask.

Measurement Views All

Examples :TRIGger:SEQuence:EVENT:INPut:FMASk:VIOLation TF
 specifies that the analyzer will trigger when the signal has crossed into the mask and then outside of the mask.

:TRIGger[:SEQuence]:EVENT:INPut:LEVel(?)

Sets or queries the trigger level for the RF input level trigger.

Syntax :TRIGger[:SEQuence]:EVENT:INPut:LEVel <value>
 :TRIGger[:SEQuence]:EVENT:INPut:LEVel?

Arguments <value>::=<NRf> specifies the trigger level.
 Range: -170 to +50 dBm.

Measurement Views All

Examples :TRIGger:SEQuence:EVENT:INPut:LEVel -10
 sets the trigger level to -10 dBm for the RF input level trigger.

:TRIGger[:SEQuence]:EVENT:INPut:SLOPe(?)

Selects or queries the trigger slope for the RF input level trigger.

Syntax :TRIGger[:SEQuence]:EVENT:INPut:SLOPe { RISE | FALL }
 :TRIGger[:SEQuence]:EVENT:INPut:SLOPe?

Arguments RISe causes the trigger event on the rising edge.
 FALL causes the trigger event on the falling edge.

Measurement Views All

Examples :TRIGger:SEQuence:EVENT:INPut:SLOPe RISE
 causes the trigger event on the rising edge of the RF input signal.

:TRIGger[:SEQuence]:EVENT:INPut:TDBWidth(?)

Sets or queries the time-domain bandwidth for the RF input power trigger. This command is effective when :TRIGger[:SEQuence]:EVENT:INPut:TDBWidth:STATe is ON.

Syntax :TRIGger[:SEQuence]:EVENT:INPut:TDBWidth <value>
:TRIGger[:SEQuence]:EVENT:INPut:TDBWidth?

Arguments <value>::=<NRf> specifies the time-domain bandwidth.
Range: 1 Hz to 60 MHz.

Measurement Views All

Examples :TRIGger:SEQuence:EVENT:INPut:TDBWidth 5MHz
sets the time-domain bandwidth to 5 MHz for the RF input power trigger.

Related Commands :TRIGger[:SEQuence]:EVENT:INPut:TDBWidth:STATe

:TRIGger[:SEQuence]:EVENT:INPut:TDBWidth:ACTual? (Query Only)

Queries the actual time-domain bandwidth for the RF input power trigger.

Syntax :TRIGger[:SEQuence]:EVENT:INPut:TDBWidth:ACTual?

Arguments None

Returns <NRf> Actual time-domain bandwidth.

Measurement Views All

Examples :TRIGger:SEQuence:EVENT:INPut:TDBWidth:ACTual?
might return 1.000E+6, indicating that the actual time-domain bandwidth is 1 MHz.

Related Commands :TRIGger[:SEQuence]:EVENT:INPut:TDBWidth

:TRIGger[:SEquence]:EVENT:INPut:TDBWidth:STATe(?)

Determines whether to set the time-domain bandwidth automatically or manually for the RF input power trigger.

Syntax :TRIGger[:SEquence]:EVENT:INPut:TDBWidth:STATe
 { OFF | ON | 0 | 1 }

 :TRIGger[:SEquence]:EVENT:INPut:TDBWidth:STATe?

Arguments OFF or 0 sets the time-domain bandwidth automatically.

 ON or 1 sets the time-domain bandwidth manually using the
 :TRIGger[:SEquence]:EVENT:INPut:TDBWidth command.

Measurement Views All

Examples :TRIGger:SEquence:EVENT:INPut:TDBWidth:STATe OFF
 sets the time-domain bandwidth automatically.

Related Commands :TRIGger[:SEquence]:EVENT:INPut:TDBWidth

:TRIGger[:SEquence]:EVENT:INPut:TYPE(?)

Selects or queries the trigger type for the source of RF input.

Syntax :TRIGger[:SEquence]:EVENT:INPut:TYPE { POWER | FMASK }

 :TRIGger[:SEquence]:EVENT:INPut:TYPE?

Arguments POWER uses the power level for triggering.

 FMASK uses the frequency mask for triggering.

Measurement Views All

Examples :TRIGger:SEquence:EVENT:INPut:TYPE FMASK
 uses the frequency mask for triggering.

:TRIGger[:SEquence]:EVENT:SOURce(?)

Selects or queries the trigger event source.

Syntax :TRIGger[:SEquence]:EVENT:SOURce
 { INPut | EXTFront | EXTrear | EXTGated | LIne }
 :TRIGger[:SEquence]:EVENT:SOURce?

Arguments Table 2-50 lists the arguments.

Table 2- 50: Trigger event source

Argument	Source
INPut	RF input
EXTFront	Trigger in (front)
EXTrear	Trigger in (rear)
EXTGated	Gate in
LIne	AC line

Measurement Views All

Examples :TRIGger:SEquence:EVENT:SOURce INPut
 specifies the trigger event source as the RF input.

:TRIGger[:SEQuence]:FORCed(?)

Determines whether or not to cause a manual trigger if the acquisition is armed, ready and waiting for a trigger. This command is valid when :TRIGger[:SEQuence]:STATus is set to On (the trigger mode is Triggered).

Syntax :TRIGger[:SEQuence]:FORCed { OFF | ON | 0 | 1 }
:TRIGger[:SEQuence]:FORCed?

Arguments OFF or 0 does not cause a manual trigger.
ON or 1 causes a manual trigger.

Measurement Views All

Examples :TRIGger:SEQuence:FORCed ON
causes a manual trigger if the acquisition is armed, ready and waiting for a trigger.

Related Commands :TRIGger[:SEQuence]:STATus

:TRIGger[:SEQuence]:IMMediate (No Query Form)

Causes a trigger immediately, skipping the event detection and delay. This command is valid when :TRIGger[:SEQuence]:STATus is set to On (the trigger mode is Triggered).

Syntax :TRIGger[:SEQuence]:IMMediate

Arguments None

Measurement Views All

Examples :TRIGger:SEQuence:IMMediate
causes a trigger immediately, skipping the event detection and delay.

Related Commands :TRIGger[:SEQuence]:STATus

:TRIGger[:SEQuence]:STATus(?)

Selects or queries the trigger mode (Free Run or Triggered).

Syntax :TRIGger[:SEQuence]:STATus { OFF | ON | 0 | 1 }
 :TRIGger[:SEQuence]:STATus?

Arguments OFF or 0 selects the free-run mode.
 ON or 1 selects the triggered mode.

Measurement Views All

Examples :TRIGger:SEQuence:STATus ON
 selects the triggered mode.

:TRIGger[:SEquence]:TIME:DElay(?)

Sets or queries the trigger delay time (after recognizing the event before actually declaring the trigger).

Syntax :TRIGger[:SEquence]:TIME:DElay <value>
 :TRIGger[:SEquence]:TIME:DElay?

Arguments <value>::=<Nrf> specifies the trigger delay time.
 Range: 0 to 60 s.

Measurement Views All

Examples :TRIGger:SEquence:TIME:DElay 1.5
 sets the trigger delay time to 1.5 s.

:TRIGger[:SEquence]:TIME:POStion(?)

Sets or queries the trigger position (location of the trigger event within the acquisition record).

Syntax :TRIGger[:SEquence]:TIME:POStion <value>
 :TRIGger[:SEquence]:TIME:POStion?

Arguments <value>::=<Nrf> specifies the trigger position.
 Range: 0 to 100%.

Measurement Views All

Examples :TRIGger:SEquence:TIME:POStion 20
 sets the trigger position to 20% of the acquisition record.

UNIT Commands

The :UNIT commands specify fundamental units for measurement.

Command Tree

Header	Parameter
:UNIT	
:POWer	DBM DBV VOLTs WATTs DBUW DBW DBUV DBMV DBUA DBUV_M DBUA_M AMPS

:UNIT:POWer(?)

Selects or queries the fundamental unit of power.
This command is equivalent to [:SENSe]:POWer:UNITs.

Syntax :UNIT:POWer { DBM | DBV | VOLTs | WATTs | DBUW | DBW
 | DBUV | DBMV | DBUA | DBUV_M | DBUA_M | AMPS }

 :UNIT:POWer?

Arguments Table 2-51 lists the arguments.

Table 2-51: Power units

Argument	Power unit
DBM	dBm
DBV	dBV
VOLTs	Volts
WATTs	Watts
DBUW	dB μ W
DBW	dBW
DBUV	dB μ V
DBMV	dBmV
DBUA	dB μ A
DBUV_M	dB μ V/m
DBUA_M	dB μ A/m
AMPS	Amps

NOTE. Select dB μ V/m or dB μ A/m unit when using an antenna table.

Measurement Views All

Examples :UNIT:POWer DBM
 specifies the fundamental unit of power as dBm.

Related Commands [:SENSe]:POWer:UNITs

Retrieving Response Message

When receiving a query command from the external controller, the analyzer puts the response message on the Output Queue. This message cannot be retrieved unless you perform retrieval operations through the external controller. (For example, call the IBRD subroutine included in the GPIB software of National Instruments.)

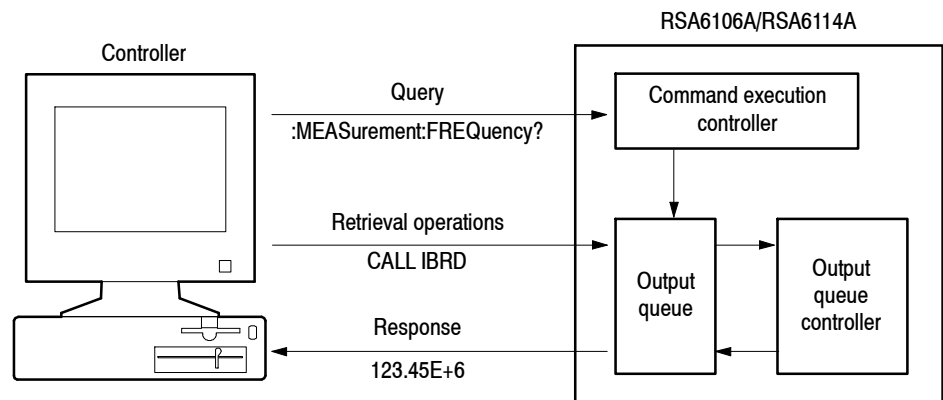


Figure 2-6: Retrieving response message

When the Output Queue contains a response message, sending another command from the external controller before retrieving this message deletes it from the queue. The Output Queue always contains the response message to the most recent query command.

You can use the MAV bit of the Status Byte Register (SBR) to check whether the Output Queue contains a response message. For details, refer to *Status Byte Register (SBR)* on page 3-4.



Status and Events

Status and Events

The SCPI interface in the analyzer includes a status and event reporting system that enables the user to monitor crucial events that occur in the instrument. The analyzer is equipped with four registers and one queue that conform to IEEE Std 488.2-1987. This section will discuss these registers and queues along with status and event processing.

Status and Event Reporting System

Figure 3-1 outlines the status and event reporting mechanism offered in the RSA6100A Series analyzers. It contains three major blocks:

- Standard Event Status
- Operation Status
- Questionable Status (fan-out structure)

The processes performed in these blocks are summarized in the Status Byte. The three blocks contain four types of registers as shown in Table 3-1.

Table 3- 1: Register type

Register	Description
Condition register	Records event occurrence in the instrument. Read only.
Transition register (positive/negative)	A positive transition filter allows an event to be reported when a condition changes from false to true. A negative filter allows an event to be reported when a condition changes from true to false. Setting both positive and negative filters true allows an event to be reported anytime the condition changes. Clearing both filters disables event reporting.
Event register	Records events filtered by the transition register. Read only.
Enable register	Masks the event register to report in the summary bit. User-definable.

* The use of Bit 15 is not allowed in SCPI.
The value of this bit is always zero.

CR: Condition Register
TR: Transition Register
EVR: Event Register
ENR: Enable Register

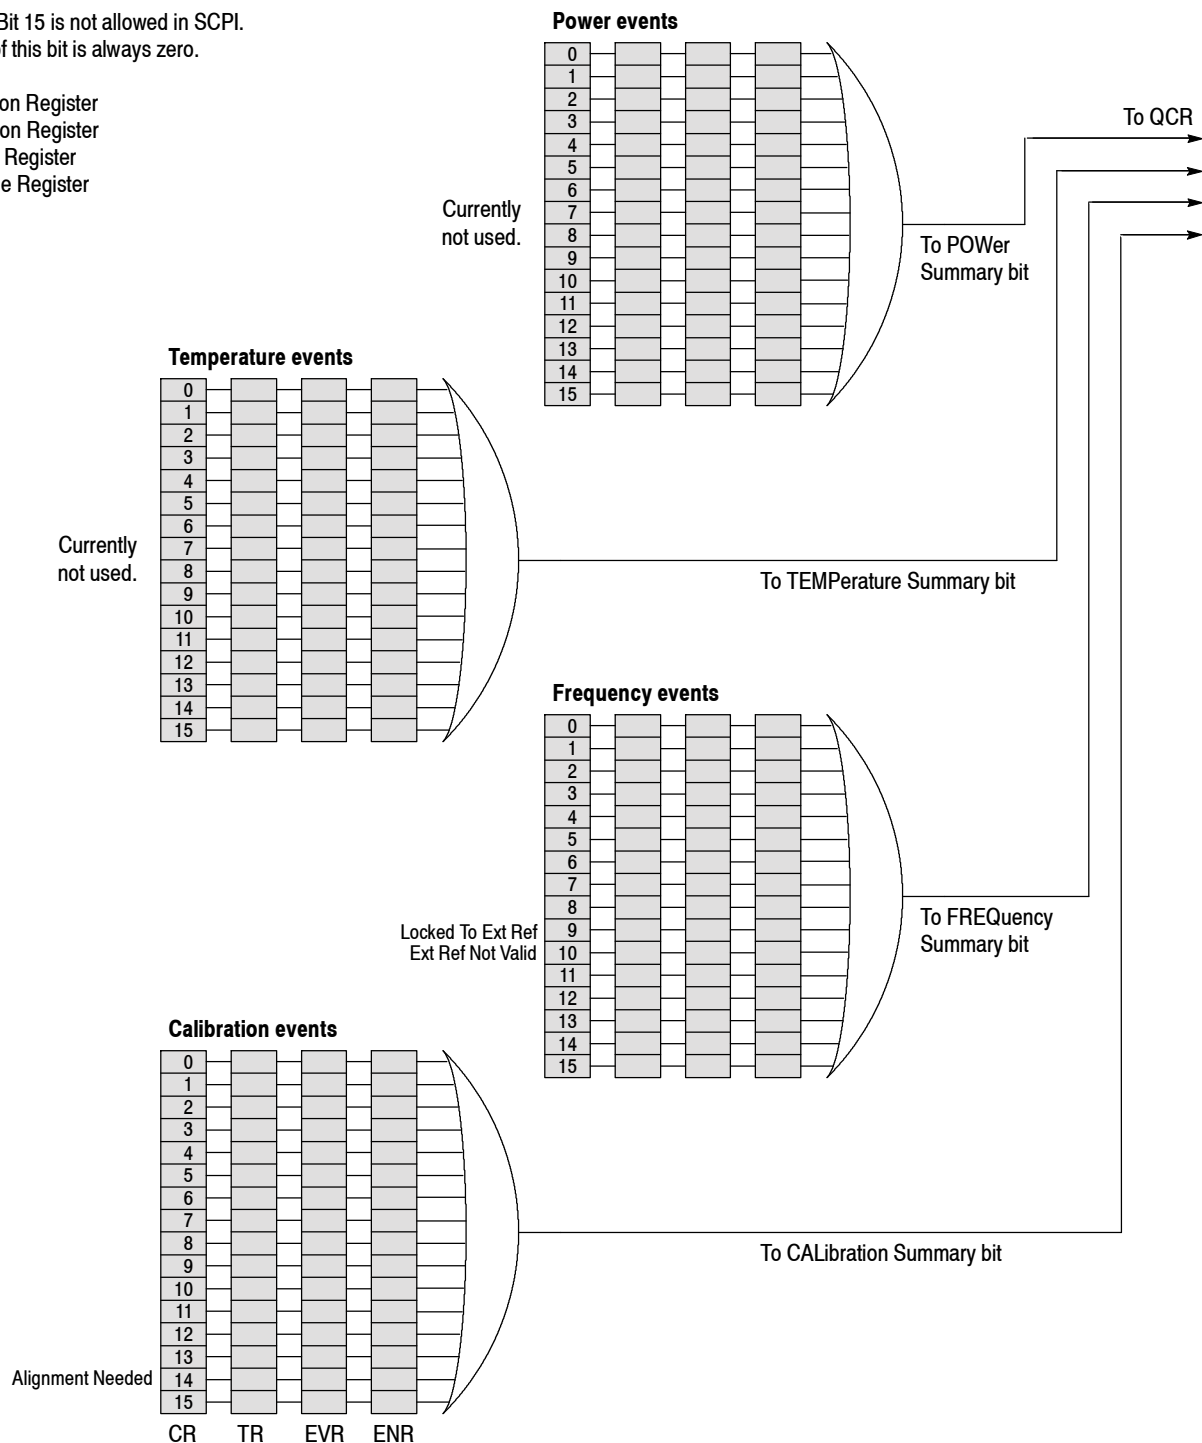


Figure 3-1: Status/Event reporting mechanism

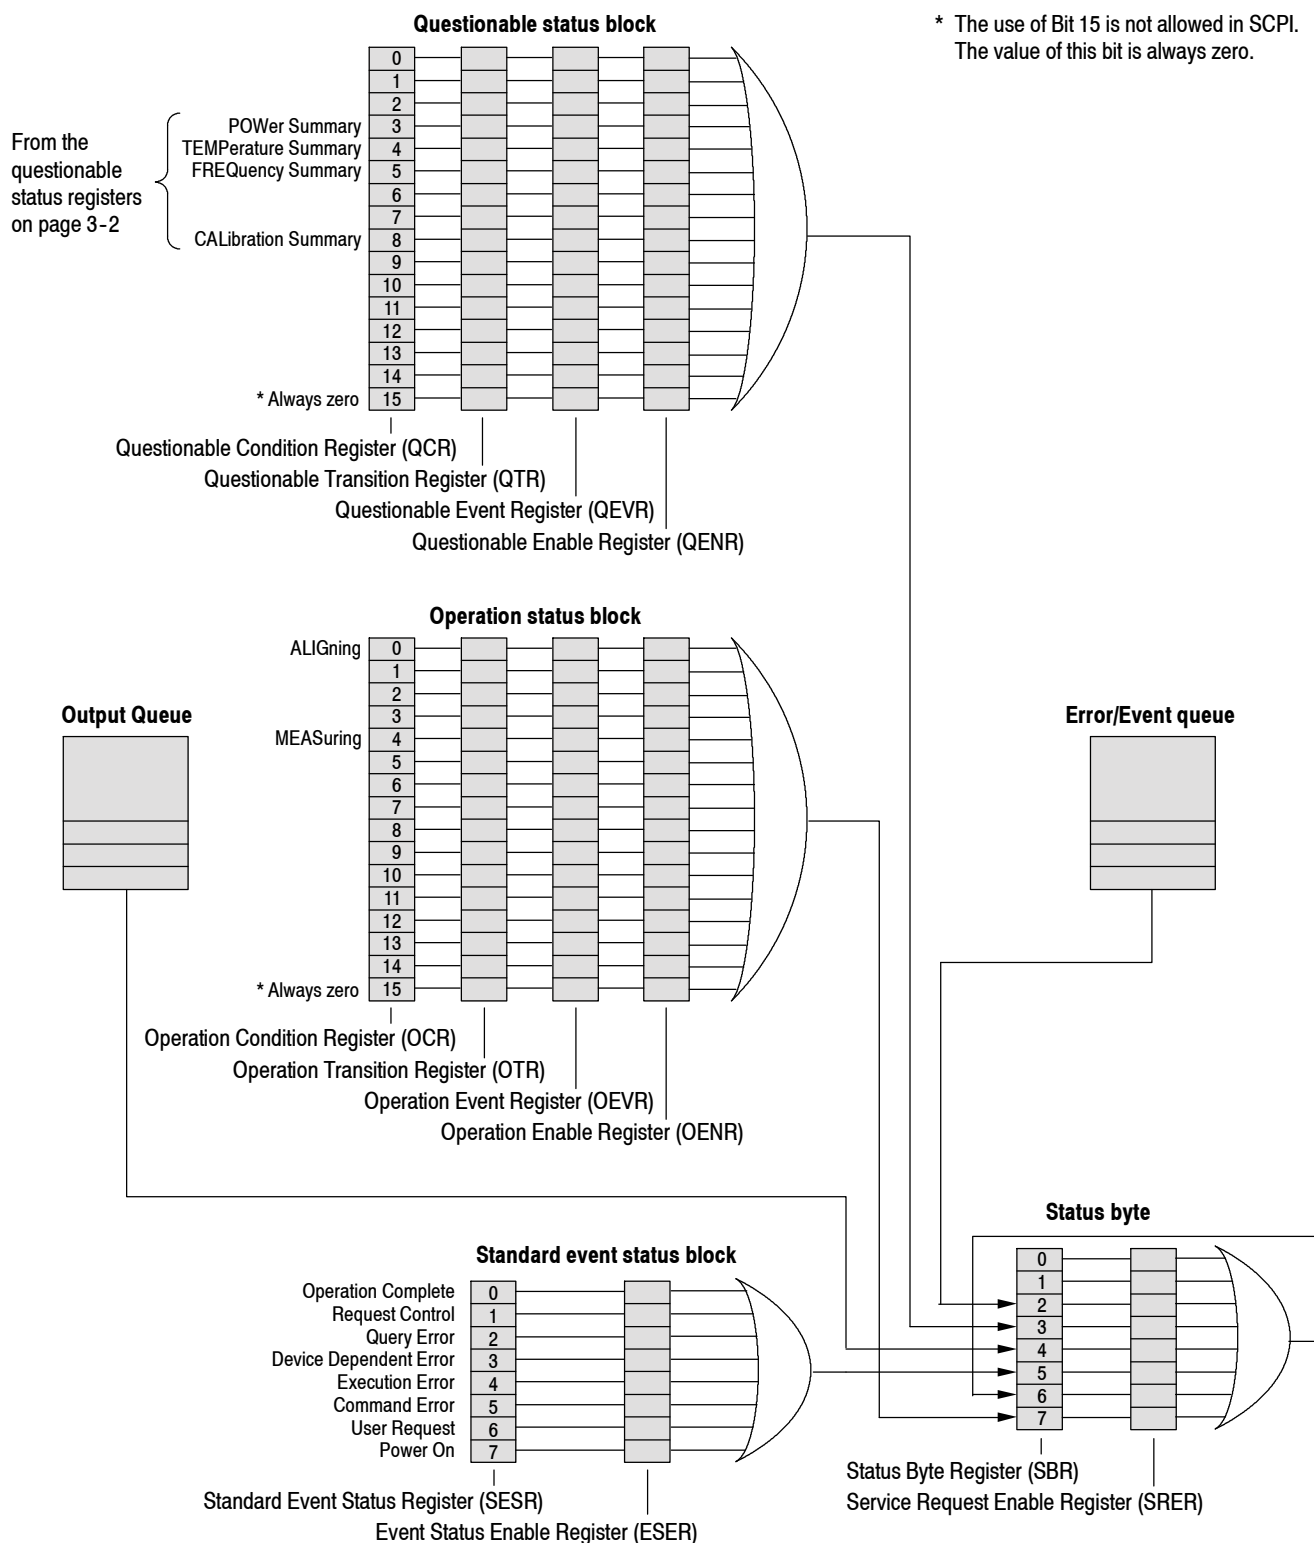


Figure 3-1: Status/Event reporting mechanism (Cont.)

Status Byte

The Status Byte contains the following two registers:

- Status Byte Register (SBR)
- Service Request Enable Register (SRER)

Status Byte Register (SBR)

The SBR is made up of 8 bits. Bits 4, 5 and 6 are defined in accordance with IEEE Std 488.2-1987 (see Figure 3-2 and Table 3-2). These bits are used to monitor the output queue, SESR and service requests, respectively. The contents of this register are returned when the *STB? query is used.

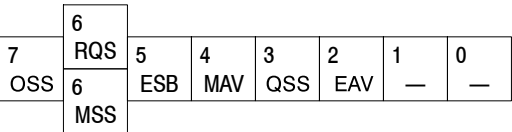


Figure 3-2: Status Byte Register (SBR)

Table 3-2: SBR bit functions

Bit	Function
7	Operation Summary Status (OSS). Summary of the operation status register.
6	<p>Request Service (RQS)/Master Status Summary (MSS). When the instrument is accessed using the GPIB serial poll command, this bit is called the Request Service (RQS) bit and indicates to the controller that a service request has occurred (in other words, that the GPIB bus SRQ line is LOW). The RQS bit is cleared when serial poll ends.</p> <p>When the instrument is accessed using the *STB? query, this bit is called the Master Status Summary (MSS) bit and indicates that the instrument has issued a service request for one or more reasons. The MSS bit is never cleared to 0 by the *STB? query.</p>
5	Event Status Bit (ESB). This bit indicates whether or not a new event has occurred after the previous Standard Event Status Register (SESR) has been cleared or after an event readout has been performed.
4	Message Available Bit (MAV). This bit indicates that a message has been placed in the output queue and can be retrieved.
3	Questionable Summary Status (QSS). Summary of the Questionable Status Byte register.
2	Event Quantity Available (EAV). Summary of the Error Event Queue.
1-0	Not used

Service Request Enable Register (SRER)

The SRER is made up of bits defined exactly the same as bits 0 through 7 in the SBR (see Figure 3-3). This register is used by the user to determine what events will generate service requests.

The SRER bit 6 cannot be set. Also, the RQS is not maskable.

The generation of a service request with the GPIB interface involves changing the SRQ line to LOW and making a service request to the controller. The result is that a status byte for which an RQS has been set is returned in response to serial polling by the controller.

Use the *SRE command to set the bits of the SRER. Use the *SRE? query to read the contents of the SRER. Bit 6 must normally be set to 0.

7	6	5	4	3	2	1	0
OSB	—	ESB	MAV	QSB	—	—	—

Figure 3-3: Service Request Enable Register (SRER)

Standard Event Status Block

Reports the power on/off state, command errors, and the running state. It consists of the following registers:

- Standard Event Status Register (SESR)
- Event Status Enable Register (ESER)

These registers are made up of the same bits defined in Figure 3-4 and Table 3-3. Use the *ESR? query to read the contents of the SESR. Use the *ESE(?) command to access the ESER.

7	6	5	4	3	2	1	0
PON	—	CME	EXE	DDE	QYE	—	OPC

Figure 3-4: Standard event status register

Table 3-3: Standard event status register bit definition

Bit	Description
7	Power On (PON). Indicates that the power to the instrument is on.
6	Not used.
5	Command Error (CME). Indicates that a command error has occurred while parsing by the command parser was in progress.
4	<p>Execution Error (EXE). Indicates that an error occurred during the execution of a command. Execution errors occur for one of the following reasons:</p> <ul style="list-style-type: none"> ■ When a value designated in the argument is outside the allowable range of the instrument, or is in conflict with the capabilities of the instrument ■ When the command could not be executed properly because the conditions for execution differed from those essentially required
3	Device-Dependent Error (DDE). An instrument error has been detected.
2	<p>Query Error (QYE). Indicates that a query error has been detected by the output queue controller. Query errors occur for one of the following reasons:</p> <ul style="list-style-type: none"> ■ An attempt was made to retrieve messages from the output queue, despite the fact that the output queue is empty or in pending status. ■ The output queue messages have been cleared despite the fact that they have not been retrieved.
1	Not used.
0	Operation Complete (OPC). This bit is set with the results of the execution of the *OPC command. It indicates that all pending operations have been completed.

When an event occurs, the SESR bit corresponding to the event is set, resulting in the event being stacked in the Error/Event Queue. The SBR OAV bit is also set. If the bit corresponding to the event has also been set in the ESER, the SBR ESB bit is also set. When a message is sent to the Output Queue, the SBR MAV bit is set.

Operation Status Block

The operation status block contains conditions that are part of the instrument's normal operation. It consists of the following registers:

- Operation Condition Register (OCR)
- Operation Positive/ Negative Transition Register (OPTR/ONTR)
- Operation Event Register (OEVR)
- Operation Enable Register (OENR)

These registers are made up of the same bits defined in Figure 3-5 and Table 3-4. Use the :STATus:OPERation commands to access the operation status register set.

15	14	13	12	11	10	9	8	7	6	5	4 MEAS	3	2	1	0 ALIG
----	----	----	----	----	----	---	---	---	---	---	-----------	---	---	---	-----------

Figure 3-5: Operation status register

Table 3-4: Operation status register bit definition

Bit	Description
15	Always zero (0).
14 - 5	Not used.
4	Measuring (MEAS). Indicates that the instrument is actively measuring. When the measurement ends after this bit is set in measurement, it is reset. "In measurement" means that one of the following commands is in execution: :INITiate commands :READ commands
3 - 1	Not used.
0	Aligning (ALIG). Indicates that the instrument is currently performing an alignment. When the alignment ends after this bit is set in alignment, it is reset.

When the specified state changes in the OCR, its bit is set or reset. This change is filtered with a transition register, and the corresponding bit of the OEVR is set. If the bit corresponding to the event has also been set in the OENR, the SBR OSS bit is also set.

Questionable Status Block

The questionable status register set contains bits which give an indication of the quality of various aspects of the signal together with the fanned out registers as described in the next subsections. It consists of the following registers:

- Questionable Condition Register (QCR)
- Questionable Positive/Negative Transition Register (QPTR/QNTR)
- Questionable Event Register (QEVN)
- Questionable Enable Register (QENR)

These registers are made up of the same bits defined in Figure 3-6 and Table 3-5. Use the :STATus:QUEStionable commands to access the questionable status register set.

15	14	13	12	11	10	9	8	7	6	5	4	3	2	1	0
	CW						CAL			FREQ	TEMP	POW			

Figure 3-6: Questionable status register

Table 3-5: Questionable status register bit definition

Bit	Description
15	Always zero (0).
14	Command Warning (CW). Indicates a non-fatal warning that relates to the instrument's interpretation of a command, query, or one or more parameters of a specific command or query.
13 - 9	Not used.
8	CALibration Summary (CAL). Summary of the Questionable Calibration register.
7, 6	Not used.
5	FREQuency Summary (FREQ). Summary of the Questionable Frequency register.
4	TEMPerature Summary (TEMP). Summary of the Questionable Temperature register.
3	POWEr Summary (POW). Summary of the Questionable Power register.
2 - 0	Not used.

When the specified state changes in the QCR, its bit is set or reset. This change is filtered with a transition register, and the corresponding bit of the QEVN is set. If the bit corresponding to the event has also been set in the QENR, the SBR QSS bit is also set.

Questionable Power Register Set

Refines the power error for the POWER bit in the QCR.
Currently not used.

Questionable Temperature Register Set

Refines the temperature error for the TEMPerature bit in the QCR.
Currently not used.

Questionable Frequency Register Set

The questionable frequency register set is made up of bits defined in Figure 3-7 and Table 3-6. It refines the frequency error for the FREQuency bit in the QCR. Use the :STATus:QUESTionable:FREQuency commands to access the questionable frequency register set.

15	14	13	12	11	10 ERNV	9 LTER	8	7	6	5	4	3	2	1	0
----	----	----	----	----	------------	-----------	---	---	---	---	---	---	---	---	---

Figure 3-7: Questionable frequency status register

Table 3-6: Questionable frequency status register bit definition

Bit	Description
15	Always zero (0).
14 - 11	Not used.
10	External Ref Not Valid (ERNV). Indicates that the external reference signal is not valid so the instrument is no longer locked to it.
9	Locked To External Ref (LTER). Indicates that the instrument is locked to the external reference signal.
8 - 0	Not used.

Questionable Calibration Register Set

The questionable calibration register set is made up of bits defined in Figure 3-8 and Table 3-7. It refines the calibration error for the CALibration bit in the QCR. Use the :STATus:QUEStionable:CALibration commands to access the questionable calibration register set.

15	14 ALN	13	12	11	10	9	8	7	6	5	4	3	2	1	0
----	-----------	----	----	----	----	---	---	---	---	---	---	---	---	---	---

Figure 3-8: Questionable calibration status register

Table 3-7: Questionable calibration status register bit definition

Bit	Description
15	Always zero.
14	Alignment Needed (ALN). Indicates the instrument needs the alignment.
13 - 0	Not used.

Queues

There are two types of queues in the status reporting system used in the analyzer: output queues and event queues.

Output Queue

The output queue is a FIFO (first in, first out) queue and holds response messages to queries, where they await retrieval. When there are messages in the queue, the SBR MAV bit is set.

The output queue will be emptied each time a command or query is received, so the controller must read the output queue before the next command or query is issued. If this is not done, an error will occur and the output queue will be emptied; however, the operation will proceed even if an error occurs.

Event Queue

The event queue is a FIFO queue and stores events as they occur in the analyzer. If more than 32 events occur, event 32 will be replaced with event code -350 (“Queue Overflow”). The error code and text are retrieved using the :SYSTem:ERRor queries.

Status and Event Processing Sequence

Figure 3-9 shows an outline of the sequence for status and event processing.

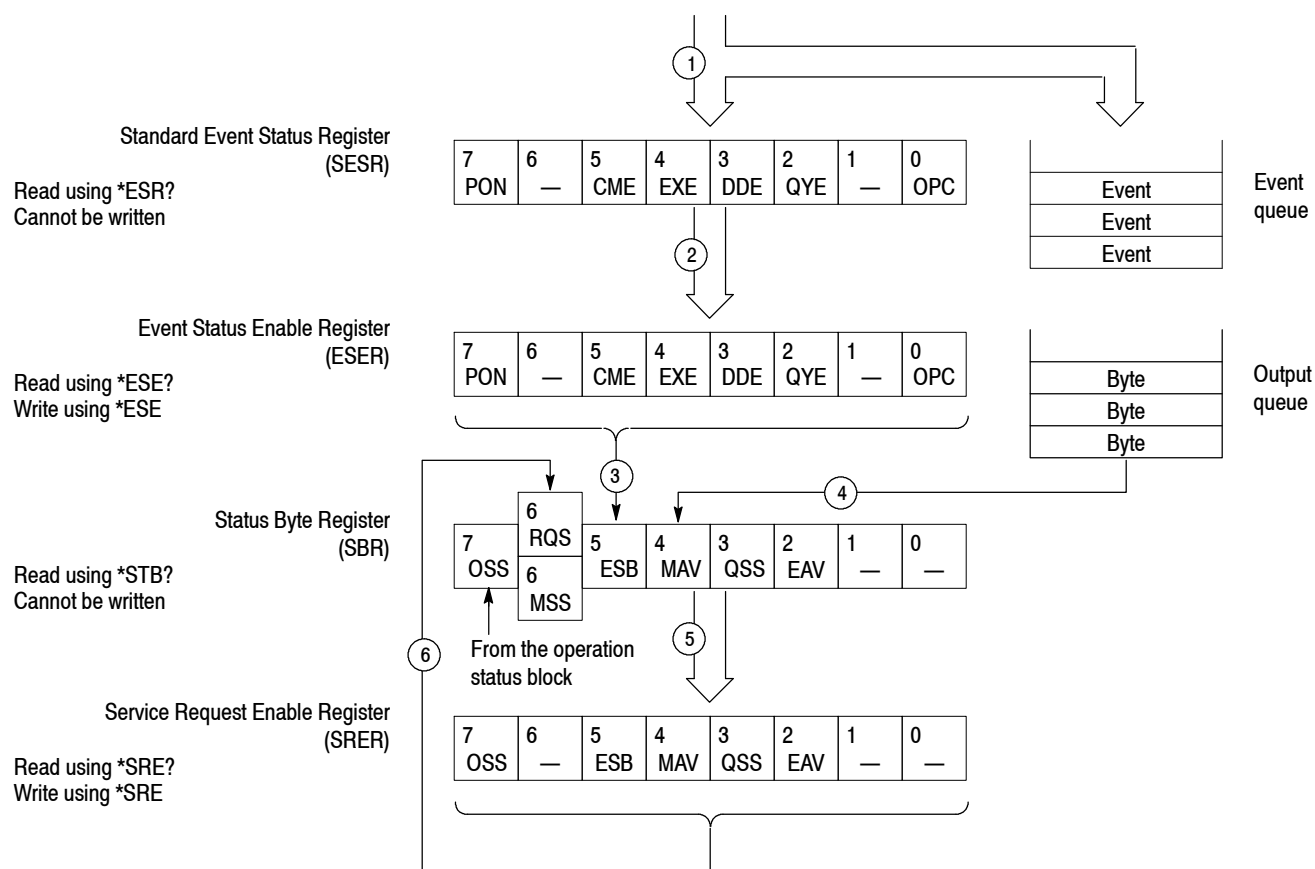


Figure 3-9: Status and event processing sequence

1. If an event has occurred, the SESR bit corresponding to that event is set and the event is placed in the event queue.
2. A bit corresponding to that event in the ESER has is set.
3. The SBR ESB bit is set to reflect the status of the ESER.
4. When a message is sent to the output queue, the SBR MAV bit is set.
5. Setting either the ESB or MAV bits in the SBR sets the respective bit in the SRER.
6. When the SRER bit is set, the SBR MSS bit is set and a service request is generated when using the GPIB interface.

Synchronizing Execution

Almost all commands are executed in the order in which they are sent from the controller, and the execution of each command is completed in a short period of time. However, the following commands perform data analysis in another thread, and another command can thus be executed concurrently:

- INITiate commands
- READ commands
- [:SENSe]:REANalyze

These commands are designed so that the next command to be sent is executed without waiting for the previous command to be completed. In some cases, a process executed by another command must first be completed before these commands can be executed; in other cases, these commands must be completed before the next command is executed.

You have two options to achieve command synchronization:

- Using the status and event reporting function
- Using synchronizing commands

Using the Status and Event Reporting Function

In the following example, a :READ command is used to obtain the measurement results while the Operation Condition Register (OCR) is being used to provide synchronization.

```
:STATus:OPERation:NTRansition 16
// Set the filter of the OCR MEASuring bit
:STATus:OPERation:ENABle 16
// Enable the filter of the OCR MEASuring bit
*SRE 128 // Set the SRER OSS bit
:READ:SPECTrum:TRACe? // Obtain the measurement results
```

The command waits for generation of SRQ.

Using Synchronizing Commands

The IEEE-488.2 common commands include the following synchronizing commands:

```
*OPC
*OPC?
*WAI
```

Using the *OPC Command. The *OPC command sets the SESR OPC bit when all the operations for which it is waiting are completed. If the GPIB interface is in use, you can synchronize the execution by using this command together with the serial polling or service request function.

The following is a command sequence example:

```
*ESE 1      // Enable the ESER OPC bit
*SRE 32     // Enable the SRER ESB bit
:ABORt;INITiate:IMMediate;*OPC
              // Wait for SRQ to provide synchronization
```

Using the Query *OPC? The query *OPC? writes ASCII code “1” into the Output Queue when all operations for which it is waiting are completed. You can provide synchronization using the command string as the following example:

```
:ABORt;INITiate:IMMediate;*OPC?
```

The command waits until “1” is written into the Output Queue. When the command goes to the Output Queue to read the data, a time-out may occur before the data is written into the queue.

Using the *WAI Command. After the process of the preceding command is completed, the *WAI command begins to execute the process of the next command as the following example:

```
:ABORt;INITiate:IMMediate;*WAI
      // Wait for the *WAI process to provide synchronization
```


Error Messages and Codes

Error codes with a negative value are SCPI standard error codes; errors with a positive value are unique to the RSA6100A Series Real-Time Spectrum Analyzers.

Event codes and messages can be obtained by using the queries : SYSTem:ERRor? and :SYSTem:ERRor:ALL? These are returned in the following format:

<event code>,"<event message>"

Command Errors

Command errors are returned when there is a syntax error in the command.

Table 3-8: Command errors

Error code	Error message
-100	command error
-101	invalid character
-102	syntax error
-103	invalid separator
-104	data type error
-105	GET not allowed
-108	parameter not allowed
-109	missing parameter
-110	command header error
-111	header separator error
-112	program mnemonic too long
-113	undefined header
-114	header suffix out of range
-120	numeric data error
-121	character
-123	exponent too large
-124	too many digits
-128	numeric data not allowed

Table 3-8: Command errors (Cont.)

Error code	Error message
-130	suffix error
-131	invalid suffix
-134	suffix too long
-138	suffix not allowed
-140	character data error
-141	invalid character data
-144	character data too long
-148	character data not allowed
-150	string data error
-151	invalid string data
-158	string data not allowed
-160	block data error
-161	invalid block data
-168	block data not allowed
-170	command expression error
-171	invalid expression
-178	expression data not allowed
-180	macro error
-181	invalid outside macro definition
-183	invalid inside macro definition
-184	macro parameter error

Execution Errors

These error codes are returned when an error is detected while a command is being executed.

Table 3-9: Execution errors

Error code	Error message
-200	execution error
-201	invalid while in local
-202	settings lost due to RTL

Table 3-9: Execution errors (Cont.)

Error code	Error message
-210	trigger error
-211	trigger ignored
-212	arm ignored
-213	init ignored
-214	trigger deadlock
-215	arm deadlock
-220	parameter error
-221	settings conflict
-222	data out of range
-223	too much data
-224	illegal parameter value
-225	out of memory
-226	lists not same length
-230	data corrupt or stale
-231	data questionable
-240	hardware error
-241	hardware missing
-250	mass storage error
-251	missing mass storage
-252	missing media
-253	corrupt media
-254	media full
-255	directory full
-256	FileName not found
-257	FileName error
-258	media protected
-260	execution expression error
-261	math error in expression
-270	execution macro error
-271	macro syntax error
-272	macro execution error
-273	illegal macro label
-274	execution macro parameter error

Table 3-9: Execution errors (Cont.)

Error code	Error message
-275	macro definition too long
-276	macro recursion error
-277	macro redefinition not allowed
-278	macro header not found
-280	program error
-281	cannot create program
-282	illegal program name
-283	illegal variable name
-284	program currently running
-285	program syntax error
-286	program runtime error

Device Specific Errors

These error codes are returned when an internal instrument error is detected. This type of error may indicate a hardware problem.

Table 3-10: Device specific errors

Error code	Error message
-300	device specific error
-310	system error
-311	memory error
-312	PUD memory lost
-313	calibration memory lost
-314	save/recall memory lost
-315	configuration memory lost
-330	self test failed
-350	queue overflow

Query Errors

These error codes are returned in response to an unanswered query.

Table 3-11: Query errors

Error code	Error message
-400	query error
-410	query interrupted
-420	query untermiated
-430	query deadlocked
-440	query untermiated after indefinite period

Device Errors

These error codes are unique to the RSA6100A Series. They are classified into three groups: global, measurement, and source conditions, as shown in Tables 3-12, 3-13, and 3-14, respectively.

Table 3-12: Device errors, global condition

Error code	Error message
100	setup error
101	disabled: data is from swept acquisition
102	disabled: swept settings; Acquire data while display is selected
103	acquisition bandwidth too small for current setup
104	can't get acquisition data record
105	can't open the requested display
106	analysis failure
107	analysis length was limited
108	analysis length too small for current setup
109	no math trace: unmatched trace lengths
110	analysis time was adjusted
111	not enough samples for current setup
112	can't replay. Data is from swept acquisition.
113	can't replay. Live data needed for swept settings.
114	recall error: setup not completely restored
115	recall failure: problem with file or file contents

Table 3- 12: Device errors, global condition (cont.)

Error code	Error message
116	save failure: file not saved
117	unexpected software error. Please cycle power and try again.
118	export failure: file not saved
119	export failure: unable to open results file for export. File not saved.

Table 3- 13: Device errors, measurement condition

Error code	Error message
1000	TDBW actual (TDBW: Time Domain Bandwidth)
1001	average transmit not available in volts units
1002	RBW increased to
1003	RBW limited by acquisition bandwidth to
1004	RBW conflict. Increase span or analysis length
1005	analysis stopped: ambiguous pulse shape
1006	setup error: Phase measurement location
1007	no pulses found
1008	no FFT (not all pulses have results)
1009	no burst detected

Table 3- 14: Device errors, source condition

Error code	Error message
2000	data acquired during RF ADC overrange
2001	(internal use only)
2002	(internal use only)
2003	preamp not specified for frequencies > 3 GHz
2004	data acquired using preamp
2005	aligning
2006	not aligned
2007	data from unaligned instrument
2008	not calibrated
2009	data from uncalibrated instrument

Table 3- 14: Device errors, source condition (cont.)

Error code	Error message
2010	dither: manual control
2011	hardware failure - see Windows Event Viewer
2012	data acquired during hardware failure
2013	hardware failure detected by diagnostics
2014	data acquired during RF digital gain overflow
2015	locking to external frequency reference signal
2016	locked to external reference
2017	No_RF_Deck mode
2018	RF attenuator: manual control
2019	saving acquisition data
2020	restoring acquisition data
2021	simulated data
2022	disabled: data is from swept acquisition
2023	disabled: frequency mask trigger in use
2024	span > RF acquisition bandwidth
2025	RBW not valid for current acquisition bandwidth
2026	acquisition sampling parameters: manual control
2027	swept: RF trigger invalid for most signals
2028	external frequency reference signal not valid. Using internal reference.
2029	unable to lock to external frequency reference. Using internal reference.
2030	data acquired during RF ADC overrange
2031	data acquired during RF digital gain overflow
2032	source factory error
2033	Alignment error. Please run alignment again. If the problem persists, contact your Tektronix Service Center.
2034	Operational error: unable to complete operation. Please try again. If the problem persists, contact your Tektronix Service Center. See Windows Event Viewer for error detail.
2035	Hardware error: unable to configure hardware. Please try again. If the problem persists, contact your Tektronix Service Center. See Windows Event Viewer for error detail.
2036	Shutting down - internal temperature is too high. Check fans and airflow. If the problem persists, contact your Tektronix Service Center.
2037	Hardware error detected. To clear error, exit and restart the application. If the problem persists, contact your Tektronix Service Center.



Appendices


Appendix A: Character Charts

The ASCII and GPIB code chart is shown in Table A-1 on page A-2.

Table A-1: ASCII & GPIB code chart

B7 B6 B5 BITS B4 B3 B2 B1	0 0 0		0 0 1		0 1 0		0 1 1		1 0 0		1 0 1		1 1 0		1 1 1	
	CONTROL				NUMBERS SYMBOLS				UPPER CASE				LOWER CASE			
0 0 0 0	0 NUL	20 DLE	40 SP	60 0	100 @	120 P	140 ,	160 p	0 0	20 0	40 0	60 0	80 0	100 0	120 0	140 0
0 0 0 1	1 SOH	21 DC1	41 !	61 1	101 A	121 Q	141 a	161 q	1 1	21 1	41 1	61 1	81 1	101 1	121 1	141 1
0 0 1 0	2 STX	22 DC2	42 "	62 2	102 B	122 R	142 b	162 r	2 2	22 2	42 2	62 2	82 2	102 2	122 2	142 2
0 0 1 1	3 ETX	23 DC3	43 #	63 3	103 C	123 S	143 c	163 s	3 3	23 3	43 3	63 3	83 3	103 3	123 3	143 3
0 1 0 0	4 EOT	24 DC4	44 \$	64 4	104 D	124 T	144 d	164 t	4 4	24 4	44 4	64 4	84 4	104 4	124 4	144 4
0 1 0 1	5 ENQ	25 NAK	45 %	65 5	105 E	125 U	145 e	165 u	5 5	25 5	45 5	65 5	85 5	105 5	125 5	145 5
0 1 1 0	6 ACK	26 SYN	46 &	66 6	106 F	126 V	146 f	166 v	6 6	26 6	46 6	66 6	86 6	106 6	126 6	146 6
0 1 1 1	7 BEL	27 ETB	47 ,	67 7	107 G	127 W	147 g	167 w	7 7	27 7	47 7	67 7	87 7	107 7	127 7	147 7
1 0 0 0	10 BS	30 CAN	50 (70 8	110 H	130 X	150 h	170 x	8 8	30 8	50 8	70 8	90 8	110 8	130 8	150 8
1 0 0 1	11 HT	31 EM	51)	71 9	111 I	131 Y	151 i	171 y	9 9	31 9	51 9	71 9	91 9	111 9	131 9	151 9
1 0 1 0	12 LF	32 SUB	52 *	72 :	112 J	132 Z	152 j	172 z	10 A	32 1A	52 2A	72 3A	92 4A	112 5A	132 6A	152 7A
1 0 1 1	13 VT	33 ESC	53 +	73 ;	113 K	133 [153 k	173 {	11 B	33 1B	53 2B	73 3B	93 4B	113 5B	133 6B	153 7B
1 1 0 0	14 FF	34 FS	54 ,	74 <	114 L	134 \ 	154 l	174 	12 C	34 1C	54 2C	74 3C	94 4C	114 5C	134 6C	154 7C
1 1 0 1	15 CR	35 GS	55 -	75 =	115 M	135]	155 m	175 }	13 D	35 1D	55 2D	75 3D	95 4D	115 5D	135 6D	155 7D
1 1 1 0	16 SO	36 RS	56 .	76 >	116 N	136 ^	156 n	176 ~	14 E	36 1E	56 2E	76 3E	96 4E	116 5E	136 6E	156 7E
1 1 1 1	17 SI	37 US	57 /	77 ?	117 O	137 - 	157 o	177 RUBOUT (DEL)	15 F	37 1F	57 2F	77 3F	97 4F	117 5F	137 6F	157 7F
	ADDRESSED COMMANDS		UNIVERSAL COMMANDS		LISTEN ADDRESSES				TALK ADDRESSES				SECONDARY ADDRESSES OR COMMANDS			

KEY



Tektronix

REF: ANSI STD X3.4-1977
 IEEE STD 488.1-1987
 ISO STD 646-2973

Appendix B: GPIB Interface Specification

This appendix lists and describes the GPIB functions and messages the instrument can implement.

Interface Functions

Table B-1 lists the GPIB interface functions this instrument implements. Each function is briefly described on page B-2.

Table B-1: GPIB interface function implementation

Interface function	Implemented subset	Capability
Source Handshake (SH)	SH1	Complete
Acceptor Handshake (AH)	AH1	Complete
Talker (T)	T6	Basic Talker, Serial Poll Unaddress if my-listen-address (MLA) No Talk Only mode
Listener (L)	L4	Basic Listener Unaddress if my talk address (MTA) No Listen Only mode
Service Request (SR)	SR1	Complete
Remote/Local (RL)	RL0	None
Parallel Poll (PP)	PP0	None
Device Clear (DC)	DC1	Complete
Device Trigger (DT)	DT0	None
Controller (C)	C0	None
Electrical Interface	E2	Three-state driver

- Source Handshake (SH). Enables a talking device to support the coordination of data transfer. The SH function controls the initiation and termination of data byte transfers.
- Acceptor Handshake (AH). Enables a listening device to coordinate data reception. The AH function delays data transfer initiation or termination until the listening device is ready to receive the next data byte.
- Talker (T). Enables a device to send device-dependent data over the interface. This capability is available only when the device is addressed to talk, and uses a one-byte address.
- Listener (L). Enables a device to receive device-dependent data over the interface. This capability is available only when the device is addressed to listen, and uses a one-byte address.
- Service Request (SR). Enables a device to assert an SRQ (Service Request) line to notify the controller when it requires service.
- Remote/Local (RL). Enables a device to respond to both the GTL (Go To Local) and LLO (Local Lock Out) interface messages.
- Parallel Poll (PP). Enables a device to respond to the following interface messages: PPC, PPD, PPE, and PPU, as well as to send out a status message when the ATN (Attention) and EOI (End or Identify) lines are asserted simultaneously.
- Device Clear (DC). Enables a device to be cleared or initialized, either individually, or as part of a group of devices.
- Device Trigger (DT). Enables a device to respond to the GET (Group Execute Trigger) interface message when acting as a listener.
- Controller (C). Enables a device that has this capability to send its address, universal commands, and addressed commands to other devices over the interface.
- Electrical Interface (E). Identifies the electrical interface driver type. The notation E1 means the electrical interface uses open collector drivers, E2 means the electrical interface uses three-state drivers.

Interface Messages

Table B-2 shows the standard interface messages that are supported by the analyzer.

Table B-2: Standard interface messages

Message	Type	Implemented
Device Clear (DCL)	UC	Yes
Local Lockout (LLO)	UC	No
Serial Poll Disable (SPD)	UC	Yes
Serial Poll Enable (SPE)	UC	Yes
Parallel Poll Unconfigure (PPU)	UC	No
Go To Local (GTL)	AC	Yes
Selected Device Clear (SDC)	AC	Yes
Group Execute Trigger (GET)	AC	No
Take Control (TCT)	AC	No
Parallel Poll Configure (PPC)	AC	No

UC: Universal command; AC: Address command

- Device Clear (DCL). Will clear (initialize) all devices on the bus that have a device clear function, whether or not the controller has addressed them.
- Local Lockout (LLO). Disables the return to local function.
- Serial Poll Disable (SPD). Changes all devices on the bus from the serial poll state to the normal operating state.
- Serial Poll Enable (SPE). Puts all bus devices that have a service request function into the serial poll enabled state. In this state, each device sends the controller its status byte, instead of its normal output, after the device receives its talk address on the data lines. This function may be used to determine which device sent a service request.
- Go To Local (GTL). Causes the listen-addressed device to switch from remote to local (front-panel) control.
- Select Device Clear (SDC). Clears or initializes all listen-addressed devices.
- Group Execute Trigger (GET). Triggers all applicable devices and causes them to initiate their programmed actions.
- Take Control (TCT). Allows the controller in charge to pass control of the bus to another controller on the bus.
- Parallel Poll Configure (PPC). Causes the listen-addressed device to respond to the secondary commands Parallel Poll Enable (PPE) and Parallel Poll Disable (PPD), which are placed on the bus following the PPC command. PPE enables a device with parallel poll capability to respond on a particular data line. PPD disables the device from responding to the parallel poll.

Appendix C: Factory Initialization Settings

The factory initialization settings provide a known state for the analyzer. The *RST command returns the instrument settings to the factory defaults. Factory initialization sets values as shown in Table C-1 through C-11.

Table C- 1: Factory initialization settings, IEEE common commands

Header	Default value
*ESE	0
*OPC	0
*SRE	0

Table C- 2: Factory initialization settings, CALibration commands

Header	Default value
:CALibration:AUTO	ON
:CALibration:CORRection:EXTErnal:EDIT<n>:LABel	Ext Gain Table n
:CALibration:CORRection:EXTErnal:EDIT<n>:STATe	OFF
:CALibration:CORRection:EXTErnal:GAIN[:MAGNitude]	30 dB
:CALibration:CORRection:EXTErnal:GAIN:STATe	OFF
:CALibration:CORRection:EXTErnal:PROBE:STATe	OFF

Table C- 3: Factory initialization settings, CALCulate commands

Header	Default value
:CALCulate basic command subgroup	
:CALCulate:MARKer:MODE	ABSolute
:CALCulate:MARKer:PEAK:EXCursion	6 dB
:CALCulate:MARKer:PEAK:THReshold	-150 dBm
:CALCulate:SEARch:LIMit:MATCH:BEEP[:STATe]	OFF
:CALCulate:SEARch:LIMit:MATCH:SACQuire[:STATe]	OFF
:CALCulate:SEARch:LIMit:MATCH:SDATa[:STATe]	OFF
:CALCulate:SEARch:LIMit:MATCH:SPICture[:STATe]	OFF
:CALCulate:SEARch:LIMit:MATCH:STRace[:STATe]	OFF

Table C-3: Factory initialization settings, CALCulate commands (Cont.)

Header	Default value
:CALCulate:SEARch:LIMit:OPERation	GT
:CALCulate:SEARch:LIMit:OPERation:FEED	"Spectrum", "Trace 1"
:CALCulate:SEARch:LIMit:OPERation:SLIMit	-20 dBm
:CALCulate:SEARch:LIMit:STATe	OFF
:CALCulate:DPSA subgroup	
:CALCulate:DPSA:MARKer<x>:TRACe	TRACE1
:CALCulate:SPECTrum subgroup	
:CALCulate:SPECTrum:MARKer<x>:TRACe	TRACE1

Table C-4: Factory initialization settings, DISPlay commands

Header	Default value
:DISPlay:ACPower subgroup	
:DISPlay:ACPower:MARKer:SHOW:STATe	ON
:DISPlay:ACPower:PLEVel:SHOW:STATe	ON
:DISPlay:ACPower:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:ACPower:X[:SCALe]	13.84 MHz
:DISPlay:ACPower:X[:SCALe]:OFFSet	1.5 GHz
:DISPlay:ACPower:Y[:SCALe]	100 dB
:DISPlay:ACPower:Y[:SCALe]:OFFSet	0
:DISPlay:AVTime subgroup	
:DISPlay:AVTime:MARKer:SHOW:STATe	ON
:DISPlay:AVTime:TRIGger:LEVel:STATe	ON
:DISPlay:AVTime:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:AVTime:X[:SCALe]:AUTO:STATe	ON
:DISPlay:AVTime:X[:SCALe]:OFFSet	0
:DISPlay:AVTime:Y[:SCALe]:FULL	100 dB
:DISPlay:AVTime:Y[:SCALe]:OFFSet	0
:DISPlay:CONSte subgroup	
:DISPlay:CONSte:WINDow:TRACe:GRATicule:GRID:STATe	ON

Table C- 4: Factory initialization settings, DISPlay commands (Cont.)

Header	Default value
:DISPlay:DDEMod subgroup	
:DISPlay:DDEMod:RADix	BiNary
:DISPlay:DDEMod:X[:SCALe]	128 symbols
:DISPlay:DDEMod:X[:SCALe]:AUTO:STATe	ON
:DISPlay:DDEMod:X[:SCALe]:OFFSet	-1 symbol
:DISPlay:DPSA subgroup	
:DISPlay:DPSA:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:DPSA:Y[:SCALe]:PDIVision	10 dB/div
:DISPlay:EVM subgroup	
:DISPlay:EVM:Y[:SCALe]	1%
:DISPlay:EVM:Y[:SCALe]:OFFSet	0
:DISPlay:FVTime subgroup	
:DISPlay:FVTime:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:FVTime:X[:SCALe]:AUTO:STATe	ON
:DISPlay:FVTime:X[:SCALe]:OFFSet	0
:DISPlay:FVTime:Y[:SCALe]	10 Hz
:DISPlay:FVTime:Y[:SCALe]:OFFSet	0
:DISPlay:GENeral subgroup	
:DISPlay:GENeral:MEASview:SElect	SPECTrum
:DISPlay:IQVTime subgroup	
:DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:IQVTime:X[:SCALe]:AUTO:STATe	ON
:DISPlay:IQVTime:X[:SCALe]:OFFSet	0
:DISPlay:IQVTime:Y[:SCALe]	1 μ V
:DISPlay:IQVTime:Y[:SCALe]:OFFSet	0
:DISPlay:MCPower subgroup	
:DISPlay:MCPower:MARKer:SHOW:STATe	ON
:DISPlay:MCPower:PLEVel:SHOW:STATe	ON
:DISPlay:MCPower:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:MCPower:X[:SCALe]	38.84 MHz
:DISPlay:MCPower:X[:SCALe]:OFFSet	1.5 GHz
:DISPlay:MCPower:Y[:SCALe]	100 dB
:DISPlay:MCPower:Y[:SCALe]:OFFSet	0

Table C-4: Factory initialization settings, DISPlay commands (Cont.)

Header	Default value
:DISPlay:MERRor subgroup	
:DISPlay:MERRor:Y[:SCALe]	1%
:DISPlay:MERRor:Y[:SCALe]:OFFSet	0
:DISPlay:OBWidth subgroup	
:DISPlay:OBWidth:MARKer:SHOW:STATe	ON
:DISPlay:OBWidth:SELected:BANDwidth	OBWidth
:DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:OBWidth:X[:SCALe]:OFFSet	0
:DISPlay:OBWidth:Y[:SCALe]	100 dB
:DISPlay:OBWidth:Y[:SCALe]:OFFSet	0
:DISPlay:PERRor subgroup	
:DISPlay:PERRor:Y[:SCALe]	1°
:DISPlay:PERRor:Y[:SCALe]:OFFSet	0
:DISPlay:PHVTime subgroup	
:DISPlay:PHVTime:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:PHVTime:X[:SCALe]:AUTO:STATe	ON
:DISPlay:PHVTime:X[:SCALe]:OFFSet	0
:DISPlay:PHVTime:Y[:SCALe]	1°
:DISPlay:PHVTime:Y[:SCALe]:AXIS	MODulopi
:DISPlay:PHVTime:Y[:SCALe]:AXIS:REFerence	0
:DISPlay:PHVTime:Y[:SCALe]:OFFSet	0
:DISPlay:PULSe subgroup	
:DISPlay:PULSe:RESult:ATX	OFF
:DISPlay:PULSe:RESult:AVERage	ON
:DISPlay:PULSe:RESult:DROop	OFF
:DISPlay:PULSe:RESult:DUTPct	OFF
:DISPlay:PULSe:RESult:DUTRatio	OFF
:DISPlay:PULSe:RESult:FALL	OFF
:DISPlay:PULSe:RESult:FRDeviation	OFF
:DISPlay:PULSe:RESult:MFRerror	OFF
:DISPlay:PULSe:RESult:MPHerror	OFF
:DISPlay:PULSe:RESult:PHDeviation	OFF
:DISPlay:PULSe:RESult:PPFRequency	OFF

Table C-4: Factory initialization settings, DISPlay commands (Cont.)

Header	Default value
:DISPlay:PULSe:RESult:PPOWer	OFF
:DISPlay:PULSe:RESult:PPPHase	OFF
:DISPlay:PULSe:RESult:RIPPlE	OFF
:DISPlay:PULSe:RESult:RMSFreqerror	OFF
:DISPlay:PULSe:RESult:RMSPherror	OFF
:DISPlay:PULSe:RESult:RRATe	OFF
:DISPlay:PULSe:RESult:RINTerval	OFF
:DISPlay:PULSe:RESult:RISE	OFF
:DISPlay:PULSe:RESult:TIME	OFF
:DISPlay:PULSe:RESult:WIDTh	OFF
:DISPlay:PULSeSElect:NUMBer	0
:DISPlay:PULSeSElect:RESult	AVERage
:DISPlay:PULSe:STATistics:MARKer:SHOW:STATe	ON
:DISPlay:PULSe:STATistics:PLOT	TREND
:DISPlay:PULSe:STATistics:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:PULSe:STATistics:X[:SCALE]:NUMBer	1
:DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet	0
:DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet	0
:DISPlay:PULSe:STATistics:Y[:SCALE]:FULL	100 dB
:DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet	0
:DISPlay:PULSe:TRACe:MARKer:SHOW:STATe	ON
:DISPlay:PULSe:TRACe:POINt:SHOW	ON
:DISPlay:PULSe:TRACe:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:PULSe:TRACe:X[:SCALE]:FULL	SElected
:DISPlay:PULSe:TRACe:X[:SCALE]:OFFSet	0
:DISPlay:PULSe:TRACe:X[:SCALE]:PDIVision	10 μ s
:DISPlay:PULSe:TRACe:Y[:SCALE]:FULL	100 dB
:DISPlay:PULSe:TRACe:Y[:SCALE]:OFFSet	0
:DISPlay:SGRam subgroup	
:DISPlay:SGRam:FREQuency:OFFSet	1.5 GHz
:DISPlay:SGRam:FREQuency:SCALE	40 MHz

Table C-4: Factory initialization settings, DISPlay commands (Cont.)

Header	Default value
:DISPlay:SGRam:TIME:OFFSet	0
:DISPlay:SGRam:TIME:OVERlap	ON
:DISPlay:SGRam:TIME:SCAlE	0
:DISPlay:SPECTrum subgroup	
:DISPlay:SPECTrum:MARKer:NOISe:MODE	OFF
:DISPlay:SPECTrum:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:SPECTrum:Y[:SCAlE]:PDIVision	10 dB/div
:DISPlay:TOVerview subgroup	
:DISPlay:TOVerview:WINDow:TRACe:GRATicule:GRID:STATe	ON
:DISPlay:TOVerview:X[:SCAlE]:OFFSet	0
:DISPlay:TOVerview:Y[:SCAlE]	100 dB
:DISPlay:TOVerview:Y[:SCAlE]:OFFSet	0

Table C-5: Factory initialization settings, INITiate commands

Header	Default value
:INITiate:CONTinuous	ON

Table C-6: Factory initialization settings, INPut commands

Header	Default value
:INPut[:RF]:ATTenuation	20 dB
:INPut[:RF]:ATTenuation:AUTO	ON
:INPut[:RF]:GAIN:STATe	OFF
:INPut:MLEVel[:RLEVel]	0 dBm

Table C-7: Factory initialization settings, OUTPut commands

Header	Default value
:OUTPut:NOISe[:STATe]	OFF
:OUTPut:IF[:STATe] (Option 05 only)	OFF
:OUTPut:IF:BANDwidth[:BWIDth] (Option 05 only)	FLATtop
:OUTPut:IQ[:STATe] (Option 05 only)	OFF

Table C-8: Factory initialization settings, SENSE commands

Header	Default value
[[:SENSe]] basic command subgroup	
[[:SENSe]]:ACQuisition:FFRame:Limit	1
[[:SENSe]]:ACQuisition:FFRame:STATe	OFF
[[:SENSe]]:ACQuisition:MODE(?)	AUTO
[[:SENSe]]:ANALysis:ADVanced:DITHer	AUTO
[[:SENSe]]:ANALysis:LENGth	7.44 μ s
[[:SENSe]]:ANALysis:LENGth:AUTO	ON
[[:SENSe]]:ANALysis:REFerence	ACQSTART
[[:SENSe]]:ANALysis:STARt	0
[[:SENSe]]:ANALysis:STARt:AUTO	ON
[[:SENSe]]:POWer:UNITs	DBM
[[:SENSe]]:ROSCillator:SOURce	INTernal
[[:SENSe]]:SPECtrum:LENGth	7.44 μ s
[[:SENSe]]:SPECtrum:LENGth:AUTO	ON
[[:SENSe]]:SPECtrum:STARt	0
[[:SENSe]]:SPECtrum:TIME:MODE	COMMOn
[[:SENSe]]:ACPower subgroup	
[[:SENSe]]:ACPower:AVERage	OFF
[[:SENSe]]:ACPower:AVERage:COUNt	10
[[:SENSe]]:ACPower:BANDwidth[:BWIDth[:RESolution]]	30 kHz
[[:SENSe]]:ACPower:BANDwidth[:BWIDth[:RESolution]]:AUTO	ON
[[:SENSe]]:ACPower:CHANnel:BANDwidth[:BWIDth]	3.84 MHz
[[:SENSe]]:ACPower:CHANnel:FILTer	RRCosine

Table C-8: Factory initialization settings, SENSE commands (Cont.)

Header	Default value
[SENSe]:ACPower:CHANnel:PAIRs	1
[SENSe]:ACPower:CHANnel:SPACing	5 MHz
[SENSe]:ACPower:CHIPrate	3.84 MHz
[SENSe]:ACPower:FREQuency:STEP	1 MHz
[SENSe]:ACPower:FREQuency:STEP:AUTO	ON
[SENSe]:ACPower:NFLoor:STATe	OFF
[SENSe]:ACPower:OPTimize:SPAN	DRANge
[SENSe]:ACPower:RRCRolloff	0.22
[SENSe]:AVTime subgroup	
[SENSe]:AVTime:BANDwith :BWIDth	1 MHz
[SENSe]:AVTime:MAXTracepoints	HUNDredk
[SENSe]:AVTime:METHod	SPAN
[SENSe]:AVTime:SPAN	40 MHz
[SENSe]:CCDF subgroup	
[SENSe]:CCDF:BANDwidth :BWIDth	40 MHz
[SENSe]:CCDF:TIME:AUTO	ON
[SENSe]:CCDF:TIME:TYPE	SINGLe
[SENSe]:DDEMod subgroup	
[SENSe]:DDEMod:ANALysis:LENGth	128 symbols
[SENSe]:DDEMod:ANALysis:LENGth:AUTO	ON
[SENSe]:DDEMod:BURSt:DETECT	OFF
[SENSe]:DDEMod:BURSt:THREShold	-20 dBc
[SENSe]:DDEMod:CARRier:OFFSet	0
[SENSe]:DDEMod:FILTer:ALPHa	0.22
[SENSe]:DDEMod:FILTer:MEASurement	RRCosine
[SENSe]:DDEMod:FILTer:REFerence	RCOSine
[SENSe]:DDEMod:MAGNitude:NORMALize	RSYMBOL
[SENSe]:DDEMod:MODulation:TYPE	QPSK
[SENSe]:DDEMod:SRATe	3.84 MHz
[SENSe]:DDEMod:SWAP:IQ	OFF

Table C-8: Factory initialization settings, SENSE commands (Cont.)

Header	Default value
[[:SENSe]:DDEMod:SYMBOL:POINTs	FOUR
[[:SENSe]:DDEMod:SYNCh:WORD	OFF
[[:SENSe]:DDEMod:SYNCh:WORD:SYMBOL	#10
[[:SENSe]:DDEMod:TIME:UNITs	SYMBOLs
[[:SENSe]:DPSA subgroup	
[[:SENSe]:DPSA:AUDio:DEMod:GAIN	3
[[:SENSe]:DPSA:AUDio:DEMod:RXBWidth	30 kHz
[[:SENSe]:DPSA:AUDio:DEMod:STATe	OFF
[[:SENSe]:DPSA:AUDio:DEMod:TUNE	SMARker
[[:SENSe]:DPSA:AUDio:DEMod:TYPE	FM
[[:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]	400 kHz
[[:SENSe]:DPSA:BANDwidth[:BWIDth[:RESolution]:AUTO	ON
[[:SENSe]:DPSA:COLor	TEMPerature
[[:SENSe]:DPSA:COLor:MAXimum	100%
[[:SENSe]:DPSA:COLor:MINimum	0%
[[:SENSe]:DPSA:FREQuency:CENTer	1.5 GHz
[[:SENSe]:DPSA:FREQuency:SPAN	40 MHz
[[:SENSe]:DPSA:FREQuency:START	1.48 GHz
[[:SENSe]:DPSA:FREQuency:STEP	2 MHz
[[:SENSe]:DPSA:FREQuency:STEP:AUTO	ON
[[:SENSe]:DPSA:FREQuency:STOP	1.52 GHz
[[:SENSe]:FVTime subgroup	
[[:SENSe]:FVTime:FREQuency:CENTer	1.5 GHz
[[:SENSe]:FVTime:FREQuency:SPAN	40 MHz
[[:SENSe]:FVTime:FREQuency:START	1.48 GHz
[[:SENSe]:FVTime:FREQuency:STEP	2 MHz
[[:SENSe]:FVTime:FREQuency:STEP:AUTO	ON
[[:SENSe]:FVTime:FREQuency:STOP	1.52 GHz
[[:SENSe]:FVTime:MAXTracepoints	HUNDredk
[[:SENSe]:IQVTime subgroup	
[[:SENSe]:IQVTime:FREQuency:CENTer	1.5 GHz
[[:SENSe]:IQVTime:FREQuency:SPAN	40 MHz
[[:SENSe]:IQVTime:FREQuency:START	1.48 GHz

Table C-8: Factory initialization settings, SENSE commands (Cont.)

Header	Default value
[SENSe]:IQVTime:FREQuency:STEP	2 MHz
[SENSe]:IQVTime:FREQuency:STEP:AUTO	ON
[SENSe]:IQVTime:FREQuency:STOP	1.52 GHz
[SENSe]:IQVTime:MAXTracepoints	HUNDredk
[SENSe]:MCPower subgroup	
[SENSe]:MCPower:AVERAge	OFF
[SENSe]:MCPower:AVERAge:COUNT	10
[SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]	30 kHz
[SENSe]:MCPower:BANDwidth[:BWIDth[:RESolution]:AUTO	ON
[SENSe]:MCPower:CHANnel:BANDwidth	3.84 MHz
[SENSe]:MCPower:CHANnel:FILTer	RRCosine
[SENSe]:MCPower:CHANnel:MAIN:BANDwidth[:BWIDth	3.84 MHz
[SENSe]:MCPower:CHANnel:MAIN:COUNT	4
[SENSe]:MCPower:CHANnel:MAIN:INACTive	NONE
[SENSe]:MCPower:CHANnel:MAIN:SPACing	5 MHz
[SENSe]:MCPower:CHIPRate	3.84 MHz
[SENSe]:MCPower:FREQuency:STEP	2 MHz
[SENSe]:MCPower:FREQuency:STEP:AUTO	ON
[SENSe]:MCPower:NFLoor:STATe	OFF
[SENSe]:MCPower:OPTimize:SPAN	DRANge
[SENSe]:MCPower:RRCRolloff	0.22
[SENSe]:OBWidth subgroup	
[SENSe]:OBWidth:AVERAge	OFF
[SENSe]:OBWidth:AVERAge:COUNT	10
[SENSe]:OBWidth:BANDwidth[:BWIDth:MEASurement	10 MHz
[SENSe]:OBWidth:BANDwidth[:BWIDth[:RESolution]	33 kHz
[SENSe]:OBWidth:BANDwidth[:BWIDth[:RESolution]:AUTO	ON
[SENSe]:OBWidth:FREQuency:CENTer	1.5 GHz
[SENSe]:OBWidth:FREQuency:STEP	2 MHz
[SENSe]:OBWidth:FREQuency:STEP:AUTO	ON
[SENSe]:OBWidth:PERCent	99%
[SENSe]:OBWidth:XDBLevel	-26 dB

Table C-8: Factory initialization settings, SENSE commands (Cont.)

Header	Default value
[[:SENSe]:PHVTime subgroup	
[[:SENSe]:PHVTime:FREQuency:CENTer	1.5 GHz
[[:SENSe]:PHVTime:FREQuency:SPAN	40 MHz
[[:SENSe]:PHVTime:FREQuency:START	1.48 GHz
[[:SENSe]:PHVTime:FREQuency:STEP	2 MHz
[[:SENSe]:PHVTime:FREQuency:STEP:AUTO	ON
[[:SENSe]:PHVTime:FREQuency:STOP	1.52 GHz
[[:SENSe]:PHVTime:MAXTracepoints	HUNDredk
[[:SENSe]:PULSe subgroup	
[[:SENSe]:PULSe:ANALyze:LEVel	VOLTage
[[:SENSe]:PULSe:ANALyze:LEVel:FIFTy	VOLTage
[[:SENSe]:PULSe:ANALyze:LEVel:HUNDred	AVERage
[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:AUTO	ON
[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:START	0
[[:SENSe]:PULSe:ANALyze:MEASurement:TIME:STOP	0
[[:SENSe]:PULSe:ANALyze:PMLocation	500 ns
[[:SENSe]:PULSe:ANALyze:POINt:LOCation	AVERage
[[:SENSe]:PULSe:ANALyze:RFALI	WIDE
[[:SENSe]:PULSe:ANALyze:RIPple	50%
[[:SENSe]:PULSe:CARRier:OFFSet	0
[[:SENSe]:PULSe:CARRier:SEARch	AUTO
[[:SENSe]:PULSe:DETEct:MEASurement	OFF
[[:SENSe]:PULSe:DETEct:NUMBer	100
[[:SENSe]:PULSe:DETEct:POWer[:THReshold]	-10 dBc
[[:SENSe]:PULSe:DETEct:TIME[:THReshold]	1 ns
[[:SENSe]:PULSe:FILTer:BANDwidth[:BWIDth]	20 MHz (Standard) 60 MHz (Option 110)
[[:SENSe]:PULSe:FILTer:MEASurement	GAUSSian
[[:SENSe]:PULSe:FREFerence:AUTO	ON
[[:SENSe]:PULSe:FREFerence:CHIRpbw	1 MHz
[[:SENSe]:PULSe:FREFerence:OFFSet	0

Table C-8: Factory initialization settings, SENSE commands (Cont.)

Header	Default value
[.SENSe]:PULSe:MODulation:TYPE	CWConst
[.SENSe]:PULSe:SIGNAL:TYPE	CWConst
[.SENSe]:SGRam subgroup	
[.SENSe]:SGRam:BANDwidth[:BWIDth:OPTimization]	AUTO
[.SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]]	300 kHz
[.SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:AUTO]	ON
[.SENSe]:SGRam:BANDwidth[:BWIDth[:RESolution]:MODE]	ON
[.SENSe]:SGRam:COLor	TEMPerature
[.SENSe]:SGRam:COLor:MAX	0 dBm
[.SENSe]:SGRam:COLor:MIN	-100 dBm
[.SENSe]:SGRam:FFT:WINDow	KAISer
[.SENSe]:SGRam:FREQuency:CENTer	1.5 GHz
[.SENSe]:SGRam:FREQuency:SPAN	40 MHz
[.SENSe]:SGRam:FREQuency:SPAN:BANDwidth[:RESolution]:RATio	100
[.SENSe]:SGRam:FREQuency:STARt	1.48 GHz
[.SENSe]:SGRam:FREQuency:STEP	2 MHz
[.SENSe]:SGRam:FREQuency:STEP:AUTO	ON
[.SENSe]:SGRam:FREQuency:STOP	1.52 GHz
[.SENSe]:SPECtrum subgroup	
[.SENSe]:SPECtrum:BANDwidth[:BWIDth:OPTimization]	AUTO
[.SENSe]:SPECtrum:BANDwidth[:BWIDth[:RESolution]]	300 kHz
[.SENSe]:SPECtrum:BANDwidth[:BWIDth[:RESolution]:AUTO]	ON
[.SENSe]:SPECtrum:BANDwidth[:BWIDth[:RESolution]:MODE]	ON
[.SENSe]:SPECtrum:FFT:WINDow	KAISer
[.SENSe]:SPECtrum:FREQuency:CENTer	1.5 GHz
[.SENSe]:SPECtrum:FREQuency:SPAN	40 MHz
[.SENSe]:SPECtrum:FREQuency:SPAN:BANDwidth[:RESolution]:RATio	100
[.SENSe]:SPECtrum:FREQuency:STARt	1.48 GHz
[.SENSe]:SPECtrum:FREQuency:STEP	2 MHz
[.SENSe]:SPECtrum:FREQuency:STEP:AUTO	ON
[.SENSe]:SPECtrum:FREQuency:STOP	1.52 GHz
[.SENSe]:SPECtrum:POINts:COUNT	P801

Table C-8: Factory initialization settings, SENSE commands (Cont.)

Header	Default value
[[:SENSe]:TOVerview subgroup	
[[:SENSe]:TOVerview:FREQuency:CENTer	1.5 GHz
[[:SENSe]:]TOVerview:MAXTracepoints	HUNDredk

Table C-9: Factory initialization settings, TRACe commands

Header	Default value
:TRACe<x>:AVTime subgroup	
:TRACe<x>:AVTime	<x>=1: ON <x>=2 to 4: OFF
:TRACe<x>:AVTime:AVERage:COUNT	10
:TRACe<x>:AVTime:COUNT	10
:TRACe<x>:AVTime:COUNT:ENABLE	ON
:TRACe<x>:AVTime:FREeze	OFF
:TRACe<x>:AVTime:FUNCTion	NORMal
:TRACe<x>:AVTime:LEFToperand	TRACE2
:TRACe<x>:AVTime:RIGHToperand	TRACE1
:TRACe<x>:CCDF subgroup	
:TRACe<x>:CCDF:FREeze	OFF
:TRACe<x>:CCDF:SHOW	x=1: ON x=2 and 3: OFF
:TRACe<x>:CCDF:X	3 dB
:TRACe<x>:CONSte subgroup	
:TRACe<x>:CONSte:MODE	VECTors
:TRACe<x>:DPSA subgroup	
:TRACe<x>:DPSA	x=1 and 5: ON x=2 to 4: OFF
:TRACe<x>:DPSA:AVERage:COUNT	10
:TRACe<x>:DPSA:COLor:INTensity	25 %
:TRACe5:DPSA:DOT:PERSistent	ON
:TRACe5:DPSA:DOT:PERSistent:TYPE	VARiable
:TRACe5:DPSA:DOT:PERSistent:VARiable	10
:TRACe<x>:DPSA:FREeze	OFF

Table C-9: Factory initialization settings, TRACe commands (Cont.)

Header	Default value
:TRACe<x>:DPSA:FUNCTION	NORMAL
:TRACe<x>:DPSA:LEFToperand	TRACE1
:TRACe<x>:DPSA:RIGHToperand	TRACE3
:TRACe:FVTime subgroup	
:TRACe:FVTime:COUNt	10
:TRACe:FVTime:COUNt:ENABle	ON
:TRACe:FVTime:FREeze	OFF
:TRACe:FVTime:FUNCTION	NORMAL
:TRACe:IQVTime subgroup	
:TRACe:IQVTime:COUNt	10
:TRACe:IQVTime:COUNt:ENABle	ON
:TRACe:IQVTime:ENABle:I	ON
:TRACe:IQVTime:ENABle:Q	ON
:TRACe:IQVTime:FREeze	OFF
:TRACe:IQVTime:FUNCTION	NORMAL
:TRACe:IQVTime:SELEct:I	ON
:TRACe:IQVTime:SELEct:Q	OFF
:TRACe:OBWidth subgroup	
:TRACe:OBW:MAXHold	OFF
:TRACe:PHVTime subgroup	
:TRACe:PHVTime:COUNt	10
:TRACe:PHVTime:COUNt:ENABle	ON
:TRACe:PHVTime:FREeze	OFF
:TRACe:PHVTime:FUNCTION	NORMAL
:TRACe<x>:SGRam subgroup	
:TRACe<x>:SGRam:DETEction	POSitive
:TRACe<x>:SGRam:FREeze	OFF
:TRACe<x>:SGRam:FUNCTION	NONE
:TRACe<x>:SGRam:FUNCTION:TIME	0.02 minutes
:TRACe<x>:SGRam:SELEct:LINE	0

Table C- 9: Factory initialization settings, TRACe commands (Cont.)

Header	Default value
:TRACe<x>:SPECTrum subgroup	
:TRACe<x>:SPECTrum	x=1: ON x=2 to 4: OFF
:TRACe<x>:SPECTrum:AVERage:COUNT	10
:TRACe<x>:SPECTrum:COUNT	10
:TRACe<x>:SPECTrum:COUNT:ENABLE	ON
:TRACe<x>:SPECTrum:DETEction	POSitive
:TRACe<x>:SPECTrum:FREeze	OFF
:TRACe<x>:SPECTrum:FUNCTion	NONE
:TRACe<x>:SPECTrum:LEFToperand	TRACE2
:TRACe<x>:SPECTrum:RIGHToperand	TRACE1

Table C- 10: Factory initialization settings, TRIGger commands

Header	Default value
:TRIGger[:SEQuence]:ADVanced:SWEep:MODE	OFF
:TRIGger[:SEQuence]:EVENT:EXTFront:IMPedance	5 k Ω
:TRIGger[:SEQuence]:EVENT:EXTFront:LEVel	1.6 V
:TRIGger[:SEQuence]:EVENT:EXTFront:SLOPe	RISe
:TRIGger[:SEQuence]:EVENT:GATed	HIGH
:TRIGger[:SEQuence]:EVENT:INPut:FMASK:VIOLation	FT
:TRIGger[:SEQuence]:EVENT:INPut:LEVel	-10 dBm
:TRIGger[:SEQuence]:EVENT:INPut:SLOPe	RISe
:TRIGger[:SEQuence]:EVENT:INPut:TDBWidth	1 MHz
:TRIGger[:SEQuence]:EVENT:INPut:TDBWidth:STATe	ON
:TRIGger[:SEQuence]:EVENT:INPut:TYPE	POWer
:TRIGger[:SEQuence]:EVENT:SOURce	INPut
:TRIGger[:SEQuence]:FORCed	OFF
:TRIGger[:SEQuence]:STATus	OFF
:TRIGger[:SEQuence]:TIme:DELay	0 s
:TRIGger[:SEQuence]:TIme:POSition	25%

Table C- 11: Factory initialization settings, UNIT commands

Header	Default value
:UNIT:POWer	dBm

Appendix D: SCPI Conformance Information

All commands for the RSA6100A Series analyzers are based on SCPI Version 1999.0. Table D-1 lists the commands that are defined in the SCPI 1999.0 Standard. The other commands not listed in the table are not defined in the SCPI 1999.0 Standard.

Table D- 1: SCPI 1999.0-defined commands

Command group	Command
IEEE common	*CAL?
	*CLS
	*ESE
	*ESR?
	*IDN?
	*OPC
	*OPT?
	*RST
	*SRE
	*STB?
	*TRG
	*WAI
ABORt	:ABORt
INITiate	:INITiate :CONTInuous [:IMMediate]
STATus	:STATus :OPERation :CONDition? :ENABle [:EVENT]? :NTRansition :PTRansition :PRESet :QUESTionable :CONDition? :ENABle [:EVENT]?

Table D- 1: SCPI 1999.0-defined commands (Cont.)

Command group	Command				
				:NTRansition	
				:PTRansition	
SYSTem	:SYSTem	:COMMunicate	:GPIB	[:SELF]	:ADDRess
		:DATE			
		:ERRor	:ALL?		
			:CODE	:ALL?	
				[:NEXT]?	
			:COUNT?		
			[:NEXT]?		
		:PRESet			
		:TIME			
		:VERSion?			
UNIT	:UNIT	:POWER			



Glossary and Index

Glossary

ASCII

Acronym for the American Standard Code for Information Interchange. Controllers transmit commands to the instrument using ASCII character encoding.

ASK

Acronym for Amplitude Shift Keying. The process, or result of a process, in which the amplitude of the carrier is varied in accordance with the state of a digital input signal.

BNF (Backus-Naur Form)

A standard notation system for command syntax diagrams. The syntax diagrams in this manual use BNF notation.

Controller

A computer or other device that sends commands to and accepts responses from the analyzer.

EVM (Error Vector Magnitude)

The magnitude of an error of an actual signal relative to an ideal signal in a constellation display.

GPIB

Acronym for General Purpose Interface Bus, the common name for the communications interface system defined in IEEE Std 488.

IEEE

Acronym for the Institute for Electrical and Electronic Engineers.

IS95

Acronym for Interim Standard-95. The standards name for first-generation CDMA cellphone technology.

Modulation

The process of varying some characteristic of a signal with a second signal.

PSK

Acronym for Phase Shift Keying. The process, or result of a process, in which the carrier phase is varied discretely in accordance with a digital code.

QAM

Acronym for Quadrature Amplitude Modulation. The process, or result of a process, in which the amplitude and phase of the carrier are varied concurrently by synthesizing two orthogonal ASK waves (see ASK).

Index

A

Abbreviations, commands, queries, and parameters, 2-5

:ABORt, 2-67

ABORt command group, 2-14

ABORt commands, 2-67

ACPR, measurement mode, 2-12

Arguments, parameters, 2-4

B

Backus-Naur Form, 2-1

BNF (Backus-Naur form), 2-1

C

*CAL, 2-56

:CALCulate basic command subgroup, 2-71

CALCulate command group, 2-15

CALCulate commands, 2-69

:CALCulate:ACPower subgroup, 2-86

:CALCulate:ACPower:MARKer<x>:DELtA:X?, 2-87

:CALCulate:ACPower:MARKer<x>:DELtA:Y?, 2-87

:CALCulate:ACPower:MARKer<x>:MAXimum, 2-88

:CALCulate:ACPower:MARKer<x>:PEAK:LEFT, 2-89

:CALCulate:ACPower:MARKer<x>:PEAK:RIGHT, 2-89

:CALCulate:ACPower:MARKer<x>:X(?), 2-90

:CALCulate:ACPower:MARKer<x>:Y?, 2-90

:CALCulate:AVTime subgroup, 2-91

:CALCulate:AVTime:MARKer<x>:DELtA:X?, 2-92

:CALCulate:AVTime:MARKer<x>:DELtA:Y?, 2-92

:CALCulate:AVTime:MARKer<x>:MAXimum, 2-93

:CALCulate:AVTime:MARKer<x>:PEAK:HIGHer, 2-94

:CALCulate:AVTime:MARKer<x>:PEAK:LEFT, 2-94

:CALCulate:AVTime:MARKer<x>:PEAK:LOWer, 2-95

:CALCulate:AVTime:MARKer<x>:PEAK:RIGHT, 2-95

:CALCulate:AVTime:MARKer<x>:TRACe(?), 2-96

:CALCulate:AVTime:MARKer<x>:X(?), 2-97

:CALCulate:AVTime:MARKer<x>:Y?, 2-97

CALCulate:CONSt:MARKer<x> subgroup, 2-98

:CALCulate:CONSt:MARKer<x>:DELtA:X?, 2-98

:CALCulate:CONSt:MARKer<x>:MAGNitude?, 2-99

:CALCulate:CONSt:MARKer<x>:MAXimum, 2-99

:CALCulate:CONSt:MARKer<x>:PEAK:LEFT, 2-100

:CALCulate:CONSt:MARKer<x>:PEAK:RIGHT, 2-100

:CALCulate:CONSt:MARKer<x>:PHASe?, 2-101

:CALCulate:CONSt:MARKer<x>:SYMBol?, 2-101

:CALCulate:CONSt:MARKer<x>:VALue?, 2-102

:CALCulate:CONSt:MARKer<x>:X(?), 2-102

:CALCulate:DPSA subgroup, 2-103

:CALCulate:DPSA:MARKer<x>:DELtA:X?, 2-104

:CALCulate:DPSA:MARKer<x>:DELtA:Y?, 2-104

:CALCulate:DPSA:MARKer<x>:MAXimum, 2-105

:CALCulate:DPSA:MARKer<x>:PEAK:HIGHer, 2-105

:CALCulate:DPSA:MARKer<x>:PEAK:LEFT, 2-106

:CALCulate:DPSA:MARKer<x>:PEAK:LOWer, 2-106

:CALCulate:DPSA:MARKer<x>:PEAK:RIGHT, 2-107

:CALCulate:DPSA:MARKer<x>:TRACe(?), 2-108

:CALCulate:DPSA:MARKer<x>:X(?), 2-109

:CALCulate:DPSA:MARKer<x>:Y?, 2-109

:CALCulate:DPSA:MARKer<x>[:SET]:CENTer, 2-107

:CALCulate:EVM subgroup, 2-110

:CALCulate:EVM:MARKer<x>:DELtA:X?, 2-111

:CALCulate:EVM:MARKer<x>:DELtA:Y?, 2-111

:CALCulate:EVM:MARKer<x>:MAXimum, 2-112

:CALCulate:EVM:MARKer<x>:PEAK:HIGHer, 2-113

:CALCulate:EVM:MARKer<x>:PEAK:LEFT, 2-113

:CALCulate:EVM:MARKer<x>:PEAK:LOWer, 2-114

:CALCulate:EVM:MARKer<x>:PEAK:RIGHT, 2-114

:CALCulate:EVM:MARKer<x>:X(?), 2-115

:CALCulate:EVM:MARKer<x>:Y?, 2-115

:CALCulate:FVTime subgroup, 2-116

:CALCulate:FVTime:MARKer<x>:DELtA:X?, 2-117

:CALCulate:FVTime:MARKer<x>:DELtA:Y?, 2-117

:CALCulate:FVTime:MARKer<x>:MAXimum, 2-118

:CALCulate:FVTime:MARKer<x>:PEAK:HIGHer, 2-119

:CALCulate:FVTime:MARKer<x>:PEAK:LEFT, 2-119

:CALCulate:FVTime:MARKer<x>:PEAK:LOWer, 2-120

:CALCulate:FVTime:MARKer<x>:PEAK:RIGHT, 2-120

:CALCulate:FVTime:MARKer<x>:X(?), 2-121

:CALCulate:FVTime:MARKer<x>:Y?, 2-121

:CALCulate:IQVTime subgroup, 2-122

:CALCulate:IQVTime:MARKer<x>:DELtA:X?, 2-123

:CALCulate:IQVTime:MARKer<x>:DELta:Y?, 2-123
:CALCulate:IQVTime:MARKer<x>:MAXimum,
2-124
:CALCulate:IQVTime:MARKer<x>:PEAK:HIGHer,
2-125
:CALCulate:IQVTime:MARKer<x>:PEAK:LEFT,
2-125
:CALCulate:IQVTime:MARKer<x>:PEAK:LOWer,
2-126
:CALCulate:IQVTime:MARKer<x>:PEAK:RIGHT,
2-126
:CALCulate:IQVTime:MARKer<x>:TRACe(?), 2-127
:CALCulate:IQVTime:MARKer<x>:X(?), 2-128
:CALCulate:IQVTime:MARKer<x>:Y?, 2-128
:CALCulate:MARKer:ADD, 2-72
:CALCulate:MARKer:AOff, 2-72
:CALCulate:MARKer:DELeTe, 2-73
:CALCulate:MARKer:MODE(?), 2-73
:CALCulate:MARKer:PEAK:EXCURsion(?), 2-74
:CALCulate:MARKer:PEAK:THReShold(?), 2-74
:CALCulate:MCPower subgroup, 2-129
:CALCulate:MCPower:MARKer<x>:DELta:X?, 2-130
:CALCulate:MCPower:MARKer<x>:DELta:Y?, 2-130
:CALCulate:MCPower:MARKer<x>:MAXimum,
2-131
:CALCulate:MCPower:MARKer<x>:PEAK:LEFT,
2-132
:CALCulate:MCPower:MARKer<x>:PEAK:RIGHT,
2-132
:CALCulate:MCPower:MARKer<x>:X(?), 2-133
:CALCulate:MCPower:MARKer<x>:Y?, 2-133
:CALCulate:MERRor subgroup (option 21 only),
2-134
:CALCulate:MERRor:MARKer<x>:DELta:X?, 2-135
:CALCulate:MERRor:MARKer<x>:DELta:Y?, 2-135
:CALCulate:MERRor:MARKer<x>:MAXimum, 2-136
:CALCulate:MERRor:MARKer<x>:PEAK:HIGHer,
2-137
:CALCulate:MERRor:MARKer<x>:PEAK:LEFT,
2-137
:CALCulate:MERRor:MARKer<x>:PEAK:LOWer,
2-138
:CALCulate:MERRor:MARKer<x>:PEAK:RIGHT,
2-138
:CALCulate:MERRor:MARKer<x>:X(?), 2-139
:CALCulate:MERRor:MARKer<x>:Y?, 2-139
:CALCulate:OBWidth subgroup, 2-140
:CALCulate:OBWidth:MARKer<x>:DELta:X?, 2-141
:CALCulate:OBWidth:MARKer<x>:DELta:Y?, 2-141
:CALCulate:OBWidth:MARKer<x>:MAXimum,
2-142

:CALCulate:OBWidth:MARKer<x>:PEAK:HIGHer,
2-142
:CALCulate:OBWidth:MARKer<x>:PEAK:LEFT,
2-143
:CALCulate:OBWidth:MARKer<x>:PEAK:LOWer,
2-143
:CALCulate:OBWidth:MARKer<x>:PEAK:RIGHT,
2-144
:CALCulate:OBWidth:MARKer<x>:X(?), 2-145
:CALCulate:OBWidth:MARKer<x>:Y?, 2-145
:CALCulate:OBWidth:MARKer<x>[:SET]:CENTer,
2-144
:CALCulate:PERRor subgroup (option 21 only), 2-146
:CALCulate:PERRor:MARKer<x>:DELta:X?, 2-147
:CALCulate:PERRor:MARKer<x>:DELta:Y?, 2-147
:CALCulate:PERRor:MARKer<x>:MAXimum, 2-148
:CALCulate:PERRor:MARKer<x>:PEAK:HIGHer,
2-149
:CALCulate:PERRor:MARKer<x>:PEAK:LEFT,
2-149
:CALCulate:PERRor:MARKer<x>:PEAK:LOWer,
2-150
:CALCulate:PERRor:MARKer<x>:PEAK:RIGHT,
2-150
:CALCulate:PERRor:MARKer<x>:X(?), 2-151
:CALCulate:PERRor:MARKer<x>:Y?, 2-151
:CALCulate:PHVTime subgroup, 2-152
:CALCulate:PHVTime:MARKer<x>:DELta:X?, 2-153
:CALCulate:PHVTime:MARKer<x>:DELta:Y?, 2-153
:CALCulate:PHVTime:MARKer<x>:MAXimum,
2-154
:CALCulate:PHVTime:MARKer<x>:PEAK:HIGHer,
2-155
:CALCulate:PHVTime:MARKer<x>:PEAK:LEFT,
2-155
:CALCulate:PHVTime:MARKer<x>:PEAK:LOWer,
2-156
:CALCulate:PHVTime:MARKer<x>:PEAK:RIGHT,
2-156
:CALCulate:PHVTime:MARKer<x>:X(?), 2-157
:CALCulate:PHVTime:MARKer<x>:Y?, 2-157
:CALCulate:PULSe subgroup (Option 20 only), 2-158
:CALCulate:PULSe:STATic:MARKer<x>:MAXimum,
2-160
:CALCulate:PULSe:STATic:MARKer<x>:X(?), 2-163
:CALCulate:PULSe:STATic:MARKer<x>:Y?, 2-163
:CALCulate:PULSe:STATistics:MARKer<x>:DELta
:X?, 2-159
:CALCulate:PULSe:STATistics:MARKer<x>:DELta
:Y?, 2-159

- :CALCulate:PULSe:STATistics:MARKer<x>:PEAK
:HIGHer, 2-160
- :CALCulate:PULSe:STATistics:MARKer<x>:PEAK
:LEFT, 2-161
- :CALCulate:PULSe:STATistics:MARKer<x>:PEAK
:LOWer, 2-161
- :CALCulate:PULSe:STATistics:MARKer<x>:PEAK
:RIGHt, 2-162
- :CALCulate:PULSe:TRACe:MARKer<x>:MAXimum,
2-165
- :CALCulate:PULSe:TRACe:MARKer<x>:PEAK
:HIGHer, 2-165
- :CALCulate:PULSe:TRACe:MARKer<x>:PEAK
:LEFT, 2-166
- :CALCulate:PULSe:TRACe:MARKer<x>:PEAK
:LOWer, 2-166
- :CALCulate:PULSe:TRACe:MARKer<x>:PEAK
:RIGHt, 2-167
- :CALCulate:PULSe:TRACe:MARKer<x>:X(?), 2-168
- :CALCulate:PULSe:TRACe:MARKer<x>:Y?, 2-168
- :CALCulate:SEARCh:LIMit:FAIL?, 2-75
- :CALCulate:SEARCh:LIMit:MATCH:BEEP[:STATe]
(?), 2-76
- :CALCulate:SEARCh:LIMit:MATCH:SACQuire
[:STATe](?), 2-76
- :CALCulate:SEARCh:LIMit:MATCH:SDATa[:STATe]
(?), 2-77
- :CALCulate:SEARCh:LIMit:MATCH:SPICture[:STATe]
(?), 2-78
- :CALCulate:SEARCh:LIMit:MATCH:STRace[:STATe]
(?), 2-79
- :CALCulate:SEARCh:LIMit:OPERation:FEED(?),
2-81
- :CALCulate:SEARCh:LIMit:OPERation:MASK
:LOAD, 2-82
- :CALCulate:SEARCh:LIMit:OPERation:MASK
:STORE, 2-82
- :CALCulate:SEARCh:LIMit:OPERation:SLIMit(?),
2-83
- :CALCulate:SEARCh:LIMit:OPERation(?), 2-80
- :CALCulate:SEARCh:LIMit:REPort:DATA?, 2-84
- :CALCulate:SEARCh:LIMit:REPort:POINts?, 2-84
- :CALCulate:SEARCh:LIMit:STATe(?), 2-85
- :CALCulate:SGRam subgroup, 2-169
- :CALCulate:SGRam:MARKer<x>:DELTA:X
:FREQuency?, 2-170
- :CALCulate:SGRam:MARKer<x>:DELTA:X[:TIME]?,
2-170
- :CALCulate:SGRam:MARKer<x>:DELTA:Y?, 2-171
- :CALCulate:SGRam:MARKer<x>:MAXimum, 2-171
- :CALCulate:SGRam:MARKer<x>:PEAK:HIGHer,
2-172
- :CALCulate:SGRam:MARKer<x>:PEAK:LEFT, 2-172
- :CALCulate:SGRam:MARKer<x>:PEAK:LOWer,
2-173
- :CALCulate:SGRam:MARKer<x>:PEAK:RIGHt,
2-173
- :CALCulate:SGRam:MARKer<x>:X:FREQuency(?),
2-174
- :CALCulate:SGRam:MARKer<x>:X[:TIME](?), 2-175
- :CALCulate:SGRam:MARKer<x>:Y?, 2-175
- :CALCulate:SGRam:MARKer<x>[:SET]:CENTer,
2-174
- :CALCulate:SPECtrum subgroup, 2-176
- :CALCulate:SPECtrum:MARKer<x>:DELTA:X?,
2-177
- :CALCulate:SPECtrum:MARKer<x>:DELTA:Y?,
2-177
- :CALCulate:SPECtrum:MARKer<x>:MAXimum,
2-178
- :CALCulate:SPECtrum:MARKer<x>:PEAK:HIGHer,
2-178
- :CALCulate:SPECtrum:MARKer<x>:PEAK:LEFT,
2-179
- :CALCulate:SPECtrum:MARKer<x>:PEAK:LOWer,
2-179
- :CALCulate:SPECtrum:MARKer<x>:PEAK:RIGHt,
2-180
- :CALCulate:SPECtrum:MARKer<x>:TRACe(?),
2-181
- :CALCulate:SPECtrum:MARKer<x>:X(?), 2-182
- :CALCulate:SPECtrum:MARKer<x>:Y?, 2-182
- :CALCulate:SPECtrum:MARKer<x>[:SET]:CENTer,
2-180
- :CALCulate:TOVerview subgroup, 2-183
- :CALCulate:TOVerview:MARKer<x>:DELTA:X?,
2-184
- :CALCulate:TOVerview:MARKer<x>:DELTA:Y?,
2-184
- :CALCulate:TOVerview:MARKer<x>:MAXimum,
2-185
- :CALCulate:TOVerview:MARKer<x>:PEAK:HIGHer,
2-186
- :CALCulate:TOVerview:MARKer<x>:PEAK:LEFT,
2-186
- :CALCulate:TOVerview:MARKer<x>:PEAK:LOWer,
2-187
- :CALCulate:TOVerview:MARKer<x>:PEAK:RIGHt,
2-187
- :CALCulate:TOVerview:MARKer<x>:X(?), 2-188
- :CALCulate:TOVerview:MARKer<x>:Y?, 2-188
- CALibration command group, 2-21
- CALibration commands, 2-189
- CALibration:ABORT, 2-190

- :CALibration:AUTO(?), 2-190
- :CALibration:CORRection:EXTErnal:EDIT<x>:LABel(?), 2-191
- :CALibration:CORRection:EXTErnal:EDIT<x>:STATe(?), 2-191
- :CALibration:CORRection:EXTErnal:GAIN:STATe(?), 2-192
- :CALibration:CORRection:EXTErnal:GAIN[:MAGNitude](?), 2-192
- :CALibration:CORRection:EXTErnal:PROBe:CONNEct?, 2-193
- :CALibration:CORRection:EXTErnal:PROBe:STATe(?), 2-194
- :CALibration:CORRection:EXTErnal:PROBe[:MAGNitude]?, 2-193
- Case sensitivity, 2-8
- Character chart, A-1
- *CLS, 2-57
- Command group
 - ABORt, 2-14
 - CALCulate, 2-15
 - CALibration, 2-21
 - DISPlay, 2-21
 - FETCh, 2-28
 - IEEE common, 2-14
 - INITiate, 2-33
 - INPUt, 2-33
 - MMEMory, 2-34
 - OUTPUt, 2-35
 - READ, 2-36
 - SENSe, 2-41
 - STATus, 2-48
 - SYSTem, 2-49
 - TRACe, 2-50
 - TRIGger, 2-53
 - UNIT, 2-53
- Commands
 - chaining, 2-6
 - rules for forming, 2-1
 - structure of IEEE 488.2 commands, 2-9
 - syntax, 2-1
- Conformance information, D-1
- Creating commands, 2-3

D

- :DISPlay basic command subgroup, 2-196
- :DISPlay command group, 2-21
- DISPlay commands, 2-195
- :DISPlay:ACPower subgroup, 2-199
- :DISPlay:ACPower:MARKer:SHOW:STATe(?), 2-200
- :DISPlay:ACPower:PLEVel:SHOW:STATe(?), 2-200

- :DISPlay:ACPower:RESet:SCALe, 2-201
- :DISPlay:ACPower:WINDow:TRACe:GRATICule:GRID:STATe(?), 2-201
- :DISPlay:ACPower:X[:SCALe]:AUTO, 2-202
- :DISPlay:ACPower:X[:SCALe]:OFFSet(?), 2-203
- :DISPlay:ACPower:X[:SCALe](?), 2-202
- :DISPlay:ACPower:Y[:SCALe]:AUTO, 2-204
- :DISPlay:ACPower:Y[:SCALe]:OFFSet(?), 2-204
- :DISPlay:ACPower:Y[:SCALe](?), 2-203
- :DISPlay:AVTime subgroup, 2-205
- :DISPlay:AVTime:MARKer:SHOW:STATe(?), 2-206
- :DISPlay:AVTime:RESet, 2-206
- :DISPlay:AVTime:TRIGger:LEVel:STATe(?), 2-207
- :DISPlay:AVTime:WINDow:TRACe:GRATICule:GRID:STATe(?), 2-207
- :DISPlay:AVTime:X:RSCale, 2-208
- :DISPlay:AVTime:X[:SCALe]:AUTO, 2-209
- :DISPlay:AVTime:X[:SCALe]:AUTO:STATe(?), 2-209
- :DISPlay:AVTime:X[:SCALe]:FULL(?), 2-210
- :DISPlay:AVTime:X[:SCALe]:MAXimum?, 2-211
- :DISPlay:AVTime:X[:SCALe]:MINimum?, 2-211
- :DISPlay:AVTime:X[:SCALe]:OFFSet:MAXimum?, 2-213
- :DISPlay:AVTime:X[:SCALe]:OFFSet:MINimum?, 2-213
- :DISPlay:AVTime:X[:SCALe]:OFFSet(?), 2-212
- :DISPlay:AVTime:Y:RSCale, 2-214
- :DISPlay:AVTime:Y[:SCALe]:FULL(?), 2-215
- :DISPlay:AVTime:Y[:SCALe]:OFFSet(?), 2-215
- :DISPlay:CONSte subgroup, 2-216
- :DISPlay:CONSte:WINDow:TRACe:GRATICule:GRID:STATe(?), 2-216
- :DISPlay:DDEMod subgroup, 2-217
- :DISPlay:DDEMod:MEASview:DELeTe, 2-218
- :DISPlay:DDEMod:MEASview:NEW, 2-219
- :DISPlay:DDEMod:MEASview:SELeCt(?), 2-219
- :DISPlay:DDEMod:RADix(?), 2-220
- :DISPlay:DDEMod:X[:SCALe]:AUTO, 2-221
- :DISPlay:DDEMod:X[:SCALe]:AUTO:STATe(?), 2-221
- :DISPlay:DDEMod:X[:SCALe]:MAXimum?, 2-222
- :DISPlay:DDEMod:X[:SCALe]:MINimum?, 2-222
- :DISPlay:DDEMod:X[:SCALe]:OFFSet:MAXimum?, 2-224
- :DISPlay:DDEMod:X[:SCALe]:OFFSet:MINimum?, 2-224
- :DISPlay:DDEMod:X[:SCALe]:OFFSet(?), 2-223
- :DISPlay:DDEMod:X[:SCALe]:RESet, 2-225
- :DISPlay:DDEMod:X[:SCALe](?), 2-220
- :DISPlay:DPsA subgroup, 2-226
- :DISPlay:DPsA:WINDow:TRACe:GRATICule:GRID:STATe(?), 2-226

:DISPlay:DPSA:Y[:SCALe]:PDIVision(?), 2-227
 :DISPlay:EVM subgroup, 2-228
 :DISPlay:EVM:Y[:SCALe]:AUTO, 2-229
 :DISPlay:EVM:Y[:SCALe]:OFFSet(?), 2-229
 :DISPlay:EVM:Y[:SCALe](?), 2-228
 :DISPlay:FVTime subgroup, 2-230
 :DISPlay:FVTime:WINDow:TRACe:GRATicule:GRID:STATe(?), 2-231
 :DISPlay:FVTime:X[:SCALe]:AUTO, 2-233
 :DISPlay:FVTime:X[:SCALe]:AUTO:STATe(?), 2-233
 :DISPlay:FVTime:X[:SCALe]:MAXimum?, 2-234
 :DISPlay:FVTime:X[:SCALe]:MINimum?, 2-234
 :DISPlay:FVTime:X[:SCALe]:OFFSet:MAXimum?, 2-236
 :DISPlay:FVTime:X[:SCALe]:OFFSet:MINimum?, 2-236
 :DISPlay:FVTime:X[:SCALe]:OFFSet(?), 2-235
 :DISPlay:FVTime:X[:SCALe](?), 2-232
 :DISPlay:FVTime:Y[:SCALe]:AUTO, 2-237
 :DISPlay:FVTime:Y[:SCALe]:OFFSet(?), 2-238
 :DISPlay:FVTime:Y[:SCALe](?), 2-237
 :DISPlay:GENeral subgroup, 2-239
 :DISPlay:GENeral:MEASview:DELeTe, 2-240
 :DISPlay:GENeral:MEASview:NEW, 2-241
 :DISPlay:GENeral:MEASview:SELeCt(?), 2-242
 :DISPlay:GPRF subgroup, 2-243
 :DISPlay:GPRF:MEASview:DELeTe, 2-243
 :DISPlay:GPRF:MEASview:NEW, 2-244
 :DISPlay:GPRF:MEASview:SELeCt(?), 2-245
 :DISPlay:IQVTime subgroup, 2-246
 :DISPlay:IQVTime:WINDow:TRACe:GRATicule:GRID:STATe(?), 2-247
 :DISPlay:IQVTime:X[:SCALe]:AUTO, 2-249
 :DISPlay:IQVTime:X[:SCALe]:AUTO:STATe(?), 2-249
 :DISPlay:IQVTime:X[:SCALe]:MAXimum?, 2-250
 :DISPlay:IQVTime:X[:SCALe]:MINimum?, 2-250
 :DISPlay:IQVTime:X[:SCALe]:OFFSet:MAXimum?, 2-252
 :DISPlay:IQVTime:X[:SCALe]:OFFSet:MINimum?, 2-252
 :DISPlay:IQVTime:X[:SCALe]:OFFSet(?), 2-251
 :DISPlay:IQVTime:X[:SCALe](?), 2-248
 :DISPlay:IQVTime:Y[:SCALe]:AUTO, 2-253
 :DISPlay:IQVTime:Y[:SCALe]:OFFSet(?), 2-254
 :DISPlay:IQVTime:Y[:SCALe]:RESCale, 2-254
 :DISPlay:IQVTime:Y[:SCALe](?), 2-253
 :DISPlay:MCPower subgroup, 2-255
 :DISPlay:MCPower:MARKer:SHOW:STATe(?), 2-256
 :DISPlay:MCPower:PLEVel:SHOW:STATe(?), 2-256
 :DISPlay:MCPower:RESet:SCALe, 2-257
 :DISPlay:MCPower:WINDow:TRACe:GRATicule:GRID:STATe(?), 2-257
 :DISPlay:MCPower:X[:SCALe]:AUTO, 2-258
 :DISPlay:MCPower:X[:SCALe]:OFFSet(?), 2-259
 :DISPlay:MCPower:X[:SCALe](?), 2-258
 :DISPlay:MCPower:Y[:SCALe]:AUTO, 2-260
 :DISPlay:MCPower:Y[:SCALe]:OFFSet(?), 2-260
 :DISPlay:MCPower:Y[:SCALe](?), 2-259
 :DISPlay:MERRor subgroup, 2-261
 :DISPlay:MERRor:Y[:SCALe]:AUTO, 2-262
 :DISPlay:MERRor:Y[:SCALe]:OFFSet(?), 2-262
 :DISPlay:MERRor:Y[:SCALe](?), 2-261
 :DISPlay:OBWidth subgroup, 2-263
 :DISPlay:OBWidth:MARKer:SHOW:STATe(?), 2-264
 :DISPlay:OBWidth:RESet:SCALe, 2-264
 :DISPlay:OBWidth:SELeCted:BANDwidth(?), 2-265
 :DISPlay:OBWidth:WINDow:TRACe:GRATicule:GRID:STATe(?), 2-265
 :DISPlay:OBWidth:X[:SCALe]:AUTO, 2-266
 :DISPlay:OBWidth:X[:SCALe]:OFFSet(?), 2-267
 :DISPlay:OBWidth:X[:SCALe](?), 2-266
 :DISPlay:OBWidth:Y[:SCALe]:AUTO, 2-268
 :DISPlay:OBWidth:Y[:SCALe]:OFFSet(?), 2-268
 :DISPlay:OBWidth:Y[:SCALe](?), 2-267
 :DISPlay:PERRor subgroup, 2-269
 :DISPlay:PERRor:Y[:SCALe]:AUTO, 2-270
 :DISPlay:PERRor:Y[:SCALe]:OFFSet(?), 2-270
 :DISPlay:PERRor:Y[:SCALe](?), 2-269
 :DISPlay:PHVTime subgroup, 2-271
 :DISPlay:PHVTime:WINDow:TRACe:GRATicule:GRID:STATe(?), 2-272
 :DISPlay:PHVTime:X[:SCALe]:AUTO, 2-274
 :DISPlay:PHVTime:X[:SCALe]:AUTO:STATe(?), 2-274
 :DISPlay:PHVTime:X[:SCALe]:MAXimum?, 2-275
 :DISPlay:PHVTime:X[:SCALe]:MINimum?, 2-275
 :DISPlay:PHVTime:X[:SCALe]:OFFSet:MAXimum?, 2-277
 :DISPlay:PHVTime:X[:SCALe]:OFFSet:MINimum?, 2-277
 :DISPlay:PHVTime:X[:SCALe]:OFFSet(?), 2-276
 :DISPlay:PHVTime:X[:SCALe](?), 2-273
 :DISPlay:PHVTime:Y[:SCALe]:AUTO, 2-278
 :DISPlay:PHVTime:Y[:SCALe]:AXIS:REFeRence(?), 2-279
 :DISPlay:PHVTime:Y[:SCALe]:AXIS(?), 2-279
 :DISPlay:PHVTime:Y[:SCALe]:OFFSet(?), 2-280
 :DISPlay:PHVTime:Y[:SCALe]:RESCale, 2-280
 :DISPlay:PHVTime:Y[:SCALe](?), 2-278
 :DISPlay:PULSe subgroup (Option 20 only), 2-281
 :DISPlay:PULSe:MEASview:DELeTe, 2-283

:DISPlay:PULSe:MEASview:NEW, 2-283
:DISPlay:PULSe:MEASview:SElect(?), 2-284
:DISPlay:PULSe:RESult:ATX(?), 2-284
:DISPlay:PULSe:RESult:AVERage(?), 2-285
:DISPlay:PULSe:RESult:DROop(?), 2-285
:DISPlay:PULSe:RESult:DUTPct(?), 2-286
:DISPlay:PULSe:RESult:DUTRatio(?), 2-286
:DISPlay:PULSe:RESult:FALL(?), 2-287
:DISPlay:PULSe:RESult:FRDeviation(?), 2-287
:DISPlay:PULSe:RESult:MFRReqerror(?), 2-288
:DISPlay:PULSe:RESult:MPHerror(?), 2-288
:DISPlay:PULSe:RESult:PHDeviation(?), 2-289
:DISPlay:PULSe:RESult:PPFRequency(?), 2-289
:DISPlay:PULSe:RESult:PPOWer(?), 2-290
:DISPlay:PULSe:RESult:PPPHase(?), 2-290
:DISPlay:PULSe:RESult:RINTerval(?), 2-291
:DISPlay:PULSe:RESult:RIPple(?), 2-291
:DISPlay:PULSe:RESult:RISE(?), 2-292
:DISPlay:PULSe:RESult:RMSFreqerror(?), 2-292
:DISPlay:PULSe:RESult:RMSPherror(?), 2-293
:DISPlay:PULSe:RESult:RRATe(?), 2-293
:DISPlay:PULSe:RESult:TIME(?), 2-294
:DISPlay:PULSe:RESult:WIDTh(?), 2-294
:DISPlay:PULSe:SElect:NUMBer(?), 2-295
:DISPlay:PULSe:SElect:RESult(?), 2-296
:DISPlay:PULSe:STATistics:MARKer:SHOW:STATe
(?), 2-297
:DISPlay:PULSe:STATistics:PLOT(?), 2-298
:DISPlay:PULSe:STATistics:WINDow:TRACe
:GRATicule:GRID:STATe(?), 2-298
:DISPlay:PULSe:STATistics:X:RSCale, 2-299
:DISPlay:PULSe:STATistics:X[:SCALE]:NUMBer(?),
2-299
:DISPlay:PULSe:STATistics:X[:SCALE]:OFFSet(?),
2-300
:DISPlay:PULSe:STATistics:Y:RSCale, 2-300
:DISPlay:PULSe:STATistics:Y[:SCALE]:FULL(?),
2-301
:DISPlay:PULSe:STATistics:Y[:SCALE]:OFFSet(?),
2-302
:DISPlay:PULSe:STATistics:Y[:SCALE]:STOP?, 2-303
:DISPlay:PULSe:TRACe:MARKer:SHOW:STATe(?),
2-303
:DISPlay:PULSe:TRACe:POINt:SHOW(?), 2-304
:DISPlay:PULSe:TRACe:WINDow:TRACe
:GRATicule:GRID:STATe(?), 2-304
:DISPlay:PULSe:TRACe:X:RSCale, 2-305
:DISPlay:PULSe:TRACe:X[:SCALE]:FULL(?), 2-306
:DISPlay:PULSe:TRACe:X[:SCALE]:OFFSet(?),
2-307
:DISPlay:PULSe:TRACe:X[:SCALE]:PDIVision(?),
2-307

:DISPlay:PULSe:TRACe:X[:SCALE](?), 2-305
:DISPlay:PULSe:TRACe:Y:RSCale, 2-308
:DISPlay:PULSe:TRACe:Y[:SCALE]:FULL(?), 2-308
:DISPlay:PULSe:TRACe:Y[:SCALE]:OFFSet(?),
2-309
:DISPlay:PULSe:TRACe:Y[:SCALE]:STOP?, 2-309
:DISPlay:SGRam subgroup, 2-310
:DISPlay:SGRam:FREQuency:AUTO, 2-310
:DISPlay:SGRam:FREQuency:OFFSet(?), 2-311
:DISPlay:SGRam:FREQuency:SCALE(?), 2-311
:DISPlay:SGRam:TIME:AUTO, 2-312
:DISPlay:SGRam:TIME:OFFSet(?), 2-312
:DISPlay:SGRam:TIME:OVERlap(?), 2-313
:DISPlay:SGRam:TIME:SCALE(?), 2-313
:DISPlay:SPECtrum subgroup, 2-314
:DISPlay:SPECtrum:MARKer:NOISe:MODE(?),
2-315
:DISPlay:SPECtrum:WINDow:TRACe:GRATicule
:GRID:STATe(?), 2-316
:DISPlay:SPECtrum:Y[:SCALE]:PDIVision(?), 2-316
:DISPlay:TOVerview subgroup, 2-317
:DISPlay:TOVerview:WINDow:TRACe:GRATicule
:GRID:STATe(?), 2-317
:DISPlay:TOVerview:X[:SCALE]:AUTO, 2-319
:DISPlay:TOVerview:X[:SCALE]:OFFSet(?), 2-319
:DISPlay:TOVerview:X[:SCALE](?), 2-197, 2-318
:DISPlay:TOVerview:Y[:SCALE]:AUTO, 2-320
:DISPlay:TOVerview:Y[:SCALE]:OFFSet(?), 2-321
:DISPlay:TOVerview:Y[:SCALE]:RESCale, 2-321
:DISPlay:TOVerview:Y[:SCALE](?), 2-320
:DISPlay:WINDow:OPTimized:MEASurement?, 2-198
DPX spectrum, measurement mode, 2-12

E

Error codes, 3-15
 commands, 3-15
 device specific, 3-18
 execution, 3-16
 hardware, 3-18, 3-19
 query, 3-19
 unique, 3-19
*ESE(?), 2-58
*ESR?, 2-59

F

:FETCh basic command subgroup, 2-324
FETCh command group, 2-28
FETCh commands, 2-323
:FETCh:ACPower subgroup, 2-329

:FETCh:ACPower?, 2-330
 :FETCh:ACPower:CHANnel:POWer?, 2-331
 :FETCh:ACPower:SPECtrum?, 2-331
 :FETCh:AVTime subgroup, 2-332
 :FETCh:AVTime:AVERage?, 2-332
 :FETCh:AVTime:FIRSt|:SECond|:THIRd|:FOURth?, 2-333
 :FETCh:AVTime:MAXimum?, 2-334
 :FETCh:AVTime:MAXLocation?, 2-334
 :FETCh:AVTime:MINimum?, 2-335
 :FETCh:AVTime:MINLocation?, 2-335
 :FETCh:AVTime:RESult?, 2-336
 :FETCh:CCDF subgroup, 2-337
 :FETCh:CCDF?, 2-338
 :FETCh:CCDF:FIRSt|:SECond|:THIRd?, 2-339
 :FETCh:CONSte subgroup (Option 21 only), 2-340
 :FETCh:CONSte:RESults?, 2-340
 :FETCh:CONSte:TRACe?, 2-341
 :FETCh:DDEMod subgroup, 2-342
 :FETCh:DDEMod:STABle?, 2-342
 :FETCh:DDEMod:SYNCh:WORD:LENGth?, 2-343
 :FETCh:DDEMod:SYNCh:WORD:POSition?, 2-343
 :FETCh:DPSA subgroup, 2-344
 :FETCh:DPSA:TRACe:AVERage?, 2-344
 :FETCh:DPSA:TRACe:MATH?, 2-345
 :FETCh:DPSA:TRACe:MAXimum?, 2-346
 :FETCh:DPSA:TRACe:MINimum?, 2-347
 :FETCh:EVM subgroup, 2-348
 :FETCh:EVM:FERRor?, 2-348
 :FETCh:EVM:PEAK?, 2-349
 :FETCh:EVM:PINDex?, 2-349
 :FETCh:EVM:RMS?, 2-350
 :FETCh:EVM:TRACe?, 2-350
 :FETCh:FVTime subgroup, 2-351
 :FETCh:FVTime?, 2-351
 :FETCh:FVTime:MAX?, 2-352
 :FETCh:FVTime:MAXLocation?, 2-352
 :FETCh:FVTime:MIN?, 2-353
 :FETCh:FVTime:MINLocation?, 2-353
 :FETCh:FVTime:RESult?, 2-354
 :FETCh:IQVTime subgroup, 2-355
 :FETCh:IQVTime:I?, 2-355
 :FETCh:IQVTime:MAX?, 2-356
 :FETCh:IQVTime:MAXLocation?, 2-356
 :FETCh:IQVTime:MIN?, 2-357
 :FETCh:IQVTime:MINLocation?, 2-357
 :FETCh:IQVTime:Q?, 2-358
 :FETCh:IQVTime:RESult?, 2-359
 :FETCh:MCPower subgroup, 2-360
 :FETCh:MCPower:ADJacent:CHANnels?, 2-361
 :FETCh:MCPower:CHANnel:POWer?, 2-362
 :FETCh:MCPower:MAIN:CHANnels?, 2-363
 :FETCh:MCPower:SPECtrum?, 2-364
 :FETCh:MERRor subgroup, 2-365
 :FETCh:MERRor:FERRor?, 2-365
 :FETCh:MERRor:PEAK?, 2-366
 :FETCh:MERRor:PINDex?, 2-366
 :FETCh:MERRor:RMS?, 2-367
 :FETCh:MERRor:TRACe?, 2-367
 :FETCh:OBWidth subgroup, 2-368
 :FETCh:OBWidth:FREQuency:ERRor?, 2-369
 :FETCh:OBWidth:OBWidth:BANDwidth?, 2-369
 :FETCh:OBWidth:OBWidth:LEFT:FREQuency?, 2-370
 :FETCh:OBWidth:OBWidth:LEFT:LEVel?, 2-370
 :FETCh:OBWidth:OBWidth:POWer?, 2-371
 :FETCh:OBWidth:OBWidth:RIGHT:FREQuency?, 2-372
 :FETCh:OBWidth:OBWidth:RIGHT:LEVel?, 2-372
 :FETCh:OBWidth:SPECtrum?, 2-373
 :FETCh:OBWidth:XDBBbandwidth:BANDwidth?, 2-373
 :FETCh:OBWidth:XDBBbandwidth:LEFT:FREQuency?, 2-374
 :FETCh:OBWidth:XDBBbandwidth:LEFT:LEVel?, 2-374
 :FETCh:OBWidth:XDBBbandwidth:POWer?, 2-375
 :FETCh:OBWidth:XDBBbandwidth:RIGHT:FREQuency?, 2-376
 :FETCh:OBWidth:XDBBbandwidth:RIGHT:LEVel?, 2-376
 :FETCh:PERRor subgroup, 2-377
 :FETCh:PERRor:FERRor?, 2-377
 :FETCh:PERRor:PEAK?, 2-378
 :FETCh:PERRor:PINDex?, 2-378
 :FETCh:PERRor:RMS?, 2-379
 :FETCh:PERRor:TRACe?, 2-379
 :FETCh:PHVTime subgroup, 2-380
 :FETCh:PHVTime?, 2-380
 :FETCh:PHVTime:MAX?, 2-381
 :FETCh:PHVTime:MAXLocation?, 2-381
 :FETCh:PHVTime:MIN?, 2-382
 :FETCh:PHVTime:MINLocation?, 2-382
 :FETCh:PHVTime:RESult?, 2-383
 :FETCh:PULSe subgroup (Option 20 only), 2-384
 :FETCh:PULSe:STATic:ATX?, 2-402
 :FETCh:PULSe:STATic:AVERage?, 2-403
 :FETCh:PULSe:STATic:DROop?, 2-404
 :FETCh:PULSe:STATic:DUTPct?, 2-405
 :FETCh:PULSe:STATic:DUTRatio?, 2-406
 :FETCh:PULSe:STATic:FALL?, 2-407
 :FETCh:PULSe:STATic:PPOWer?, 2-413
 :FETCh:PULSe:STATic:PPPHase?, 2-414
 :FETCh:PULSe:STATic:RINTerval?, 2-415
 :FETCh:PULSe:STATic:RIPple?, 2-416

:FETCh:PULSe:STATic:RISE?, 2-417
:FETCh:PULSe:STATic:RRATe?, 2-420
:FETCh:PULSe:STATic:WIDTh?, 2-421
:FETCh:PULSe:STATistics?, 2-401
:FETCh:PULSe:STATistics:FRDeviation?, 2-408
:FETCh:PULSe:STATistics:MFReqerror?, 2-409
:FETCh:PULSe:STATistics:MPHerror?, 2-410
:FETCh:PULSe:STATistics:PHDeviation?, 2-411
:FETCh:PULSe:STATistics:PPFRequency?, 2-412
:FETCh:PULSe:STATistics:RMSFreqerror?, 2-418
:FETCh:PULSe:STATistics:RMSPherror?, 2-419
:FETCh:PULSe:TRACe?, 2-422
:FETCh:PULSe[:RESult]:ATX?, 2-385
:FETCh:PULSe[:RESult]:AVERage?, 2-386
:FETCh:PULSe[:RESult]:DROop?, 2-387
:FETCh:PULSe[:RESult]:DUTPct?, 2-387
:FETCh:PULSe[:RESult]:DUTRatio?, 2-388
:FETCh:PULSe[:RESult]:FALL?, 2-388
:FETCh:PULSe[:RESult]:FRDeviation?, 2-389
:FETCh:PULSe[:RESult]:MFReqerror?, 2-390
:FETCh:PULSe[:RESult]:MPHerror?, 2-391
:FETCh:PULSe[:RESult]:PHDeviation?, 2-392
:FETCh:PULSe[:RESult]:PPFRequency?, 2-393
:FETCh:PULSe[:RESult]:PPOWer?, 2-394
:FETCh:PULSe[:RESult]:PPPHase?, 2-395
:FETCh:PULSe[:RESult]:RINTerval?, 2-396
:FETCh:PULSe[:RESult]:RIPple?, 2-396
:FETCh:PULSe[:RESult]:RISE?, 2-397
:FETCh:PULSe[:RESult]:RMSFreqerror?, 2-397
:FETCh:PULSe[:RESult]:RMSPherror?, 2-398
:FETCh:PULSe[:RESult]:RRATe?, 2-399
:FETCh:PULSe[:RESult]:TIME?, 2-400
:FETCh:PULSe[:RESult]:WIDTh?, 2-400
:FETCh:RFIN:IQ?, 2-325
:FETCh:RFIN:IQ:HEADer?, 2-326
:FETCh:RFIN:IQ:SCALe?, 2-327
:FETCh:RFIN:RECORD:IDS?, 2-328
:FETCh:SGRam subgroup, 2-423
:FETCh:SGRam?, 2-423
:FETCh:SPECTrum subgroup, 2-424
:FETCh:SPECTrum:TRACe<x>?, 2-425
:FETCh:SQUAL subgroup, 2-426
:FETCh:SQUALity:FREQuency:ERRor?, 2-427
:FETCh:SQUALity:GAIN:IMBalance?, 2-427
:FETCh:SQUALity:ORIGin:OFFSet?, 2-428
:FETCh:SQUALity:PEAK:EVM?, 2-428
:FETCh:SQUALity:PEAK:EVM:DB?, 2-429
:FETCh:SQUALity:PEAK:EVM:LOCation?, 2-429
:FETCh:SQUALity:PEAK:MERRor?, 2-430
:FETCh:SQUALity:PEAK:MERRor:DB?, 2-430
:FETCh:SQUALity:PEAK:MERRor:LOCation?, 2-431
:FETCh:SQUALity:PEAK:PERRor?, 2-432
:FETCh:SQUALity:PEAK:PERRor:LOCation?, 2-432

:FETCh:SQUALity:QUADrature:ERRor?, 2-433
:FETCh:SQUALity:RHO?, 2-433
:FETCh:SQUALity:RMS:EVM?, 2-434
:FETCh:SQUALity:RMS:EVM:DB?, 2-434
:FETCh:SQUALity:RMS:MERRor?, 2-435
:FETCh:SQUALity:RMS:MERRor:DB?, 2-435
:FETCh:SQUALity:RMS:PERRor?, 2-436
:FETCh:TOVerview subgroup, 2-437
:FETCh:TOVerview?, 2-437
File, specifying, 2-445
Functional groups, 2-13

G

GPIO

- configurations, 1-4
- connection rules, 1-4
- interface specification, B-1
- setting GPIO address, 1-5

H

Hierarchy tree, 2-2

I

*IDN?, 2-60
IEEE 488.2 common commands, 2-9
IEEE common command group, 2-14
IEEE common commands, 2-55
IEEE Std 488.2-1987, 2-1
Initialization settings, C-1
INITiate command group, 2-33
INITiate commands, 2-439
:INITiate:CONTInuous(?), 2-439
:INITiate[:IMMediate], 2-440
INPut command group, 2-33
INPut commands, 2-441
:INPut:MLEVel[:RLEVel(?), 2-443
:INPut[:RF]:ATTenuation:AUTO(?), 2-442
:INPut[:RF]:ATTenuation(?), 2-442
:INPut[:RF]:GAIN:STATe(?), 2-443
Interface message, B-3

M

Marker mnemonics, 2-70
MCPR, measurement mode, 2-12
Measurement views, description, 2-11
:MMEMory basic command subgroup, 2-446
MMEMory command group, 2-34

MMEMory commands, 2-445
 :MMEMory:AVTime subgroup, 2-454
 :MMEMory:AVTime:LOAD:TRACe<x>, 2-455
 :MMEMory:AVTime:STORE:TRACe<x>, 2-455
 :MMEMory:CALibration:LOAD:CORRection
 :EXTernal:EDIT<x>, 2-447
 :MMEMory:CALibration:STORE:CORRection
 :EXTernal:EDIT<x>, 2-447
 :MMEMory:CCDF subgroup, 2-456
 :MMEMory:CCDF:LOAD:TRACe<x>, 2-457
 :MMEMory:CCDF:STORE:TRACe<x>, 2-457
 :MMEMory:DPSA Subgroup, 2-458
 :MMEMory:DPSA:LOAD:TRACe<x>, 2-459
 :MMEMory:DPSA:STORE:TRACe<x>, 2-459
 :MMEMory:FVTime subgroup, 2-460
 :MMEMory:FVTime:LOAD:TRACe, 2-461
 :MMEMory:FVTime:STORE:TRACe, 2-461
 :MMEMory:IQVTime subgroup, 2-462
 :MMEMory:IQVTime:LOAD:TRACe:I, 2-463
 :MMEMory:IQVTime:LOAD:TRACe:Q, 2-463
 :MMEMory:IQVTime:STORE:TRACe:I, 2-464
 :MMEMory:IQVTime:STORE:TRACe:Q, 2-464
 :MMEMory:LOAD:IQ, 2-448
 :MMEMory:LOAD:STATe, 2-448
 :MMEMory:LOAD:TRACe, 2-449
 :MMEMory:PHVTime subgroup, 2-465
 :MMEMory:PHVTime:LOAD:TRACe, 2-466
 :MMEMory:PHVTime:STORE:TRACe, 2-466
 :MMEMory:SPECTrum subgroup, 2-467
 :MMEMory:SPECTrum:LOAD:TRACe<x>, 2-468
 :MMEMory:SPECTrum:STORE:TRACe<x>, 2-468
 :MMEMory:STORE:IQ, 2-450
 :MMEMory:STORE:IQ:CSV, 2-451
 :MMEMory:STORE:IQ:MAT, 2-451
 :MMEMory:STORE:MSTate, 2-452
 :MMEMory:STORE:RESults, 2-452
 :MMEMory:STORE:STATe, 2-453
 :MMEMory:STORE:TRACe, 2-453
 Mnemonics, constructed, 2-9

O

*OPC(?), 2-60
 *OPT?, 2-61
 OUTPut command group, 2-35
 OUTPut commands, 2-469
 :OUTPut:IF:BANDwidth(?), 2-470
 :OUTPut:IF[:STATe](?), 2-470
 :OUTPut:NOISe[:STATe](?), 2-471

P

Parameter Types Used in Syntax Descriptions, 2-4

Q

Queries, 2-3
 Query Responses, 2-3
 Queues
 event, 3-10
 output, 3-10
 Quotes, 2-8

R

READ command group, 2-36
 READ commands, 2-473
 :READ:ACPower subgroup, 2-474
 :READ:ACPower?, 2-475
 :READ:ACPower:CHANnel:POWer?, 2-476
 :READ:ACPower:SPECTrum?, 2-476
 :READ:AVTime subgroup, 2-477
 :READ:AVTime:AVERage?, 2-477
 :READ:AVTime:FIRSt|:SECond|:THIRd|:FOURth?,
 2-478
 :READ:AVTime:MAXimum?, 2-479
 :READ:AVTime:MAXLocation?, 2-479
 :READ:AVTime:MINimum?, 2-480
 :READ:AVTime:MINLocation?, 2-480
 :READ:AVTime:RESult?, 2-481
 :READ:CCDF subgroup, 2-482
 :READ:CCDF?, 2-483
 :READ:CCDF:FIRSt|:SECond|:THIRd?, 2-484
 :READ:CONSte subgroup (Option 21 only), 2-485
 :READ:CONSte:RESults?, 2-485
 :READ:CONSte:TRACe?, 2-486
 :READ:DDEMod subgroup (Option 21 only), 2-487
 :READ:DDEMod:STABle?, 2-487
 :READ:DPSA subgroup, 2-488
 :READ:DPSA:TRACe:AVERage?, 2-488
 :READ:DPSA:TRACe:MATH?, 2-489
 :READ:DPSA:TRACe:MAXimum?, 2-490
 :READ:DPSA:TRACe:MINimum?, 2-491
 :READ:EVM subgroup, 2-492
 :READ:EVM:FERRor?, 2-492
 :READ:EVM:PEAK?, 2-493
 :READ:EVM:PINDex?, 2-493
 :READ:EVM:RMS?, 2-494

:READ:EVM:TRACe?, 2-494
:READ:FVTime subgroup, 2-495
:READ:FVTime?, 2-495
:READ:FVTime:MAX?, 2-496
:READ:FVTime:MAXLocation?, 2-496
:READ:FVTime:MIN?, 2-497
:READ:FVTime:MINLocation?, 2-497
:READ:FVTime:RESult?, 2-498
:READ:IQVTime subgroup, 2-499
:READ:IQVTime:I?, 2-499
:READ:IQVTime:MAX?, 2-500
:READ:IQVTime:MAXLocation?, 2-500
:READ:IQVTime:MIN?, 2-501
:READ:IQVTime:MINLocation?, 2-501
:READ:IQVTime:Q?, 2-502
:READ:IQVTime:RESult?, 2-503
:READ:MCPowe:MAIN:CHANnels?, 2-507
:READ:MCPower subgroup, 2-504
:READ:MCPower:ADJacent:CHANnels?, 2-505
:READ:MCPower:CHANnel:POWer?, 2-506
:READ:MCPower:SPECtrum?, 2-508
:READ:MERRor subgroup, 2-509
:READ:MERRor:FERRor?, 2-509
:READ:MERRor:PEAK?, 2-510
:READ:MERRor:PINdex?, 2-510
:READ:MERRor:RMS?, 2-511
:READ:MERRor:TRACe?, 2-511
:READ:OBWidth subgroup, 2-512
:READ:OBWidth:FREQuency:ERRor?, 2-513
:READ:OBWidth:OBWidth:BANDwidth?, 2-513
:READ:OBWidth:OBWidth:LEFT:FREQuency?,
2-514
:READ:OBWidth:OBWidth:LEFT:LEVel?, 2-514
:READ:OBWidth:OBWidth:POWer?, 2-515
:READ:OBWidth:OBWidth:RIGHT:FREQuency?,
2-516
:READ:OBWidth:OBWidth:RIGHT:LEVel?, 2-516
:READ:OBWidth:SPECtrum?, 2-517
:READ:OBWidth:XDBBbandwidth:BANDwidth?,
2-517
:READ:OBWidth:XDBBbandwidth:LEFT:FREQuency?,
2-518
:READ:OBWidth:XDBBbandwidth:LEFT:LEVel?,
2-518
:READ:OBWidth:XDBBbandwidth:POWer?, 2-519
:READ:OBWidth:XDBBbandwidth:RIGHT
:FREQuency?, 2-520
:READ:OBWidth:XDBBbandwidth:RIGHT:LEVel?,
2-520
:READ:PERRor subgroup, 2-521
:READ:PERRor:FERRor?, 2-521
:READ:PERRor:PEAK?, 2-522
:READ:PERRor:PINdex?, 2-522
:READ:PERRor:RMS?, 2-523
:READ:PERRor:TRACe?, 2-523
:READ:PHVTime subgroup, 2-524
:READ:PHVTime?, 2-524
:READ:PHVTime:MAX?, 2-525
:READ:PHVTime:MAXLocation?, 2-525
:READ:PHVTime:MIN?, 2-526
:READ:PHVTime:MINLocation?, 2-526
:READ:PHVTime:RESult?, 2-527
:READ:PULSe subgroup (Option 20 only), 2-528
:READ:PULSe:STATIC:ATX?, 2-546
:READ:PULSe:STATIC:AVERage?, 2-547
:READ:PULSe:STATIC:DROOp?, 2-548
:READ:PULSe:STATIC:DUTPct?, 2-549
:READ:PULSe:STATIC:DUTRatio?, 2-550
:READ:PULSe:STATIC:FALL?, 2-551
:READ:PULSe:STATIC:PPOWer?, 2-557
:READ:PULSe:STATIC:PPPHase?, 2-558
:READ:PULSe:STATIC:RINTerval?, 2-559
:READ:PULSe:STATIC:RIPple?, 2-560
:READ:PULSe:STATIC:RISE?, 2-561
:READ:PULSe:STATIC:RRATE?, 2-564
:READ:PULSe:STATIC:WIDTH?, 2-565
:READ:PULSe:STATistics?, 2-545
:READ:PULSe:STATistics:FRDeviation?, 2-552
:READ:PULSe:STATistics:MFRreqerror?, 2-553
:READ:PULSe:STATistics:MPHerror?, 2-554
:READ:PULSe:STATistics:PHDeviation?, 2-555
:READ:PULSe:STATistics:PPFRequency?, 2-556
:READ:PULSe:STATistics:RMSFreqerror?, 2-562
:READ:PULSe:STATistics:RMSPherror?, 2-563
:READ:PULSe:TRACe?, 2-566
:READ:PULSe[:RESult]:ATX?, 2-529
:READ:PULSe[:RESult]:AVERage?, 2-530
:READ:PULSe[:RESult]:DROOp?, 2-531
:READ:PULSe[:RESult]:DUTPct?, 2-531
:READ:PULSe[:RESult]:DUTRatio?, 2-532
:READ:PULSe[:RESult]:FALL?, 2-532
:READ:PULSe[:RESult]:FRDeviation?, 2-533
:READ:PULSe[:RESult]:MFRreqerror?, 2-534
:READ:PULSe[:RESult]:MPHerror?, 2-535
:READ:PULSe[:RESult]:PHDeviation?, 2-536
:READ:PULSe[:RESult]:PPFRequency?, 2-537
:READ:PULSe[:RESult]:PPOWer?, 2-538
:READ:PULSe[:RESult]:PPPHase?, 2-539
:READ:PULSe[:RESult]:RINTerval?, 2-540
:READ:PULSe[:RESult]:RIPple?, 2-540
:READ:PULSe[:RESult]:RISE?, 2-541
:READ:PULSe[:RESult]:RMSFreqerror?, 2-541
:READ:PULSe[:RESult]:RMSPherror?, 2-542
:READ:PULSe[:RESult]:RRATE?, 2-543

:READ:PULSe[:RESult]:TIME?, 2-544
 :READ:PULSe[:RESult]:WIDTH?, 2-544
 :READ:SGRam subgroup, 2-567
 :READ:SGRam?, 2-567
 :READ:SPECtrum subgroup, 2-568
 :READ:SPECtrum:TRACe<x>?, 2-569
 :READ:SQUAL subgroup, 2-570
 :READ:SQUALity:FREQuency:ERRor, 2-571
 :READ:SQUALity:GAIN:IMBalance?, 2-571
 :READ:SQUALity:ORIGin:OFFSet?, 2-572
 :READ:SQUALity:PEAK:EVM?, 2-572
 :READ:SQUALity:PEAK:EVM:DB?, 2-573
 :READ:SQUALity:PEAK:EVM:LOCation?, 2-573
 :READ:SQUALity:PEAK:MERRor:DB?, 2-574
 :READ:SQUALity:PEAK:MERRor:LOCation?, 2-575
 :READ:SQUALity:PEAK:PERRor?, 2-576
 :READ:SQUALity:PEAK:PERRor:LOCation?, 2-576
 :READ:SQUALity:QUADrature:ERRor?, 2-577
 :READ:SQUALity:RHO?, 2-577
 :READ:SQUALity:RMS:EVM?, 2-578
 :READ:SQUALity:RMS:EVM:DB?, 2-578
 :READ:SQUALity:RMS:MERRor?, 2-579
 :READ:SQUALity:RMS:MERRor:DB?, 2-579
 :READ:SQUALity:RMS:PERRor?, 2-580
 :READ:TOVerview subgroup, 2-581
 :READ:TOVerview?, 2-581
 Registers, Service Request Enable Register (SRER),
 3-5
 Retrieving response message, 2-845
 *RST, 2-62
 Rules
 command forming, 2-1
 for using SCPI commands, 2-8

S

SCPI
 abbreviating, 2-5
 chaining commands, 2-6
 commands, 2-2
 conformance information, D-1
 general rules, 2-8
 parameter types, 2-4
 subsystem hierarchy tree, 2-2
 SCPI commands and queries syntax, 2-2
 creating commands, 2-3
 creating queries, 2-3
 SENSE command group, 2-41
 SENSE commands, 2-583
 [:SENSe]:ACPower subgroup, 2-604
 [:SENSe]:ACPower:AVERage:COUNT(?), 2-605

[:SENSe]:ACPower:AVERage(?), 2-605
 [:SENSe]:ACPower:BANDwidth[:BWIDth
 [:RESolution]:ACTual?, 2-606
 [:SENSe]:ACPower:BANDwidth[:BWIDth
 [:RESolution]:AUTO(?), 2-607, 2-675
 [:SENSe]:ACPower:BANDwidth[:BWIDth
 [:RESolution](?), 2-606, 2-674
 [:SENSe]:ACPower:CHANnel:BANDwidth[:BWIDth
 (?), 2-608
 [:SENSe]:ACPower:CHANnel:FILTer(?), 2-608
 [:SENSe]:ACPower:CHANnel:PAIRs(?), 2-609
 [:SENSe]:ACPower:CHANnel:SPACing(?), 2-609
 [:SENSe]:ACPower:CHIPrate(?), 2-610
 [:SENSe]:ACPower:CLear:RESults, 2-610
 [:SENSe]:ACPower:FREQuency:STEP:AUTO(?),
 2-611
 [:SENSe]:ACPower:FREQuency:STEP(?), 2-611
 [:SENSe]:ACPower:NFLoor:STATe(?), 2-612
 [:SENSe]:ACPower:OPTimize:SPAN(?), 2-612
 [:SENSe]:ACPower:RRCRolloff(?), 2-613
 [:SENSe]:ACQuisition:BANDwidth[:BWIDth(?),
 2-586
 [:SENSe]:ACQuisition:FFRame:ACTual?, 2-586
 [:SENSe]:ACQuisition:FFRame:LIMit(?), 2-587
 [:SENSe]:ACQuisition:FFRame:STATe(?), 2-587
 [:SENSe]:ACQuisition:MEMory:AVAILable:SAMPLEs?,
 2-588
 [:SENSe]:ACQuisition:MEMory:CAPacity[:TIME]?,
 2-588
 [:SENSe]:ACQuisition:MEMory:USED[:PERCent]?,
 2-589
 [:SENSe]:ACQuisition:MODE(?), 2-589
 [:SENSe]:ACQuisition:SAMPLEs(?), 2-590
 [:SENSe]:ACQuisition:SEConds(?), 2-590
 [:SENSe]:ANALysis subgroup, 2-584
 [:SENSe]:ANALysis:ADVanced:DITHer:HWAre
 :STATus?, 2-592
 [:SENSe]:ANALysis:ADVanced:DITHer(?), 2-591
 [:SENSe]:ANALysis:LENGth:ACTual?, 2-594
 [:SENSe]:ANALysis:LENGth:AUTO(?), 2-594
 [:SENSe]:ANALysis:LENGth(?), 2-593
 [:SENSe]:ANALysis:REFErence(?), 2-595
 [:SENSe]:ANALysis:START:AUTO(?), 2-596
 [:SENSe]:ANALysis:START(?), 2-595
 [:SENSe]:AVTime subgroup, 2-614
 [:SENSe]:AVTime:BANDwidth[:BWIDth:ACTual?,
 2-615
 [:SENSe]:AVTime:BANDwidth[:BWIDth(?), 2-615
 [:SENSe]:AVTime:CLear:RESults, 2-616
 [:SENSe]:AVTime:MAXTracepoints(?), 2-616
 [:SENSe]:AVTime:METHod(?), 2-617
 [:SENSe]:AVTime:SPAN(?), 2-618

- [SENSe]:CCDF subgroup, 2-619
- [SENSe]:CCDF:BANDwidth|BWIDth(?), 2-619
- [SENSe]:CCDF:CLEar, 2-620
- [SENSe]:CCDF:TIME:AUTO(?), 2-621
- [SENSe]:CCDF:TIME:LENGth(?), 2-620
- [SENSe]:DDEMod subgroup, 2-622
- [SENSe]:DDEMod:ANALysis:LENGth:ACTual?, 2-624
- [SENSe]:DDEMod:ANALysis:LENGth:AUTO(?), 2-624
- [SENSe]:DDEMod:ANALysis:LENGth(?), 2-623
- [SENSe]:DDEMod:BURSt:DETECT(?), 2-625
- [SENSe]:DDEMod:BURSt:THREShold(?), 2-626
- [SENSe]:DDEMod:CARRier:OFFSet(?), 2-626
- [SENSe]:DDEMod:FILTer:ALPHa(?), 2-627
- [SENSe]:DDEMod:FILTer:MEASurement(?), 2-628
- [SENSe]:DDEMod:FILTer:REFERENCE(?), 2-629
- [SENSe]:DDEMod:MAGNitude:NORMAlize(?), 2-629
- [SENSe]:DDEMod:MODulation:TYPE(?), 2-630
- [SENSe]:DDEMod:SRATe(?), 2-631
- [SENSe]:DDEMod:SWAP:IQ(?), 2-631
- [SENSe]:DDEMod:SYMBOL:POINTs(?), 2-632
- [SENSe]:DDEMod:SYNCh:WORD:SYMBOL(?), 2-634
- [SENSe]:DDEMod:SYNCh:WORD(?), 2-633
- [SENSe]:DDEMod:TIME:UNITs(?), 2-634
- [SENSe]:DPSA subgroup, 2-635
- [SENSe]:DPSA:AUDio:DEMod:GAIN(?), 2-636
- [SENSe]:DPSA:AUDio:DEMod:RXBWidth(?), 2-636
- [SENSe]:DPSA:AUDio:DEMod:RXFREquency?, 2-637
- [SENSe]:DPSA:AUDio:DEMod:STATe(?), 2-637
- [SENSe]:DPSA:AUDio:DEMod:TUNE(?), 2-638
- [SENSe]:DPSA:AUDio:DEMod:TYPE(?), 2-639
- [SENSe]:DPSA:BANDwidth|BWIDth|RESolution|:AUTO(?), 2-640
- [SENSe]:DPSA:BANDwidth|BWIDth|RESolution|(?), 2-639
- [SENSe]:DPSA:CLEar:RESults, 2-640
- [SENSe]:DPSA:COLor:MAXimum(?), 2-642
- [SENSe]:DPSA:COLor:MINimum(?), 2-642
- [SENSe]:DPSA:COLor(?), 2-641
- [SENSe]:DPSA:FREquency:CENTer(?), 2-643
- [SENSe]:DPSA:FREquency:SPAN(?), 2-643
- [SENSe]:DPSA:FREquency:START(?), 2-644
- [SENSe]:DPSA:FREquency:STEP:AUTO(?), 2-645
- [SENSe]:DPSA:FREquency:STEP(?), 2-645
- [SENSe]:DPSA:FREquency:STOP(?), 2-646
- [SENSe]:FVTime subgroup, 2-647
- [SENSe]:FVTime:CLEar:RESults, 2-647
- [SENSe]:FVTime:FREquency:CENTer(?), 2-648
- [SENSe]:FVTime:FREquency:SPAN(?), 2-649
- [SENSe]:FVTime:FREquency:START(?), 2-649
- [SENSe]:FVTime:FREquency:STEP:AUTO(?), 2-650
- [SENSe]:FVTime:FREquency:STEP(?), 2-650
- [SENSe]:FVTime:FREquency:STOP(?), 2-651
- [SENSe]:FVTime:MAXTracepoints(?), 2-652
- [SENSe]:IQVTime subgroup, 2-653
- [SENSe]:IQVTime:CLEar:RESults, 2-653
- [SENSe]:IQVTime:FREquency:CENTer(?), 2-654
- [SENSe]:IQVTime:FREquency:SPAN(?), 2-655
- [SENSe]:IQVTime:FREquency:START(?), 2-655
- [SENSe]:IQVTime:FREquency:STEP:AUTO(?), 2-656
- [SENSe]:IQVTime:FREquency:STEP(?), 2-656
- [SENSe]:IQVTime:FREquency:STOP(?), 2-657
- [SENSe]:IQVTime:MAXTracepoints(?), 2-658
- [SENSe]:MCPower subgroup, 2-659
- [SENSe]:MCPower:AVERage:COUNt(?), 2-660
- [SENSe]:MCPower:AVERage(?), 2-660
- [SENSe]:MCPower:BANDwidth|BWIDth|RESolution|:ACTual?, 2-661
- [SENSe]:MCPower:BANDwidth|BWIDth|RESolution|:AUTO(?), 2-662
- [SENSe]:MCPower:BANDwidth|BWIDth|RESolution|(?), 2-661
- [SENSe]:MCPower:CHANnel:ADJacent:ADD, 2-663
- [SENSe]:MCPower:CHANnel:ADJacent:DELeTe, 2-663
- [SENSe]:MCPower:CHANnel:FILTer(?), 2-664
- [SENSe]:MCPower:CHANnel:MAIN:BANDwidth|BWIDth(?), 2-664
- [SENSe]:MCPower:CHANnel:MAIN:COUNt(?), 2-665
- [SENSe]:MCPower:CHANnel:MAIN:INACTive(?), 2-665
- [SENSe]:MCPower:CHANnel:MAIN:SPACing(?), 2-666
- [SENSe]:MCPower:CHIPrate(?), 2-666
- [SENSe]:MCPower:CLEar:RESults, 2-667
- [SENSe]:MCPower:FREquency:STEP:AUTO(?), 2-668
- [SENSe]:MCPower:FREquency:STEP(?), 2-668
- [SENSe]:MCPower:NFLoor:STATe(?), 2-669
- [SENSe]:MCPower:OPTimize(?), 2-669
- [SENSe]:MCPower:RCHannels?, 2-670
- [SENSe]:MCPower:RCHannels:MAIN<x>, 2-670
- [SENSe]:MCPower:RCHannels:TOTal, 2-671
- [SENSe]:MCPower:RRCRolloff(?), 2-671
- [SENSe]:MEASurement:FREquency(?), 2-596
- [SENSe]:OBWidth subgroup, 2-672
- [SENSe]:OBWidth:AVERage:COUNt(?), 2-673
- [SENSe]:OBWidth:AVERage(?), 2-673

- [:SENSe]:OBWidth:BANDwidth[:BWIDth]
 - [:RESolution]:ACTual?, 2-675
- [:SENSe]:OBWidth:CLEar:RESults, 2-676
- [:SENSe]:OBWidth:FREQuency:CENTer(?), 2-676
- [:SENSe]:OBWidth:FREQuency:STEP:AUTO(?), 2-677
- [:SENSe]:OBWidth:FREQuency:STEP(?), 2-677
- [:SENSe]:OBWidth:PERCent(?), 2-678
- [:SENSe]:OBWidth:XDBLevel(?), 2-678
- [:SENSe]:PHVTime subgroup, 2-679
- [:SENSe]:PHVTime:CLEar:RESults, 2-679
- [:SENSe]:PHVTime:FREQuency:CENTer(?), 2-680
- [:SENSe]:PHVTime:FREQuency:SPAN(?), 2-681
- [:SENSe]:PHVTime:FREQuency:STARt(?), 2-681
- [:SENSe]:PHVTime:FREQuency:STEP:AUTO(?), 2-682
- [:SENSe]:PHVTime:FREQuency:STEP(?), 2-682
- [:SENSe]:PHVTime:FREQuency:STOP(?), 2-683
- [:SENSe]:PHVTime:MAXTracepoints(?), 2-684
- [:SENSe]:POWEr:UNITs(?), 2-597
- [:SENSe]:PULSe subgroup (Option 20 only), 2-685
- [:SENSe]:PULSe:ANALyze:LEVel:FIFTy(?), 2-686
- [:SENSe]:PULSe:ANALyze:LEVel:HUNDred(?), 2-687
- [:SENSe]:PULSe:ANALyze:LEVel(?), 2-686
- [:SENSe]:PULSe:ANALyze:MEASurement:TIME:
 - AUTO(?), 2-688
- [:SENSe]:PULSe:ANALyze:MEASurement:TIME:
 - STARt(?), 2-689
- [:SENSe]:PULSe:ANALyze:MEASurement:TIME:
 - STOP(?), 2-689
- [:SENSe]:PULSe:ANALyze:PMLocation(?), 2-690
- [:SENSe]:PULSe:ANALyze:POINt:LOCation(?), 2-690
- [:SENSe]:PULSe:ANALyze:RFAlI(?), 2-691
- [:SENSe]:PULSe:ANALyze:RIPple(?), 2-691
- [:SENSe]:PULSe:CARRier:OFFSet(?), 2-692
- [:SENSe]:PULSe:CARRier:SEARch(?), 2-692
- [:SENSe]:PULSe:DETEct:MEASurement(?), 2-693
- [:SENSe]:PULSe:DETEct:NUMBer(?), 2-694
- [:SENSe]:PULSe:DETEct:POWEr[:THReshold](?), 2-695
- [:SENSe]:PULSe:DETEct:TIME[:THReshold](?), 2-695
- [:SENSe]:PULSe:FILTer:BANDwidth[:BWIDth](?), 2-696
- [:SENSe]:PULSe:FILTer:MEASurement(?), 2-697
- [:SENSe]:PULSe:FREFeRence:AUTO(?), 2-698
- [:SENSe]:PULSe:FREFeRence:CHIRpbw(?), 2-699
- [:SENSe]:PULSe:FREFeRence:OFFSet(?), 2-699
- [:SENSe]:PULSe:MODulation:TYPE(?), 2-700
- [:SENSe]:PULSe:SIGNal:TYPE(?), 2-700
- [:SENSe]:REANalyze, 2-598
- [:SENSe]:ROSCillator:SOURce(?), 2-599
- [:SENSe]:SGRam subgroup, 2-701
- [:SENSe]:SGRam:BANDwidth[:BWIDth]:OPTimization(?), 2-702
- [:SENSe]:SGRam:BANDwidth[:BWIDth]:RESolution(?), 2-702
- [:SENSe]:SGRam:BANDwidth[:BWIDth]:RESolution:
 - ACTual?, 2-703
- [:SENSe]:SGRam:BANDwidth[:BWIDth]:RESolution:
 - AUTO(?), 2-703
- [:SENSe]:SGRam:BANDwidth[:BWIDth]:RESolution:
 - MODE(?), 2-704
- [:SENSe]:SGRam:COLor:MAX(?), 2-706
- [:SENSe]:SGRam:COLor:MIN(?), 2-706
- [:SENSe]:SGRam:COLor(?), 2-705
- [:SENSe]:SGRam:FFT:WINDow(?), 2-707
- [:SENSe]:SGRam:FREQuency:CENTer(?), 2-708
- [:SENSe]:SGRam:FREQuency:SPAN:BANDwidth:
 - RESolution:RATio(?), 2-709
- [:SENSe]:SGRam:FREQuency:SPAN:MAXimum, 2-710
- [:SENSe]:SGRam:FREQuency:SPAN(?), 2-709
- [:SENSe]:SGRam:FREQuency:STARt(?), 2-710
- [:SENSe]:SGRam:FREQuency:STEP:AUTO(?), 2-711
- [:SENSe]:SGRam:FREQuency:STEP(?), 2-711
- [:SENSe]:SGRam:FREQuency:STOP(?), 2-712
- [:SENSe]:SPECtrum subgroup, 2-713
- [:SENSe]:SPECtrum:BANDwidth[:BWIDth]:
 - OPTimization(?), 2-714
- [:SENSe]:SPECtrum:BANDwidth[:BWIDth]:
 - RESolution:ACTual?, 2-715
- [:SENSe]:SPECtrum:BANDwidth[:BWIDth]:
 - RESolution:AUTO(?), 2-715
- [:SENSe]:SPECtrum:BANDwidth[:BWIDth]:
 - RESolution:MODE(?), 2-716
- [:SENSe]:SPECtrum:BANDwidth[:BWIDth]:
 - RESolution[?], 2-714
- [:SENSe]:SPECtrum:CLEar:RESults, 2-716
- [:SENSe]:SPECtrum:FFT:WINDow(?), 2-717
- [:SENSe]:SPECtrum:FREQuency:CENTer(?), 2-718
- [:SENSe]:SPECtrum:FREQuency:SPAN:BANDwidth:
 - RESolution:RATio(?), 2-719
- [:SENSe]:SPECtrum:FREQuency:SPAN(?), 2-719
- [:SENSe]:SPECtrum:FREQuency:STARt(?), 2-720
- [:SENSe]:SPECtrum:FREQuency:STEP:AUTO(?), 2-721
- [:SENSe]:SPECtrum:FREQuency:STEP(?), 2-721
- [:SENSe]:SPECtrum:FREQuency:STOP(?), 2-722
- [:SENSe]:SPECtrum:LENGth:ACTual?, 2-601
- [:SENSe]:SPECtrum:LENGth:AUTO(?), 2-601
- [:SENSe]:SPECtrum:LENGth(?), 2-600

[SENSe]:SPEctrum:MAX:SPAN, 2-723
[SENSe]:SPEctrum:POINts:COUNt(?), 2-723
[SENSe]:SPEctrum:STARt(?), 2-602
[SENSe]:SPEctrum:TIME:MODE(?), 2-603
[SENSe]:TOVerview subgroup, 2-724
[SENSe]:TOVerview:FREQuency:CENTer(?), 2-725
[SENSe]:TOVerview:MAXTracepoints(?), 2-725
SI prefix and unit, 2-7
Special characters, 2-5
Specifying the file, 2-445
*SRE(?), 2-63
STATus command group, 2-48
STATus commands, 2-727
:STATus:ACPower:EVENTs?, 2-729
:STATus:AVTime:EVENTs?, 2-730
:STATus:CCDF:EVENTs?, 2-731
:STATus:CONSt:EVENTs?, 2-732
:STATus:DPSA:EVENTs?, 2-733
:STATus:EVM:EVENTs?, 2-734
:STATus:FVTime:EVENTs?, 2-735
:STATus:IQVTime:EVENTs?, 2-736
:STATus:MCPower:EVENTs?, 2-737
:STATus:MERRor:EVENTs?, 2-738
:STATus:OBWidth:EVENTs?, 2-739
:STATus:OPERation:CONDition?, 2-740
:STATus:OPERation:ENABle(?), 2-740
:STATus:OPERation:NTRansition(?), 2-741
:STATus:OPERation:PTRansition(?), 2-742
:STATus:OPERation[:EVENT]?, 2-741
:STATus:PERRor:EVENTs?, 2-743
:STATus:PHVTime:EVENTs?, 2-744
:STATus:PRESet, 2-744
:STATus:PULSe:RESult:EVENTs?, 2-745
:STATus:PULSe:STATistics:EVENTs?, 2-746
:STATus:PULSe:TRACe:EVENTs?, 2-747
:STATus:QUEStionable:CALibration:CONDition?, 2-750
:STATus:QUEStionable:CALibration:ENABle(?), 2-751
:STATus:QUEStionable:CALibration:NTRansition(?), 2-753
:STATus:QUEStionable:CALibration:PTRansition(?), 2-754
:STATus:QUEStionable:CALibration[:EVENT]?, 2-752
:STATus:QUEStionable:CONDition?, 2-748
:STATus:QUEStionable:ENABle(?), 2-748
:STATus:QUEStionable:FREQuency:CONDition?, 2-754
:STATus:QUEStionable:FREQuency:ENABle(?), 2-755
:STATus:QUEStionable:FREQuency:NTRansition(?), 2-757

:STATus:QUEStionable:FREQuency:PTRansition(?), 2-758
:STATus:QUEStionable:FREQuency[:EVENT]?, 2-756
:STATus:QUEStionable:NTRansition(?), 2-749
:STATus:QUEStionable:PTRansition(?), 2-750
:STATus:QUEStionable[:EVENT]?, 2-749
:STATus:SGRAM:EVENTs?, 2-759
:STATus:SPEctrum:EVENTs?, 2-760
:STATus:SQUALity:EVENTs?, 2-761
*STB?, 2-64
Syntax, command, 2-1
SYSTem command group, 2-49
SYSTem commands, 2-763
:SYSTem:COMMunicate:GPiB[:SELF]:ADDRes(?), 2-764
:SYSTem:DATE(?), 2-764
:SYSTem:ERRor:ALL?, 2-765
:SYSTem:ERRor:CODE:ALL?, 2-766
:SYSTem:ERRor:CODE[:NEXT]?, 2-767
:SYSTem:ERRor:COUNt?, 2-767
:SYSTem:ERRor[:NEXT]?, 2-768
:SYSTem:OPTions?, 2-769
:SYSTem:PRESet, 2-769
:SYSTem:TIME(?), 2-770
:SYSTem:VERSion?, 2-770

T

TekVISA, 1-6
TRACe command group, 2-50
TRACe commands, 2-771
:TRACe:FVTime subgroup, 2-798
:TRACe:FVTime:AVERage:COUNt(?), 2-799
:TRACe:FVTime:FREeze(?), 2-801
:TRACe:FVTime:FUNCTion(?), 2-801
:TRACe:FVTime(?), 2-798
:TRACe:IQVTime subgroup, 2-802
:TRACe:IQVTime:AVERage:COUNt(?), 2-803
:TRACe:IQVTime:COUNt:ENABle(?), 2-804
:TRACe:IQVTime:COUNt:RESet, 2-804
:TRACe:IQVTime:COUNt(?), 2-803
:TRACe:IQVTime:ENABle:I(?), 2-805
:TRACe:IQVTime:ENABle:Q(?), 2-805
:TRACe:IQVTime:FREeze(?), 2-806
:TRACe:IQVTime:FUNCTion(?), 2-806
:TRACe:IQVTime:SElect:I(?), 2-807
:TRACe:IQVTime:SElect:Q(?), 2-808
:TRACe:OBW subgroup, 2-809
:TRACe:OBW:MAXHold(?), 2-809
:TRACe:PHVTime subgroup, 2-810
:TRACe:PHVTime:COUNt:ENABle(?), 2-812

- :TRACe:PHVTime:COUNT:RESet, 2-812
 - :TRACe:PHVTime:COUNT(?), 2-811
 - :TRACe:PHVTime:FREeze(?), 2-813
 - :TRACe:PHVTime:FUNCTION(?), 2-813
 - :TRACe:PVTime:AVERage:COUNT(?), 2-811
 - :TRACe:PVTime(?), 2-810
 - :TRACe:SGRAM subgroup, 2-814
 - :TRACe:SGRam:DETection(?), 2-814
 - :TRACe:SGRam:FREeze(?), 2-815
 - :TRACe:SGRam:FUNCTION:TIME(?), 2-816
 - :TRACe:SGRam:FUNCTION(?), 2-815
 - :TRACe:SGRam:SElect:LINE(?), 2-816
 - :TRACe<x>:AVTime, 2-772
 - :TRACe<x>:AVTime:AVERage:COUNT(?), 2-773
 - :TRACe<x>:AVTime:AVERage:RESet, 2-774
 - :TRACe<x>:AVTime:COUNT:ENABLE(?), 2-776
 - :TRACe<x>:AVTime:COUNT:RESet, 2-777
 - :TRACe<x>:AVTime:COUNT(?), 2-775
 - :TRACe<x>:AVTime:FREeze(?), 2-777
 - :TRACe<x>:AVTime:FUNCTION(?), 2-778
 - :TRACe<x>:AVTime:LEFToperand(?), 2-779
 - :TRACe<x>:AVTime:RIGHToperand(?), 2-780
 - :TRACe<x>:AVTime:SElect(?), 2-781
 - :TRACe<x>:AVTime(?), 2-773
 - :TRACe<x>:CCDF subgroup, 2-782
 - :TRACe<x>:CCDF:FREeze(?), 2-782
 - :TRACe<x>:CCDF:SElect(?), 2-783
 - :TRACe<x>:CCDF:SHOW(?), 2-784
 - :TRACe<x>:CCDF:X(?), 2-785
 - :TRACe<x>:CCDF:Y?, 2-786
 - :TRACe<x>:CONSte subgroup, 2-787
 - :TRACe<x>:CONSte:MODE(?), 2-787
 - :TRACe<x>:DPSA subgroup, 2-788
 - :TRACe<x>:DPSA:AVERage:COUNT(?), 2-789
 - :TRACe<x>:DPSA:COLor:INTensity(?), 2-790
 - :TRACe<x>:DPSA:DOT:PERsistent:TYPE(?), 2-791
 - :TRACe<x>:DPSA:DOT:PERsistent:VARiable(?), 2-792
 - :TRACe<x>:DPSA:DOT:PERsistent(?), 2-790
 - :TRACe<x>:DPSA:FREeze(?), 2-793
 - :TRACe<x>:DPSA:FUNCTION(?), 2-794
 - :TRACe<x>:DPSA:LEFToperand(?), 2-795
 - :TRACe<x>:DPSA:RIGHToperand(?), 2-796
 - :TRACe<x>:DPSA:SElect(?), 2-797
 - :TRACe<x>:DPSA(?), 2-789
 - :TRACe<x>:FVTime:COUNT:ENABLE(?), 2-800
 - :TRACe<x>:FVTime:COUNT:RESet, 2-800
 - :TRACe<x>:FVTime:COUNT(?), 2-799
 - :TRACe<x>:SPECtrum subgroup, 2-817
 - :TRACe<x>:SPECtrum:AVERage:COUNT(?), 2-819
 - :TRACe<x>:SPECtrum:AVERage:RESet, 2-819
 - :TRACe<x>:SPECtrum:COUNT:ENABLE(?), 2-821, 2-822
 - :TRACe<x>:SPECtrum:COUNT(?), 2-820
 - :TRACe<x>:SPECtrum:DETection(?), 2-823
 - :TRACe<x>:SPECtrum:FREeze(?), 2-824
 - :TRACe<x>:SPECtrum:FUNCTION(?), 2-825
 - :TRACe<x>:SPECtrum:LEFToperand(?), 2-826
 - :TRACe<x>:SPECtrum:RIGHToperand(?), 2-827
 - :TRACe<x>:SPECtrum:SElect(?), 2-828
 - :TRACe<x>:SPECtrum(?), 2-818
 - *TRG, 2-65
 - TRIGger command group, 2-53
 - TRIGger commands, 2-829
 - :TRIGger:MASK:NEW, 2-830
 - :TRIGger:MASK:OPEN, 2-831
 - :TRIGger:MASK:SAVE, 2-831
 - :TRIGger[SEquence]:ADVanced:SWEEP:MODE(?), 2-832
 - :TRIGger[SEquence]:EVENT:EXTFront:IMPedance(?), 2-832
 - :TRIGger[SEquence]:EVENT:EXTFront:LEVel(?), 2-833
 - :TRIGger[SEquence]:EVENT:EXTFront:SLOPe(?), 2-833
 - :TRIGger[SEquence]:EVENT:EXTRear:SLOPe(?), 2-834
 - :TRIGger[SEquence]:EVENT:GATed(?), 2-834
 - :TRIGger[SEquence]:EVENT:INPut:FMASK:VIOLation(?), 2-835
 - :TRIGger[SEquence]:EVENT:INPut:LEVel(?), 2-836
 - :TRIGger[SEquence]:EVENT:INPut:SLOPe(?), 2-836
 - :TRIGger[SEquence]:EVENT:INPut:TDBWidth:ACTual?, 2-837
 - :TRIGger[SEquence]:EVENT:INPut:TDBWidth:STATe(?), 2-838
 - :TRIGger[SEquence]:EVENT:INPut:TDBWidth(?), 2-837
 - :TRIGger[SEquence]:EVENT:INPut:TYPE(?), 2-838
 - :TRIGger[SEquence]:EVENT:SOURce(?), 2-839
 - :TRIGger[SEquence]:FORCed(?), 2-840
 - :TRIGger[SEquence]:IMMediate, 2-840
 - :TRIGger[SEquence]:STATus(?), 2-841
 - :TRIGger[SEquence]:TIME:DELay(?), 2-842
 - :TRIGger[SEquence]:TIME:POSition(?), 2-842
- U**
- Unit and SI prefix, 2-7
 - UNIT command group, 2-53
 - UNIT commands, 2-843

:UNIT:POWer(?), 2-844

W

*WAI, 2-65