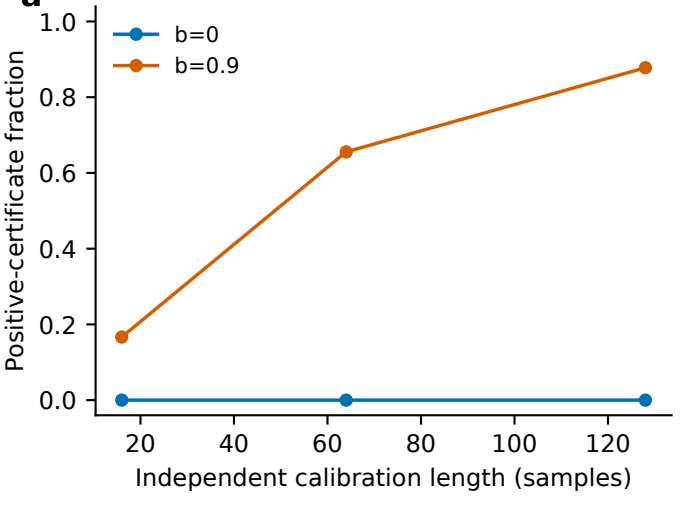
a
b=0
b=0.9
Positive-certificate fraction
1.0
0.8
0.6
0.4
0.2
0.0
20
40
60
80
100
120
Independent calibration length (samples)

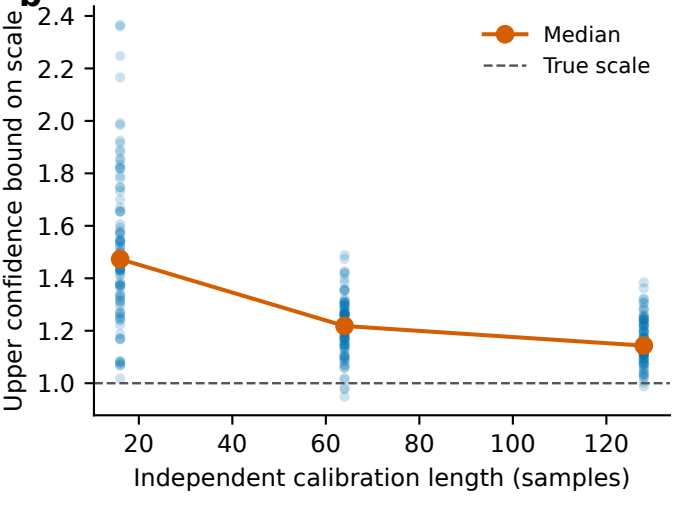
b
Median
True scale
Upper confidence bound on scale
2.4
2.2
2.0
1.8
1.6
1.4
1.2
1.0
20
40
60
80
100
120
Independent calibration length (samples)