


Reference PPG spectral sensitivity: a single-recording case study

UBFC subject3 | Contact PPG reference analysis, not a comparison of model performance

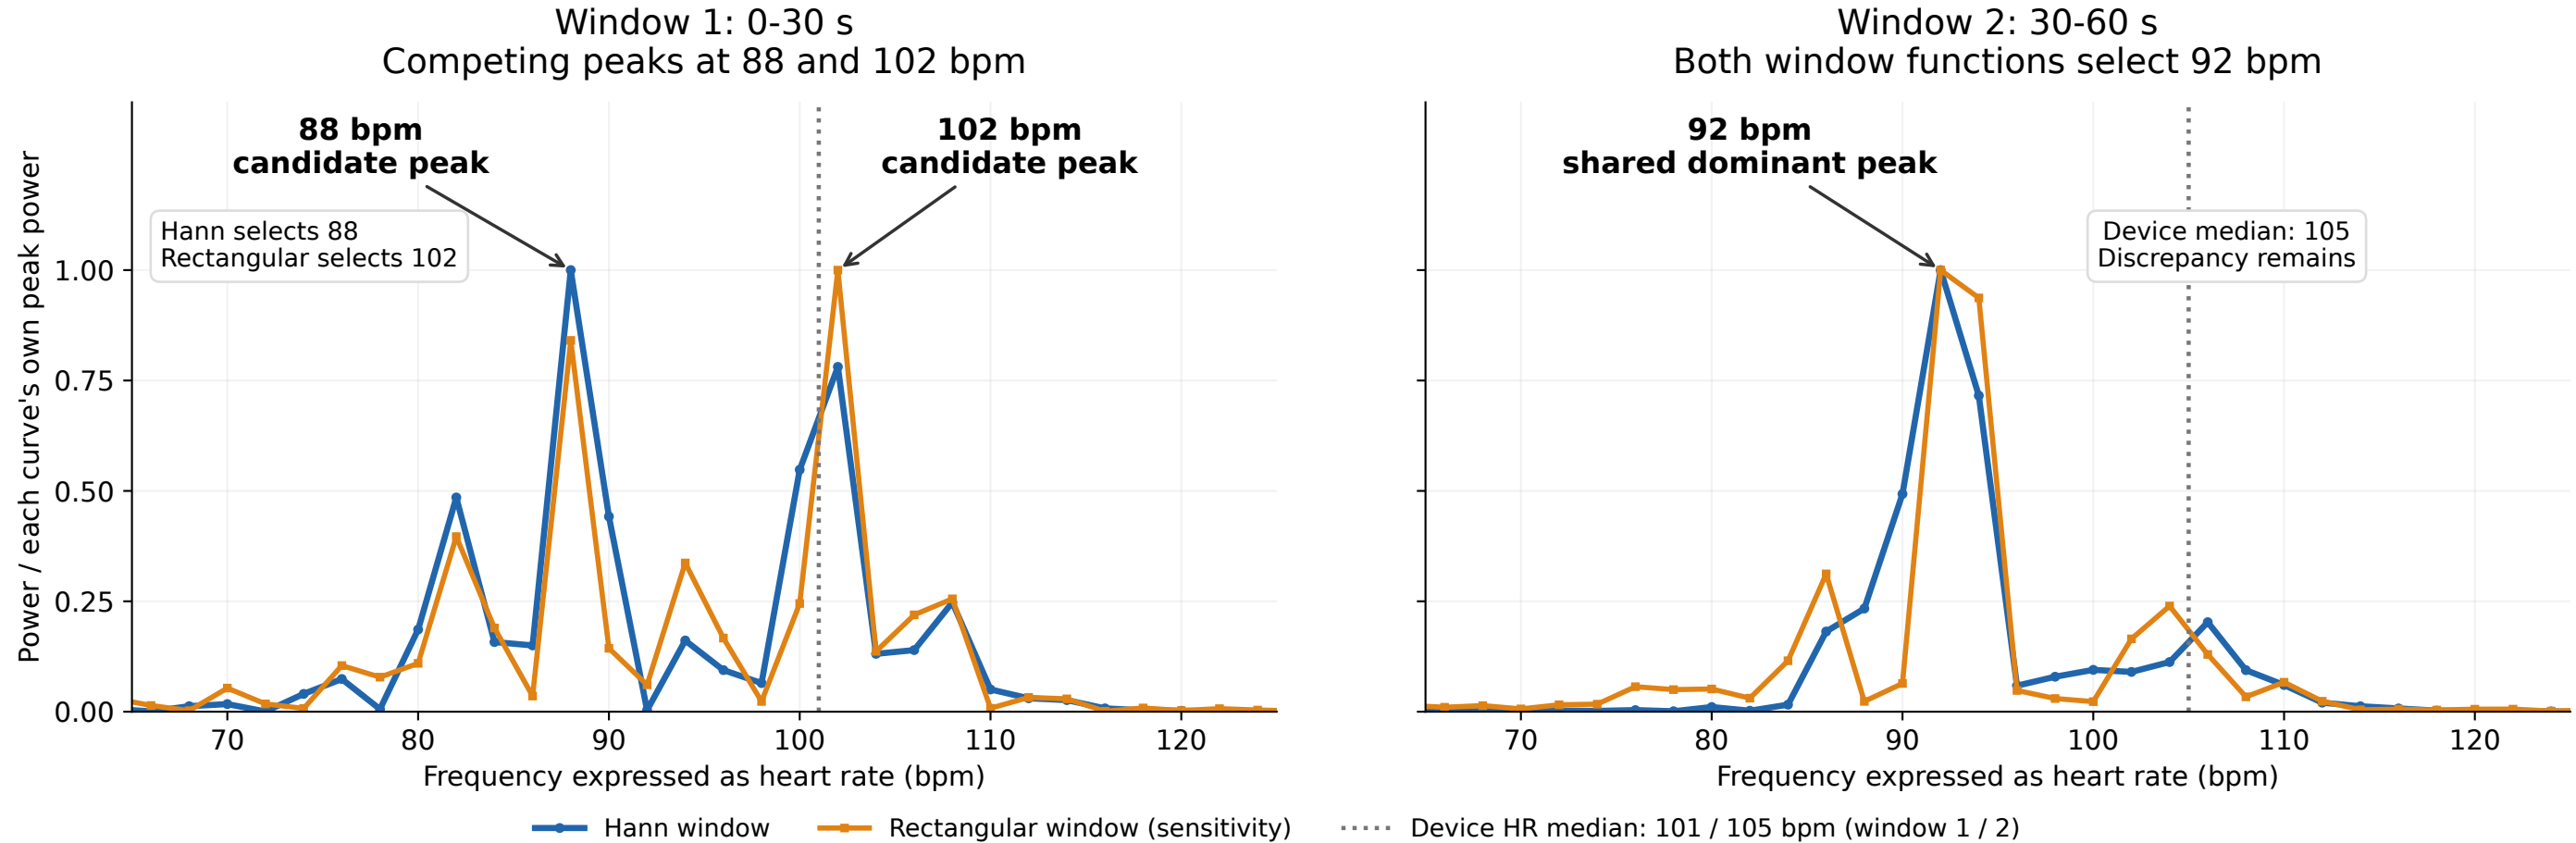

Each curve is normalized by its own peak within 45-150 bpm: compare peak locations and relative shapes, not absolute power.
Identical 30 Hz interpolated PPG; no bandpass or zero padding; 2 bpm frequency bins. Original evaluation retained; no device-guided selection.
Two windows from one recording cannot establish the true heart rate or represent the full UBFC dataset.