METAFuN Manual of Procedures

Project Overview

The Manual of Procedures describes the methods of the UAB Alzheimer's Disease Research Center (ADRC) project “A Multimodal Examination of Tau and Functional Networks (METAFuN)”. This manual covers the out-of-scanner behavioral tasks as well as in-scanner behavioral tasks.

Participants are recruited through the UAB ADRC. ADRC Participant ID and Imaging Tracer used can be found in the calendar event located in the “ADRC TAU SCAN” Outlook calendar. The time a visit is scheduled for on this calendar is the time the participant is told to arrive at the UAB Wallace Tumor Institute (WTI) Basement Floor PET Waiting Room.

Order of operations is generally as follows:

1) Meet Participants at the PET/MRI waiting area (Basement of WTI).
2) ADRC/Radiology staff invites them to an uptake room to begin radiotracer injection.
3) Radiotracer injection starts a 75 minute timer before the MRI scans must begin.
4) After injection, METAFUN staff will conduct behavioral testing (~60 min).
5) ADRC/Radiology staff escort the participant into the PET MRI room, MR technicians conduct safety protocols, technicians place the participant inside the PET/MR scanner, and METAFUN staff set up hardware.
6) Conduct sequence of MRI scans (PET, Structural, and Functional) (~60 min)
7) Extract data from MRI scanner and Behavioral equipment (~20 min)

Study Contacts

Name	Email	Role
Dr. Kristina Visscher	kmv@uab.edu	Principal Investigator
Dr. David Jin	djin@uab.edu	Research Staff
Dr. Pinar Demirayak	pinarde@uab.edu	Research Staff
Pauline Stewart	pstew@uab.edu	Research Staff
Alex Kahn	atkahn@uab.edu	Research Staff

Glossary

ADRC = Alzheimer’s Disease Research Center, *VIS* = Visual Stimuli, *AUD* = Auditory Stimuli, *SAT* = Sensory Attention Task, *NNL* = NordicNeuroLabs

Study Timeline

Session	Detailed Procedures	Time
Behavioral Assessments	I. Hardware Setup a. NIH Toolbox iPad b. Behavioral Laptop II. Sensory Acuity Assessments a. Near Visual Acuity b. Hearing Threshold c. Words-in-Noise III. Behavioral Tasks a. Stroop Squared Task b. Sensory Attention Task Practice	60 min
PET/MR Imaging Assessments	I. Hardware Setup a. MRI Equipment Setup b. Eye Tracking Setup c. Nordic NeuroLabs Tablet Setup II. PET/MR Structural Scans (Localizer & T1) 1. 3-Plane Localizer Tau PET Simultaneous Acquisition 2. T1 BRAVO III. PET/MR Functional Scans (Rest, Task, & Field Map) 3. Sensory Attention Task Run 1 BOLD 4. Field Map 1 - ALT ON 5. Field Map 1 - ALT OFF 6. Sensory Attention Task Run 2 BOLD 7. Sensory Attention Task Run 3 BOLD 8. Field Map 2 - ALT ON 9. Field Map 2 - ALT OFF 10. Sensory Attention Task Run 4 BOLD 11. Post-Task Resting State 1 BOLD 12. Field Map 3 - ALT ON 13. Field Map 3 - ALT OFF 14. Post-Task Resting State 2 BOLD IV. PET/MR Structural Scans (T2) 15. Sagittal T2	60 min
Data Transfer	I. Anonymize Data II. Transfer Options a. XNAT b. 2TB Hard Drive c. Thumb Drive	20 min

Behavioral Assessments

I. Hardware Setup

1. All materials for this study are located in the rolling computer bag. All materials listed below including their requisite charging cables should be kept in this bag at all times.
    a. Check Behavioral Laptop is fully charged
        i. If not, allow computer to charge during the NIH Toolbox portion of assessments
    b. Check NIH Toolbox iPad and Bluetooth Keyboard are charged
    c. Check Sennheiser HD 280 Pro Headphones, Headphone Jack Adapter, and tape measure are with testing materials
    d. Check for proper USB drive to export data from laptop and iPad

2. Make sure iPad is Connected to Bluetooth and WiFi, Do Not Disturb is turned on, Brightness is set to the maximum level, and all other apps are closed
3. Obtain subject participant ID (ADC ID) from staff or ADRC Tau Scan Calendar.
4. Meet the participant following PET tracer injection and **note Uptake Room #**
5. Instruct care partners to stay in an appropriate waiting area.

★ ONCE TRACER IS INJECTED, PARTICIPANT MUST BE AT PET/MR IN 60 MINUTES!

II. Sensory Acuity Assessments

1. Open assessment tablet
    a. Turn On “Do Not Disturb” and Turn OFF “WiFi”
    b. iPad Passcode: 1719
2. Open NIH Toolbox App (Located on bottom doc bar)
    a. NIH Toolbox Passcode: 17191719

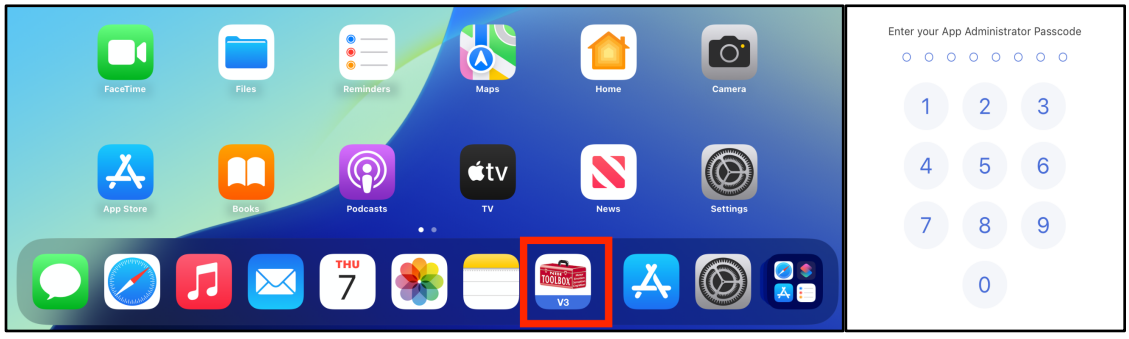

3. Ask Participants if they have
    a. **Corrected Vision: Yes or No**
    b. **Corrected Hearing: Yes or No**
4. Select "**New Participant**"
    a. Enter "**Identifier**"
    b. Enter "**Date of Birth**"
    c. Enter "**Handedness**"
    d. Click "**Next**" → Click "**Save**"

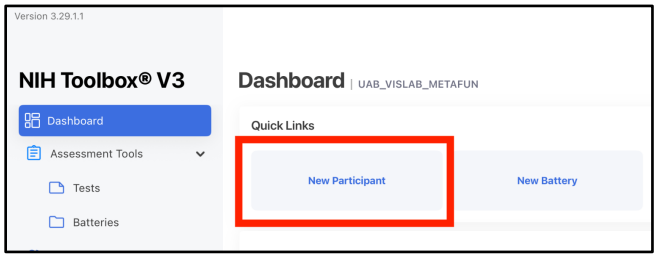

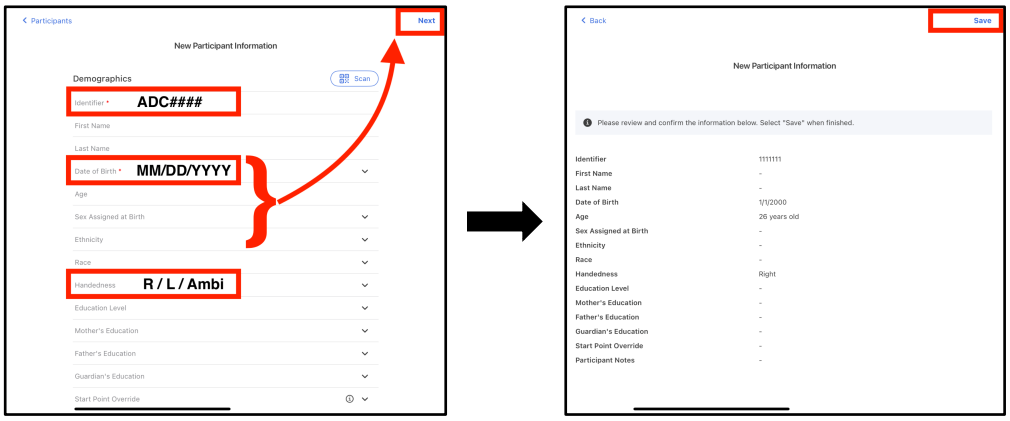

e. Click "**New Assessment**" → Click "**Add Tools**" → Select "**Batteries**"

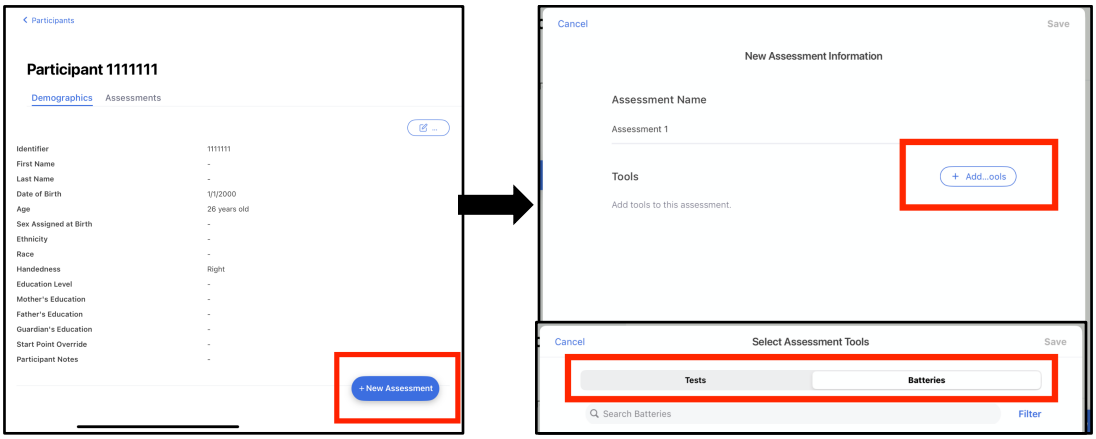

i. <u>If participant has corrected vision</u>: Select "**METAFUN Prescan Behavioral Assessments - Visual Correction**" → Click "**Save**" → Type "**Corrected Vision**" into the Assessment name → Click "**Save**"

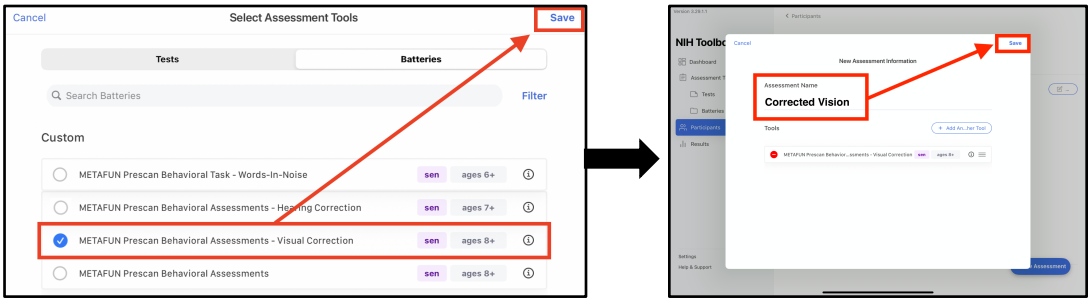

ii. If participant has corrected hearing: Select "**METAFUN Prescan Behavioral Assessments - Hearing Correction**" → Click "**Save**" → Type "**Corrected Hearing**" into the Assessment Name → Click "**Save**"

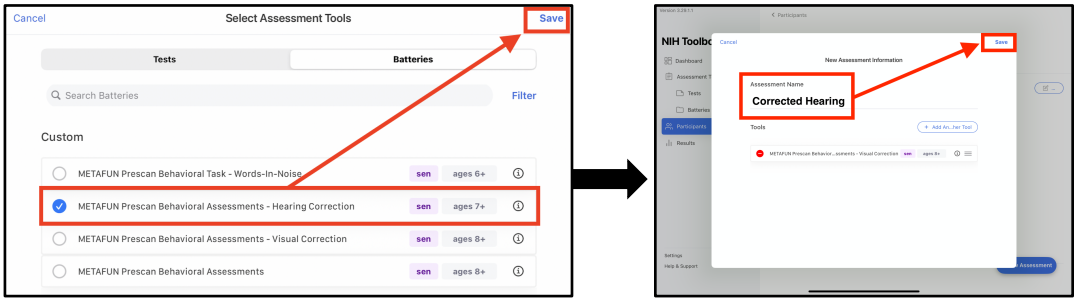

iii. If the participant has neither: Select "**METAFUN Prescan Behavioral Assessments**" → Click "**Save**" → Type "**Uncorrected Assessments**" into the Assessment Name → Click "**Save**"

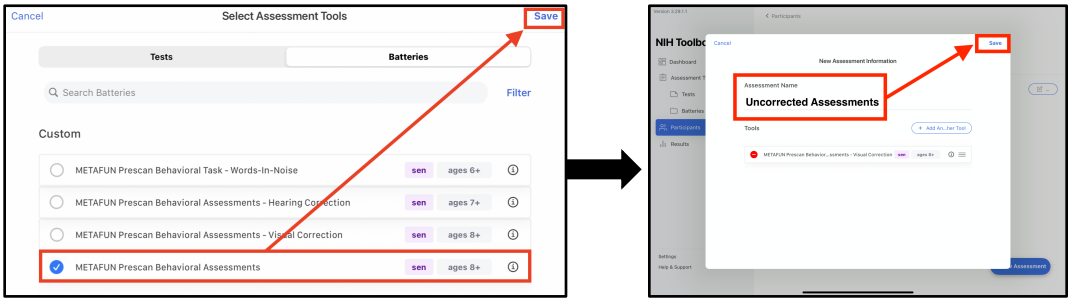

iv. *Note: If attempting to add "Corrected" assessments with the full assessments, you will be shown a duplicate assessment warning").*



5. Select "**Assessments**" tab within Participant profile
   a. To run corrected vision task: Select "**Corrected Vision**" → "**Start Assessment**"
   b. To run corrected hearing task: Select "**Corrected Hearing**" → "**Start Assessment**"
   c. To run uncorrected tasks: Select "**Uncorrected Assessments**" → "**Start Assessment**"

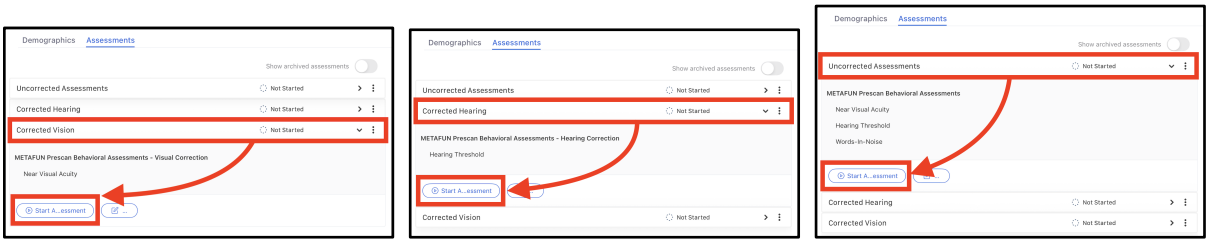

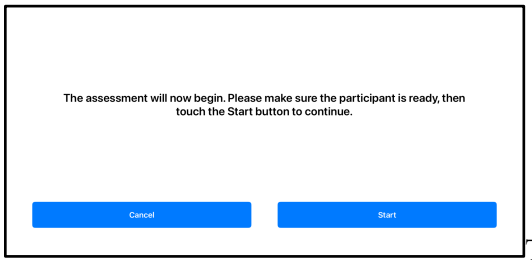

6. Once NIH Toolbox tasks are complete, navigate to the participant completed session by Selecting the participant → Select "**Assessments**" → Select "**Uncorrected Assessments**" → Open the **Assessment Report PDF**
7. Scroll down to Page 2 of the report and locate the results of the Sensory Domain Tasks
    a. For the visual tasks, log the **STATIC VISUAL ACUITY SNELLEN** on the PI sheet
    b. For the auditory tasks, log the **WORDS-IN-NOISE THRESHOLDS** on the PI sheet

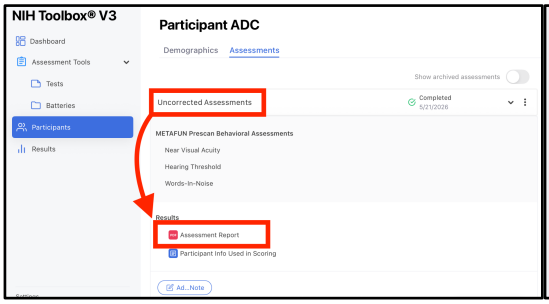

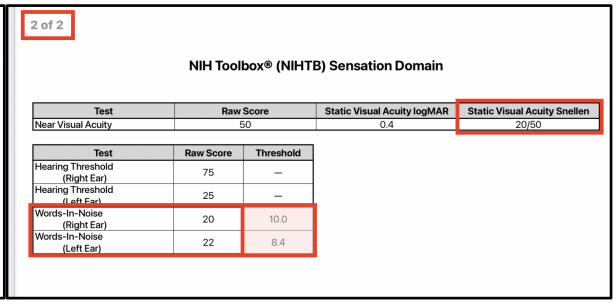

Visual Snellen Acuity	Starting Visual Weber (%)	Words-In-Noise Threshold (Better of 2 Ears)	Starting Auditory Weber (%)
20/20 or Better	50%	3.99 or Lower	50%
20/20.1 – 20/40	75%	4.00 – 7.99	75%
20/40.1 – 20/60	100%	8.00 – 11.99	100%
20/60.1 – 20/80	125%	12.00 – 15.99	125%
20/80.1 or Worse	150%	16.00 or Greater	150%

III. Behavioral Tasks

1. Open Dell behavioral laptop and ensure it is fully charged.
2. Place colored tape over "Q" and "P" keys as left arrow and right arrow, respectively.
3. Username: VisLab / Password: p**a*
4. Open PsychoPy (*default opening window is the PsychoPy Runner*)
    a. Along the menu bar, Click "**View**" → "**Show Coder**". In Coder, select "**File**" → "**Open**"

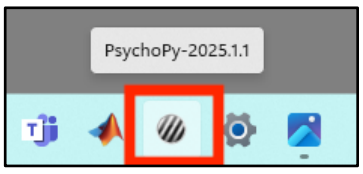

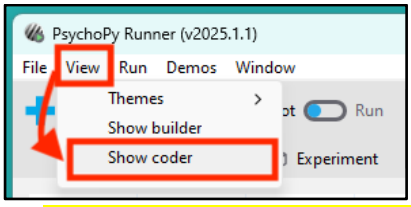

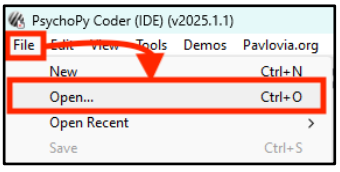

    b. In file browser, Select "**METAFUN_StroopClassic.py**" → "**Open**"
    c. In file browser, Select "**METAFUN_SAT_FinalVersion.py**" → "**Open**"

A. Stroop Squared Task

1. Open "**/Desktop/StroopTaskDemo.pptx**". Explain the task and walk through the powerpoint.

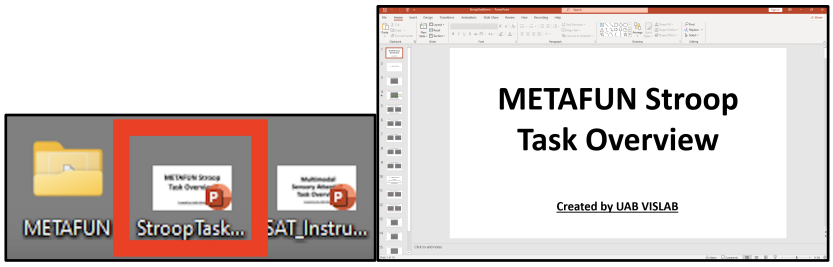

2. Select "**METAFUN_StroopClassic.py**" tab in PsychoPy Coder window

   a. Confirm the experiment toggle is set to "Run"
   b. Click the "**green play button**" in the Desktop section of the top bar to begin the task

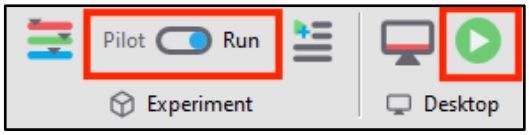

★ *If the experiment toggle is set to "Pilot", the play button will display Orange.* ***THIS IS NOT CORRECT!***



   c. In Trial GUI:
      - Enter Participant ID (Format: ADC#####)
      - Set "Session" to 001 (*Default: 001*).
      - ★ If the participant needs to stop and restart the task, increase "Session" sequentially.

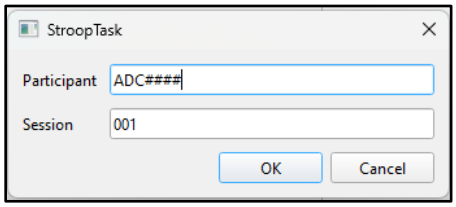

   d. Click "**OK**". This will run the Stroop task.
   Confirm the participant understands the instructions written on screen before proceeding.

B. Sensory Attention Task Practice

1. Open "**/Desktop/SAT_Instructions.pptx**". Explain the task and walk through the powerpoint. Check with the participant that stimuli are visible and audible.

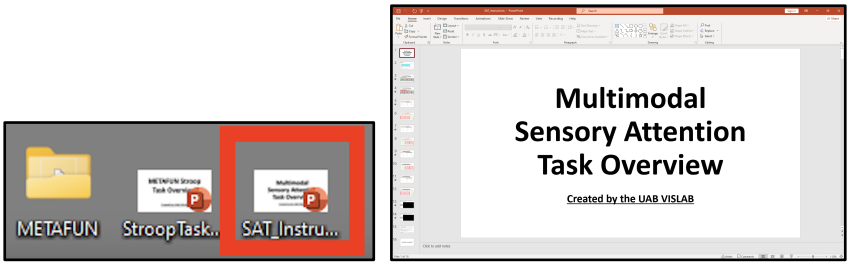

2. Set Behavioral Laptop Volume to 20% and Note Value in PI Sheet



   ★ If the participant requires an increase in volume, increase by increments of 2.

3. Open "**METAFUN_SAT_FinalVersion.py**" tab in PsychoPy Coder



a. Confirm the experiment toggle is set to "Run"
b. Click the "**green play button**" in the Desktop section of the top bar to begin task



c. In Trial GUI:
   - Enter "Participant ID" (ADC####)
   - **Set Starting Modality and note in PI sheet: either "Auditory" or "Visual"**
   - **Input Starting Weber % Values based on NIH Toolbox Performance**
   - Set "Auditory Stimulus Family" to "WhiteNoise_RippleRate"
   - Set "Auditory Output Device" to "**Headphones(2- RealTek(R) Audio)**"

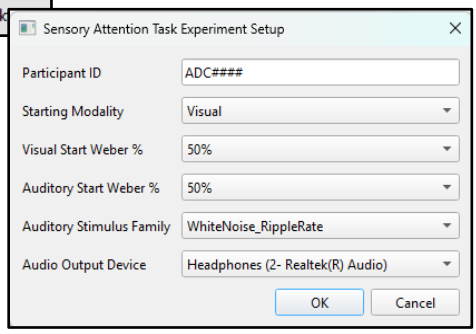

d. Click "**OK**". This will run the practice SAT task.

4. On the desktop, Open "**METAFUN**" folder → Open "**MultimodalSwitch_data**" folder
   a. In the folder "MultimodalSwitchData", open the Excel spreadsheet that matches the participant number, and log values onto the PI sheet.
      - **Final Visual Weber % (Column AR: VIS_WEBER_PCT_EXACT)**
      - **Final Auditory Weber % (Column AS: AUD_WEBER_PCT_EXACT)**

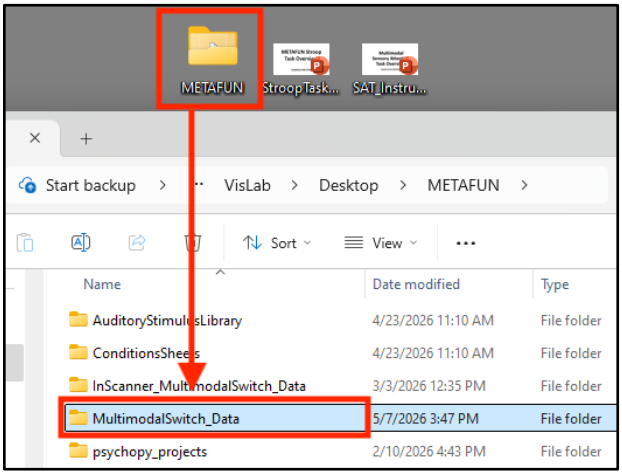



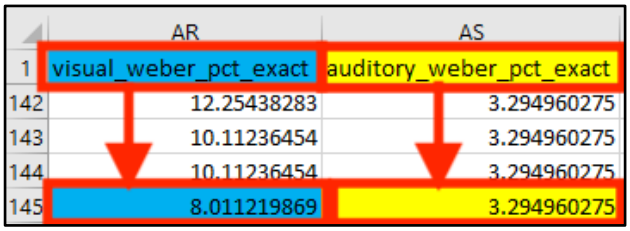

5. After logging the Auditory and Visual Weber percents in the PI sheet, pack up all belongings, and inform ADRC staff that the participant is ready to go to the PET/MR scanner.

PET/MR Imaging Assessments

I. Hardware Setup

A. MRI Equipment Setup

1. Place the frame plate and the NOVA 32 Channel Head Coil with Mirror Attached in position on the scanner bed. *(Handled by PET/MR technologists)*
    a. To confirm the head coil is properly positioned, check that the notches on either side of the head coil, and confirm the notches are securely slotted into the inserts on both sides.
2. Turn on NordicNeuroLabs TV inside the scanning room
    a. The power box is a gray box located on the floor adjacent to the back right corner of the scanner and next to the end of the table along the back wall inside the scan room. The power button will light up green to indicate power is on. The TV will also not display any input unless the HDMI cord is properly plugged into the NordicNeuroLabs Tablet dock.
3. Allow PET/MR Technologist to conduct safety protocols and place participant inside the scanner

B. Eye Tracking Setup

1. In the scanner room, insert the serial cord into ports 107 and 108 in the wall panel. Also ensure that the power cord of the camera is plugged into the surge protector on the equipment room side. Red should be plugged into 107, and white into 108.
2. Connect the power side of the serial cable to the EyeLink Camera.
3. Check that the orange fiber optic data cable is plugged into the camera.
4. Check that no loops have been formed by any cable
5. Turn on the EyeLink Computer
    a. Once open, to the EyeLink or Windows screen arrow and press “Enter” on EyeLink
6. Turn on the capture card computer. User: VisLab, Password: p**a*

7. Unplug the blue USB cable from its position behind the NNL tablet.

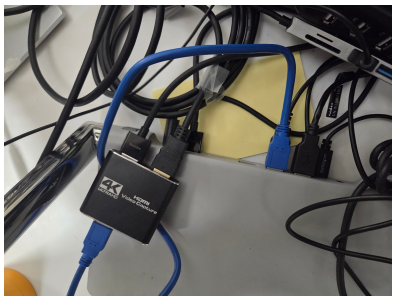

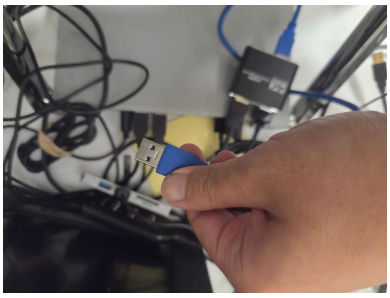

8. Connect the capture card from the EyeLink computer to the right USB hub of the computer
9. Connect the capture card from the NNL tablet to the left USB hub of the capture computer
10. On the capture computer, open OBS
11. In OBS, delete all existing scenes except "NNL and EyeLink Capture".
12. Click the plus sign on the Source sign and select "**Video Capture Device**". In the Video Capture Device, select "**AFN_Cap video**" which corresponds to the EyeLink capture.
    a. Click "**OK**". This will create a window capture of the Eyelink.
    b. Maximize this so that it covers the entire screen.

13. Click the plus sign on the Source sign and select "**Video Capture Device**" again. In the Video Capture Device, select **USB Video**, which corresponds to the NNL capture.
    a. Press OK. This will create a window capture of the NNL tablet.
    b. Resize the window to fit 1/2 of the screen. Ensure participant's eyes are in view.

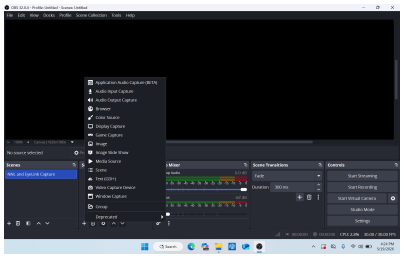

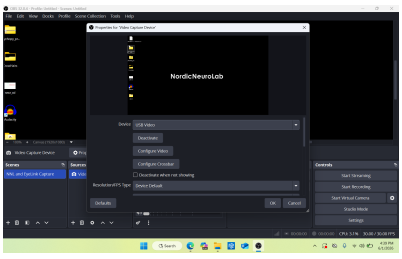

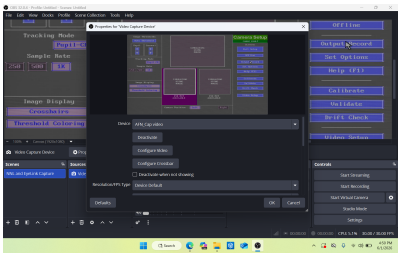

14. Select "**Start Recording**"'

C. Nordic NeuroLabs Tablet Setup

1. Flip both power switches on the NNL sync box to reset. Turn on the NNL sync box.
2. Plug in headphone jack into the NordicNeuroLabs Tablet
3. On the NNL Tablet, open PsychoPy (all three windows should be open: Builder, Runner, Coder)



4. In top menu bar, Select "**View**" → "**Show Builder**"
    a. Select "**File**" → "**Open**" → Select "**METAFUN_SAT_InScanner.psyexp**"
        i. located at /Desktop/psychopy_projects/4_30_versions/randomize_image

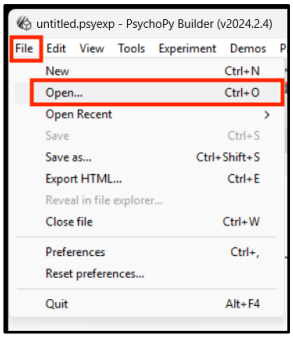

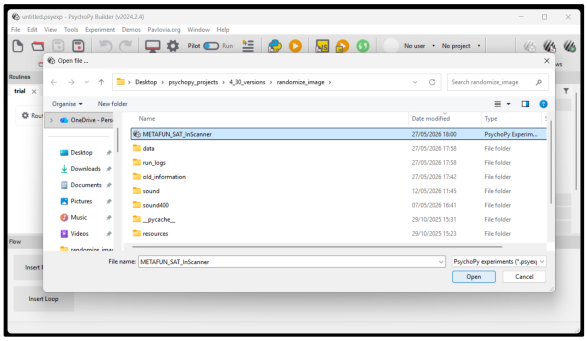

    b. Input Subject ID and Starting Weber Percents in text files (**located at /Desktop/psychopy_projects/4_30_versions/ randomize_image**)

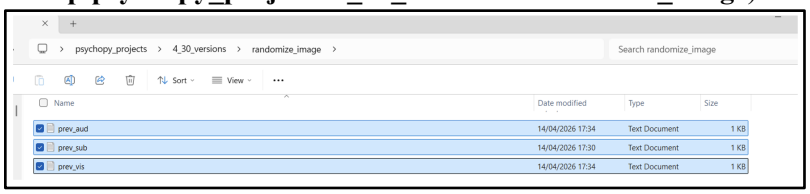

        i. Open "**prev_sub.txt**" and type in the Participant ID *(Format: ADC####)*
        ii. Open "**prev_vis.txt**" → Type in **Final Visual Weber %** *(Format: ##.##)*
        iii. Open "**prev_aud.txt**" → Type in **Final Auditory Weber %** *(Format: ##.##)*

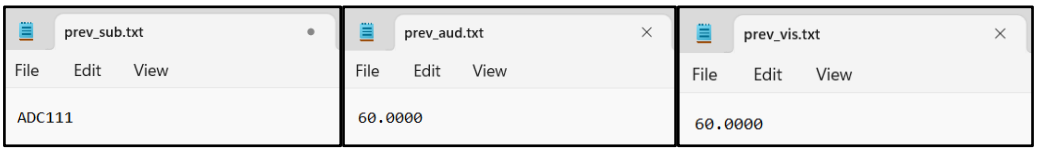

5. Minimize PsychoPy and open "**/Desktop/FixationCross.png**"

~~~~~ MR Technologists will bring the participant into the scanner. ~~~~~

PET/MR Scan Protocols:

- "**1.79 - PET/MR VISLAB Alzheimer's F-18 AV1451 V2 5/27/26**".....(ADRC: AV1451 + Task)
- "**1.68 - PET/MR VISLAB CLARITI MK6240 WITH TASK**".....(CLARITI: MK6240 + Task)
- "**1.101 - VISSCHER ADRC MMS TASK 05/05/2026 FINAL VERSION**".....(Task Sequence Only)
    - ★ *NOTE*: If any errors arise is sequence setup, you can recreate the scans run in the 1.79 and 1.68 protocols be re-adding the 1.101 protocol sequence to the scan
    - ★ When loading the protocol: Set **Study Description = "Project: METAFUN"** for XNAT routing

II. PET/MR Structural Scans (Localizer & T1)

(1) 3-Plane Localizer

1. Click "**3-Plane Localizer**" → "**Save Rx**" → "**Scan**"

INITIALIZE SIMULTANEOUS PET ACQUISITION

1. Begin "**PET Task**", "**MRAC1 - PET BRAIN**", and "**ZTE-MRAC GEM HNU - PET BRAIN**"

2. After simultaneous acquisition begins, sequentially single-click selecting the scans (below), click "**Setup**" → Confirm bounding boxes and number of slices → Select "**Save Rx**"

(2) T1 BRAVO + In-Scanner Task Practice

1. Single Click "**3D_Sag_T1_BRAVO_1mm_Isotropic_Hypersense**" Configure task code for anatomical practice

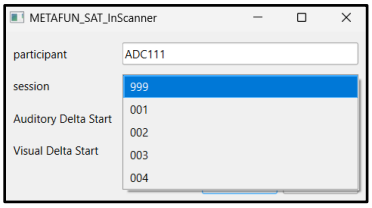



   a. In Psychopy Builder, click the green "Run" symbol
   b. In Task GUI:
      i. Confirm Participant ID matches "prev_sub.txt"
      ii. In "Session" dropdown, set to "999"
      iii. Confirm that "Auditory Delta Start" and "Visual Delta Start" values
         1. In PsychoPy Runner window, values for the input weber %, multiplied weber %, and converted delta values will be shown:
      iv. Click "OK"
   c. Confirm that participant heard test beep
2. Power cycle NNL syncbox and test the participant answer buttons.
   a. On the lower box, when the participant clicks the **left trigger, light #2 will illuminate**
   b. On the lower box, when the participant clicks the **right trigger, light #3 will illuminate**
3. Confirm with the participant that they are ready to begin and that they understand the instructions.
4. ***Simultaneously*** Press "**Space**" on the NNL tablet and "**Start Scan**" button on MRI console

5. Confirm that the Volume number on the sync box is increasing by 1.
6. **Log Final Task Data in PI Sheet**
7. Check in with the participant after the scan and confirm they understand the task instructions
8. Once the run is complete, you can confirm values saved for the next run in the "run_logs" folder

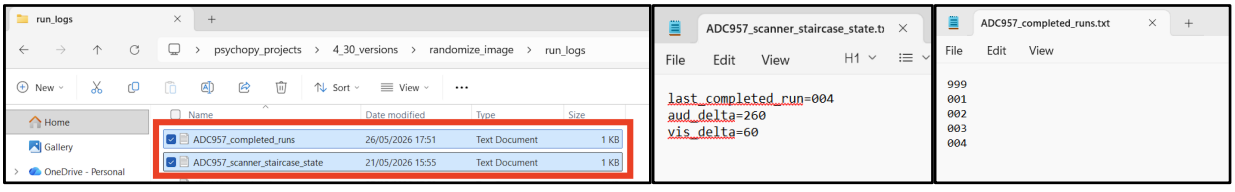

   a. The "completed_runs" text file contains the scan sessions IDs completed in each row
   b. The "scanner_staircase_state" text file contains the last completed run and the final delta value for each modality

III. PET/MR Functional Scans (Rest, Task, & Field Map)

1. Minimize PsychoPy and Open "**FixationCross.png**" on the NNL desktop

2. Power cycle switches on the NNL sync boxes

(3) Sensory Attention Task Run 1 BOLD

1. Single Click "**Ax_Task_Run1_HB2x3_2200TR_2_1iso**" → Open Scan Dropdown Menu and click "**Prep Scan**"
2. In PsychoPy Builder Window, confirm the experiment toggle is set to **RUN** and click the green "Run" button.
    a. Task GUI:
        i. Confirm that the Participant ID matches "prev_sub.txt"
        ii. In the "Session" dropdown, set to "001"
        iii. Confirm "Auditory Delta Start" and "Visual Delta Start" values
        iv. Click OK.

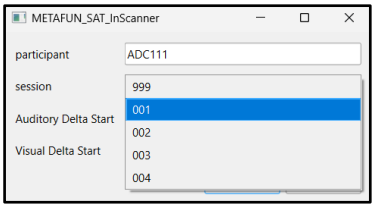

    b. Confirm that participant heard test beep
    c. Press "**Space Bar**" on NNL Tablet keyboard
        i. Confirm NNL syncbox is holding at Volume 1 out of 400
    d. Press "**Scan**" on the MRI console
        i. Confirm on the NNL syncbox screen the number of volumes is increasing by 1 and that the first colored fixation cross appears at Volume 7.
    ★ **IF VOLUMES ARE NOT INCREASING OR TASK DOES NOT START, STOP THE SCAN. We can duplicate the task run scan and restart from the beginning of these instructions**
3. Log Task Run Data in PI Sheet
4. Check in with the participant after BOLD task Run 1.

(4) Field Map 1 - ALT ON

1. Inform participant that we will now run two short scans totalling one minute (field mapping)
2. Click "**ALT_ON_1_Spin_Echo_EPI**" → "**Scan**"

(5) Field Map 1 - ALT OFF

1. Click "**ALT_OFF_1_Spin_Echo_EPI**" → "**Scan**"
2. Check in with participant after field mapping

(6) Sensory Attention Task Run 2 BOLD

1. Single Click "**Ax_Task_Run2_HB2x3_2200TR_2_1iso**" → Open Scan Dropdown Menu and click "**Prep Scan**"
2. In PsychoPy Builder Window, confirm the experiment toggle is set to **RUN** and click the green "Run" button.

a. Task GUI:
    i. Confirm that the Participant ID matches "prev_sub.txt"
    ii. In the "Session" dropdown, set to "002"
    iii. Confirm "Auditory Delta Start" and "Visual Delta Start" values
    iv. Click OK.

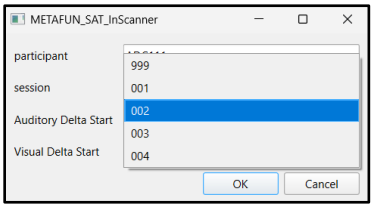

b. Confirm that participant heard test beep
c. Press "**Space Bar**" on NNL Tablet keyboard
    i. Confirm NNL syncbox is holding at Volume 1 out of 400
d. Press "**Scan**" on the MRI console
    i. Confirm on the NNL syncbox screen the number of volumes is increasing by 1 and that the first colored fixation cross appears at Volume 7.

★ **IF VOLUMES ARE NOT INCREASING OR TASK DOES NOT START, STOP THE SCAN. We can duplicate the task run scan and restart from the beginning of these instructions**

3. Log Task Run Data in PI Sheet
4. Check in with the participant after BOLD task Run 1.

(7) Sensory Attention Task Run 3 BOLD

1. Single Click "**Ax_Task_Run3_HB2x3_2200TR_2_1iso**" → Open Scan Dropdown Menu and click "**Prep Scan**"
2. In PsychoPy Builder Window, confirm the experiment toggle is set to **RUN** and click the green "Run" button.
    a. Task GUI:
        i. Confirm that the Participant ID matches "prev_sub.txt"
        ii. In the "Session" dropdown, set to "003"
        iii. Confirm "Auditory Delta Start" and "Visual Delta Start" values
        iv. Click OK.

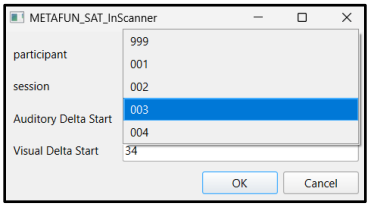

    b. Confirm that participant heard test beep
    c. Press "**Space Bar**" on NNL Tablet keyboard
        i. Confirm NNL syncbox is holding at Volume 1 out of 400
    d. Press "**Scan**" on the MRI console
        i. Confirm on the NNL syncbox screen the number of volumes is increasing by 1 and that the first colored fixation cross appears at Volume 7.

    ★ **IF VOLUMES ARE NOT INCREASING OR TASK DOES NOT START, STOP THE SCAN. We can duplicate the task run scan and restart from the beginning of these instructions**

3. Log Task Run Data in PI Sheet
4. Immediately proceed to Mid-Task Field Maps.

(8) Field Map 2 - ALT ON

1. Inform participant that we will now run two short scans totalling one minute (field mapping)
2. Single Click "**ALT_ON_2_Spin_Echo_EPI**" → "**Scan**"

(9) Field Map 2 - ALT OFF

1. Single Click "**ALT_OFF_2_Spin_Echo_EPI**" → "**Scan**"
2. Check in with participant after field mapping

(10) Sensory Attention Task Run 4 BOLD

1. Single Click "**Ax_Task_Run4_HB2x3_2200TR_2_1iso**" → Open Scan Dropdown Menu and click "**Prep Scan**"
2. In PsychoPy Builder Window, confirm the experiment toggle is set to **RUN** and click the green "Run" button.
    a. Task GUI:
        i. Confirm that the Participant ID matches "prev_sub.txt"
        ii. In the "Session" dropdown, set to "004"
        iii. Confirm "Auditory Delta Start" and "Visual Delta Start" values
        iv. Click OK.

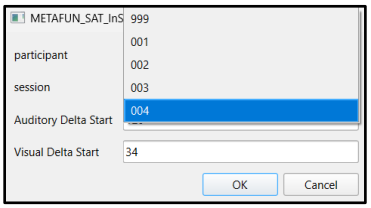

    b. Confirm that participant heard test beep
    c. Press "**Space Bar**" on NNL Tablet keyboard
        i. Confirm NNL syncbox is holding at Volume 1 out of 400
    d. Press "**Scan**" on the MRI console
        i. Confirm on the NNL syncbox screen the number of volumes is increasing by 1 and that the first colored fixation cross appears at Volume 7.

    ★ **IF VOLUMES ARE NOT INCREASING OR TASK DOES NOT START, STOP THE SCAN. We can duplicate the task run scan and restart from the beginning of these instructions**
3. Log Task Run Data in PI Sheet
4. Check in with the participant after BOLD task Run 3.

(11) Post-Task Resting State Run 1 BOLD

1. Read participant instructions on Resting State.
2. Single Click "**Ax Rest 1 HB 2x3 2200TR 2_1 iso**" → "**Scan**"
3. Check in with the participant.

(12) Field Map 3 - ALT ON

1. Inform participant that we will now run two short scans totalling one minute (field mapping)
2. Single Click "**ALT_ON_3_Spin_Echo_EPI**" → "**Scan**"

(13) Field Map 3 - ALT OFF

1. Single Click "**ALT_OFF_3_Spin_Echo_EPI**" → "**Scan**"
2. Check in with participant after field mapping

(14) Post-Task Resting State Run 2 BOLD

1. Read participant instructions on Resting state.
2. Single Click "**Ax Rest 2 HB 2x3 2200TR 2_1 iso**" → "**Scan**"
3. Check in with the participant after the scan.

IV. PET/MR Structural Scans (T2s)

(15) SAG T2

1. Check in with the participant after section III.
2. Single Click "**SAG_3D_T2**" → "**Scan**"

~~~~~ MR Technologists will bring the participant out of the scanner. ~~~~~

Cleanup

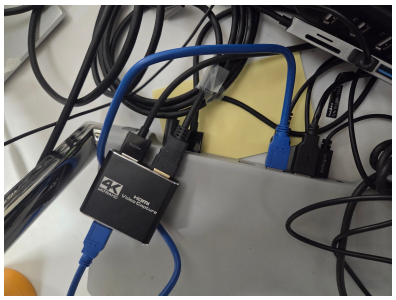

1. On the EyeLink laptop, press "**Stop Recording**" in OBS.
    a. Unplug the blue cable and return to its original place on the NNL tablet base
    b. Unplug the EyeLink Video Capture cord and wrap around the NNL tablet base.
2. Check that the answer paddles are coiled and placed on the wall
3. Turn off the EyeLink Computer
4. Remove the orange fiber optic cable from the EyeLink camera, coil, and hang by the drawer
5. Unplug EyeLink serial cable from the wall inside the scan room and place it inside the cabinet.

Data Transfer

I. Anonymize data

a. After all scanning is complete, at the top of the scan window select "End" → Reason For Ending = "Successfully Completed" → "End" → "Accept"
b. Now in the Protocol Manager tab (middle of the three icons at the top of the console screen), scroll to the top of the Protocol window (upper window) and find the scan session matching the session ID and ADC ID
c. Select the protocol by double clicking and in the lower Series Window, Shift+Select all series
d. With all the series selected, select "Tools" → "De-Identification"

i. **This step can not be interrupted! If there are scans immediately following ours, only use XNAT for data transfer and complete this step and the 2TB SSD step later!**

e. De-Identification will create an exact copy of the series, prepended with "ANON"

f. Scroll to the bottom of the upper Protocol Window and find the now anonymized series

II. Transfer Options

A. XNAT

1. Select all of the Anonymized Scans in the lower Series Window
2. At the bottom of the console screen along the lower bar, scroll and select "XNAT"
3. The status window will update saying data has successfully began transferring to XNAT

B. 2TB SSD or Thumbdrive (*backup method 1*)

1. Connect the 2TB SSD to the USB-C port of the control room computer
2. In protocol manager dropdown menu, select "Open Command Window" and type "nautilus" (this will open a file explorer window on the MRI console)
3. Find device named "VISLAB", Right Click the drive, and select "Mount"
4. Close out of nautilus window and close out of command window
5. Open a new command window and type [".." + Enter] until reaching the root directory (i.e. you have reached the base directory)
6. Enter "cd /run/media/sdc/VISLAB"
7. Enter "dumpDB SERIES #####" (name must match scanner session ID)
    a. If data transferring terminates prematurely or drive is full, stop transfer, and remove all data from the drive safely. Then, on a windows computer, and once data is successfully transferred off, right click the drive → Erase & Reformat → Unit Size = 4096 kB

C. NordicNeuroLabs Behavior Data

1. Locate the path: "/desktop/psychopy_projects/4_30version/randomize_image/data"
2. Copy all of the participants csv, psydat, and log files on to the lab SSD or to Cheaha. Naming convention: "ADC###_RUN###_METAFUN_SAT_InScanner_YYYYMMDD_HHMMSS"

D. Video Capture Transfer

1. Log into UAB Box → Open Eye Recordings folder (https://uab.box.com/s/zdkckv1bm2t59icba0g841gxcwm07vcp)
2. Create a folder with the participant's ADC###
3. In File Explorer, Open the "Videos" folder → Copy the participant's .mp4 video (In the format YYYY-MM-DD HH-mm-ss) to the participant folder in Box.