How much does unmeasured TEC behavior above 300 K affect the detector?

Published source curve unchanged to 300 K; only the tangent continuation beyond 300 K varies.

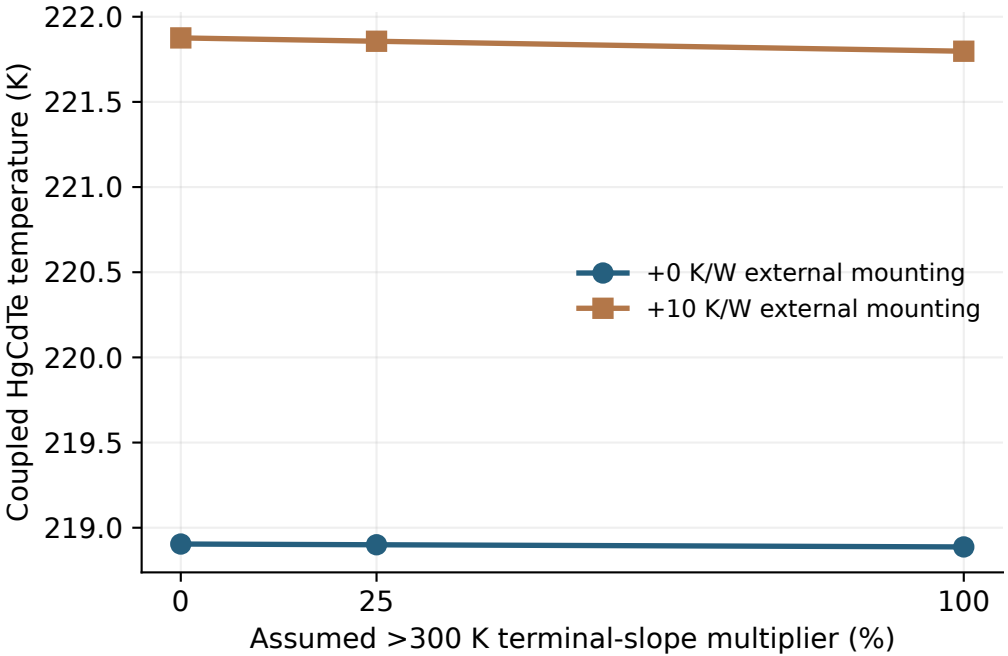

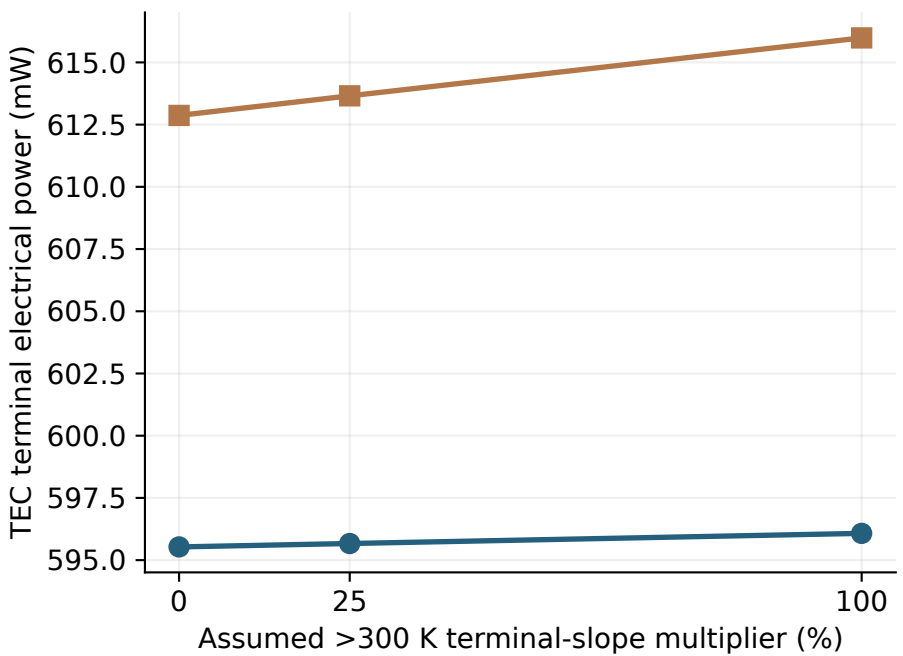

0.400 A TEC, 300 K reservoir, 0.866 V HgCdTe bias, 0.5 mW absorbed heat and 100 Pa krypton

Hypothesis sensitivity only; not an extrapolation confidence interval, measured grade or calibrated device prediction.