TEC operating envelope: cooling versus electrical input

300 K sink | 2.00 mW imposed detector heat | 100 Pa krypton | unchanged V3.5 physical laws

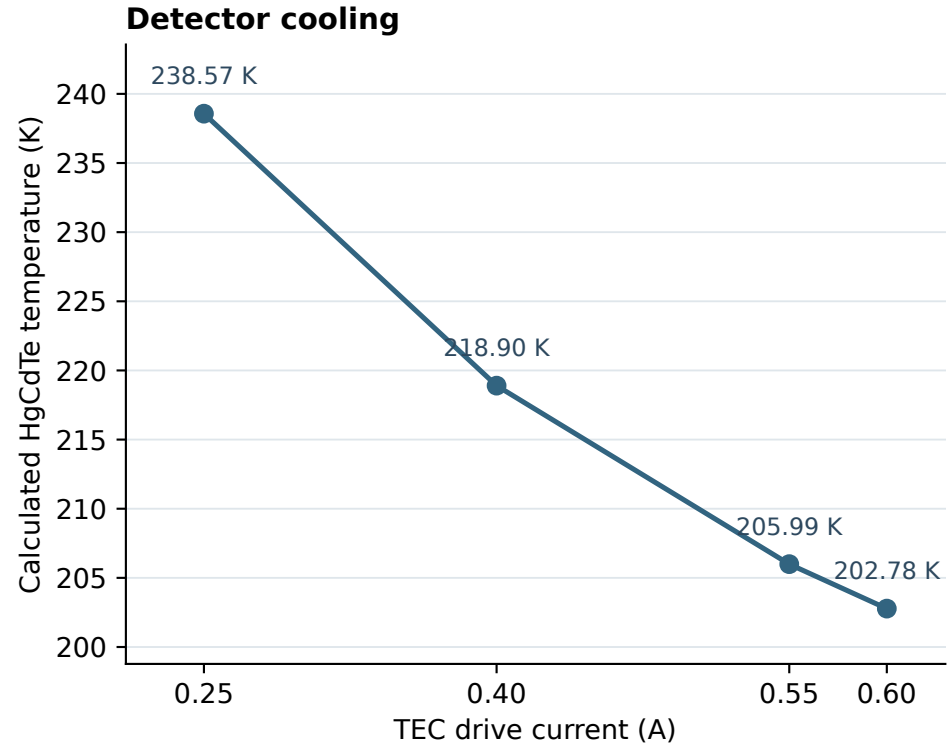

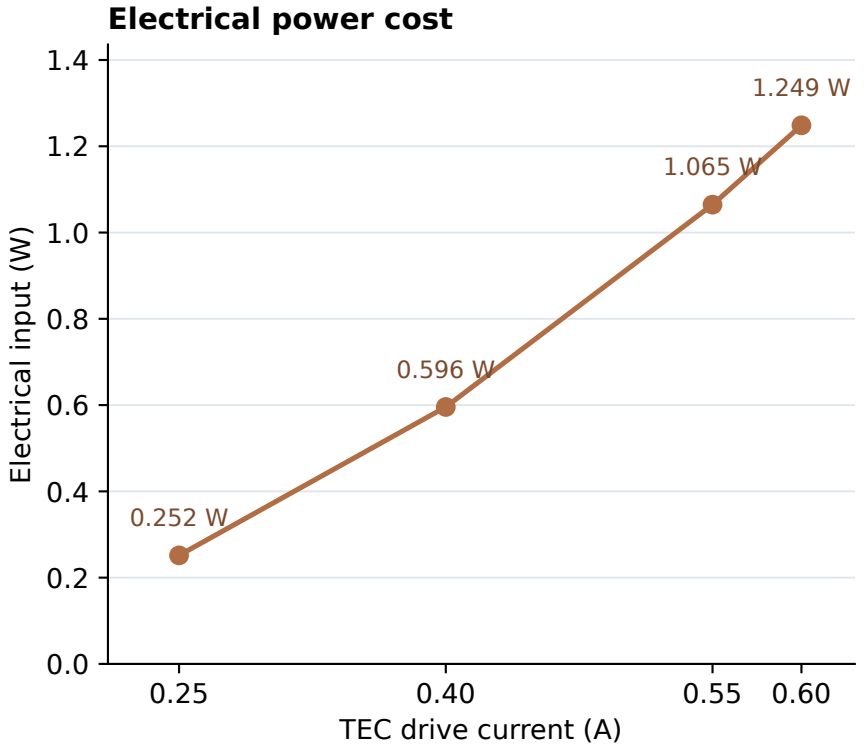

Four individually converged synthetic full-system cases; line segments guide the eye. Not a fitted optimum or measured response.