


Filename: 2024-10-11 - 16.07.29.HSD1000

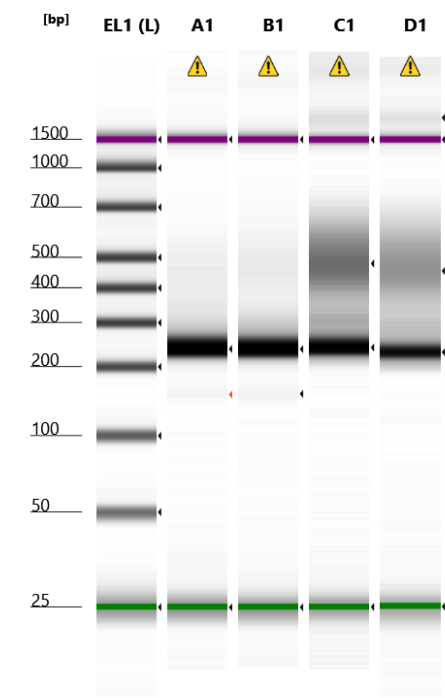


Default image (Contrast 100%)

Sample Info

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	2350	Electronic Ladder		Ladder
A1	1540	1A - PCR2		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range
B1	1530	1B - PCR2		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range
C1	2240	6A - PCR2		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range
D1	1480	6B - PCR2		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range; Peak out of Sizing Range

EL1: Electronic Ladder

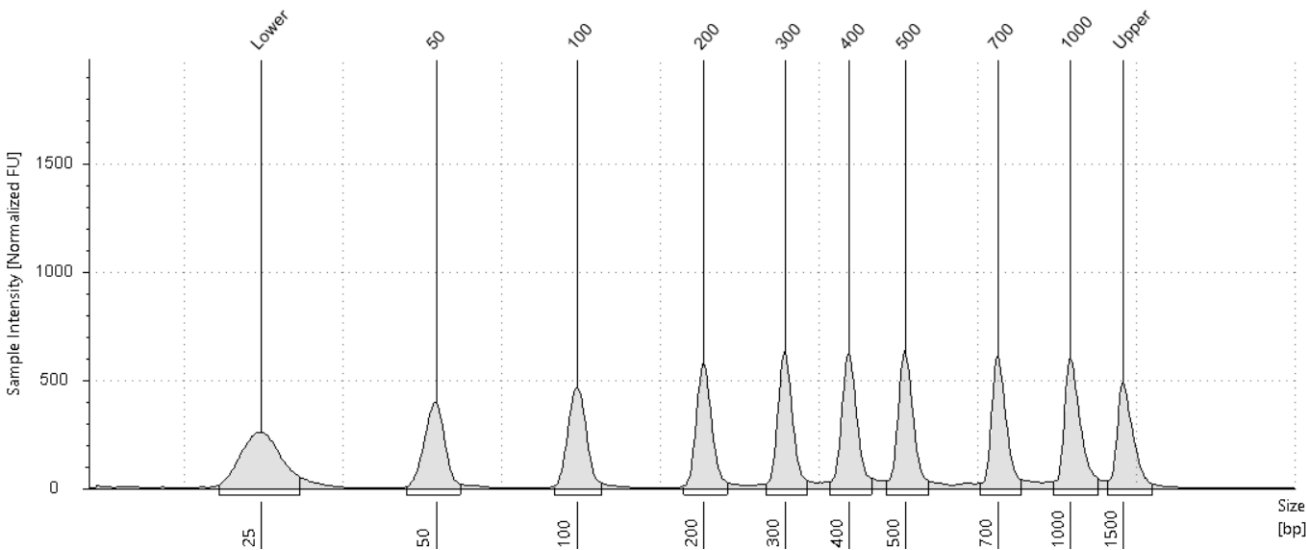


Sample Table

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	2350	Electronic Ladder		Ladder

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	340	-	20900	-		Lower Marker
50	265	-	8160	11.28		
100	278	-	4270	11.82		
200	290	-	2230	12.32		
300	304	-	1560	12.95		
400	306	-	1180	13.00		
500	312	-	961	13.29		
700	286	-	629	12.19		
1000	309	-	476	13.15		
1500	250	250	256	-		Upper Marker

A1: 1A - PCR2

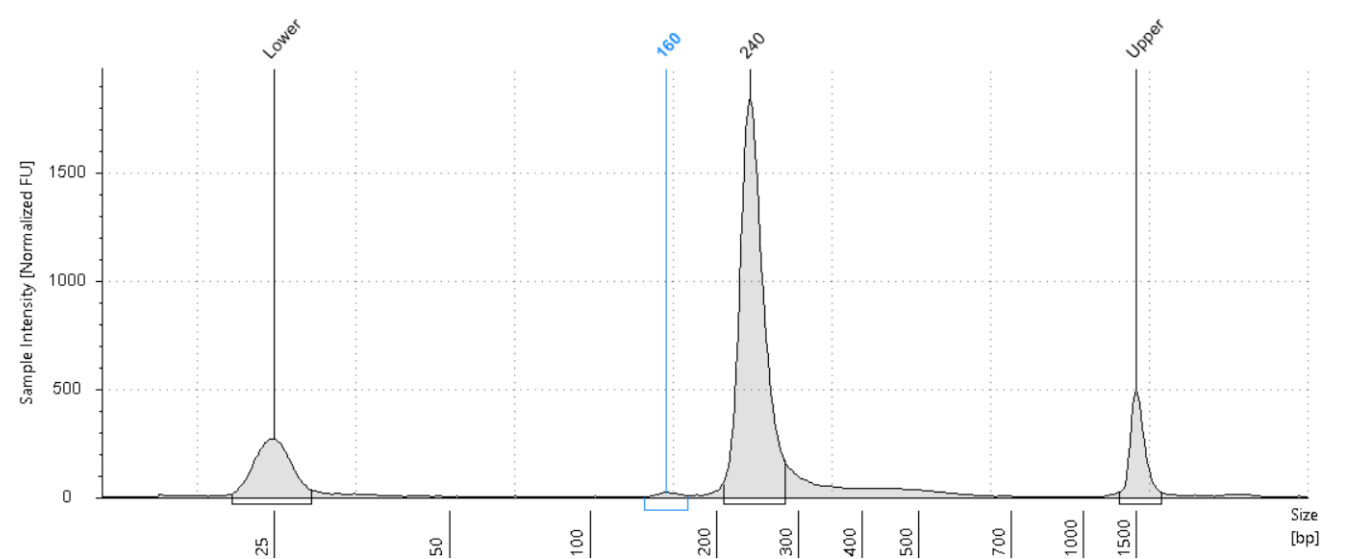


Sample Table

Well	Conc. [pg/μl]	Sample Description	Alert	Observations
A1	1540	1A - PCR2		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [pg/μl]	Assigned Conc. [pg/μl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	358	-	22000	-		Lower Marker
160	17.7	-	170	1.15		
240	1520	-	9730	98.85		
1500	250	250	256	-		Upper Marker

B1: 1B - PCR2

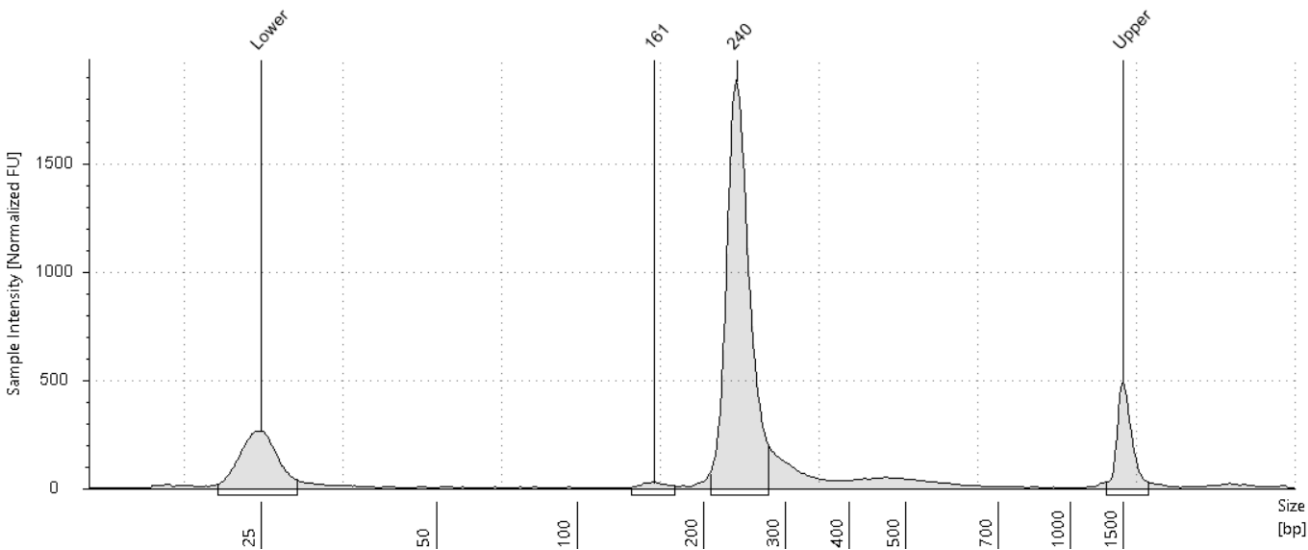


Sample Table

Well	Conc. [pg/μl]	Sample Description	Alert	Observations
B1	1530	1B - PCR2		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [pg/μl]	Assigned Conc. [pg/μl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	352	-	21600	-		Lower Marker
161	23.5	-	225	1.53		
240	1510	-	9660	98.47		
1500	250	250	256	-		Upper Marker

C1: 6A - PCR2

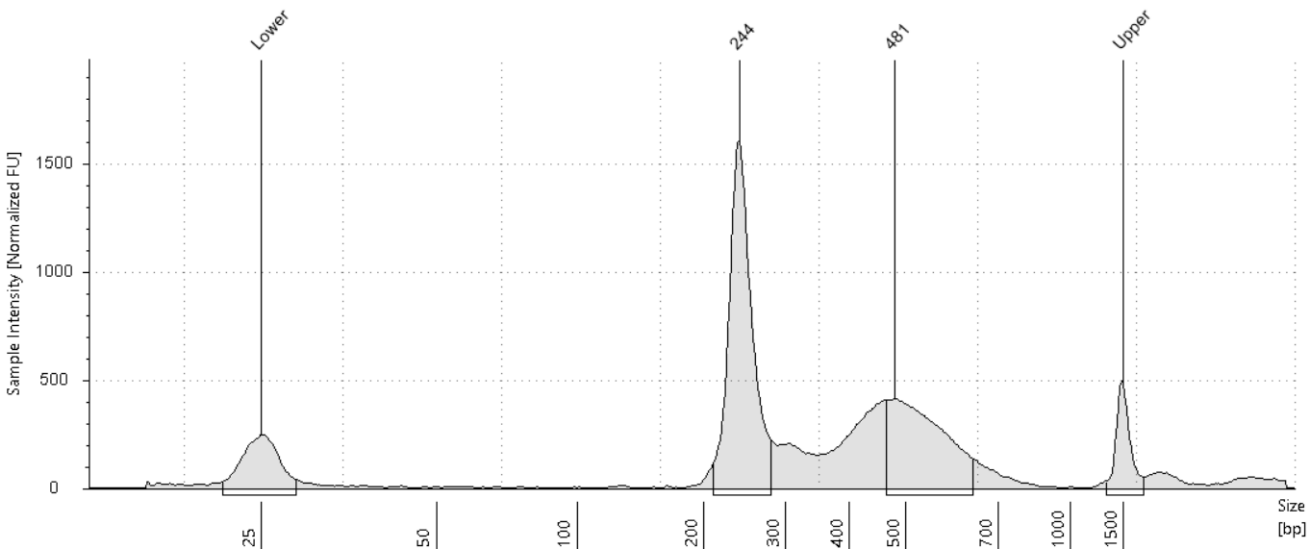


Sample Table

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
C1	2240	6A - PCR2		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	342	-	21100	-		Lower Marker
244	1380	-	8700	61.52		
481	862	-	2760	38.48		
1500	250	250	256	-		Upper Marker

D1: 6B - PCR2

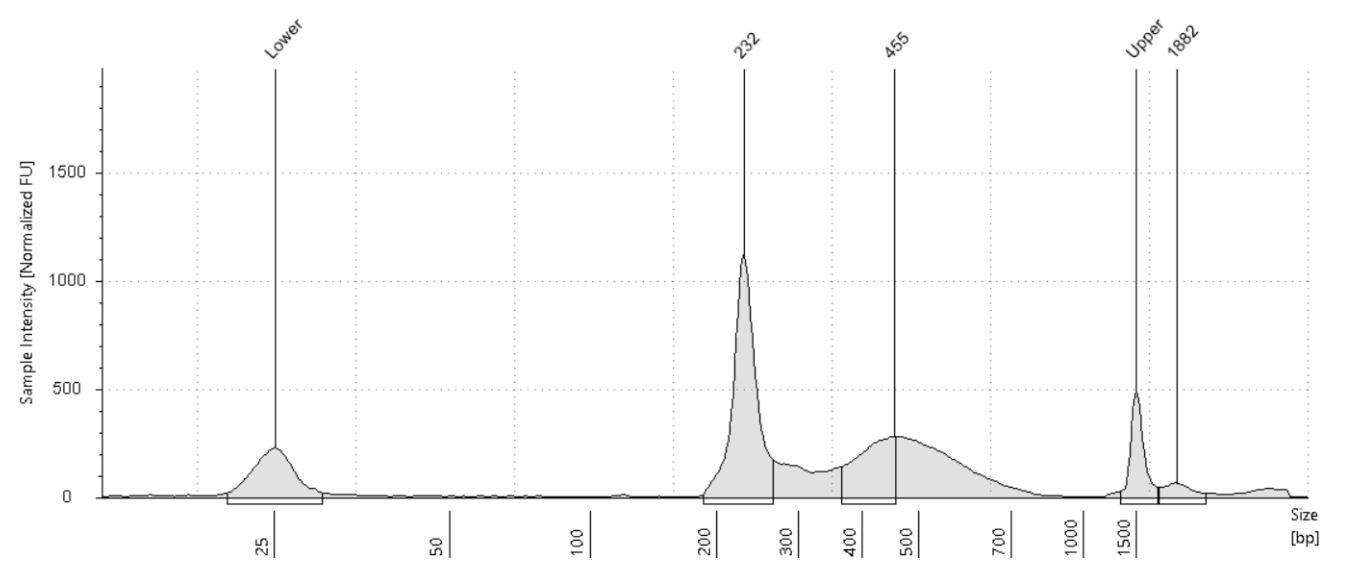

Sample Table

Well	Conc. [pg/μl]	Sample Description	Alert	Observations
D1	1480	6B - PCR2		Caution! Expired ScreenTape device (used after two weeks of first use); Sample concentration outside recommended range; Peak out of Sizing Range

Peak Table

Size [bp]	Calibrated Conc. [pg/μl]	Assigned Conc. [pg/μl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	375	-	23100	-		Lower Marker
232	997	-	6600	67.43		
455	410	-	1390	27.74		
1500	250	250	256	-		Upper Marker
1882	71.4	-	58.4	4.83		Peak outside of Sizing Range