

CARDIAC PRE-STROKE

AI-ASSISTED ECG ANALYSIS


Generated: 2026-08-08 20:55:55 | Layout: Approved

Patient ID	-	Recording ID	000	Metric	Value	
Age	-	Sex	-	Classification	Elevated pre-stroke ECG risk pattern	
Date	-	Duration	00:10	Model Score	99.98%	
Sampling Rate	100 Hz	Number of Leads	12	Threshold	0.520	
Signal Quality	POOR			Screening Status	ELEVATED	

CLINICAL SUMMARY

Overall result: Elevated pre-stroke ECG risk pattern (99.98%).
Signal reliability: POOR (51.92).
Main findings: HR 179.94 BPM, rhythm Tachycardic rhythm, QRS 42.68 ms.
Next action: Immediate clinical evaluation recommended..

MAIN ECG VISUALIZATION

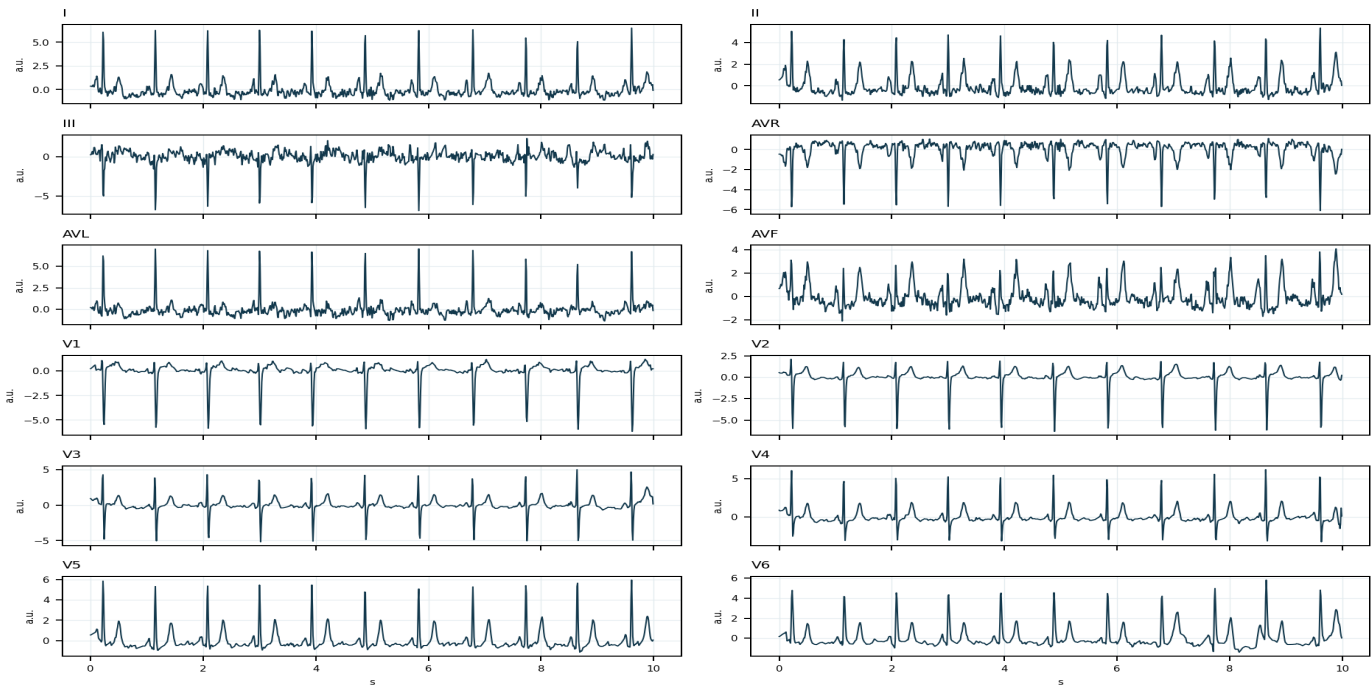


Parameter	Result	Status	Finding	Evidence	Importance
Heart Rate	179.94 BPM	Automated	Heart rate mean	179.94 BPM	Moderate
PR	200.00 ms	Automated / Verify	Heart rate range	86.96 BPM to 240.00 BPM	Moderate
QRS	42.68 ms	Automated	RR variability	SD 103.07 ms	Moderate
QT	390.00 ms	Automated / Verify	Signal quality	51.92	High
QTc	718.13 ms	Automated / Verify			
ST	-0.0691	Automated / Verify			

RECOMMENDED NEXT STEPS

Finding	Action
Poor Signal Quality	Repeat the recording with improved electrode contact and reduced movement.
Elevated AI screening result	Immediate clinical evaluation recommended.

DETAILED ECG ANALYSIS


SUPPORTING ECG GRAPHS

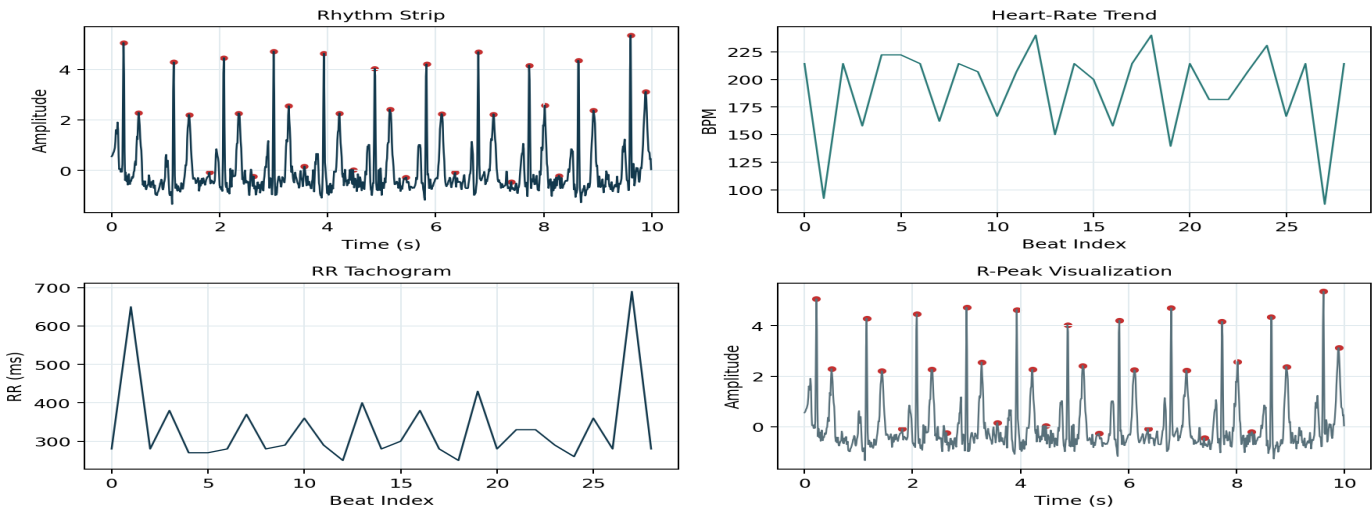

Parameter	Result	Unit
Heart Rate	179.94	BPM
HR Range	86.96 - 240.00	BPM
Mean RR	333.45	ms
RR SD	103.07	ms
SDNN	103.07	ms
RMSSD	168.06	ms
pNN50	64.29	%

Parameter	Value	Source	Reliability
PR	200.00 ms	Existing pipeline	Heuristic / Expert
QRS	42.68 ms	Existing pipeline	Automated
QT	390.00 ms	Existing pipeline	Heuristic / Expert
QTc	718.13 ms	Existing pipeline	Heuristic / Expert
ST	-0.0691	Existing pipeline	Heuristic / Expert


HEART RATE / HRV ANALYSIS

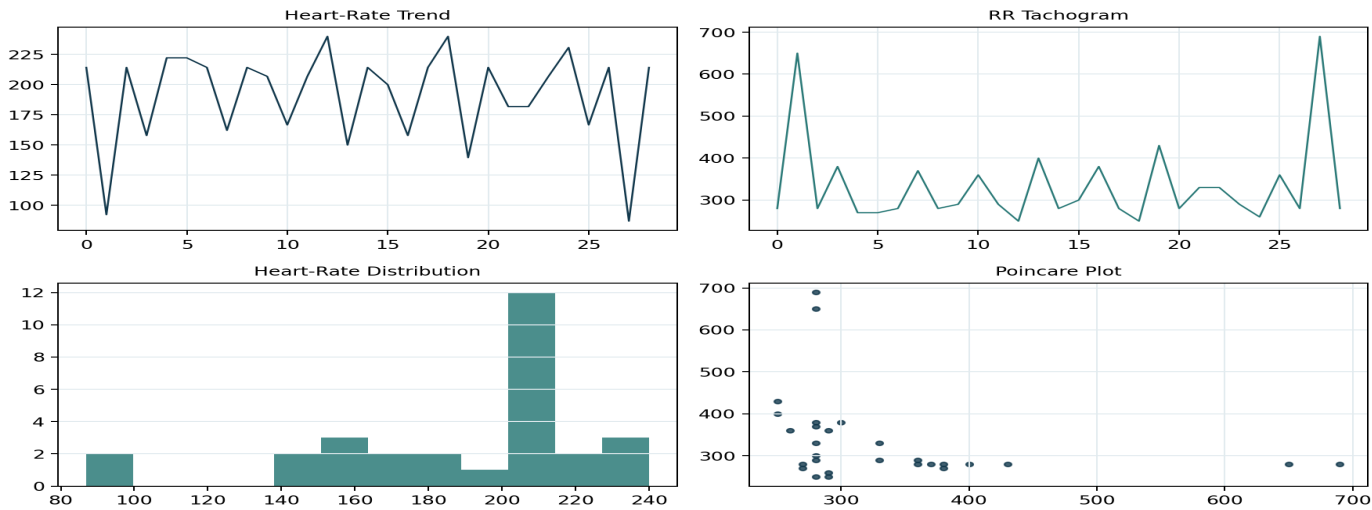

SIGNAL QUALITY

Metric	Value
Signal Quality	51.92
Noise Level	High
Baseline Wander	0.37
Noise Ratio	11.11
Clipping Ratio	0.00


FREQUENCY ANALYSIS

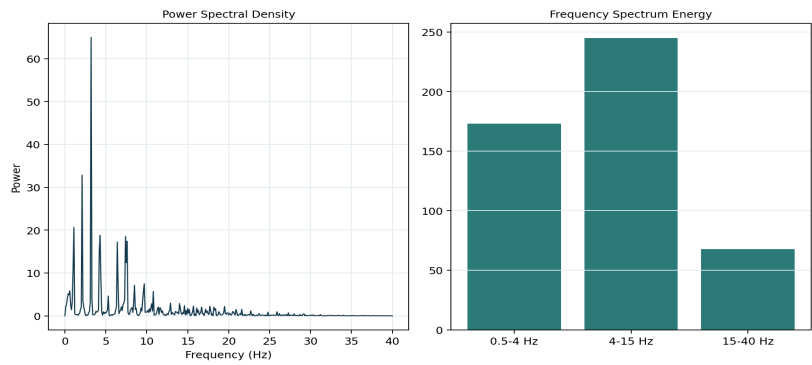


Metric	Value
Spectral Entropy	4.40
Dominant Frequency	3.20 Hz
0.5-4 Hz Energy	173.01
4-15 Hz Energy	244.99
15-40 Hz Energy	67.81

AI & EVIDENCE ANALYSIS

Metric	Value
Classification	Elevated pre-stroke ECG risk
Model Score	99.98%
Threshold	0.520
Screening Status	ELEVATED

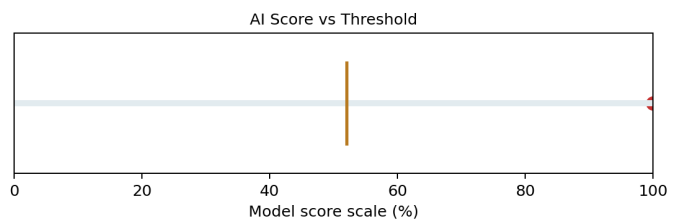

MODEL EXPLAINABILITY

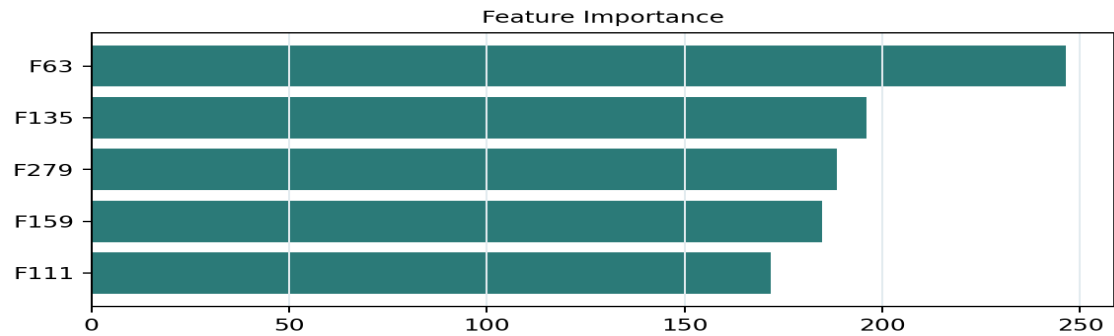

EVIDENCE SUMMARY

Finding	Observed Value	Evidence	Significance	Review
Heart rate mean	179.94 BPM	Detected RR intervals	Supports rhythm and rate review	Clinical review
Heart rate range	86.96 BPM to 240.00 BPM	Detected RR intervals	Shows short-record rate spread	Contextual review
RR variability	SD 103.07 ms	Detected RR intervals	Reflects beat-to-beat timing variability	HRV review
Signal quality	51.92	Signal-quality audit	Affects confidence in derived measurements	Repeat ECG if poor
AI elevated classification	99.98%	ML model	Model-derived screening result	Immediate clinical evaluation recommended.
PR Interval	200.00 ms	Waveform interval engine	Experimental waveform estimate	Manual ECG confirmation
QRS Duration	42.68 ms	Waveform interval engine	Representative-lead waveform estimate	Manual ECG confirmation

OVERALL ASSESSMENT

OVERALL RESULT Elevated pre-stroke ECG risk pattern 99.98% PRIORITY REVIEW	MAIN FACTORS
	Heart rate mean
	Heart rate range
	RR variability
	Signal quality
	AI elevated classification

LIMITATIONS


Limitation	Impact
Poor Signal Quality	Noise and baseline distortion may reduce confidence in interval and AI measurements.
Research prototype	Not a diagnostic medical device.

CLINICAL DISCLAIMER

Research-use AI-assisted ECG screening report. Automated measurements and model-derived scores require independent clinical review.

ADDITIONAL TECHNICAL VISUALIZATION

ECG MORPHOLOGY

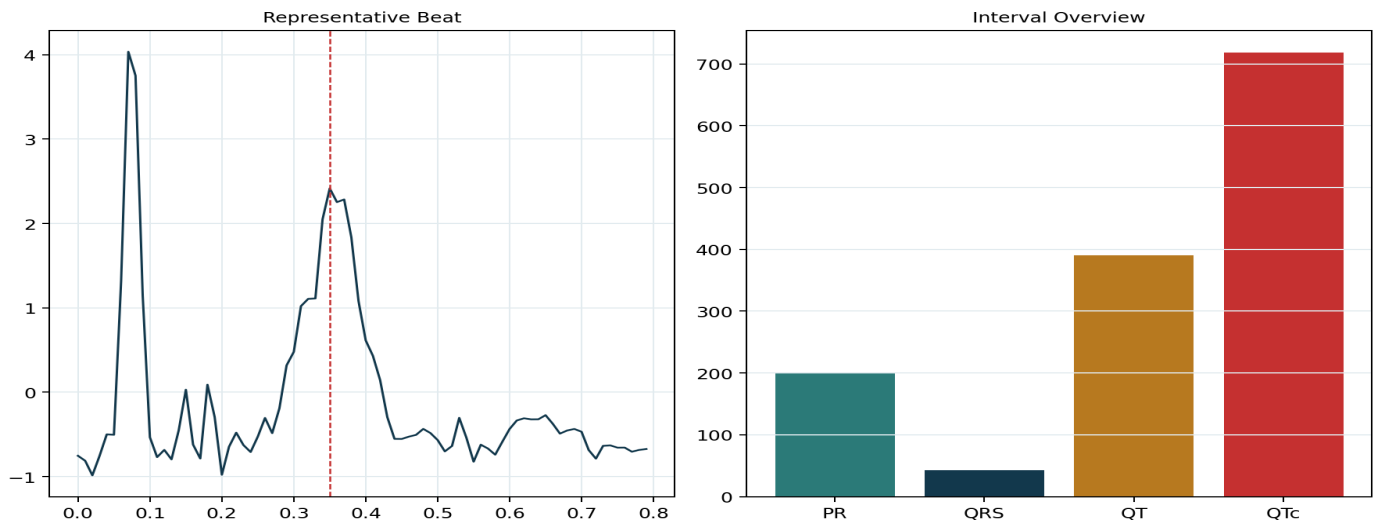

ADDITIONAL ECG / SPECTRAL REVIEW

