


Fertiscan (Computer Assisted Semen Analysis)

The system follows WHO 6 (2021) criteria for motility, count, and morphology for human semen

Age	30 years old
Lab ID	4243

Date	8 Aug 2024
Patient Name	Karim mohamed ahmed
Ref. By	Dr. Abeer elawdy

Physical Properties		
Abstinence	3	2 - 7 Days
Collection	Masturbation At Lab	
Volume	2 ml	1.5 - 6 ml
Color	Offwhite (Normal)	
Oder	Chlorine (Normal)	
PH	7.6	7.2 - 8
Viscosity	Normal	
Liquefaction Time	30 min	30 - 60 min
Liquefaction State	Completed	

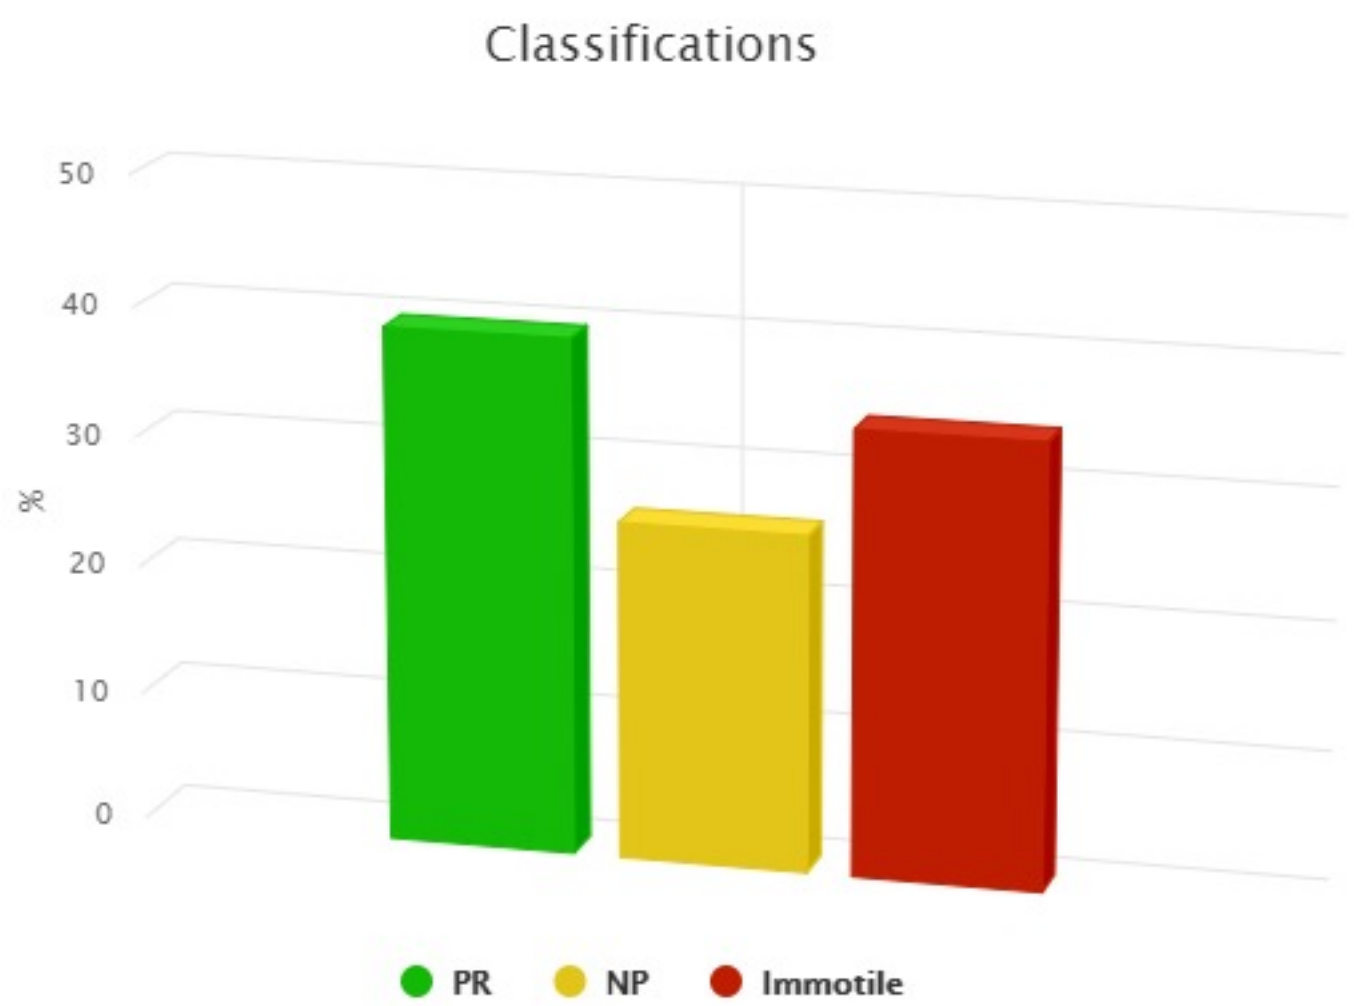

Result

Test	Result	Status	Reference Value
Concentration	47.00 Million	Passed	> 15 Million/ml
Total Sperm Count	94.00 Million	Passed	> 39 Million
Progressive Motility (PR) (A + B)	39.73 %	Passed	> 32 %
Total Motility (PR + NP) (A + B + C)	65.76 %	Passed	> 40 %
Morphology Normal	9.09 %	Passed	Passed if ≥ 4 %
Morphology Index	1.00		
Vitality	66.67 %	Passed	> 58 %

Aggregation & Agglutination

Aggregation	Nil
Agglutination	Nil
MAR Test	- ve

Other Cells

Test	Result	Reference Value
WBC	0.25 Million	< 1 (Million/ml)
Immature Cell	0.14 Million	< 1 (Million/ml)
Round Cell	0 Million	< 1 (Million/ml)

Conclusion


Normozoospermia - Total number of spermatozoa, and percentages of progressively motile (A+B) and morphologically normal spermatozoa, equal to or above the lower reference

Fertiscan (Computer Assisted Semen Analysis)

Motility Report

Patient Name	Karim mohamed ahmed	Lab ID	4243
--------------	---------------------	--------	------

Dynamic Parameters (I)			
Class	Percentage (%)	Conc. (Million/ml)	Total Number/Million
Class A (fast & prog)	31.51	14.81	47.79
Class B (slow & prog)	8.22	3.86	12.47
Class C (non progressive)	26.03	12.23	39.48
Class D (immotile)	34.24	16.09	51.93

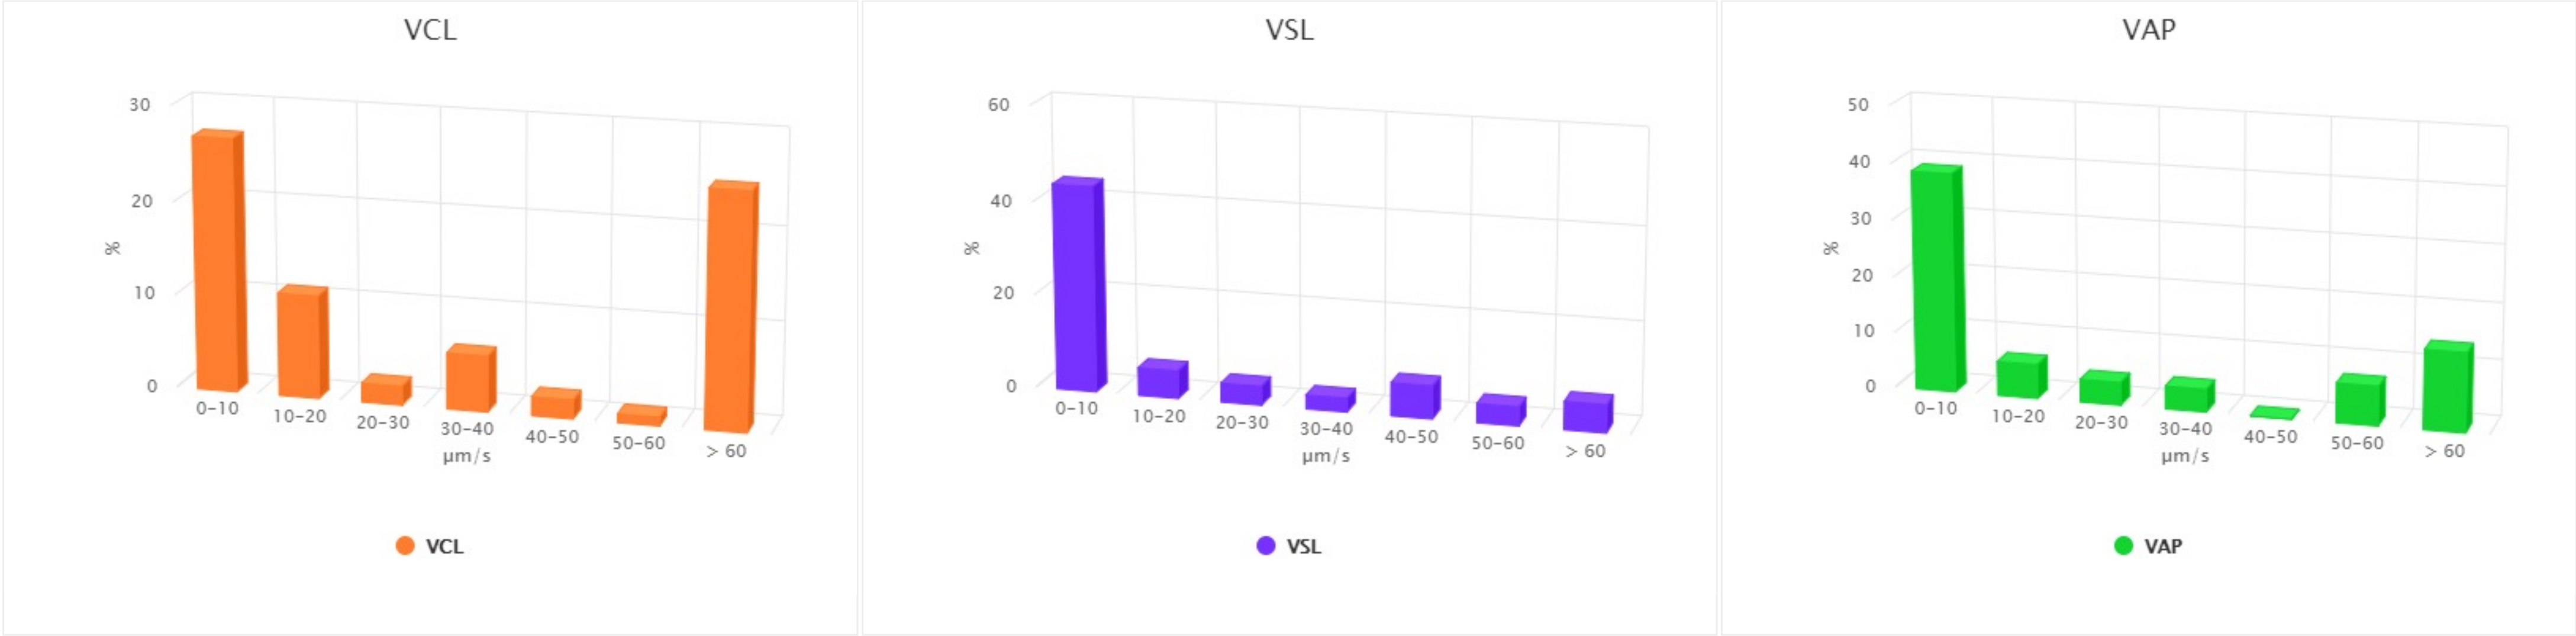

Dynamic Parameters (II)									
	VCL	VSL	VAP	ALH	BCF	LIN	STR	WOB	MAD
Class A	99.07	52.58	61.83	3.29	5.14	54.39	84.16	63.69	50.43
Class B	33.87	12.48	18.80	1.96	3.62	36.45	67.38	54.65	67.04
Class C	41.19	3.73	14.11	1.59	3.30	12.30	25.13	33.47	60.36
Class D	4.23	0.23	1.85	0.29	0.80	2.89	7.33	18.79	39.91
Total	178.35	69.01	96.59	7.13	12.86	106.04	184.00	170.61	217.75

VCL: Curvilinear Velocity

ALH:Amplitude of Lot Head disp

LIN: Linearity (VSL/VCL)

VSL: Straight Line Velocity



BCF: Beat Across Freq.

WOB: Wobble (VAP/VCL)

VAP: Average Path Velocity

STR: Straightness (VSL/VAP)

MAD: Mean Angle Degree

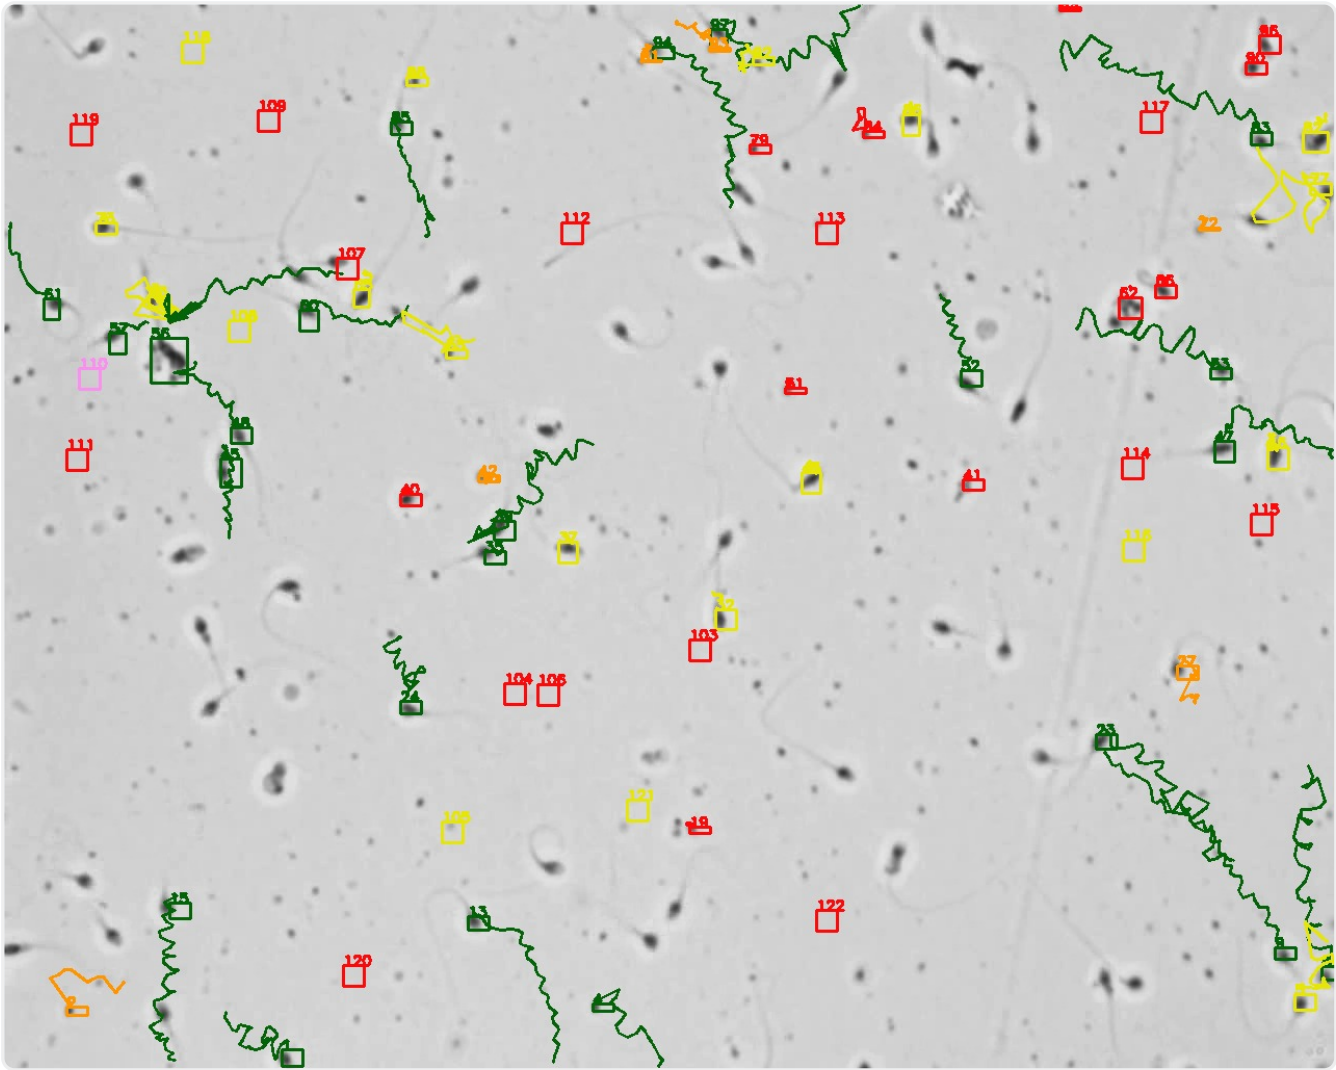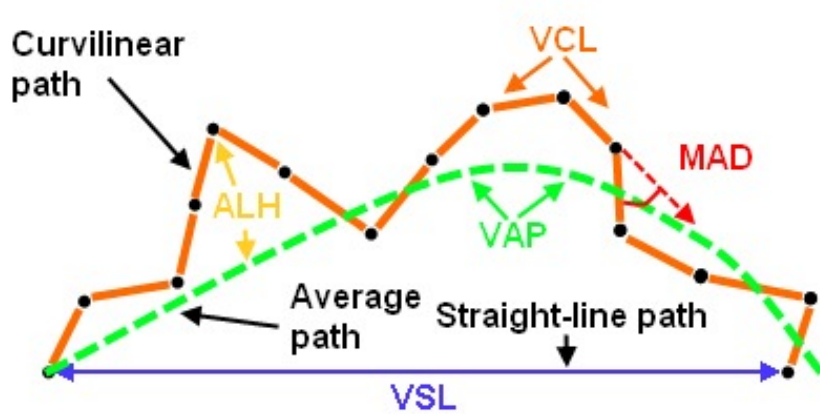





Fertiscan (Computer Assisted Semen Analysis)

Vitality Report


Patient Name Karim mohamed ahmed

Lab ID 4243

Detailed Vitality Study		
Status	Passed	> 58 %
Vitality	66.67 %	
Dead	33.33 %	

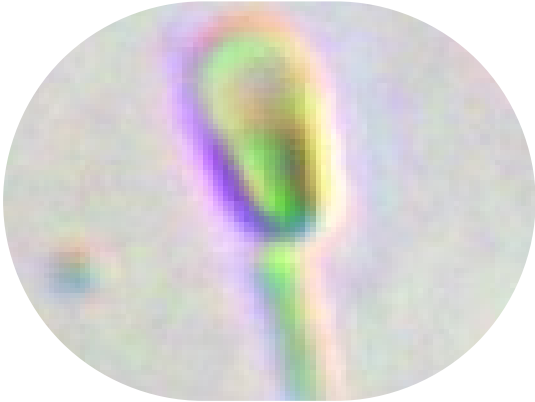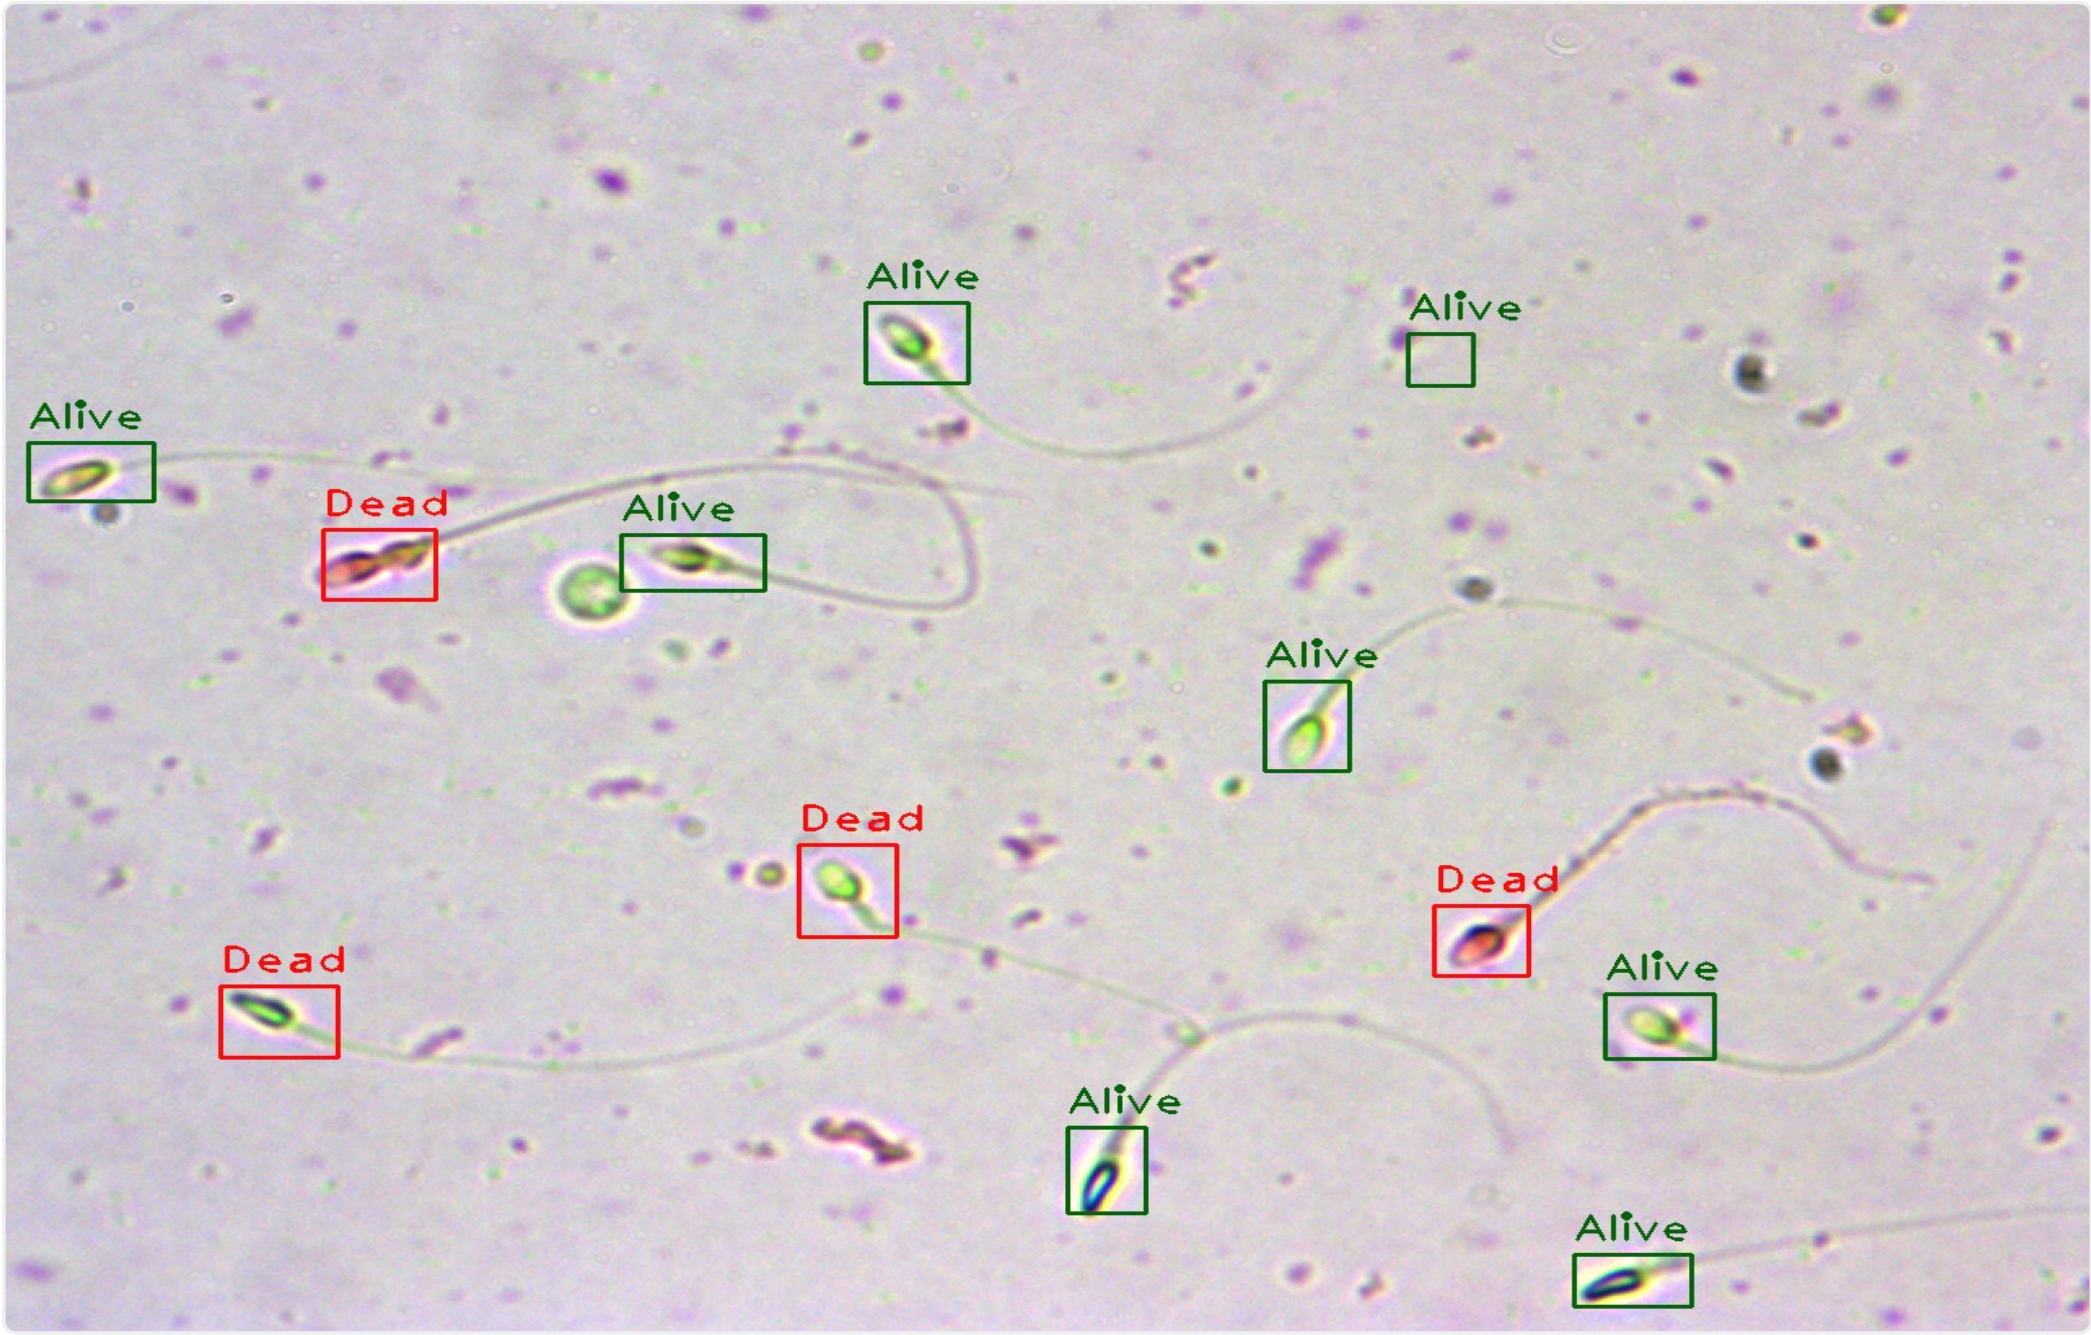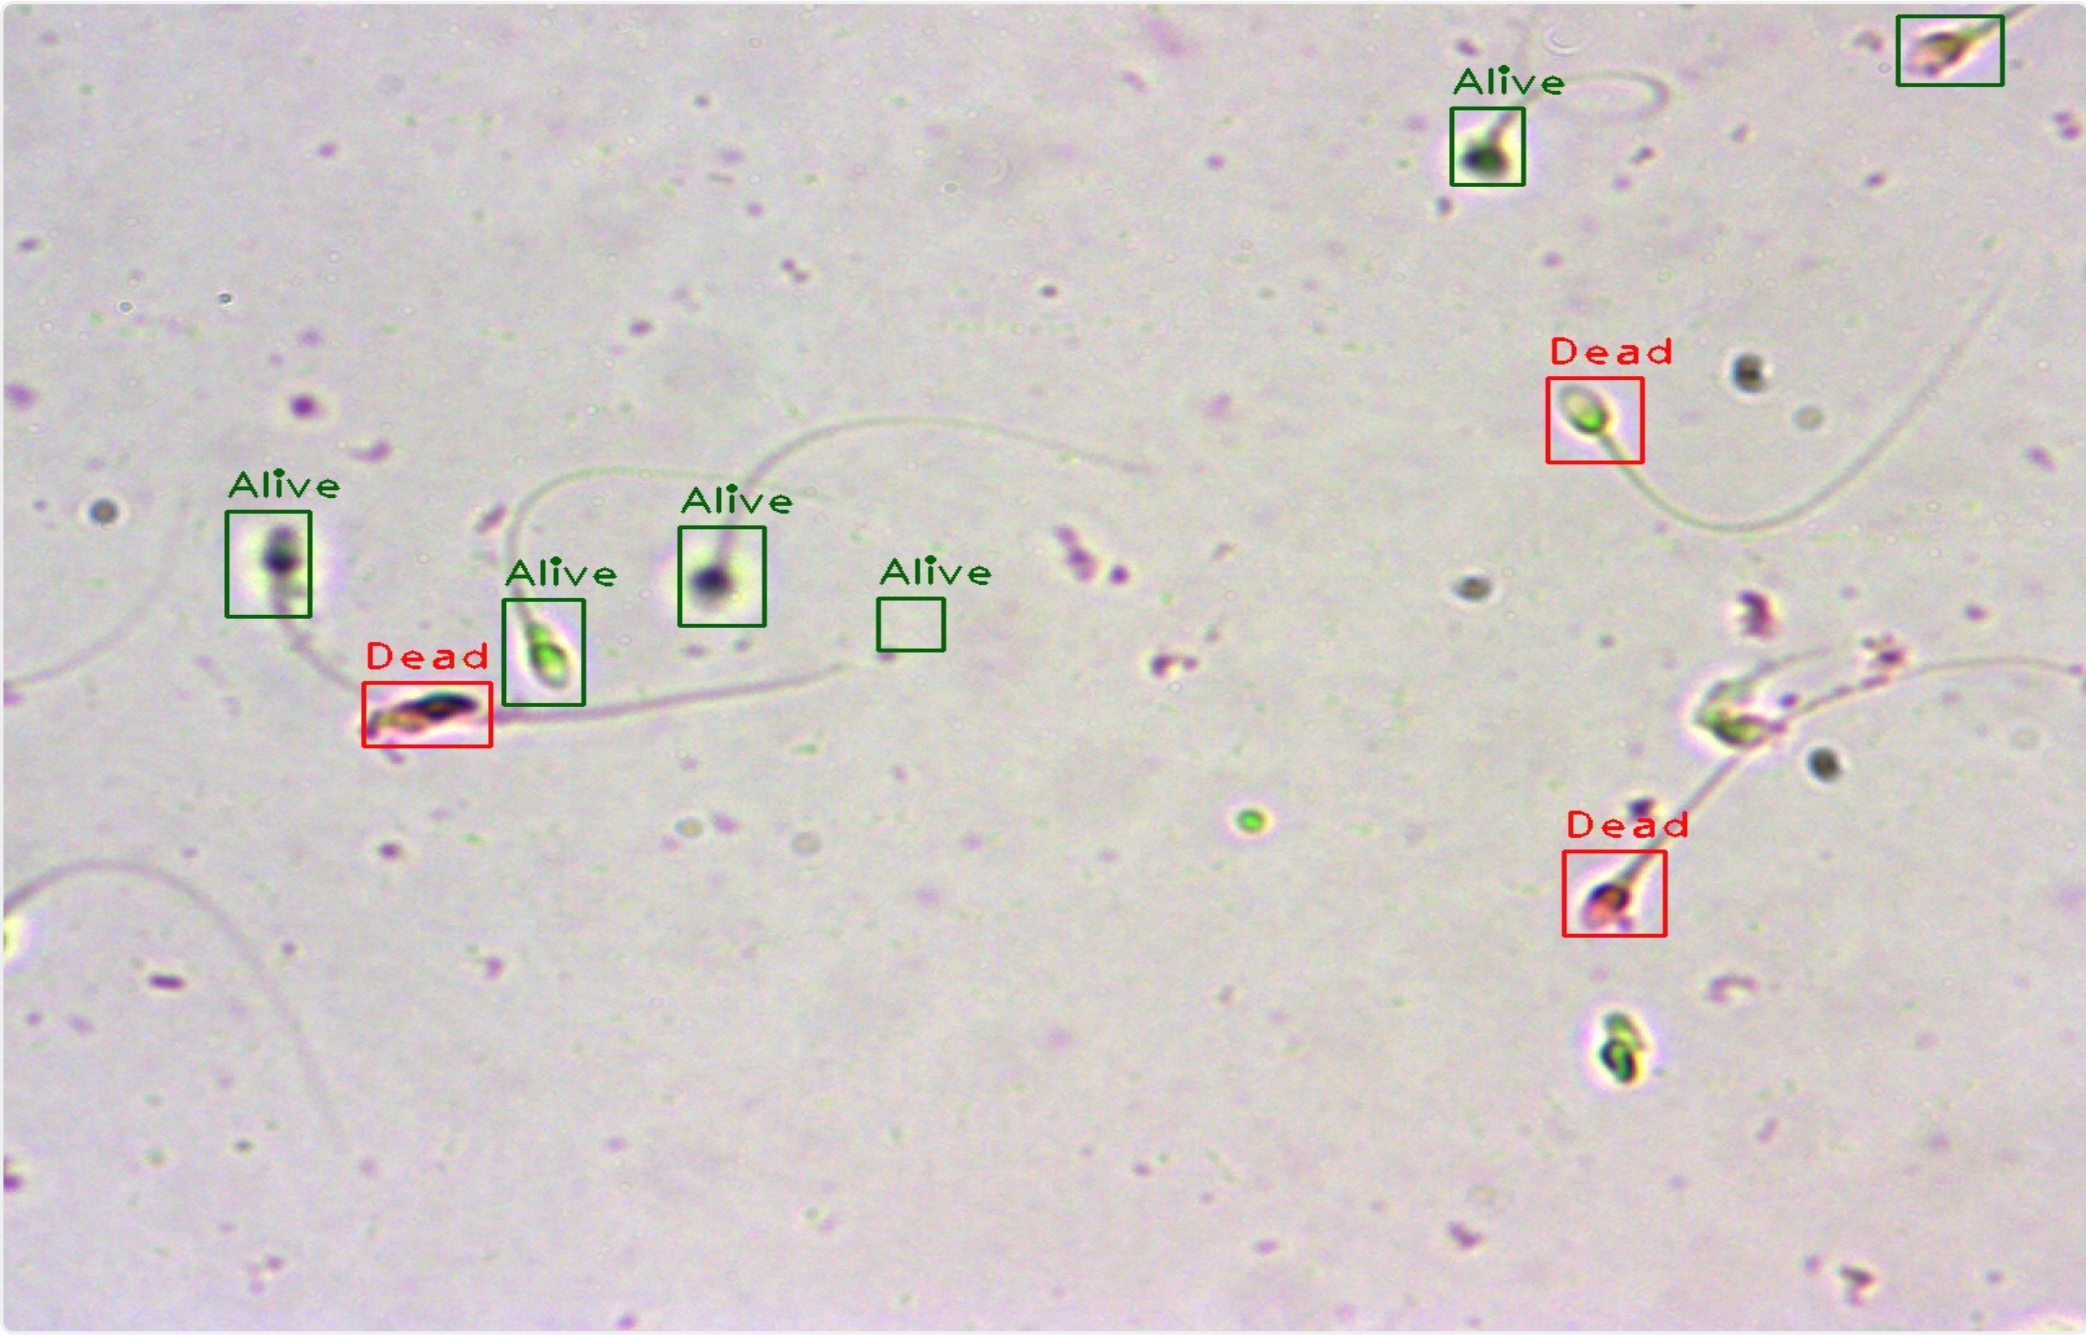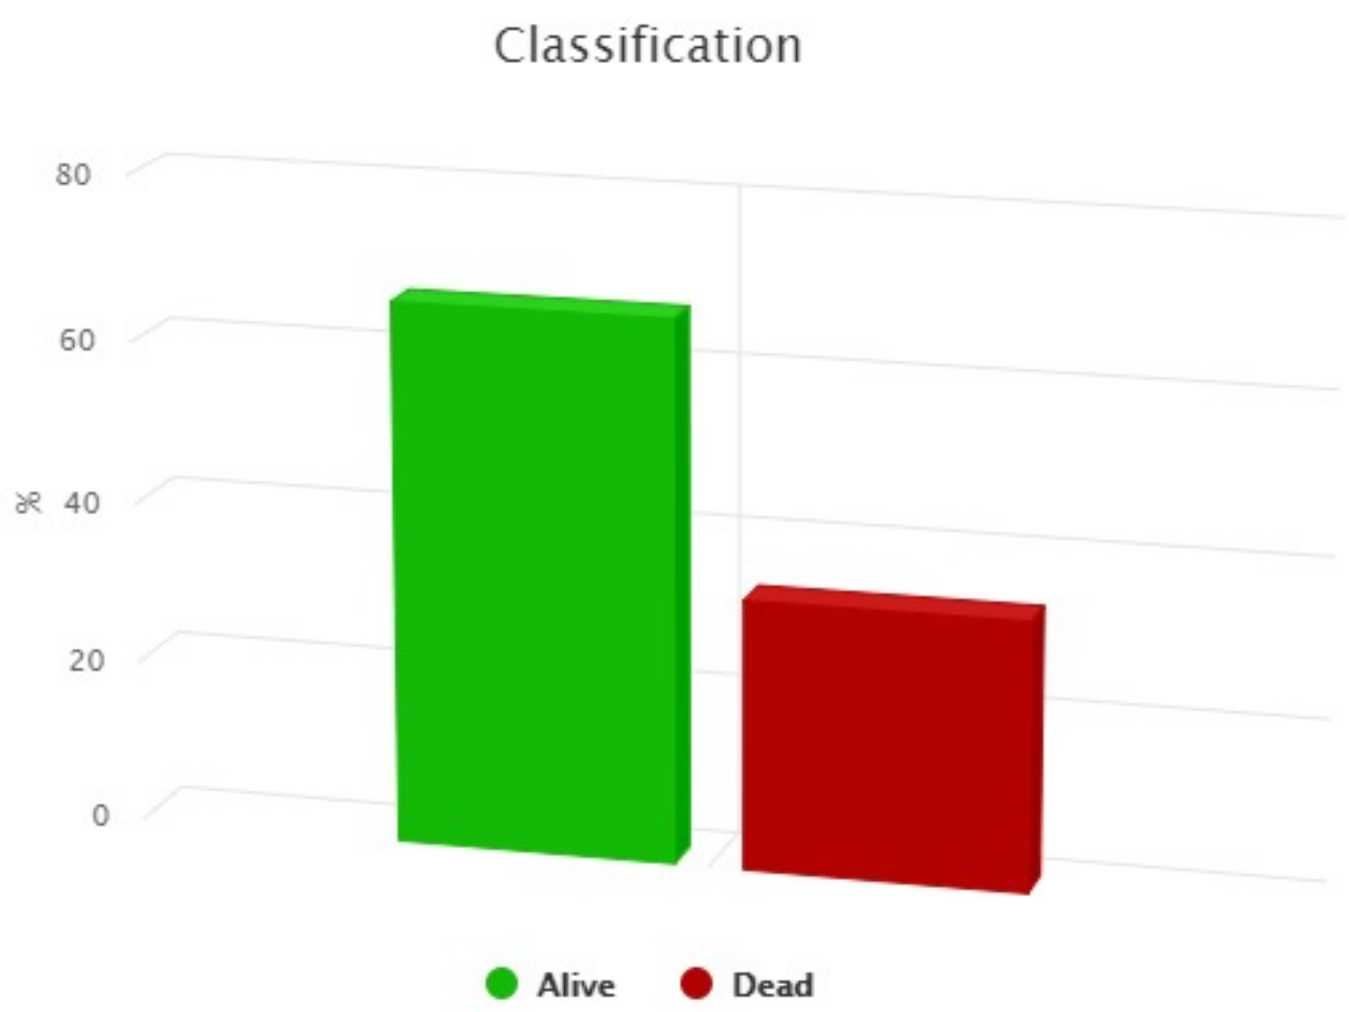

Alive

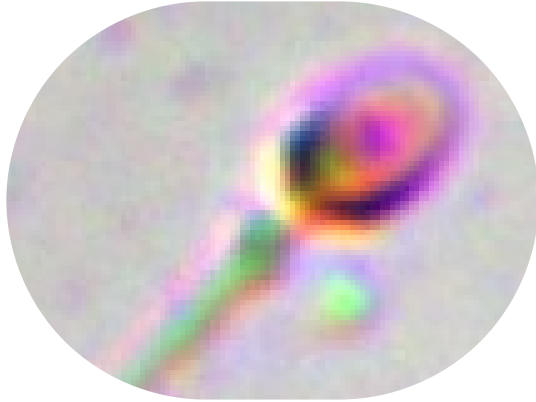

Dead

Fertiscan (Computer Assisted Semen Analysis)

Morphology Report


Patient Name	Karim mohamed ahmed	Lab ID	4243
--------------	---------------------	--------	------

	Result	Status	N.Value
Normal sperm (Morphology index)	9.09	Passed	Passed if ≥ 4 %

A. Head Pathology	
Class I	Totals
Big Head	9.09
Tapered Head	9.09
Pyriform Head	9.09
Amorphous	9.09
Vacuolated	9.09
Round & No acrosome	9.09
Round & Small	0
Small acrosome	9.09
Double Head	0
Pinhead	0
B. Neck Pathology	
Class II	Totals
Bent Neck	0
Asymmetrical	0
Thick	9.09
Thin	9.09

C. Tail Pathology	
Class III	Totals
Short Tail	9.09
Bent Tail	0
Coiled Tail	0
Double Tail	0
D. Other	
Class IV	Totals
ERC	0

TZI (Teratozoospermic Index)	1.00
Total number of defects divided by the number of abnormal sperms	

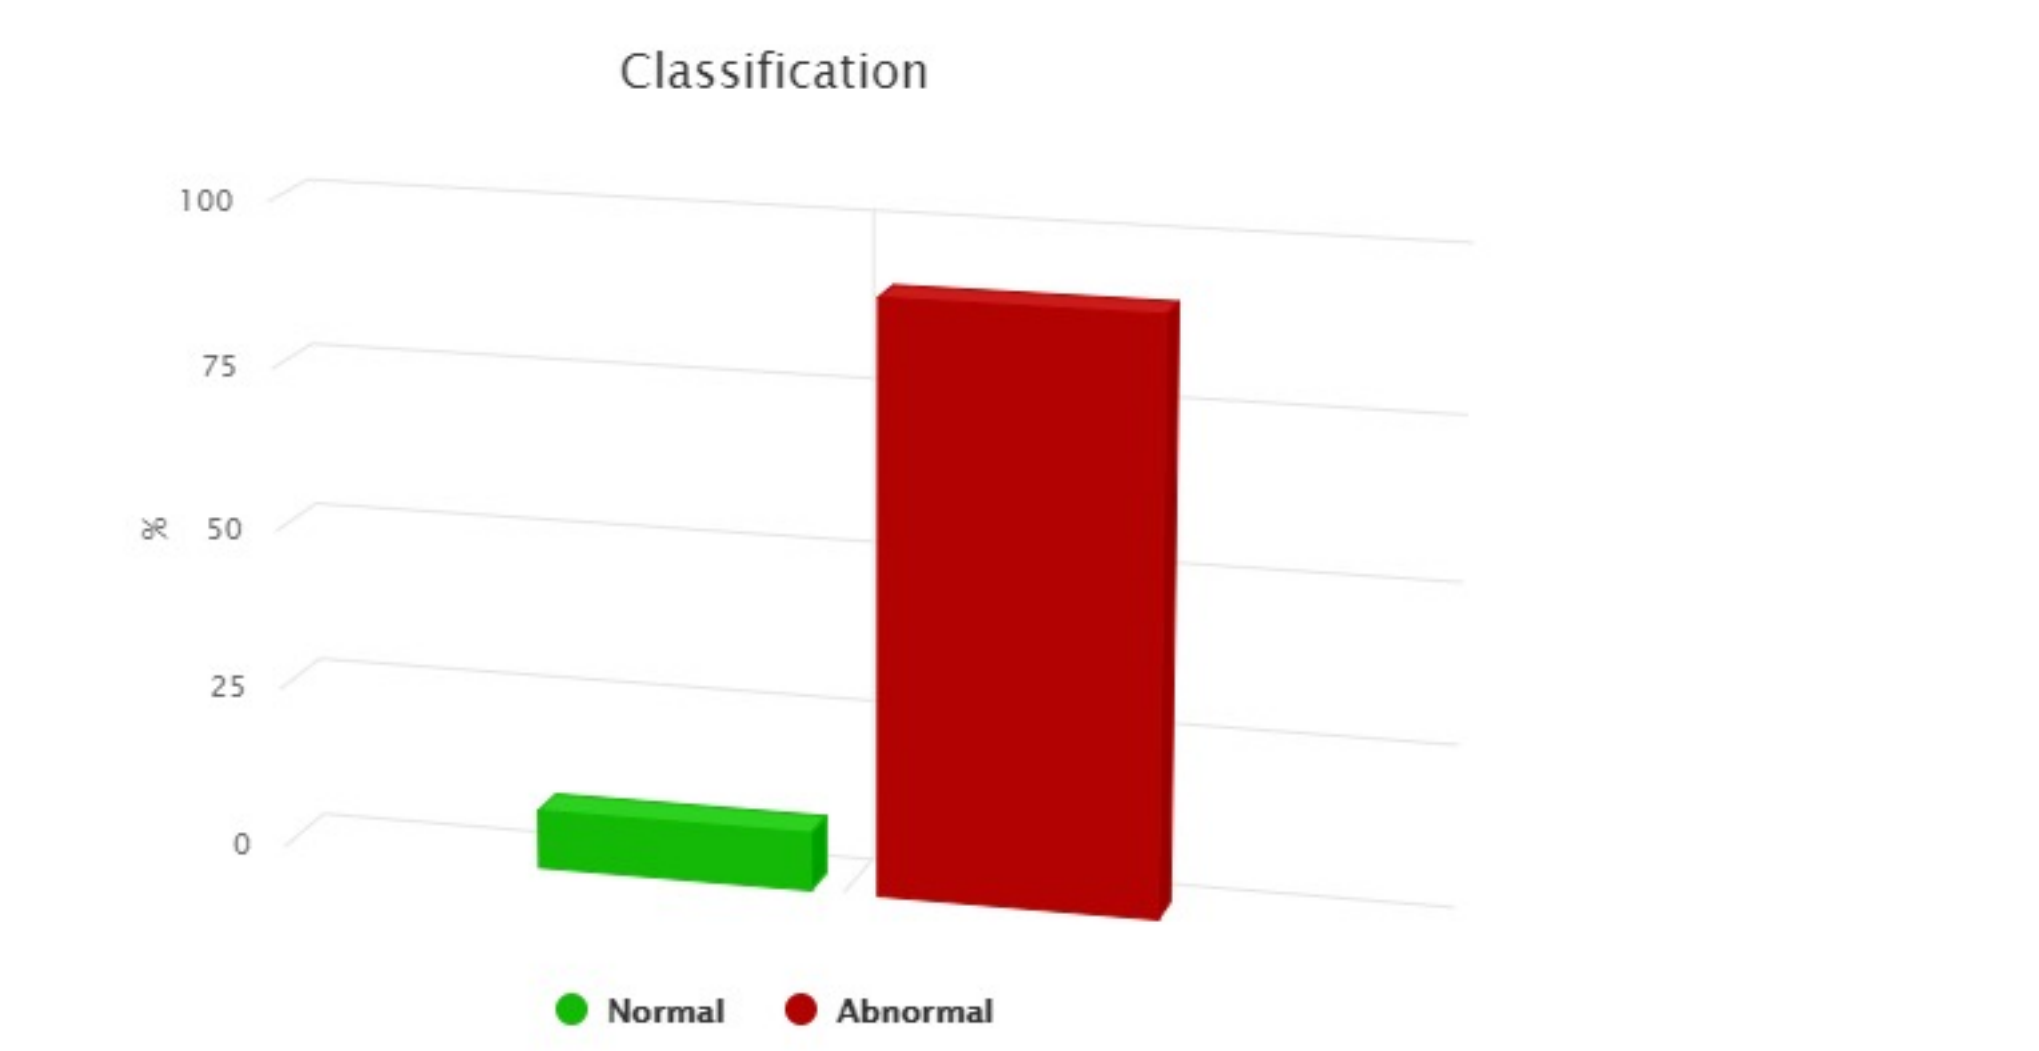




Morphology Statistics						
Class	Head Length	Head Width	Elongation	Head Area	FFE	Acrosome (%)
Mean of normal sperms	1.27	0.88	0.36	3.53	0.25	0.09
Mean of pathologic sperms	1.38	1.01	0.34	4.34	0.25	0.11

Fertiscan (Computer Assisted Semen Analysis)


Morphology Report

Patient Name Karim mohamed ahmed

Lab ID 4243

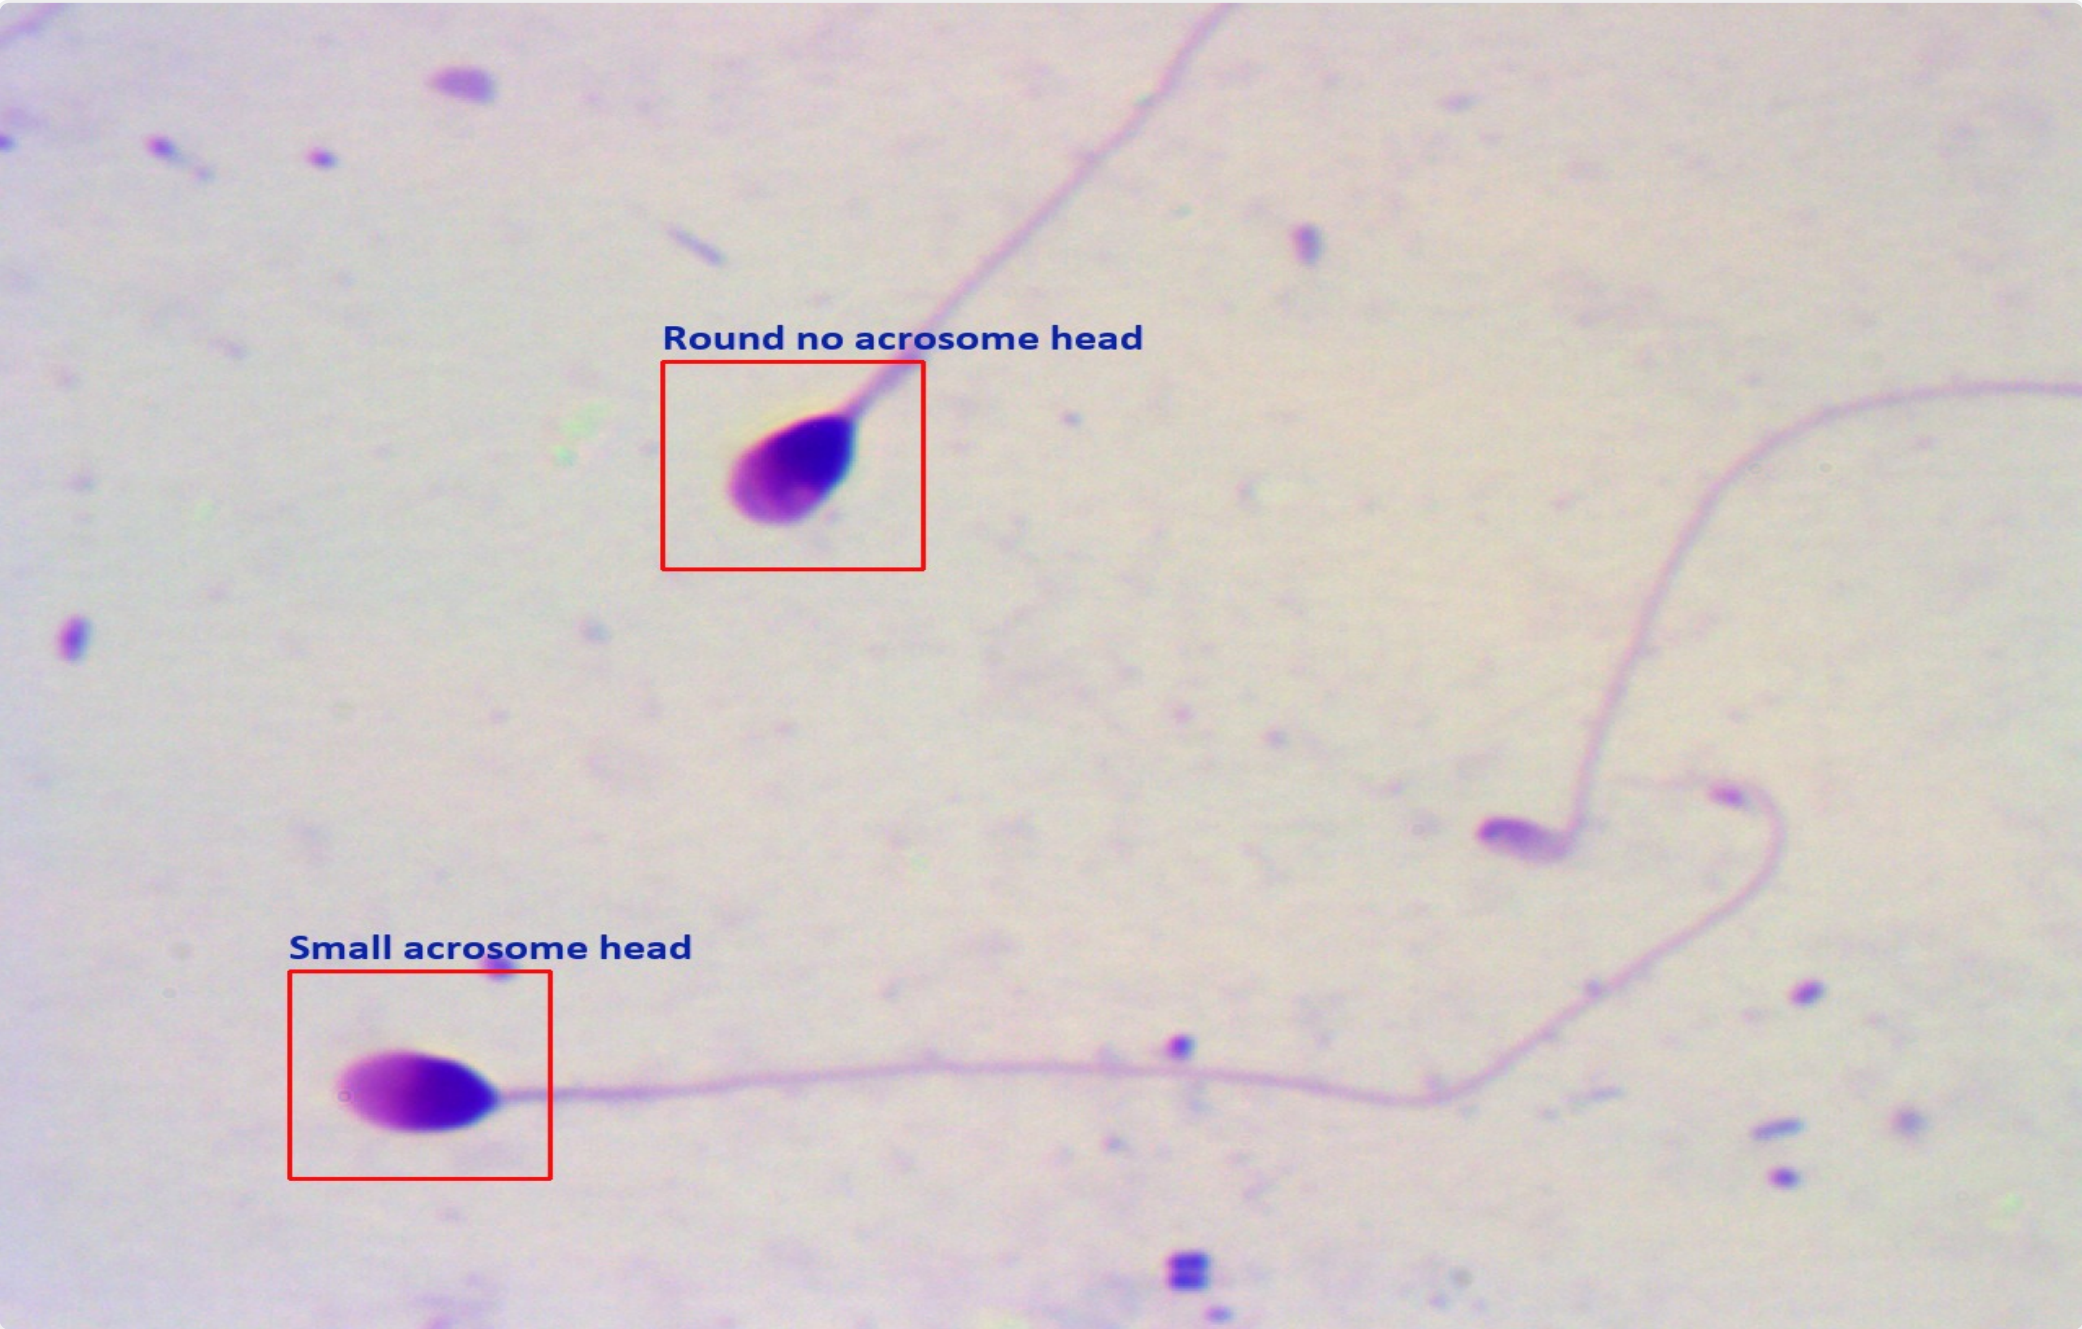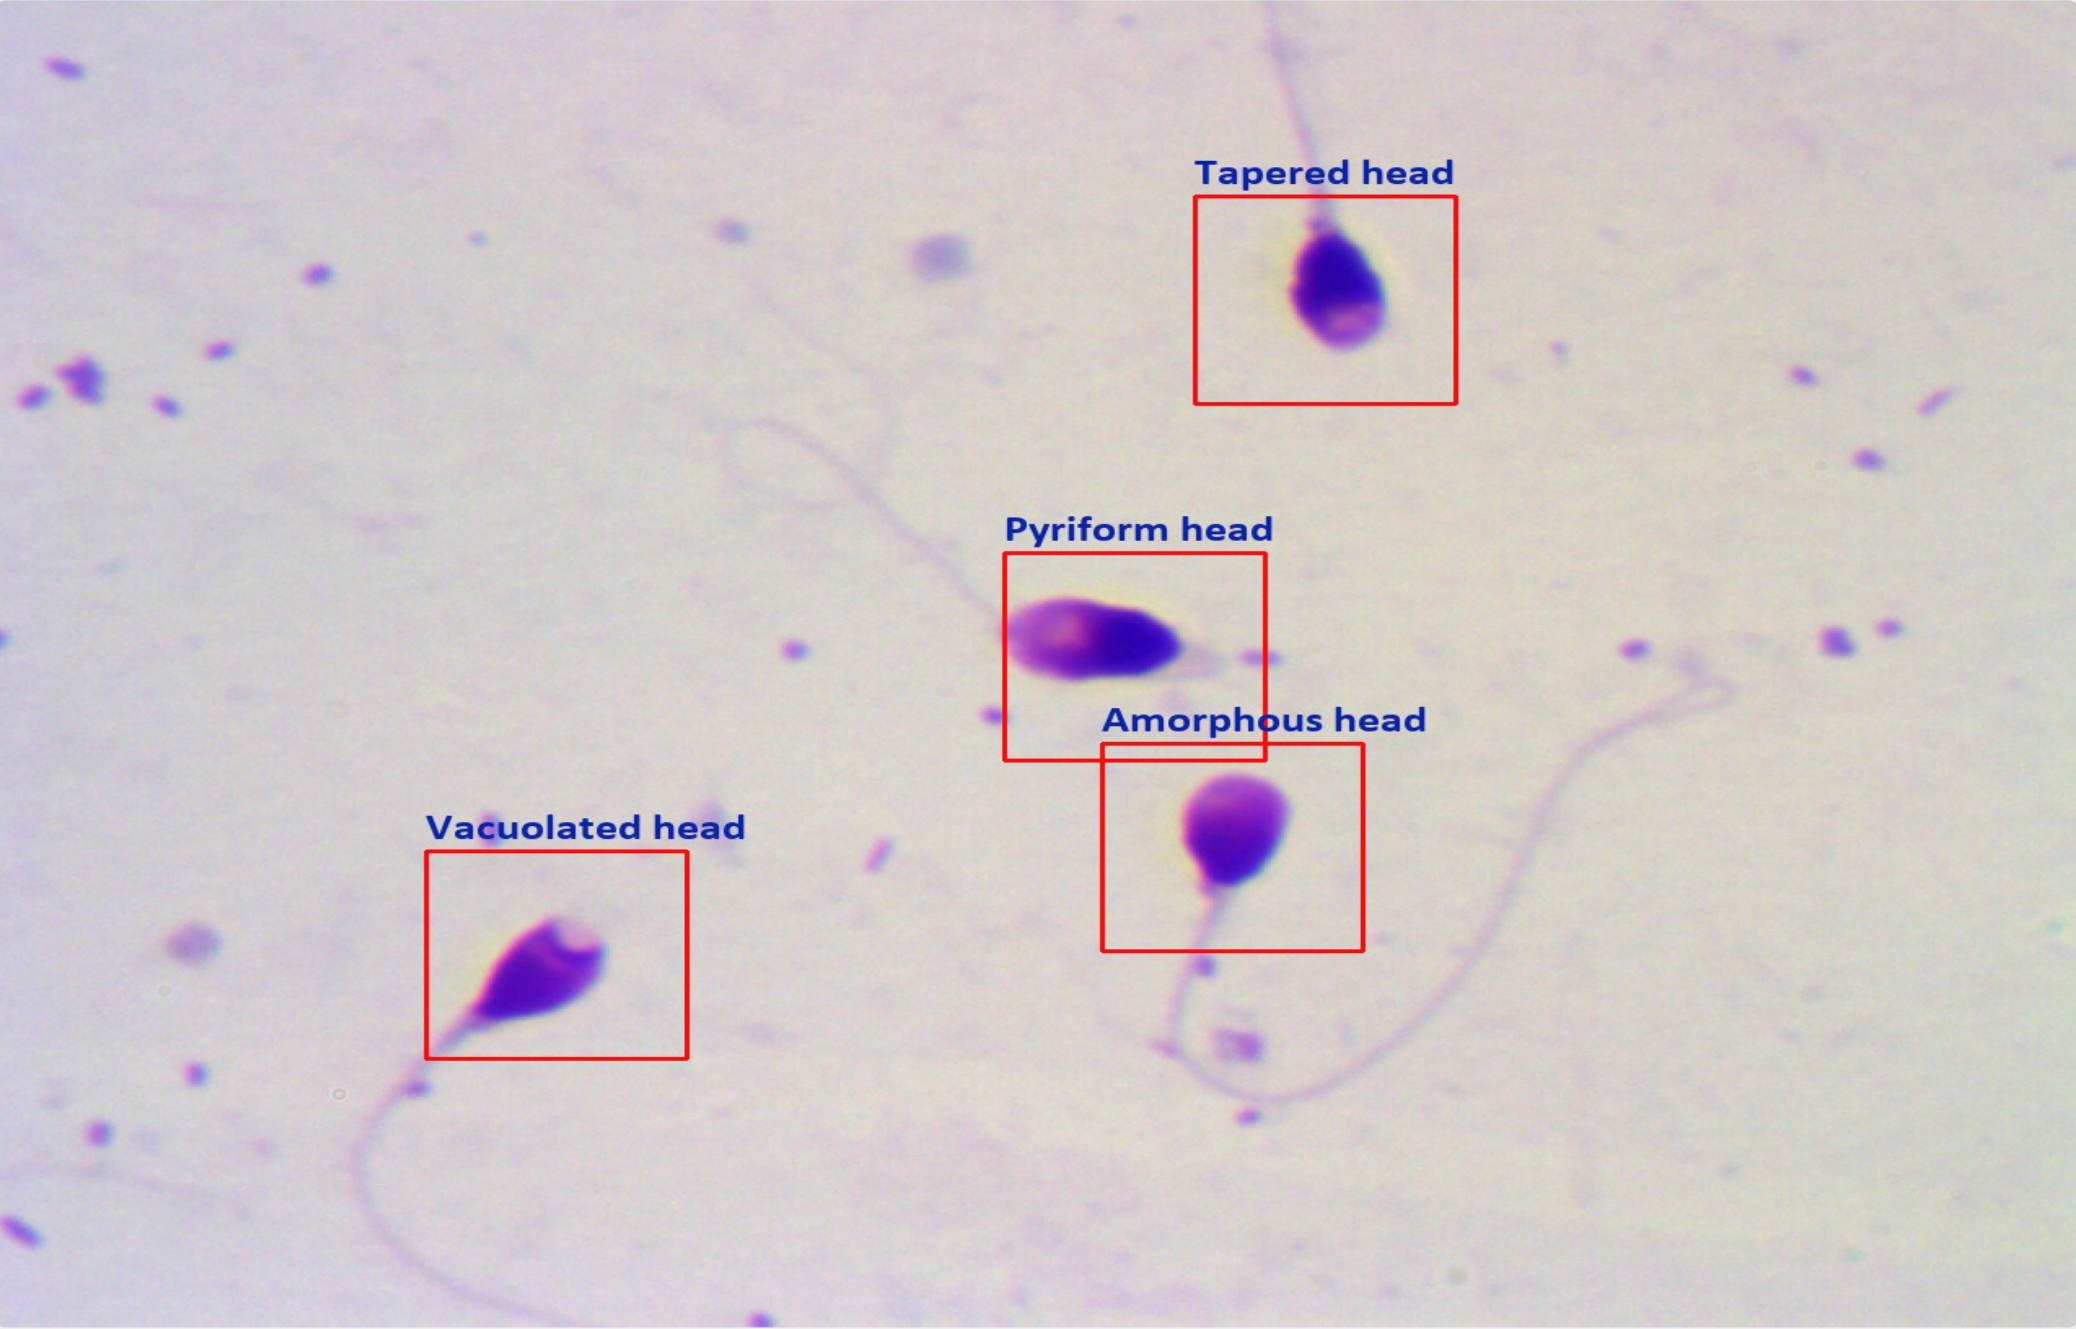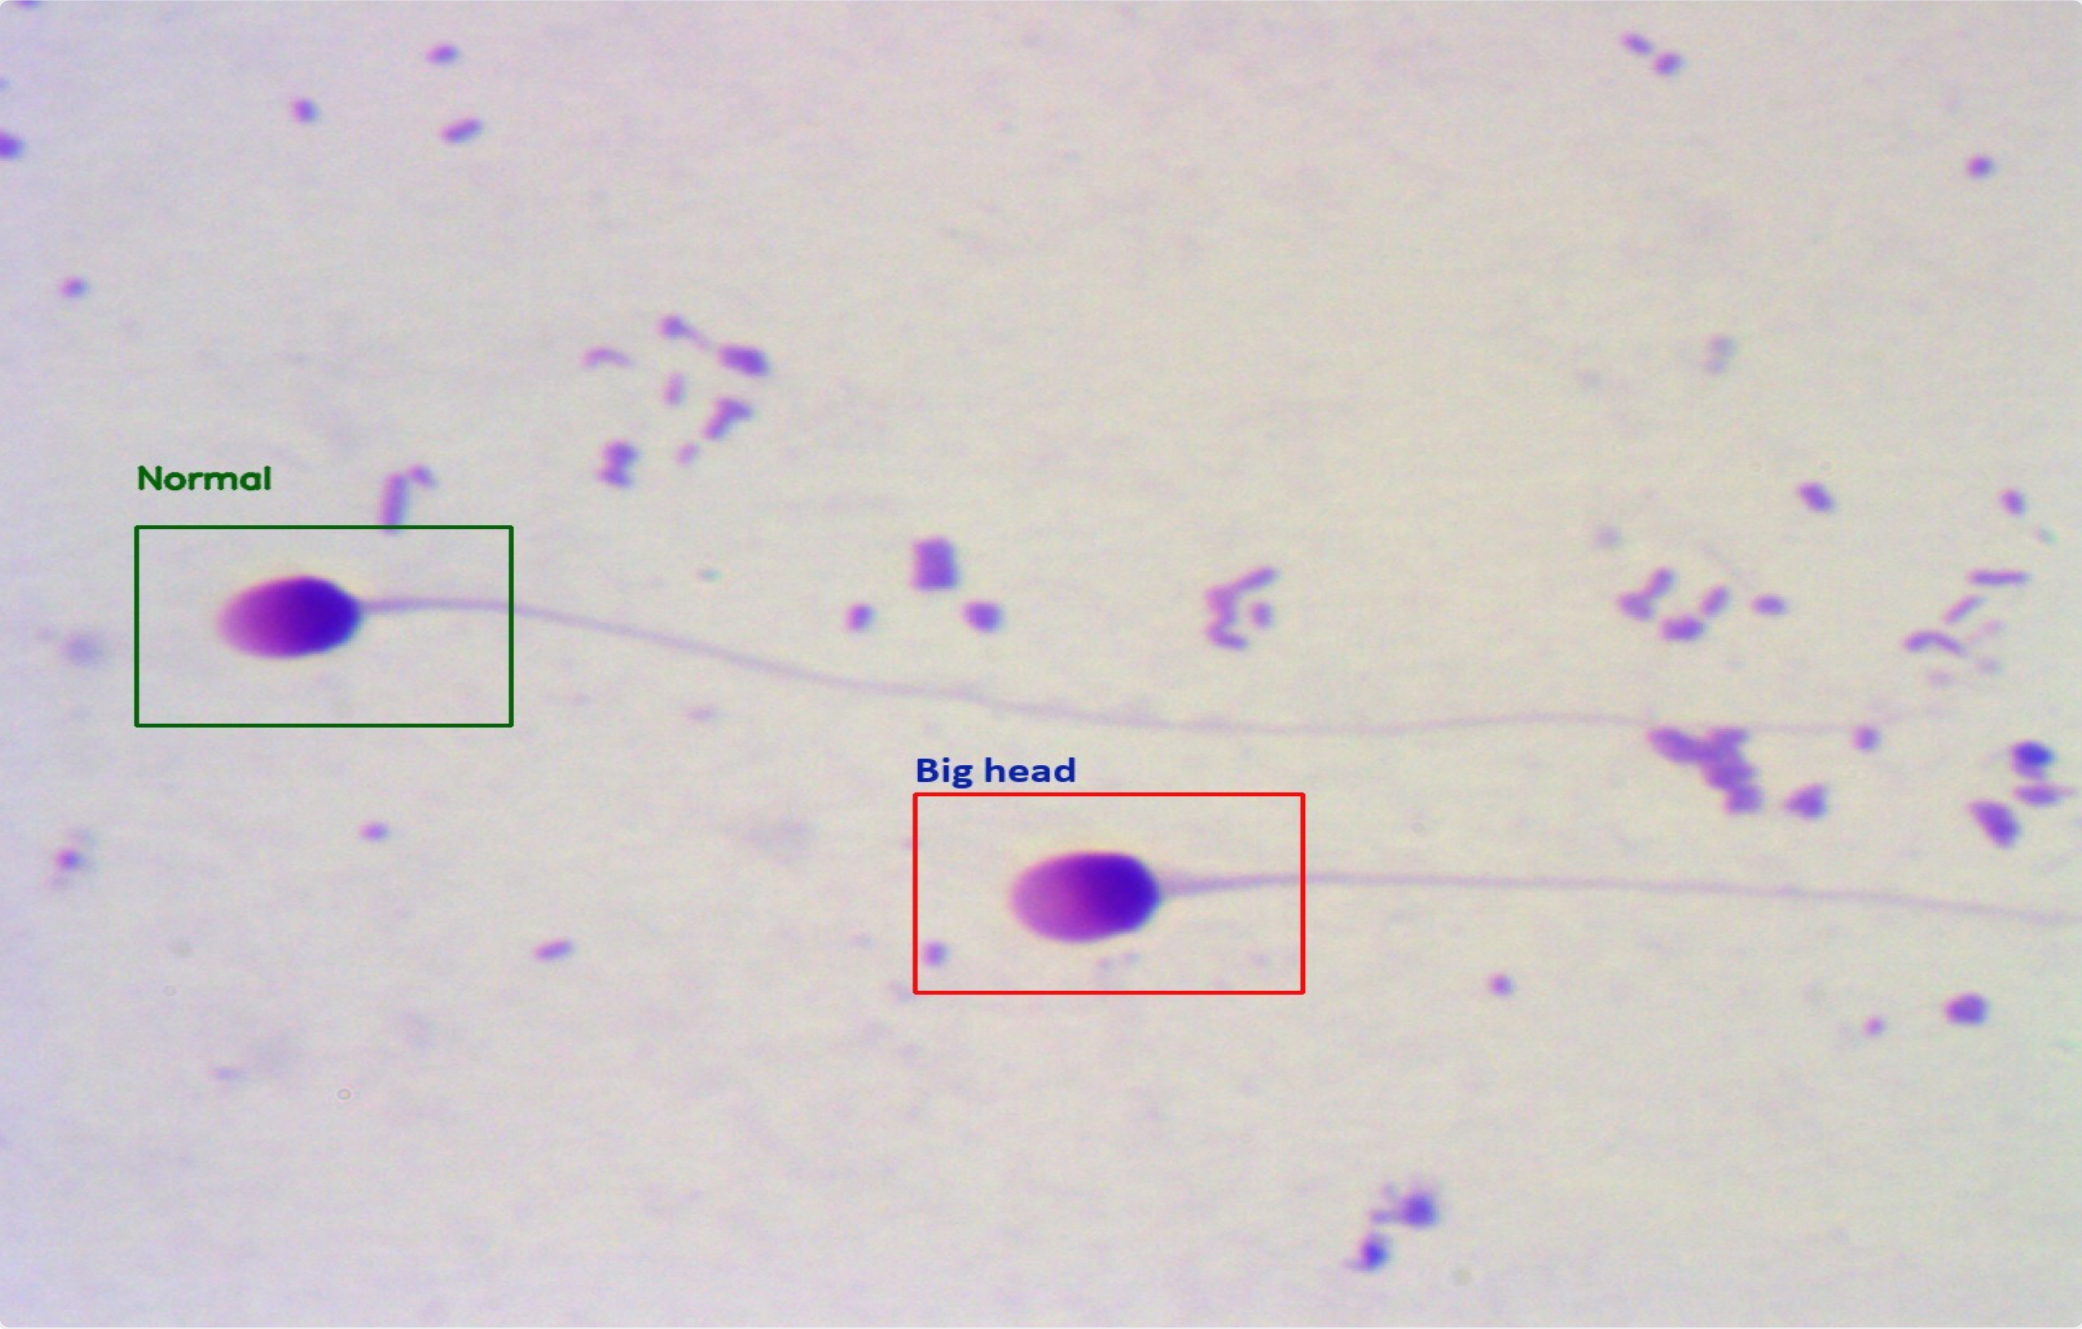

Head defects			Neck & midpiece defects		Tail defects	
Tapered	Pyriform	Round	Sharply bent	Asymmetrical	Short	Bent
Amorphous	Vacuolated	Small acrosome	Thick	Thin	Coiled	ERC

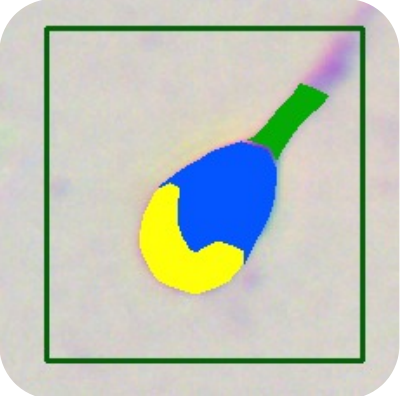

● Normal



● Pathology