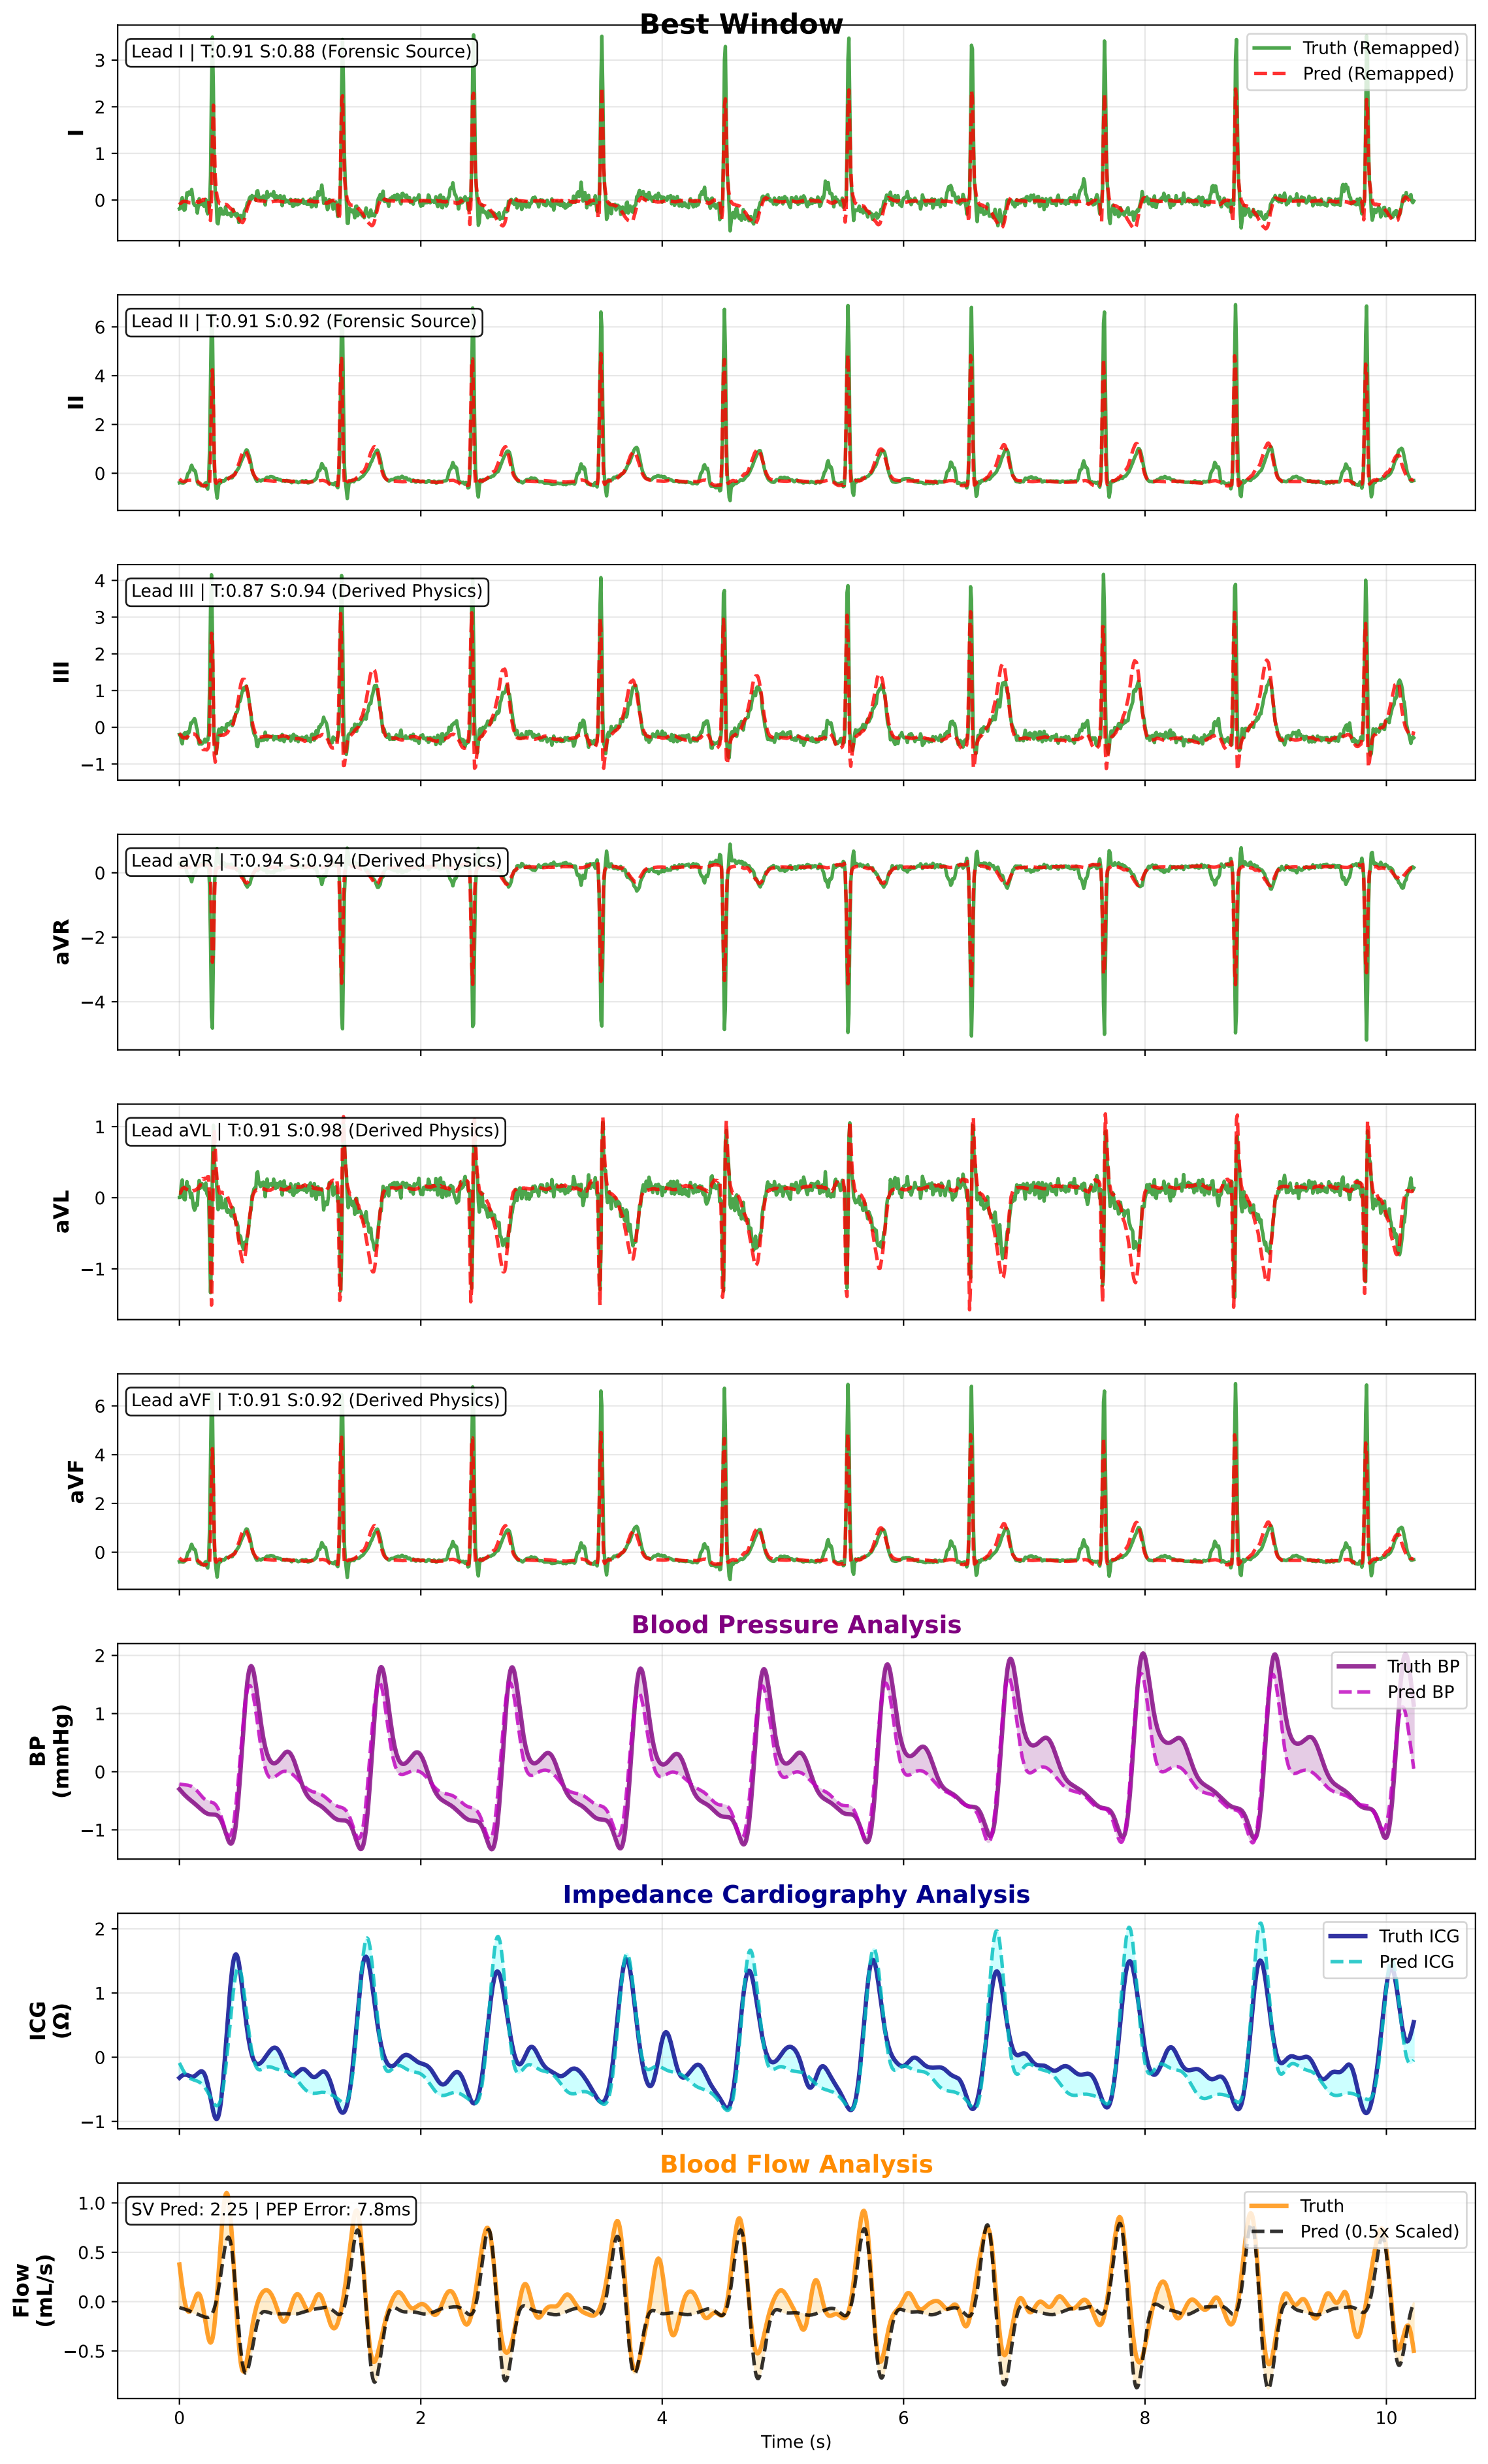
Best Window
Lead I | T:0.91 S:0.88 (Forensic Source)
Truth (Remapped)
Pred (Remapped)
I
Lead II | T:0.91 S:0.92 (Forensic Source)
II
Lead III | T:0.87 S:0.94 (Derived Physics)
III
Lead aVR | T:0.94 S:0.94 (Derived Physics)
aVR
Lead aVL | T:0.91 S:0.98 (Derived Physics)
aVL
Lead aVF | T:0.91 S:0.92 (Derived Physics)
aVF
Blood Pressure Analysis
BP (mmHg)
Truth BP
Pred BP
Impedance Cardiography Analysis
ICG (Ω)
Truth ICG
Pred ICG
Blood Flow Analysis
SV Pred: 2.25 | PEP Error: 7.8ms
Flow (mL/s)
Truth
Pred (0.5x Scaled)
Time (s)