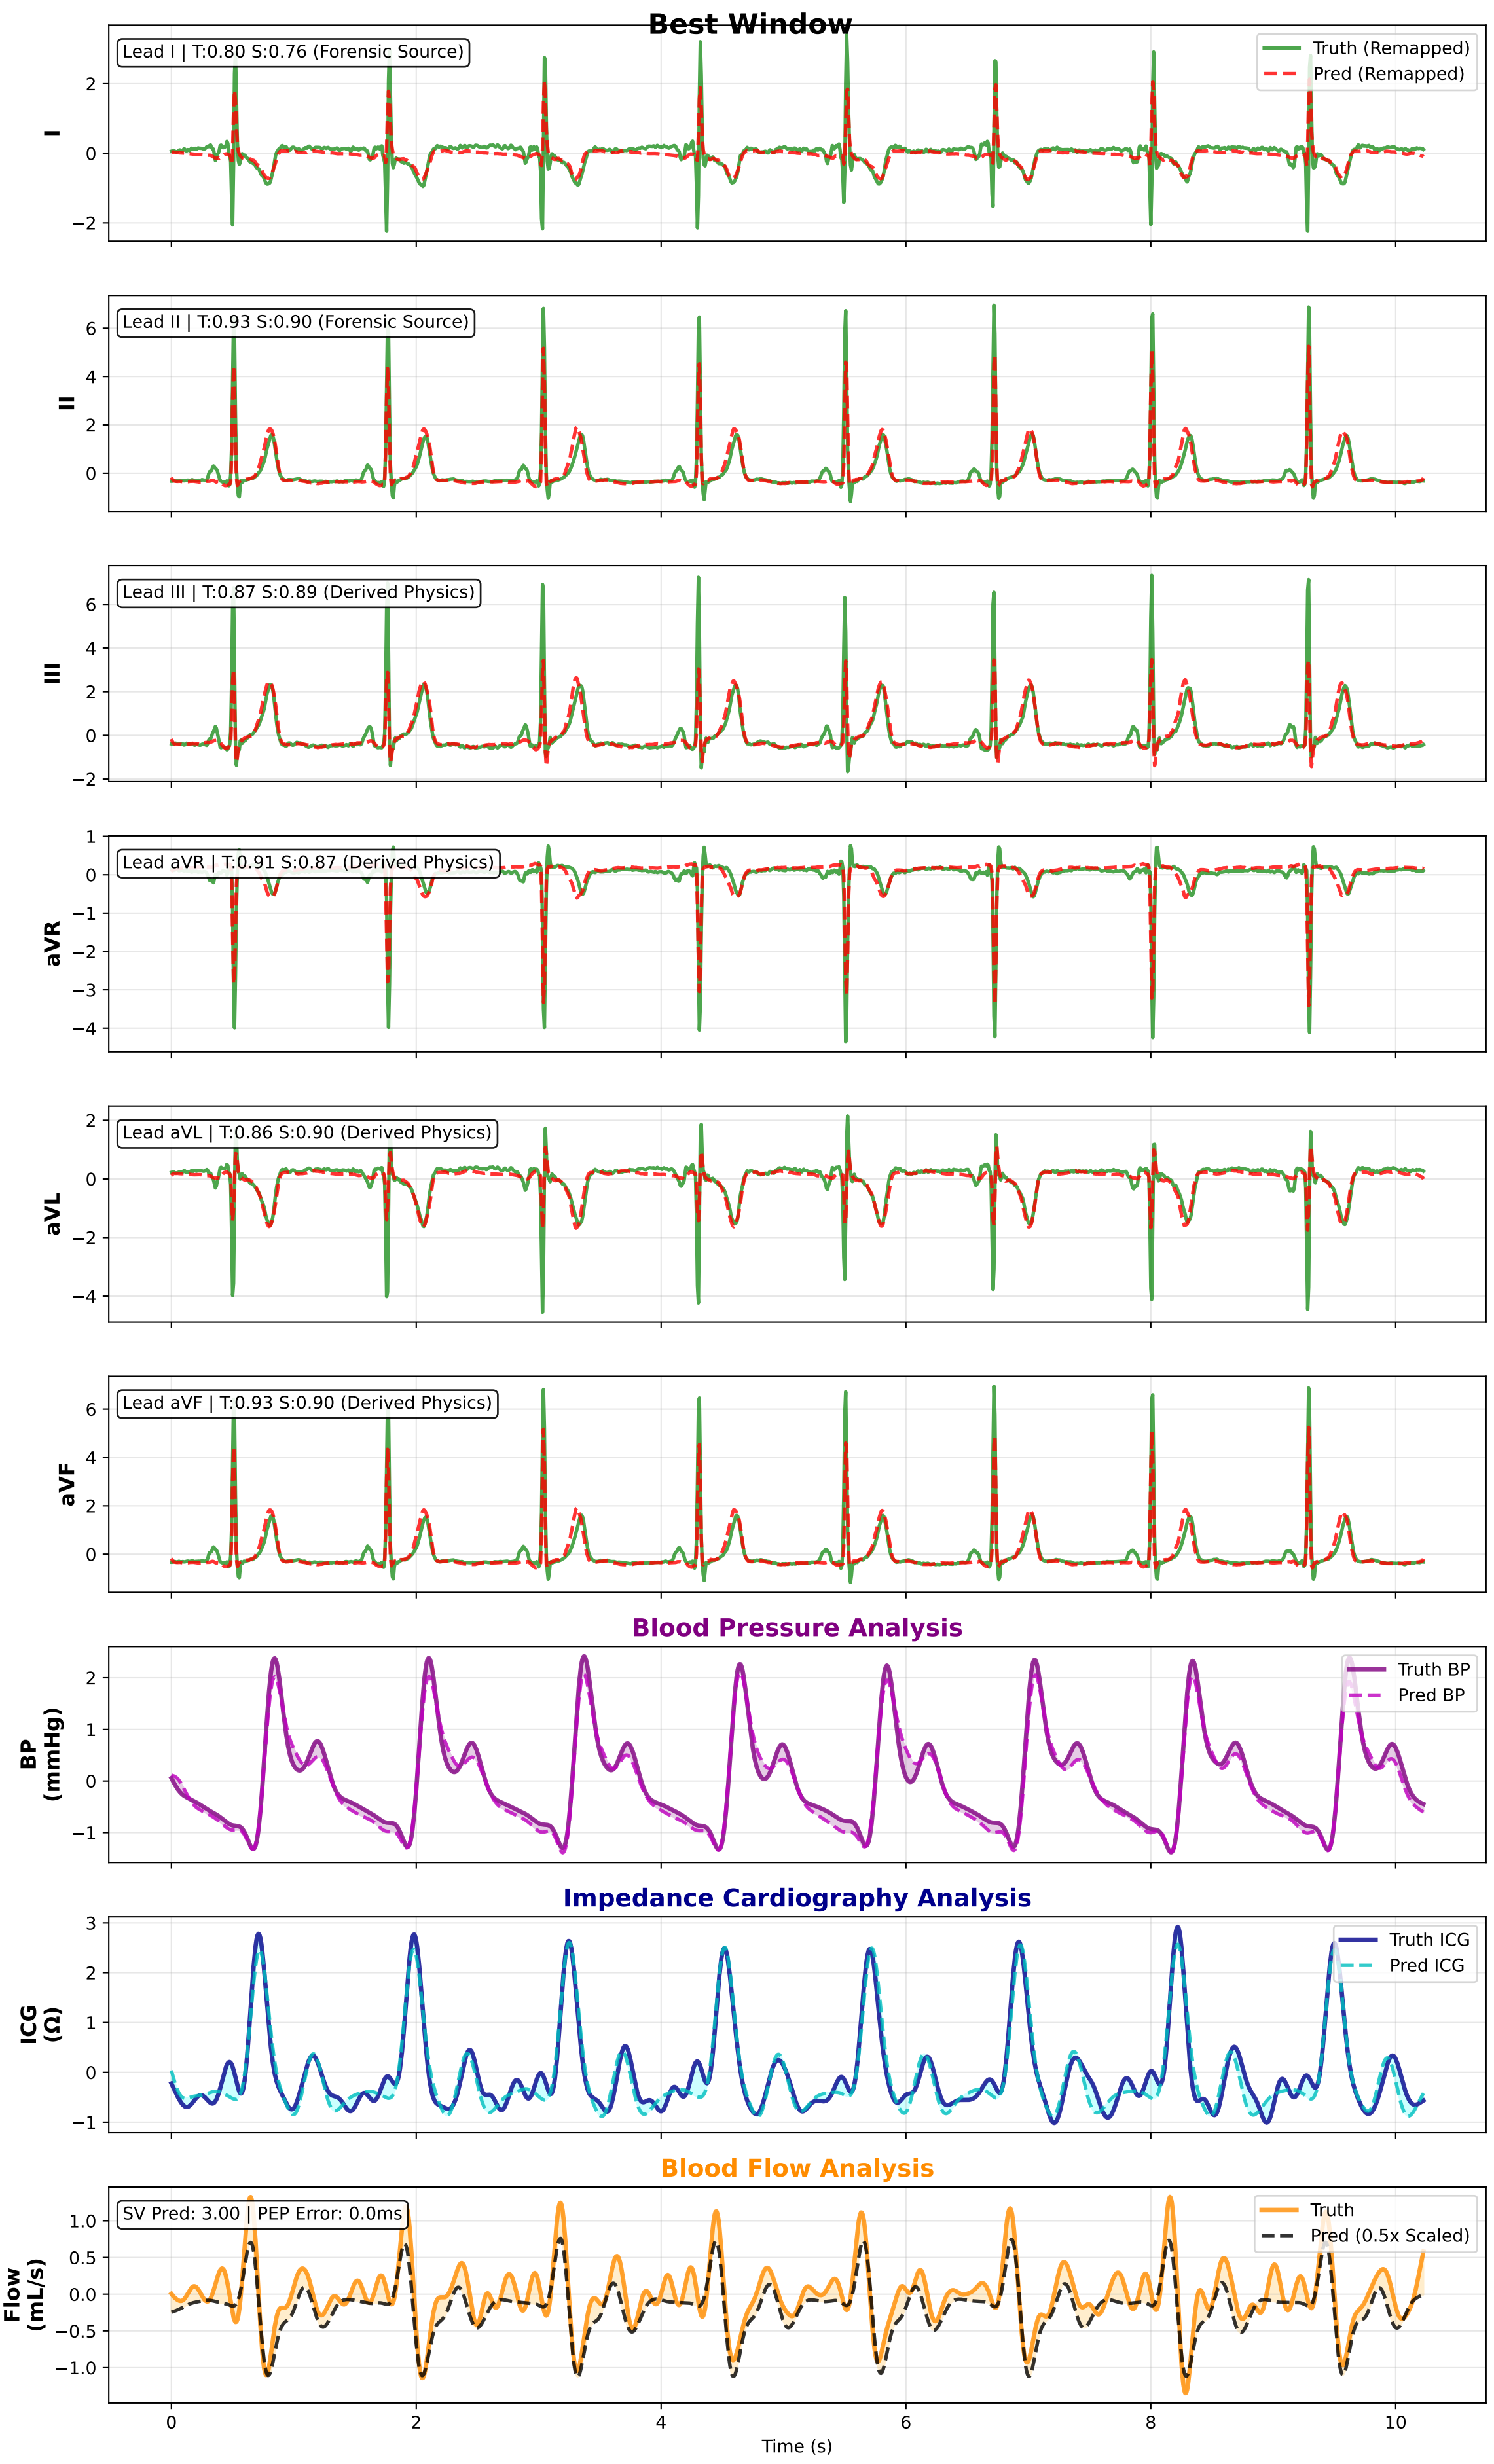
Best Window
Lead I | T:0.80 S:0.76 (Forensic Source)
Truth (Remapped)
Pred (Remapped)
I
Lead II | T:0.93 S:0.90 (Forensic Source)
II
Lead III | T:0.87 S:0.89 (Derived Physics)
III
Lead aVR | T:0.91 S:0.87 (Derived Physics)
aVR
Lead aVL | T:0.86 S:0.90 (Derived Physics)
aVL
Lead aVF | T:0.93 S:0.90 (Derived Physics)
aVF
Blood Pressure Analysis
Truth BP
Pred BP
BP (mmHg)
Impedance Cardiography Analysis
Truth ICG
Pred ICG
ICG (Ω)
Blood Flow Analysis
SV Pred: 3.00 | PEP Error: 0.0ms
Truth
Pred (0.5x Scaled)
Flow (mL/s)
Time (s)