




Exploratory plots: PFAS

Comparing bottled and tap water

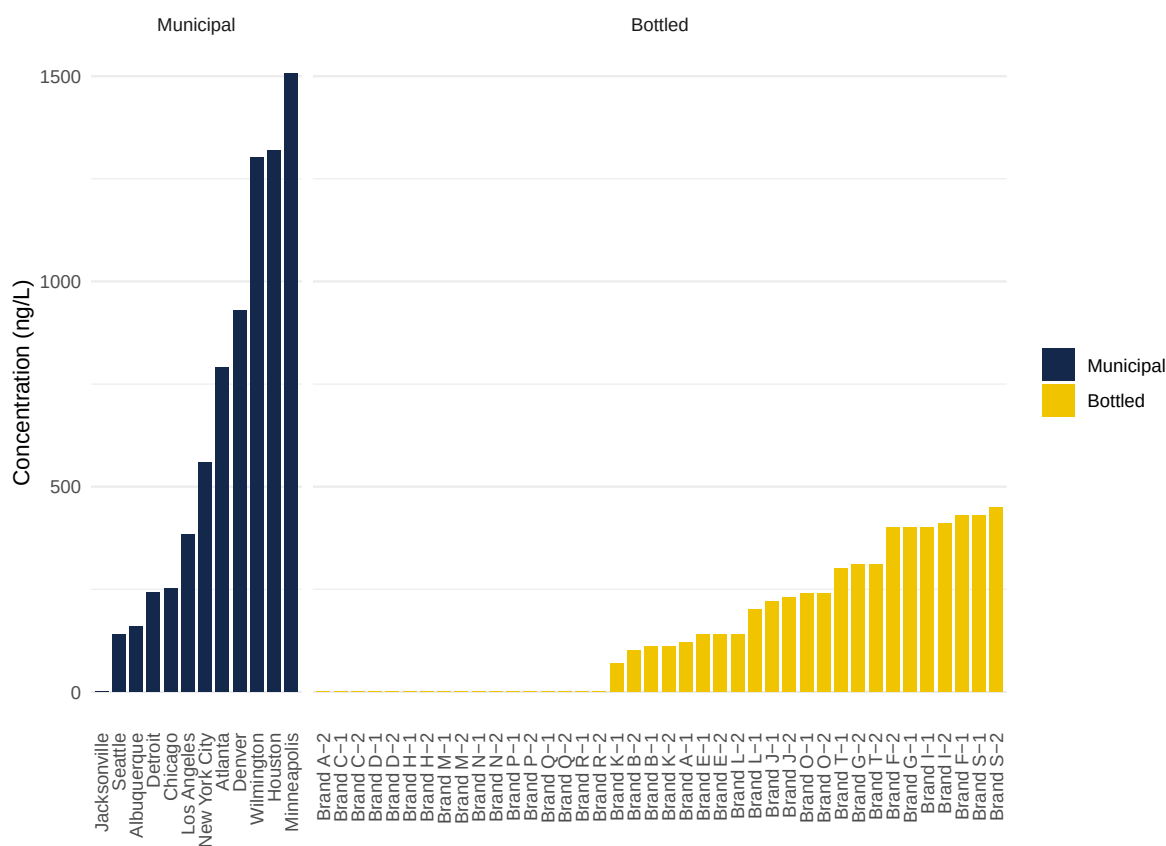


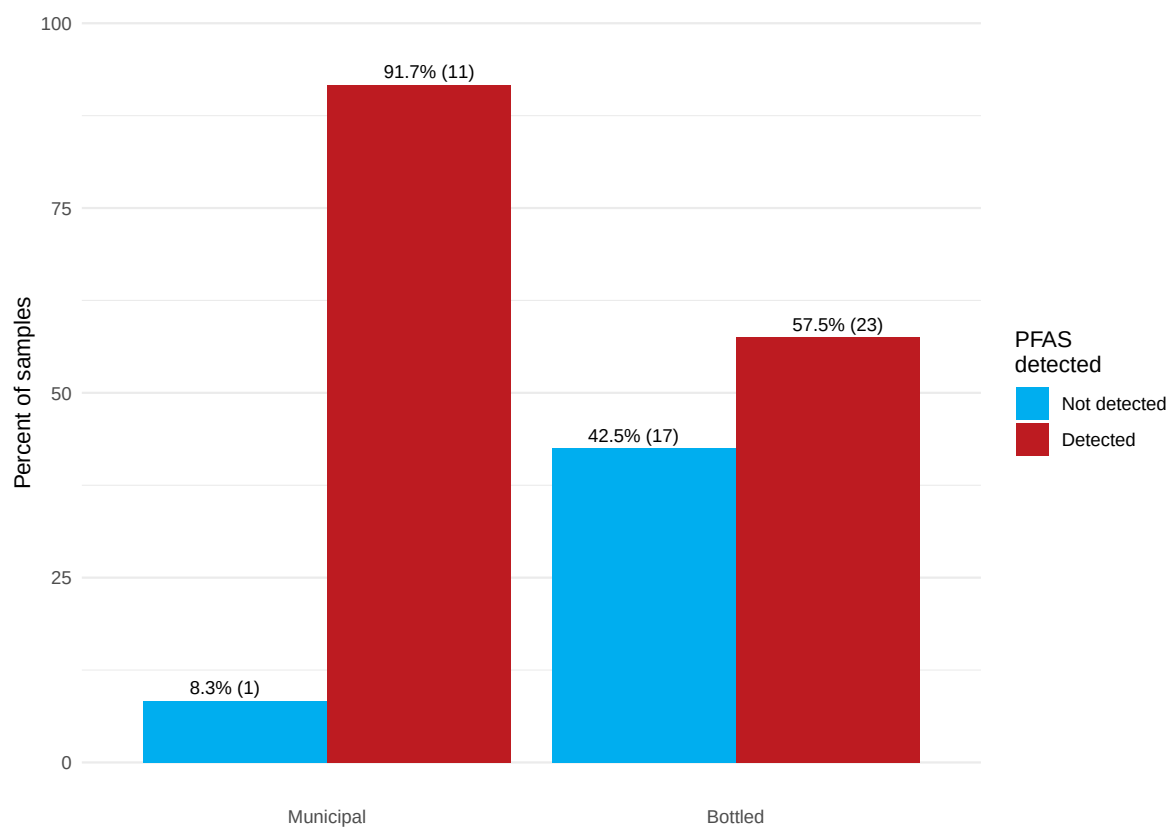

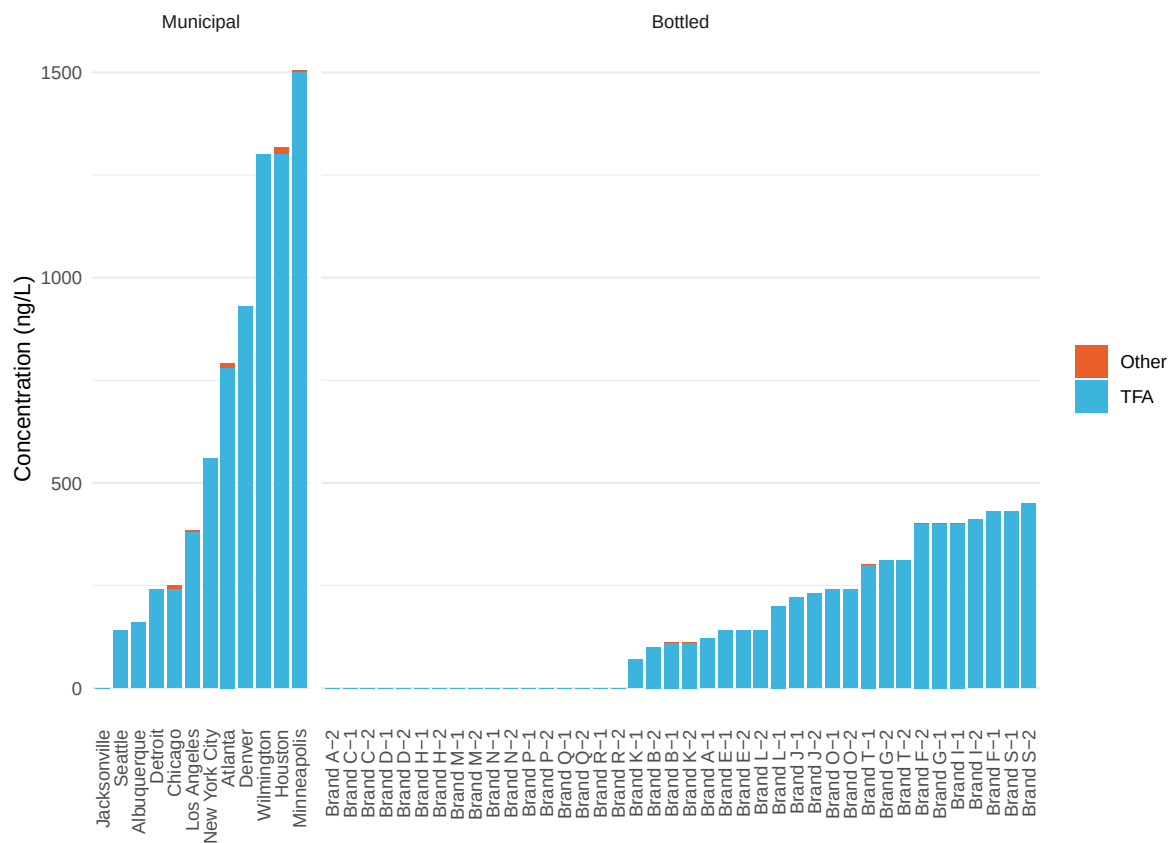


Concentration of non-TFA analytes


TFA comprises 99.6% of the sample. The remaining 0.4% is broken down into the following analytes.

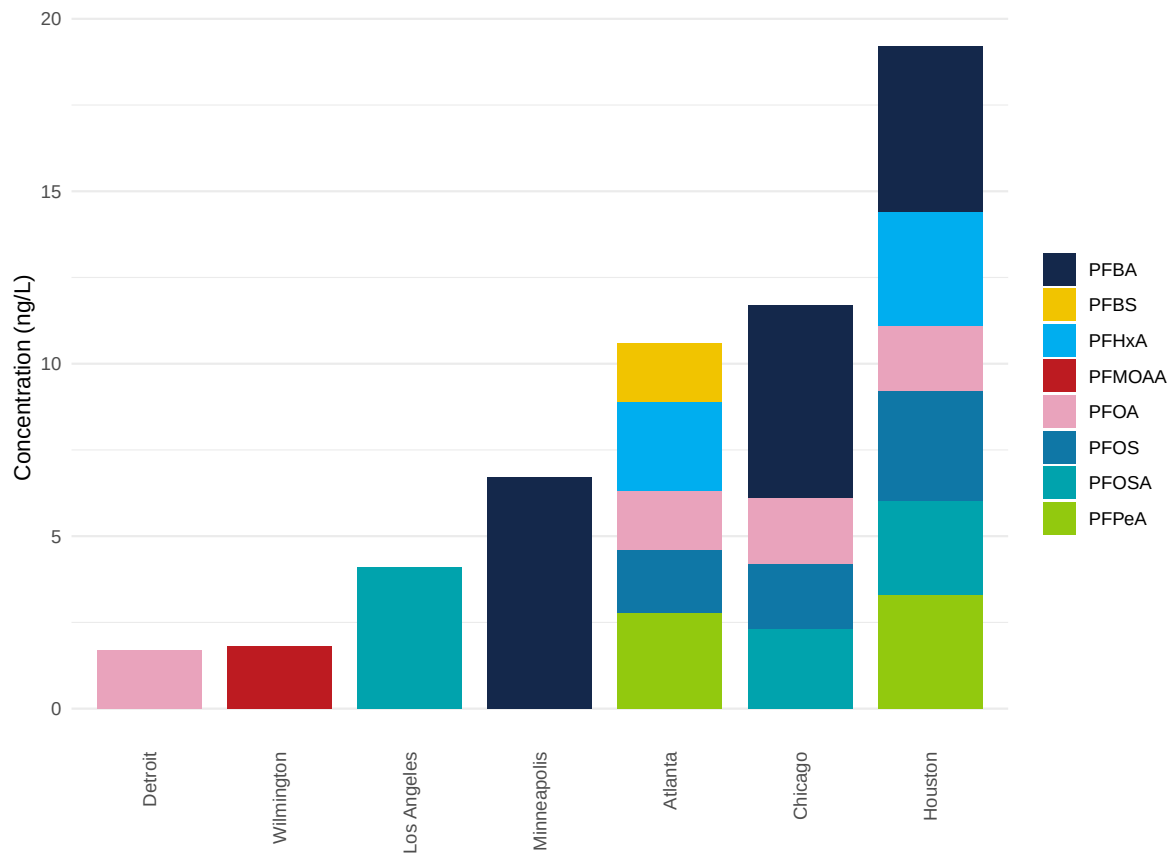


Analyte distribution

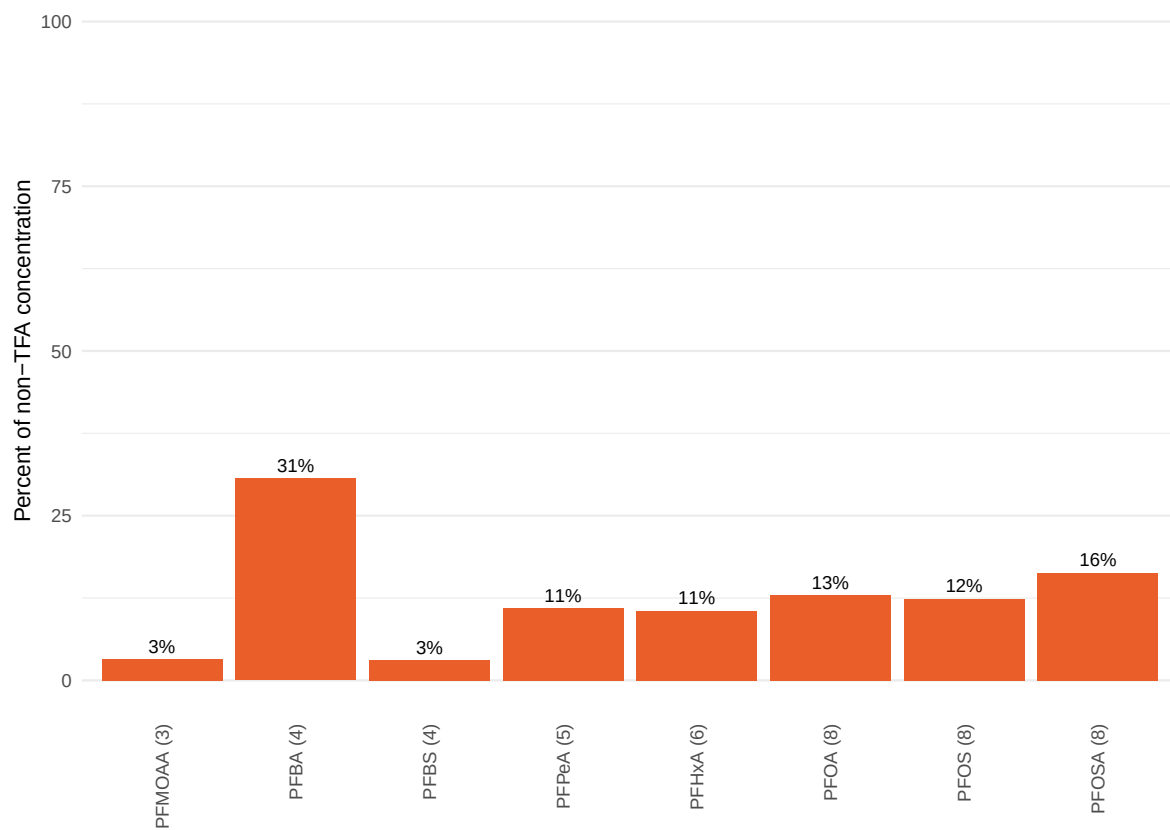


Comparing source type

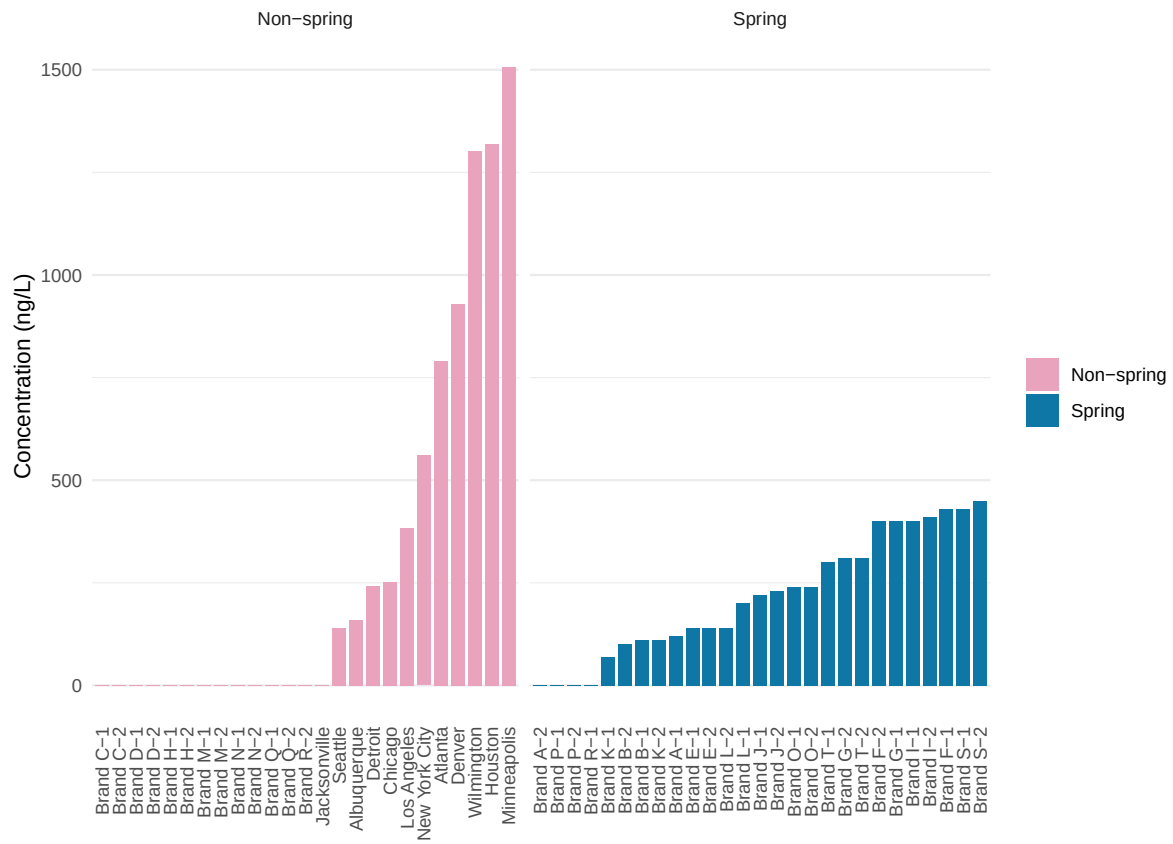

Comparing source type among bottled water samples

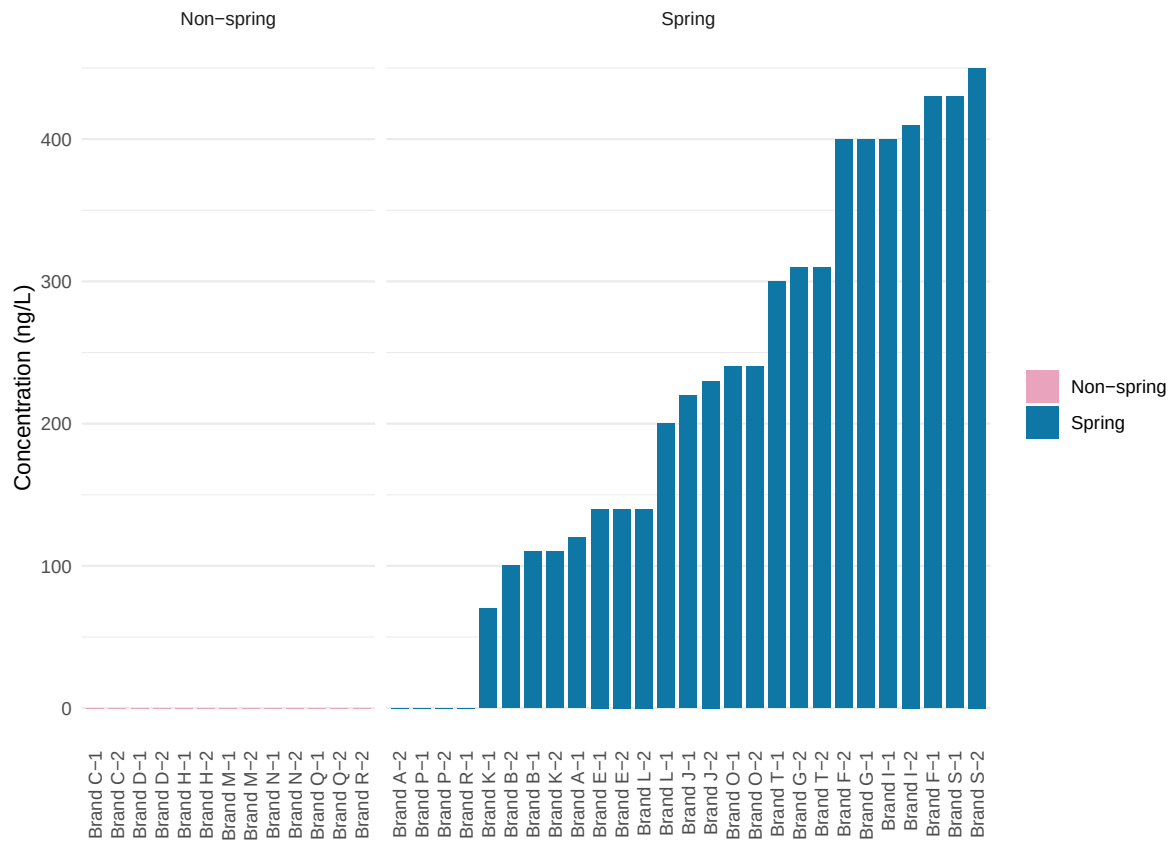

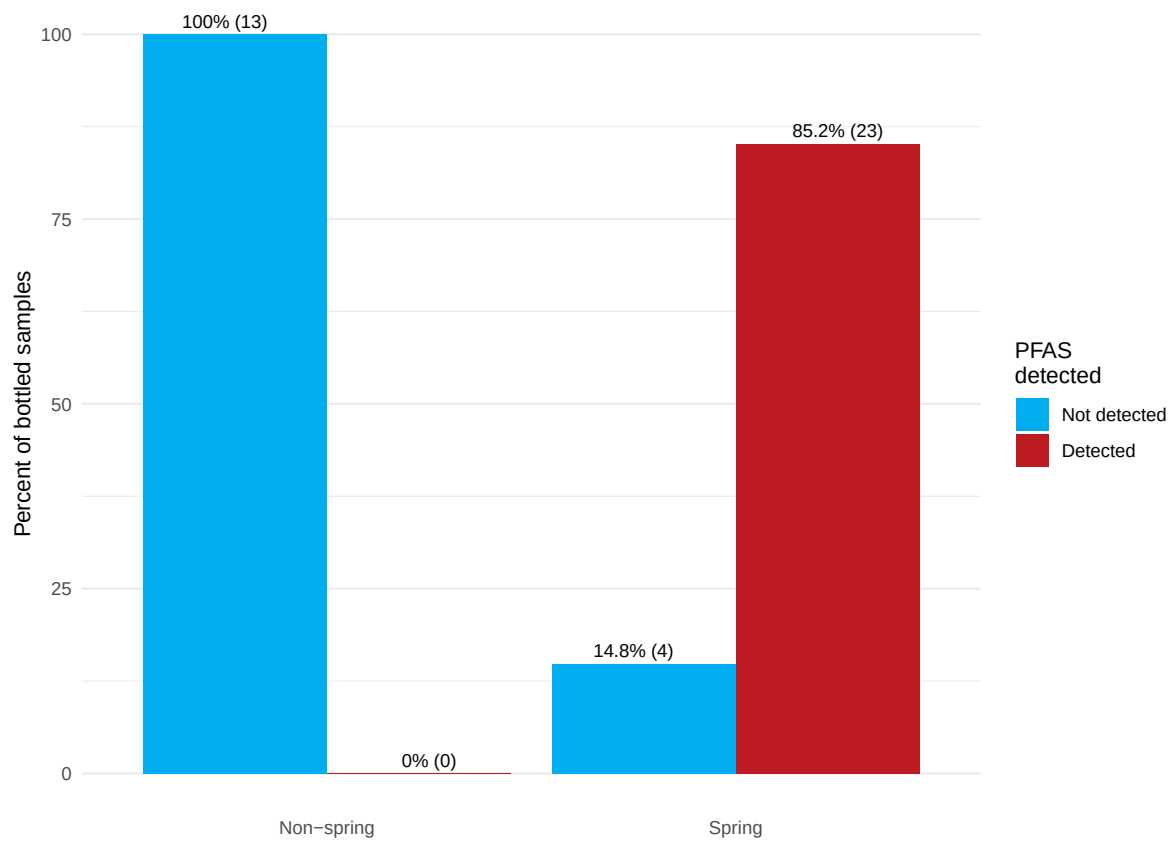

Comparing advanced filtration

