Ablation study: The incremental value of DAMS (AIPW)
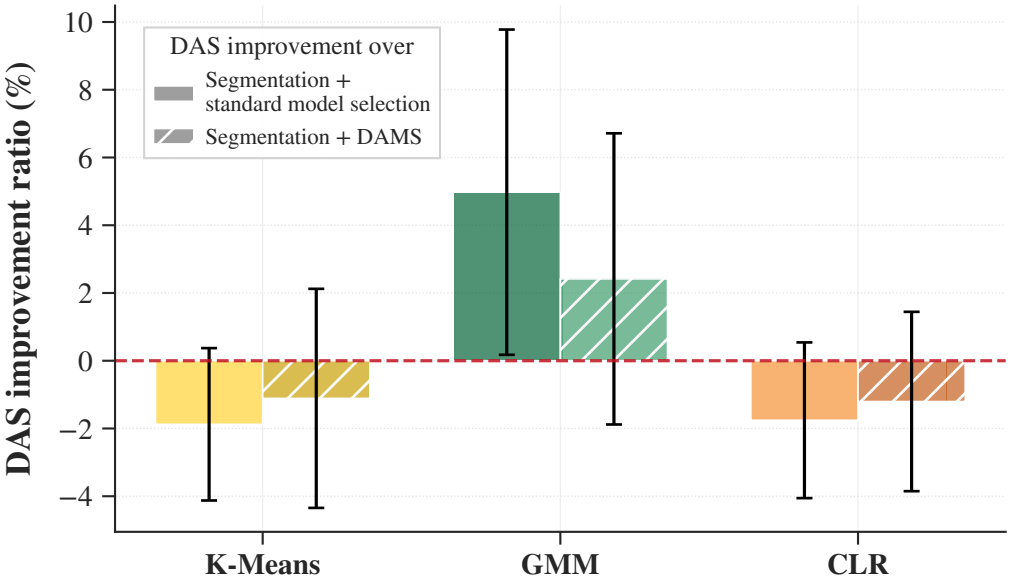
Each bar: mean ± 95% CI (50 runs);
higher = DAS better than comparator