


RETINAL SCREENING | RESEARCH PROTOTYPE

Case: IDRI_D_001 | 2026-09-25 14:19:07 | Quality: enhanced


Original (preview)

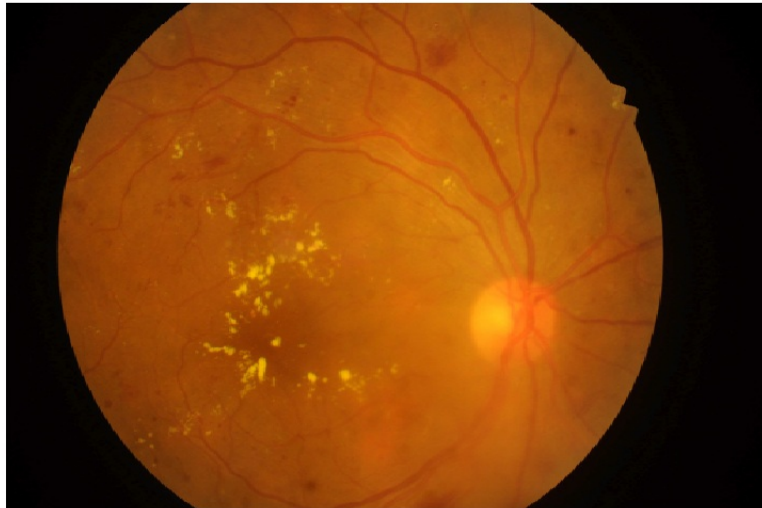


Enhanced / unchanged (preview)



Structure and lesion CANDIDATES

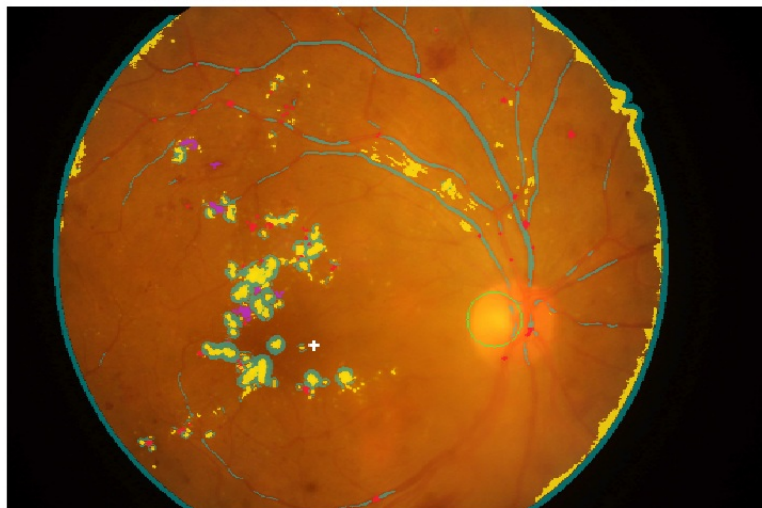

Grad-CAM | CNN attention

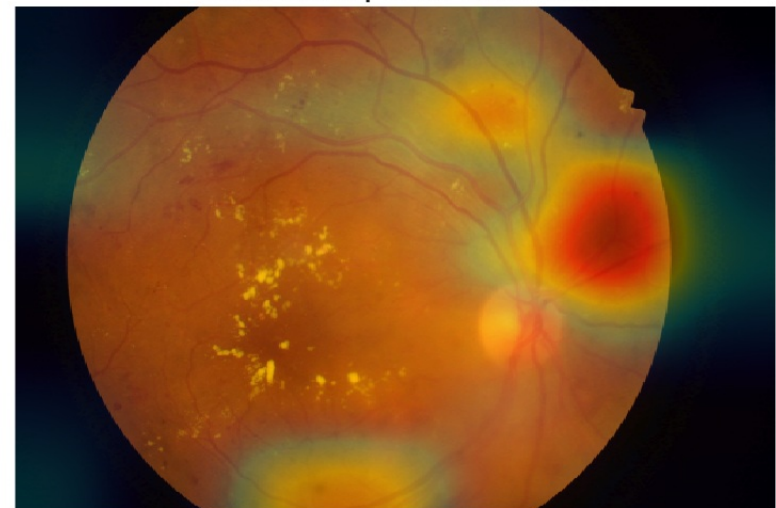

Overlay: cyan vessels | red MA candidates | purple hemorrhage candidates | yellow exudate candidates | green disc estimate | white fovea estimate

NOT A DIAGNOSIS. Unvalidated screening estimate; ophthalmologist confirmation required.

RESULTS, EVIDENCE AND REVIEW

Model grade: 4 / 4
Uncalibrated model score: 50.9%
Grade 2+ score: 99.0% | Meets configured referral threshold
Classifier: Trained CNN
Research screening estimate; doctor confirmation required.

Untrained candidates: MA 56 | Hemorrhages 6 | Exudates 151
Vessel area fraction: 0.055
Neovascularization: Not assessed: specialist review required
Optic disc/fovea: geometric estimates; anatomical coverage is not verified.
Analysis resolution: 768 x 511; native input: 4288 x 2848.

Quality: enhanced | Focus 0.000130886 | Mean intensity 0.355
Contrast 0.507 | Illumination CV 0.340 | Noise 0.0026
Operations: bounded illumination normalization
Feedback: Enhanced image passes provisional checks; compare with original.

Review: Pending | Reviewer: Nurse onsite
Doctor-recorded grade: Not recorded
Notes: High ablood Pressure

Research demo: no sensitivity/specificity guarantee. Lesion candidates require confirmation. Grad-CAM explains CNN attention and does not prove clinical correctness.
This report supplies no treatment or prescription.

RESULTS, EVIDENCE AND REVIEW

Model grade: 4 / 4
Uncalibrated model score: 50.9%
Grade 2+ score: 99.0% | Meets configured referral threshold
Classifier: Trained CNN
Research screening estimate; doctor confirmation required.

Untrained candidates: MA 56 | Hemorrhages 6 | Exudates 151
Vessel area fraction: 0.055
Neovascularization: Not assessed: specialist review required
Optic disc/fovea: geometric estimates; anatomical coverage is not verified.
Analysis resolution: 768 x 511; native input: 4288 x 2848.

Quality: enhanced | Focus 0.000130886 | Mean intensity 0.355
Contrast 0.507 | Illumination CV 0.340 | Noise 0.0026
Operations: bounded illumination normalization
Feedback: Enhanced image passes provisional checks; compare with original.

Review: Pending | Reviewer: Nurse onsite
Doctor-recorded grade: Not recorded
Notes: High ablood Pressure

Research demo: no sensitivity/specificity guarantee. Lesion candidates require confirmation. Grad-CAM explains CNN attention and does not prove clinical correctness.
This report supplies no treatment or prescription.