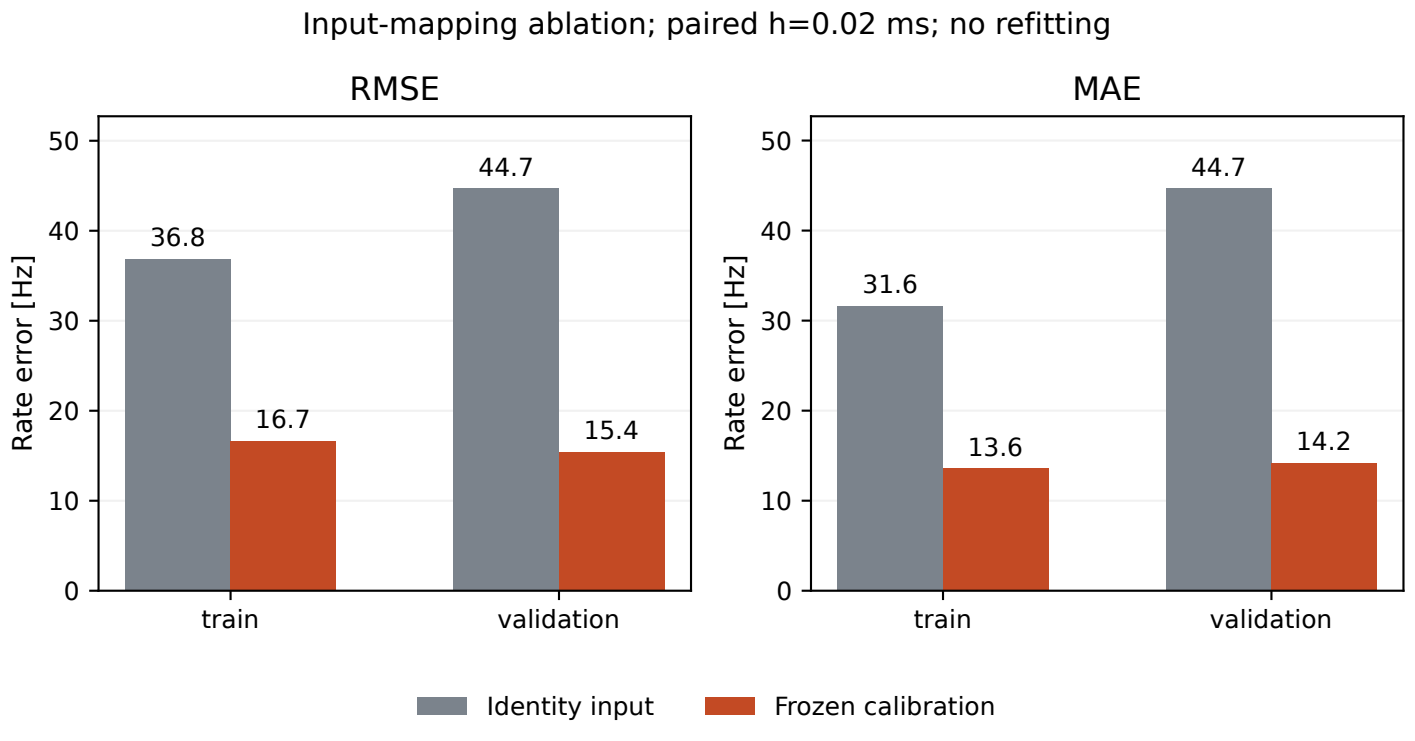
Input-mapping ablation; paired h=0.02 ms; no refitting
RMSE
MAE
Rate error [Hz]
0
10
20
30
40
50
36.8
16.7
44.7
15.4
31.6
13.6
44.7
14.2
train
validation
Identity input
Frozen calibration