



660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

CERTIFICATE OF ANALYSIS

Chlorpyrifos Oxon

CATALOG NUMBER MET-11459B-100MG
LOT NUMBER 11213100
DATE CERTIFIED 04/10/19
EXPIRATION DATE 04/30/22
CAS NUMBER 5598-15-2
MOLECULAR FORMULA C₉H₁₁Cl₃NO₄P
MOLECULAR WEIGHT 334.53
STORAGE Refrigerator storage (2 - 8 °C)
HANDLING See Safety Data Sheet
INTENDED USE For laboratory use only.
ISO 17034:2016 CERTIFIED []

Analytical Test	Value
% PURITY (GC/FID)	99.0

Chem Service, Inc. guarantees the purity to be +/- 0.5% deviation prior to the expiration date shown on the label and exclusive of any customer contamination.

Certified By:

Mary Beth O'Donnell

Mary Beth O'Donnell
CSM/TC

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



COA Form
Revision 3 (3/2015)

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

Gas

Data file: C:\CHEM3\

Sample name: Chlorpyrifos

CERTIFICATE OF ANALYSIS

Instrument: GC 2

Injection date: 4/10/2019 12:55:14 PM


Acq. method: MIX1.M

Column name: HP-5

Sample type:

Location: Vial 2

Injection volume: 1.0uL

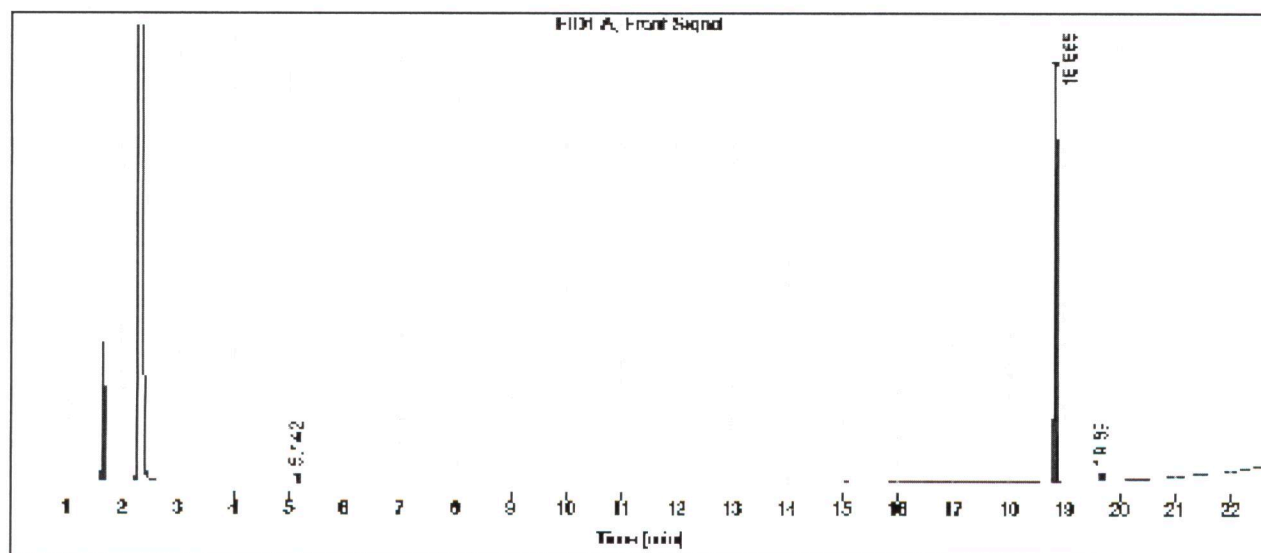

Signal: FID1 A, Front Signal

RT [min]	Type	Width [min]	Area	Height	Area%
5.142	BB	0.0320	7.4564	3.6229	0.38
18.655	BB	0.0352	1955.7860	870.0022	99.19
19.690	BB	0.0372	8.4708	3.6364	0.43
		Sum	1971.7132		

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015

