




(a) As recorded (ATR, 4 cm^{-1})

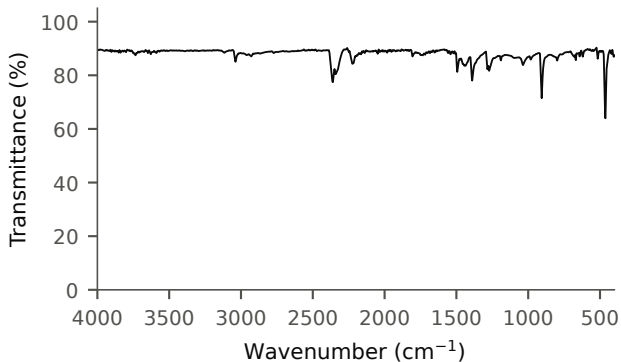

(b) Absorbance and baseline estimate

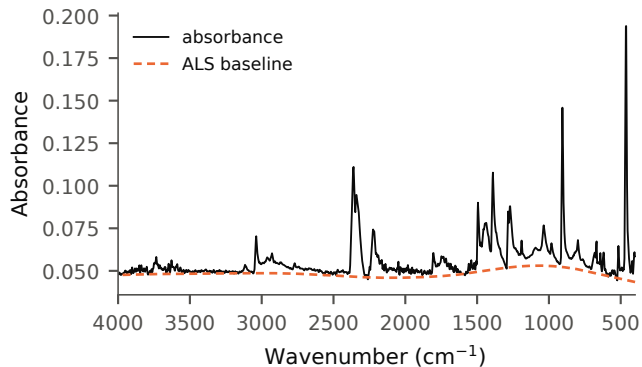

(c) Baseline corrected, normalised, bands detected

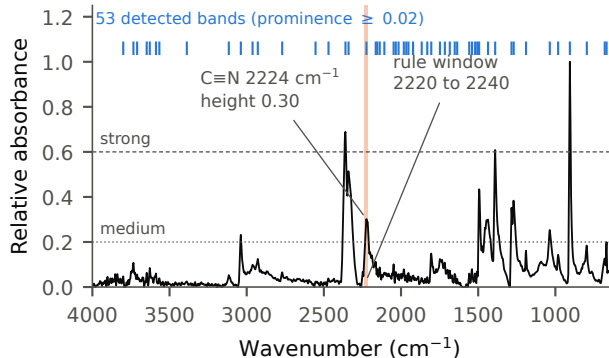

(d) Scoring the rule as a diagnostic test

Rule: aromatic nitrile, 2220 to 2240, intense
This spectrum:

position inside window yes
intensity $0.30 < 0.6$ no

All 1539 spectra, 69 nitriles:

position only

sens 0.78 spec 0.92
LR+ 10 LR- 0.24

with intensity clause

sens 0.06 spec 1.00
LR+ 189 LR- 0.94