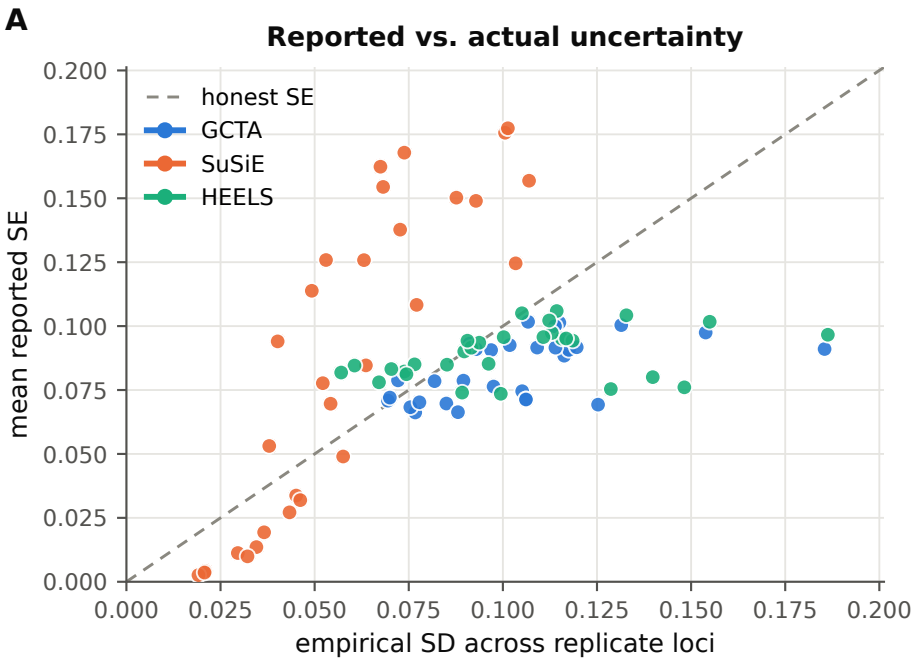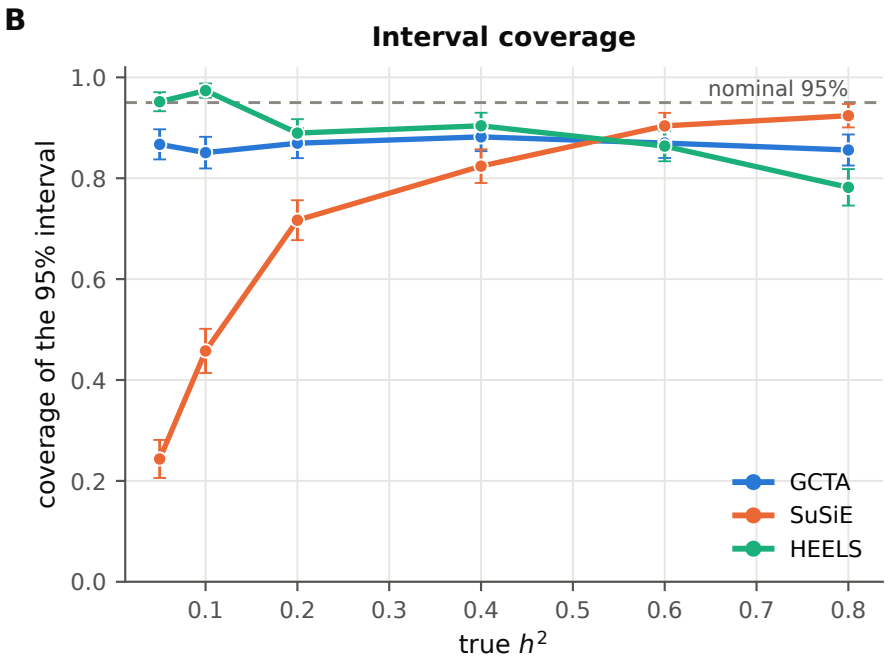# Calibration of the reported standard errors