

Certificate of Analysis

Product Information

Customer Code:Peptide KP3270-1
Lot No.:20240202
M. W.:2203.59
Sequence:YIGSGLNIMQLQHGLEEIMG
Store at:-20°C

KSVP Code:KP3270-1
Formula:
Quantity:3.0mg

Analytical Results

Tests	Specifications	Results
Appearance	white powder	Conforms
Purity(HPLC)	≥98%	99.73%
MS(ESI)	Calc.2203.59	Obs.2203.30

Prepared By:

Checked by:

Date:


HPLC Report

Sample Information

Customer Code: Peptide KP3270-1 KSVP Code: KP3270-1
 Lot No.: 20240202
 Phase A: 0.1% TFA in deionized water
 Phase B: 0.08% TFA in acetonitrile
 Flow rate: 1.0mL/min
 Wavelength: 214nm
 Analytical column type: ReproSil-Pur Basic-C18、5um、4.6*250mm
 Dissolution method: 20%ACN+80%H2O
 Inj. Volume: 10uL
 Date Acquired: 20240202, 09:43:04
 Gradient:


Time (min)	Phase A	Phase B
0.01	85%	15%
2.00	85%	15%
22.00	1%	99%
30.00	Stop	

Chromatogram

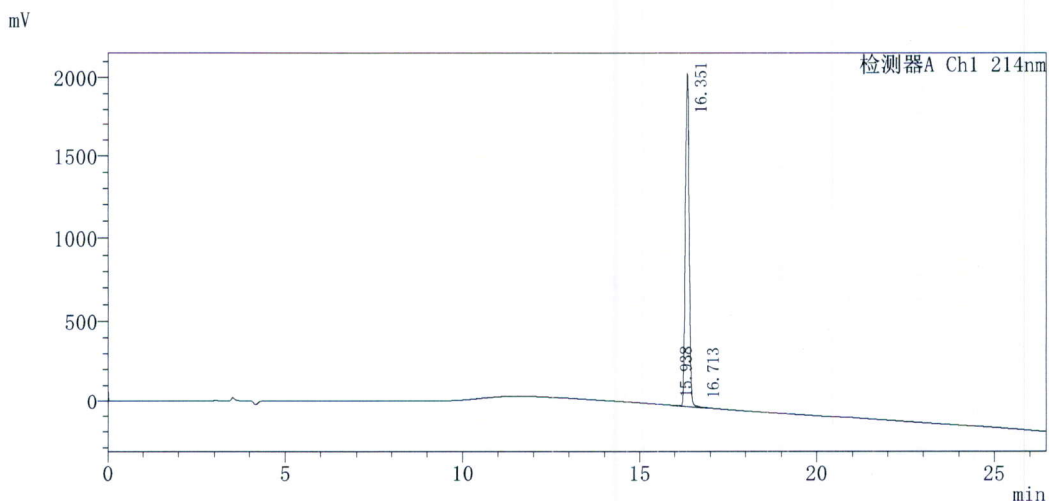

峰号	保留时间	峰面积	峰面积%	峰高	峰高%
1	15.938	15493	0.094	109	0.005
2	16.351	16472284	99.738	2065927	99.771
3	16.713	27788	0.168	4633	0.224

Mass Spectrometry Report

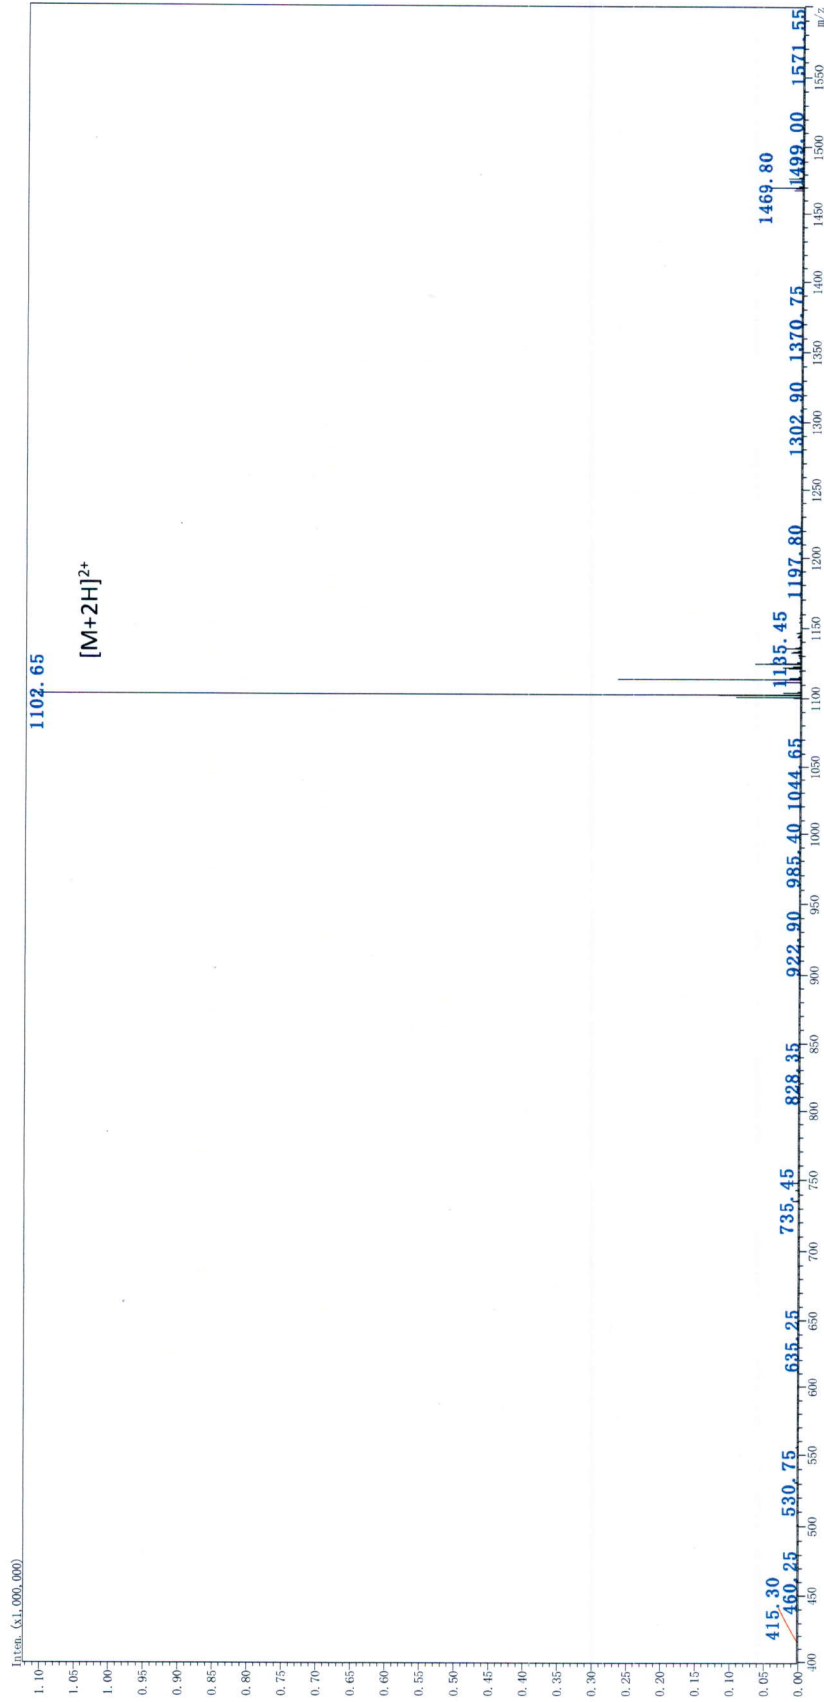

Sample Description

Analyzed date: 20240202,09:18

Analyst: WLL

Sample: KP32270-1:Peptide KP32270-1

M.W.: 2203.59

Lot. No.: 20240202

Instrument

Probe:

Nebulizer Gas Flow:

CDL:

CDL Temp.:

Block Temp.:

SHIMADZU LCMS-2020

ESI

1.5L/min

-20.0v

250 °C

200 °C

Probe Bias: +4.5kv

Detector: 1.5kv

T. Flow: 0.2ml/min

B. Conc.: 30%H₂O/30%ACN/40%MEOH

Certificate of Analysis

Product Information

Customer Code:Peptide KP3270-2
Lot No.:20240130
M. W.:2353.50
Sequence:ADARDGYGPHHLAELWWDDE
Store at:-20°C

KSVP Code:KP3270-2
Formula:
Quantity:3.0mg

Analytical Results

Tests	Specifications	Results
Appearance	white powder	Conforms
Purity(HPLC)	≥98%	98.10%
MS(ESI)	Calc.2353.50	Obs.2353.15

Prepared By:

Checked by:

Date:


HPLC Report

Sample Information

Customer Code: Peptide KP3270-2 KSVP Code: KP3270-2
 Lot No.: 20240130
 Phase A: 0.1% TFA in deionized water
 Phase B: 0.08% TFA in acetonitrile
 Flow rate: 1.0 mL/min
 Wavelength: 214 nm
 Analytical column type: Agilent 5 TC-C18、120A、5 μm、4.6*250 mm
 Dissolution method: 20% ACN + 80% H₂O
 Inj. Volume: 2 μL
 Date Acquired: 20240130, 19:57:54
 Gradient:


Time (min)	Phase A	Phase B
0.01	99%	1%
2.00	99%	1%
22.00	1%	99%
30.00	Stop	

Chromatogram

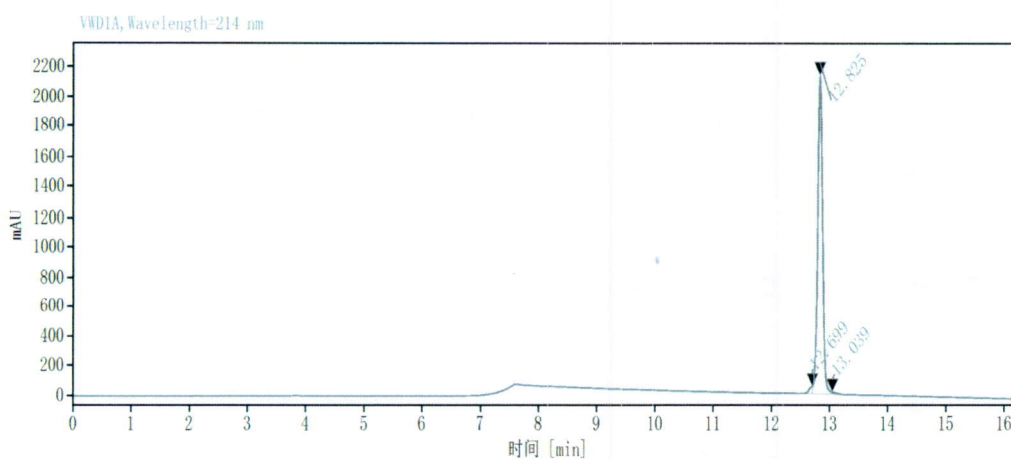

峰号	保留时间	峰面积	峰面积%	峰高	峰高%
1	12.699	182.6513	1.41	46.637	2.12
2	12.825	12739.2541	98.10	2137.695	97.30
3	13.039	64.2457	0.49	12.717	0.58

Mass Spectrometry Report

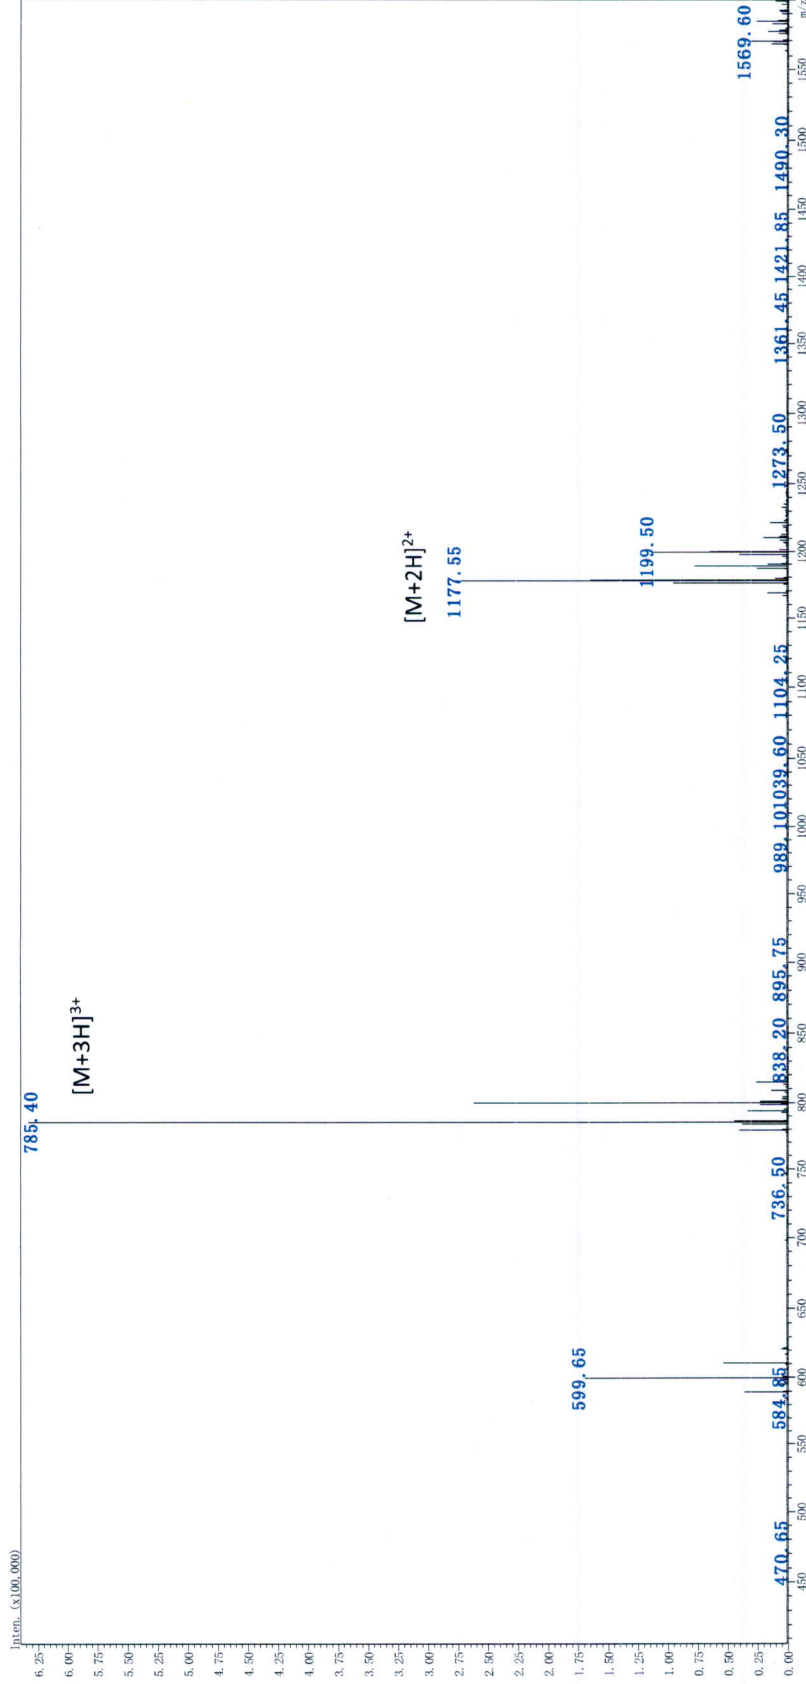

Sample Description

Analyzed date: 20240130,17:07

Analyst: WLL

Sample: KP3270-2:Peptide KP3270-2

M.W.: 2353.50

Lot. No.: 20240130

Instrument

Probe: ESI

Nebulizer Gas Flow: 1.5L/min

CDL: -20.0v

CDL Temp.: 250 °C

Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv

Detector: 1.5kv

T. Flow: 0.2ml/min

B. Conc.: 30%H₂O/30%ACN/40%MEOH

Certificate of Analysis

Product Information

Customer Code:Peptide KP3270-4
Lot No.:20240124
M. W.:2199.60
Sequence:PNLAEGMILHKGLEKLEIHHG
Store at:-20°C

KSVP Code:KP3270-4
Formula:
Quantity:3.0mg

Analytical Results

Tests	Specifications	Results
Appearance	white powder	Conforms
Purity(HPLC)	≥98%	99.32%
MS(ESI)	Calc.2199.60	Obs.2199.25

Prepared By:

Checked by:

Date:


HPLC Report

Sample Information

Customer Code: Peptide KP3270-4 KSVP Code: KP3270-4
 Lot No.: 20240124
 Phase A: 0.1% TFA in deionized water
 Phase B: 0.08% TFA in acetonitrile
 Flow rate: 1.0 mL/min
 Wavelength: 214 nm
 Analytical column type: YMC-Pack ODS-A、120A、5 μm、4.6*250 mm
 Dissolution method: 100% H₂O
 Inj. Volume: 5 μL
 Date Acquired: 20240124, 15:03:16
 Gradient:


Time (min)	Phase A	Phase B
0.01	85%	15%
2.00	85%	15%
22.00	1%	99%
30.00	Stop	

Chromatogram

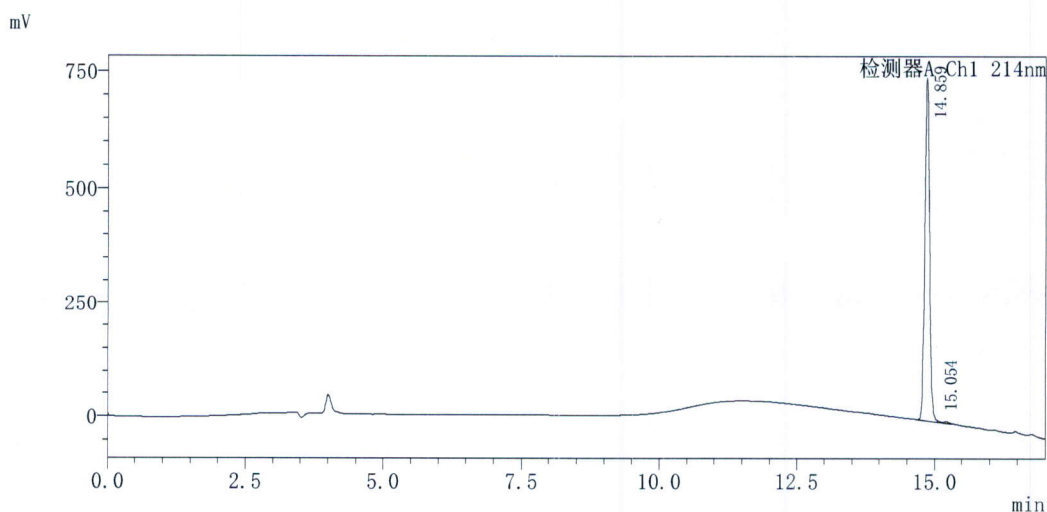

峰号	保留时间	峰面积	峰面积%	峰高	峰高%
1	14.859	4469207	99.328	747158	99.575
2	15.054	30239	0.672	3192	0.425

Mass Spectrometry Report

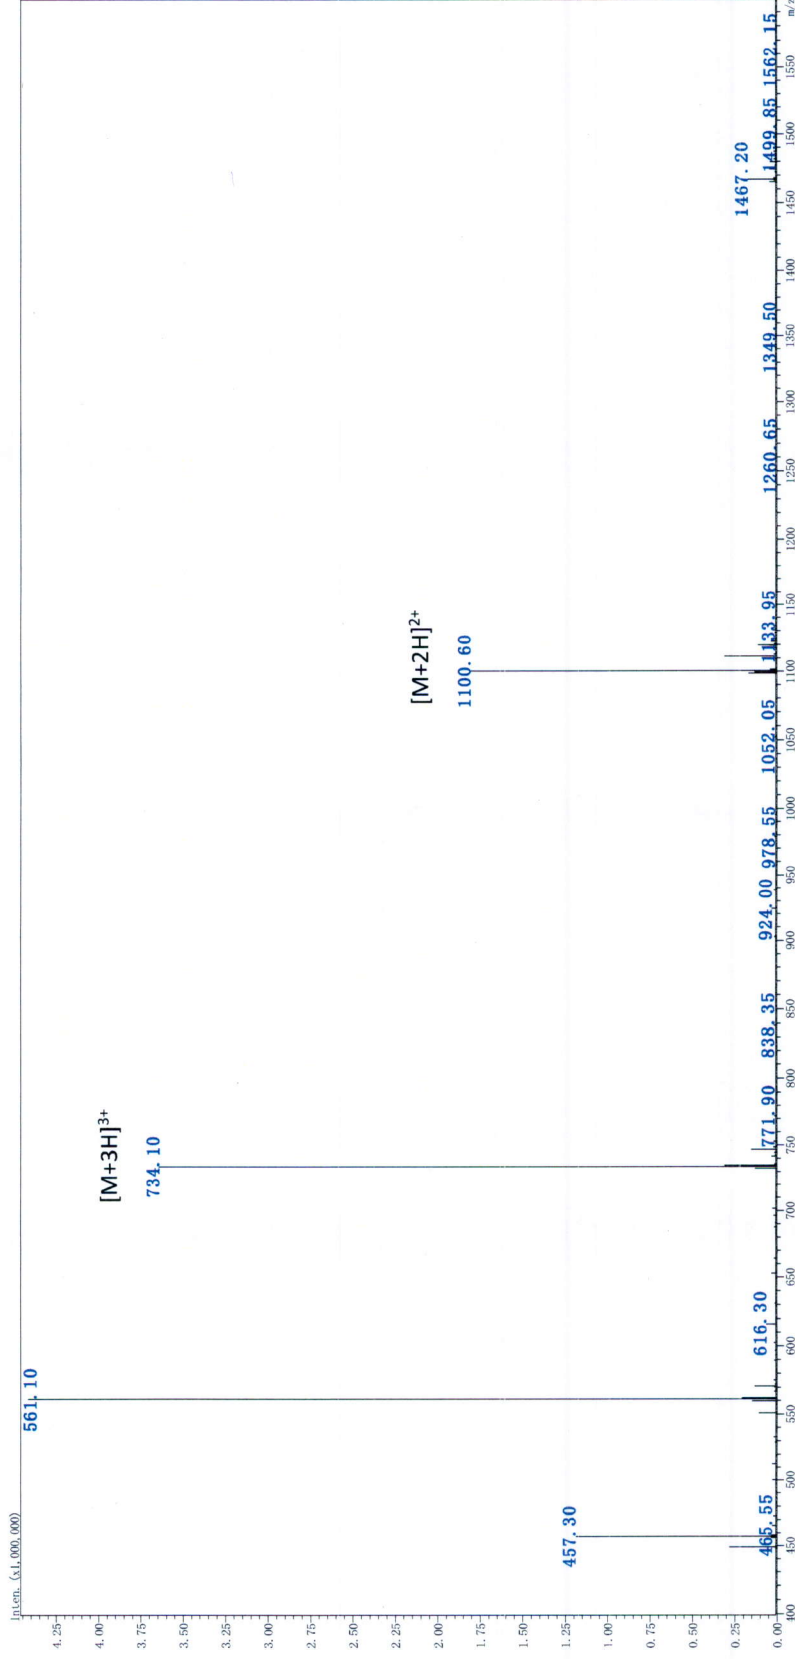

Sample Description

Analyzed date: 20240124,13:46

Analyst: WLL

Sample: KP3270-4:Peptide KP3270-4

M.W.: 2199.60

Lot. No.: 20240124

Instrument

Probe: ESI

Nebulizer Gas Flow: 1.5L/min

CDL: -20.0v

CDL Temp.: 250 °C

Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv

Detector: 1.5kv

T. Flow: 0.2ml/min

B. Conc.: 30%H₂O/30%ACN/40%MEOH

Certificate of Analysis

Product Information

Customer Code:Peptide KP3270-6

Lot No.:20240124

M. W.:2420.67

Sequence:IGIYSFSQTHFEHFLSHIQE

Store at:-20°C

KSVP Code:KP3270-6

Formula:

Quantity:3.0mg

Analytical Results

Tests	Specifications	Results
Appearance	white powder	Conforms
Purity(HPLC)	≥98%	99.36%
MS(ESI)	Calc.2420.67	Obs.2420.42

Prepared By:

Checked by:

Date:

HPLC Report

Sample Information

Customer Code:Peptide KP3270-6

KSVP Code:KP3270-6

Lot No.:20240124

Phase A: 0.1% TFA in deionized water

Phase B: 0.08% TFA in acetonitrile

Flow rate:1.0mL/min

Wavelength:214nm

Analytical column type:YMC-Pack ODS-A、120A、5um、4.6*250mm

Dissolution method:100%H2O


Inj. Volume:5uL

Date Acquired:20240124,13:42:10

Gradient:


Time (min)	Phase A	Phase B
0.01	85%	15%
2.00	85%	15%
22.00	1%	99%
30.00	Stop	

Chromatogram

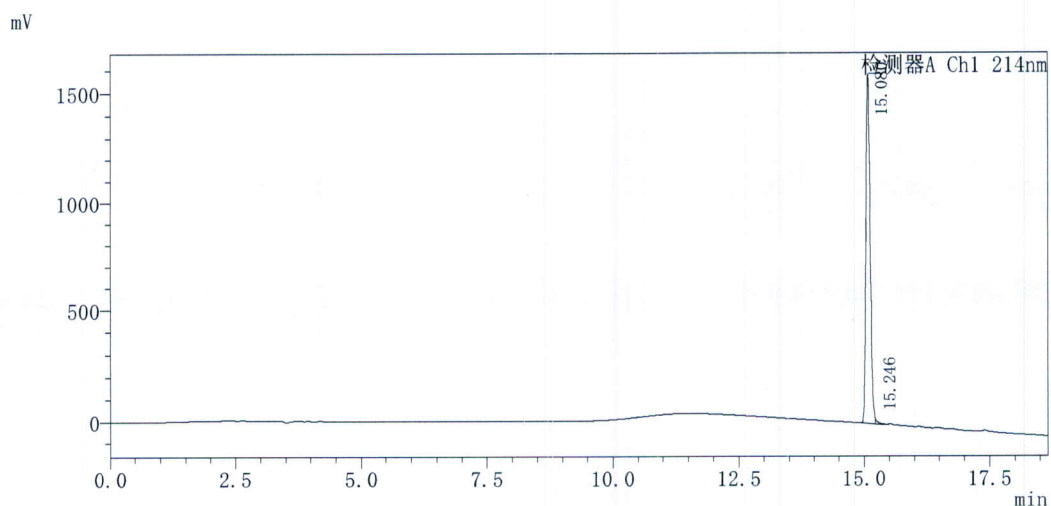

峰号	保留时间	峰面积	峰面积%	峰高	峰高%
1	15.08	9476418	99.367	1590715	99.148
2	15.246	60326	0.633	13675	0.852

Mass Spectrometry Report

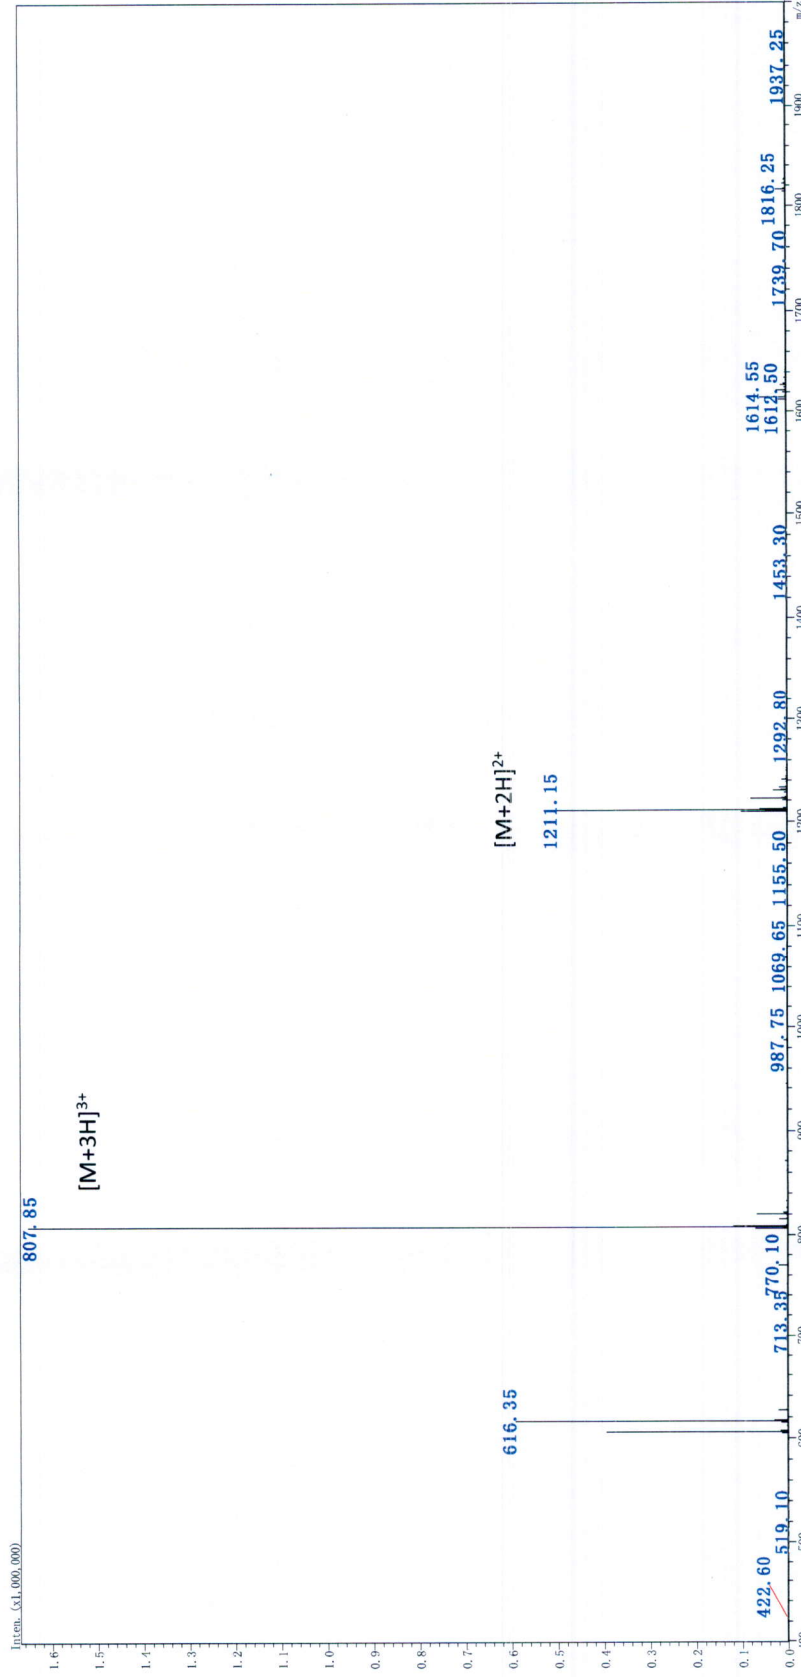

Sample Description

Analyzed date: 20240124,14:18

Analyst: WLL

Sample: KP3270-6:Peptide KP3270-6

M.W.: 2420.67

Lot. No.: 20240124

Instrument

Probe:

Nebulizer Gas Flow:

CDL:

CDL Temp.:

Block Temp.:

SHIMADZU LCMS-2020

ESI

1.5L/min

-20.0v

250 °C

200 °C

Probe Bias: +4.5kv

Detector: 1.5kv

T. Flow: 0.2ml/min

B. Conc.: 30%H₂O/30%ACN/40%MEOH

Certificate of Analysis

Product Information

Customer Code: Peptide KP3270-8
Lot No.: 20240124
M. W.: 2387.64
Sequence: QQAYEKILRQYEYAQRGTAA
Store at: -20°C

KSVP Code: KP3270-8
Formula:
Quantity: 3.0mg

Analytical Results

Tests	Specifications	Results
Appearance	white powder	Conforms
Purity(HPLC)	≥98%	98.11%
MS(ESI)	Calc.2387.64	Obs.2387.75

Prepared By:

Checked by:

Date:


HPLC Report

Sample Information

Customer Code: Peptide KP3270-8 KSVP Code: KP3270-8
 Lot No.: 20240124
 Phase A: 0.1% TFA in deionized water
 Phase B: 0.08% TFA in acetonitrile
 Flow rate: 1.0 mL/min
 Wavelength: 214 nm
 Analytical column type: Agilent 5 TC-C18、120A、5μm、4.6*250mm
 Dissolution method: 100% H₂O
 Inj. Volume: 10 μL
 Date Acquired: 20240124, 09:52:55
 Gradient:


Time (min)	Phase A	Phase B
0.01	85%	15%
2.00	85%	15%
22.00	1%	99%
30.00	Stop	

Chromatogram

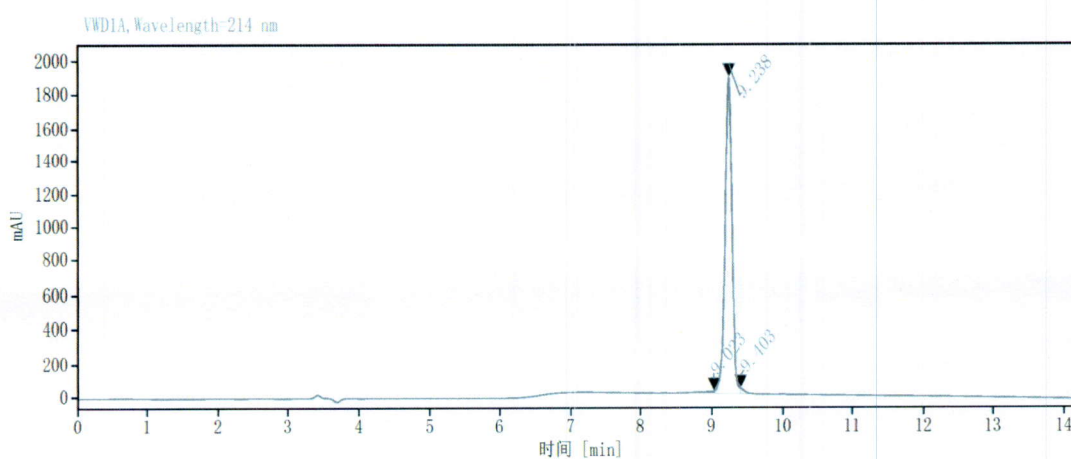

峰号	保留时间	峰面积	峰面积%	峰高	峰高%
1	9.023	116.1067	0.89	10.894	0.57
2	9.238	12845.0746	98.11	1882.458	97.80
3	9.403	130.7247	1.00	31.430	1.63

Mass Spectrometry Report

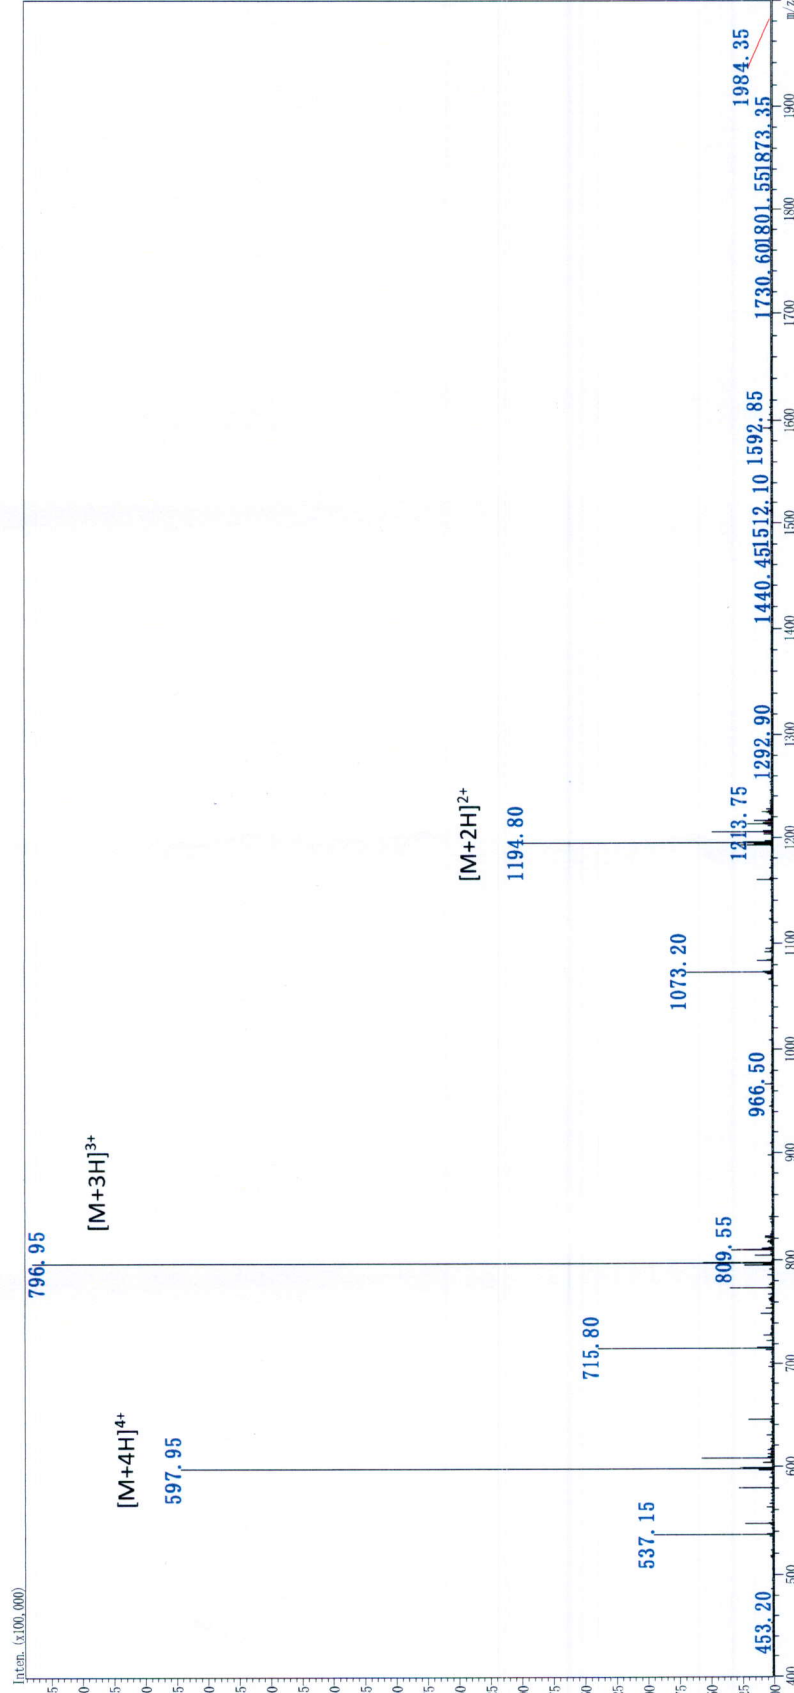

Sample Description

Analyzed date: 20240124,09:47

Analyst: WLL

Sample: KP3270-8:Peptide KP3270-8

M.W.: 2387.64

Lot. No.: 20240124

Instrument

Probe: ESI

Nebulizer Gas Flow: 1.5L/min

CDL: -20.0v

CDL Temp.: 250 °C

Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv

Detector: 1.5kv

T. Flow: 0.2ml/min

B. Conc.: 30%H₂O/30%ACN/40%MEOH

Certificate of Analysis

Product Information

Customer Code:Peptide KP3270-10
Lot No.:20240123
M. W.:2495.82
Sequence:SRWQQLQRYLRYLQRSEGG
Store at:-20°C

KSVP Code:KP3270-10
Formula:
Quantity:3.0mg

Analytical Results

Tests	Specifications	Results
Appearance	white powder	Conforms
Purity(HPLC)	≥98%	99.46%
MS(ESI)	Calc.2495.82	Obs.2495.27

Prepared By:

Checked by:

Date:


HPLC Report

Sample Information

Customer Code: Peptide KP3270-10 KSVP Code: KP3270-10
 Lot No.: 20240123
 Phase A: 0.1% TFA in deionized water
 Phase B: 0.08% TFA in acetonitrile
 Flow rate: 1.0 mL/min
 Wavelength: 214 nm
 Analytical column type: Agilent 5 TC-C18、120A、5 μm、4.6*250 mm
 Dissolution method: 100% H₂O
 Inj. Volume: 10 μL
 Date Acquired: 20240123, 16:53:23
 Gradient:


Time (min)	Phase A	Phase B
0.01	90%	10%
2.00	90%	10%
22.00	1%	99%
30.00	Stop	

Chromatogram

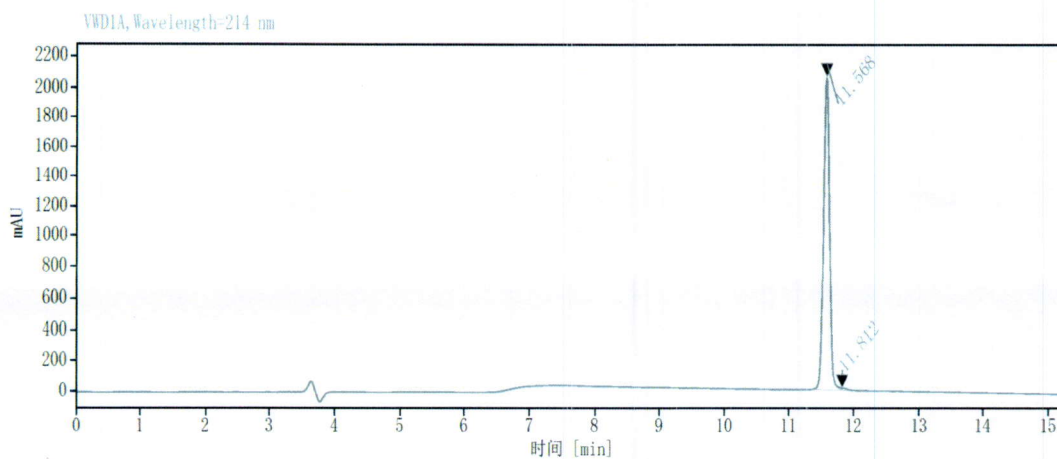

峰号	保留时间	峰面积	峰面积%	峰高	峰高%
1	11.568	13277.2081	99.46	2056.100	99.37
2	11.812	71.9785	0.54	13.114	0.63

Mass Spectrometry Report

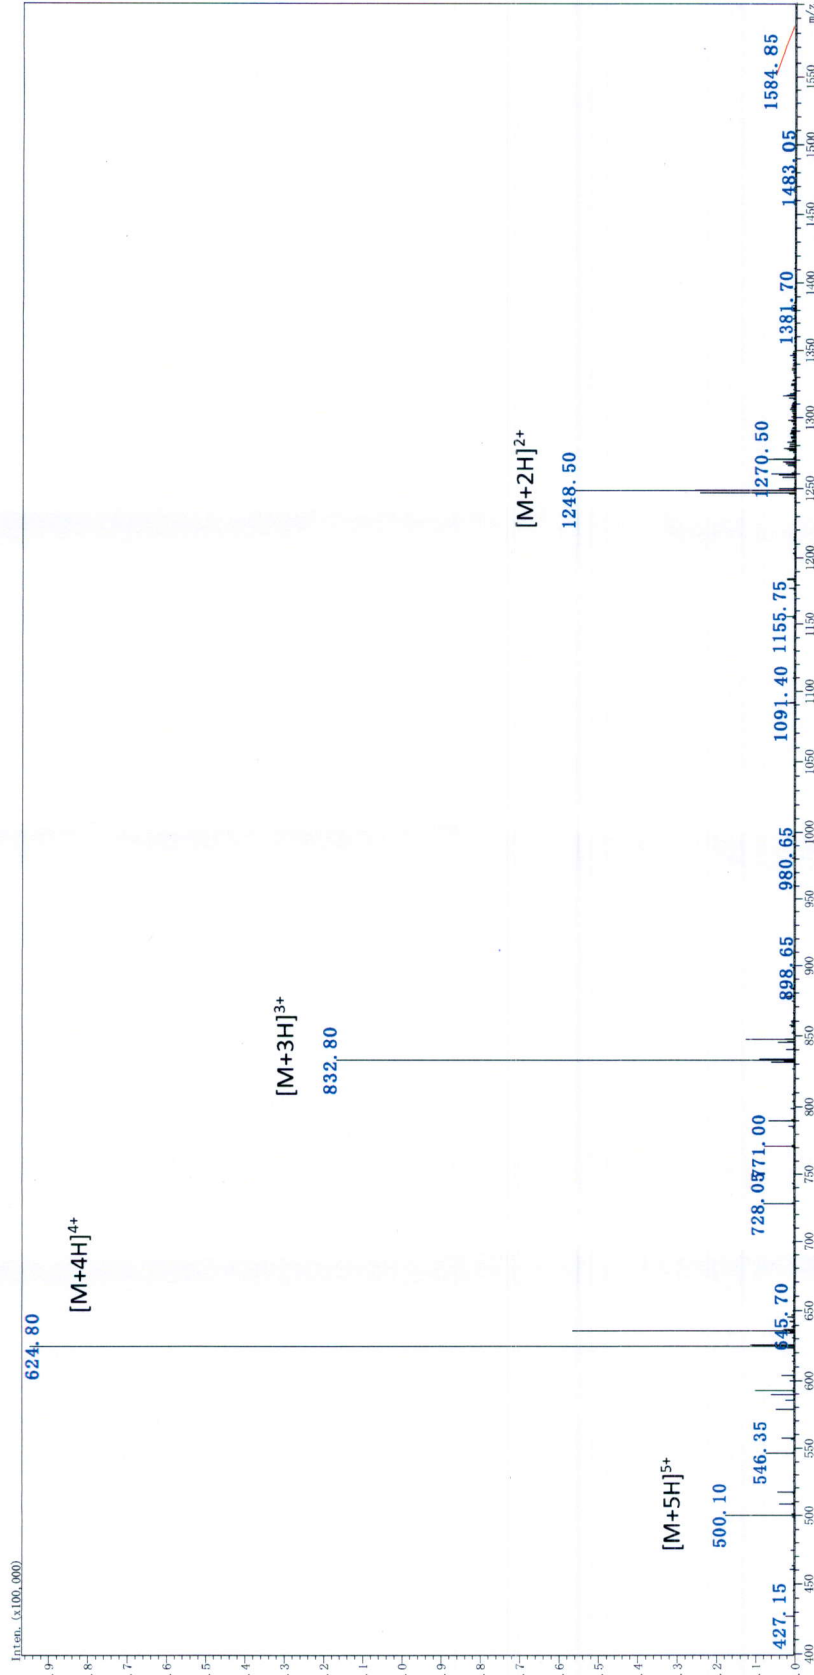

Sample Description

Analyzed date: 20240123,15:37

Analyst: WLL

Sample: KP3270-10:Peptide KP3270-10

M.W.: 2495.82

Lot. No.: 20240123

Instrument

Probe: ESI

Nebulizer Gas Flow: 1.5L/min

CDL: -20.0v

CDL Temp.: 250 °C

Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv

Detector: 1.5kv

T. Flow: 0.2ml/min

B. Conc.: 30%H₂O/30%ACN/40%MEOH