

Ayati Devices


Report no :
Patient ID :

Name :


Report no :
Age :

Perfusion Study

BRIEF EXAMINATION NOTES:

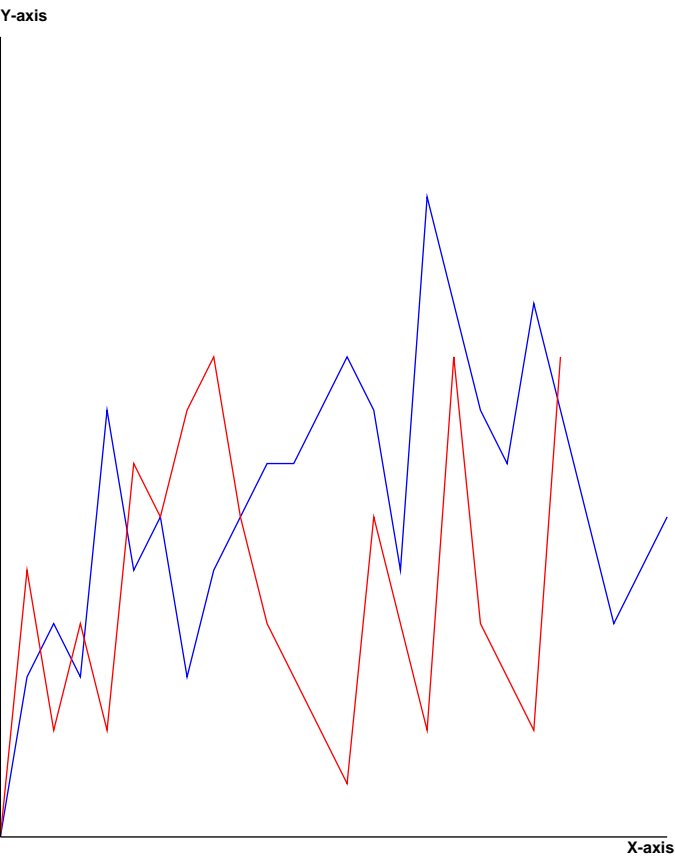

PERFUSION IMAGE

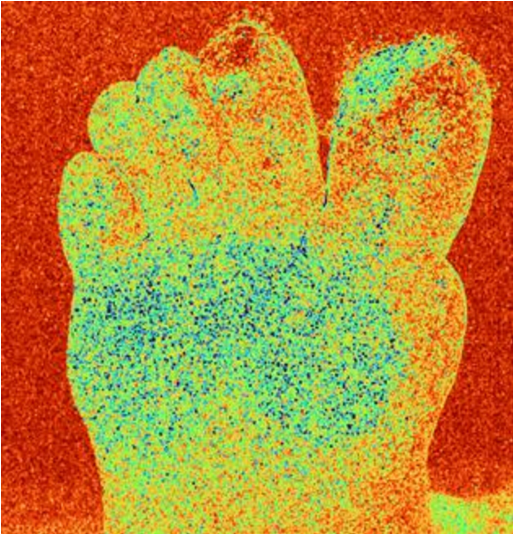

NORMAL IMAGE



Rol No	Mean	Std dev	%	Median	Min	Max
1	35	10	Ref	117	110	130
2	28	11	75%	117	110	130

Ayati Devices


Report no :
Patient ID :

Name :


Report no :
Age :

PORH Study

BRIEF EXAMINATION NOTES:

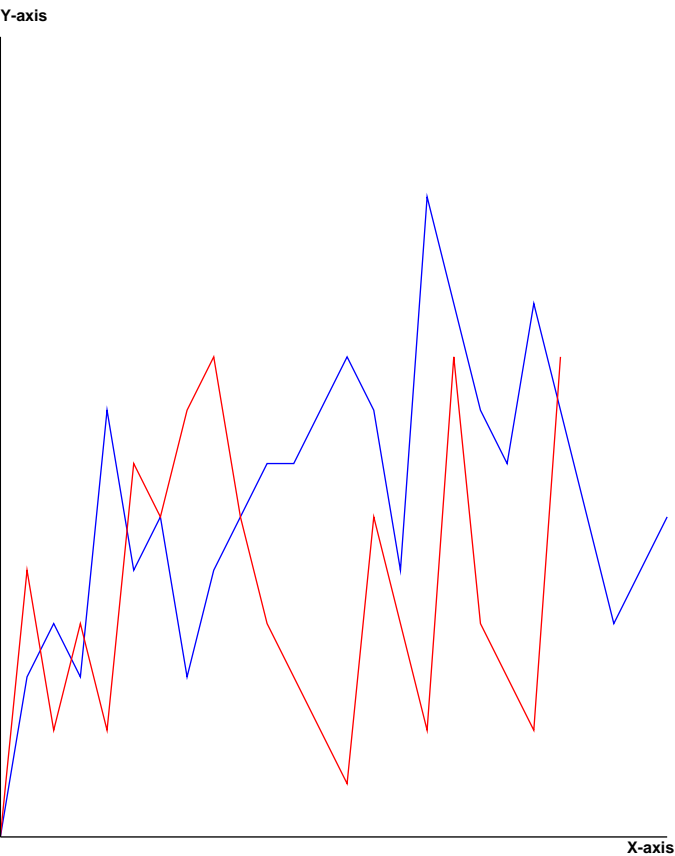

PERFUSION IMAGE

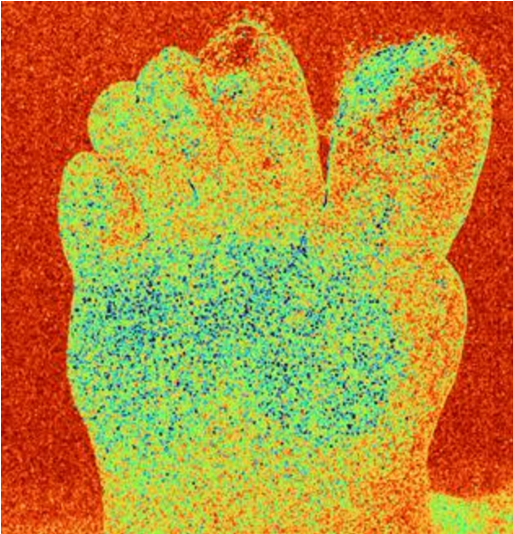

NORMAL IMAGE



Rol No	Mean	Std dev	%	Median	Min	Max
1	35	10	Ref	117	110	130
2	28	11	75%	117	110	130