

North Coast Occupational Health

DR DG GOVENDER

PR NO: 1476971; MP NO: 0219177

MbChB (Natal); Mmed Sci (Sports Medicine) (Natal); DOH (Dip Occupational Health) (Natal)
Senior AME (CAA)(Pretoria); Certificate in Travel Medicine(Wits); Basic Underwater Medicine(Stellenbosch)

MEDICAL REPORT

NAME	SONWABO CELU	
ID NUMBER	8212095949080	
COMPANY	LANDSCAPERS INC	
JOB DESCRIPTION	LANDSCAPER	

Medical History	HT	DM	Asthma	Arthritis	PU	Allergies	TB	Epilepsy
-----------------	----	----	--------	-----------	----	-----------	----	----------

Medication:

nlu

Occ. Injuries / Diseases

nlu

Occupational Exposures	(Noise)	(Dust)	Radiation
	Asbestos	(Heights)	(Heat / Cold)

Social Habits	Alcohol : <u>Yes</u> / No	Smoker : Yes / <u>No</u>
---------------	---------------------------	--------------------------

General Examination:

Healthy

Height	Weight	BMI	BP	Pulse	Urine
1.68	67		134 / 90	87	-

Vision: Right: 20 / 20 Left: 20 / 20 with / without Glasses Colour Vision: Normal

Special Investigations:

Spirometry:

FVC	FEV 1	FEV1 / FVC
3.18	2.82	88

Audiogram: PLH: 1.80 % CXR: - Resting/ Stress ECG: -

Drugs of Abuse screen: -

Working at heights evaluation: YES / NO

Blood Tests: YES / NO

31 ZENITH DRIVE
UMHLANGA RIDGE
031: 566 2066

CELL: 083661 4332

16 RAILWAY STREET
TONGAAT
032: 944 7617

North Coast Occupational Health
DR DG GOVENDER
PR NO: 1476971; MP NO: 0219177
MbChB (Natal); Mmed Sci (Sports Medicine) (Natal); DOH (Dip Occupational Health) (Natal)
Senior AME (CAA)(Pretoria);Certificate in Travel Medicine(Wits);Basic Underwater Medicine(Stellenbosch)

CERTIFICATE OF FITNESS

I, DR DG GOVENDER (OMP), hereby confirm that in accordance to the contractor job specification presented to me,

NAME	SONWABO CELU
ID NUMBER	8212095949080
COMPANY	LANDSCAPERS INC
JOB DESCRIPTION	LANDSCAPER


The above mentioned has been examined according to the protocols as follows:

General medical examination	/	Audiogram	/
Chest x-ray		Lung function test	/
Keystone Vision testing		Snellen's eye test	/
Drugs of abuse screen		Working at Heights evaluation	/
Cannabis urine screen		Stress ECG	
Blood tests		Resting ECG	

And their fitness to carry out tasks required by the job follows

Fit with no restrictions	/
Fit with the following restrictions:	
Temporary Unfit Until (Date)	
Permanently Unfit	

This "certificate of fitness" expires on 16/07/2027 being one year from date of examination.

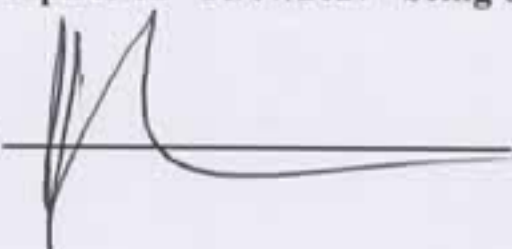(OMP) DR DG GOVENDER: 

DATE: 16/07/2026

STAMP

DR DG GOVENDER

NORTH COAST OCCUPATIONAL HEALTH

PR NO 1476971 SAS 0454

Tel: 031 566 2066 Cell: 083 661 4332

The Zen, 31 Zenith Drive, Umhlanga Riv

31 ZENITH DRIVE UMHLANGA RIDGE 031: 566 2066	CELL: 083661 4332	16 RAILWAY STREET TONGAAT 032: 944 7617
--	-------------------	---

North Coast Occupational Health
DR DG GOVENDER
PR NO: 1476971; MP NO: 0219177
MbChB (Natal); Mmed Sci (Sports Medicine) (Natal); DOH (Dip Occupational Health) (Natal)
Senior AME (CAA)(Pretoria);Certificate in Travel Medicine(Wits);Basic Underwater Medicine(Stellenbosch)

WORKING AT HEIGHTS EVALUATION

NAME	SONWABO CELU
ID NUMBER	8212095949080
COMPANY	LANDSCAPERS INC
JOB DESCRIPTION	LANDSCAPER

STATUS	YES	NO
Have you ever had a blackout?		✓
Have you ever had an epileptic fit?		✓
Are you afraid of heights?		✓
Is there any reason that you should not be working at heights?		✓
Are you on any medication at the moment?		✓

If yes please elaborate

Office use only

Is this person fit to work at heights? (YES) NO

If no, what are the reasons?

DR DG GOVENDER
NORTH COAST OCCUPATIONAL HEALTH
PR NO 1476971 SAS 0454
Tel: 031 566 2066 Cell: 083 661 4332
The Zen, 31 Zenith Drive, Umhlanga Rock

DATE: 16/07/2026

31 ZENITH DRIVE UMHLANGA RIDGE 031: 566 2066	CELL: 083661 4332	16 RAILWAY STREET TONGAAT 032: 944 7617
--	-------------------	---

North Coast Occupational Health

DR DG GOVENDER

PR NO: 1476971; MP NO: 0219177

MbChB (Natal); Mmed Sci (Sports Medicine) (Natal); DOH (Dip Occupational Health) (Natal)

Senior AME (CAAP/Pretoria); Certificate in Travel Medicine (Wits); Basic Underwater Medicine (Stellenbosch)

ANNEXURE 3

OCCUPATIONAL HEALTH AND SAFETY ACT

COMPANY : LANDSCAPERS INC

NAME OF EMPLOYEE: SONWABO CELU

ID NUMBER : 8212095949080

Possible exposures										Job Specific Requirements							Protective Equipment							
	*	*			*												*	*	*	*	*	*	*	
	Heat	Noise	Working At Heights	Confined Space	Dust	Hazardous Chemicals	Fumes	Excavations	Scaffolding	General Labour	Bricklayer	Scaffolding	Painting	Plumbing	LANDSCAPER	X	Ear Plugs	Hard Hat	Reflective Vest	Glasses	Overalls	Gloves	Dust Masks	

Declaration by the Medical Health Examiner :

I certify that I have, by examination and testing, using the above criteria specified by the employer, satisfied myself that the abovementioned employee is fit to perform the duties as described by the employer in the matrix above.

OCCUPATIONAL HEALTH PRACTITIONER:

Date: 16/07/2026

Signature: DR DG GOVENDER

Employee signature: _____

Employer Signature : _____

DR DG GOVENDER
NORTH COAST OCCUPATIONAL HEALTH
PR NO 1476971 MP NO 0219177
Tel: 031 566 2066 Cell: 083 661 4332
The Zen, 31 Zenith Drive, Umhlanga Rock

Pat-Name: **Celu Sonwabo**
Pat-No: **8212095949080**

Case No.:

Born: 09.12.1982
Age: 43 Y
Sex: Male
Height: 168.0 cm
Weight: 67.0 kg
Ethnic: Non-Caucasian

Indic:
Med:
Rem:



FVC
FEV 1.0
FEV 1.0/FVC
FEF 25-75%
PEF

ECCS / Quanjer	Pred	PRE Best	%Pred	Meas1	Meas2	Meas3
[l]	3.79	3.18	84	3.18	2.69	2.46
[l]	3.14	2.82	90	2.82	2.66	2.45
[%]	72	88	124	88	99	100
[l/s]	3.70	3.87	105	3.87	5.32	5.08
[l/s]	7.77	8.29	107	8.29	8.68	9.26

Smoking History
- gr/day / - yrs

Interpretation
Normal Condition

Validated by

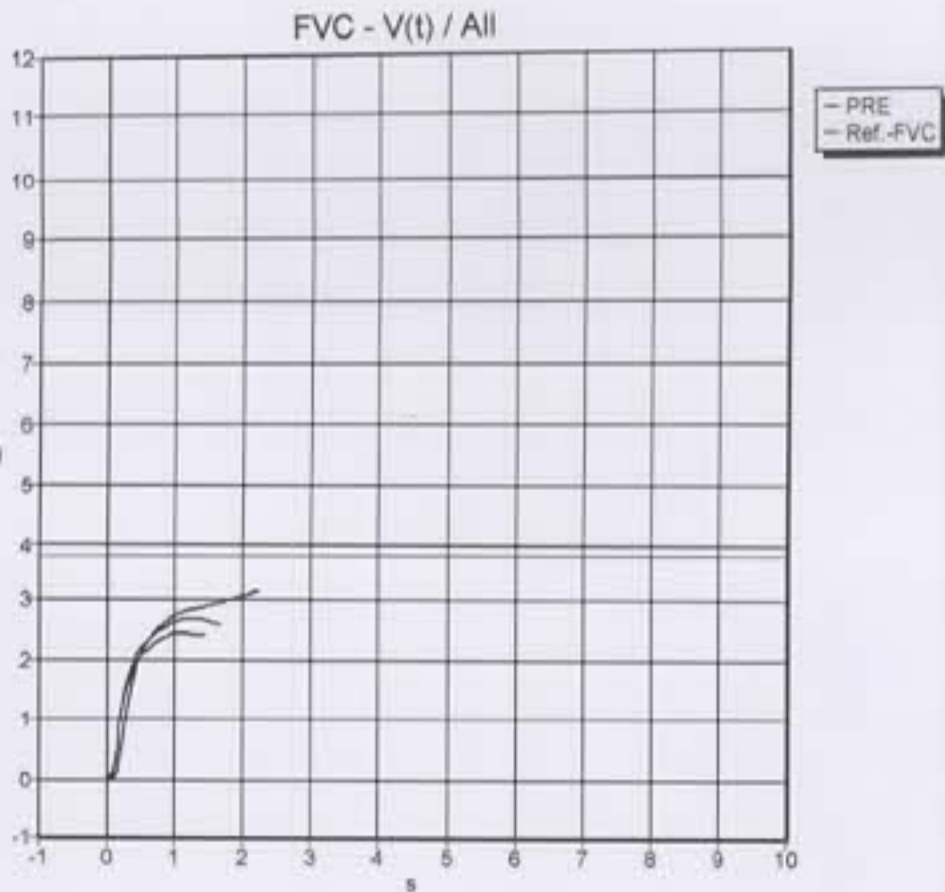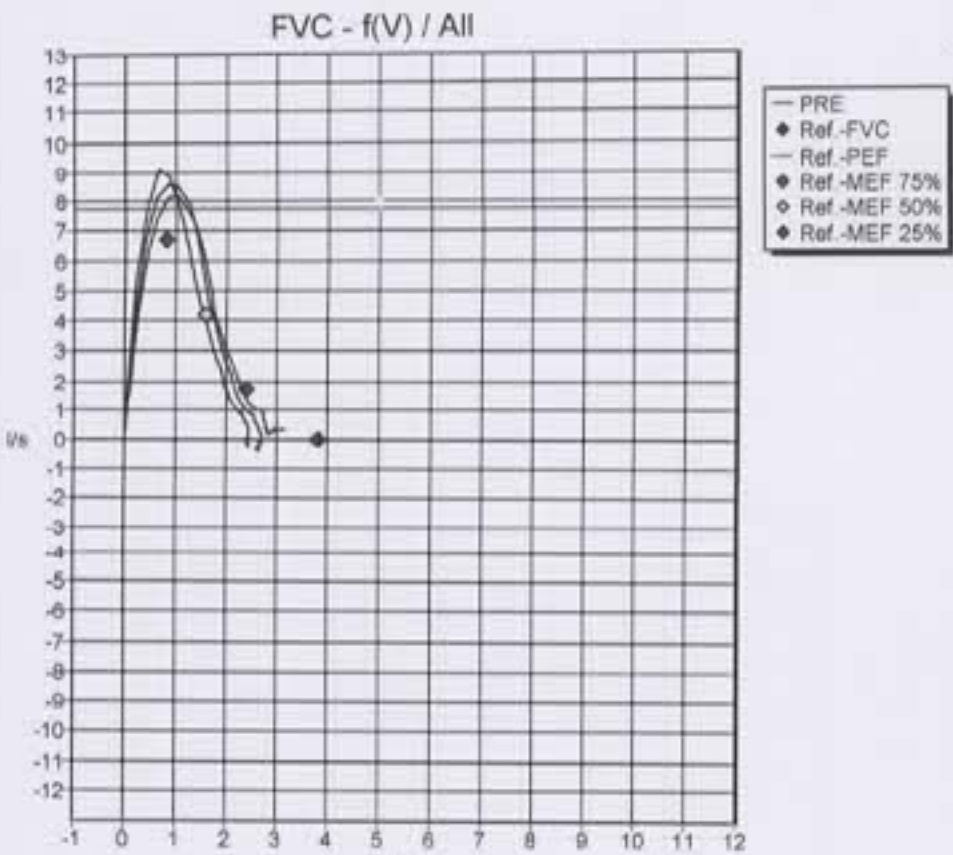

Patient

Celu Sonwabo
16.07.2026 13:44:26

Technician


Clinic

Patient Number: 8212095949080
Patient Name: CELU, SONWABO
Gender / ID No.: Male / 8212095949080


Date of Birth: 1982-12-09
Employment Date:
Noise Exposure:

Company:
Department:
Position:

LEFT

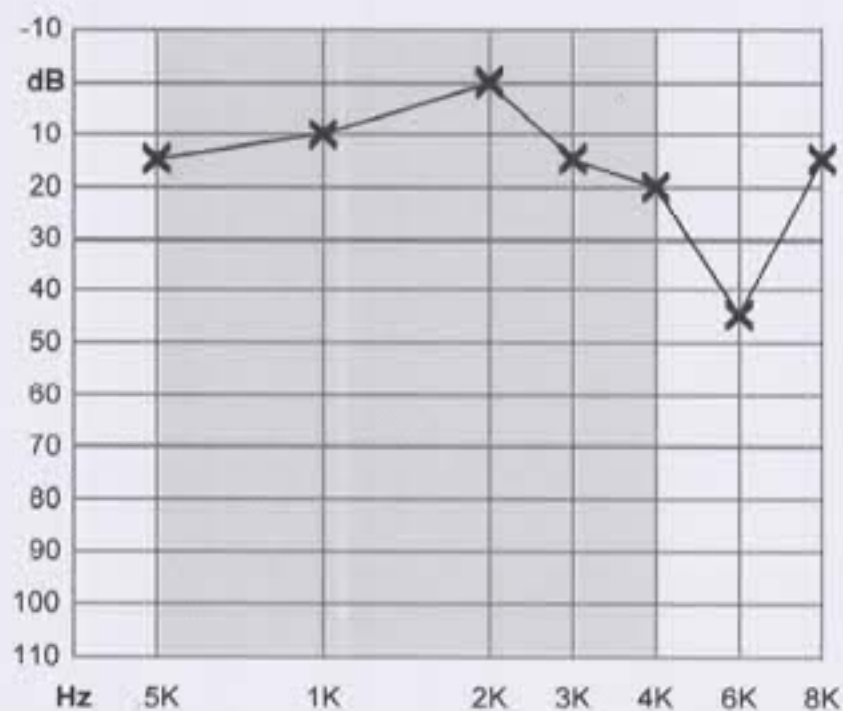

RIGHT

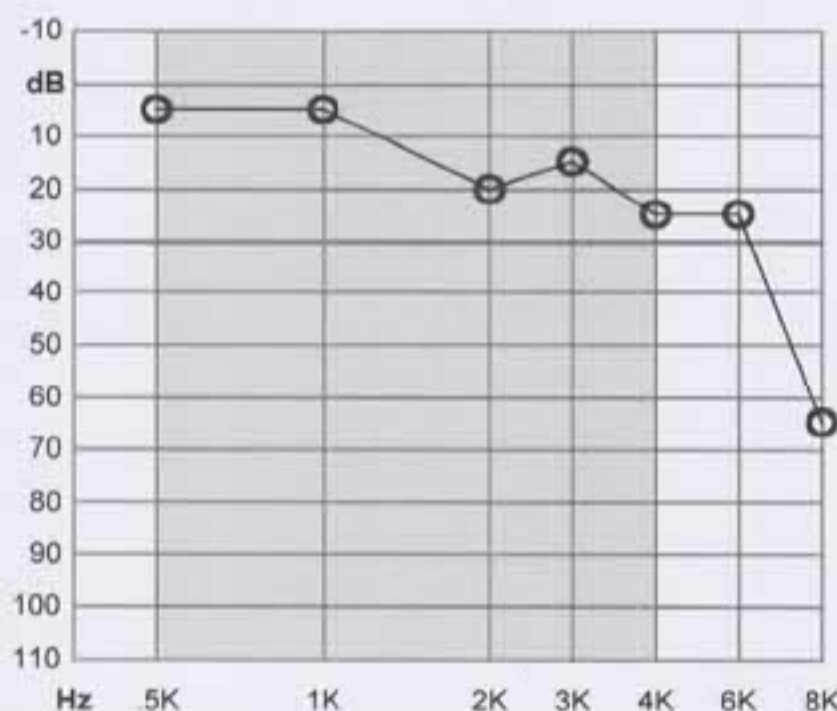

Identifier	Test Date	Type	Baseline	Serial No.	Operator	PLH	PLHD	PLHS / PD (c)	PLHS / PD (b)
Blue	O 2026-07-16 13:59	Screening	-	062544 (2544)	clinic user	1.50	-	-	-

Identifier	Test Date	L 500	L 1K	L 2K	L 3K	L 4K	L 6K	L 8K	R 500	R 1K	R 2K	R 3K	R 4K	R 6K	R 8K
Blue	O 2026-07-16 13:59	15	10	0	15	20	45	15	5	5	20	15	25	25	65

Identifier	Test Date	Age	Noise	Lo Cat	Hi Cat	CAT	PBI	RTS	DSHL ... (L/R)	ABHL	5DSHL ... (L/R)	5ABHL
Blue	O 2026-07-16 13:59	43	-	1	2	2	0.00	0	40 45	10.62	60	70 13.00

Acknowledgement >>

Operator:

Date:

Patient:

Date:

Audiometer	Tremetrics RA300
Serial No.	062544 (2544)
Last Calibration	2026-03-31
Next Calibration	2027-03-31
Calibrated By	Musa Nzama