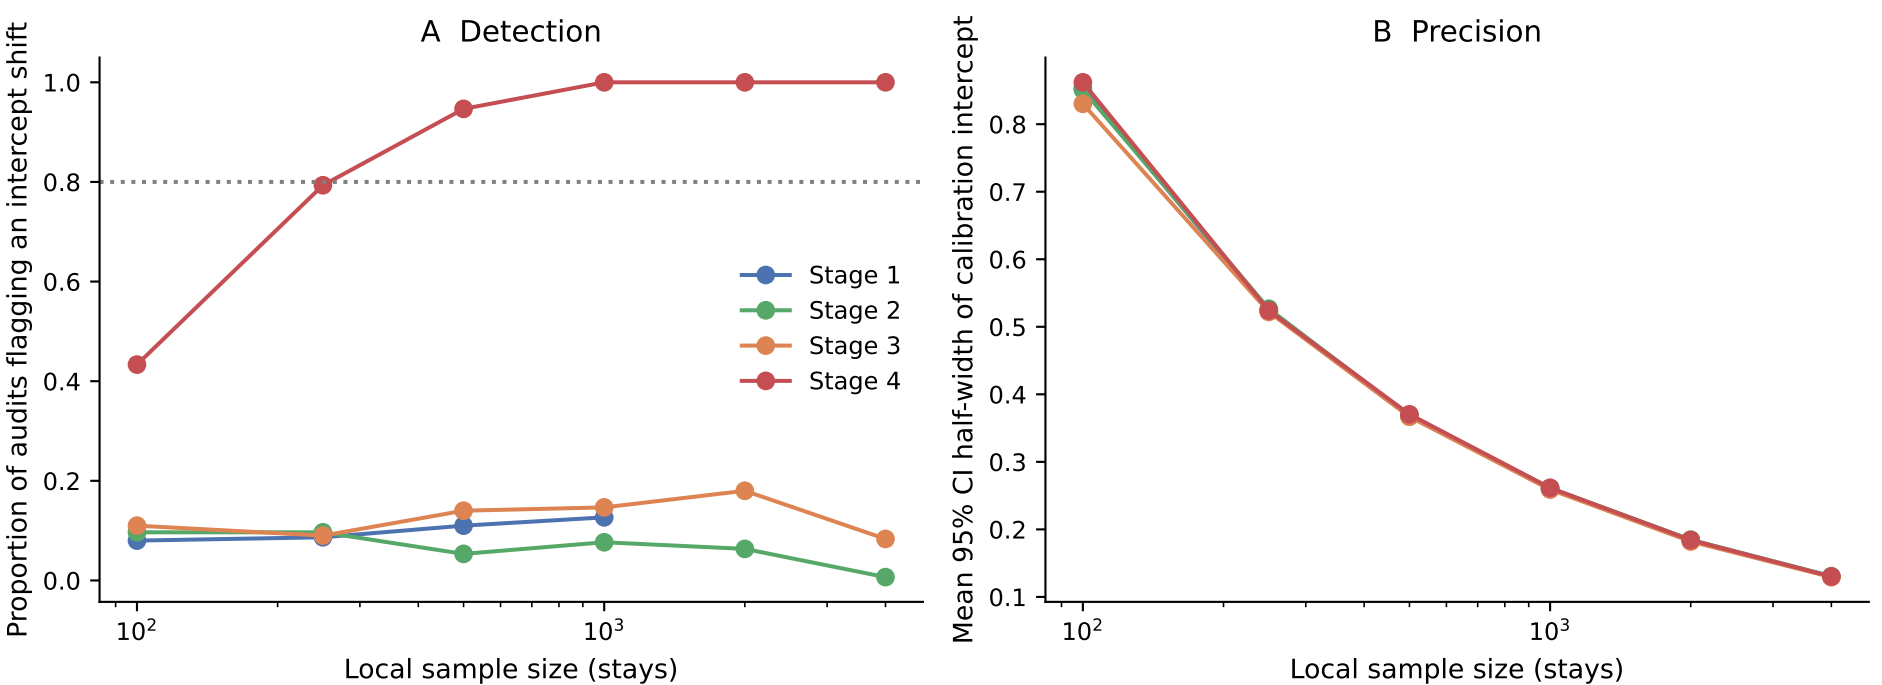
A Detection
Proportion of audits flagging an intercept shift
1.0
0.8
0.6
0.4
0.2
0.0
Stage 1
Stage 2
Stage 3
Stage 4
10^2
10^3
Local sample size (stays)
B Precision
Mean 95% CI half-width of calibration intercept
0.8
0.7
0.6
0.5
0.4
0.3
0.2
0.1
10^2
10^3
Local sample size (stays)