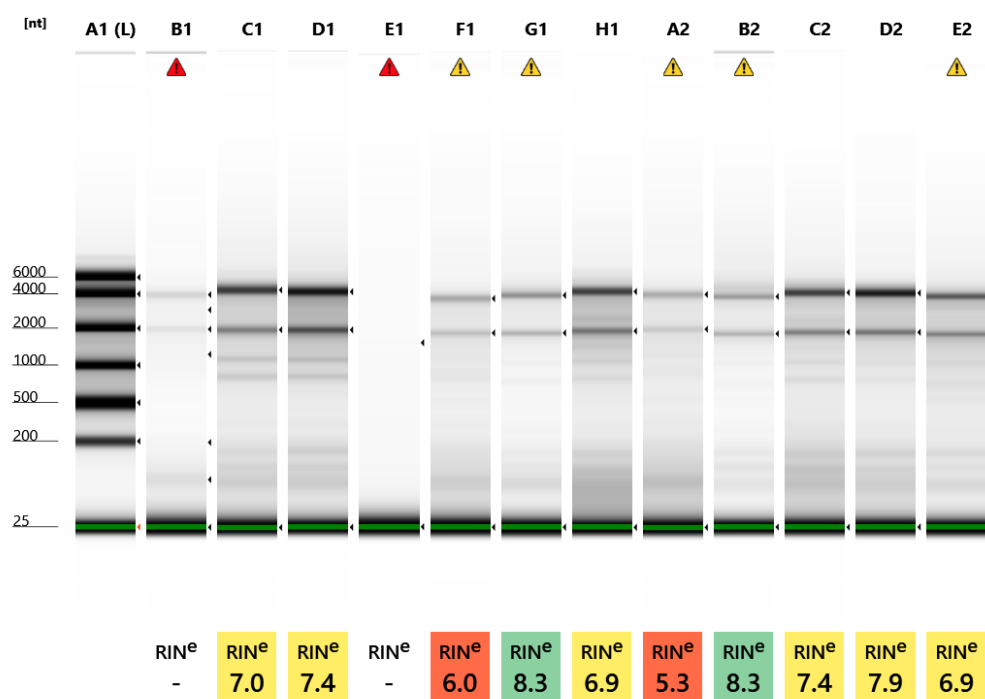


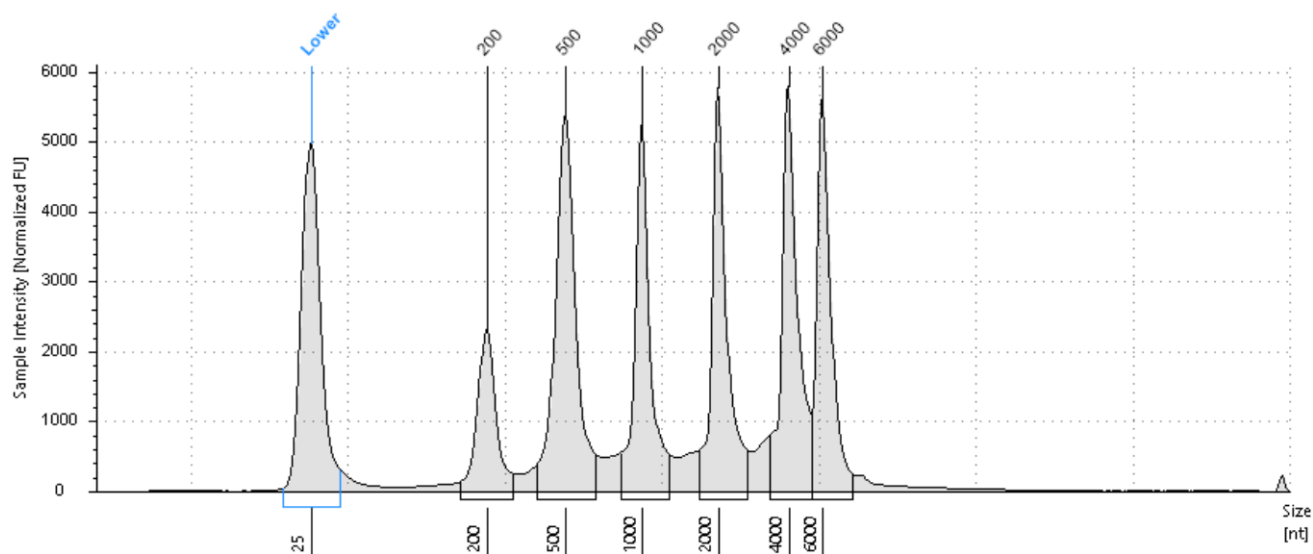
Filename: 2021-09-21 - 14.20.16.RNA



Default image (Contrast 100%)

Sample Info

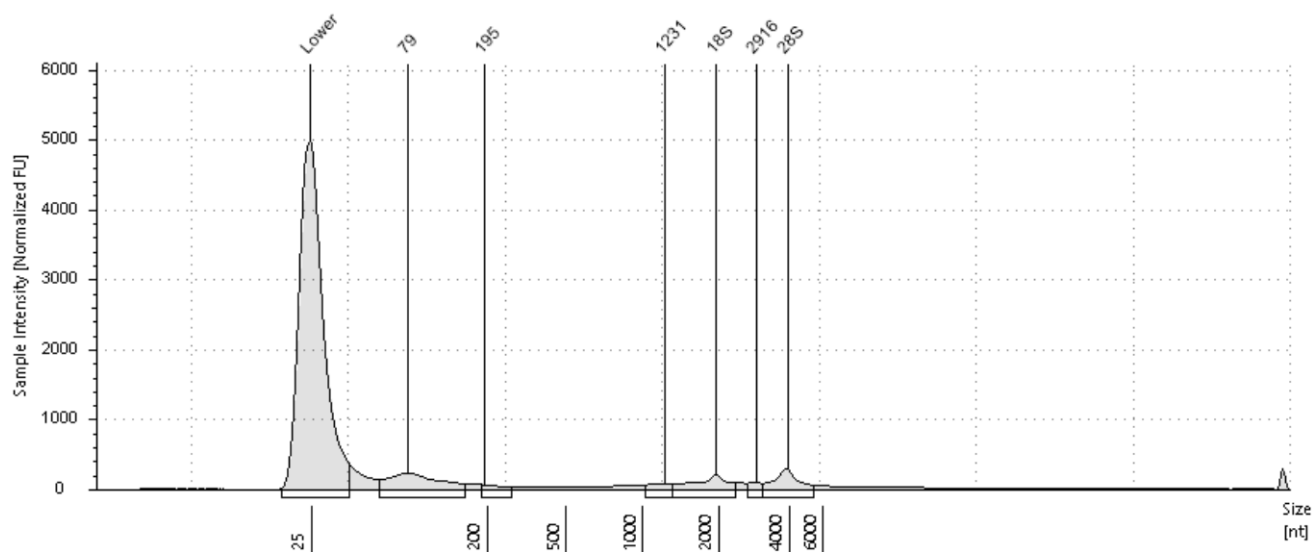
Well	RIN ^e	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	-	-	129	Ladder		Ladder
B1	-	-	8.51	231	▲	Sample concentration outside functional range for RIN ^e and the assay
C1	7.0	1.7	30.6	237		
D1	7.4	1.4	42.2	247		
E1	-	-	4.07	455	▲	Sample concentration outside functional range for RIN ^e and the assay
F1	6.0	1.5	16.6	467	▲	Sample concentration outside functional range for RIN ^e and the assay
G1	8.3	1.6	13.7	475	▲	Sample concentration outside functional range for RIN ^e and the assay
H1	6.9	1.6	35.6	651		
A2	5.3	1.6	19.4	673	▲	Sample concentration outside functional range for RIN ^e and the assay
B2	8.3	1.2	16.1	677	▲	Sample concentration outside functional range for RIN ^e and the assay
C2	7.4	1.9	29.8	789		
D2	7.9	1.9	29.5	805		
E2	6.9	1.0	24.3	807	▲	Sample concentration outside functional range for RIN ^e and the assay

A1: Ladder**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	-	-	129	Ladder		Ladder

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
200	10.0	-	148	8.77		
500	26.0	-	153	22.66		
1000	18.6	-	54.6	16.21		
2000	19.8	-	29.2	17.31		
4000	21.6	-	15.9	18.82		
6000	18.6	-	9.12	16.23		

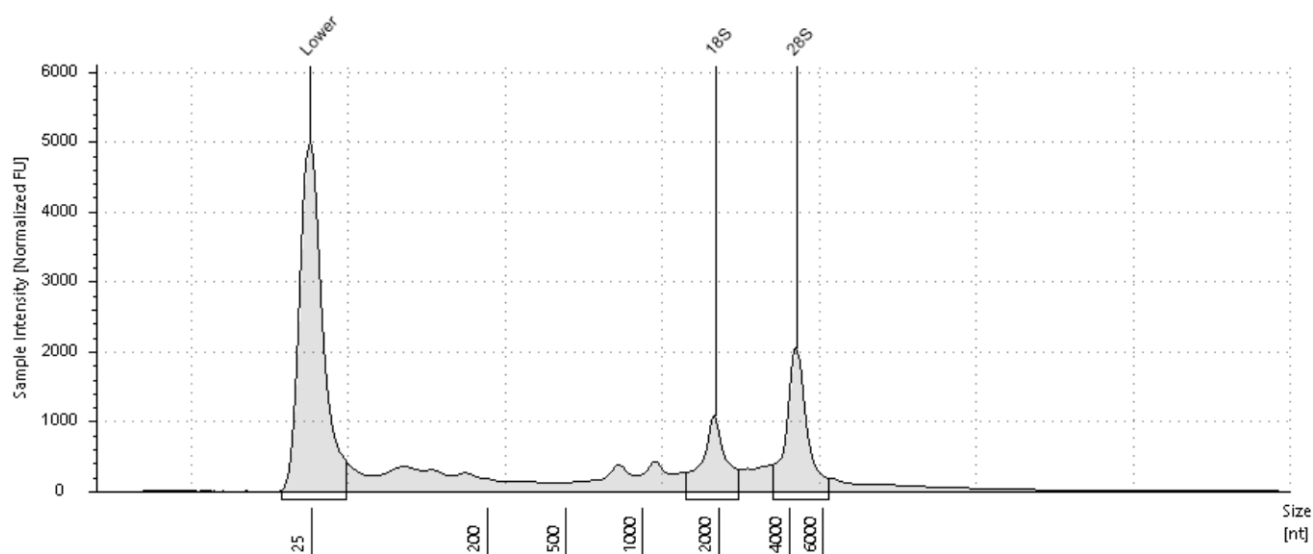
B1: 231**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
B1	-	-	8.51	231	▲	Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
79	2.13	-	79.0	40.45		
195	0.231	-	3.48	4.39		
1231	0.318	-	0.759	6.02		
1974	1.14	-	1.70	21.65		18S
2916	0.229	-	0.231	4.34		
3963	1.22	-	0.906	23.15		28S

C1: 237

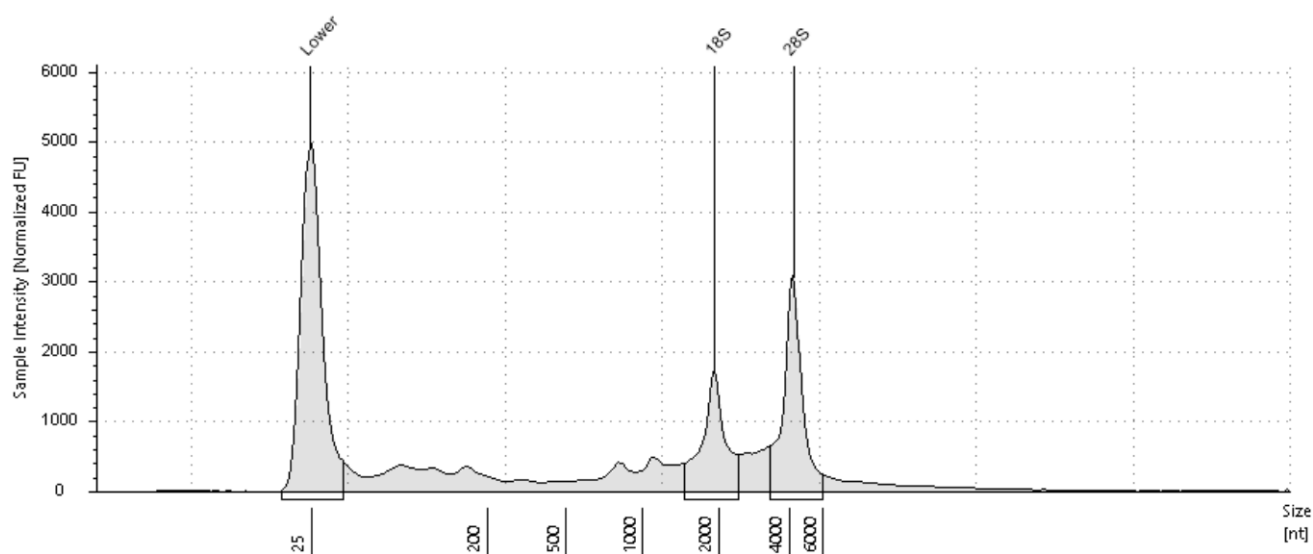


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
C1	7.0	1.7	30.6	237		

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1959	4.79	-	7.20	37.42		18S
4442	8.02	-	5.31	62.58		28S

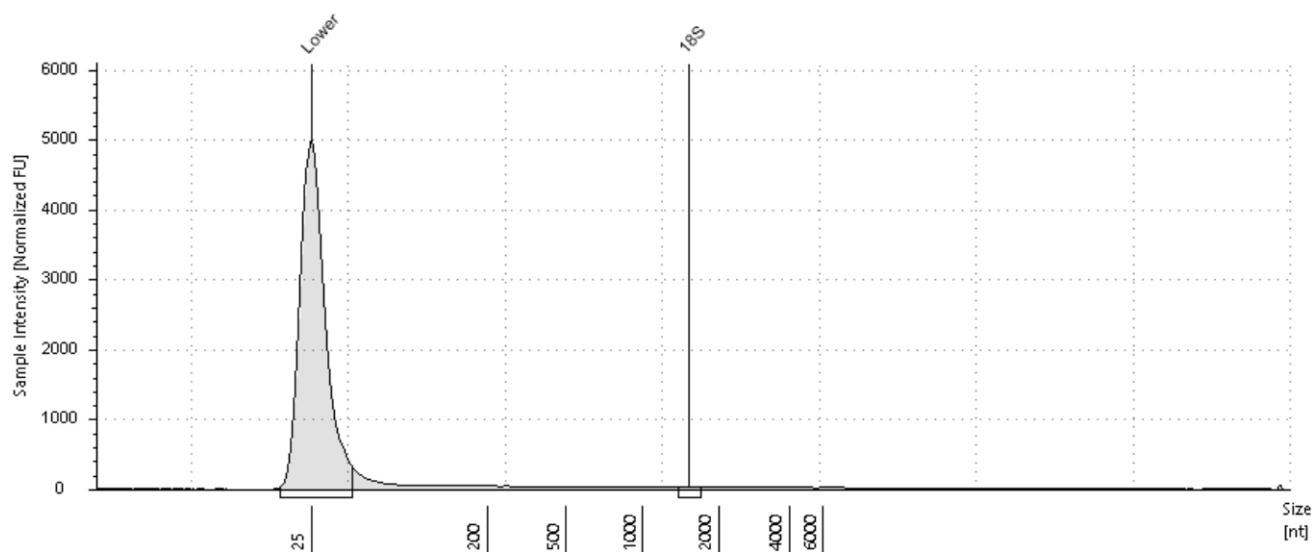
D1: 247**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
D1	7.4	1.4	42.2	247		

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1949	8.24	-	12.4	41.17		18S
4253	11.8	-	8.14	58.83		28S

E1: 455

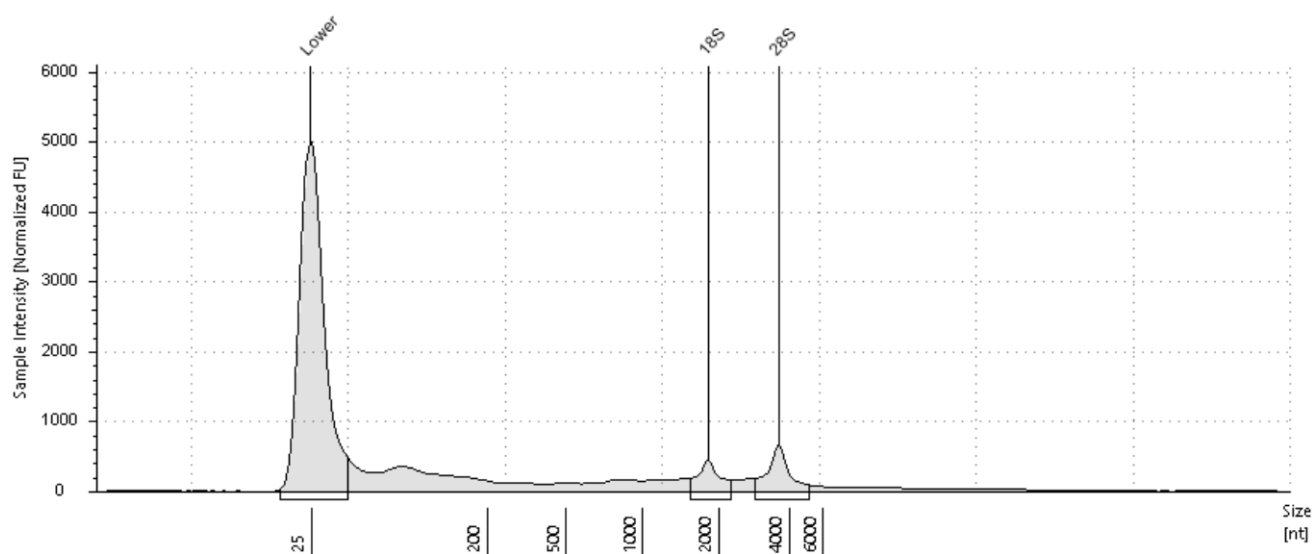


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
E1	-	-	4.07	455	▲	Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1519	0.119	-	0.231	100.00		18S

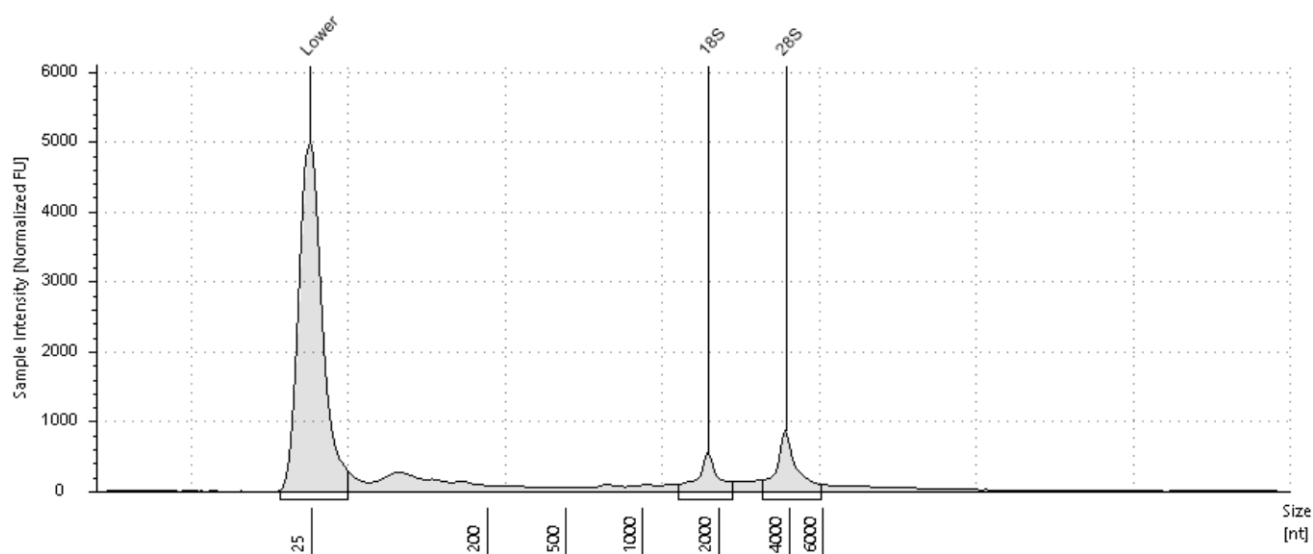
F1: 467**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
F1	6.0	1.5	16.6	467	⚠	Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1836	1.72	-	2.75	40.70		18S
3656	2.51	-	2.02	59.30		28S

G1: 475

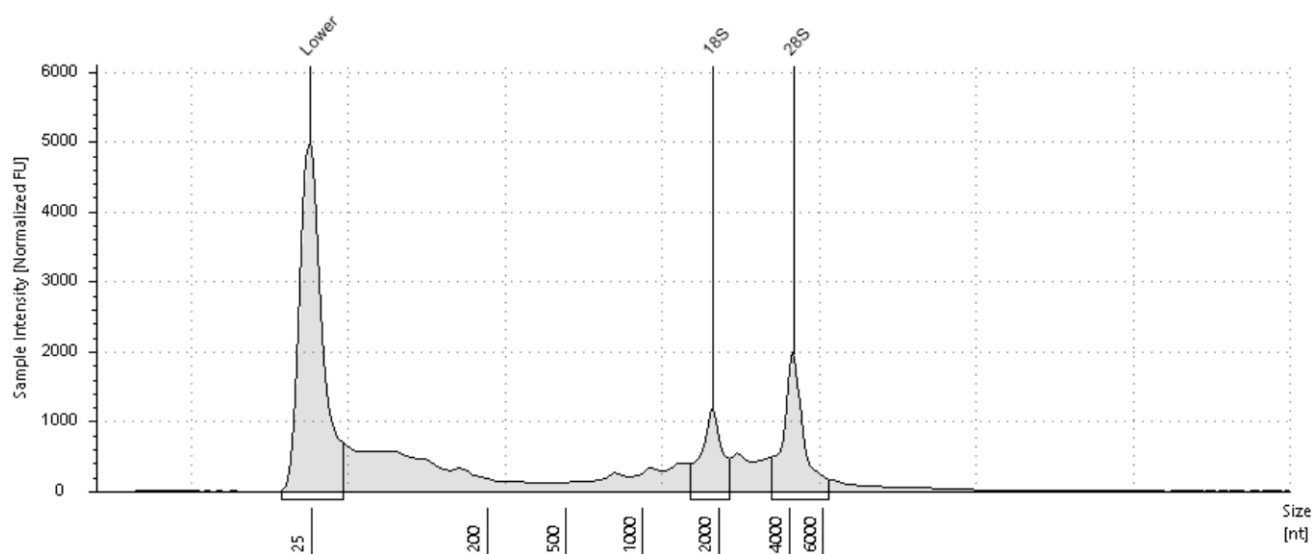


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
G1	8.3	1.6	13.7	475	⚠	Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1836	2.07	-	3.32	39.05		18S
3902	3.23	-	2.44	60.95		28S

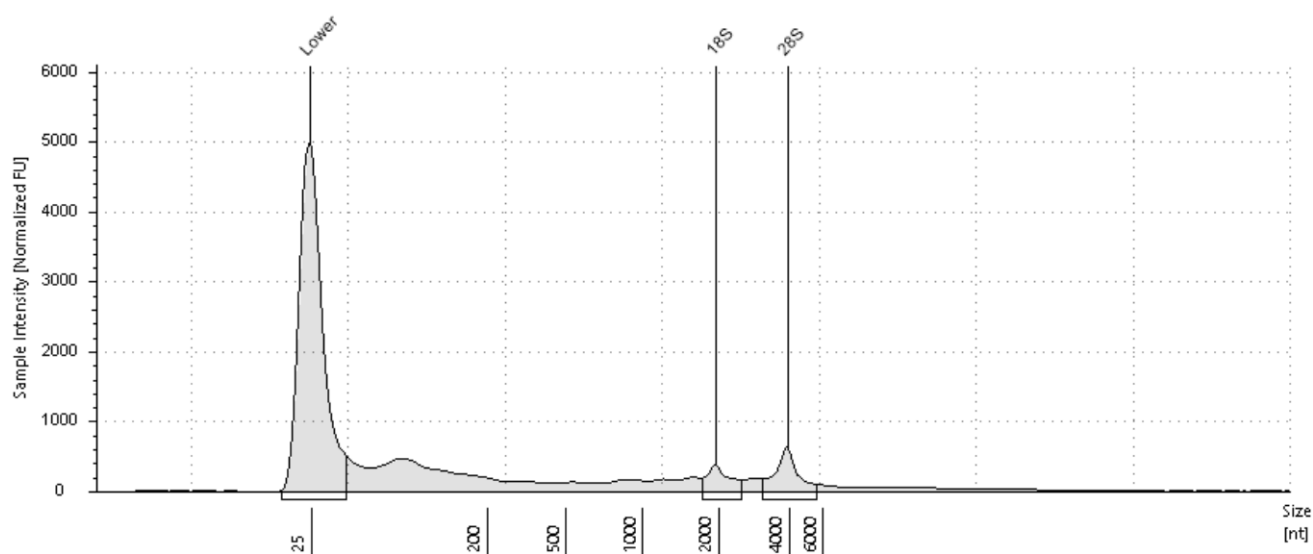
H1: 651**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
H1	6.9	1.6	35.6	651		

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1907	4.75	-	7.32	38.26		18S
4259	7.66	-	5.29	61.74		28S

A2: 673

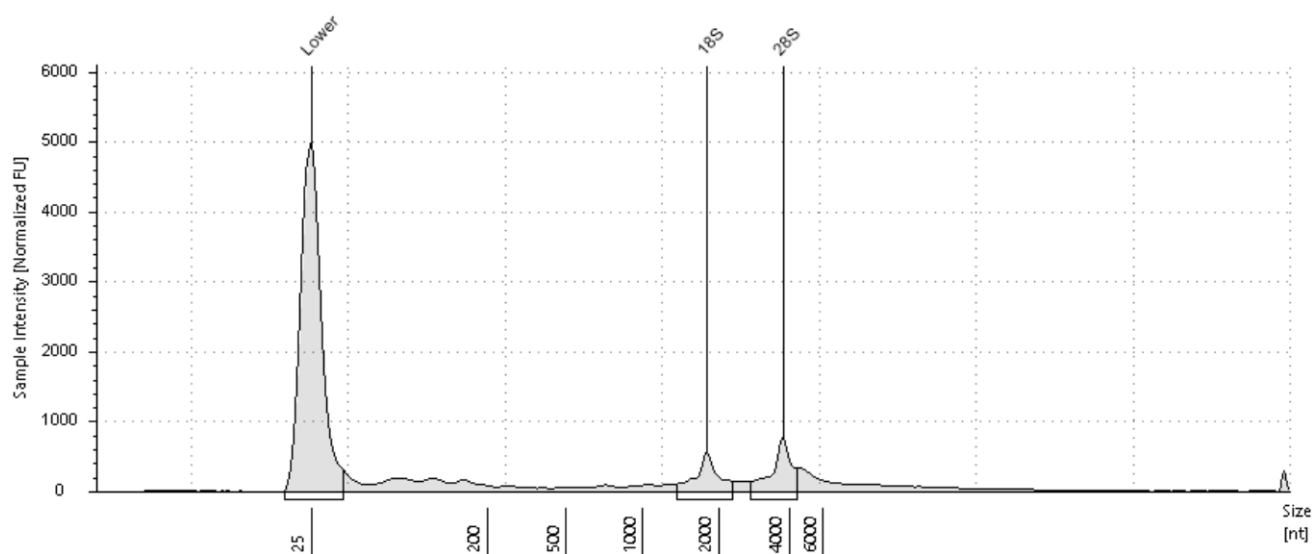


Sample Table

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
A2	5.3	1.6	19.4	673	⚠	Sample concentration outside functional range for RINe and the assay

Peak Table

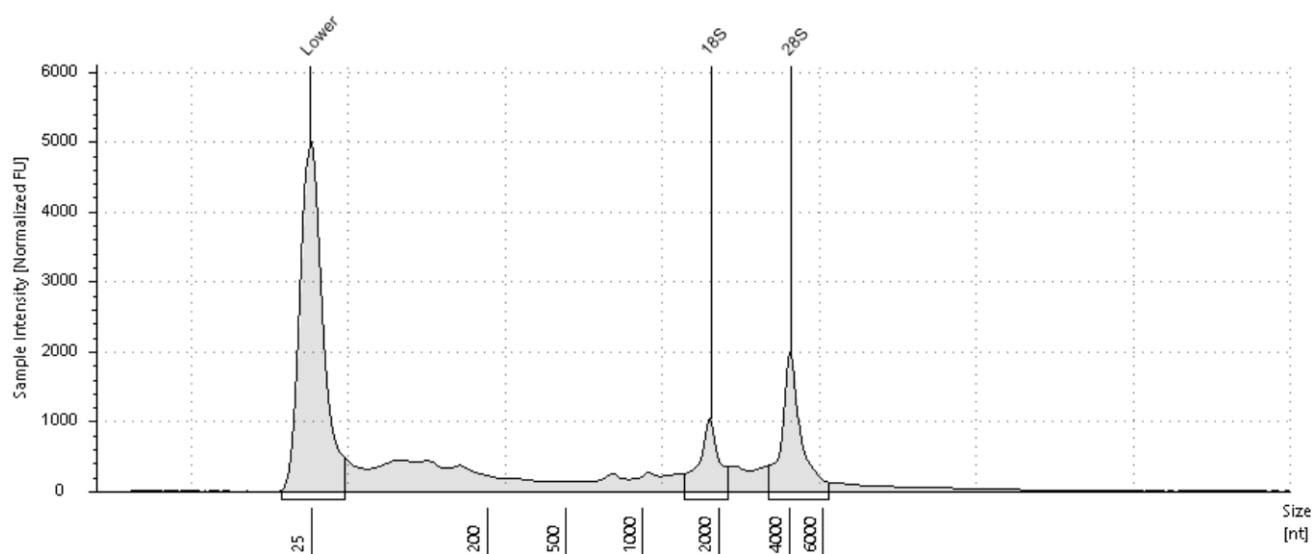
Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1976	1.58	-	2.35	38.50		18S
3977	2.52	-	1.87	61.50		28S

B2: 677**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
B2	8.3	1.2	16.1	677	⚠	Sample concentration outside functional range for RINe and the assay

Peak Table

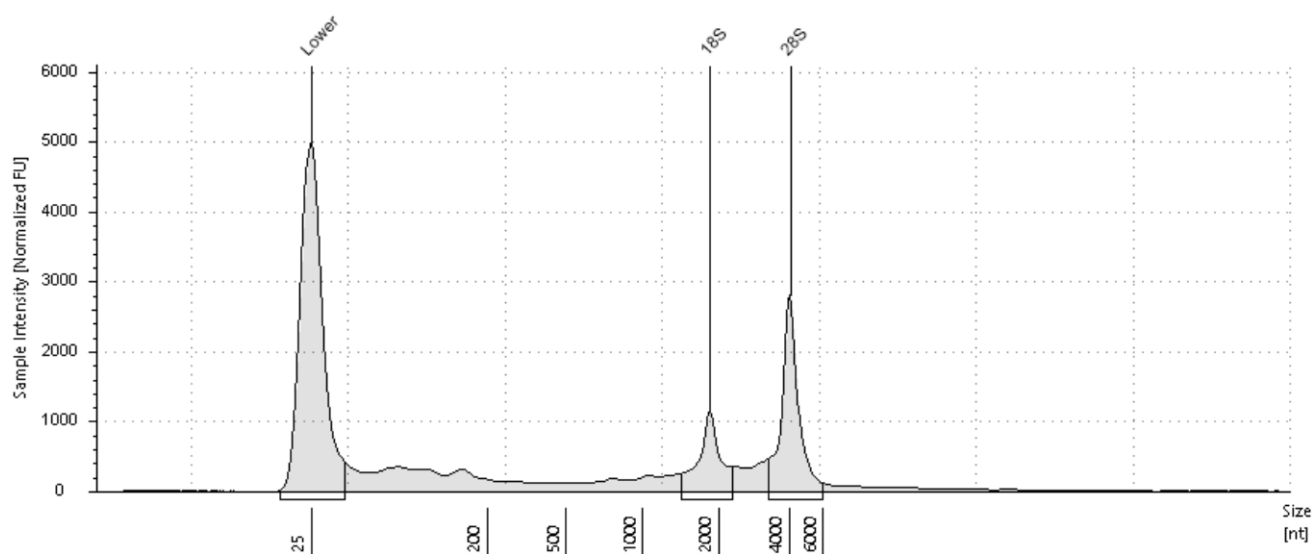
Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1805	2.47	-	4.02	44.89		18S
3786	3.03	-	2.35	55.11		28S

C2: 789**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
C2	7.4	1.9	29.8	789		

Peak Table

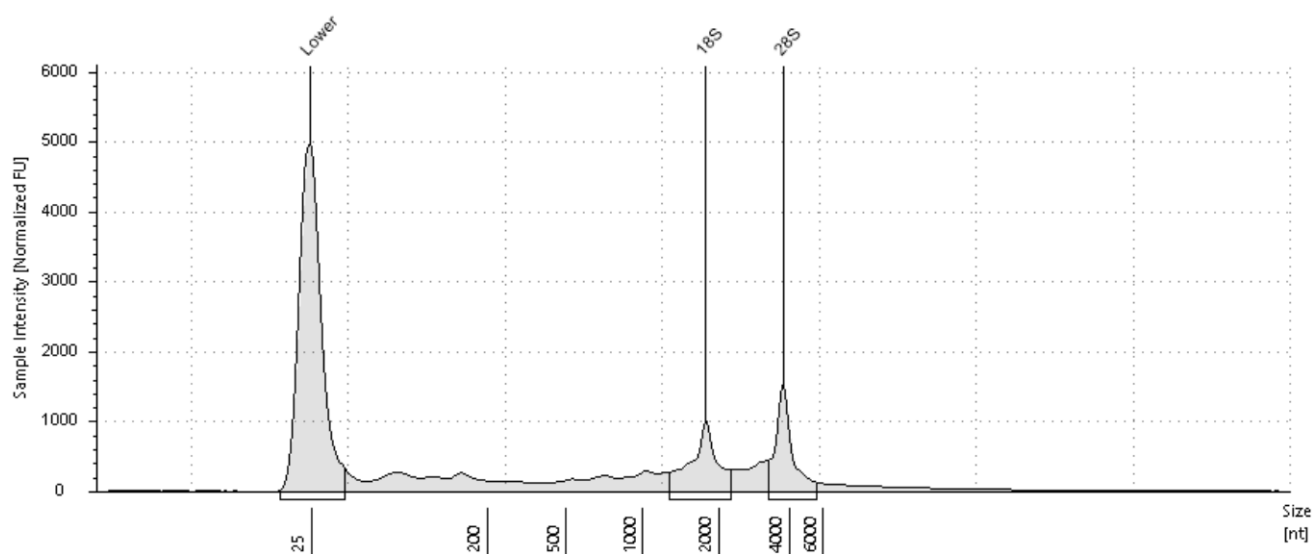
Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1865	3.85	-	6.07	34.86		18S
4146	7.19	-	5.10	65.14		28S

D2: 805**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/ul]	Sample Description	Alert	Observations
D2	7.9	1.9	29.5	805		

Peak Table

Size [nt]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1858	4.76	-	7.53	34.26		18S
4100	9.13	-	6.55	65.74		28S

E2: 807**Sample Table**

Well	RINe	28S/18S (Area)	Conc. [ng/μl]	Sample Description	Alert	Observations
E2	6.9	1.0	24.3	807	⚠	Sample concentration outside functional range for RINe and the assay

Peak Table

Size [nt]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	40.0	40.0	4710	-		Lower Marker
1793	4.96	-	8.14	49.90		18S
3841	4.98	-	3.81	50.10		28S