

Operational Qualification

LIMS

Test Case Summary

Project Name :	Veeva Vault v24R1 Veeva Vault Basics LIMS
Vault :	Spotline Vault
Test Case # :	BASICS-PQ-LIMS-14
Operator :	Automation
Start :	08-OCT-2026 07:29:37 GMT-07:00
End :	08-OCT-2026 09:30:01 GMT-07:00

Table of Contents

1 Test Case Summary 3
1.1 BASICS_PQ_LIMS_14 Test Cancellation (Virtual Vault) Report 4

1 Test Case Summary

This section lists all the test scripts used during the exeuction of the test case run.

Test Case ID	Script Version#	Test Case Name	Description	Req#	Pass/Fail	Start Time/ End Time
BASICS-PQ-LIMS-14	1.1	Spec Execution, Sample, and Test Cancellation (Virtual Vault)	Verify the cancellation workflows for Spec Execution, Sample, and Test.	R2	PASS	08-OCT-2026 07:29:41 08-OCT-2026 09:30:01

1.1 BASICS_PQ_LIMS_14 Test Cancellation (Virtual Vault) Report

This section lists all the test steps performed during the test case exeuction.


Step #	Description of Action	Expected Results	Actual Results	Pass/Fail
1	Log into Vault as USER1. From the LIMS tab collection, navigate to Release Testing > Spec Execution. Locate the SPEX1 from the setup steps and click the name link to open the record.	The Spec Execution is displayed.	The Spec Execution is displayed.	PASS
2	Navigate to the Tests section. Click Show in Tab. Use a filter or the favorites option so that only two tests are displayed. From the All Actions Menu, select Start Workflow. Within the Workflow dropdown select Test: Cancel. Click Continue. Click Start.	The workflow is started.	The workflow is started.	PASS
3	From the notifications confirm there is a task notification "Cancel Test" for the selected tests.	There is a task notification "Cancel Test" for the selected tests.	There is a task notification "Cancel Test" for the selected tests.	PASS
4	Navigate to the Home tab. Click the link to open the envelope for the cancellation task. Click Complete in the task bar. Select Do not Cancel Test verdict. Click Complete.	The workflow ends. Both tests are in the Not Started state.	The workflow ends. Both tests are in the Not Started state.	PASS
5	Navigate to SPEX1 and expand the Tests section. Click Show in Tab. Use a filter or the favorites option so that only two tests are displayed. From the All Actions Menu, select Start Workflow. Within the Workflow dropdown select Test: Cancel. Click Continue. Click Start.	The workflow is started.	The workflow is started.	PASS
6	Navigate to the Home tab. Click the link to open the envelope for the cancellation task. Click Complete in the task bar. Select Cancel Test verdict. Enter the Reason for Cancellation. Select an Electronic Signature Meaning, complete the e-signature. Click Complete.	The workflow ends. Both tests are in the Cancelled state. The Spec Execution and the Sample remain in the Not Started state.	The workflow ends. Both tests are in the Cancelled state. The Spec Execution and the Sample remain in the Not Started state.	PASS
7	From the LIMS tab collection, navigate to Release Testing > Spec Execution. Locate the SPEX2 from the setup steps and click the name link to open the record.	The Spec Execution is displayed.	The Spec Execution is displayed.	PASS
8	Navigate to the Samples section. Click Show in	The workflow is started.	The workflow is started.	PASS

Step #	Description of Action	Expected Results	Actual Results	Pass/Fail
	Tab. From the All Actions Menu, select Start Workflow. Within the Workflow dropdown select Sample: Cancel. Click Continue. Click Start.			
9	From the notifications confirm there is a task notification "Cancel Sample" for the selected samples.	There is a task notification "Cancel Sample" for the selected samples.	There is a task notification "Cancel Sample" for the selected samples.	PASS
10	Navigate to the Home tab. Click the link to open the envelope for the cancellation task. Click Complete in the task bar. Select Do not Cancel Sample verdict. Click Complete.	The workflow ends. Both samples are in the Not Started state.	The workflow ends. Both samples are in the Not Started state.	PASS
11	Navigate to SPEX2 and expand the Samples section. Click Show in Tab. From the All Actions Menu, select Start Workflow. Within the Workflow dropdown select Sample: Cancel. Click Continue. Click Start.	The workflow is started.	The workflow is started.	PASS
12	Navigate to the Home tab. Click the link to open the envelope for the cancellation task. Click Complete in the task bar. Select Cancel Sample verdict. Enter the Reason for Cancellation. Select an Electronic Signature Meaning, complete the e-signature. Click Complete.	The workflow ends. Both Samples are in the Cancelled state. All tests are in the Cancelled state. The Spec Execution remains in the Not Started state.	The workflow ends. Both Samples are in the Cancelled state. All tests are in the Cancelled state. The Spec Execution remains in the Not Started state.	PASS
13	Log into Vault as USER2. From the LIMS tab collection, navigate to Release Testing > Spec Execution. Use a filter or the favorites option so that only SPEX3 and SPEX4 are displayed.	SPEX3 and SPEX4 are displayed.	SPEX3 and SPEX4 are displayed.	PASS
14	From the All Actions Menu, select Start Workflow. Within the Workflow dropdown select Spec Execution: Cancel. Click Continue. Click Start.	The workflow is started.	The workflow is started.	PASS
15	From the notifications confirm there is a task notification "Cancel Spec execution" for the selected spec executions	There is a task notification "Cancel Spec execution" for the selected spec executions.	There is a task notification "Cancel Spec execution" for the selected spec executions.	PASS
16	Navigate to the Home tab. Click the link to open the envelope for the cancellation task. Click Complete in the task bar. Select Do not Cancel Spec execution verdict. Click Complete.	The workflow ends. SPEX3 is in the Not Started state, SPEX4 is in the Logged state.	The workflow ends. SPEX3 is in the Not Started state, SPEX4 is in the Logged state.	PASS
17	From the LIMS tab collection, navigate to Release Testing > Spec Execution. Use a filter or the favorites option so that only SPEX3 and	The workflow is started.	The workflow is started.	PASS


Step #	Description of Action	Expected Results	Actual Results	Pass/Fail
	SPEX4 are displayed. From the All Actions Menu, select Start Workflow. Within the Workflow dropdown select Spec Execution: Cancel. Click Continue. Click Start.			
18	Navigate to the Home tab. Click the link to open the envelope for the cancellation task. Click Complete in the task bar. Select Cancel Spec Execution verdict. Enter the Reason for Cancellation. Select an Electronic Signature Meaning, complete the e-signature. Click Complete.	The workflow ends. Both Spec Executions are in the Cancelled state. The samples and tests associated to SPEX3 are in the Cancelled state. The batches associated with SPEX3 and SPEX4 are in the Cancelled state.	The workflow ends. Both Spec Executions are in the Cancelled state. The samples and tests associated to SPEX3 are in the Cancelled state. The batches associated with SPEX3 and SPEX4 are in the Cancelled state.	PASS

Comments	
Screenshots Attached: YES	If yes, Number of Screenshots Attached: 18


Step #1 Screenshot Screenshot Time: 08-OCT-2026 08:44:08 GMT-07:00

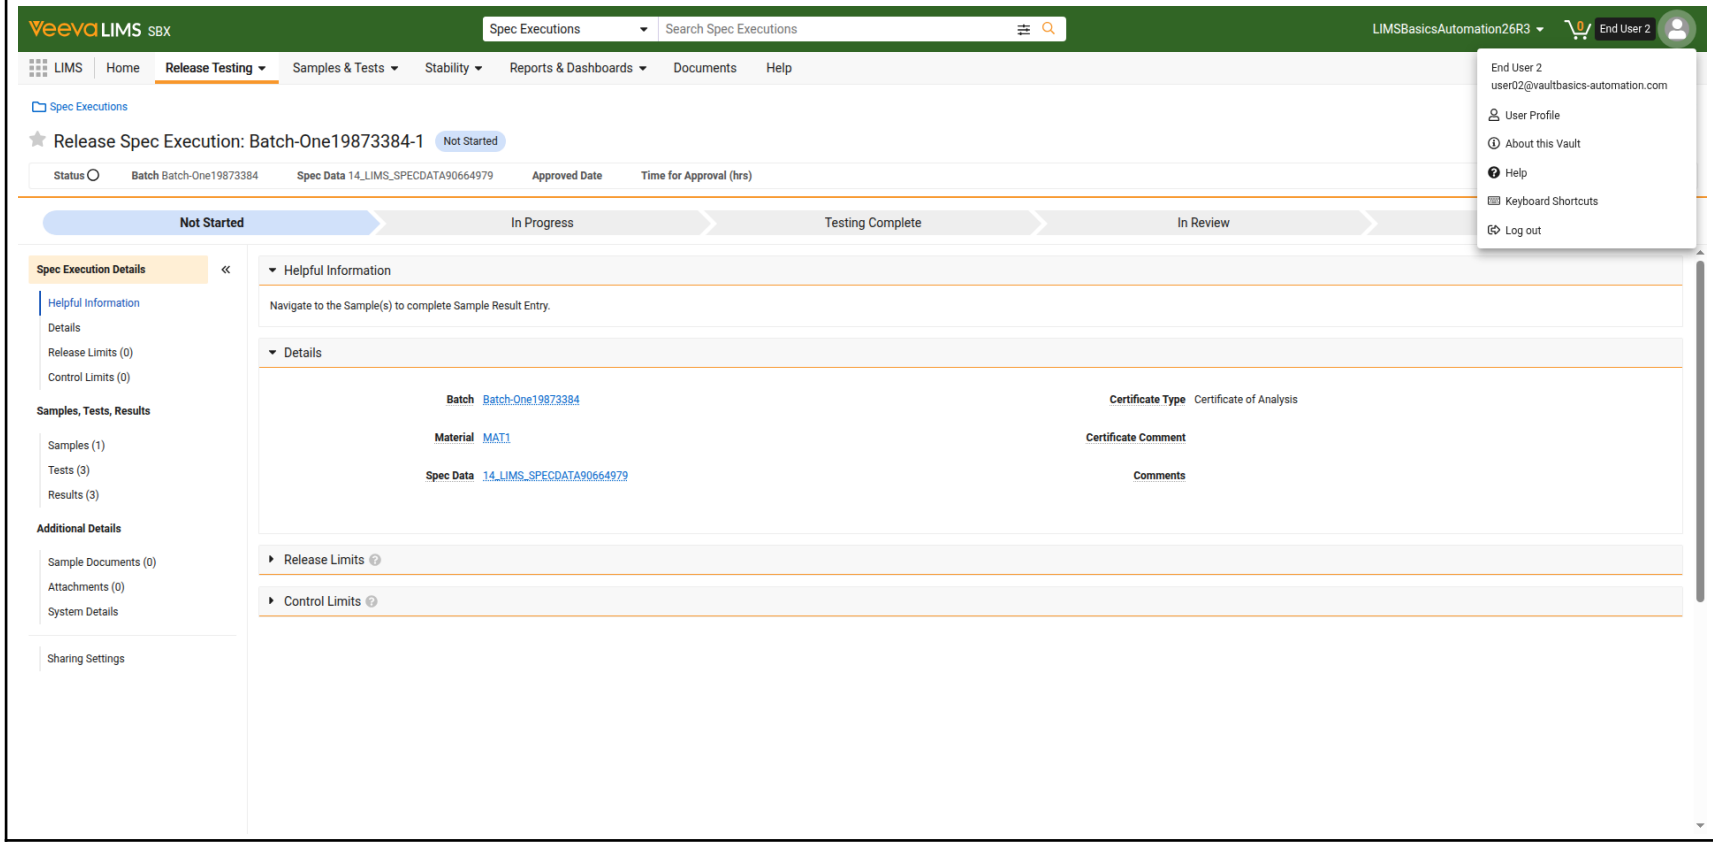


Step #2 Screenshot Screenshot Time: 08-OCT-2026 08:45:11 GMT-07:00

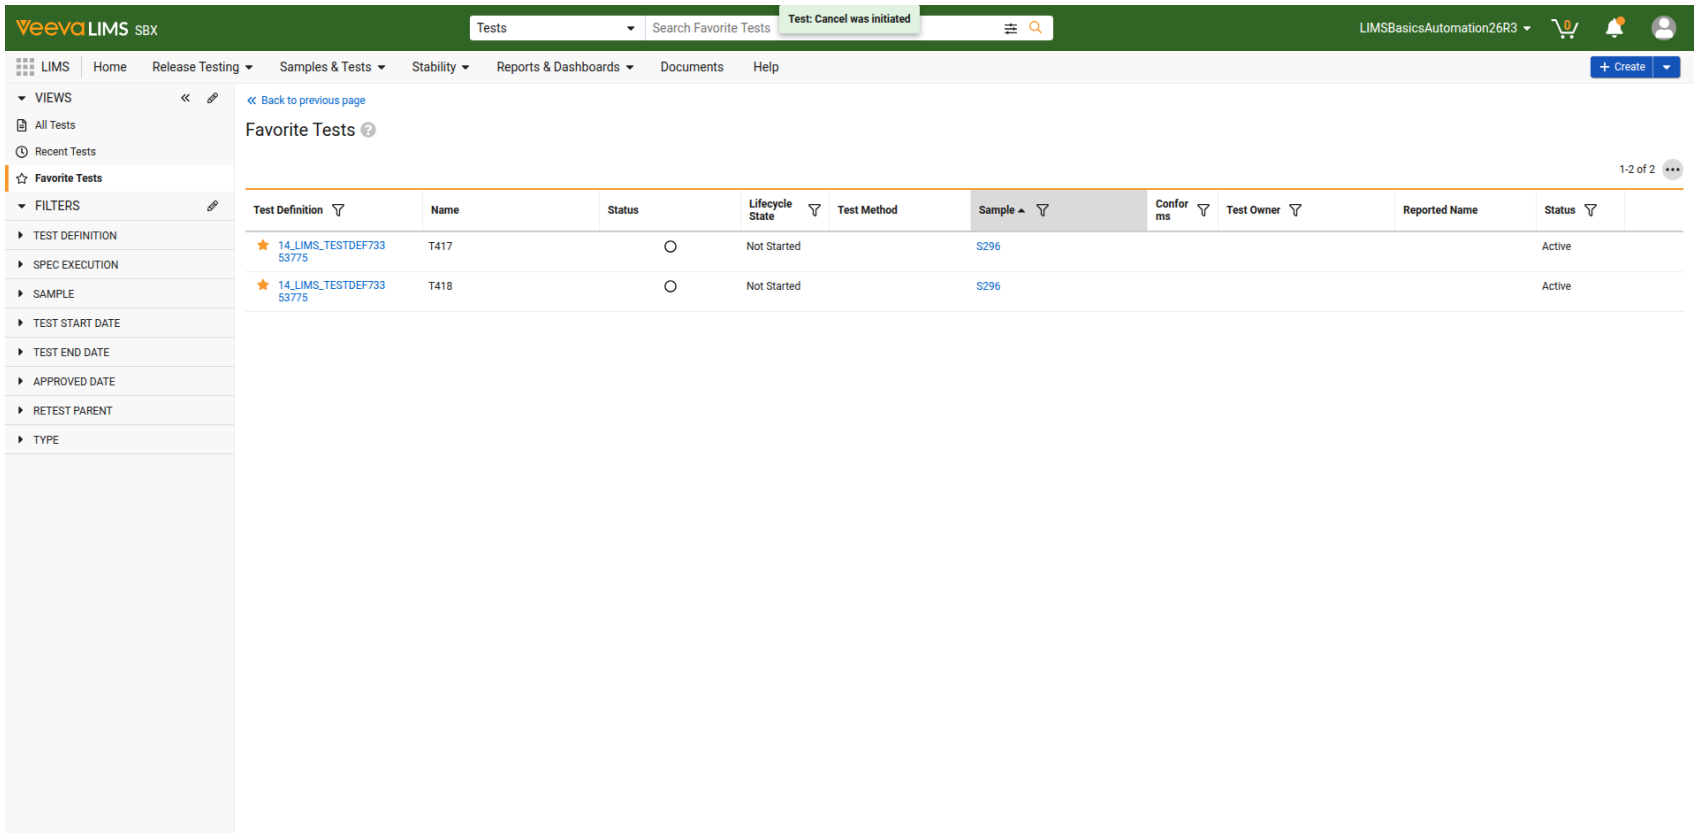


Step #3 Screenshot Screenshot Time: 08-OCT-2026 08:45:20 GMT-07:00

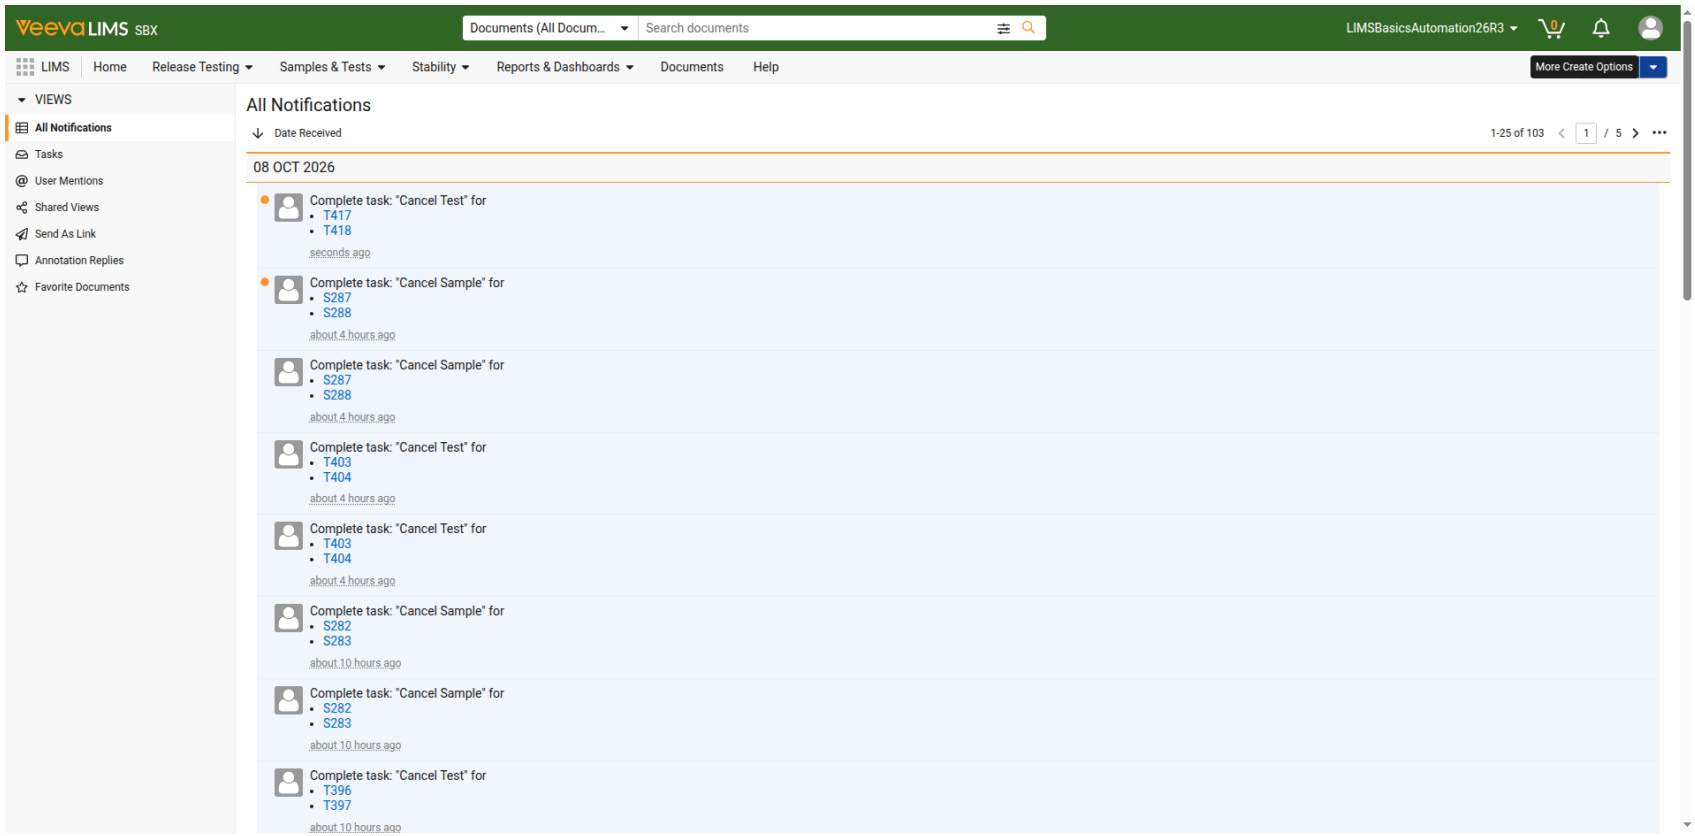


Step #4 Screenshot Screenshot Time: 08-OCT-2026 08:46:10 GMT-07:00,08-OCT-2026 08:46:17 GMT-07:00

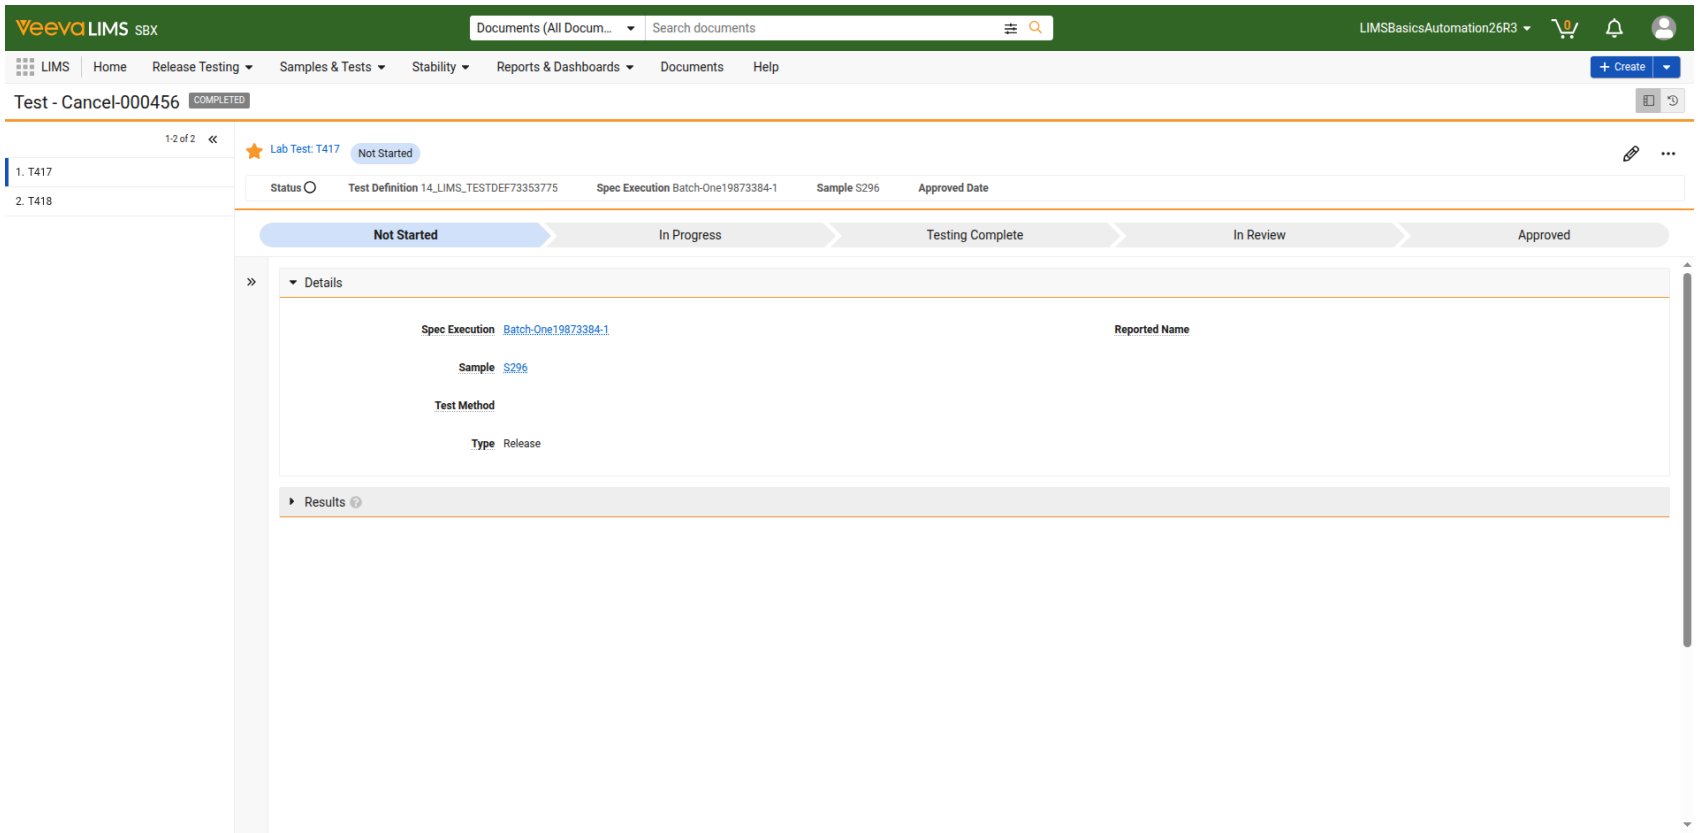


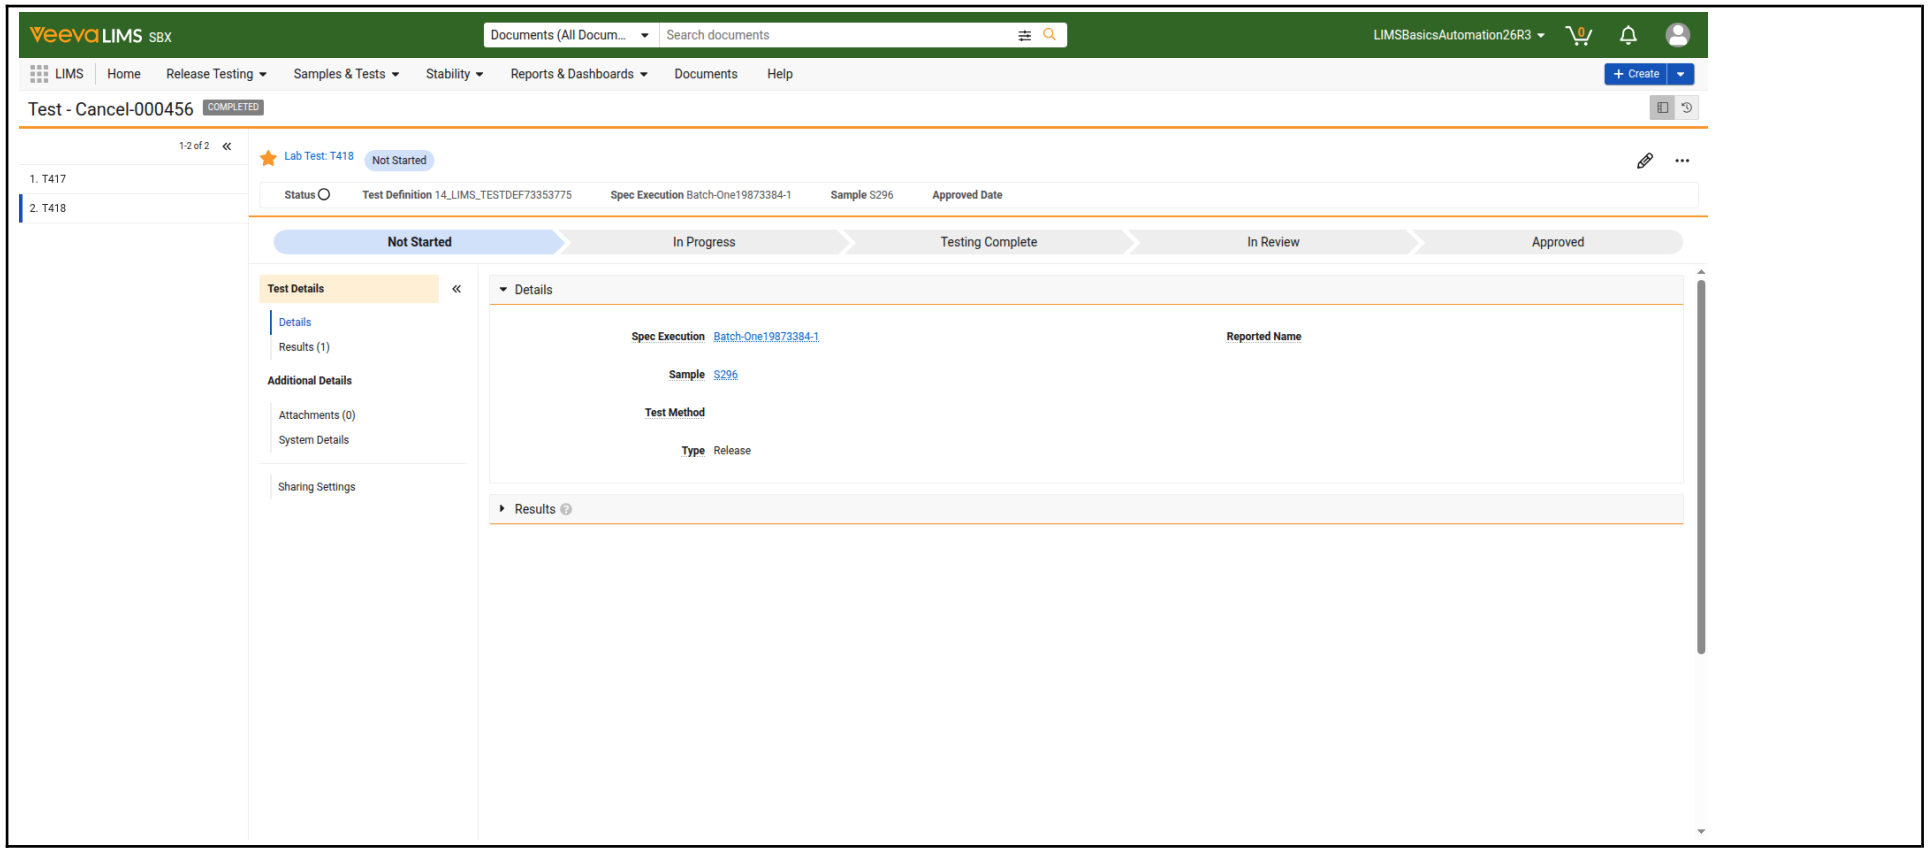

Veeva LIMS SBX
Documents (All Docum...
Search documents
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
+ Create
Test - Cancel-000456
COMPLETED
1-2 of 2
1. T417
2. T418
Lab Test: T418
Not Started
Status
Test Definition 14_LIMS_TESTDEF73353775
Spec Execution Batch-One19873384-1
Sample S296
Approved Date
Not Started
In Progress
Testing Complete
In Review
Approved
Test Details
Details
Results (1)
Additional Details
Attachments (0)
System Details
Sharing Settings
Details
Spec Execution Batch-One19873384-1
Reported Name
Sample S296
Test Method
Type Release
Results


Step #5 Screenshot Screenshot Time: 08-OCT-2026 08:47:06 GMT-07:00

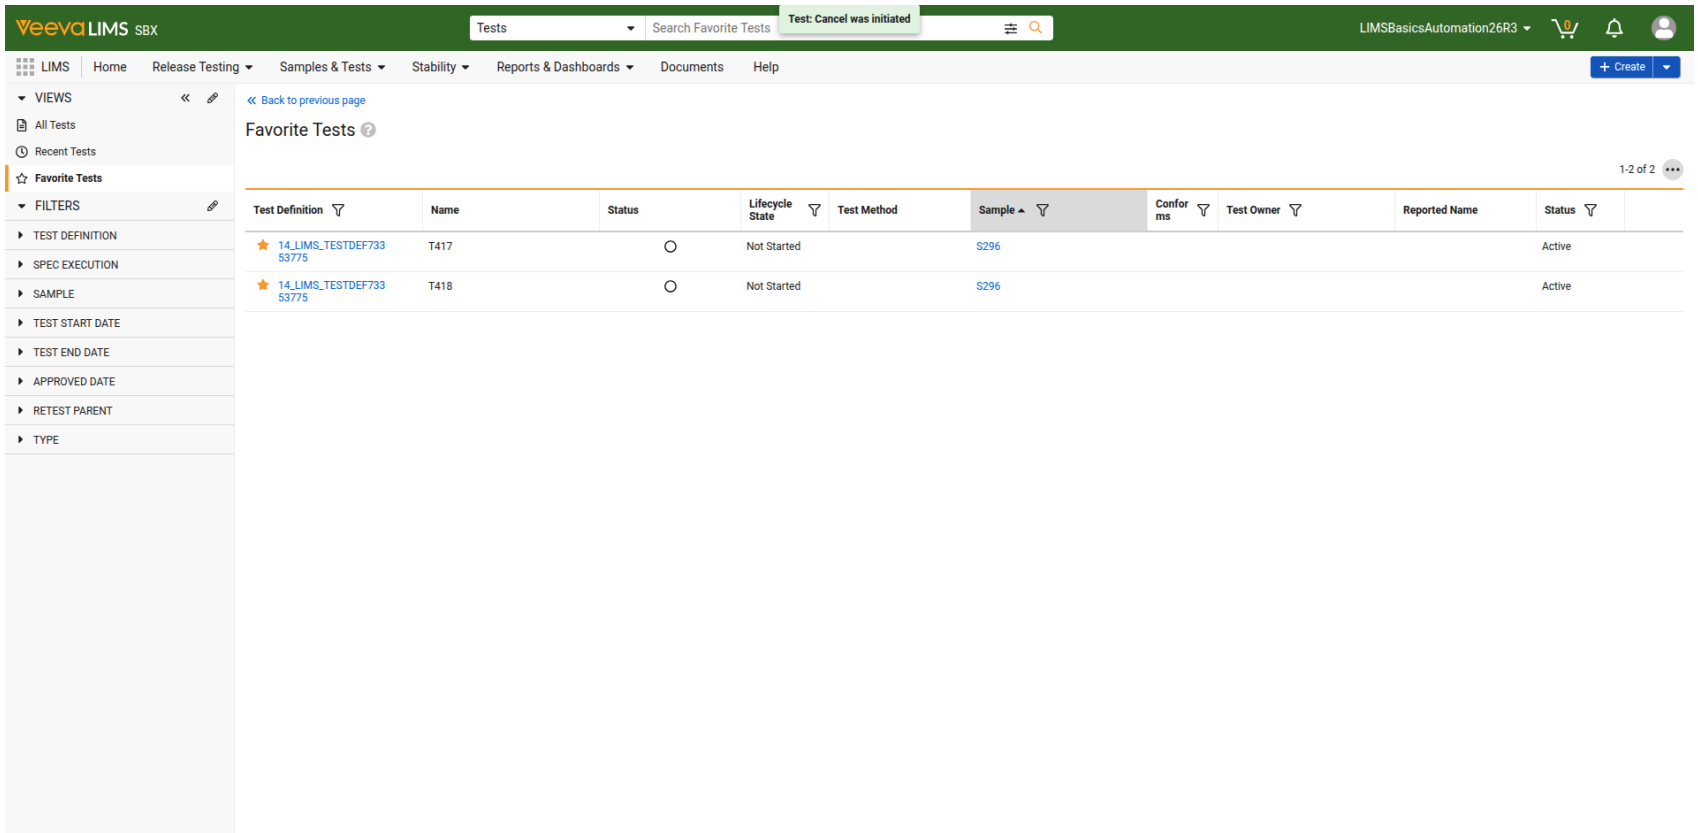


Step #6 Screenshot Screenshot Time: 08-OCT-2026 08:48:23 GMT-07:00,08-OCT-2026 08:48:31 GMT-07:00,08-OCT-2026 08:48:38 GMT-07:00,08-OCT-2026 08:48:49 GMT-07:00

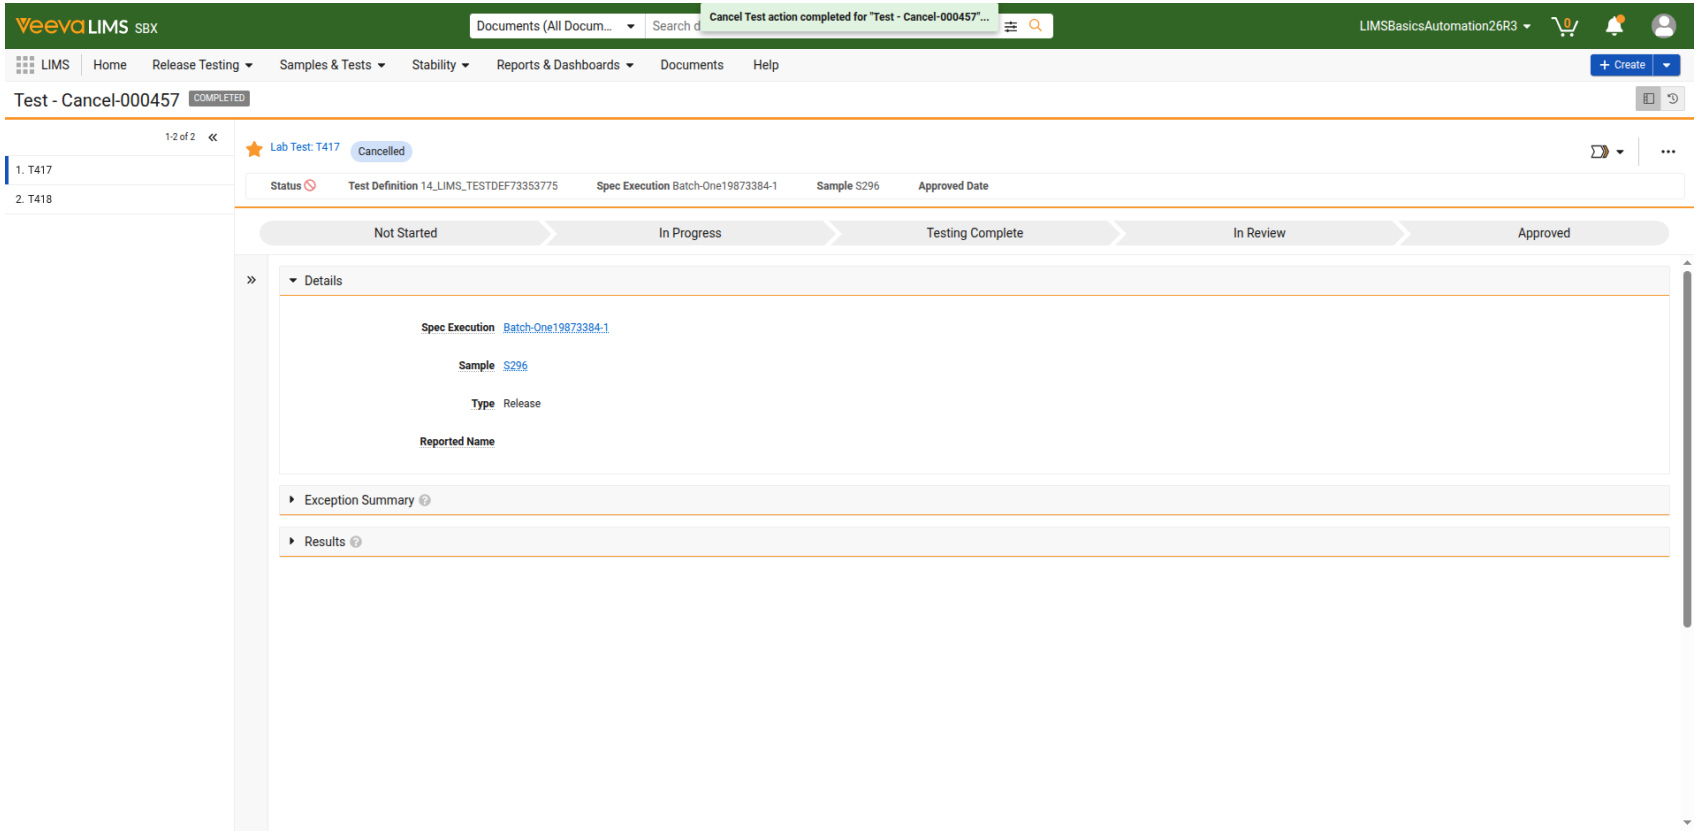


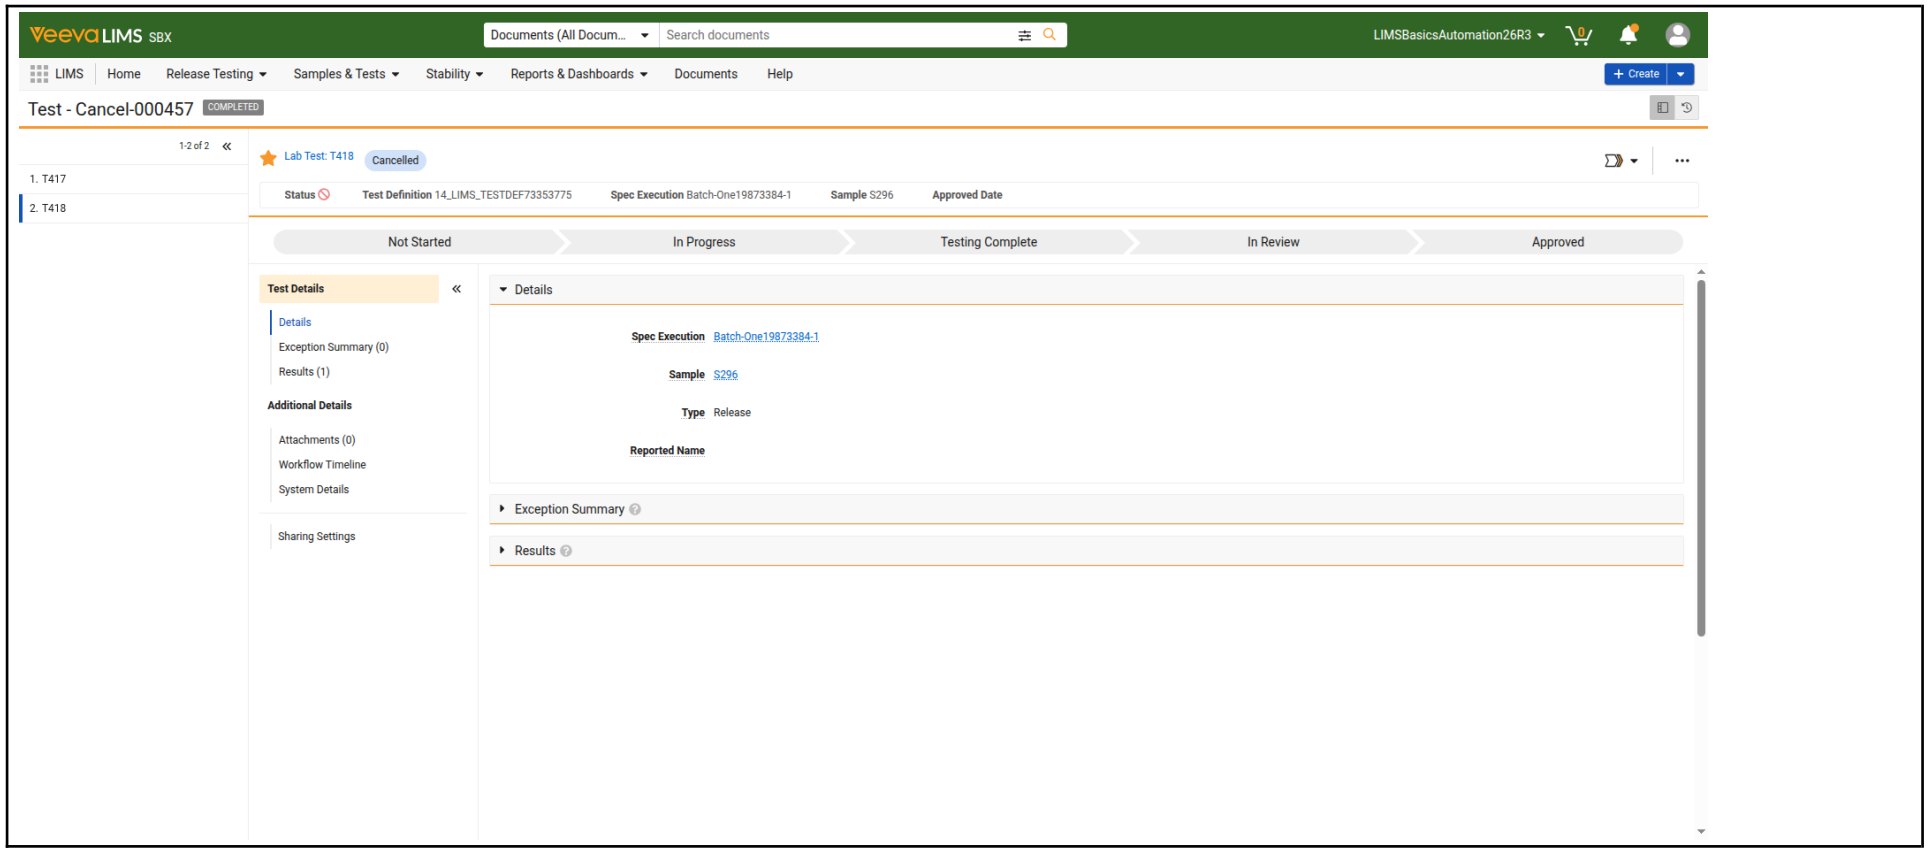
Veeva LIMS SBX
Documents (All Docum...
Search documents
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
Create
Test - Cancel-000457
COMPLETED
1-2 of 2
1. T417
2. T418
Lab Test: T418
Cancelled
Status
Test Definition 14_LIMS_TESTDEF73353775
Spec Execution Batch-One19873384-1
Sample S296
Approved Date
Not Started
In Progress
Testing Complete
In Review
Approved
Test Details
Details
Exception Summary (0)
Results (1)
Additional Details
Attachments (0)
Workflow Timeline
System Details
Sharing Settings
Details
Spec Execution Batch-One19873384-1
Sample S296
Type Release
Reported Name
Exception Summary
Results

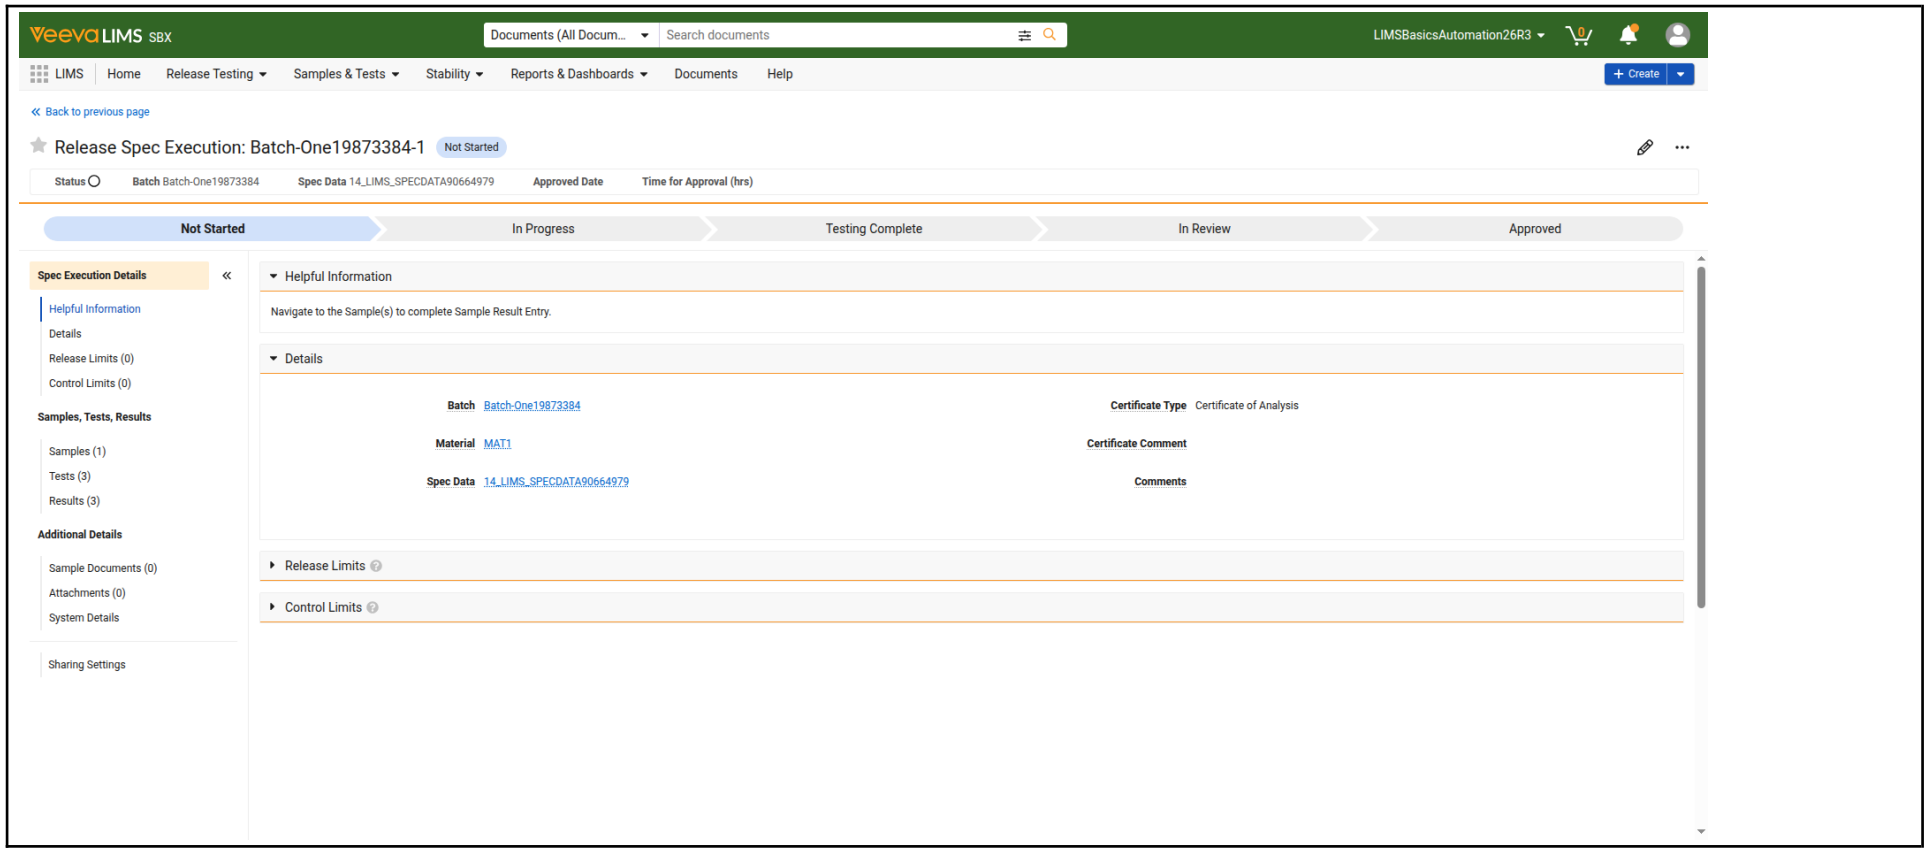

Veeva LIMS SBX
Documents (All Docum...
Search documents
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
Create
Back to previous page
Release Spec Execution: Batch-One19873384-1
Not Started
Status
Batch Batch-One19873384
Spec Data 14_LIMS_SPECDATA90664979
Approved Date
Time for Approval (hrs)
Not Started
In Progress
Testing Complete
In Review
Approved
Spec Execution Details
Helpful Information
Details
Release Limits (0)
Control Limits (0)
Samples, Tests, Results
Samples (1)
Tests (3)
Results (3)
Additional Details
Sample Documents (0)
Attachments (0)
System Details
Sharing Settings
Helpful Information
Navigate to the Sample(s) to complete Sample Result Entry.
Details
Batch Batch-One19873384
Material MAT1
Spec Data 14_LIMS_SPECDATA90664979
Certificate Type Certificate of Analysis
Certificate Comment
Comments
Release Limits
Control Limits

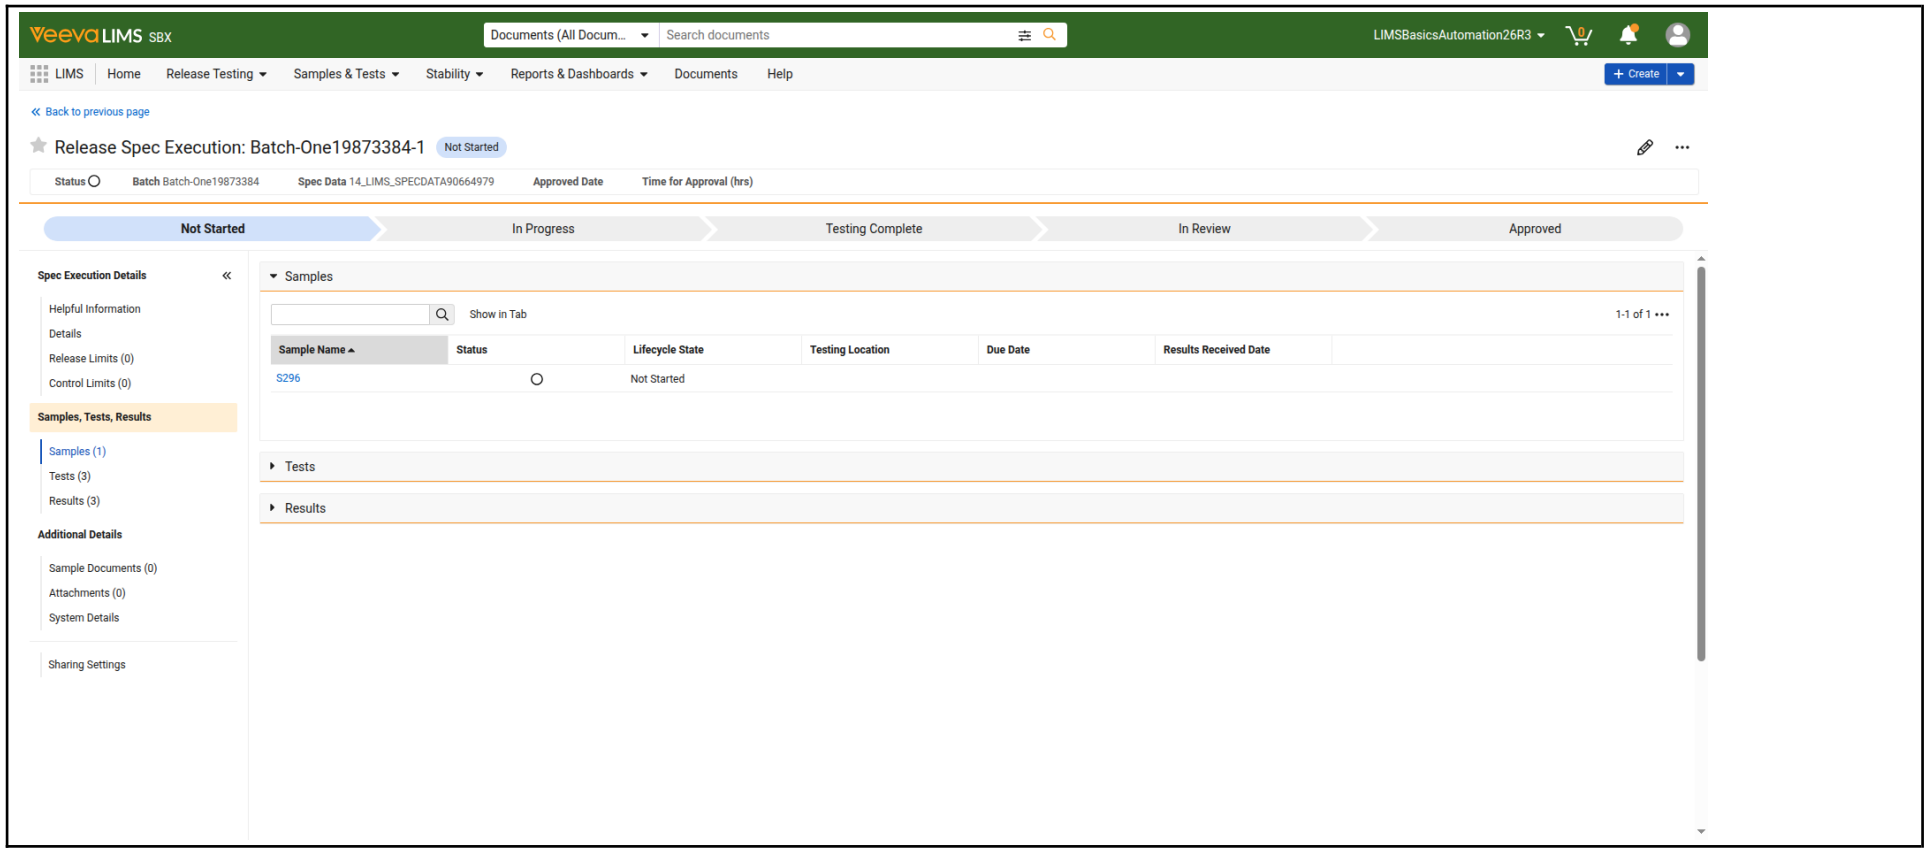
Veeva LIMS SBX
Documents (All Docum...
Search documents
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
Create
Back to previous page
Release Spec Execution: Batch-One19873384-1
Not Started
Status
Batch Batch-One19873384
Spec Data 14_LIMS_SPECDATA90664979
Approved Date
Time for Approval (hrs)
Not Started
In Progress
Testing Complete
In Review
Approved
Spec Execution Details
Helpful Information
Details
Release Limits (0)
Control Limits (0)
Samples, Tests, Results
Samples (1)
Tests (3)
Results (3)
Additional Details
Sample Documents (0)
Attachments (0)
System Details
Sharing Settings
Samples
Show in Tab
1-1 of 1
Sample Name
Status
Lifecycle State
Testing Location
Due Date
Results Received Date
S296
Not Started
Tests
Results


Step #7 Screenshot Screenshot Time: 08-OCT-2026 08:50:31 GMT-07:00

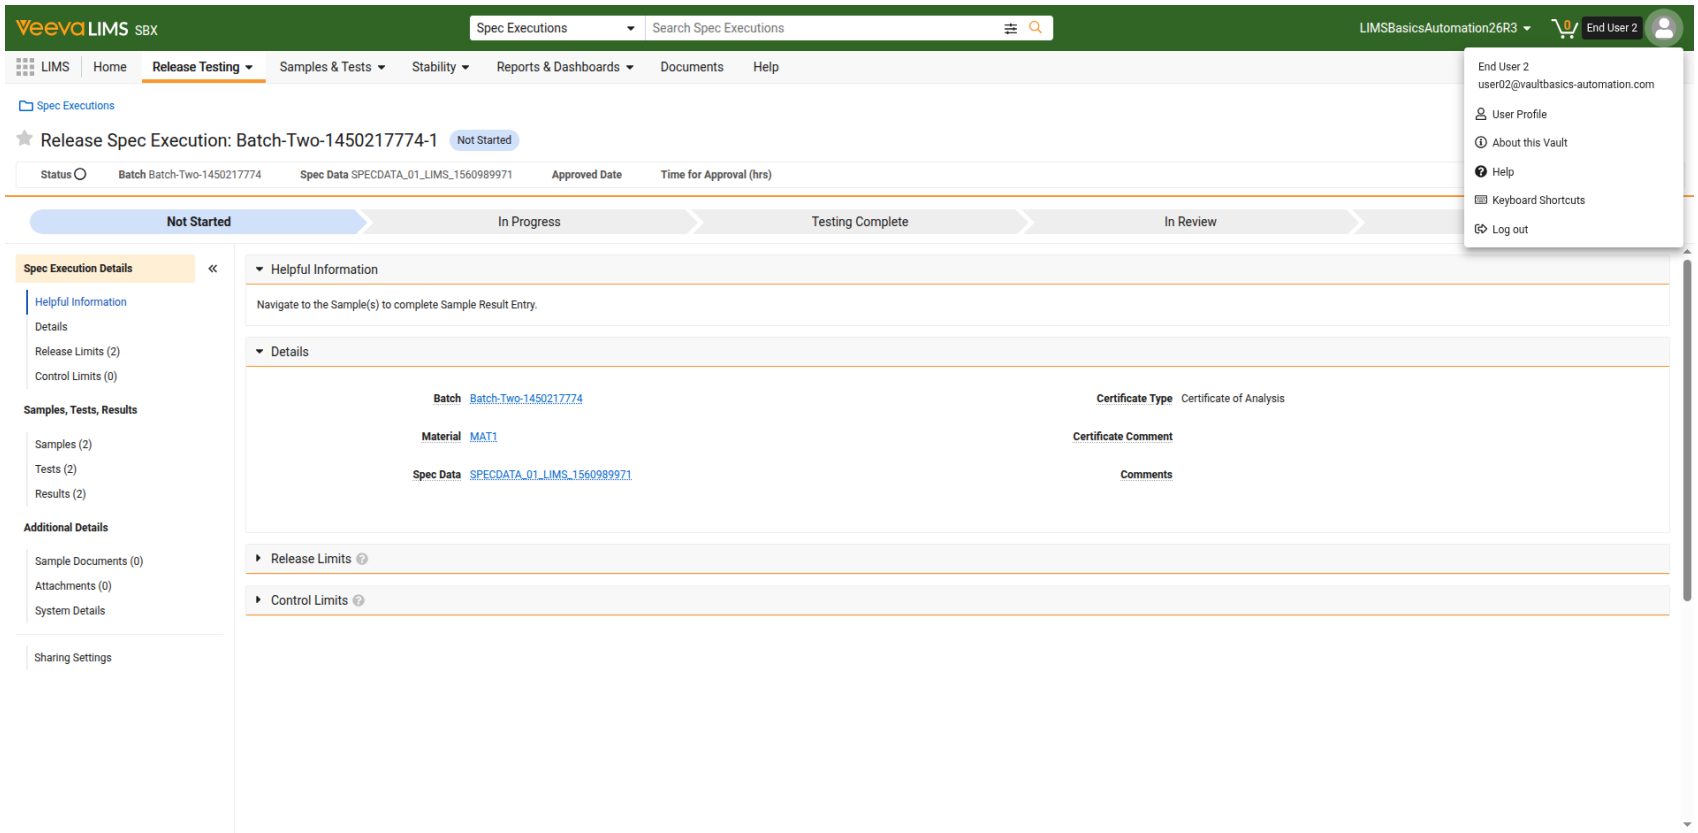


Step #8 Screenshot Screenshot Time: 08-OCT-2026 08:51:24 GMT-07:00

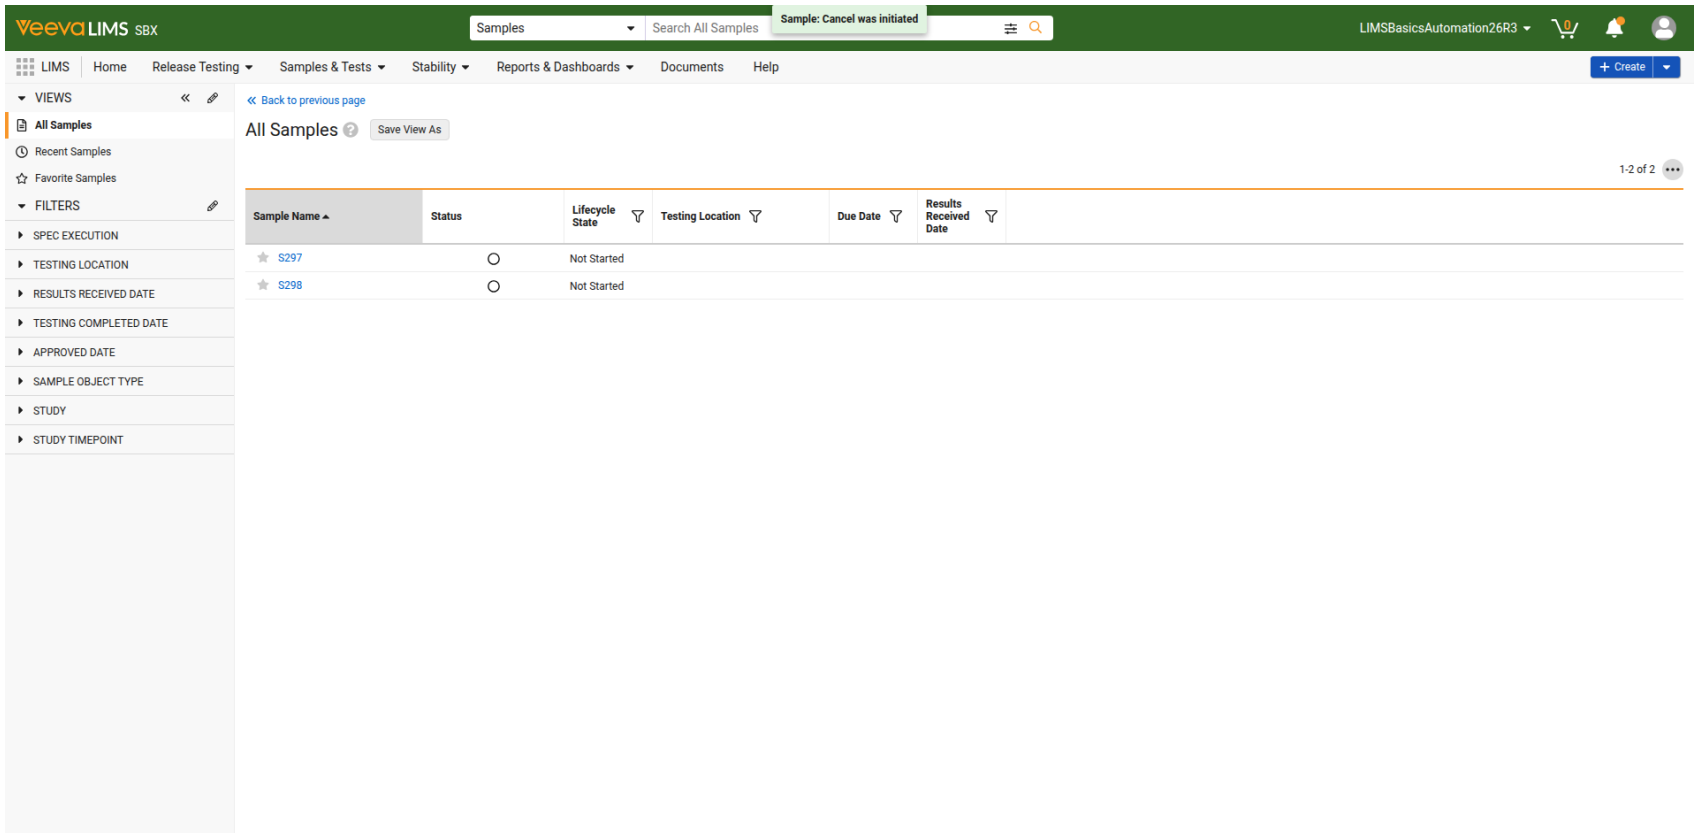


Step #9 Screenshot Screenshot Time: 08-OCT-2026 08:51:34 GMT-07:00

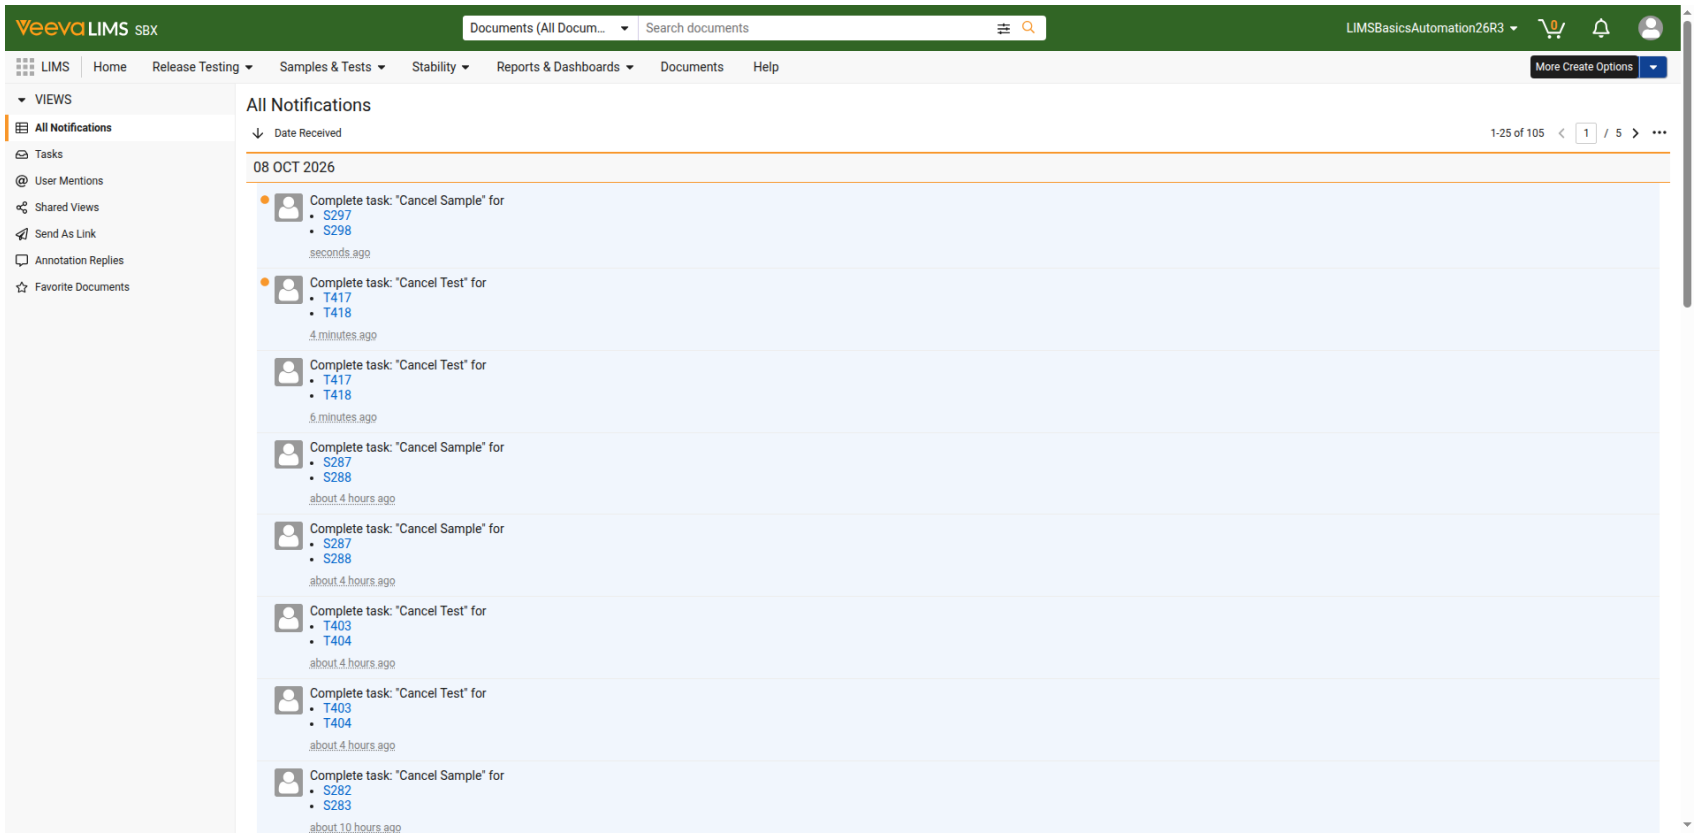


Step #10 Screenshot Screenshot Time: 08-OCT-2026 08:53:44 GMT-07:00,08-OCT-2026 08:53:52 GMT-07:00

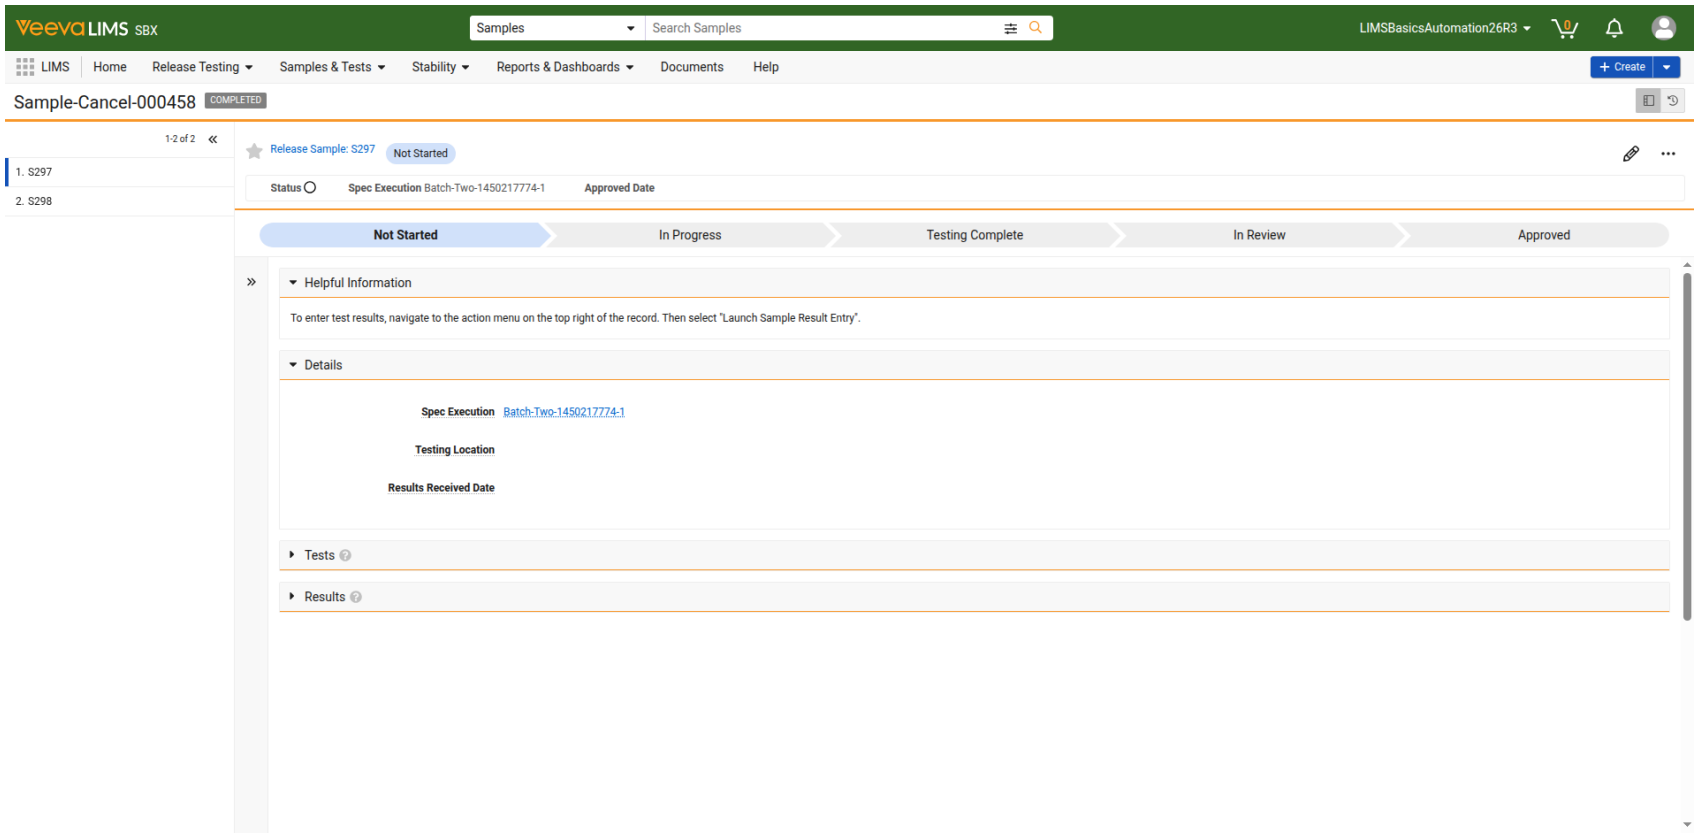


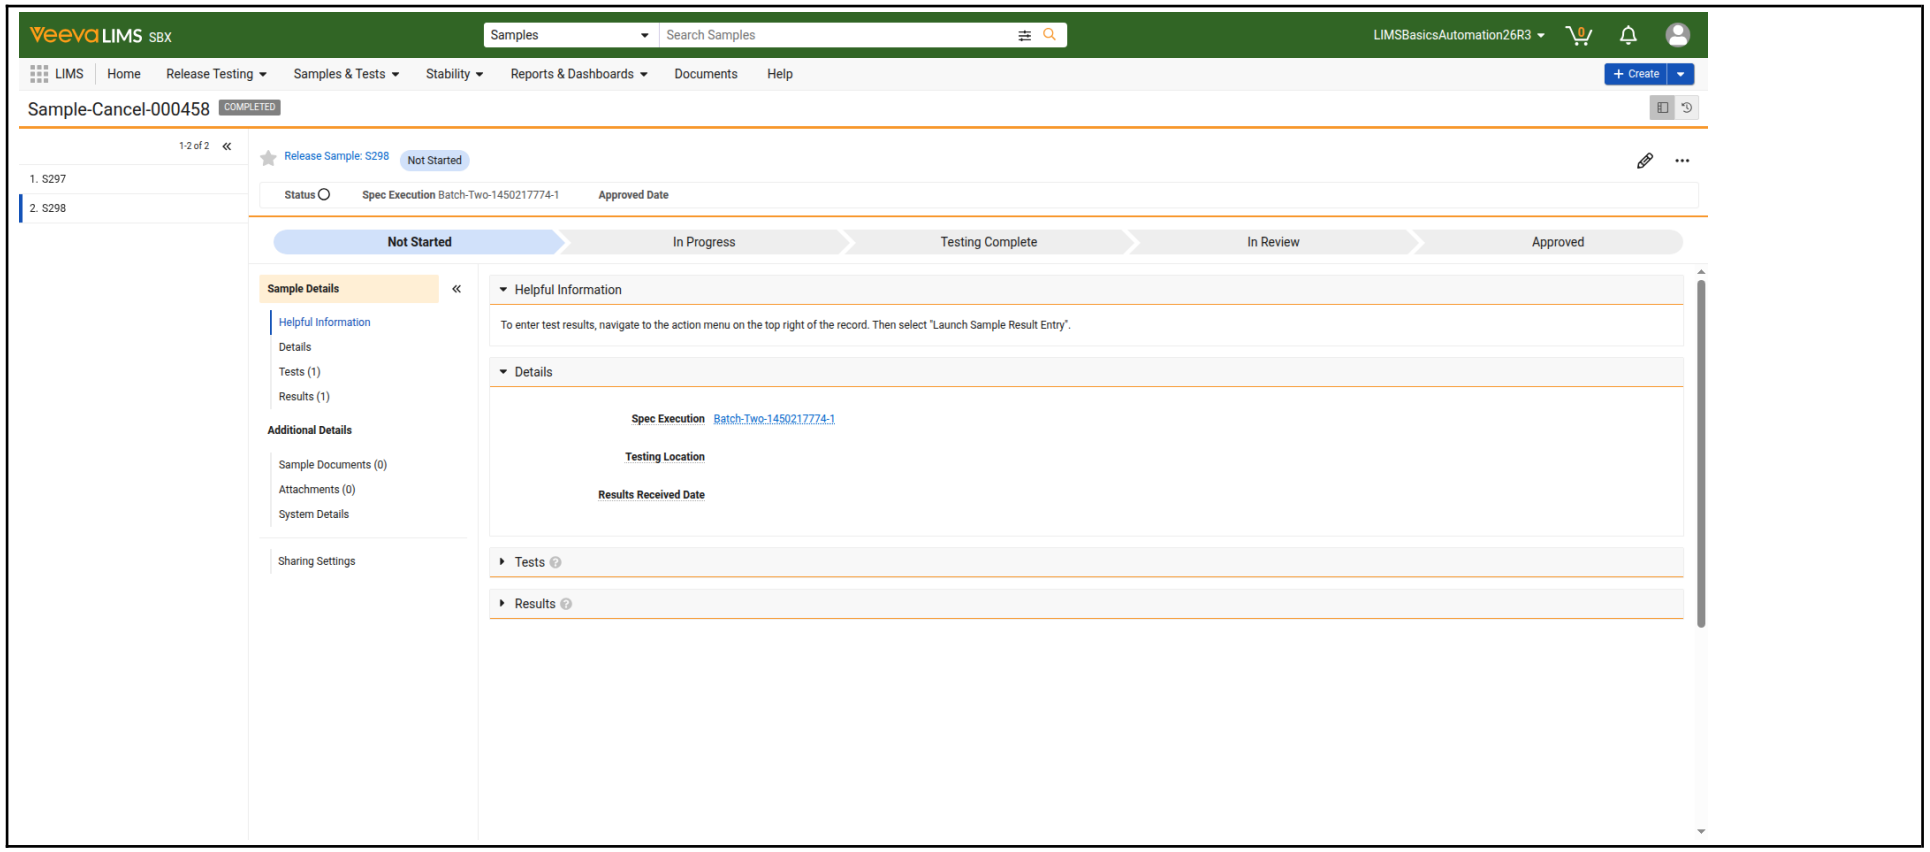

Veeva LIMS SBX
Samples
Search Samples
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
+ Create
Sample-Cancel-000458
COMPLETED
1-2 of 2
1. S297
2. S298
Release Sample: S298
Not Started
Status
Spec Execution Batch-Two-1450217774-1
Approved Date
Not Started
In Progress
Testing Complete
In Review
Approved
Sample Details
Helpful Information
Details
Tests (1)
Results (1)
Additional Details
Sample Documents (0)
Attachments (0)
System Details
Sharing Settings
Helpful Information
To enter test results, navigate to the action menu on the top right of the record. Then select "Launch Sample Result Entry".
Details
Spec Execution
Batch-Two-1450217774-1
Testing Location
Results Received Date
Tests
Results


Step #11 Screenshot Screenshot Time: 08-OCT-2026 08:54:38 GMT-07:00

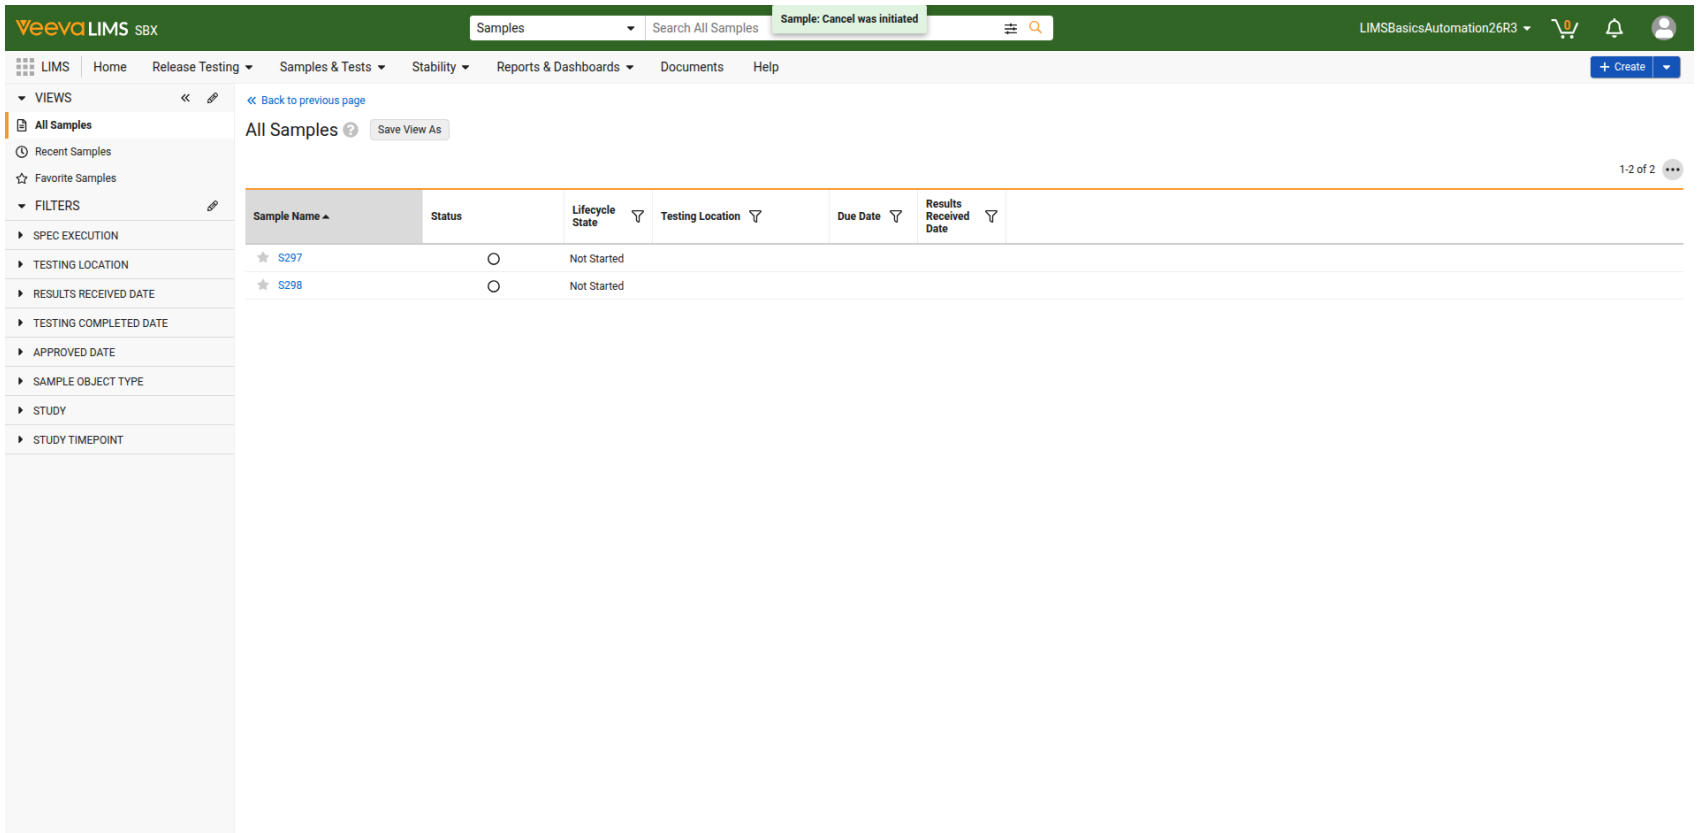


Step #12 Screenshot Screenshot Time: 08-OCT-2026 09:02:16 GMT-07:00,08-OCT-2026 09:02:31 GMT-07:00,08-OCT-2026 09:08:22 GMT-07:00

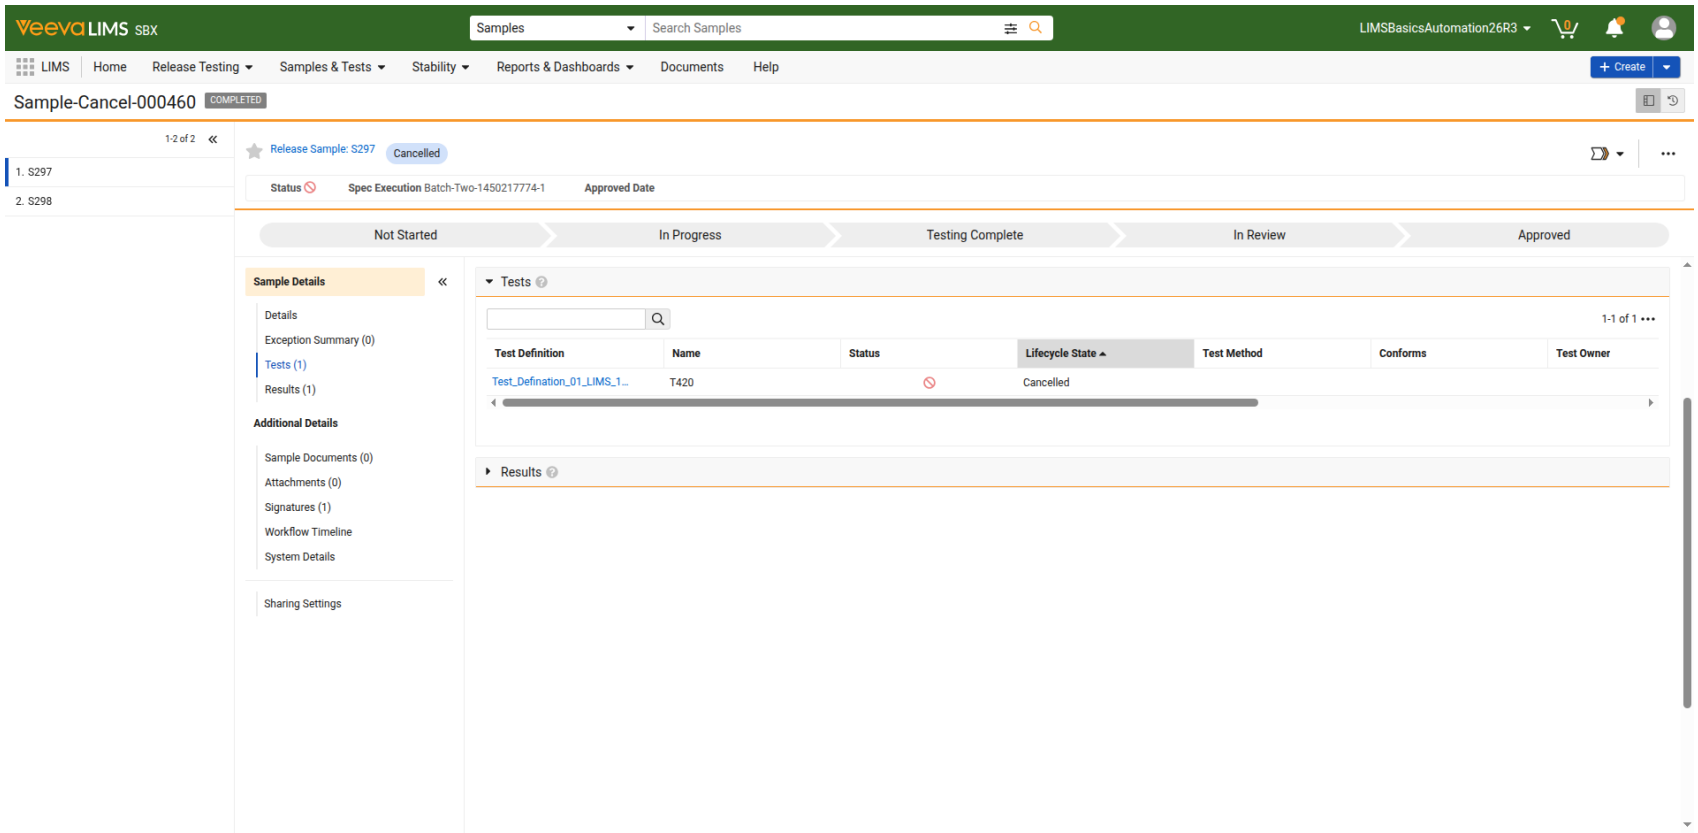

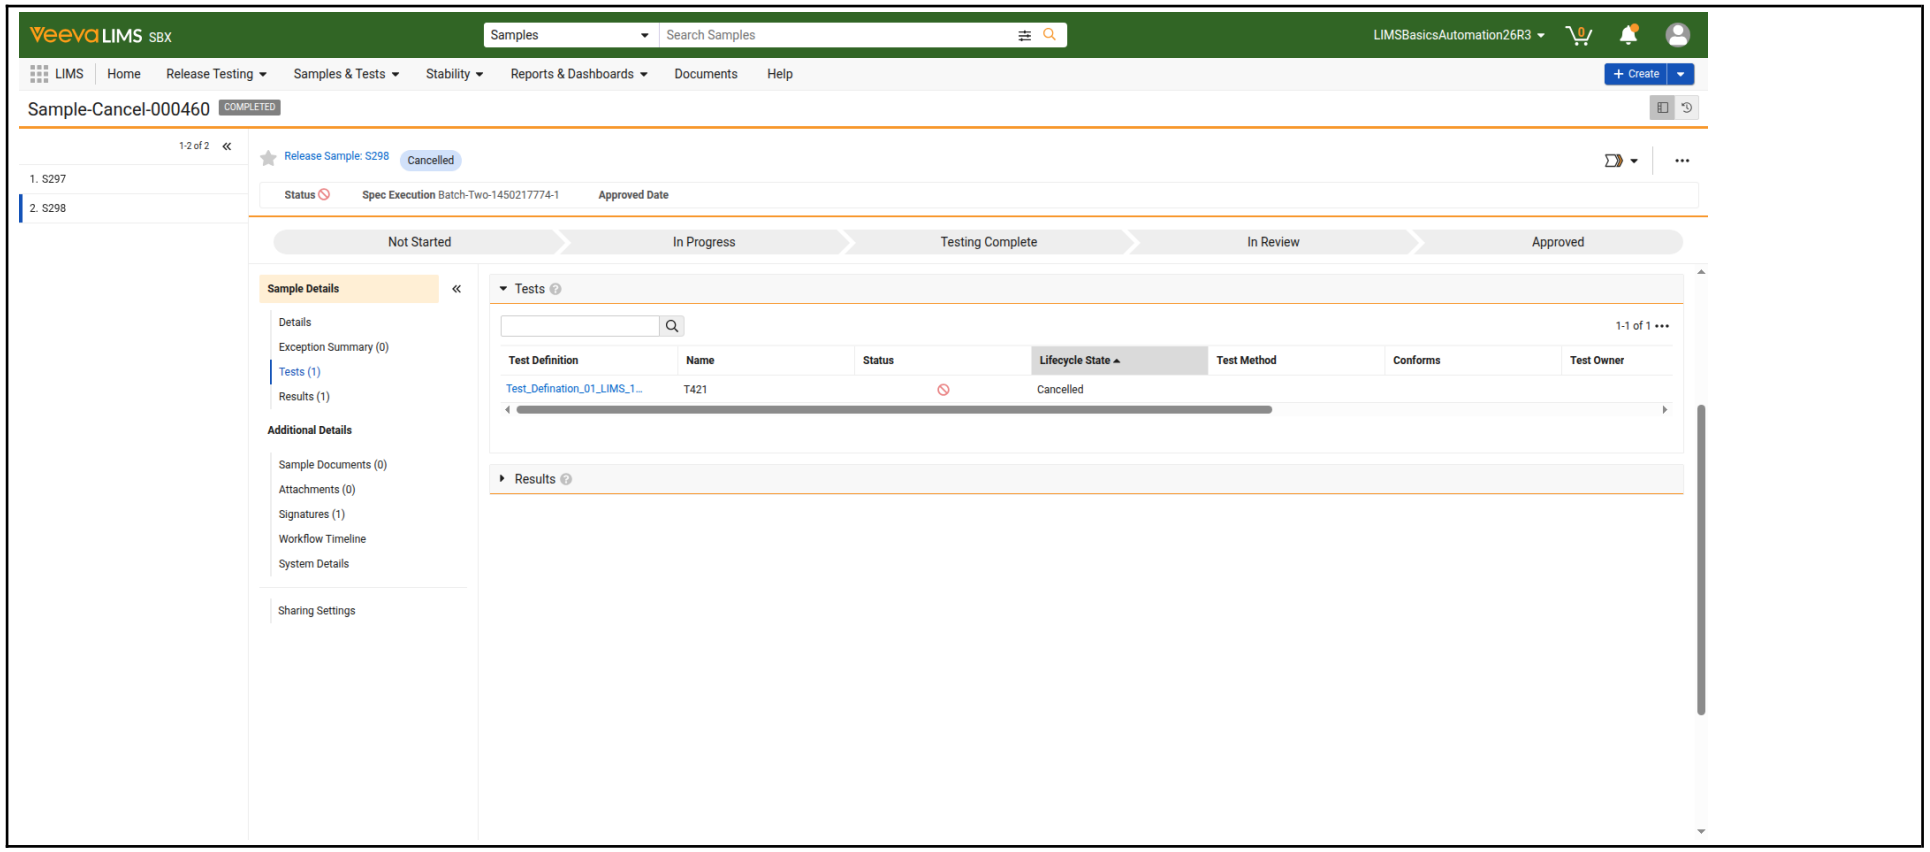

Veeva LIMS SBX
Samples
Search Samples
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
Create
Sample-Cancel-000460
COMPLETED
1-2 of 2
1. S297
2. S298
Release Sample: S298
Cancelled
Status
Spec Execution Batch-Two-1450217774-1
Approved Date
Not Started
In Progress
Testing Complete
In Review
Approved
Sample Details
Details
Exception Summary (0)
Tests (1)
Results (1)
Additional Details
Sample Documents (0)
Attachments (0)
Signatures (1)
Workflow Timeline
System Details
Sharing Settings
Tests
1-1 of 1
Test Definition
Name
Status
Lifecycle State
Test Method
Conforms
Test Owner
Test_Defination_01_LIMS_1...
T421
Cancelled
Results

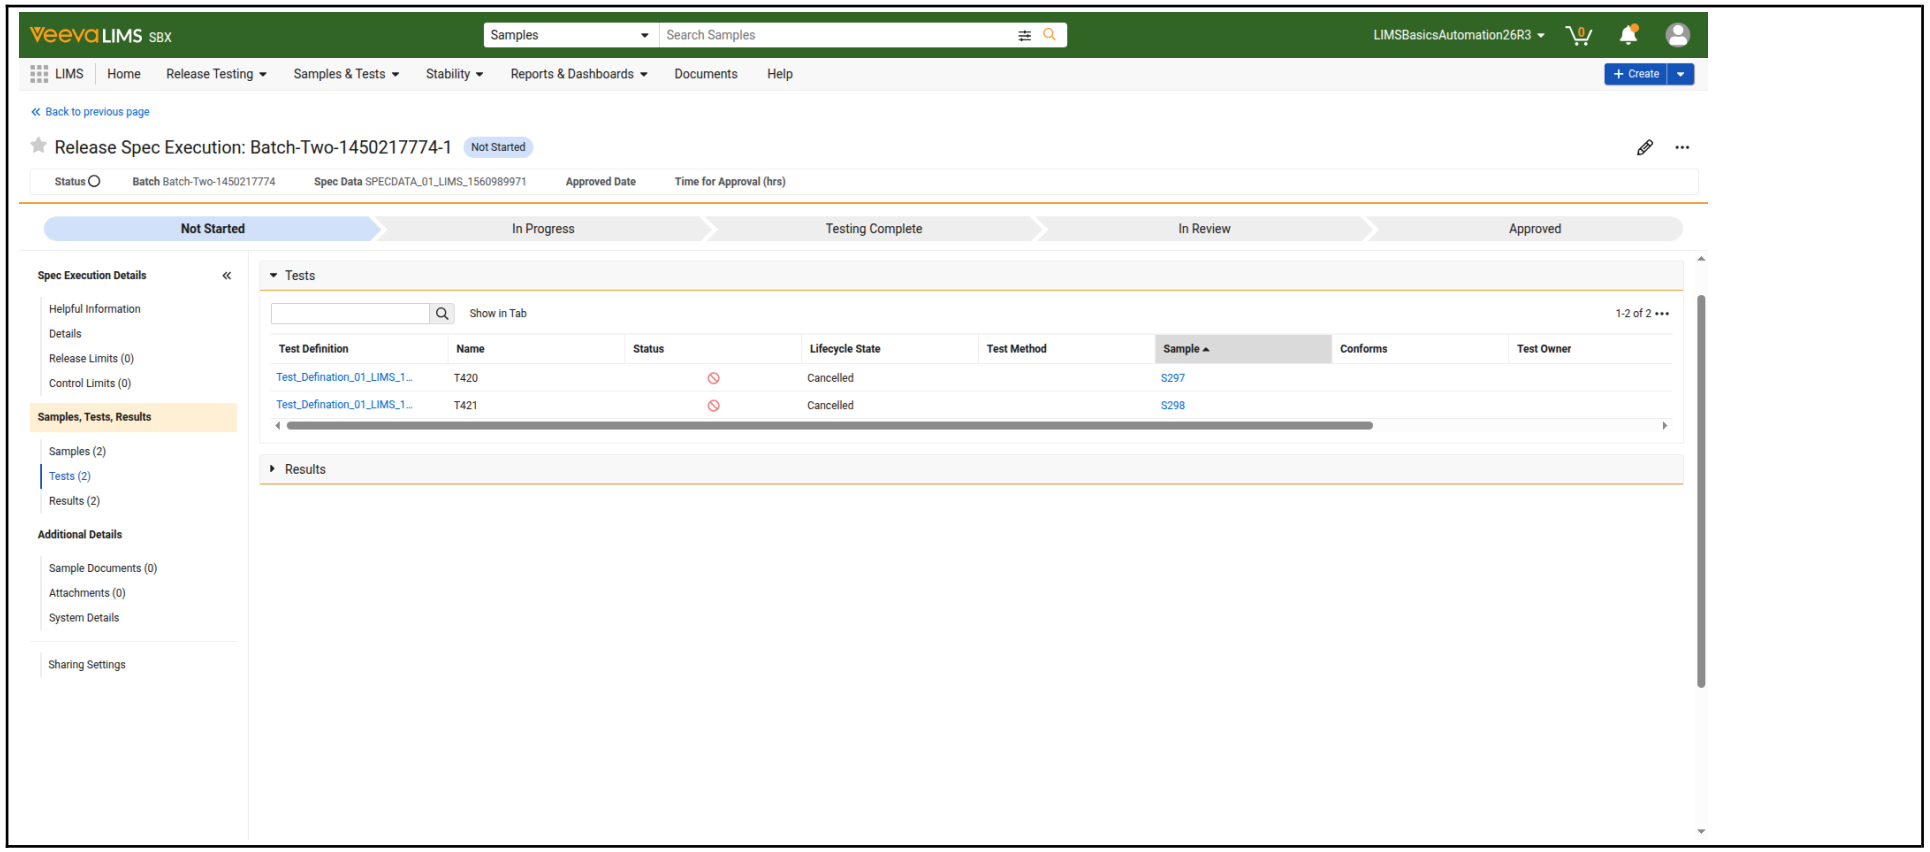
Veeva LIMS SBX
Samples
Search Samples
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
Create
Back to previous page
Release Spec Execution: Batch-Two-1450217774-1
Not Started
Status
Batch Batch-Two-1450217774
Spec Data SPECDATA_01_LIMS_1560989971
Approved Date
Time for Approval (hrs)
Not Started
In Progress
Testing Complete
In Review
Approved
Spec Execution Details
Helpful Information
Details
Release Limits (0)
Control Limits (0)
Samples, Tests, Results
Samples (2)
Tests (2)
Results (2)
Additional Details
Sample Documents (0)
Attachments (0)
System Details
Sharing Settings
Tests
Show in Tab
1-2 of 2
Test Definition
Name
Status
Lifecycle State
Test Method
Sample
Conforms
Test Owner
Test_Defination_01_LIMS_1...
T420
Cancelled
S297
Test_Defination_01_LIMS_1...
T421
Cancelled
S298
Results


Step #13 Screenshot Screenshot Time: 08-OCT-2026 09:11:09 GMT-07:00

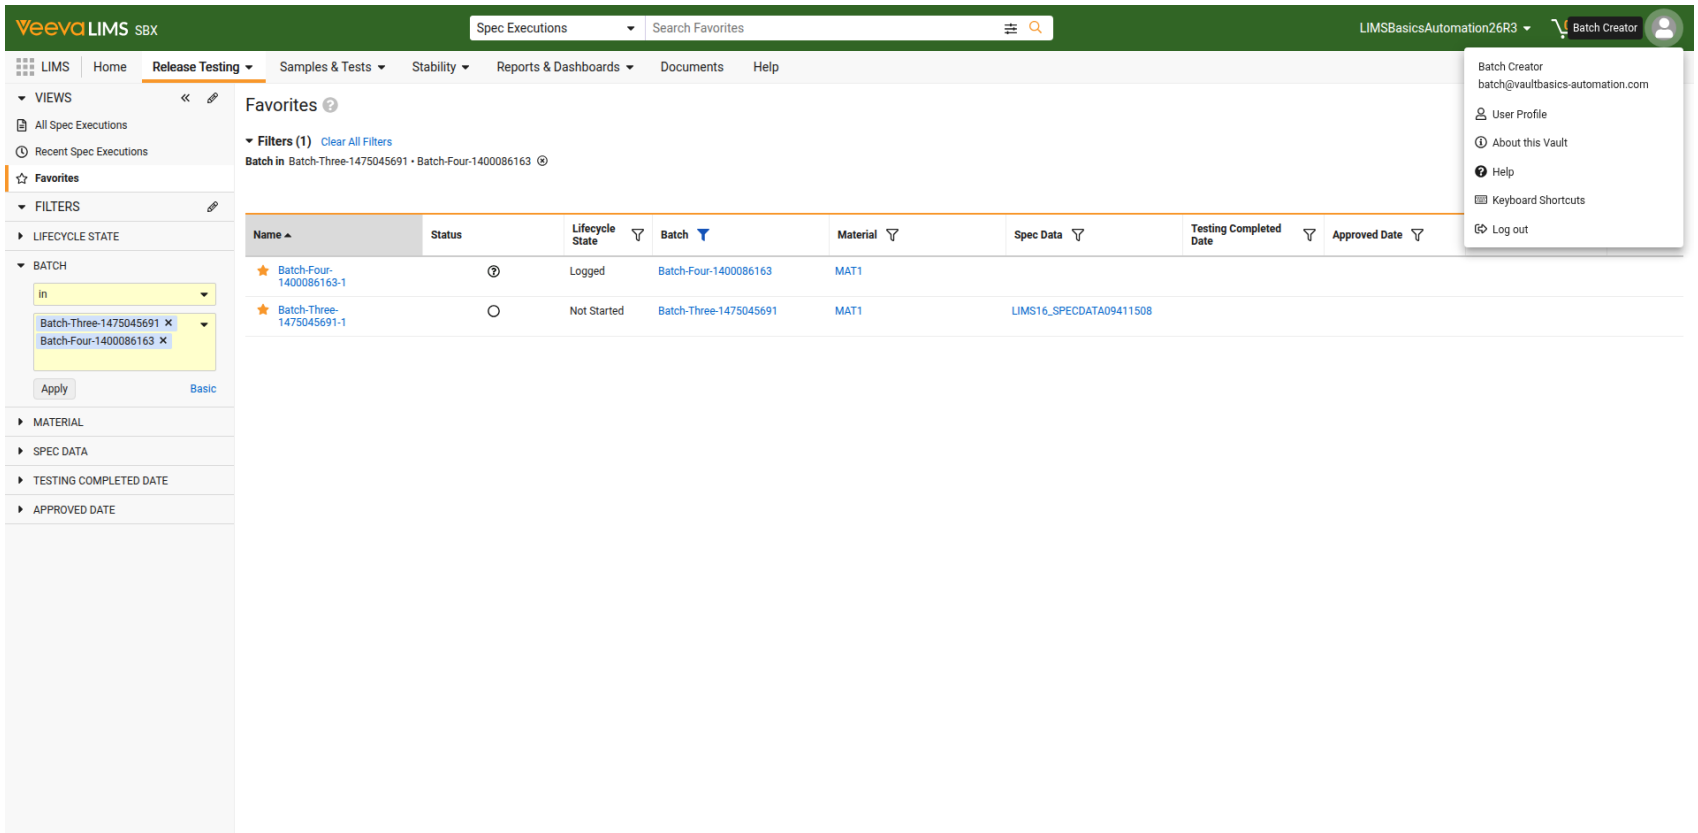


Step #14 Screenshot Screenshot Time: 08-OCT-2026 09:11:41 GMT-07:00

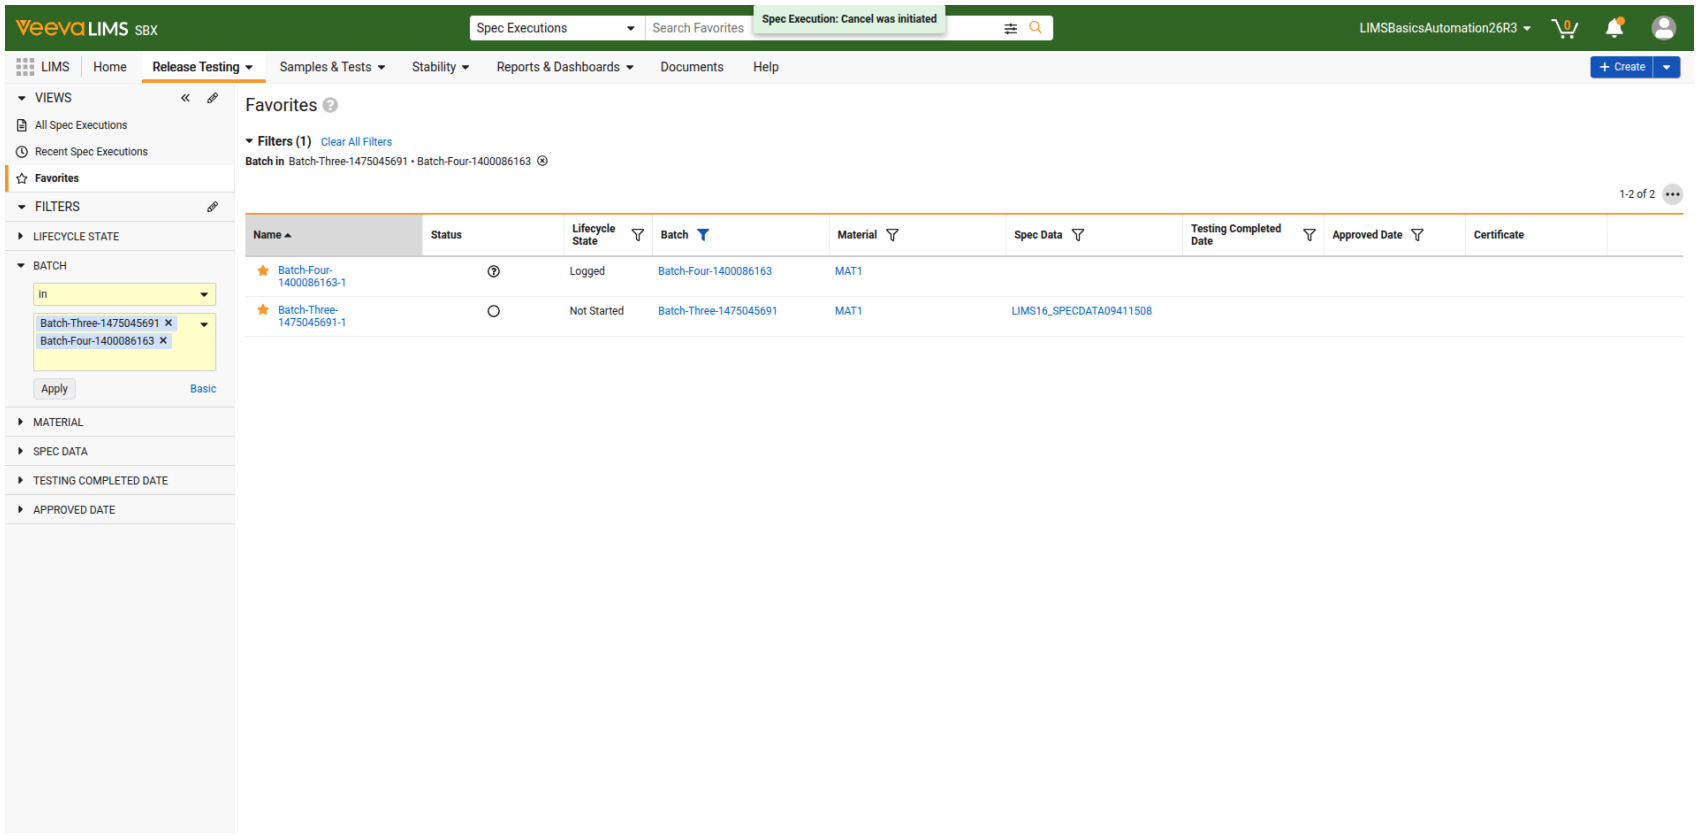


Step #15 Screenshot Screenshot Time: 08-OCT-2026 09:11:48 GMT-07:00

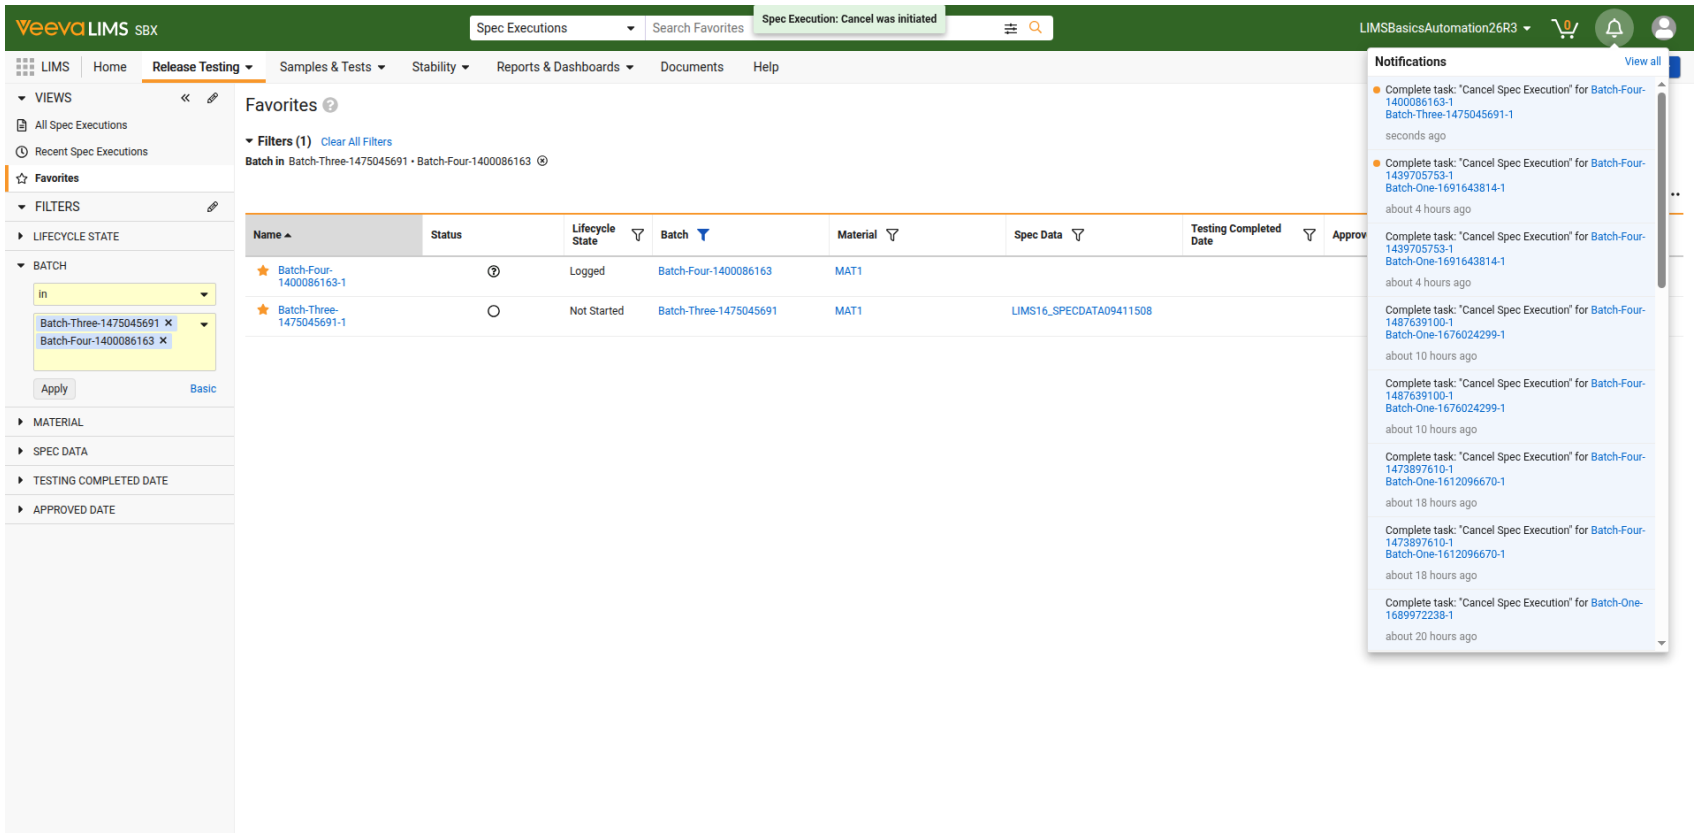


Step #16 Screenshot Screenshot Time: 08-OCT-2026 09:14:00 GMT-07:00,08-OCT-2026 09:14:08 GMT-07:00

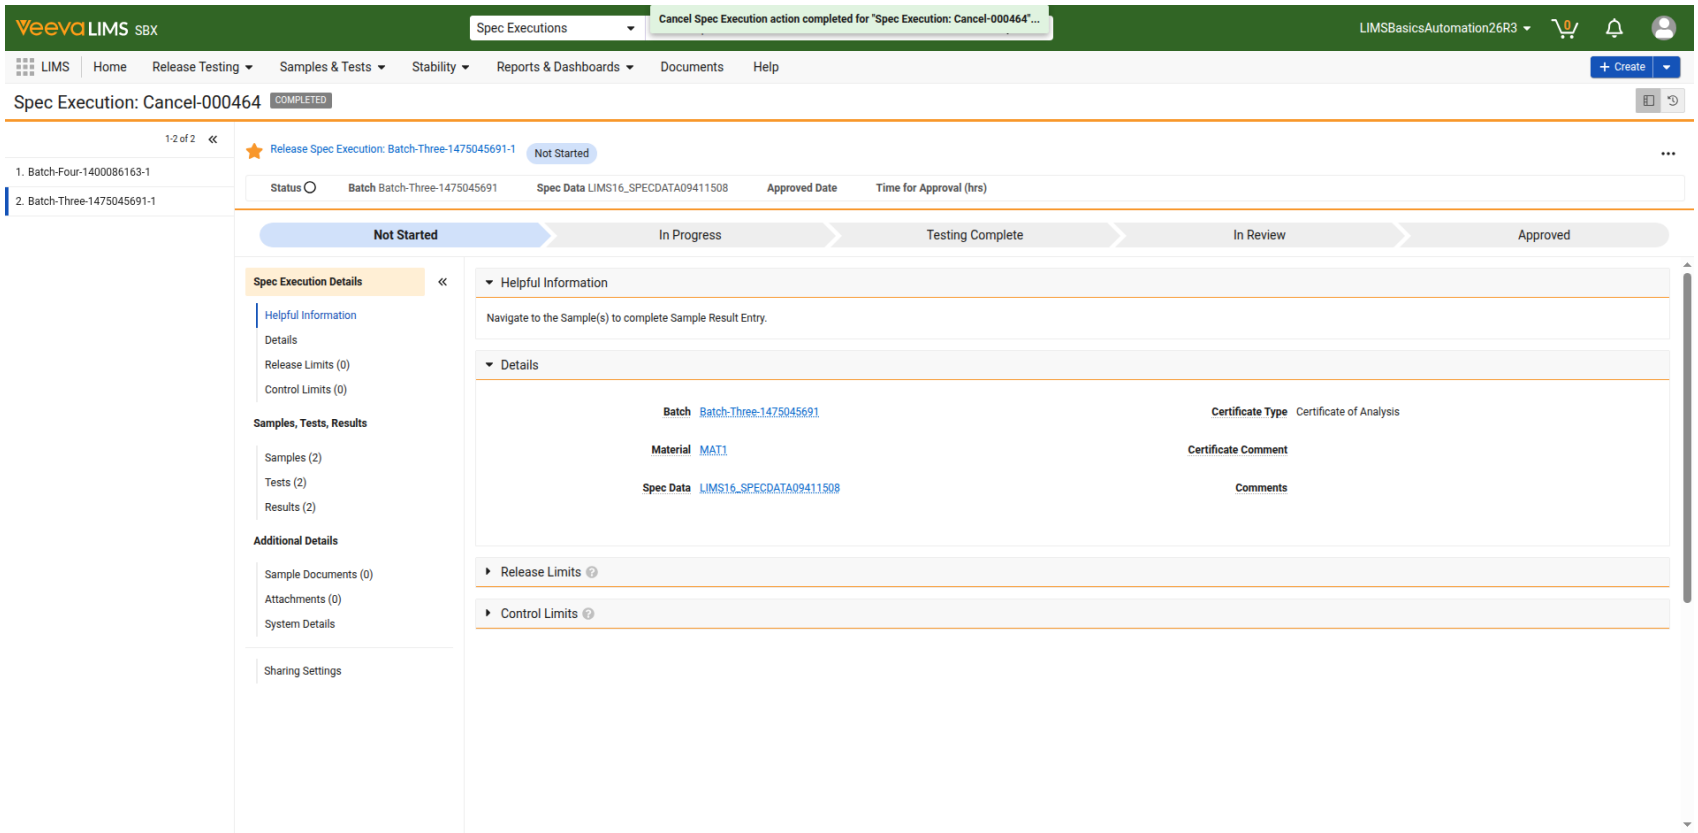


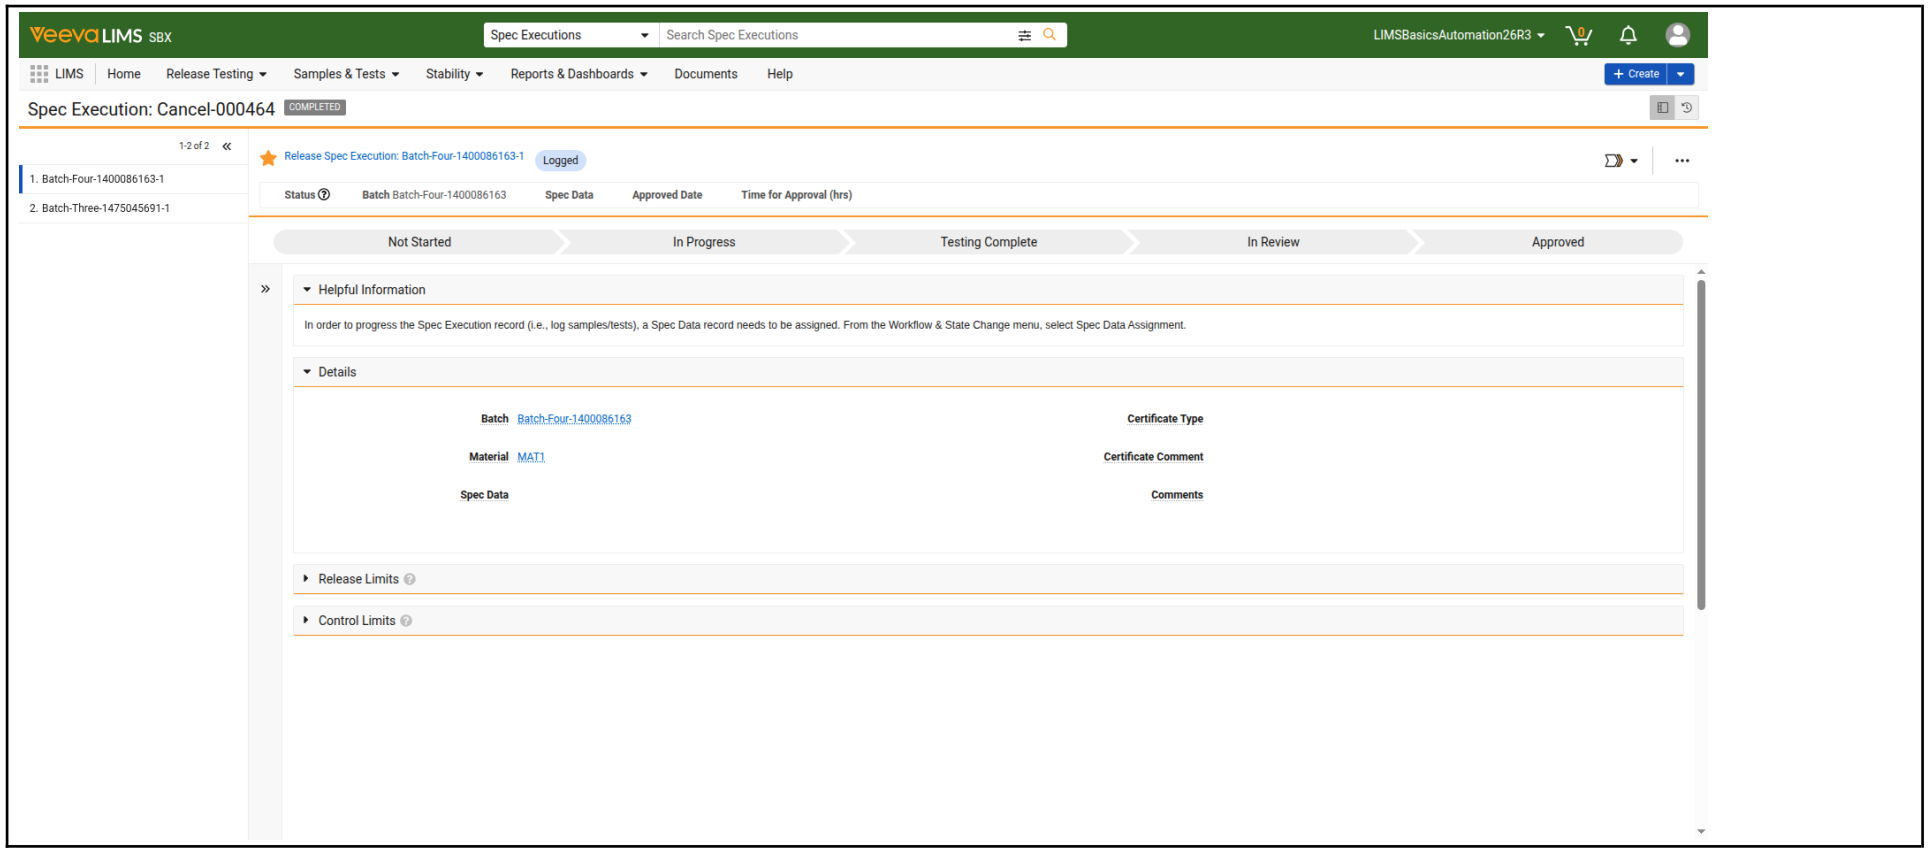

Veeva LIMS SBX
Spec Executions
Search Spec Executions
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
+ Create
Spec Execution: Cancel-000464
COMPLETED
1-2 of 2
1. Batch-Four-1400086163-1
2. Batch-Three-1475045691-1
Release Spec Execution: Batch-Four-1400086163-1
Logged
Status
Batch Batch-Four-1400086163
Spec Data
Approved Date
Time for Approval (hrs)
Not Started
In Progress
Testing Complete
In Review
Approved
Helpful Information
In order to progress the Spec Execution record (i.e., log samples/tests), a Spec Data record needs to be assigned. From the Workflow & State Change menu, select Spec Data Assignment.
Details
Batch
Batch-Four-1400086163
Material
MAT1
Spec Data
Certificate Type
Certificate Comment
Comments
Release Limits
Control Limits


Step #17 Screenshot Screenshot Time: 08-OCT-2026 09:16:45 GMT-07:00

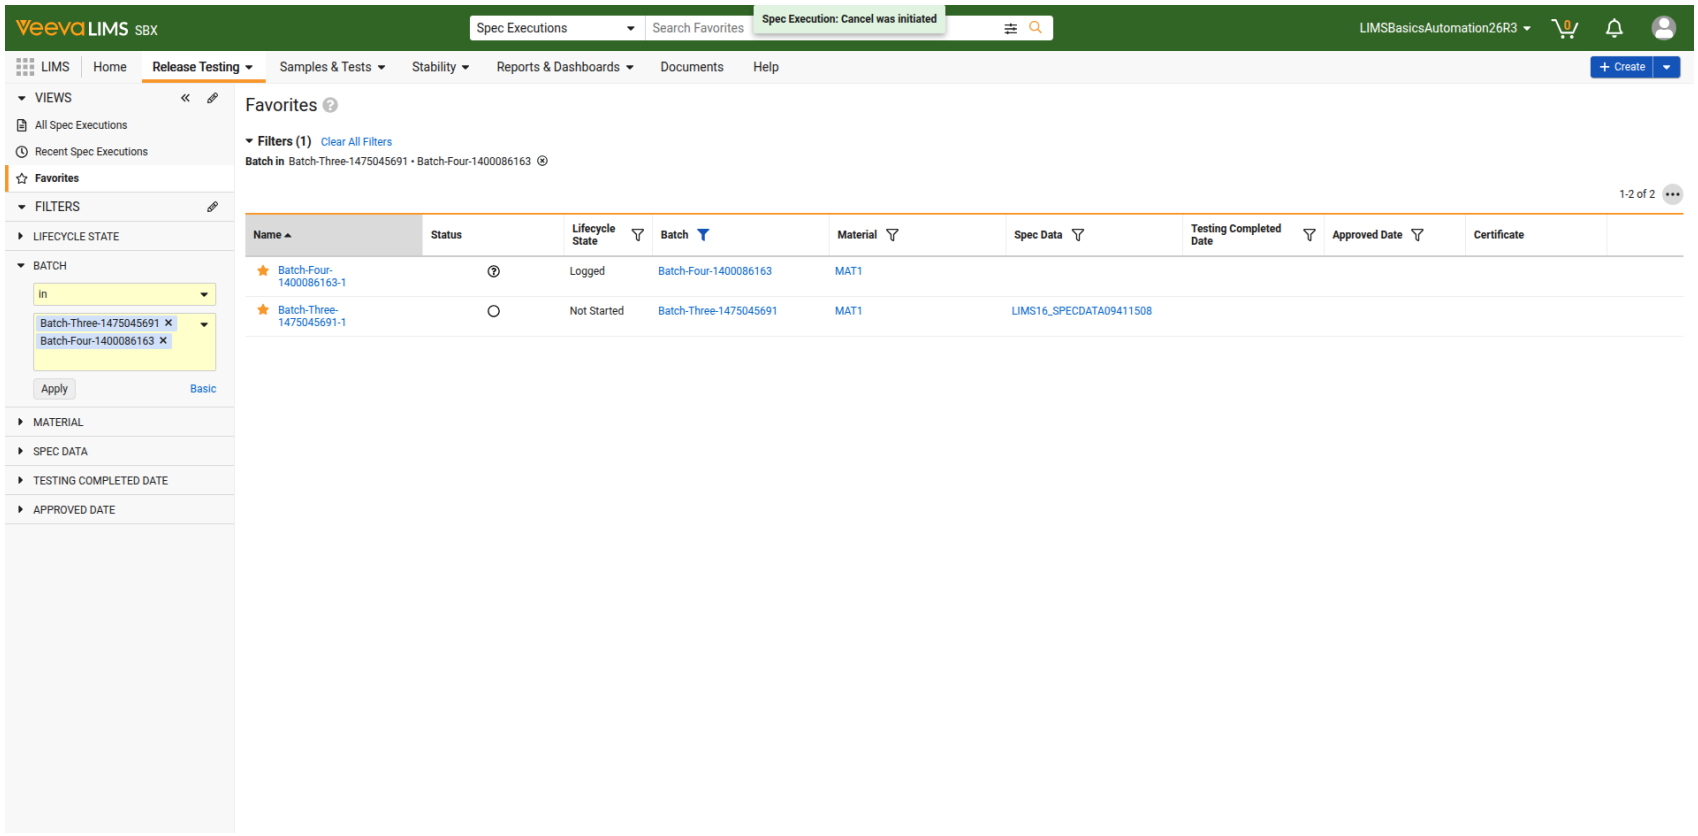



Step #18 Screenshot Screenshot Time: 08-OCT-2026 09:19:19 GMT-07:00,08-OCT-2026 09:19:27 GMT-07:00,08-OCT-2026 09:21:05 GMT-07:00,08-OCT-2026 09:26:48 GMT-07:00,08-OCT-2026 09:28:25 GMT-07:00,08-OCT-2026 09:30:01 GMT-07:00

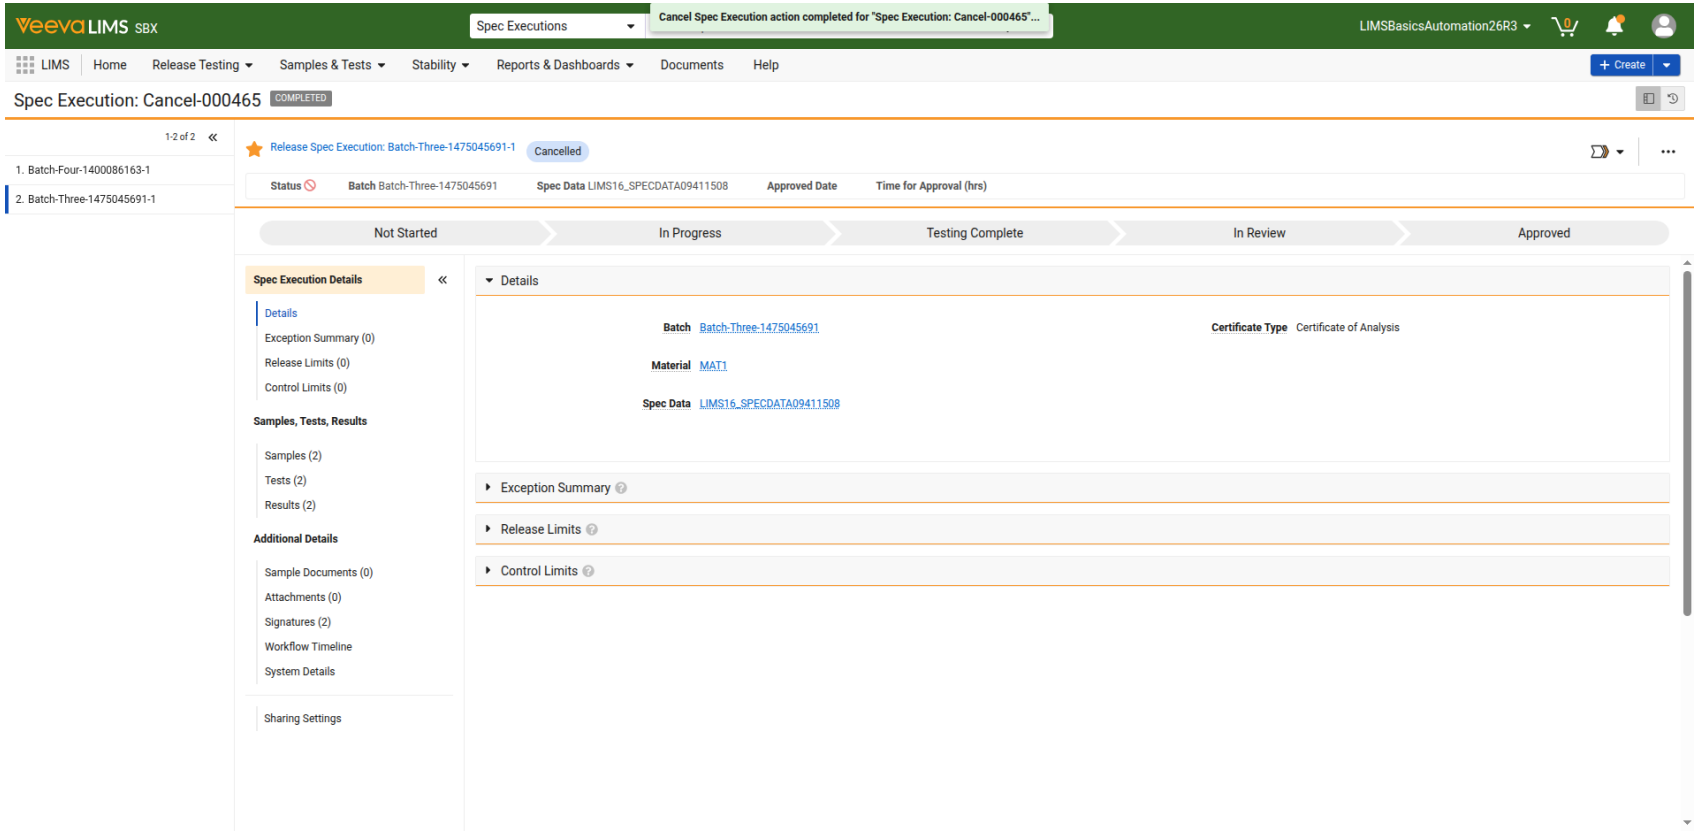


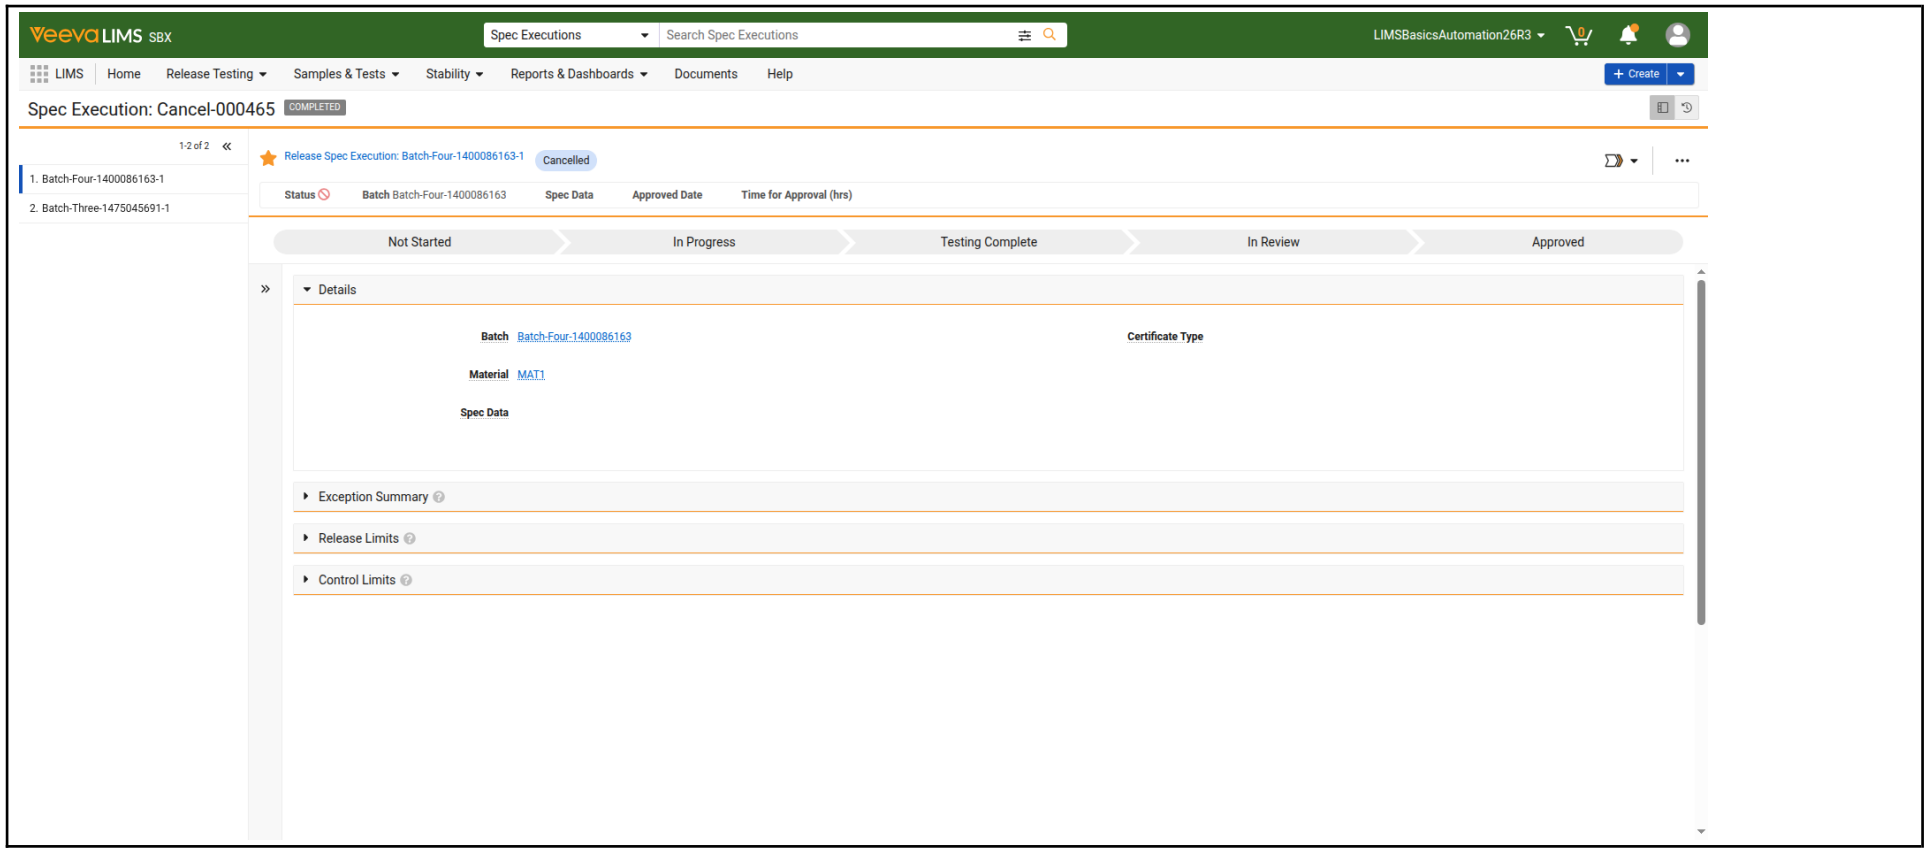
Veeva LIMS SBX
Spec Executions
Search Spec Executions
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
Create
Spec Execution: Cancel-000465
COMPLETED
1-2 of 2
1. Batch-Four-1400086163-1
2. Batch-Three-1475045691-1
Release Spec Execution: Batch-Four-1400086163-1
Cancelled
Status
Batch Batch-Four-1400086163
Spec Data
Approved Date
Time for Approval (hrs)
Not Started
In Progress
Testing Complete
In Review
Approved
Details
Batch Batch-Four-1400086163
Material MAT1
Spec Data
Certificate Type
Exception Summary
Release Limits
Control Limits

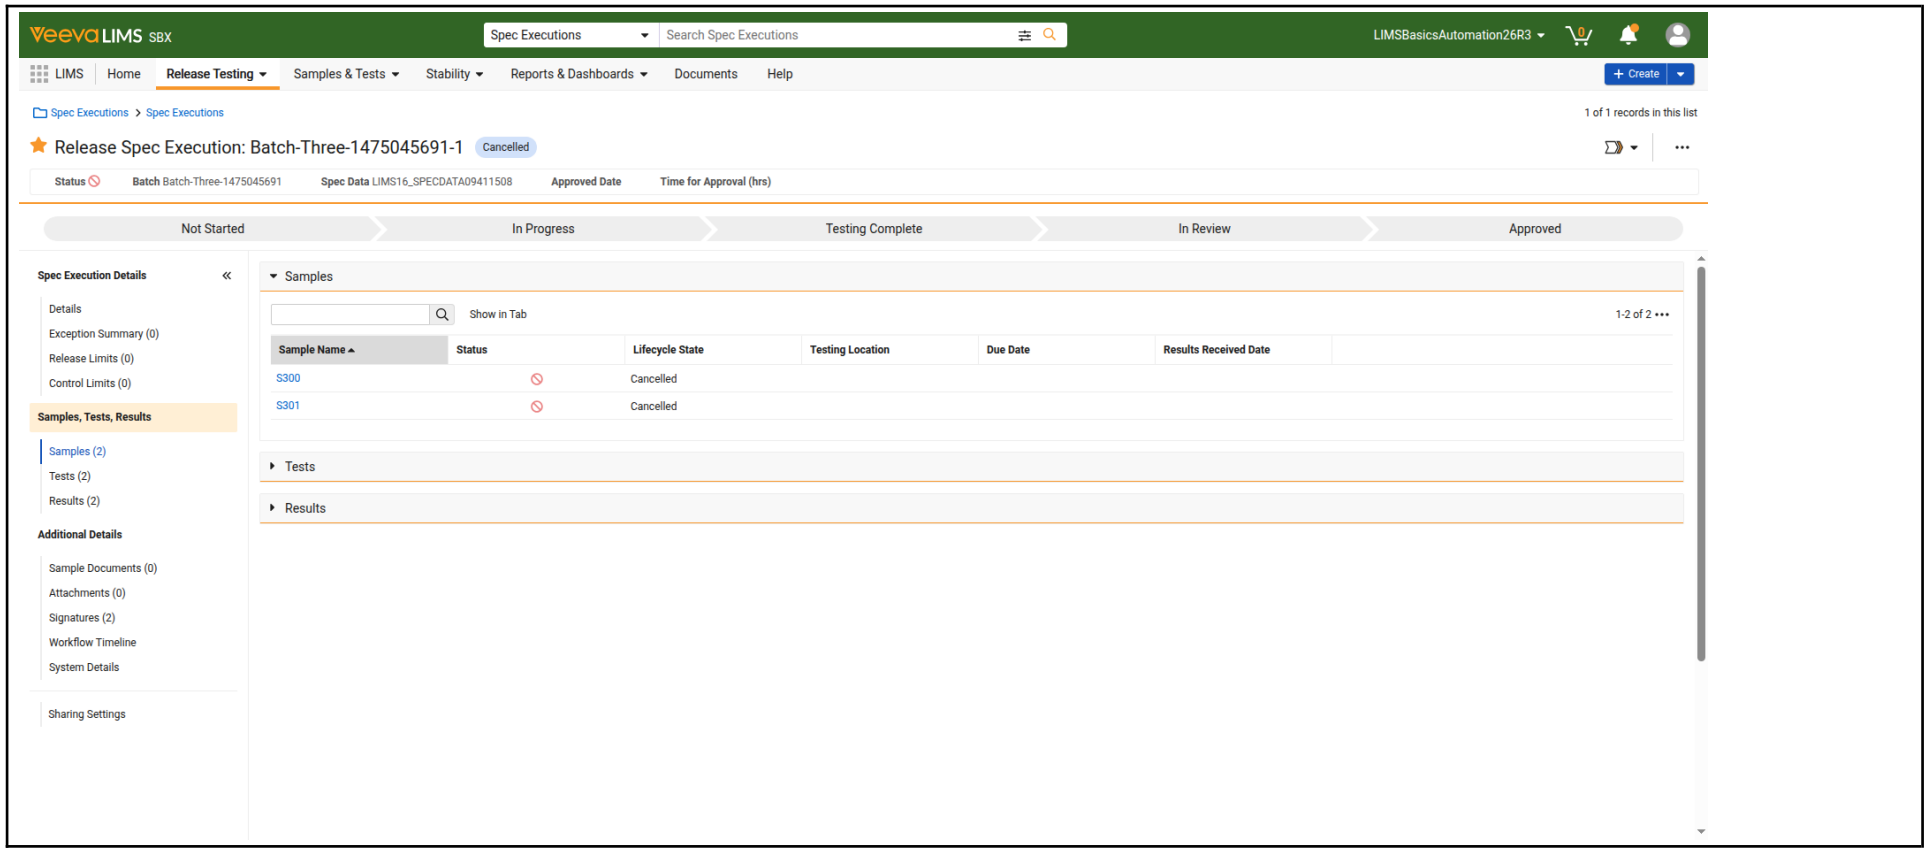
Veeva LIMS SBX
Spec Executions
Search Spec Executions
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
Create
Spec Executions > Spec Executions
1 of 1 records in this list
Release Spec Execution: Batch-Three-1475045691-1
Cancelled
Status
Batch Batch-Three-1475045691
Spec Data LIMS16_SPECDATA09411508
Approved Date
Time for Approval (hrs)
Not Started
In Progress
Testing Complete
In Review
Approved
Spec Execution Details
Details
Exception Summary (0)
Release Limits (0)
Control Limits (0)
Samples, Tests, Results
Samples (2)
Tests (2)
Results (2)
Additional Details
Sample Documents (0)
Attachments (0)
Signatures (2)
Workflow Timeline
System Details
Sharing Settings
Samples
Show in Tab
1-2 of 2
Sample Name
Status
Lifecycle State
Testing Location
Due Date
Results Received Date
S300
Cancelled
S301
Cancelled
Tests
Results

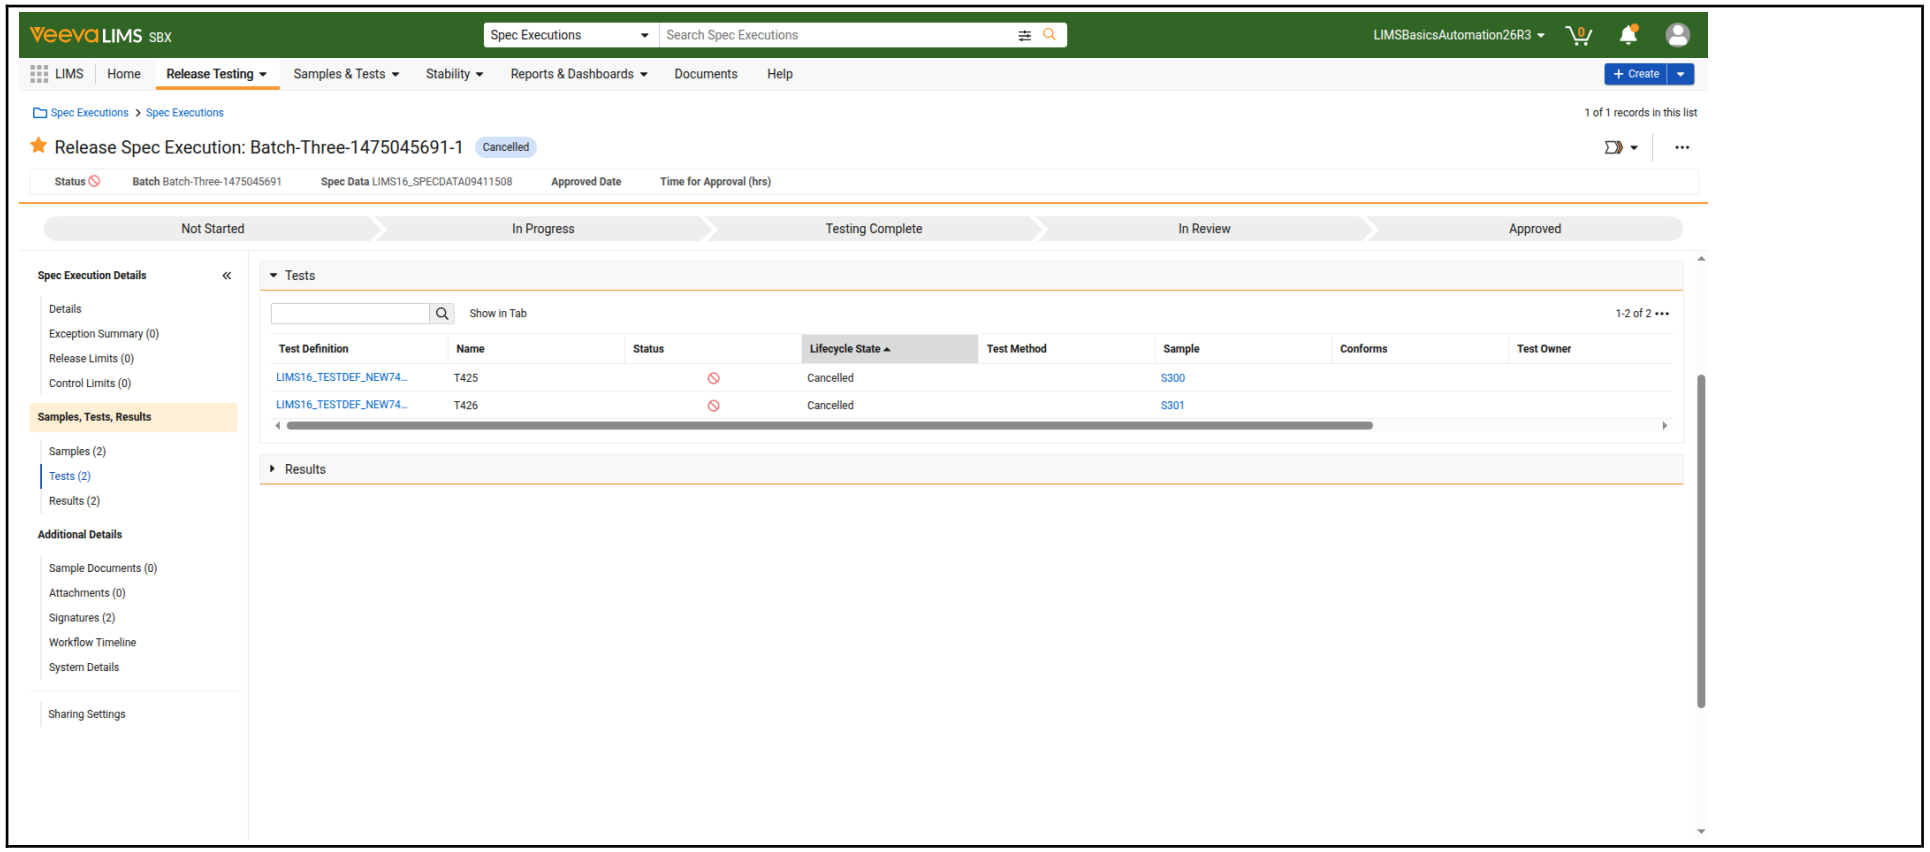
Veeva LIMS SBX
Spec Executions
Search Spec Executions
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
Create
Spec Executions > Spec Executions
1 of 1 records in this list
Release Spec Execution: Batch-Three-1475045691-1
Cancelled
Status
Batch Batch-Three-1475045691
Spec Data LIMS16_SPECDATA09411508
Approved Date
Time for Approval (hrs)
Not Started
In Progress
Testing Complete
In Review
Approved
Spec Execution Details
Details
Exception Summary (0)
Release Limits (0)
Control Limits (0)
Samples, Tests, Results
Samples (2)
Tests (2)
Results (2)
Additional Details
Sample Documents (0)
Attachments (0)
Signatures (2)
Workflow Timeline
System Details
Sharing Settings
Tests
Show in Tab
1-2 of 2
Test Definition
Name
Status
Lifecycle State
Test Method
Sample
Conforms
Test Owner
LIMS16_TESTDEF_NEW74...
T425
Cancelled
S300
LIMS16_TESTDEF_NEW74...
T426
Cancelled
S301
Results

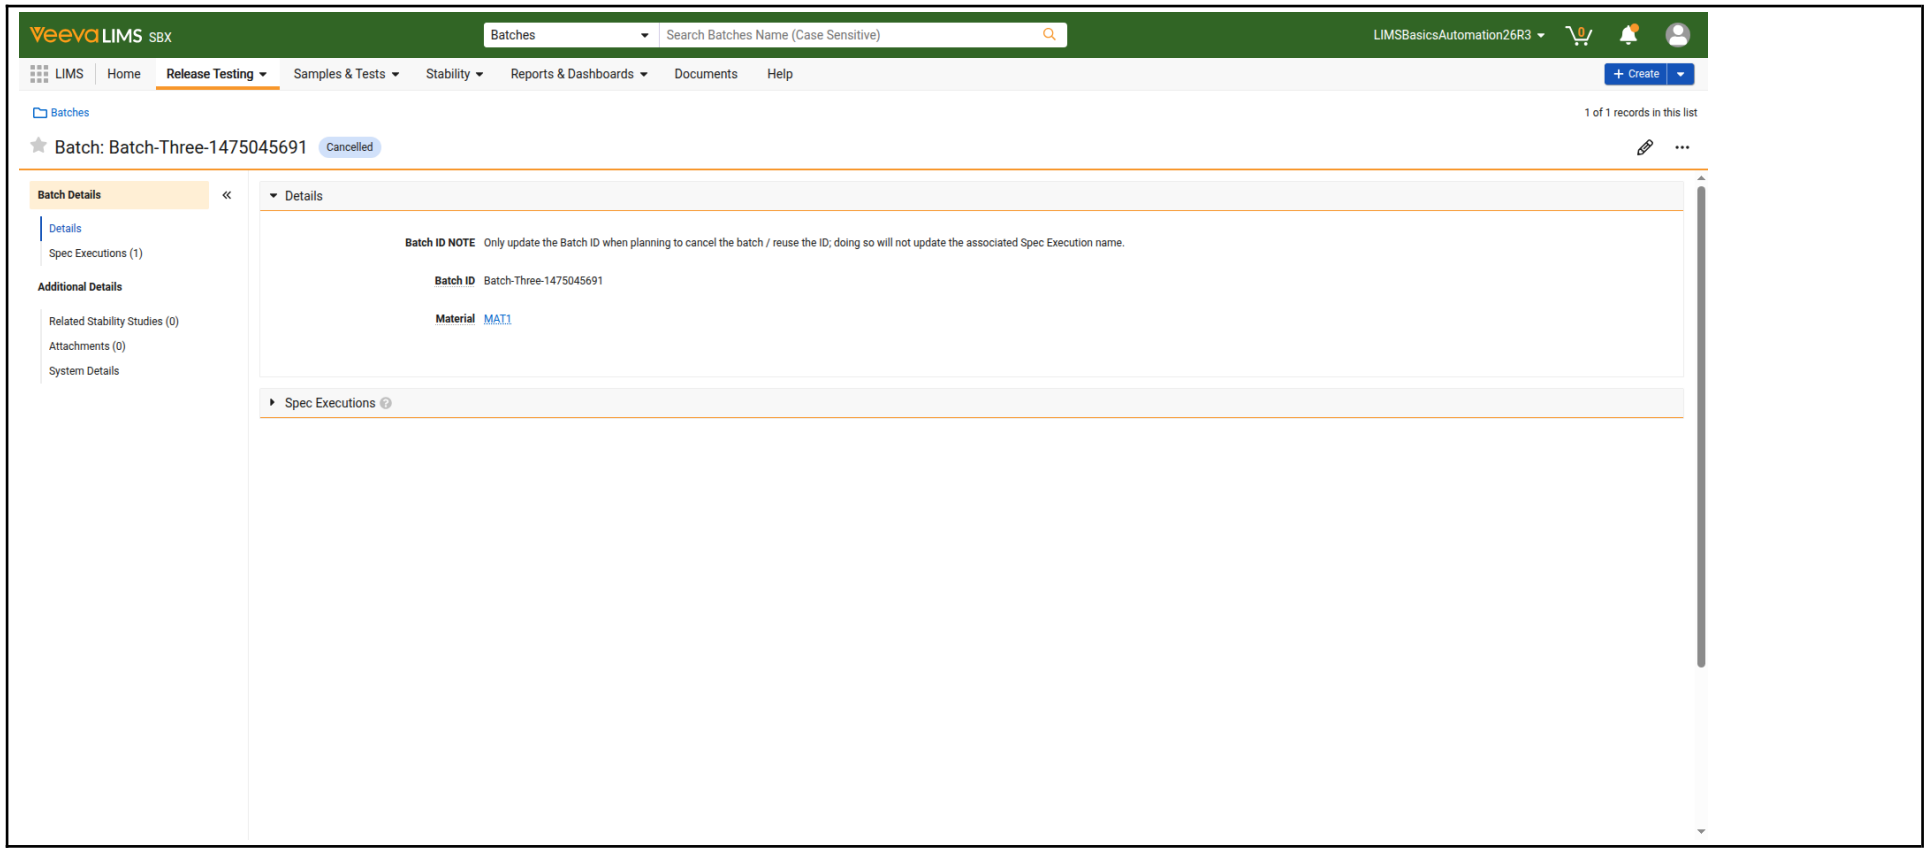
Veeva LIMS SBX
Batches
Search Batches Name (Case Sensitive)
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
+ Create
Batches
1 of 1 records in this list
Batch: Batch-Three-1475045691
Cancelled
Batch Details
Details
Spec Executions (1)
Additional Details
Related Stability Studies (0)
Attachments (0)
System Details
Details
Batch ID NOTE Only update the Batch ID when planning to cancel the batch / reuse the ID; doing so will not update the associated Spec Execution name.
Batch ID Batch-Three-1475045691
Material MAT1
Spec Executions

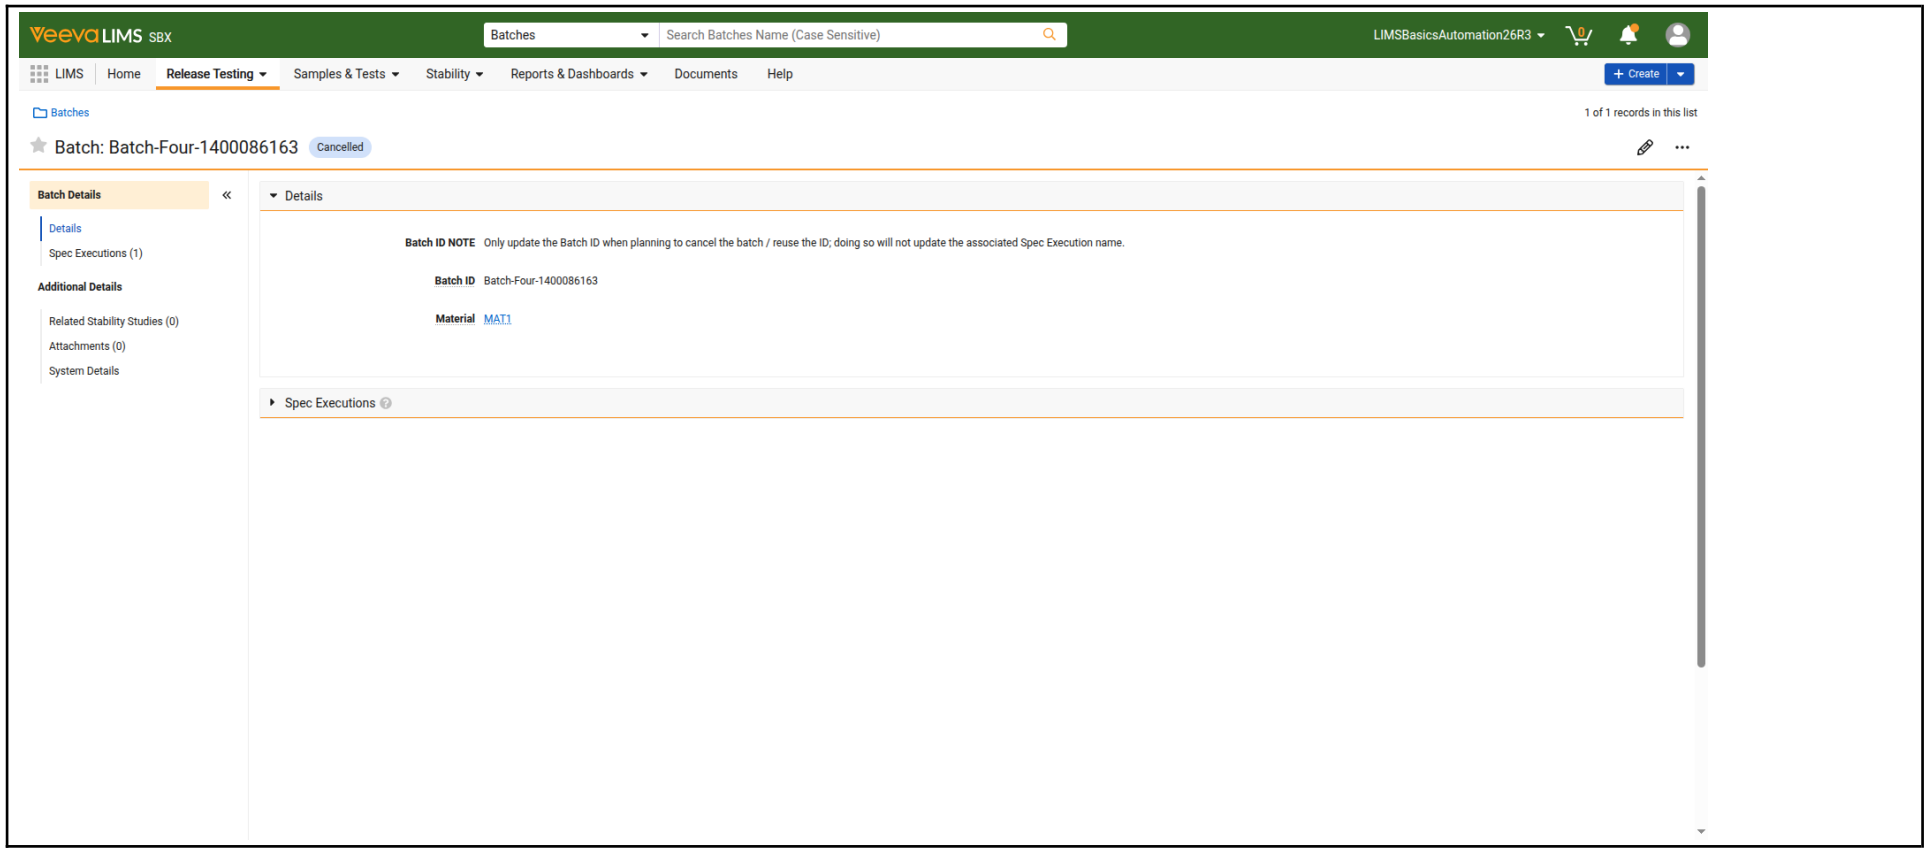
Veeva LIMS SBX
Batches
Search Batches Name (Case Sensitive)
LIMSBasicsAutomation26R3
LIMS
Home
Release Testing
Samples & Tests
Stability
Reports & Dashboards
Documents
Help
+ Create
Batches
1 of 1 records in this list
Batch: Batch-Four-1400086163
Cancelled
Batch Details
Details
Spec Executions (1)
Additional Details
Related Stability Studies (0)
Attachments (0)
System Details
Details
Batch ID NOTE
Only update the Batch ID when planning to cancel the batch / reuse the ID; doing so will not update the associated Spec Execution name.
Batch ID
Batch-Four-1400086163
Material
MAT1
Spec Executions

Script Execution Approval - to be completed by Validation Lead	
Deviations	Were there any deviations that were observed during the execution? NO
	If yes, have they been successfully resolved?
Acceptance Criteria	Have all test steps been successfully executed? YES
Validation Lead	Electronically signed through Veeva
Quality Assurance Approver	Electronically signed through Veeva